



Designation: D4875 – 18

Standard Test Methods of Polyurethane Raw Materials: Determination of the Polymerized Ethylene Oxide Content of Polyether Polyols¹

This standard is issued under the fixed designation D4875; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

1. Scope*

1.1 *Test Method A*—Proton Nuclear Magnetic Resonance Spectroscopy (^1H NMR) measures polymerized ethylene oxide (EO) content of ethylene oxide (EO) propylene oxide (PO) polyether polyols used in flexible polyurethane foams and non-foams. It is suitable for diols initiated from glycols of EO or PO containing EO percentages >5 . For triols initiated with glycerol (glycerin) and trimethylolpropane, an uncorrected EO value is obtained since both initiators have protons that contribute to the EO measurement.

1.2 *Test Method B*—Carbon-13 Nuclear Magnetic Resonance Spectroscopy (^{13}C NMR) measures the polymerized EO content of EO-PO polyether polyols used in flexible polyurethane foams and non-foams. It is suitable for diols and triols made from the commonly used initiators and containing EO percentages >5 .

1.3 The values stated in SI units are to be regarded as standard.

1.4 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety, health, and environmental practices and determine the applicability of regulatory limitations prior to use.*

NOTE 1—There is no known ISO equivalent to this standard.

1.5 *This international standard was developed in accordance with internationally recognized principles on standardization established in the Decision on Principles for the Development of International Standards, Guides and Recommendations issued by the World Trade Organization Technical Barriers to Trade (TBT) Committee.*

¹ These test methods are under the jurisdiction of ASTM Committee D20 on Plastics and is the direct responsibility of Subcommittee D20.22 on Cellular Materials - Plastics and Elastomers.

Current edition approved April 1, 2018. Published April 2018. Originally approved in 1988. Last previous edition approved in 2011 as D4875 - 11. DOI: 10.1520/D4875-18.

2. Referenced Documents

- 2.1 *ASTM Standards*:²
 - D883 Terminology Relating to Plastics
 - E691 Practice for Conducting an Interlaboratory Study to Determine the Precision of a Test Method
 - E2977 Practice for Measuring and Reporting Performance of Fourier-Transform Nuclear Magnetic Resonance (FT-NMR) Spectrometers for Liquid Samples

3. Terminology

3.1 *Definitions*—For definitions of terms that appear in this method refer to Terminology D883 and Practice E2977.

3.2 *Definitions of Terms Specific to This Standard*:

3.2.1 *heteric polyol, n*—a polyether polyol in which ethylene oxide and propylene oxide units are randomly arranged.

3.2.2 *initiator, n*—a substance with which ethylene oxide or propylene oxide reacts to form a polyether polyol.

3.2.2.1 *Discussion*—One initiator unit is incorporated into each polymer or oligomer molecule.

3.2.3 *EO capped polyol*—a polyol that contains a terminal block of ethylene oxide units

4. Summary of Test Methods

4.1 *Test Method A*—The ^1H NMR spectra of polyether polyols show two groups of resonance peaks. The first group corresponds to the methyl protons of propylene oxide (PO). The second group corresponds to the methylene and methine protons of PO and the methylene protons of EO. The EO peak area is obtained by subtracting the area of the PO methyl peaks from the area of the methylene and methine peaks. Initiators other than glycols of EO and PO give systematic errors (see Note 2).

NOTE 2—The initiator error can be estimated by calculating the

² For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

*A Summary of Changes section appears at the end of this standard

theoretical contribution of initiator protons to the EO and PO peak areas. This calculation is outside the scope of this method.

4.2 *Test Method B*—The ^{13}C NMR spectra of polyether polyols contain multiple resonances arising from initiator, EO, PO, EO-PO sequencing, tacticity, and end-group distribution. The EO content can be determined relative to PO and EO or, relative to the triol initiator if present. In the former, the area of the EO methylene carbons is ratioed to the total area of PO methylene and methine carbons and EO methylene carbons. In the latter, the area of the EO methylene carbons is ratioed to the area of two initiator carbons. This test method describes the determination of EO relative to PO and EO only.

5. Significance and Use

5.1 Measurements of EO content correlate to polyol reactivity (as related to primary hydroxyl content), linearity of foam rise, and hydrophilicity of the polyol and final product.

TEST METHOD A—PROTON NMR

6. Apparatus

6.1 *Fourier Transform NMR (FT-NMR) Spectrometer*, with a proton resonance frequency of 200 MHz or higher. The spectrometer is to have a minimum proton signal-to-noise ratio of 100:1 based on a 0.1 % ethylbenzene in deuterated chloroform (CDCl_3) sample that has been pulsed once using a 90° pulse angle under the conditions described in Practice E2977.

6.2 *NMR sample tubes*, having outside diameters of 5 mm.

6.3 *NMR spinners*.

7. Reagents and Materials

7.1 All reagents are to be spectroscopic grade and free of magnetic materials.

7.2 *Trifluoroacetic acid*.

7.3 *Deuterated chloroform*, containing tetramethylsilane (TMS) as an internal standard.

8. Hazards

8.1 *Magnetic Fields*—Follow the manufacturer's recommendation for the safe operation of the instrument.

8.1.1 Persons with implanted or attached medical devices such as pacemakers and prosthetic parts must remain outside the 5-gauss perimeter.

8.1.2 Objects made of ferromagnetic material will be attracted to the magnet and are to be kept a safe distance away.

9. Preparation of Apparatus

9.1 Prepare a proton NMR experiment selecting appropriate parameters to obtain quantitative integration of the spectrum.

9.1.1 *Pulse Angle and Sequence Delay Time*—Select a 90 degree pulse angle with a delay of $10 \times T_1$ of the peak with the longest relaxation time in the spectrum. It is acceptable to use a different pulse angle/sequence delay combination provided that quantitative data acquisition is not compromised.

9.1.2 *Number of Scans*—Select the appropriate number to yield a signal to noise of >100:1 between 2 and 0.5 ppm (usually 16 to 64).

9.1.3 *Sweep Width*—~14 ppm.

9.1.4 *Transmitter Frequency*—~6 ppm.

9.1.5 *Acquisition Time*—2 to 4 s.

10. Calibration and Standardization

10.1 This test method does not require standards. To evaluate the test method, standards can be prepared by blending commercially available poly(propylene oxide) and poly(ethylene oxide) diols. The molecular weights of the diols should ideally be 300 or more since lower molecular weight polyols can contain structural configurations that are not typical of polyether polyols used in flexible polyurethane foams and non-foams.

11. Procedure

11.1 Prepare a solution of the polyol in deuterated chloroform. A 0.5-5 % solution is recommended. Add one to two drops of trifluoroacetic acid and mix well. More acid will be required if a higher than recommended concentration of polyol is used (see NOTE 3).

11.2 Transfer an appropriate amount of the sample solution to an NMR tube.

11.3 Place the NMR tube into a spinner, adjust it to the appropriate depth and insert it into the spectrometer probe.

11.4 Obtain a stable lock on the solvent.

11.5 Tune and match the probe.

11.6 Shim the sample to optimize field-homogeneity.

11.7 Acquire the NMR data.

11.8 Zero fill the data. The recommended value is 1 or 2 x number of points.

11.9 Apply a spectral weighting function (apodization) and Fourier Transform the Free Induction Decay (FID). The recommended apodization is an exponential window multiplication and a typical line broadening value is 1/acquisition time.

11.10 Phase and baseline correct the spectrum.

11.11 Set the internal TMS reference to 0 ppm.

11.12 Expand and integrate the peaks of interest. The methyl protons of PO typically resonate in the 0.5-1.7 ppm region (Area A). The methylene and methine protons of PO and the methylene protons of EO typically resonate in the 2.8-4.8 ppm region (Area B). An example is shown in Fig. 1 (see Note 4).

NOTE 3—Trifluoroacetic acid is added to move hydroxyl (OH) protons to a higher chemical shift and away from the regions of interest. The sample should be run as soon as practical after preparation to minimize the formation of esters of trifluoroacetic acid.

NOTE 4—Allyl unsaturation, if present, will contribute to the integral value of Area B. This contribution is expected to be minor for typical EO-PO polyether polyols and can be corrected by subtracting the integral value of two ally protons that have chemical shifts outside the regions of interest. This correction is not included in the scope of this method.

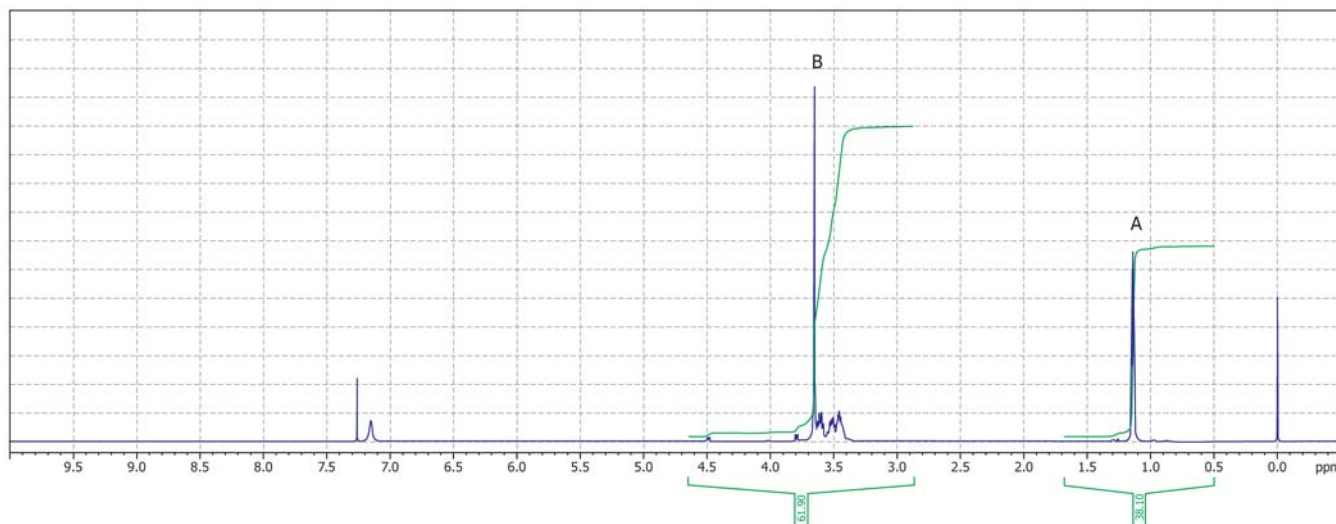


FIG. 1 ¹H NMR Spectrum of a DPG Initiated EO/PO Polyol (BB23798)

12. Calculation

12.1 Calculate the weight percent EO content using the following equation:

$$EO, wt\% = \frac{C * 44.05 * 100}{(C * 44.05) + (D * 58.08)} \times 100 \quad (1)$$

where:

- A = area of methyl PO protons,
- B = area of methylene and methine PO protons and area of methylene EO protons,
- C = (B-A)/4 integral per EO proton,
- D = A/3 integral per PO proton,
- 44.05 = g EO/mole, and
- 58.08 = g PO/mole.

13. Report

13.1 Report the % EO content to two decimal places. For polyether polyols with initiators other than glycols of EO and PO, report that the value is uncorrected for the initiator.

14. Precision and Bias

14.1 **Table 1** is based on a round robin conducted in 2016 in accordance with Practice **E691**, involving five materials tested by six laboratories. For each material, all the samples were prepared at one source, but the individual specimens were prepared at the laboratories which tested them. Each test result was a single determination. Each laboratory obtained two test results for each material.

14.2 **Caution**—The explanation of “r” and “R” is only intended to present a meaningful way of considering the approximate precision of this test method. Do not apply the data in **Table 1** to accept or reject materials, as these data apply only to the materials tested in the round robin and are unlikely to be rigorously representative of other lots, formulations, conditions, materials, or laboratories. Users of this test method need to apply the principles outlined in Practice **E691** to

generate data specific to their materials and laboratory (or between specific laboratories). The principles would then be valid for such data.

14.3 **Repeatability**—Precision under repeatability conditions.

14.4 **Reproducibility**—Precision under reproducibility conditions.

14.5 Any judgment in accordance with the repeatability and reproducibility statements shown would have an approximate 95 % (0.95) probability of being correct.

14.6 There are no recognized standards by which to estimate bias of this method.

TEST METHOD B—CARBON-13 NMR

15. Apparatus

15.1 **High Resolution Fourier-Transform NMR Spectrometer**, with carbon-13 capability, and a carbon-13 resonance frequency of 50 MHz (proton resonance frequency of 200 MHz) or higher. The spectrometer is to have a minimum carbon-13 signal-to-noise ratio of 70:1 based on the benzene carbon signal in 60 % benzene-d₆, 40 % p-dioxane (v/v) sample (ASTM NMR standard) that has been pulsed once using a 90° pulse angle under the conditions described in Practice **E2977**.

15.2 **NMR sample tubes**, having outside diameters of 5 mm or more.

15.3 **NMR spinners**.

16. Reagents and Materials

16.1 All reagents are to be spectroscopic grade and free of magnetic materials.

16.1.1 **Deuterated acetone**, containing tetramethylsilane (TMS) as an internal standard.