



Designation: C1156 – 18

Standard Guide for Establishing Calibration for a Measurement Method Used to Analyze Nuclear Fuel Cycle Materials¹

This standard is issued under the fixed designation C1156; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

1. Scope

1.1 This guide provides the basis for establishing calibration for a measurement method typically used in an analytical chemistry laboratory analyzing nuclear materials. Guidance is included for such activities as preparing a calibration procedure, selecting a calibration standard, controlling calibrated equipment, and documenting calibration. The guide is generic and any required technical information specific for a given method must be obtained from other sources.

1.2 The guidance information is provided in the following sections:

General Considerations	5
Calibration Procedure	6
Calibration Standard	7
Control of Calibrated Equipment	8
Documentation	9
Keywords	10

1.3 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety, health, and environmental practices and determine the applicability of regulatory limitations prior to use.*

1.4 *This international standard was developed in accordance with internationally recognized principles on standardization established in the Decision on Principles for the Development of International Standards, Guides and Recommendations issued by the World Trade Organization Technical Barriers to Trade (TBT) Committee.*

2. Referenced Documents

2.1 ASTM Standards:²

[C859 Terminology Relating to Nuclear Materials](#)

¹ This guide is under the jurisdiction of ASTM Committee C26 on Nuclear Fuel Cycle and is the direct responsibility of Subcommittee C26.08 on Quality Assurance, Statistical Applications, and Reference Materials

Current edition approved Sept. 1, 2018. Published October 2018. Originally approved in 1990. Last previous edition approved in 2011 as C1156 – 03 (2011). DOI: 10.1520/C1156-18.

² For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

[C1009 Guide for Establishing and Maintaining a Quality Assurance Program for Analytical Laboratories Within the Nuclear Industry](#)

[C1068 Guide for Qualification of Measurement Methods by a Laboratory Within the Nuclear Industry](#)

[C1128 Guide for Preparation of Working Reference Materials for Use in Analysis of Nuclear Fuel Cycle Materials](#)

[C1210 Guide for Establishing a Measurement System Quality Control Program for Analytical Chemistry Laboratories Within the Nuclear Industry](#)

[C1215 Guide for Preparing and Interpreting Precision and Bias Statements in Test Method Standards Used in the Nuclear Industry](#)

[C1297 Guide for Qualification of Laboratory Analysts for the Analysis of Nuclear Fuel Cycle Materials](#)

2.2 ISO Standard:

[ISO/IEC 17025 General Requirements for the Competence of Testing and Calibration Laboratories³](#)

3. Terminology

3.1 For definitions of terms used in this guide but not defined herein, refer to Terminology [C859](#).

4. Significance and Use

4.1 Calibration is a fundamental part of making measurements and its effect on the quality of measurement data is significant. Thus, sufficient attention must be given to calibration when it is established for a measurement method so that the data produced will be acceptable. The use of an inappropriate calibration standard, inadequate instructions for calibration, and poor documentation of the calibration process are examples of circumstances that can adversely affect the validity of a calibration. Thus, the calibration process must conform to criteria established to ensure the validity of calibration results and any associated measurement data. Such criteria are given in Guide [C1009](#), in which calibration is identified as a component of laboratory quality assurance (see [Fig. 1](#)). This guide expands upon those criteria to provide more comprehensive guidance for establishing calibration.

³ Available from American National Standards Institute (ANSI), 25 W. 43rd St., 4th Floor, New York, NY 10036, <http://www.ansi.org>.

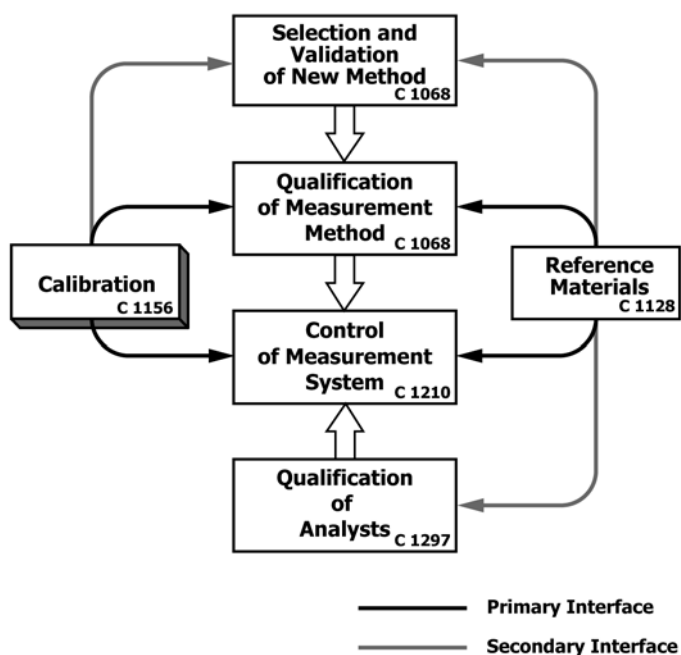


FIG. 1 Quality Assurance of Analytical Laboratory Data

4.2 The manner of calibration and other technical requirements for calibrating a measurement method are usually established when a method is first introduced into a laboratory, which may be through validation and qualification as defined by Guide C1068 (see Fig. 1). However, calibration involves more than the technical aspects of the calibration process. The other dimension of the process is the operational requirements that are necessary to ensure that calibration results are valid and that they are documented and verifiable should their integrity be questioned. The provisions of this guide provide those operational requirements and should be considered whenever calibration is planned and established.

5. General Considerations

5.1 The degree of attention and effort given to calibration should depend on how the measurement data are to be used. In the analysis of nuclear materials, for example, measurement data produced for the control and accountability of nuclear material would normally require more attention than data produced for process control during the processing of that material. The areas in which the level of attention and effort could vary are: the calibration standard, number of calibration points, calibration acceptance criteria, frequency of calibration, and frequency of calibration verification.

5.2 Many of the provisions of this guide would not apply to the calibration of certain instruments when their calibration is an integral part of the analysis procedure involving a simple one- or two-step adjustment of a meter or gage. The pH meter is an example when a buffer is used to calibrate the meter just before a pH reading is taken for a sample solution.

5.3 There are generally two approaches regarding frequency of calibration. In one case, the method is calibrated each time it is used. In the other, calibration is established for a specified period of time, and the method must be recalibrated before that

time period elapses to retain calibration. When a calibration period is used, calibration verification should be used. A calibration period might be defined in terms of weeks or months, or defined as a run of a series of samples over a relatively short period of time. In the latter case, calibration verification could involve analyzing a standard periodically during the sample run, for example, after every fifth sample.

5.4 Under no circumstances it is justifiable to use the results of a calibration verification to adjust a pre-existing calibration. More information regarding measurement control may be found in Guide C1210.

5.5 When calibration is being planned and established, a statistician should be consulted regarding the treatment of calibration data, the frequency of calibration, the frequency of calibration checks, and the criteria that determine when calibration has been achieved (see Guide C1215). This is to ensure that the calibration procedure is appropriate for the method and that the uncertainty estimate for the method (as determined during validation or qualification) remains valid.

5.6 The organizational responsibility and authority for calibration should be defined and documented. Normally, responsibility for calibrating an individual method rests with the analyst using the method. If the responsibility for calibrating an instrument or class of instruments is contracted to another organization, the laboratory is still responsible for ensuring that calibration requirements are being met by the organization doing the calibration.

6. Calibration Procedure

6.1 Calibration should be established as a written procedure. The procedure should provide instructions for those performing the calibration, and it should document the basis for calibration, which can be used to substantiate the validity of the calibration process, should that be required.

6.2 *Preparation*—The calibration procedure can be prepared as a separate procedure from the one written for the measurement method or it can be a section of the method’s procedure as long as the provisions given in 6.3 are addressed. If the former approach is used, the applicable measurement method should be clearly identified in the calibration procedure. The calibration procedure should be reviewed for technical adequacy and approved by the appropriate level of management. The provisions contained in the Procedure section of Guide C1009 regarding the preparation, review, and approval of procedures should be considered. Also, calibration procedures should be revised, distributed, and controlled according to the provisions in the Procedure section of Guide C1009.

6.3 *Content*—The following subjects should be addressed in the procedure:

6.3.1 Identification of the equipment or portion of the measurement apparatus that requires calibration,

6.3.2 Description of the calibration standard or standards that will be used and inclusion of instructions for the preparation, pretreatment, and use of the standard(s) as appropriate;