



Designation: F2516 – 18

# Standard Test Method for Tension Testing of Nickel-Titanium Superelastic Materials<sup>1</sup>

This standard is issued under the fixed designation F2516; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reappraisal. A superscript epsilon ( $\epsilon$ ) indicates an editorial change since the last revision or reappraisal.

## 1. Scope

1.1 This test method covers the tension testing of superelastic nickel-titanium (nitinol) materials, specifically the methods for determination of upper plateau strength, lower plateau strength, residual elongation, tensile strength, and elongation.

1.2 The values stated in SI units are to be regarded as standard. No other units of measurement are included in this standard.

1.3 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety, health, and environmental practices and determine the applicability of regulatory limitations prior to use.*

1.4 *This international standard was developed in accordance with internationally recognized principles on standardization established in the Decision on Principles for the Development of International Standards, Guides and Recommendations issued by the World Trade Organization Technical Barriers to Trade (TBT) Committee.*

## 2. Referenced Documents

2.1 *ASTM Standards:*<sup>2</sup>

**E6 Terminology Relating to Methods of Mechanical Testing**  
**E8/E8M Test Methods for Tension Testing of Metallic Materials**

**E83 Practice for Verification and Classification of Extensometer Systems**

**E111 Test Method for Young's Modulus, Tangent Modulus, and Chord Modulus**

**E177 Practice for Use of the Terms Precision and Bias in ASTM Test Methods**

**E691 Practice for Conducting an Interlaboratory Study to Determine the Precision of a Test Method**

<sup>1</sup> This test method is under the jurisdiction of ASTM Committee F04 on Medical and Surgical Materials and Devices and is the direct responsibility of Subcommittee F04.15 on Material Test Methods.

Current edition approved Oct. 1, 2018. Published October 2018. Originally approved in 2005. Last previous edition approved in 2014 as F2516 – 14. DOI: 10.1520/F2516-18.

<sup>2</sup> For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

**E1876 Test Method for Dynamic Young's Modulus, Shear Modulus, and Poisson's Ratio by Impulse Excitation of Vibration**

**E3098 Test Method for Mechanical Uniaxial Pre-strain and Thermal Free Recovery of Shape Memory Alloys**

**F2004 Test Method for Transformation Temperature of Nickel-Titanium Alloys by Thermal Analysis**

**F2005 Terminology for Nickel-Titanium Shape Memory Alloys**

**F2082/F2082M Test Method for Determination of Transformation Temperature of Nickel-Titanium Shape Memory Alloys by Bend and Free Recovery**

## 3. Terminology

3.1 The definitions of terms relating to tension testing appearing in Terminology **E6** and the terms relating to nickel-titanium shape memory alloys appearing in Terminology **F2005** shall be considered as applying to the terms used in this test method. Engineering stress and strain are assumed unless otherwise noted. Additional terms being defined are as follows (see Fig. 1):

3.2 *Definitions:*

3.2.1 *alignment stress, n*—stress (not to exceed 7 MPa) applied to the specimen after it is installed in the grips to ensure that the specimen is straight and aligned to the grips.

3.2.2 *elongation at fracture (El<sub>F</sub>), n*—elongation measured just prior to the sudden decrease in force associated with fracture. See Fig. 1 and X1.2. **E6**

3.2.2.1 *Discussion*—Elongation at fracture results may be very sensitive to test variables such as test speed, specimen geometry, heat dissipation, surface finish, and alignment. See Test Methods **E8/E8M**.

3.2.2.2 *Discussion*—Corrections for non-uniform strains between the extensometer attachments, including in the necked region, are beyond the scope of this standard. See Test Methods **E8/E8M**.

3.2.3 *fracture ductility (ε<sub>f</sub>), n*—true plastic strain at fracture. See X1.2. **E6**

3.2.3.1 *Discussion*—For prismatic specimens, the fracture ductility is calculated as follows:

$$\epsilon_f = \ln\left(\frac{A_o}{A_f}\right) = \ln\left(\frac{1}{1 - RA\%/100}\right) \quad (1)$$

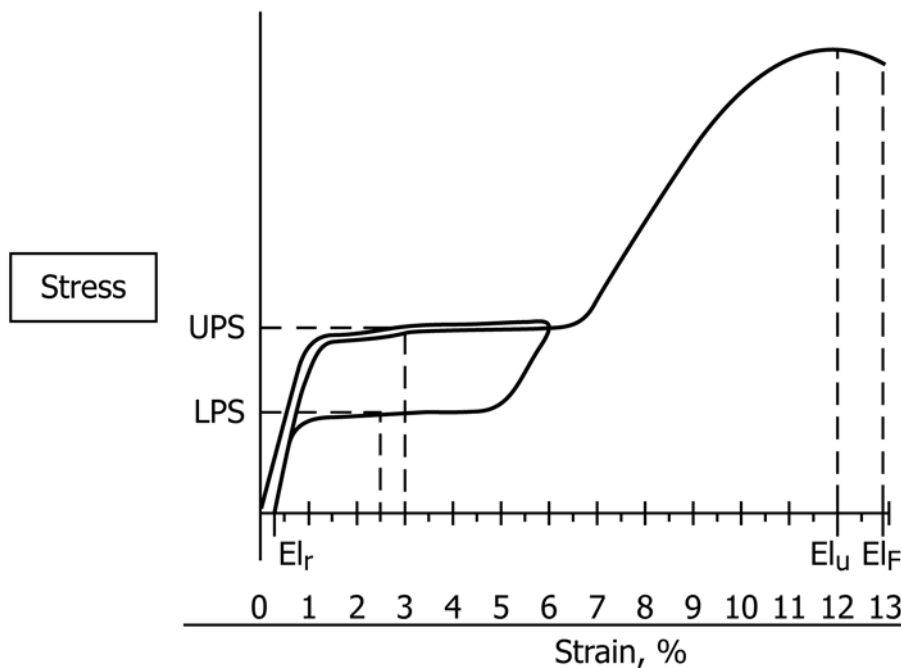


FIG. 1 Terms Illustrated on Typical Stress-Strain Diagram of Superelastic Nitinol

where:

- $A_o$  = original cross-sectional area,
- $A_f$  = area at fracture of its smallest cross section after testing, and
- RA% = reduction of area, %. See Terminology E6.

3.2.4 lower plateau strength (LPS),  $n$ —stress at 2.5 % strain during unloading of the sample, after loading to 6 % strain. See Fig. 1. E6

3.2.5 reduction of area percent (RA%),  $n$ —percent difference between the original cross-sectional area of a tension test specimen and the area of its smallest cross section after fracture.

3.2.5.1 Discussion—When the specimen necks prior to fracture, reduction in area provides a measure of the material ductility. The reduction of area of a prismatic specimen is calculated using the difference in the original cross-sectional area,  $A_o$ , of a specimen and the area at fracture of its smallest cross section,  $A_f$ , after testing as follows:

$$RA\% = 100\% \frac{A_o - A_f}{A_o} \quad (2)$$

3.2.5.2 Discussion—For measuring a specimen's  $A_f$  with an original circular or rectangular cross sections, see Test Methods E8/E8M, Section 7.12.

3.2.6 residual elongation,  $El_r$ , %—difference between the strain at a set stress at or between the alignment stress and a maximum of 7 MPa during unloading and the strain at that same set stress during the initial loading. See Fig. 1 and X1.4.

3.2.7 uniform elongation,  $El_u$ , %—elongation determined at the maximum force sustained by the test piece just prior to necking, or fracture, or both. See Fig. 1.

3.2.7.1 Discussion—Uniform elongation is not an accurate measure of ductility. See X1.2.

3.2.8 upper plateau strength (UPS)—stress at 3 % strain during loading of the sample. See Fig. 1. E6

#### 4. Summary of Test Method

4.1 Using conventional tensile testing apparatus, the material is pulled to 6 % strain, then unloaded to less than 7 MPa, then pulled to failure.

#### 5. Significance and Use

5.1 Tension tests provide information on the strength and the elastic and plastic properties of materials under uniaxial tensile stresses.

5.2 Tension tests, as described in this test method, also provide information on the superelasticity, as defined in Terminology F2005, of the material at the test temperature.

#### 6. Apparatus

6.1 Apparatus is as described in Test Methods E8/E8M.

#### 7. Test Specimen

7.1 Test specimens are as described in Test Methods E8/E8M.

#### 8. Procedure

8.1 Procedure shall be per Test Methods E8/E8M with the following additions:

8.1.1 The material should be tested at a temperature that is a minimum of 5°C above the austenitic finish transformation temperature ( $A_f$ ) in order to prevent testing of a partially transformed material. The temperature of the test should be  $22.0 \pm 2.0^\circ\text{C}$  or  $37 \pm 2.0^\circ\text{C}$ , unless otherwise specified. See Terminology F2005 for the definition of  $A_f$ . See Test Methods F2004, F2082/F2082M, and E3098 to determine  $A_f$ .

8.1.2 The free-running crosshead speed shall be limited per **Table 1**. See **X1.3**.

8.1.3 The test shall consist of zeroing the test machine per Test Method **E8/E8M**, gripping the specimen, loading the specimen to the alignment stress, pulling the specimen to 6 % strain, reversing the motion to unload the specimen to the alignment stress, and then pulling the specimen to failure. See **X1.4**.

8.1.4 For materials with diameter greater than 0.2 mm, strain shall be determined by use of a calibrated extensometer of class C or better (see Practice **E83**). For materials with diameter less than or equal to 0.2 mm, strain may be determined by use of an extensometer or by crosshead motion. When using crosshead motion to calculate strain, the length between the grips shall be a minimum of 150 mm. See **X1.5**.

**NOTE 1**—Strain should be measured using extensometer versus crosshead displacement as this will result in a more accurate measurement of strain.

8.1.4.1 When using a clip-on extensometer with small-diameter wire, care shall be taken not to bend or distort the wire when attaching the extensometer.

8.1.5 Upper plateau strength shall be determined as the value of the stress at a strain of 3.0 % during the initial loading of the specimen.

8.1.6 Lower plateau strength shall be determined as the value of the stress at a strain of 2.5 % during the unloading of the specimen.

8.1.7 Residual elongation shall be determined by the difference between the strain at a set stress at or between the alignment stress and a maximum of 7 MPa during unloading and the strain at that same set stress during the initial loading.

8.1.8 The uniform elongation shall be determined by elongation when the maximum force is reached just prior to necking or fracture, or both.

8.1.9 The elongation at fracture shall be determined by elongation measured just prior to the sudden decrease in force associated with fracture.

## 9. Report

9.1 The report shall include the following information, unless otherwise specified:

- 9.1.1 Material and sample identification,
- 9.1.2 Specimen type,
- 9.1.3 Upper plateau strength,
- 9.1.4 Lower plateau strength,
- 9.1.5 Residual elongation,
- 9.1.6 Tensile strength,
- 9.1.7 Uniform elongation, if required,
- 9.1.8 Elongation at fracture,
- 9.1.9 Test temperature,
- 9.1.10 Strain determination method (extensometer or crosshead),
- 9.1.11 Crosshead speed, and
- 9.1.12 Gage length (length of reduced section or distance between grips for specimens not having reduced sections).

## 10. Precision and Bias<sup>3</sup>

10.1 An interlaboratory study was conducted in accordance with Practice **E691** using three different diameters of superelastic wire. For wire diameters of 0.2 and 0.5 mm, eleven laboratories participated in the study with each laboratory obtaining three results for each diameter. For the 2.5 mm diameter wire, eight laboratories participated in the study with each laboratory obtaining three results. The details are given in ASTM Research Report RR:F04-1010.<sup>3</sup>

10.2 The results are summarized in **Tables 2-6** for each tensile parameter. The terms *repeatability limit* and *reproducibility limit* are used as specified in Practice **E177**.<sup>8</sup>

10.3 No measurement of bias is possible with this test method since there is presently no accepted reference material.

## 11. Keywords

11.1 lower plateau strength; nickel titanium; nitinol; residual elongation; shape memory; superelasticity; upper plateau strength

**TABLE 1 Crosshead Speed Limits**

<i>d</i> , diameter or thickness (mm) <sup>A</sup>	Maximum crosshead speed in mm/min per mm of initial length of reduced section (or initial distance between grips for specimens not having reduced sections)	
	First Cycle (load to 6 % strain and unload)	Second Cycle (load to failure)
$d \leq 0.2$	0.08	0.8
$0.2 < d \leq 0.5$	0.04	0.4
$0.5 < d \leq 2.5$	0.02	0.2
$d > 2.5$	0.01	0.1

<sup>A</sup> For tubing, use *d* that gives an equivalent surface area to diameter ratio; for round tubing,  $d = (\text{outer diameter}) - (\text{inner diameter})$ .

<sup>3</sup> Supporting data have been filed at ASTM International Headquarters and may be obtained by requesting Research Report RR:F04-1010.

**TABLE 2 Precision of Upper Plateau Strength (MPa)**

Diameter (mm)	Grand Mean	Repeatability Standard Deviation	Reproducibility Standard Deviation	Repeatability Limit	Reproducibility Limit
0.2	499	13	55	36	154
0.5	492	11	35	30	98
2.5	500	13	25	35	71

**TABLE 3 Precision of Lower Plateau Strength (MPa)**

Diameter (mm)	Grand Mean	Repeatability Standard Deviation	Reproducibility Standard Deviation	Repeatability Limit	Reproducibility Limit
0.2	196	10	35	27	97
0.5	146	9	27	26	75
2.5	138	13	19	36	52

**TABLE 4 Precision of Residual Elongation (%)**

Diameter (mm)	Grand Mean	Repeatability Standard Deviation	Reproducibility Standard Deviation	Repeatability Limit	Reproducibility Limit
0.2	0.11	0.09	0.13	0.24	0.36
0.5	0.07	0.03	0.04	0.09	0.10
2.5	0.11	0.05	0.12	0.13	0.33

**TABLE 5 Precision of Ultimate Tensile Strength (%)**

Diameter (mm)	Grand Mean	Repeatability Standard Deviation	Reproducibility Standard Deviation	Repeatability Limit	Reproducibility Limit
0.2	1459	45	135	125	377
0.5	1325	23	43	65	120
2.5	1268	15	15	42	41

**TABLE 6 Precision of Uniform Elongation (%)**

Diameter (mm)	Grand Mean	Repeatability Standard Deviation	Reproducibility Standard Deviation	Repeatability Limit	Reproducibility Limit
0.2	11.5	0.7	1.2	2.0	3.5
0.5	12.4	0.4	1.0	1.3	2.8
2.5	13.3	0.6	0.7	1.8	1.9

[ASTM F2516-18](https://standards.iteh.ai/catalog/standards/sist/f723e6f2-5028-44d3-9404-31aefe35dec3/astm-f2516-18)

<https://standards.iteh.ai/catalog/standards/sist/f723e6f2-5028-44d3-9404-31aefe35dec3/astm-f2516-18>

## APPENDIXES

### (Nonmandatory Information)

#### X1. RATIONALE

X1.1 Measurement of modulus of elasticity requires very precise measurements beyond the scope of this test method. Test Methods **E111** and **E1876** address determination of modulus of elasticity. For superelastic nitinol, the dynamic method (Test Method **E1876**) is preferred. Note that the modulus of elasticity exhibits large variation with the martensitic transformation **(1)**.<sup>4</sup>

X1.2 Tensile loading of nickel-titanium superelastic materials to fracture will generally encompass elastic strains, phase transformation strains, martensite reorientation strains (twining) and plastic strains **(2)**. Tensile loading following plastic yielding and the accompanying drop in tangent modulus,

usually results in an instability that localizes the highest stress into a narrowed neck region and ends in fracture. The Uniform Elongation measurement, which is determined at the onset of necking, is not an accurate measure of ductility. However, Uniform Elongation can be useful as a process control measure. Elongation at Fracture provides an overall elongation value that includes elongation between the extensometer attachment points, including the necking elongation, but is dependent on the gage length and underestimates the strain in the necked fracture region. Conventionally, Reduction of Area and Fracture Ductility are used to estimate the high strains in the necked region. They are interpreted as measures of material ductility, the ability of a material to deform plastically before fracturing (see Terminology **E6**). In addition, by measuring the longitudinal shape of the neck, an estimate of the true stress at

<sup>4</sup> The boldface numbers in parentheses refer to a list of references at the end of this standard.