



Designation: **F2516 – 14** **F2516 – 18**

# Standard Test Method for Tension Testing of Nickel-Titanium Superelastic Materials<sup>1</sup>

This standard is issued under the fixed designation F2516; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reappraisal. A superscript epsilon ( $\epsilon$ ) indicates an editorial change since the last revision or reappraisal.

## 1. Scope

1.1 This test method covers the tension testing of superelastic nickel-titanium (nitinol) materials, specifically the methods for determination of upper plateau strength, lower plateau strength, residual elongation, tensile strength, and elongation.

1.2 The values stated in SI units are to be regarded as standard. No other units of measurement are included in this standard.

1.3 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety, health, and environmental practices and determine the applicability of regulatory limitations prior to use.*

1.4 *This international standard was developed in accordance with internationally recognized principles on standardization established in the Decision on Principles for the Development of International Standards, Guides and Recommendations issued by the World Trade Organization Technical Barriers to Trade (TBT) Committee.*

## 2. Referenced Documents

2.1 *ASTM Standards:*<sup>2</sup>

[E6 Terminology Relating to Methods of Mechanical Testing](#)

[E8E8/E8M Test Methods for Tension Testing of Metallic Materials \[Metric\] E0008\\_E0008M](#)

[E83 Practice for Verification and Classification of Extensometer Systems](#)

[E111 Test Method for Young's Modulus, Tangent Modulus, and Chord Modulus](#)

[E177 Practice for Use of the Terms Precision and Bias in ASTM Test Methods](#)

[E691 Practice for Conducting an Interlaboratory Study to Determine the Precision of a Test Method](#)

[E1876 Test Method for Dynamic Young's Modulus, Shear Modulus, and Poisson's Ratio by Impulse Excitation of Vibration](#)

[E3098 Test Method for Mechanical Uniaxial Pre-strain and Thermal Free Recovery of Shape Memory Alloys](#)

[F2004 Test Method for Transformation Temperature of Nickel-Titanium Alloys by Thermal Analysis](#)

[F2005 Terminology for Nickel-Titanium Shape Memory Alloys](#)

[F2082/F2082M Test Method for Determination of Transformation Temperature of Nickel-Titanium Shape Memory Alloys by Bend and Free Recovery](#)

## 3. Terminology

3.1 The definitions of terms relating to tension testing appearing in Terminology [E6](#) and the terms relating to nickel-titanium shape memory alloys appearing in Terminology [F2005](#) shall be considered as applying to the terms used in this test method. Engineering stress and strain are assumed unless otherwise noted. Additional terms being defined are as follows (see [Fig. 1](#)):

3.2 *Definitions:*

3.2.1 *alignment stress,  $n$* —stress (not to exceed 7 MPa) applied to the specimen after it is installed in the grips to ensure that the specimen is straight and aligned to the grips.

3.2.2 *elongation at fracture ( $El_F$ ),  $n$* —elongation measured just prior to the sudden decrease in force associated with fracture. See [Fig. 1](#) and [X1.2](#). **E6**

3.2.2.1 *Discussion—*

<sup>1</sup> This test method is under the jurisdiction of ASTM Committee [F04](#) on Medical and Surgical Materials and Devices and is the direct responsibility of Subcommittee [F04.15](#) on Material Test Methods.

Current edition approved Oct. 1, 2014. Published February 2015. Originally approved in 2005. Last previous edition approved in 2007 as [F2516 – 07](#)/[F2516 – 14](#). DOI: [10.1520/F2516-14](#).[10.1520/F2516-18](#).

<sup>2</sup> For referenced ASTM standards, visit the ASTM website, [www.astm.org](#), or contact ASTM Customer Service at [service@astm.org](#). For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

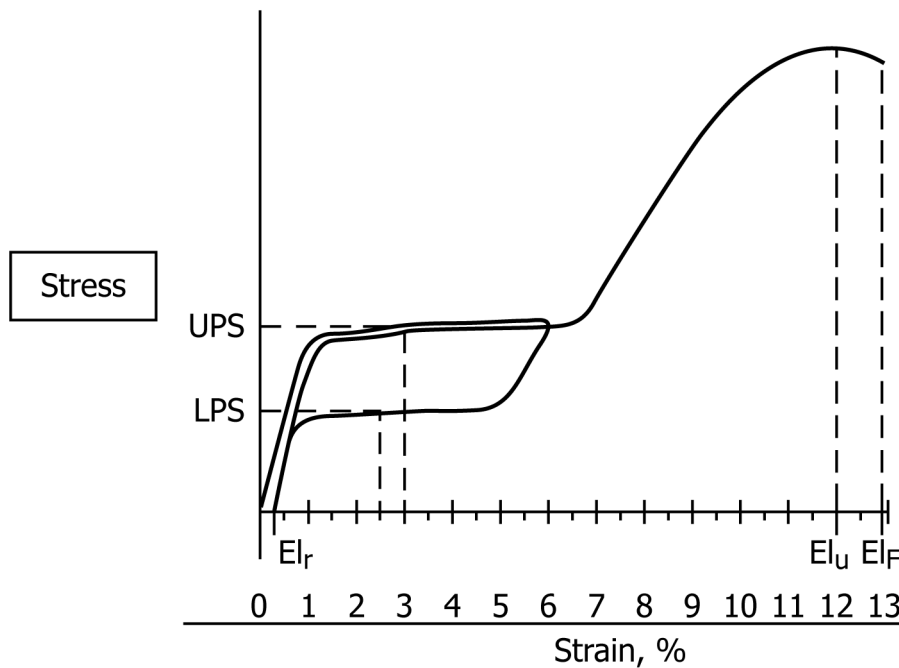


FIG. 1 Terms Illustrated on Typical Stress-Strain Diagram of Superelastic Nitinol

Elongation at fracture results may be very sensitive to test variables such as test speed, specimen geometry, heat dissipation, surface finish, and alignment. See Test Methods E8/E8M.

3.2.2.2 Discussion—

Corrections for non-uniform strains between the extensometer attachments, including in the necked region, are beyond the scope of this standard. See Test Methods E8/E8M.

3.2.3 fracture ductility ( $\epsilon_f$ ),  $n$ —true plastic strain at fracture. See X1.2. E6

3.2.3.1 Discussion—

For prismatic specimens, the fracture ductility is calculated as follows:

$$\epsilon_f = \ln\left(\frac{A_o}{A_f}\right) = \ln\left(\frac{1}{1 - RA\%/100}\right) \tag{1}$$

where:

- $A_o$  = original cross-sectional area,
- $A_f$  = area at fracture of its smallest cross section after testing, and
- $RA\%$  = reduction of area, %. See Terminology E6.

3.2.4 lower plateau strength (LPS)—(LPS),  $n$ —the stress at 2.5 % strain during unloading of the sample, after loading to 6 % strain. See Fig. 1. E6

3.2.5 reduction of area percent (RA%),  $n$ —percent difference between the original cross-sectional area of a tension test specimen and the area of its smallest cross section after fracture.

3.2.5.1 Discussion—

When the specimen necks prior to fracture, reduction in area provides a measure of the material ductility. The reduction of area of a prismatic specimen is calculated using the difference in the original cross-sectional area,  $A_o$ , of a specimen and the area at fracture of its smallest cross section,  $A_f$ , after testing as follows:

$$RA\% = 100\% \frac{A_o - A_f}{A_o} \tag{2}$$

### 3.2.5.2 Discussion—

For measuring a specimen's  $A_f$  with an original circular or rectangular cross sections, see Test Methods [E8/E8M](#), Section 7.12.

3.2.6 *residual elongation,  $El_{r1}$  [%]*—~~the difference between the strain at a stress of 7.0 MPa set stress at or between the alignment stress and a maximum of 7 MPa during unloading and the strain at a stress of 7.0 MPa during loading, that same set stress during the initial loading.~~ See [Fig. 1](#) and [X1.4](#).

3.2.7 *uniform elongation,  $El_{u1}$  [%]*—~~the elongation determined at the maximum force sustained by the test piece just prior to necking, or fracture, or both.~~ See [Fig. 1](#).

### 3.2.7.1 Discussion—

Uniform elongation is not an accurate measure of ductility. See [X1.2](#).

3.2.8 *upper plateau strength (UPS)*—~~the stress at 3 % strain during loading of the sample.~~ See [Fig. 1](#). **E6**

## 4. Summary of Test Method

4.1 Using conventional tensile testing apparatus, the material is pulled to 6 % strain, then unloaded to less than 7 MPa, then pulled to failure.

## 5. Significance and Use

5.1 Tension tests provide information on the strength and ductility ~~the elastic and plastic properties~~ of materials under uniaxial tensile stresses.

5.2 Tension tests, as described in this test method, also provide information on the superelasticity, as defined in Terminology [F2005](#), of the material at the test temperature.

## 6. Apparatus

6.1 Apparatus is as described in Test Methods [E8E8/E8M](#).

## 7. Test Specimen

7.1 Test specimens are as described in Test Methods [E8E8/E8M](#).

## 8. Procedure

8.1 Procedure shall be per Test Methods [E8E8/E8M](#) with the following additions:

8.1.1 Unless otherwise specified, the temperature of the test shall be  $22.0 \pm 2.0^\circ\text{C}$ . It is recommended that the material ~~the material should~~ be tested at a temperature that is a minimum of  $5^\circ\text{C}$  above the austenitic finish transformation temperature ( $A_f$ ) in order to prevent testing of a partially transformed material. ~~The temperature of the test should be  $22.0 \pm 2.0^\circ\text{C}$  or  $37 \pm 2.0^\circ\text{C}$ , unless otherwise specified.~~ See Terminology [F2005](#) for the definition of  $A_f$ . See Test Methods [F2004](#), [F2082/F2082M](#), and [E3098](#) to determine  $A_f$ .

8.1.2 The free-running crosshead speed shall be limited per [Table 1](#). See [X1.3](#).

8.1.3 The test shall consist of zeroing the ~~force transducer, test machine~~ per Test Method [E8/E8M](#), gripping the specimen, ~~loading the specimen to the alignment stress, pulling the specimen to 6 % strain, reversing the motion to unload the specimen to less than 7 MPa, the alignment stress,~~ and then pulling the specimen to failure. See [X1.4](#).

**TABLE 1 Crosshead Speed Limits**

$d$ , diameter or thickness (mm) <sup>A</sup>	Maximum crosshead speed in mm/min per mm of initial length of reduced section (or initial distance between grips for specimens not having reduced sections)	
	First Cycle (load to 6 % strain and unload)	Second Cycle (load to failure)
$d \leq 0.2$	0.08	0.8
$0.2 < d \leq 0.5$	0.04	0.4
$0.5 < d \leq 2.5$	0.02	0.2
$d > 2.5$	0.01	0.1

<sup>A</sup> For tubing, use  $d$  that gives an equivalent surface area to diameter ratio; for round tubing,  $d = (\text{outer diameter}) - (\text{inner diameter})$ .

8.1.4 For materials with diameter greater than 0.2 mm, strain shall be determined by use of a calibrated extensometer of class C or better (see Practice E83). For materials with diameter less than or equal to 0.2 mm, strain may be determined by use of an extensometer or by crosshead motion. When using crosshead motion to calculate strain, the length between the grips ~~must be~~ shall be a minimum of 150 mm. See X1.5.

NOTE 1—~~It is recommended that strain~~ Strain should be measured using extensometer versus crosshead displacement as this will result in a more accurate measurement of strain.

8.1.4.1 When using a clip-on extensometer with small-diameter wire, care ~~must~~ shall be taken not to bend or distort the wire when attaching the extensometer.

8.1.5 Upper plateau strength shall be determined as the value of the stress at a strain of 3.0 % during the initial loading of the specimen.

8.1.6 Lower plateau strength shall be determined as the value of the stress at a strain of 2.5 % during the unloading of the specimen.

8.1.7 Residual elongation shall be determined by the difference between the strain at a ~~stress of 7.0 set stress~~ stress at or between the alignment stress and a maximum of 7 MPa during unloading and the strain at a ~~stress of 7.0 MPa during~~ that same set stress during the initial loading.

8.1.8 The uniform elongation shall be determined by elongation when the maximum force is reached just prior to necking or fracture, or both.

8.1.9 The elongation at fracture shall be determined by elongation measured just prior to the sudden decrease in force associated with fracture.

## 9. Report

9.1 The report shall include the following information, unless otherwise specified:

9.1.1 Material and sample identification,

9.1.2 Specimen type,

9.1.3 Upper plateau strength,

9.1.4 Lower plateau strength,

9.1.5 Residual elongation,

9.1.6 Tensile strength,

9.1.7 Uniform elongation, if required,

9.1.8 Elongation at fracture,

9.1.9 Test temperature,

9.1.10 Strain determination method (extensometer or crosshead),

9.1.11 Crosshead speed, and

9.1.12 Gage length (length of reduced section or distance between grips for specimens not having reduced sections).

## 10. Precision and Bias<sup>3</sup>

10.1 An interlaboratory study was conducted in accordance with Practice E691 using three different diameters of superelastic wire. For wire diameters of 0.2 and 0.5 mm, eleven laboratories participated in the study with each laboratory obtaining three results for each diameter. For the 2.5 mm diameter wire, eight laboratories participated in the study with each laboratory obtaining three results. The details are given in ASTM Research Report RR:F04-1010.<sup>3</sup>

10.2 The results are summarized in Tables 2-6 for each tensile parameter. The terms *repeatability limit* and *reproducibility limit* are used as specified in Practice E177.

10.3 No measurement of bias is possible with this test method since there is presently no accepted reference material.

## 11. Keywords

11.1 lower plateau strength; nickel titanium; nitinol; residual elongation; shape memory; superelasticity; upper plateau strength

**TABLE 2 Precision of Upper Plateau Strength (MPa)**

Diameter (mm)	Grand Mean	Repeatability Standard Deviation	Reproducibility Standard Deviation	Repeatability Limit	Reproducibility Limit
0.2	499	13	55	36	154
0.5	492	11	35	30	98
2.5	500	13	25	35	71

<sup>3</sup> Supporting data have been filed at ASTM International Headquarters and may be obtained by requesting Research Report RR:F04-1010.