



Designation: D5594 – 18a

Standard Test Method for Determination of the Vinyl Acetate Content of Ethylene-Vinyl Acetate (EVA) Copolymers by Fourier Transform Infrared Spectroscopy (FT-IR)¹

This standard is issued under the fixed designation D5594; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

1. Scope*

1.1 This test method covers infrared procedures for determining the vinyl acetate content of EVA copolymers using pressed films (Procedure A) or molded plaques (Procedure B) and internal corrections for sample thickness.

1.2 This test method is applicable to the analysis of EVA copolymers containing 0.5 to 55 % vinyl acetate except as specified in 1.3.

1.3 Talc interferes with the 1020 cm^{-1} vinyl acetate band. Resins containing <5 % vinyl acetate and talc are excluded from the scope of this test method.

1.4 The values stated in SI units are to be regarded as the standard. The values given in parentheses are provided for information purposes only.

1.5 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety, health, and environmental practices and determine the applicability of regulatory limitations prior to use. Specific precautionary statements are given in Section 8.*

NOTE 1—There is no known ISO equivalent to this standard.

1.6 *This international standard was developed in accordance with internationally recognized principles on standardization established in the Decision on Principles for the Development of International Standards, Guides and Recommendations issued by the World Trade Organization Technical Barriers to Trade (TBT) Committee.*

2. Referenced Documents

2.1 *ASTM Standards:*²

[E131 Terminology Relating to Molecular Spectroscopy](#)

¹ This test method is under the jurisdiction of ASTM Committee D20 on Plastics and is the direct responsibility of Subcommittee D20.70 on Analytical Methods.

Current edition approved Nov. 1, 2018. Published November 2018. Originally approved in 1994. Last previous edition approved in 2018 as D5594 - 18. DOI: 10.1520/D5594-18A.

² For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

[E168 Practices for General Techniques of Infrared Quantitative Analysis](#)

[E177 Practice for Use of the Terms Precision and Bias in ASTM Test Methods](#)

[E691 Practice for Conducting an Interlaboratory Study to Determine the Precision of a Test Method](#)

[IEEE/ASTM SI-10 Use of the International System of Units \(SI\): The Modern Metric System](#)

[E691 Practice for Conducting an Interlaboratory Study to Determine the Precision of a Test Method](#)

2.2 *ISO Standard:*

[ISO 8985 Plastics—Ethylene/Vinyl Acetate Copolymer Thermoplastics—Determination of Vinyl Acetate](#)³

3. Terminology

3.1 *Definitions:*

3.1.1 Units, symbols, and abbreviations used in this test method appear in Terminology [E131](#) or [IEEE/ASTM SI-10](#).

3.2 *Abbreviations:*

3.2.1 *EVA*—ethylene-vinyl acetate copolymer.

3.2.2 *PTFE*—tetrafluorethylene polymer.

3.2.3 *FT-IR*—Fourier transform infrared.

4. Summary of Test Method

4.1 The vinyl acetate content is measured using infrared absorption band at 1020 cm^{-1} (0.5 to 5 % vinyl acetate) or 609 cm^{-1} (5 to 55 % vinyl acetate).

4.2 Sample thickness is measured internally using an ethylene infrared absorption band at 720 cm^{-1} (28 to 55 % vinyl acetate), 2020 cm^{-1} (0.5 to 28 % vinyl acetate), or 4250 cm^{-1} (5 to 28 % vinyl acetate).

4.3 Regression analysis is performed on vinyl acetate/ethylene ratios versus known vinyl acetate contents for EVA copolymer standards. The resulting equation is used to calculate the vinyl acetate content for subsequent EVA copolymer samples.

³ Available from American National Standards Institute (ANSI), 25 W. 43rd St., 4th Floor, New York, NY 10036, <http://www.ansi.org>.

*A Summary of Changes section appears at the end of this standard

5. Significance and Use

5.1 Properties of EVA copolymers are affected by the amount of vinyl acetate incorporated in the copolymer: This test method provides a means to determine the vinyl acetate level in copolymer samples.

5.2 Before proceeding with this test method, reference should be made to the specification of the material being tested. Any test specimen preparation, conditioning, dimensions, or testing parameters, or a combination thereof, covered in the materials specification shall take precedence over those mentioned in this test method. If there are no material specifications, then the default conditions apply.

6. Apparatus

6.1 *Fourier Transform Infrared (FT-IR) Spectrophotometer*, equipped with a detector, which gives a linear response over the desired concentration range, is capable of 4-cm^{-2} resolution (nominal), and is able to scan from 4400 to 450 cm^{-1} .

NOTE 2—A DTGS detector has been found suitable for this application.

6.2 *Hot Plate*, (Sample Preparation Procedure A only).

6.3 *Microscope Slides*, (Sample Preparation Procedure A only).

6.4 *Laboratory Press*, capable of at least 9 000 kg (20 000 lb) 150°C (300°F), (Sample Preparation Procedure B only).

6.5 *Backing Plates*, steel or aluminum (Sample Preparation Procedure B only).

6.6 *Brass Shim Stock (Roll)*, 50 to $150\text{ }\mu\text{m}$ (2 to 6 mil) thick and 150 mm (6 in.) wide (Sample Preparation Procedure B only).

6.7 *Polyester Sheet*, or fiberglass impregnated PTFE cloth (Sample Preparation Procedure B only).

6.8 *PTFE Film* (Sample Preparation Procedure B, resins containing $\geq 40\%$ vinyl acetate only).

6.9 *Templates*, (mold) with $150 \times 150\text{ mm}$ ($6 \times 6\text{ in.}$) pieces of paper or brass shim stock (item 6.6) containing cavities of a size and shape appropriate for the sample holders used, and, if applicable, sheets of items 6.7 and 6.8 (Sample Preparation Procedure B only).

6.10 *Cooling Block*, steel or aluminum, at least $150 \times 150\text{ mm}$ ($6 \times 6\text{ in.}$), approximately 25 mm (1 in.) thick, channeled for cooling water (Sample Preparation Procedure B only).

7. Materials

7.1 EVA copolymer standards containing nominal vinyl acetate concentrations of 0.5 to 55 %, by weight.

7.2 Dry ice (Sample Preparation B Procedure A only).

8. Hazards

8.1 Care shall be taken to avoid burns when handling microscope slides on the hot-plate (Sample Preparation Procedure A), and gloves shall be worn when plaques are prepared using a heated press (Sample Preparation Procedure B).

8.2 Care also shall be taken to avoid breaking the microscope slides while removing the pressed polymer film.

8.3 Care shall be taken to avoid burns when handling dry ice.

9. Specimen Preparation

9.1 Procedure A:

9.1.1 Control the hot-plate temperature at $250 \pm 10^{\circ}\text{C}$.

9.1.2 Place a microscope slide, containing a fraction of the sample pellet, on the hot-plate.

9.1.3 Cover the sample with another slide and press with a wooden pestle. Use film circular motions to press a uniform film.

9.1.4 Remove the microscope slide from the hot-plate and quench the pressed polymer film by dipping the two slides into a beaker of cold water. Remove the film and blot dry with an absorbent towel.

9.1.5 Absorption maxima, measured on film produced by this procedure, shall not exceed 1.5 absorbance units for either of the analytical bands used.

9.2 Procedure B:

NOTE 3—Omit 9.2.1 to 9.2.11 for analysis of blown film.

9.2.1 Select a brass or paper mold with a thickness appropriate to the vinyl acetate content of the sample. The absorption maxima of the vinyl acetate and ethylene bands measured on the plaque are not to exceed 1.5 absorbance units.

NOTE 4—To meet the absorbance requirement specified in 9.2.1 it will be necessary to vary the mold thickness as the vinyl acetate content changes. The mold thickness required typically will be between 50 and $150\text{ }\mu\text{m}$ (2 to 6 mil).

9.2.2 Place a polyester sheet (or fiberglass impregnated PTFE cloth) followed by a brass or paper mold on a backing plate.

NOTE 5—For resins with vinyl acetate content $\geq 40\%$, a PTFE film should be placed on top of the brass mold, or, if using a paper mold, under the paper.

9.2.3 Place a quantity of sample, appropriate to the thickness of the mold used, in the center of each opening in the mold. Do not overfill the mold openings.

NOTE 6—If flashing occurs, the brass mold and backing plates can be cleaned with a nylon scrubbing pad.

9.2.4 Place another piece of polyester sheet (or fiberglass impregnated PTFE cloth) and a backing plate on top of the sample.

NOTE 7—For resins with vinyl acetate content $\geq 40\%$, a PTFE film should be placed over the sample before the polyester sheet (or fiberglass impregnated PTFE cloth).

9.2.5 Place the resulting “sandwich” in the press with the platens heated at 150 to 175°C .

9.2.6 Close the press until the top platen barely touches the top plate and leave for sufficient time to permit the sample to soften and outgas.

NOTE 8—Acceptable plaques, free of gas bubbles, have been obtained when the sample is allowed to soften for 3 min.

9.2.7 Close the press completely and apply at least 9 000 kg (20 000 lb) force for approximately 1 min.

9.2.8 Cool the “sandwich” to room temperature, release the pressure, and remove the “sandwich” from the press.

9.2.9 In cases where the press does not have cooling capability or where sample throughput needs to be increased, the following alternative to 9.2.8 may be used. The “sandwich” is removed from the press hot and placed on a metal cooling block through which cold water is circulated. A mass of at least 4 kg (9 lb) is placed on top to the “sandwich” while it cools to room temperature.

9.2.10 For resins with vinyl acetate content <40 %, separate the backing plates and remove the plaques from the mold.

9.2.11 For resins with vinyl acetate content ≥40 %, place the “sandwich” on dry ice for at least 15 s before separating the backing plate, polyester sheet (or fiberglass impregnated PTFE cloth), and the PTFE film from the plaque.

9.2.12 Select plaques that are clear and of uniform thickness for the FT-IR analysis.

10. Calibration

10.1 Record the open beam background spectrum from 4400 to 450 cm^{-1} at a nominal resolution of 4 cm^{-1} .

10.2 Place a standard EVA copolymer film (plaque), prepared as described in 9.1 or 9.2, in the sample beam of the FT-IR spectrometer.

10.3 Record the infrared spectrum from 4400 to 450 cm^{-1} at a nominal resolution of 4 cm^{-1} . The signal-to-noise ratio, S/N, should be acceptable for the desired precision. A typical EVA copolymer spectrum (9.0 % vinyl acetate) is shown in Fig. 1.

10.4 Ratio the sample spectrum to the background spectrum and convert the results to absorbance.

10.5 Measure the area of one vinyl acetate band and one ethylene band selected from the choices given in Table 1. Absorbance maxima for the analytical bands chosen are not to exceed 1.5 absorbance units.

10.6 Draw a baseline tangent to the absorption minima on either side of each peak. Determine the area of each peak above the baseline.

10.7 Calculate the vinyl acetate/ethylene area ratio for the appropriate data reduction procedure defined in 12.1.

10.7.1 For linear regression analysis:

$$r = A_{va}/A_{et} \quad (1)$$

10.7.2 For nonlinear regression analysis:⁴

$$R = A_{va}/(A_{va} + A_{et}) \quad (2)$$

where:

A_{va} = Area of vinyl acetate band, and

A_{et} = Area of ethylene band.

10.8 Repeat 10.2 through 10.7.2 for each standard EVA copolymer film (plaque).

10.9 A minimum of five standards shall be used for the linear regression of the 0.5 to 5.0 % vinyl acetate range. The number of standards used for the nonlinear regression of either the 5.0 to 28 % or 28 to 55 % vinyl acetate ranges shall not be less than six.

10.10 The standards must cover the full range of vinyl acetates to be analyzed. Extrapolation is not permitted.

11. Procedure

11.1 Prepare samples as described in 9.1 for films or 9.2 for plaques.

11.2 Record the open beam background spectrum from 4400 to 450 cm^{-1} at a nominal resolution of 4 cm^{-1} .

11.3 Place a sample film (plaque) in the sample beam of the FT-IR spectrometer.

11.4 Record the infrared spectrum from 4400 to 450 cm^{-1} at a nominal resolution of 4 cm^{-1} . The signal-to-noise ratio, S/N, should be acceptable for the desired precision.

11.5 Ratio the sample spectrum to the background spectrum and convert the result to absorbance.

11.6 Measure the area of one vinyl acetate and one ethylene band selected from the options given in Table 1. Absorbance maxima for the analytical bands chosen are not to exceed 1.5 absorbance units.

11.7 Draw a baseline tangent to the absorption minima on either side of each peak. Determine the area of each peak above the baseline.

11.8 Calculate the vinyl acetate to ethylene area ratio as specified in 10.7.

12. Calculation

12.1 *Regression Analysis:*

12.1.1 For vinyl acetate standards between 0.5 and 5.0 %, use linear regression analysis to determine the calibration equation of the data obtained in 10.7 and 10.8.

12.1.2 For vinyl acetate standards covering the range 5.0 to 28 % or 28 to 55 %, use nonlinear regression analysis, of the data obtained in 10.7 and 10.8, to determine an equation of the form:

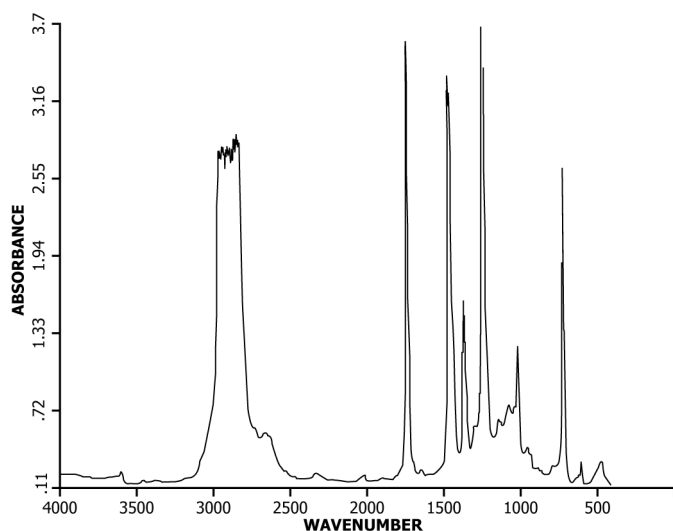


FIG. 1 FT-IR Spectrum of EVA Copolymer Standard (4.8 % Vinyl Acetate) Analyzed by Procedure B

⁴ Cole, K. C., Pellerius, T. E., D***, M. M., and Paroli, R. M., “New Approach to Quantitative Analysis of Two-Component Polymer Systems by Infrared Spectroscopy,” *Applied Spectroscopy*, Vol 50, No. 6, June 1996, pp. 774–780.