

# INTERNATIONAL STANDARD

## NORME INTERNATIONALE

**Environmental testing –**  
**Part 3-7: Supporting documentation and guidance – Measurements in**  
**temperature chambers for tests A (Cold) and B (Dry heat) (with load)**

**Essais d'environnement –**  
**Partie 3-7: Documentation d'accompagnement et recommandations –**  
**Mesurages dans les chambres d'essai en température pour les essais A (froid)**  
**et B (chaleur sèche) (avec charge)**



## THIS PUBLICATION IS COPYRIGHT PROTECTED

Copyright © 2020 IEC, Geneva, Switzerland

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either IEC or IEC's member National Committee in the country of the requester. If you have any questions about IEC copyright or have an enquiry about obtaining additional rights to this publication, please contact the address below or your local IEC member National Committee for further information.

Droits de reproduction réservés. Sauf indication contraire, aucune partie de cette publication ne peut être reproduite ni utilisée sous quelque forme que ce soit et par aucun procédé, électronique ou mécanique, y compris la photocopie et les microfilms, sans l'accord écrit de l'IEC ou du Comité national de l'IEC du pays du demandeur. Si vous avez des questions sur le copyright de l'IEC ou si vous désirez obtenir des droits supplémentaires sur cette publication, utilisez les coordonnées ci-après ou contactez le Comité national de l'IEC de votre pays de résidence.

IEC Central Office  
3, rue de Varembe  
CH-1211 Geneva 20  
Switzerland

Tel.: +41 22 919 02 11  
[info@iec.ch](mailto:info@iec.ch)  
[www.iec.ch](http://www.iec.ch)

### About the IEC

The International Electrotechnical Commission (IEC) is the leading global organization that prepares and publishes International Standards for all electrical, electronic and related technologies.

### About IEC publications

The technical content of IEC publications is kept under constant review by the IEC. Please make sure that you have the latest edition, a corrigendum or an amendment might have been published.

#### IEC publications search - [webstore.iec.ch/advsearchform](http://webstore.iec.ch/advsearchform)

The advanced search enables to find IEC publications by a variety of criteria (reference number, text, technical committee,...). It also gives information on projects, replaced and withdrawn publications.

#### IEC Just Published - [webstore.iec.ch/justpublished](http://webstore.iec.ch/justpublished)

Stay up to date on all new IEC publications. Just Published details all new publications released. Available online and once a month by email.

#### IEC Customer Service Centre - [webstore.iec.ch/csc](http://webstore.iec.ch/csc)

If you wish to give us your feedback on this publication or need further assistance, please contact the Customer Service Centre: [sales@iec.ch](mailto:sales@iec.ch).

#### Electropedia - [www.electropedia.org](http://www.electropedia.org)

The world's leading online dictionary on electrotechnology, containing more than 22,000 terminological entries in English and French, with equivalent terms in 16 additional languages. Also known as the International Electrotechnical Vocabulary (IEV) online.

#### IEC Glossary - [std.iec.ch/glossary](http://std.iec.ch/glossary)

67,000 electrotechnical terminology entries in English and French extracted from the Terms and Definitions clause of IEC publications issued since 2002. Some entries have been collected from earlier publications of IEC TC 37, 77, 86 and CISPR.

### A propos de l'IEC

La Commission Electrotechnique Internationale (IEC) est la première organisation mondiale qui élabore et publie des Normes internationales pour tout ce qui a trait à l'électricité, à l'électronique et aux technologies apparentées.

### A propos des publications IEC

Le contenu technique des publications IEC est constamment revu. Veuillez vous assurer que vous possédez l'édition la plus récente, un corrigendum ou amendement peut avoir été publié.

#### Recherche de publications IEC -

[webstore.iec.ch/advsearchform](http://webstore.iec.ch/advsearchform)

La recherche avancée permet de trouver des publications IEC en utilisant différents critères (numéro de référence, texte, comité d'études,...). Elle donne aussi des informations sur les projets et les publications remplacées ou retirées.

#### IEC Just Published - [webstore.iec.ch/justpublished](http://webstore.iec.ch/justpublished)

Restez informé sur les nouvelles publications IEC. Just Published détaille les nouvelles publications parues. Disponible en ligne et une fois par mois par email.

#### Service Clients - [webstore.iec.ch/csc](http://webstore.iec.ch/csc)

Si vous désirez nous donner des commentaires sur cette publication ou si vous avez des questions contactez-nous: [sales@iec.ch](mailto:sales@iec.ch).

#### Electropedia - [www.electropedia.org](http://www.electropedia.org)

Le premier dictionnaire d'électrotechnologie en ligne au monde, avec plus de 22 000 articles terminologiques en anglais et en français, ainsi que les termes équivalents dans 16 langues additionnelles. Egalement appelé Vocabulaire Electrotechnique International (IEV) en ligne.

#### Glossaire IEC - [std.iec.ch/glossary](http://std.iec.ch/glossary)

67 000 entrées terminologiques électrotechniques, en anglais et en français, extraites des articles Termes et Définitions des publications IEC parues depuis 2002. Plus certaines entrées antérieures extraites des publications des CE 37, 77, 86 et CISPR de l'IEC.

# INTERNATIONAL STANDARD

## NORME INTERNATIONALE

Environmental testing –

Part 3-7: Supporting documentation and guidance – Measurements in temperature chambers for tests A (Cold) and B (Dry heat) (with load)

[IEC 60068-3-7:2020](https://standards.iteh.ai/catalog/standards/sist/a6a12324-a3da-4a15-b822-d17884833981/iec-60068-3-7-2020)

Essais d'environnement –

Partie 3-7: Documentation d'accompagnement et recommandations –  
Mesurages dans les chambres d'essai en température pour les essais A (froid)  
et B (chaleur sèche) (avec charge)

INTERNATIONAL  
ELECTROTECHNICAL  
COMMISSION

COMMISSION  
ELECTROTECHNIQUE  
INTERNATIONALE

ICS 19.040; 29.020

ISBN 978-2-8322-8599-2

**Warning! Make sure that you obtained this publication from an authorized distributor.**  
**Attention! Veuillez vous assurer que vous avez obtenu cette publication via un distributeur agréé.**

## CONTENTS

FOREWORD .....	3
INTRODUCTION .....	5
1 Scope .....	6
2 Normative references .....	6
3 Terms and definitions .....	6
4 Measuring system .....	8
4.1 General description .....	8
4.2 Temperature .....	8
4.2.1 General .....	8
4.2.2 Temperature sensor .....	8
4.3 Humidity .....	8
4.3.1 General .....	8
4.3.2 Humidity sensor .....	9
4.4 Wall emissivity .....	9
4.5 Air velocity .....	9
4.5.1 General .....	9
4.5.2 Air velocity sensor .....	9
4.5.3 Air velocity sensor response time .....	9
4.6 Recording device .....	9
5 Determination of temperature performances .....	9
5.1 Test area environment .....	9
5.2 Chamber loading .....	9
5.2.1 General .....	9
5.2.2 Location of test load .....	10
5.3 Installation of temperature sensors .....	10
5.3.1 General .....	10
5.3.2 Position of temperature sensors .....	10
5.3.3 Position of load sensors .....	10
6 Test procedures .....	10
6.1 Confirmation methods .....	10
6.1.1 General .....	10
6.1.2 Test without load .....	10
6.1.3 Test with load .....	10
6.2 Routine monitoring methods .....	10
7 Evaluation criteria .....	11
8 Information to be given in the performance report .....	11
Bibliography .....	12
Figure 1 – Examples of artificial loads .....	8
Table 1 – Test conditions .....	7
Table 2 – Artificial load – Values .....	7

## INTERNATIONAL ELECTROTECHNICAL COMMISSION

## ENVIRONMENTAL TESTING –

**Part 3-7: Supporting documentation and guidance –  
Measurements in temperature chambers for  
tests A (Cold) and B (Dry heat) (with load)**

## FOREWORD

- 1) The International Electrotechnical Commission (IEC) is a worldwide organization for standardization comprising all national electrotechnical committees (IEC National Committees). The object of IEC is to promote international co-operation on all questions concerning standardization in the electrical and electronic fields. To this end and in addition to other activities, IEC publishes International Standards, Technical Specifications, Technical Reports, Publicly Available Specifications (PAS) and Guides (hereafter referred to as “IEC Publication(s)”). Their preparation is entrusted to technical committees; any IEC National Committee interested in the subject dealt with may participate in this preparatory work. International, governmental and non-governmental organizations liaising with the IEC also participate in this preparation. IEC collaborates closely with the International Organization for Standardization (ISO) in accordance with conditions determined by agreement between the two organizations.
- 2) The formal decisions or agreements of IEC on technical matters express, as nearly as possible, an international consensus of opinion on the relevant subjects since each technical committee has representation from all interested IEC National Committees.
- 3) IEC Publications have the form of recommendations for international use and are accepted by IEC National Committees in that sense. While all reasonable efforts are made to ensure that the technical content of IEC Publications is accurate, IEC cannot be held responsible for the way in which they are used or for any misinterpretation by any end user.
- 4) In order to promote international uniformity, IEC National Committees undertake to apply IEC Publications transparently to the maximum extent possible in their national and regional publications. Any divergence between any IEC Publication and the corresponding national or regional publication shall be clearly indicated in the latter.
- 5) IEC itself does not provide any attestation of conformity. Independent certification bodies provide conformity assessment services and, in some areas, access to IEC marks of conformity. IEC is not responsible for any services carried out by independent certification bodies.
- 6) All users should ensure that they have the latest edition of this publication.
- 7) No liability shall attach to IEC or its directors, employees, servants or agents including individual experts and members of its technical committees and IEC National Committees for any personal injury, property damage or other damage of any nature whatsoever, whether direct or indirect, or for costs (including legal fees) and expenses arising out of the publication, use of, or reliance upon, this IEC Publication or any other IEC Publications.
- 8) Attention is drawn to the Normative references cited in this publication. Use of the referenced publications is indispensable for the correct application of this publication.
- 9) Attention is drawn to the possibility that some of the elements of this IEC Publication may be the subject of patent rights. IEC shall not be held responsible for identifying any or all such patent rights.

International Standard IEC 60068-3-7 has been prepared by IEC technical committee TC 104: Environmental conditions, classification and methods of test.

This second edition cancels and replaces the first edition published in 2001. This edition constitutes a technical revision.

This edition includes the following significant technical changes with respect to the previous edition:

- a) verbal forms have, in many parts, been changed to express requirements instead of recommendations ('shall' instead of 'should');
- b) Table 1 has been updated.

The text of this International Standard is based on the following documents:

FDIS	Report on voting
104/868/FDIS	104/873/RVD

Full information on the voting for the approval of this International Standard can be found in the report on voting indicated in the above table.

This document has been drafted in accordance with the ISO/IEC Directives, Part 2.

A list of all parts in the IEC 60068 series, published under the general title *Environmental testing*, can be found on the IEC website.

The committee has decided that the contents of this document will remain unchanged until the stability date indicated on the IEC website under "<http://webstore.iec.ch>" in the data related to the specific document. At this date, the document will be

- reconfirmed,
- withdrawn,
- replaced by a revised edition, or
- amended.

**iTeh STANDARD PREVIEW**  
**(standards.iteh.ai)**

[IEC 60068-3-7:2020](https://standards.iteh.ai/catalog/standards/sist/a6a12324-a3da-4a15-b822-fdd788d87308/iec-60068-3-7-2020)

<https://standards.iteh.ai/catalog/standards/sist/a6a12324-a3da-4a15-b822-fdd788d87308/iec-60068-3-7-2020>

## INTRODUCTION

IEC 60068 (all parts) contains fundamental information on environmental testing procedures and severities.

The expression "environmental conditioning" or "environmental testing" covers the natural and artificial environments to which components or equipment may be exposed so that an assessment can be made of their performance under conditions of use, transport and storage to which they may be exposed in practice.

Temperature chambers used for "environmental conditioning" or "environmental testing" are not described in any publication, although the method of maintaining and measuring temperature and/or humidity has great influence on test results. The physical characteristics of temperature chambers can also influence test results.

## iTeh STANDARD PREVIEW (standards.iteh.ai)

[IEC 60068-3-7:2020](https://standards.iteh.ai/catalog/standards/sist/a6a12324-a3da-4a15-b822-fdd788d87308/iec-60068-3-7-2020)

<https://standards.iteh.ai/catalog/standards/sist/a6a12324-a3da-4a15-b822-fdd788d87308/iec-60068-3-7-2020>

## ENVIRONMENTAL TESTING –

### Part 3-7: Supporting documentation and guidance – Measurements in temperature chambers for tests A (Cold) and B (Dry heat) (with load)

#### 1 Scope

This part of IEC 60068 specifies a uniform and reproducible method of confirming that temperature test chambers conform to the requirements specified in the climatic test procedures of IEC 60068-2-1 and IEC 60068-2-2, when loaded with either heat-dissipating or non heat-dissipating specimens under conditions which take into account air circulation inside the working space of the chamber. This document is intended primarily for users when conducting regular chamber performance monitoring.

#### 2 Normative references

The following documents are referred to in the text in such a way that some or all of their content constitutes requirements of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

IEC 60068-3-5:2018, *Environmental testing – Part 3-5: Supporting documentation and guidance – Confirmation of the performance of temperature chambers*

<https://standards.iteh.ai/catalog/standards/sist/a6a12324-a3da-4a15-b822-fdd788d87308/iec-60068-3-7-2020>

#### 3 Terms and definitions

For the purposes of this document, the following terms and definitions apply.

ISO and IEC maintain terminological databases for use in standardization at the following addresses:

- IEC Electropedia: available at <http://www.electropedia.org/>
- ISO Online browsing platform: available at <http://www.iso.org/obp>

##### 3.1

##### **test specification**

procedure applied to test chambers with or without forced air circulation, suitable for a wide range of chamber sizes

Note 1 to entry: A summary of test conditions in IEC 60068-2-1 and IEC 60068-2-2 is given in Table 1; conditions including sudden change of temperature have been removed from earlier versions of these documents.



**Table 1 – Test conditions**

Temperature range	Test	Specimen heat-dissipation		Specimen power status		Change of temperature	Preferred air velocity	
		None	With	After stabilization	Throughout test	Gradual	High	Low
-65 °C to +5 °C	Ab	○				○	○	
	Ad		○	○		○		○
	Ae		○		○	○		○
+30 °C to +1 000 °C	Bb	○				○	○	
	Bd		○	○		○		○
	Be		○		○	○		○

**3.2****confirmation method**

specified method of making continuous measurements in order to establish whether the performance of a test chamber conforms to the requirements detailed in IEC 60068-2-1, test A and/or IEC 60068-2-2, test B

**3.3****routine monitoring method**

specified method of making measurements continuously or at intervals, to ensure that the test chamber performance is being maintained

**3.4****test load**

test specimen that is installed in the test chamber for the confirmation measurements

Note 1 to entry: The test load is defined by geometric dimensions and by thermal properties.


**3.5****artificial load**

test load made in accordance with IEC 60068-3-7 with dimensions and thermal properties related to the geometric dimensions and thermal capacity of the specimens intended to be tested in the chamber

Note 1 to entry: Table 2 provides values for an artificial load and an example is given in Figure 1.

**Table 2 – Artificial load – Values**

Dimensions	Volume approximately 20 % of working space
Heat transmission	Approximately 10 kJ/m <sup>2</sup> K
Heat radiation emissivity	> 0,7
Heat dissipation	In accordance with IEC 60068-2-2:2007, 4.1.

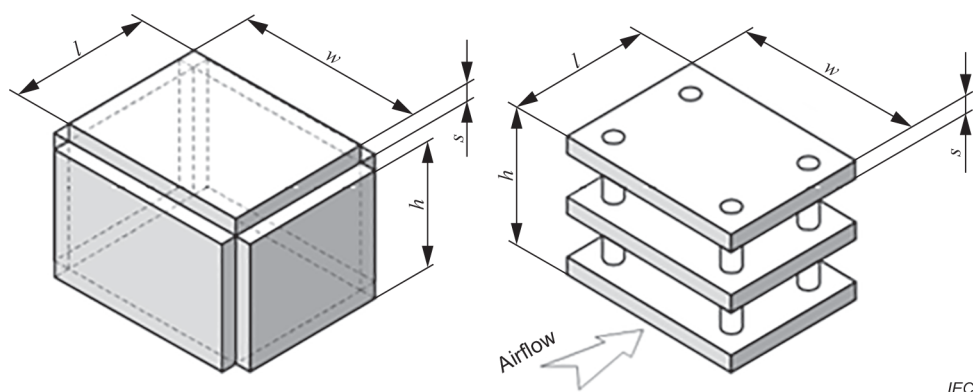

#### Key

- $h$  height
- $l$  length
- $w$  width
- $s$  thickness of material

NOTE  $s = 3$  mm stainless steel or 4 mm aluminium ( $h$ ,  $l$  and  $w$  should be smaller than the relevant dimensions of the working space).

**Figure 1 – Examples of artificial loads**

## 4 Measuring system

### 4.1 General description

The system used for the confirmation and routine monitoring measurements, either built-in or independent of the chamber, should comply with the following requirements. Measurement devices other than those listed may be used when their performance is shown to be technically equivalent or when practical concerns require alternative techniques. Deviations from these requirements shall be documented.

### 4.2 Temperature

#### 4.2.1 General

Platinum resistance thermometers (in accordance with IEC 60751) or thermocouples (in accordance with IEC 60584-1) should be used.

#### 4.2.2 Temperature sensor

In a temperature range from  $-200$  °C to  $+650$  °C the sensor measurement uncertainty should be in accordance with class A of IEC 60751.

### 4.3 Humidity

#### 4.3.1 General

The humidity test is required for confirmation of IEC 60068-2-2 tests only.

Place the independent humidity sensor as near as practical to the centre of the working space.

Types of humidity monitoring sensors are described in 4.4 of IEC 60068-3-6:2018.

#### 4.3.2 Humidity sensor

Sensor measurement uncertainty should not exceed  $\pm 3$  % RH.

#### 4.4 Wall emissivity

Emissivity of the chamber enclosure should be in accordance with IEC 60068-3-1.

#### 4.5 Air velocity

##### 4.5.1 General

An airflow sensor should be installed such that the maximum air velocity impinging on the load can be monitored.

##### 4.5.2 Air velocity sensor

The air velocity sensor measurement uncertainty should be compatible with IEC 60068-2-1 and 60068-2-2 tolerances.

##### 4.5.3 Air velocity sensor response time

The air velocity sensor response time should be greater than 5 s to avoid any influence on it by airflow fluctuation.

#### 4.6 Recording device

For confirmation monitoring, data should be recorded at least once per minute. For routine monitoring, data should be recorded at least once every 5 min. For the purpose of chamber verification, the device utilized for recording data should be independent of the chamber control system.

<https://standards.iteh.ai/catalog/standards/sist/a6a12324-a3da-4a15-b822-fdd788d87308/iec-60068-3-7-2020>

### 5 Determination of temperature performances

#### 5.1 Test area environment

The environment in the test area shall be in accordance with 4.1 of IEC 60068-3-5:2018.

#### 5.2 Chamber loading

##### 5.2.1 General

Provision is made for measurement of test chamber performance with different loading conditions.

Test loads:	heat-dissipating
	non heat-dissipating
Artificial loads:	heat-dissipating
	non heat-dissipating

NOTE However, when testing large, high heat dissipating specimens, it can be desirable to allow the specimen to develop thermal gradients by using 'free air' chambers or those with a low airflow (typically less than 0,5 m/s). In such cases it is possible that the chamber will not have a uniform temperature within the working space and it is important to monitor the temperatures of the air entering and exiting the specimen.