

INTERNATIONAL STANDARD



**Medical electrical equipment –
Part 2-21: Particular requirements for the basic safety and essential
performance of infant radiant warmers**

Document Preview

[IEC 60601-2-21:2020](#)

<https://standards.iteh.ai/catalog/standards/iec/9373f8a7-f219-4195-b237-7b20917f5eb9/iec-60601-2-21-2020>



THIS PUBLICATION IS COPYRIGHT PROTECTED
Copyright © 2020 IEC, Geneva, Switzerland

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either IEC or IEC's member National Committee in the country of the requester. If you have any questions about IEC copyright or have an enquiry about obtaining additional rights to this publication, please contact the address below or your local IEC member National Committee for further information.

IEC Central Office
3, rue de Varembe
CH-1211 Geneva 20
Switzerland

Tel.: +41 22 919 02 11
info@iec.ch
www.iec.ch

About the IEC

The International Electrotechnical Commission (IEC) is the leading global organization that prepares and publishes International Standards for all electrical, electronic and related technologies.

About IEC publications

The technical content of IEC publications is kept under constant review by the IEC. Please make sure that you have the latest edition, a corrigendum or an amendment might have been published.

IEC publications search - webstore.iec.ch/advsearchform

The advanced search enables to find IEC publications by a variety of criteria (reference number, text, technical committee,...). It also gives information on projects, replaced and withdrawn publications.

IEC Just Published - webstore.iec.ch/justpublished

Stay up to date on all new IEC publications. Just Published details all new publications released. Available online and once a month by email.

IEC Customer Service Centre - webstore.iec.ch/csc

If you wish to give us your feedback on this publication or need further assistance, please contact the Customer Service Centre: sales@iec.ch.

Electropedia - www.electropedia.org

The world's leading online dictionary on electrotechnology, containing more than 22 000 terminological entries in English and French, with equivalent terms in 16 additional languages. Also known as the International Electrotechnical Vocabulary (IEV) online.

IEC Glossary - std.iec.ch/glossary

67 000 electrotechnical terminology entries in English and French extracted from the Terms and Definitions clause of IEC publications issued since 2002. Some entries have been collected from earlier publications of IEC TC 37, 77, 86 and CISPR.

International
Standards
IEC
Document Preview

[IEC 60601-2-21:2020](#)

<https://standards.iteh.ai/catalog/standards/iec/9373f8a7-f219-4195-b237-7b20917f5eb9/iec-60601-2-21-2020>



IEC 60601-2-21

Edition 3.0 2020-09
REDLINE VERSION

INTERNATIONAL STANDARD



**Medical electrical equipment –
Part 2-21: Particular requirements for the basic safety and essential
performance of infant radiant warmers**

Document Preview

[IEC 60601-2-21:2020](#)

<https://standards.iteh.ai/catalog/standards/iec/9373f8a7-f219-4195-b237-7b20917f5eb9/iec-60601-2-21-2020>

INTERNATIONAL
ELECTROTECHNICAL
COMMISSION

ICS 11.040.10

ISBN 978-2-8322-8922-8

Warning! Make sure that you obtained this publication from an authorized distributor.

CONTENTS

FOREWORD.....	3
INTRODUCTION.....	2
201.1 Scope, object and related standards.....	7
201.2 Normative references	9
201.3 Terms and definitions	9
201.4 General requirements.....	12
201.5 General requirements for testing of ME EQUIPMENT.....	12
201.6 Classification of ME EQUIPMENT and ME SYSTEMS	13
201.7 ME EQUIPMENT identification, marking and documents.....	13
201.8 Protection against electrical HAZARDS from ME EQUIPMENT.....	15
201.9 Protection against MECHANICAL HAZARDS of ME EQUIPMENT and ME SYSTEMS.....	15
201.10 Protection against unwanted and excessive radiation HAZARDS.....	16
201.11 Protection against excessive temperatures and other HAZARDS.....	17
201.12 Accuracy of controls and instruments and protection against hazardous outputs	18
201.13 HAZARDOUS SITUATIONS and fault conditions for ME EQUIPMENT	22
201.14 PROGRAMMABLE ELECTRICAL MEDICAL SYSTEMS (PEMS)	22
201.15 Construction of ME EQUIPMENT	22
201.16 ME SYSTEMS.....	23
201.17 Electromagnetic compatibility of ME EQUIPMENT and ME SYSTEMS.....	23
202 Electromagnetic compatibility – Requirements and tests.....	23
210 Requirements for the development of physiologic closed loop controllers	23
202 Electromagnetic disturbances – Requirements and tests	23
Annexes	26
Annex AA (informative) Particular guidance and rationale.....	27
Bibliography.....	36
Index of defined terms used in this document	39
Figure 201.101 – Layout of TEST DEVICES	10
Figure 201.102 – TEST DEVICE.....	11
Figure AA.1 – Illustration of the main requirements of this document	27
Table 201.101 – Additional ESSENTIAL PERFORMANCE requirements.....	12

INTERNATIONAL ELECTROTECHNICAL COMMISSION

MEDICAL ELECTRICAL EQUIPMENT –

Part 2-21: Particular requirements for the basic safety and essential performance of infant radiant warmers

FOREWORD

- 1) The International Electrotechnical Commission (IEC) is a worldwide organization for standardization comprising all national electrotechnical committees (IEC National Committees). The object of IEC is to promote international co-operation on all questions concerning standardization in the electrical and electronic fields. To this end and in addition to other activities, IEC publishes International Standards, Technical Specifications, Technical Reports, Publicly Available Specifications (PAS) and Guides (hereafter referred to as "IEC Publication(s)"). Their preparation is entrusted to technical committees; any IEC National Committee interested in the subject dealt with may participate in this preparatory work. International, governmental and non-governmental organizations liaising with the IEC also participate in this preparation. IEC collaborates closely with the International Organization for Standardization (ISO) in accordance with conditions determined by agreement between the two organizations.
- 2) The formal decisions or agreements of IEC on technical matters express, as nearly as possible, an international consensus of opinion on the relevant subjects since each technical committee has representation from all interested IEC National Committees.
- 3) IEC Publications have the form of recommendations for international use and are accepted by IEC National Committees in that sense. While all reasonable efforts are made to ensure that the technical content of IEC Publications is accurate, IEC cannot be held responsible for the way in which they are used or for any misinterpretation by any end user.
- 4) In order to promote international uniformity, IEC National Committees undertake to apply IEC Publications transparently to the maximum extent possible in their national and regional publications. Any divergence between any IEC Publication and the corresponding national or regional publication shall be clearly indicated in the latter.
- 5) IEC provides no marking procedure to indicate its approval and cannot be rendered responsible for any equipment declared to be in conformity with an IEC Publication.
- 6) All users should ensure that they have the latest edition of this publication.
- 7) No liability shall attach to IEC or its directors, employees, servants or agents including individual experts and members of its technical committees and IEC National Committees for any personal injury, property damage or other damage of any nature whatsoever, whether direct or indirect, or for costs (including legal fees) and expenses arising out of the publication, use of, or reliance upon, this IEC Publication or any other IEC Publications.
- 8) Attention is drawn to the normative references cited in this publication. Use of the referenced publications is indispensable for the correct application of this publication.
- 9) Attention is drawn to the possibility that some of the elements of this IEC Publication may be the subject of patent rights. IEC shall not be held responsible for identifying any or all such patent rights.

This redline version of the official IEC Standard allows the user to identify the changes made to the previous edition. A vertical bar appears in the margin wherever a change has been made. Additions are in green text, deletions are in strikethrough red text.

International standard IEC 60601-2-21 has been prepared by subcommittee 62D: Electromedical equipment, of IEC technical committee 62: Electrical equipment in medical practice.

This third edition cancels and replaces the second edition published in 2009 and Amendment 1:2016. This edition constitutes a technical revision.

This edition includes the following significant technical change with respect to the previous edition: alignment with IEC 60601-1:2005 and IEC 60601-1:2005/AMD1:2012.

The text of this international standard is based on the following documents:

FDIS	Report on voting
62D/1766/FDIS	62D/1776/RVD

Full information on the voting for the approval of this International Standard can be found in the report on voting indicated in the above table.

This publication has been drafted in accordance with the ISO/IEC Directives, Part 2.

In this document, the following print types are used:

- requirements and definitions: roman type;
- *test specifications: italic type;*
- informative material appearing outside of tables, such as notes, examples and references: in smaller type. Normative text of tables is also in a smaller type;
- TERMS DEFINED IN CLAUSE 3 OF THE GENERAL STANDARD, IN THIS PARTICULAR STANDARD OR AS NOTED: SMALL CAPITALS.

In referring to the structure of this document, the term

- "clause" means one of the seventeen numbered divisions within the table of contents, inclusive of all subdivisions (e.g. Clause 7 includes subclauses 7.1, 7.2, etc.);
- "subclause" means a numbered subdivision of a clause (e.g. 7.1, 7.2 and 7.2.1 are all subclauses of Clause 7).

References to clauses within this document are preceded by the term "Clause" followed by the clause number. References to subclauses within this particular standard are by number only.

In this document, the conjunctive "or" is used as an "inclusive or" so a statement is true if any combination of the conditions is true.

The verbal forms used in this standard conform to usage described in Clause 7 of the ISO/IEC Directives, Part 2. For the purposes of this document, the auxiliary verb:

- "shall" means that compliance with a requirement or a test is mandatory for compliance with this document;
- "should" means that compliance with a requirement or a test is recommended but is not mandatory for compliance with this document;
- "may" is used to describe a permissible way to achieve compliance with a requirement or test.

An asterisk (*) as the first character of a title or at the beginning of a paragraph or table title indicates that there is guidance or rationale related to that item in Annex AA.

A list of all parts of the IEC 60601 series, published under the general title *Medical electrical equipment*, can be found on the IEC website.

The committee has decided that the contents of this document will remain unchanged until the stability date indicated on the IEC website under "<http://webstore.iec.ch>" in the data related to the specific document. At this date, the document will be

- reconfirmed,
- withdrawn,
- replaced by a revised edition, or
- amended.

NOTE The attention of users of this document is drawn to the fact that equipment manufacturers and testing organizations may need a transitional period following publication of a new, amended or revised IEC publication in which to make products in accordance with the new requirements and to equip themselves for conducting new or revised tests. It is the recommendation of the committee that the content of this publication be adopted for implementation nationally not earlier than 3 years from the date of publication.

IMPORTANT – The 'colour inside' logo on the cover page of this publication indicates that it contains colours which are considered to be useful for the correct understanding of its contents. Users should therefore print this document using a colour printer.

ITeH Standards
(<https://standards.iteh.ai>)
Document Preview

[IEC 60601-2-21:2020](#)

<https://standards.iteh.ai/catalog/standards/iec/9373f8a7-f219-4195-b237-7b20917f5eb9/iec-60601-2-21-2020>

INTRODUCTION

The minimum safety requirements specified in this particular standard are considered to provide for a practical degree of safety in the operation of INFANT RADIANT WARMER equipment.

This particular standard amends and supplements IEC 60601-1:~~2005~~, *Medical electrical equipment – Part 1: General requirements for basic safety and essential performance*, hereinafter referred to as the "general standard".

The requirements are followed by specifications for the relevant tests.

A general guidance and rationale for the requirements of this particular standard are given in Annex AA.

It is considered that knowledge of the reasons for these requirements will not only facilitate the proper application of this particular standard but will, in due course, expedite any revision necessitated by changes in clinical practice or as a result of developments in technology. However, Annex AA does not form part of the requirements of this document.

iTeh Standards
(<https://standards.iteh.ai>)
Document Preview

[IEC 60601-2-21:2020](https://standards.iteh.ai/catalog/standards/iec/9373f8a7-f219-4195-b237-7b20917f5eb9/iec-60601-2-21-2020)

<https://standards.iteh.ai/catalog/standards/iec/9373f8a7-f219-4195-b237-7b20917f5eb9/iec-60601-2-21-2020>

MEDICAL ELECTRICAL EQUIPMENT –

Part 2-21: Particular requirements for the basic safety and essential performance of infant radiant warmers

201.1 Scope, object and related standards

Clause 1 of the general standard¹ applies, except as follows:

201.1.1 * Scope

Replacement:

This part of IEC 60601 applies to the BASIC SAFETY and ESSENTIAL PERFORMANCE of INFANT RADIANT WARMERS as defined in 201.3.204, also referred to as ME EQUIPMENT.

If a clause or subclause is specifically intended to be applicable to ME EQUIPMENT only, or to ME SYSTEMS only, the title and content of that clause or subclause will say so. If that is not the case, the clause or subclause applies both to ME EQUIPMENT and to ME SYSTEMS, as relevant.

HAZARDS inherent in the intended physiological function of ME EQUIPMENT or ME SYSTEMS within the scope of this document are not covered by specific requirements in this document, except in 7.2.13 and 8.4.1 of the general standard.

NOTE See also 4.2 of the general standard.

This particular standard specifies the safety requirements for INFANT RADIANT WARMERS, but alternate methods of compliance with a specific clause, by demonstrating equivalent safety, will not be judged as non-compliant, if the MANUFACTURER has demonstrated in his RISK MANAGEMENT FILE that the RISK presented by the HAZARD has been found to be of an acceptable level when weighed against the benefit of treatment from the device.

This particular standard does not apply to:

- devices supplying heat via BLANKETS, PADS or MATTRESSES in medical use; for information, see ~~IEC 80601-2-35~~ IEC 60601-2-35;
- INFANT INCUBATORS; for information, see IEC 60601-2-19;
- INFANT TRANSPORT INCUBATORS, for information, see IEC 60601-2-20;
- INFANT PHOTOTHERAPY EQUIPMENT, for information, see IEC 60601-2-50.

SKIN TEMPERATURE SENSORS which are applied to operate a BABY CONTROLLED RADIANT WARMER including the displayed value are not considered to be a CLINICAL THERMOMETER in the sense of the particular standard ISO 80601-2-56.

¹ The general standard is IEC 60601-1:2005 and IEC 60601-1:2005/AMD1:2012, *Medical electrical equipment – Part 1: General requirements for basic safety and essential performance*.

201.1.2 Object

Replacement:

The object of this particular standard is to establish particular BASIC SAFETY and ESSENTIAL PERFORMANCE requirements for INFANT RADIANT WARMERS as defined in 201.3.204, which minimize HAZARDS to PATIENT and OPERATOR, and to specify tests by which compliance with the requirements can be verified.

201.1.3 *Collateral standards

Addition:

This particular standard refers to those applicable collateral standards that are listed in Clause 2 of the general standard and Clause 2 of this particular standard.

IEC 60601-1-2:2014 ~~and IEC 60601-1-10~~ applies as modified in Clauses 202 ~~and 210~~ ~~respectively~~. IEC 60601-1-3 and IEC 60601-1-10 do not apply. All other published collateral standards in the IEC 60601-1 series apply as published.

201.1.4 Particular standards

Replacement:

In the IEC 60601 series, particular standards may modify, replace or delete requirements contained in the general standard and collateral standards as appropriate for the particular ME EQUIPMENT under consideration, and may add other BASIC SAFETY and ESSENTIAL PERFORMANCE requirements.

A requirement of a particular standard takes priority over the general standard.

For brevity, IEC 60601-1:2005 and IEC 60601-1:2005/AMD1:2012 are referred to in this particular standard as the general standard. Collateral standards are referred to by their document number.

The numbering of clauses and subclauses of this particular standard corresponds to that of the general standard with the prefix "201" (e.g. 201.1 in this document addresses the content of Clause 1 of the general standard) or applicable collateral standard with the prefix "20x" where x is the final digit(s) of the collateral standard document number (e.g. 202.4 in this particular standard addresses the content of Clause 4 of the IEC 60601-1-2 collateral standard, 203.4 in this particular standard addresses the content of Clause 4 of the IEC 60601-1-3 collateral standard, etc.). The changes to the text of the general standard and applicable collateral standards are specified by the use of the following words:

"*Replacement*" means that the clause or subclause of the general standard or applicable collateral standard is replaced completely by the text of this particular standard.

"*Addition*" means that the text of this particular standard is additional to the requirements of the general standard or applicable collateral standard.

"*Amendment*" means that the clause or subclause of the general standard or applicable collateral standard is amended as indicated by the text of this particular standard.

Subclauses, figures or tables which are additional to those of the general standard are numbered starting from 201.101. However, due to the fact that definitions in the general standard are numbered 3.1 through ~~3.139~~ 3.147, additional definitions in this document are numbered beginning from 201.3.201. Additional annexes are lettered AA, BB, etc., and additional items aa), bb), etc.

Subclauses, figures or tables which are additional to those of a collateral standard are numbered starting from 20x, where "x" is the number of the collateral standard, e.g. 202 for IEC 60601-1-2, 203 for IEC 60601-1-3, etc.

The term "this document" is used to make reference to the general standard, any applicable collateral standards and this particular standard taken together.

Where there is no corresponding clause or subclause in this particular standard, the clause or subclause of the general standard or applicable collateral standard, although possibly not relevant, applies without modification; where it is intended that any part of the general standard or applicable collateral standard, although possibly relevant, is not to be applied, a statement to that effect is given in this particular standard.

201.2 Normative references

NOTE Informative references are listed in the Bibliography.

Clause 2 of the general standard applies, except as follows:

Amendment:

~~IEC 60601-1-2:2007, Medical electrical equipment – Part 1-2: General requirements for basic safety and essential performance – Collateral standard: Electromagnetic compatibility – Requirements and tests~~

Addition:

~~IEC 60601-1-10:2007, Medical electrical equipment – Part 1-10: General requirements for basic safety and essential performance – Collateral Standard: Requirements for the development of physiologic closed-loop controllers~~

Addition:

IEC 60601-1:2005, Medical electrical equipment – Part 1: General requirements for basic safety and essential performance
IEC 60601-1:2005/AMD1:2012

Replacement:

IEC 60601-1-2:2014, Medical electrical equipment – Part 1-2: General requirements for basic safety and essential performance – Collateral Standard: Electromagnetic disturbances – Requirements and tests

201.3 Terms and definitions

~~For the purposes of this document, the terms and definitions given in the general standard apply, except as follows:~~

For the purposes of this document, the terms and definitions specified in IEC 60601-1:2005 and IEC 60601-1:2005/AMD1:2012, and the following apply.

ISO and IEC maintain terminological databases for use in standardization at the following addresses:

- IEC Electropedia: available at <http://www.electropedia.org/>
- ISO Online browsing platform: available at <http://www.iso.org/obp>

NOTE An index of defined terms is found beginning on page 35.

Addition:

201.3.201

BABY CONTROLLED RADIANT WARMER

mode of operation in which the power output varies automatically in order to maintain the temperature as measured by a SKIN TEMPERATURE SENSOR according to the CONTROL TEMPERATURE set by the OPERATOR

~~NOTE An INFANT RADIANT WARMER operating as a BABY CONTROLLED RADIANT WARMER is a PHYSIOLOGIC CLOSED-LOOP CONTROLLER as defined in IEC 60601-1-10.~~

201.3.202

CONTROL TEMPERATURE

temperature selected at the temperature control

201.3.203

INFANT

PATIENT up to 3 months and with a weight of less than 10 kg

201.3.204

INFANT RADIANT WARMER

electrically powered device with a radiant heating source intended to maintain the thermal balance of an INFANT by direct radiation of energy in the infrared region of the electromagnetic spectrum

201.3.205

MANUAL MODE


mode of operation in which the heater output is either at a fixed level or a proportion of its maximum output set by the OPERATOR

201.3.206

MID-POINT AVERAGE TEMPERATURE

T_M

~~TEST DEVICE~~ AVERAGE TEMPERATURE of the TEST DEVICE positioned at the mid-point of the INFANT RADIANT WARMER MATTRESS (see Figure 201.101)

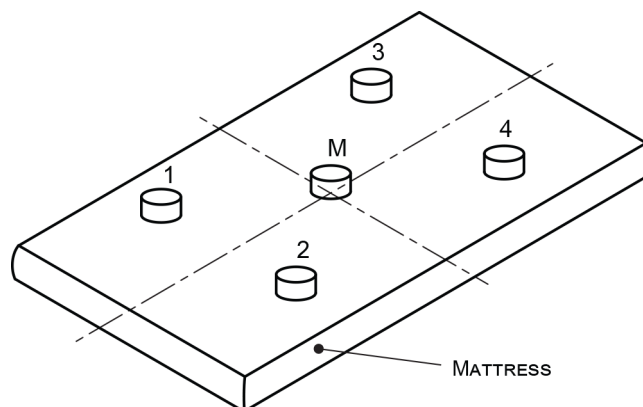

Key

~~1 = Mattress~~

Figure 201.101 – Layout of TEST DEVICES

201.3.207***PREWARM MODE**

mode of operation in which the heater output is maintained at a preset level (set by the MANUFACTURER) for the purpose of pre-warming the INFANT RADIANT WARMER and maintaining the level of warmth of the INFANT RADIANT WARMER prior to an INFANT being placed on the device

201.3.208**SKIN TEMPERATURE SENSOR**

sensing device intended to measure the INFANT'S SKIN TEMPERATURE


201.3.209**STEADY TEMPERATURE CONDITION**

condition which is reached when the temperature, measured at the centre of the TEST DEVICE positioned on the mid-point of the INFANT RADIANT WARMER MATTRESS, does not vary by more than 1 °C over a period of 1 h

201.3.210**TEST DEVICE**

totally matt blackened disc used as a reproducible receiver of radiant energy during testing of the INFANT RADIANT WARMER (see Figure 201.102)

Dimensions in millimetres

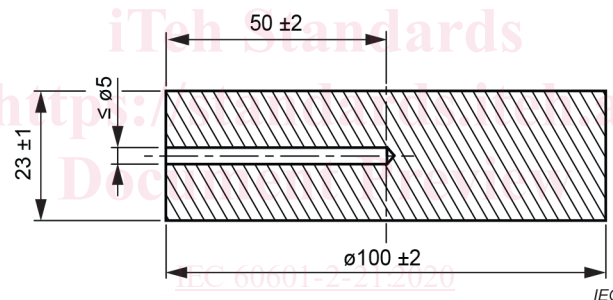

<https://standards.iteh.ai/catalog/standards/iec/9373f8a7-f219-4195-b237-7b20917f5eb9/iec-60601-2-21-2020>

Key

1 = Mattress

Surface finish: non-reflective black paint

Disc mass: 500 g ± 10 g

Disc material: aluminium of density within the range 2,6 g/cm³ and 2,9 g/cm³

Figure 201.102 – TEST DEVICE

201.3.211**TEST DEVICE AVERAGE TEMPERATURE**

$(T_1, T_2, T_3, T_4 \text{ OR } T_M)$

AVERAGE TEMPERATURE reading taken during a STEADY TEMPERATURE CONDITION at regular intervals at the centre of a TEST DEVICE

Note 1 to entry: T_M, T_1, T_2, T_3, T_4 , are expressed in °C.

201.3.212*** TEST LOAD**

array of five TEST DEVICES used in a specified configuration (see Figure 201.101) for performance tests of the INFANT RADIANT WARMER

201.4 General requirements

Clause 4 of the general standard applies, except as follows:

201.4.1 Conditions for application to ME EQUIPMENT or ME SYSTEMS

Addition:

For ME EQUIPMENT or ME SYSTEMS, which combines alternative heat sources, for instance incubators with integrated INFANT RADIANT WARMERS, devices supplying heat via BLANKETS, PADS or MATTRESSES etc., safety requirements of other relevant particular standards shall be considered. Further the safety requirements of this document shall be fulfilled with the combination of the other equipment, which is approved by the MANUFACTURER, as stated in the ACCOMPANYING DOCUMENTS according to Clause 16-~~(ME SYSTEMS)~~.

Compliance is checked by the test of Clause 201.11 and 201.15.4.2.1 of the relevant particular standards (e.g. IEC 60601-2-19:2020, etc.).

201.4.3 ESSENTIAL PERFORMANCE

Addition:

201.4.3.101 * Additional ESSENTIAL PERFORMANCE requirements

Additional ESSENTIAL PERFORMANCE requirements are found in the subclauses listed in Table 201.101.

Table 201.101 – Additional ESSENTIAL PERFORMANCE requirements

Requirement	Subclause
ESSENTIAL PERFORMANCE requirement 1	201.12.1.103, and generation of a visual and audible alarm in compliance with 201.15.4.2.1

201.5 General requirements for testing ~~of~~ ME EQUIPMENT

Clause 5 of the general standard applies, except as follows:

201.5.3 * Ambient temperature, humidity, atmospheric pressure

Addition to item a):

The ME EQUIPMENT shall comply with the requirements of this document when operating within the following conditions:

- an ambient temperature within the range 18 °C to 30 °C;
- an ambient air velocity is less than 0,3 m/s.

If not otherwise specified in this document, all tests shall be carried out at an ambient temperature within the range of 21 °C to 26 °C.

201.5.4 Other conditions

Addition:

Additional item to the existing list: