

TECHNICAL REPORT



Electronic displays – **STANDARD PREVIEW**
Part 1-31: Generic – Practical information on the use of light measuring devices
(standards.iteh.ai)

[IEC TR 62977-1-31:2021](https://standards.iteh.ai/catalog/standards/sist/1385a523-d79f-4db0-8935-cb951a3f6747/iec-tr-62977-1-31-2021)

<https://standards.iteh.ai/catalog/standards/sist/1385a523-d79f-4db0-8935-cb951a3f6747/iec-tr-62977-1-31-2021>



THIS PUBLICATION IS COPYRIGHT PROTECTED
Copyright © 2021 IEC, Geneva, Switzerland

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either IEC or IEC's member National Committee in the country of the requester. If you have any questions about IEC copyright or have an enquiry about obtaining additional rights to this publication, please contact the address below or your local IEC member National Committee for further information.

IEC Central Office
3, rue de Varembe
CH-1211 Geneva 20
Switzerland

Tel.: +41 22 919 02 11
info@iec.ch
www.iec.ch

About the IEC

The International Electrotechnical Commission (IEC) is the leading global organization that prepares and publishes International Standards for all electrical, electronic and related technologies.

About IEC publications

The technical content of IEC publications is kept under constant review by the IEC. Please make sure that you have the latest edition, a corrigendum or an amendment might have been published.

IEC publications search - webstore.iec.ch/advsearchform

The advanced search enables to find IEC publications by a variety of criteria (reference number, text, technical committee, ...). It also gives information on projects, replaced and withdrawn publications.

IEC online collection - oc.iec.ch

Discover our powerful search engine and read freely all the publications previews. With a subscription you will always have access to up to date content tailored to your needs.

IEC Just Published - webstore.iec.ch/justpublished

Stay up to date on all new IEC publications. Just Published details all new publications released. Available online and once a month by email.

Electropedia - www.electropedia.org

The world's leading online dictionary on electrotechnology, containing more than 22 000 terminological entries in English and French, with equivalent terms in 18 additional languages. Also known as the International Electrotechnical Vocabulary (IEV) online.

IEC Customer Service Centre - webstore.iec.ch/csc

If you wish to give us your feedback on this publication or need further assistance, please contact the Customer Service Centre: sales@iec.ch.

www.iec.ch IEC TR 62977-1-31:2021

<https://standards.iteh.ai/catalog/standards/sis/1385a523-d79f-4db0-8935-cb951a3f6747/iec-tr-62977-1-31-2021>

TECHNICAL REPORT



Electronic displays – **STANDARD PREVIEW**
Part 1-31: Generic – Practical information on the use of light measuring devices
(standards.iteh.ai)

[IEC TR 62977-1-31:2021](https://standards.iteh.ai/catalog/standards/sist/1385a523-d79f-4db0-8935-cb951a3f6747/iec-tr-62977-1-31-2021)

<https://standards.iteh.ai/catalog/standards/sist/1385a523-d79f-4db0-8935-cb951a3f6747/iec-tr-62977-1-31-2021>

INTERNATIONAL
ELECTROTECHNICAL
COMMISSION

ICS 31.120; 31.260

ISBN 978-2-8322-9716-2

Warning! Make sure that you obtained this publication from an authorized distributor.

CONTENTS

| | |
|--|----|
| FOREWORD..... | 6 |
| INTRODUCTION..... | 8 |
| 1 Scope..... | 9 |
| 2 Normative references | 9 |
| 3 Terms, definitions, and abbreviated terms | 9 |
| 3.1 Terms and definitions..... | 9 |
| 3.2 Abbreviated terms..... | 10 |
| 4 General information on LMDs for photometry and colorimetry | 10 |
| 4.1 General..... | 10 |
| 4.2 Photometry and colorimetry for electronic displays..... | 10 |
| 4.3 LMDs for luminance and chromaticity measurements | 11 |
| 4.3.1 Configuration of LMDs | 11 |
| 4.3.2 Input optics of LMDs | 13 |
| 4.3.3 Electronic system of LMDs | 13 |
| 4.3.4 Calibration of LMDs | 14 |
| 4.3.5 Maintenance of LMDs | 14 |
| 4.4 Setup conditions for measurement | 14 |
| 4.4.1 LMDs..... | 14 |
| 4.4.2 DUTs..... | 14 |
| 4.4.3 Environment | 14 |
| 5 Influence of LMD properties on luminance and chromaticity measurements | 14 |
| 5.1 General..... | 14 |
| 5.2 Repeatability..... | 15 |
| 5.2.1 General | 15 |
| 5.2.2 Example of the repeatability of an LMD..... | 15 |
| 5.3 Accuracy..... | 16 |
| 5.3.1 General | 16 |
| 5.3.2 Example of the accuracy of an LMD..... | 16 |
| 5.3.3 Linearity | 16 |
| 5.3.4 Range change | 17 |
| 5.4 Luminance range | 17 |
| 5.5 Spectral properties of the spectroradiometer..... | 17 |
| 5.5.1 General | 17 |
| 5.5.2 Wavelength accuracy and spectral bandwidth..... | 17 |
| 5.6 Spectral properties of the filter-type luminance meter and colorimeter | 23 |
| 5.6.1 General | 23 |
| 5.6.2 Spectral responsivity | 23 |
| 5.6.3 Methods to reduce the measurement difference..... | 25 |
| 5.7 Angular response of LMDs..... | 26 |
| 5.7.1 General | 26 |
| 5.7.2 Subtended angles..... | 26 |
| 5.7.3 Consideration of the input optics..... | 27 |
| 5.8 Measurement field | 28 |
| 5.8.1 General | 28 |
| 5.8.2 Number of pixels within the measurement field | 29 |
| 5.9 Polarization..... | 29 |

ITeH STANDARD PREVIEW
(standards.iteh.ai)

IEC TR 62977-1-31:2021
<https://standards.iteh.ai/catalog/standards/sist/1385a523-d79f-4db0-8935-cb951a316747/iec-tr-62977-1-31-2021>

| | | |
|-----------------------|---|----|
| 5.9.1 | General | 29 |
| 5.9.2 | Polarization dependence of LMDs..... | 30 |
| 5.10 | Temporal synchronization | 31 |
| 5.10.1 | General | 31 |
| 5.10.2 | Temporal synchronization of the LMD and DUT | 31 |
| 6 | Influence of LMD properties on measurements of the optical characteristics of electronic displays | 32 |
| 6.1 | General..... | 32 |
| 6.2 | Contrast ratio | 32 |
| 6.2.1 | General | 32 |
| 6.2.2 | Calculated influence of LMD properties on the contrast ratio measurements | 32 |
| 6.3 | Electro-optical transfer function (EOTF) | 35 |
| 6.3.1 | General | 35 |
| 6.3.2 | Calculated influence of the LMD properties on the EOTF measurements | 35 |
| 6.4 | Chromaticity gamut area | 36 |
| 6.4.1 | General | 36 |
| 6.4.2 | Calculated influence of LMD properties on the chromaticity gamut area measurements | 36 |
| 6.5 | Viewing direction characteristics | 38 |
| 6.5.1 | General | 38 |
| 6.5.2 | Calculated influence of the LMD properties on the viewing direction characteristics | 38 |
| 6.5.3 | Measurement field at an oblique direction..... | 40 |
| 6.6 | Spatial uniformity | 41 |
| 6.6.1 | General | 41 |
| 6.6.2 | Calculated influence of LMD properties on uniformity and non-uniformity measurements | 41 |
| 6.7 | Response time | 43 |
| 6.7.1 | General | 43 |
| 6.7.2 | Measurement of the response time | 43 |
| 6.8 | Flicker..... | 46 |
| 6.8.1 | General | 46 |
| 6.8.2 | Measurement method of the flicker | 46 |
| 6.8.3 | Low-pass filter of LMDs | 47 |
| Annex A (informative) | Photometry and colorimetry | 49 |
| A.1 | General..... | 49 |
| A.2 | Photometry | 49 |
| A.3 | Colorimetry | 49 |
| A.3.1 | General | 49 |
| A.3.2 | Standard colorimetric observer | 50 |
| A.3.3 | Tristimulus values..... | 50 |
| A.3.4 | Chromaticity diagram and colour space | 50 |
| Annex B (informative) | Method for reducing the measurement difference of colorimeters | 53 |
| B.1 | General..... | 53 |
| B.2 | Matrix calibration methods for colorimeters | 53 |
| B.2.1 | Matrix calibration process 1: RGB calibration..... | 53 |
| B.2.2 | Matrix calibration process 2: RGBW calibration | 54 |

| | |
|--|----|
| Annex C (informative) Input data in Clause 5 and Clause 6, and calculation methods in 5.8 and 6.5..... | 56 |
| C.1 General..... | 56 |
| C.2 Characteristics of DUTs | 56 |
| C.2.1 Spectral radiances of the DUTs | 56 |
| C.2.2 Directional characteristic of the DUT..... | 57 |
| C.2.3 Temporal modulation characteristics of the DUT | 57 |
| C.2.4 EOTF characteristics of the DUTs..... | 57 |
| C.2.5 Uniformity characteristics of the DUTs | 58 |
| C.3 Characteristics of the filter-type LMDs | 59 |
| C.3.1 Spectral responsivities of the filter-type LMDs | 59 |
| C.3.2 Specifications of filter-type LMDs..... | 61 |
| C.4 Influence of the number of pixels within the measurement field | 63 |
| C.5 Validity of the viewing direction dependence obtained by a simplified method | 64 |
| Annex D (informative) Instabilities of DUTs in measurement | 66 |
| D.1 General..... | 66 |
| D.2 DUT instabilities..... | 66 |
| Bibliography..... | 68 |
| | |
| Figure 1 – Block diagrams of three types of LMDs | 12 |
| Figure 2 – Example of configurations for the input optics and detector | 12 |
| Figure 3 – Example of input optics for the luminance meters..... | 13 |
| Figure 4 – Block diagram of a typical electronic system | 13 |
| Figure 5 – Examples of the repeatability of an LMD as a function of luminance | 15 |
| Figure 6 – Examples of the accuracy of an LMD as a function of luminance | 16 |
| Figure 7 – Calculated relative luminance difference as a function of wavelength error | 19 |
| Figure 8 – Calculated relative luminance difference as a function of spectral bandwidth | 20 |
| Figure 9 – Calculated chromaticity differences as a function of wavelength error | 21 |
| Figure 10 – Calculated chromaticity differences as a function of spectral bandwidth | 22 |
| Figure 11 – Calculated relative luminance difference as a function of f_1' | 24 |
| Figure 12 – Calculated chromaticity differences as a function of f_1' , xyz | 25 |
| Figure 13 – Angular aperture and measurement field angle | 27 |
| Figure 14 – Calculated relative luminance difference and chromaticity difference as a function of the angular aperture | 27 |
| Figure 15 – Diagram of light rays in object space telecentric and non-telecentric optical design..... | 28 |
| Figure 16 – Calculated chromaticity difference as a function of the number of pixels | 29 |
| Figure 17 – Measured luminance variation as a function of the rotation angle of the polarizer | 30 |
| Figure 18 – Calculated relative luminance differences as a function of sampling period | 32 |
| Figure 19 – Total measurement times for 0,3 % repeatability (2σ) in three LMDs | 36 |
| Figure 20 – Calculated relative difference, ΔGA_{xy} , by spectroradiometers | 37 |
| Figure 21 – Calculated relative difference, ΔGA_{xy} , by colorimeters | 38 |
| Figure 22 – Cone of light rays for calculating the tristimulus values measured by an LMD with the angular aperture, α , and an optical axis at an inclination angle, θ_{LMD} | 39 |

| | |
|--|----|
| Figure 23 – Calculated luminance and chromaticity dependence as a function of the inclination angle for the 2°, 6°, and 10° angular apertures..... | 40 |
| Figure 24 – Measurement field and test pattern | 41 |
| Figure 25 – Calculated non-uniformity difference by the filter-type colorimeters | 43 |
| Figure 26 – Measurement setups for response time measurements | 44 |
| Figure 27 – Response curves measured at different sampling rates..... | 44 |
| Figure 28 – Measured response subjected to various low-pass filterings..... | 45 |
| Figure 29 – Measured response curves switched from the 10 % to 90 % level | 46 |
| Figure 30 – Schematic measured temporal luminance modulation of the LCD with a common voltage offset..... | 47 |
| Figure 31 – Conceptual pseudo-temporal luminance modulation | 48 |
| Figure 32 – Simulated luminance modulations with and without high frequency noise | 48 |
| Figure C.1 – Spectral radiances..... | 56 |
| Figure C.2 – Inclination angle dependence | 57 |
| Figure C.3 – Temporal modulation of the luminance | 57 |
| Figure C.4 – EOTF characteristics | 58 |
| Figure C.5 – Spectral responsivity of the colorimeter | 61 |
| Figure C.6 – Repeatability of three LMD models | 62 |
| Figure C.7 – Three positions of a circular measurement field relative to the RGB stripes | 63 |
| Figure C.8 – Configuration to measure DUT emission by the LMD at the inclination angle, θ_{LMD} | 64 |
| Figure C.9 – Inclination angle dependence calculated by two methods using an LMD with an angular aperture of 10° | 65 |
| Figure D.1 – Changes of luminance and chromaticity after switching the grey levels..... | 66 |
| Figure D.2 – Changes of luminance after switching from the black to grey level..... | 67 |
| | |
| Table 1 – DUT characteristics for the calculations..... | 33 |
| Table 2 – Calculated results of the contrast ratio by three LMDs | 34 |
| Table 3 – Calculated durations of the EOTF measurements | 36 |
| Table 4 – Chromaticity gamut area of three DUTs | 37 |
| Table 5 – Non-uniformity of DUTs | 42 |
| Table 6 – Rise times calculated from a measured response subjected to various low-pass filterings | 45 |
| Table 7 – Rise times measured by LMDs of various $V(\lambda)$ fidelities | 46 |
| Table C.1 – Measured luminance and chromaticity at the nine positions of DUT-1 | 58 |
| Table C.2 – Measured luminance and chromaticity at the nine positions of DUT-2 | 59 |
| Table C.3 – Specifications of filter-type LMDs..... | 62 |
| Table D.1 – Luminance and chromaticity transition | 66 |
| Table D.2 – Luminance changes in two measurements | 67 |

INTERNATIONAL ELECTROTECHNICAL COMMISSION

ELECTRONIC DISPLAYS –

**Part 1-31: Generic –
Practical information on the use of light measuring devices**

FOREWORD

- 1) The International Electrotechnical Commission (IEC) is a worldwide organization for standardization comprising all national electrotechnical committees (IEC National Committees). The object of IEC is to promote international co-operation on all questions concerning standardization in the electrical and electronic fields. To this end and in addition to other activities, IEC publishes International Standards, Technical Specifications, Technical Reports, Publicly Available Specifications (PAS) and Guides (hereafter referred to as "IEC Publication(s)"). Their preparation is entrusted to technical committees; any IEC National Committee interested in the subject dealt with may participate in this preparatory work. International, governmental and non-governmental organizations liaising with the IEC also participate in this preparation. IEC collaborates closely with the International Organization for Standardization (ISO) in accordance with conditions determined by agreement between the two organizations.
- 2) The formal decisions or agreements of IEC on technical matters express, as nearly as possible, an international consensus of opinion on the relevant subjects since each technical committee has representation from all interested IEC National Committees.
- 3) IEC Publications have the form of recommendations for international use and are accepted by IEC National Committees in that sense. While all reasonable efforts are made to ensure that the technical content of IEC Publications is accurate, IEC cannot be held responsible for the way in which they are used or for any misinterpretation by any end user.
- 4) In order to promote international uniformity, IEC National Committees undertake to apply IEC Publications transparently to the maximum extent possible in their national and regional publications. Any divergence between any IEC Publication and the corresponding national or regional publication shall be clearly indicated in the latter.
- 5) IEC itself does not provide any attestation of conformity. Independent certification bodies provide conformity assessment services and, in some areas, access to IEC marks of conformity. IEC is not responsible for any services carried out by independent certification bodies.
- 6) All users should ensure that they have the latest edition of this publication.
- 7) No liability shall attach to IEC or its directors, employees, servants or agents including individual experts and members of its technical committees and IEC National Committees for any personal injury, property damage or other damage of any nature whatsoever, whether direct or indirect, or for costs (including legal fees) and expenses arising out of the publication, use of, or reliance upon, this IEC Publication or any other IEC Publications.
- 8) Attention is drawn to the Normative references cited in this publication. Use of the referenced publications is indispensable for the correct application of this publication.
- 9) Attention is drawn to the possibility that some of the elements of this IEC Publication may be the subject of patent rights. IEC shall not be held responsible for identifying any or all such patent rights.

IEC TR 62977-1-31 has been prepared by IEC technical committee 110: Electronic displays. It is a Technical Report.

The text of this Technical Report is based on the following documents:

| DTR | Report on voting |
|--------------|------------------|
| 110/1258/DTR | 110/1281A/RVDTR |

Full information on the voting for its approval can be found in the report on voting indicated in the above table.

The language used for the development of this Technical Report is English.

This document was drafted in accordance with ISO/IEC Directives, Part 2, and developed in accordance with ISO/IEC Directives, Part 1 and ISO/IEC Directives, IEC Supplement, available at www.iec.ch/members_experts/refdocs. The main document types developed by IEC are described in greater detail at www.iec.ch/standardsdev/publications.

A list of all parts in the IEC 62977 series, published under the general title *Electronic displays*, can be found on the IEC website.

The committee has decided that the contents of this document will remain unchanged until the stability date indicated on the IEC website under "<http://webstore.iec.ch>" in the data related to the specific document. At this date, the document will be

- reconfirmed,
- withdrawn,
- replaced by a revised edition, or
- amended.

IMPORTANT – The 'colour inside' logo on the cover page of this publication indicates that it contains colours which are considered to be useful for the correct understanding of its contents. Users should therefore print this document using a colour printer.

iTeh STANDARD PREVIEW
(standards.iteh.ai)

[IEC TR 62977-1-31:2021](https://standards.iteh.ai/catalog/standards/sist/1385a523-d79f-4db0-8935-cb951a3f6747/iec-tr-62977-1-31-2021)

<https://standards.iteh.ai/catalog/standards/sist/1385a523-d79f-4db0-8935-cb951a3f6747/iec-tr-62977-1-31-2021>

INTRODUCTION

Measurements of the optical characteristics of electronic displays are primarily affected by three factors: measuring procedures, displays (devices under test: DUTs), and light measuring devices (LMDs), for which there are many international standards supporting consistent and comparable measurements. Most of them, however, provide only limited information on LMDs, making it difficult to appropriately select and use the LMD for the measurement objective. The purpose of this document is to provide best practices and suggestions which are missing in the standards.

This document addresses how the major properties of a typical LMD affect the measurement results. It is often impractical and unnecessary to consider the influences of all properties of LMDs and all characteristics of DUTs as well as their interactions and influences on the measurement results. Therefore, the multiple interaction effects that exist are beyond the scope of this document. Due to the rapid innovation and abundance of LMDs, covering all types of LMDs is also outside the objectives of this document.

iTeh STANDARD PREVIEW **(standards.iteh.ai)**

[IEC TR 62977-1-31:2021](https://standards.iteh.ai/catalog/standards/sist/1385a523-d79f-4db0-8935-cb951a3f6747/iec-tr-62977-1-31-2021)

<https://standards.iteh.ai/catalog/standards/sist/1385a523-d79f-4db0-8935-cb951a3f6747/iec-tr-62977-1-31-2021>

ELECTRONIC DISPLAYS –

Part 1-31: Generic – Practical information on the use of light measuring devices

1 Scope

This part of IEC 62977 provides practical information on light measuring devices (luminance meters, colorimeters, and spectroradiometers) with luminance measuring optics for the characterization of electronic displays.

2 Normative references

There are no normative references in this document.

3 Terms, definitions, and abbreviated terms

3.1 Terms and definitions

For the purposes of this document, the following terms and definitions apply.

ISO and IEC maintain terminological databases for use in standardization at the following addresses:

- ISO Online browsing platform: available at <http://www.iso.org/obp>
- IEC Electropedia: available at <http://www.electropedia.org/>

NOTE CIE Electronic international lighting vocabulary (e-ILV) is also available at <http://cie.co.at/e-ilv>.

3.1.1

repeatability

<of an LMD> closeness of agreement between indications or measured quantity values obtained by replicated measurements over a short period of time using a specific LMD under conditions specified by the LMD manufacturer

Note 1 to entry: Repeatability of an LMD is usually expressed numerically by statistical quantities, such as standard deviation, variance, or coefficient of variation (relative standard deviation) under the specified conditions of measurement.

Note 2 to entry: The influence on measurement repeatability caused by fluctuations of the measured light source and by the measurement procedure is assumed to be negligible when the manufacturer specifies the repeatability of an LMD. Manufacturers often specify the type of light source and measurement conditions used for determining the repeatability of an LMD.

Note 3 to entry: Measurement precision is the closeness of agreement between indications or measured quantity values obtained by replicate measurements on the same or similar objects under specified conditions. Measurement repeatability is measurement precision under a set of repeatability conditions of measurement that includes the same measurement procedures, same operators, same measuring system, same operating conditions, same location, and replicate measurements on the same or similar objects over a short period of time. Measurement reproducibility is measurement precision under a set of reproducibility conditions of measurement that includes different locations, operators, measuring systems, and replicate measurements on the same or similar objects [1], [2]¹.

¹ Numbers in square brackets refer to the Bibliography.

3.1.2

accuracy

<of an LMD> difference between a measured quantity value and an accepted reference value when using a specific LMD under conditions specified by the LMD manufacturer

Note 1 to entry: This term is a quantity with a numerical value and is usually expressed as a range specification.

Note 2 to entry: The accepted reference value is a value that serves as an agreed-upon reference for comparison, and which is derived as:

- a) a theoretical or established value, based on scientific principles;
- b) an assigned or certified value, based on experimental work of some national or international organization;
- c) a consensus or certified value, based on collaborative experimental work under the auspices of a scientific or engineering group;
- d) (when a), b) and c) are not available) the expectation of the (measurable) quantity, i.e. the mean of a specified population of measurements [3].

Note 3 to entry: The influence on measurement accuracy caused by fluctuations of the measured light source and by the measurement procedure is assumed to be negligible when the manufacturer specifies the accuracy of an LMD. Manufacturers often specify the type of light source and other measurement conditions used for determining the accuracy of an LMD.

Note 4 to entry: Measurement accuracy is the closeness of agreement between a measured quantity value and the true quantity value of a measurand [1], [2]. The accuracy of measurement is not a quantity value while the accuracy of an LMD is a quantity value; thus, the term "accuracy" conventionally used for the specification of LMDs means something different than that used for measurement.

3.2 Abbreviated terms

| | |
|-------|---|
| CIE | Commission Internationale de l'Éclairage (International Commission on Illumination) |
| CMF | colour-matching function |
| DUT | device under test |
| EOTF | electro-optical transfer function |
| LCD | liquid crystal display |
| LED | light emitting diode |
| LMD | light measuring device |
| ND | neutral density |
| OLED | organic light emitting diode |
| PWM | pulse width modulation |
| RGB | red, green, and blue |
| RGBW | red, green, blue, and white |
| Vsync | vertical synchronizing signal |

4 General information on LMDs for photometry and colorimetry

4.1 General

Clause 4 describes the principles of photometry and colorimetry, configuration, calibration, and maintenance of LMDs, as well as setup conditions for measurement.

4.2 Photometry and colorimetry for electronic displays

Photometry is the measurement of quantities referring to radiation as evaluated according to a given spectral luminous efficiency (see IEC 845-25-013). Colorimetry is the measurement of colour stimuli based on a set of conventions (see IEC 845-25-014). Details on the calculation formulae and specific conditions applied to electronic display measurement are shown in Annex A.

4.3 LMDs for luminance and chromaticity measurements

4.3.1 Configuration of LMDs

The configurations of three types of LMDs are described as follows:

1) Luminance meter

A luminance meter is an instrument for measuring luminance (see IEC 845-25-021). A block diagram of the setup of a typical luminance meter is shown in Figure 1a): it consists of input optics, a detector unit for measuring the luminance, L_v , and an electronic system. An example of the configuration of the input optics and the detector unit is shown in Figure 2a), where a lens is used for the input optics. The input optics collects the light emitted from the DUT and converges it onto the detector. An optical compensation filter is arranged in front of the detector. The combination of the spectral characteristics of the filter, input optics, and detector approximates the spectral luminous efficiency function, $V(\lambda)$. A neutral density (ND) filter can be inserted into the optical path, for example when the LMD's dynamic range is insufficient and results in detector saturation. The detector receives the light and converts the optical signal to an electronic one, from which the electronic system calculates the luminance, L_v , as in [4], indicates it on an instrument display, and/or sends the result to an external system.

2) Colorimeter

A colorimeter is an instrument for measuring colorimetric quantities, such as the tristimulus values of a colour stimulus (see IEC 845-25-022). A block diagram of the most common setup for a colorimeter is shown in Figure 1b): it is conceptually similar to a luminance meter. A colorimeter has a detector unit for measuring the tristimulus values instead of one for the luminance. A colorimeter for both luminance and chromaticity measurements employs the same type of input optics as the luminance meter, as described in 4.3.1 1). An example of the configuration of the input optics and the detector unit is shown in Figure 2b), where the detector unit has three pairs of optical compensation filters and detectors. The input optics is connected to the detector unit by a three-branch optical fibre. The combined spectral characteristics of those components approximates the CIE colour-matching functions (CMFs). The electronic system calculates the tristimulus values, X , Y , and Z , where Y is practically identical to L_v (see Annex A).

3) Spectroradiometer

A spectroradiometer is an instrument for measuring radiometric quantities in narrow wavelength intervals over a given spectral region (see IEC 845-25-007). A block diagram of the general setup of a spectroradiometer is shown in Figure 1c). A spectroradiometer for spectral radiance measurements, and luminance and chromaticity calculations therefrom, employs the same type of input optics as the luminance meter, as described in 4.3.1 1). An example of the configuration of the input optics and the spectrometer is shown in Figure 2c), where the input optics is connected to the spectrometer by an optical fibre. The example spectrometer consists of an input slit, a grating, for example a concave grating [5], and an array detector, where the output of the detector is related to the spectral radiance of the DUT. The obtained spectral radiance, $L_e(\lambda)$, is converted to the luminance, L_v , or tristimulus values, X , Y , and Z , using $V(\lambda)$ or CMFs data, which are often stored in look-up tables [6], [7].

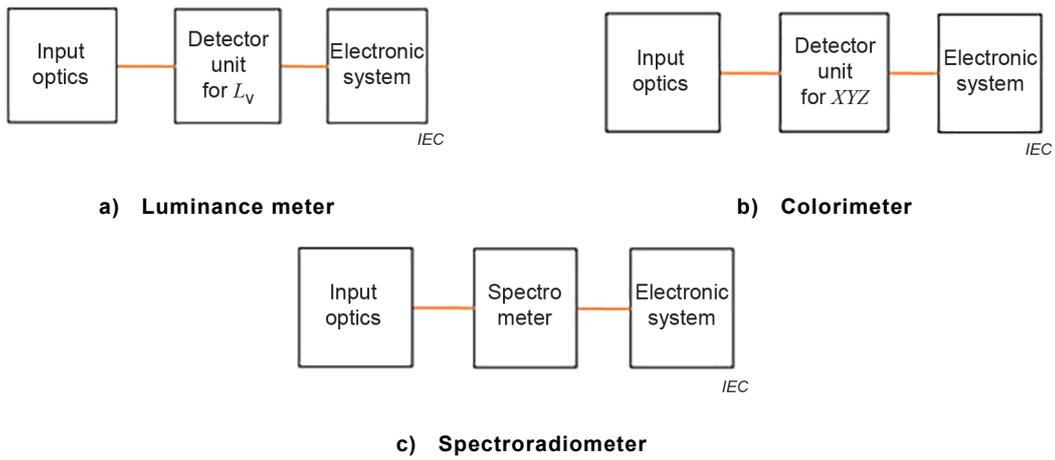


Figure 1 – Block diagrams of three types of LMDs


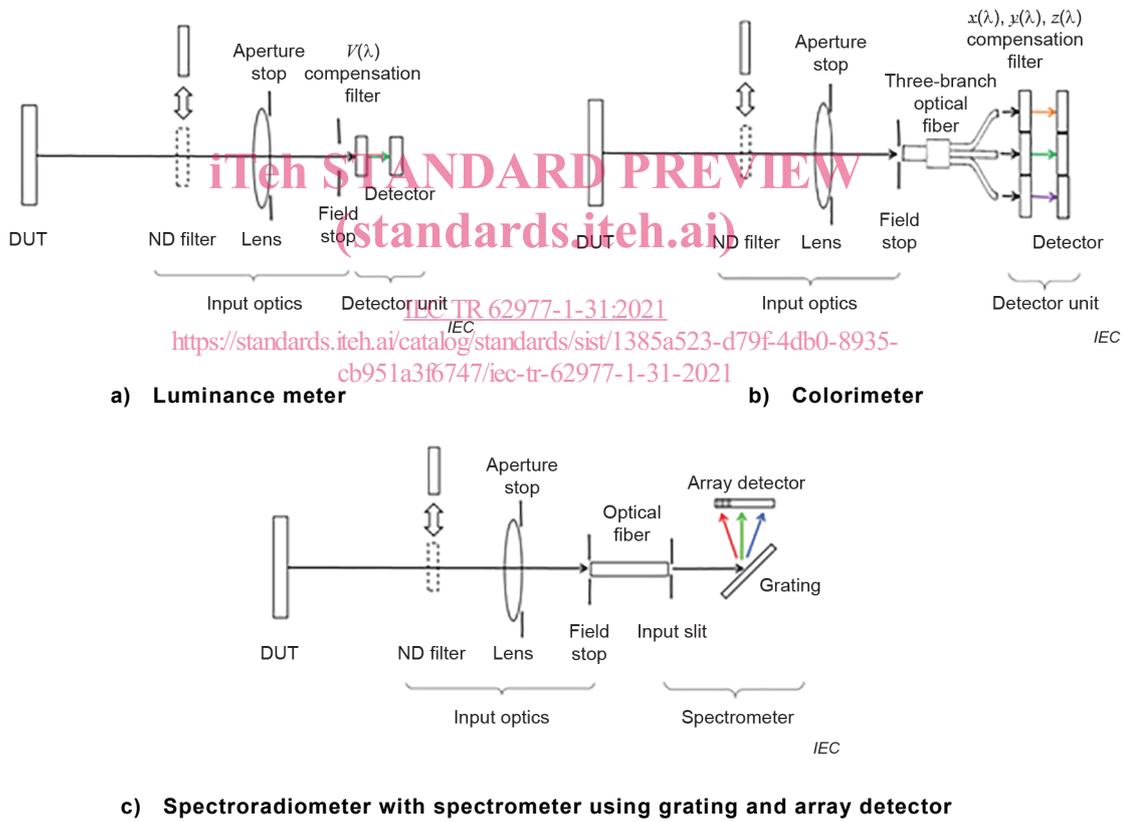


Figure 2 – Example of configurations for the input optics and detector

4.3.2 Input optics of LMDs

An LMD has an input optics system which collects the light emitted or reflected from a DUT. There are various types of imaging as well as non-imaging input optics, for example fixed-focus lens, variable-focus lens, and optical fibre. For luminance measurements, imaging optics is often used. Figure 3 shows an example of the input optics with an imaging lens, an aperture stop (aperture), a field stop, and a detector behind the field stop, together with the DUT and detector. Related optical properties are described in the following sentences. The aperture stop is an opening that defines the area over which the average optical emission is measured (see IEC 845-25-086). The entrance pupil is a virtual image of the aperture stop as viewed from the object space, and its position and size depend on the measurement distance. The angular aperture is the angle subtended by the entrance pupil. The field stop which is positioned on the image plane limits the measurement field of the DUT. The measurement field angle is the angle subtended by the measurement field at the entrance pupil.

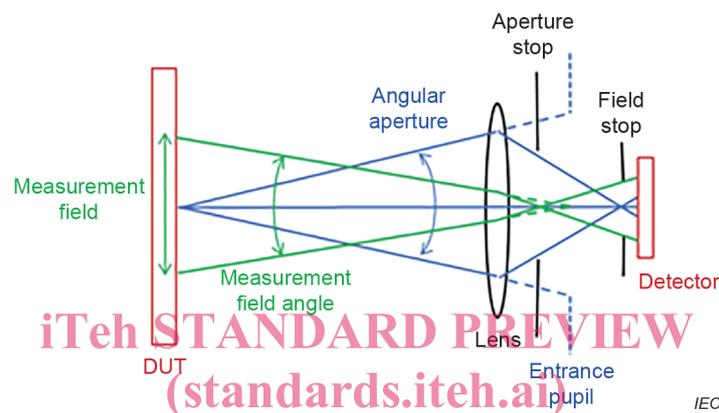


IEC TR 62977-1-31:2021

Figure 3 – Example of input optics for the luminance meters

4.3.3 Electronic system of LMDs

An LMD has an electronic system for processing the electronic signal from the detector [8] in order to deliver the measured values. Among the various types of systems, Figure 4 shows a typical one consisting of an analogue circuit amplifying the signal from the detector, an A/D converter converting the amplified signal into a digital signal, a data processor converting the digital signal to the measurement value, and a system controller controlling the whole system including the memory, display, and interface of the external devices.

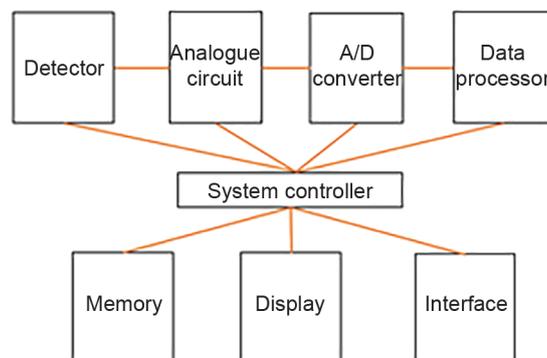

IEC

Figure 4 – Block diagram of a typical electronic system