

INTERNATIONAL STANDARD




Medical electrical equipment – Dosimetric instruments used for non-invasive measurement of X-ray tube voltage in diagnostic radiology

(<https://standards.iteh.ai>)

Document Preview

[IEC 61676:2023](#)

<https://standards.iteh.ai/catalog/standards/iec/3bde154f-2184-4ef7-a3b5-1237d112177e/iec-61676-2023>

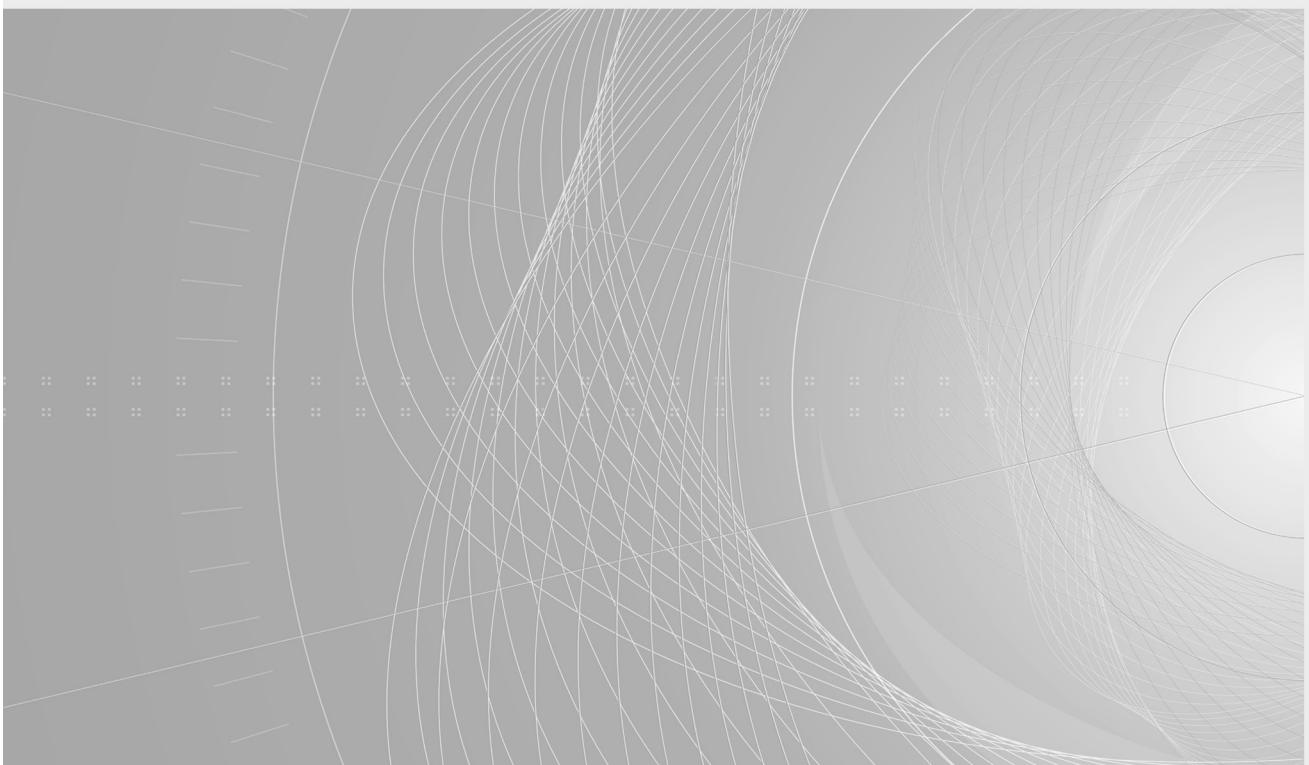



THIS PUBLICATION IS COPYRIGHT PROTECTED
Copyright © 2023 IEC, Geneva, Switzerland

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either IEC or IEC's member National Committee in the country of the requester. If you have any questions about IEC copyright or have an enquiry about obtaining additional rights to this publication, please contact the address below or your local IEC member National Committee for further information.

IEC Secretariat
3, rue de Varembe
CH-1211 Geneva 20
Switzerland

Tel.: +41 22 919 02 11
info@iec.ch
www.iec.ch

About the IEC

The International Electrotechnical Commission (IEC) is the leading global organization that prepares and publishes International Standards for all electrical, electronic and related technologies.

About IEC publications

The technical content of IEC publications is kept under constant review by the IEC. Please make sure that you have the latest edition, a corrigendum or an amendment might have been published.

IEC publications search - webstore.iec.ch/advsearchform

The advanced search enables to find IEC publications by a variety of criteria (reference number, text, technical committee, ...). It also gives information on projects, replaced and withdrawn publications.

IEC Just Published - webstore.iec.ch/justpublished

Stay up to date on all new IEC publications. Just Published details all new publications released. Available online and once a month by email.

IEC Customer Service Centre - webstore.iec.ch/csc

If you wish to give us your feedback on this publication or need further assistance, please contact the Customer Service Centre: sales@iec.ch.

IEC Products & Services Portal - products.iec.ch

Discover our powerful search engine and read freely all the publications previews. With a subscription you will always have access to up to date content tailored to your needs.

Electropedia - www.electropedia.org

The world's leading online dictionary on electrotechnology, containing more than 22 300 terminological entries in English and French, with equivalent terms in 19 additional languages. Also known as the International Electrotechnical Vocabulary (IEV) online.

International Standards
standards.iteh.ai
Document Preview

[IEC 61676:2023](#)

<https://standards.iteh.ai/catalog/standards/iec/3bde154f-2184-4ef7-a3b5-1237d112177e/iec-61676-2023>



IEC 61676

Edition 2.0 2023-03
REDLINE VERSION

INTERNATIONAL STANDARD



Medical electrical equipment – Dosimetric instruments used for non-invasive measurement of X-ray tube voltage in diagnostic radiology

*iteh Standards
(<https://standards.iteh.ai>)
Document Preview*

[IEC 61676:2023](https://standards.iteh.ai/catalog/standards/iec/3bde154f-2184-4ef7-a3b5-1237d112177e/iec-61676-2023)

<https://standards.iteh.ai/catalog/standards/iec/3bde154f-2184-4ef7-a3b5-1237d112177e/iec-61676-2023>

INTERNATIONAL
ELECTROTECHNICAL
COMMISSION

ICS 11.040.50; 11.040.55

ISBN 978-2-8322-6703-5

Warning! Make sure that you obtained this publication from an authorized distributor.

CONTENTS

FOREWORD.....	4
INTRODUCTION.....	2
1 Scope and object	7
2 Normative references	7
3 Terminology Terms and definitions	8
4 General performance requirements for measurement of PRACTICAL PEAK VOLTAGE measurements.....	11
4.1 Quantity to be measured	11
4.2 Limits of PERFORMANCE CHARACTERISTICS	12
4.2.1 Limits	12
4.2.2 Maximum error	12
4.2.3 Over and under range indications	13
4.2.4 Repeatability	13
4.2.5 Long term stability	13
4.3 LIMITS OF VARIATION for effects of INFLUENCE QUANTITIES	14
4.3.1 INFLUENCE QUANTITIES	14
4.3.2 MINIMUM RATED RANGE of use	14
4.3.3 REFERENCE CONDITIONS	14
4.3.4 STANDARD TEST CONDITIONS	14
4.3.5 LIMITS OF VARIATION.....	14
4.4 Performance test procedures	16
4.4.1 General remarks.....	16
4.4.2 Dependence of instrument RESPONSE on voltage waveform and frequency	17
4.4.3 Dependence of instrument RESPONSE on ANODE ANGLE.....	17
4.4.4 Dependence of instrument RESPONSE on FILTRATION.....	18
4.4.5 Dependence of instrument RESPONSE on dose rate	18
4.4.6 Dependence of instrument RESPONSE on IRRADIATION TIME	18
4.4.7 Dependence of instrument RESPONSE on field size	18
4.4.8 Dependence of instrument RESPONSE on focus-to-detector distance.....	19
4.4.9 Dependence of instrument RESPONSE on angle of incidence of RADIATION.....	19
4.4.10 Dependence of instrument RESPONSE on angle of detector rotation with respect to the X-RAY TUBE axis.....	19
4.4.11 Dependence of instrument RESPONSE on temperature and humidity	20
4.4.12 Dependence of instrument RESPONSE on operating voltage	20
4.4.13 Dependence of instrument RESPONSE on electromagnetic compatibility	21
4.4.14 Additional tungsten filtration (tube aging).....	23
5 Special instrumental requirements and marking.....	23
5.1 Requirements for the complete instruments	23
5.2 General.....	23
5.3 Display	24
5.4 Range of measurement.....	24
5.5 Connectors and cables	24
6 ACCOMPANYING DOCUMENTS	24
6.1 General.....	24
6.2 Information provided	24
6.3 Instrument description.....	24

6.4	Detector	24
6.5	Delay time	24
6.6	Measurement window	24
6.7	Data outlet	24
6.8	Transport and storage	25
Annex A (informative) Recommended performance criteria for the invasive divider		
Annex A (informative)	COMBINED STANDARD UNCERTAINTY	27
Annex B (informative)	Additional information on PRACTICAL PEAK VOLTAGE	28
B.1	Overview	28
B.2	Simplified formalism for the determination of the PRACTICAL PEAK VOLTAGE \hat{U}	28
Annex C (informative) Glossary of defined terms		
Bibliography	36
Index of defined terms	37
Figure B.1	– Example of a waveform of a two-pulse generator	30
Figure B.2	– Example of a waveform of a constant-voltage generator	30
Figure B.3	– Example of falling load waveform	31
Table 1	– Minimum effective ranges	11
Table 2	– Minimum RATED RANGE OF USE, REFERENCE CONDITIONS, STANDARD TEST CONDITIONS, LIMITS OF VARIATION ($\pm L$) and INTRINSIC ERROR (E) over the EFFECTIVE RANGE of use, for the pertaining INFLUENCE QUANTITY	15
Table 3	– Minimum test points and test values of PRACTICAL PEAK VOLTAGE for INFLUENCE QUANTITIES	17
Table 4	– Maximum HALF-VALUE LAYER (HVL) depending on anode angle	23
Table A.1	– Example for assessment of the COMBINED STANDARD UNCERTAINTY – Instruments used for NON-INVASIVE MEASUREMENT of X-RAY TUBE VOLTAGE	27
Table B.1	– Values of 20 samples of the falling load waveform in Figure B.3	31
Table B.2	– Voltage bins, probability and weighting factors for the 20 samples of the falling load waveform in Figure B.3	32
Table B.3	– Weighting factors for the 20 equally spaced samples of the falling load waveform in figure B.3	33

INTERNATIONAL ELECTROTECHNICAL COMMISSION

**MEDICAL ELECTRICAL EQUIPMENT – DOSIMETRIC INSTRUMENTS
USED FOR NON-INVASIVE MEASUREMENT OF X-RAY TUBE VOLTAGE
IN DIAGNOSTIC RADIOLOGY****FOREWORD**

- 1) The International Electrotechnical Commission (IEC) is a worldwide organization for standardization comprising all national electrotechnical committees (IEC National Committees). The object of IEC is to promote international co-operation on all questions concerning standardization in the electrical and electronic fields. To this end and in addition to other activities, IEC publishes International Standards, Technical Specifications, Technical Reports, Publicly Available Specifications (PAS) and Guides (hereafter referred to as "IEC Publication(s)"). Their preparation is entrusted to technical committees; any IEC National Committee interested in the subject dealt with may participate in this preparatory work. International, governmental and non-governmental organizations liaising with the IEC also participate in this preparation. IEC collaborates closely with the International Organization for Standardization (ISO) in accordance with conditions determined by agreement between the two organizations.
- 2) The formal decisions or agreements of IEC on technical matters express, as nearly as possible, an international consensus of opinion on the relevant subjects since each technical committee has representation from all interested IEC National Committees.
- 3) IEC Publications have the form of recommendations for international use and are accepted by IEC National Committees in that sense. While all reasonable efforts are made to ensure that the technical content of IEC Publications is accurate, IEC cannot be held responsible for the way in which they are used or for any misinterpretation by any end user.
- 4) In order to promote international uniformity, IEC National Committees undertake to apply IEC Publications transparently to the maximum extent possible in their national and regional publications. Any divergence between any IEC Publication and the corresponding national or regional publication shall be clearly indicated in the latter.
- 5) IEC itself does not provide any attestation of conformity. Independent certification bodies provide conformity assessment services and, in some areas, access to IEC marks of conformity. IEC is not responsible for any services carried out by independent certification bodies.
- 6) All users should ensure that they have the latest edition of this publication.
- 7) No liability shall attach to IEC or its directors, employees, servants or agents including individual experts and members of its technical committees and IEC National Committees for any personal injury, property damage or other damage of any nature whatsoever, whether direct or indirect, or for costs (including legal fees) and expenses arising out of the publication, use of, or reliance upon, this IEC Publication or any other IEC Publications.
- 8) Attention is drawn to the Normative references cited in this publication. Use of the referenced publications is indispensable for the correct application of this publication.
- 9) Attention is drawn to the possibility that some of the elements of this IEC Publication may be the subject of patent rights. IEC shall not be held responsible for identifying any or all such patent rights.

This redline version of the official IEC Standard allows the user to identify the changes made to the previous edition IEC 61676:2002+AMD1:2008 CSV. A vertical bar appears in the margin wherever a change has been made. Additions are in green text, deletions are in strikethrough red text.

IEC 61676 has been prepared by subcommittee 62C: Equipment for radiotherapy, nuclear medicine and radiation dosimetry, of IEC technical committee 62: Medical equipment, software, and systems. It is an International Standard.

This second edition of IEC 61676 cancels and replaces first edition published in 2002, Amendment 1:2008. This edition constitutes a technical revision.

It includes an assessment of the COMBINED STANDARD UNCERTAINTY for the performance of a hypothetical instrument for the non-invasive measurement of the tube high voltage (in Annex A) which replaces Annex A of the edition 1.1 titled "Recommended performance criteria for the invasive divider".

The text of this document is based on the following documents:

Draft	Report on voting
62C/830/CDV	62C/866/RVC

Full information on the voting for its approval can be found in the report on voting indicated in the above table.

The language used for the development of this International Standard is English.

This document was drafted in accordance with ISO/IEC Directives, Part 2, and developed in accordance with ISO/IEC Directives, Part 1 and ISO/IEC Directives, IEC Supplement, available at www.iec.ch/members_experts/refdocs. The main document types developed by IEC are described in greater detail at www.iec.ch/standardsdev/publications.

In this document the following document types are used:

- requirements, compliance with which can be tested, and definitions: in roman type;
- notes, explanations, advice, general statements and exceptions: in small roman type;
- *test specifications: in italic type;*
- TERMS USED THROUGHOUT THIS DOCUMENT THAT HAVE BEEN DEFINED IN CLAUSE 3 OR IN IEC 60601-1 AND ITS COLLATERAL STANDARDS: IN SMALL CAPITALS.

The committee has decided that the contents of this document will remain unchanged until the stability date indicated on the IEC website under webstore.iec.ch in the data related to the specific document. At this date, the document will be

- reconfirmed,
- withdrawn,
- replaced by a revised edition, or
- amended.

NOTE The committee knows this second edition of the document does still not address all problems associated with non-invasive high voltage measurements. For mammography only molybdenum filtration is considered in conjunction with a molybdenum anode although in addition tungsten and rhodium anodes with other filtrations are in use like rhodium, aluminium, copper, silver or titanium. At the time when this document was drafted there were not enough data available in the literature to define realistic limits of variation for these types of INFLUENCE QUANTITIES. On the other hand, the committee was informed that several international projects were started to examine the general behaviour of non-invasive X-ray multimeters of the main MANUFACTURERS. Results from these studies were to be expected within about 5 years. Therefore, the committee decided to set a short stability time for the second edition and update the document as soon as the results from these new examinations will be available.

The contents of the corrigendum 1 (2024-01) have been included in this copy.

INTRODUCTION

The result of a measurement of the X-RAY TUBE VOLTAGE by means of invasive or non-invasive instruments is normally expressed in the form of one single number for the value of the tube voltage, irrespective of whether the tube voltage is constant potential or shows a time dependent waveform. Non-invasive instruments for the measurement of the X-RAY TUBE VOLTAGE on the market usually indicate the "MEAN PEAK VOLTAGE". But the quantity "MEAN PEAK VOLTAGE" is not unambiguously defined and ~~may~~ can be any mean of all voltage peaks. It is impossible to establish test procedures for the performance requirements of non-invasive instruments for the measurement of the X-RAY TUBE VOLTAGE without the definition of the quantity under consideration. Therefore, this document is based on a quantity ~~recently proposed in the literature⁴ to be~~ called "PRACTICAL PEAK VOLTAGE". The PRACTICAL PEAK VOLTAGE is unambiguously defined and applicable to any waveform. This quantity is related to the spectral distribution of the emitted X-RADIATION and the image properties. X-RAY GENERATORS operating at the same value of the PRACTICAL PEAK VOLTAGE produce the same low-level contrast in the RADIOGRAMS, even when the waveforms of the tube voltages are different. Detailed information on this concept is provided in Annex B. An example for the calculation of the PRACTICAL PEAK VOLTAGE in the case of a "falling load" waveform is also given in Annex B.

~~As a result of introducing a new quantity, the problem arises that this standard has been written for instruments which were not explicitly designed for the measurement of the PRACTICAL PEAK VOLTAGE. However, from preliminary results of a trial type test of a non-invasive instrument currently on the market, it can be expected that future instruments and most instruments on the market will be able to fulfil the requirements stated in this standard without insurmountable difficulties. For the most critical requirements on voltage waveform and frequency dependence of the RESPONSE, it turned out from these investigations that it is even easier to comply with the standard by using the PRACTICAL PEAK VOLTAGE as the measurement quantity.~~

The CALIBRATION and adjustment of the X-RAY TUBE VOLTAGE of an X-RAY GENERATOR is generally performed by the MANUFACTURER using a direct INVASIVE MEASUREMENT. Instruments utilising NON-INVASIVE MEASUREMENTS can also be used to check the CALIBRATION or to adjust the X-RAY TUBE VOLTAGE. These instruments are ~~required~~ used to have uncertainties of the voltage measurement comparable with the INVASIVE MEASUREMENT. One of the most important parameters of diagnostic X-RAY EQUIPMENT is the voltage applied to the X-RAY TUBE, because both the image quality in diagnostic radiology and the DOSE received by the PATIENT undergoing radiological examinations are dependent on the X-RAY TUBE VOLTAGE. An overall uncertainty below $\pm 5\%$ is ~~required~~ applicable, and this value serves as a guide for the LIMITS OF VARIATION for the effects of INFLUENCE QUANTITIES.

⁴ ~~See annex B.~~

MEDICAL ELECTRICAL EQUIPMENT – DOSIMETRIC INSTRUMENTS USED FOR NON-INVASIVE MEASUREMENT OF X-RAY TUBE VOLTAGE IN DIAGNOSTIC RADIOLOGY

1 ~~Scope and object~~

This document specifies the performance requirements of instruments as used in the NON-INVASIVE MEASUREMENT of X-RAY TUBE VOLTAGE up to 150 kV and the relevant compliance tests. This document also describes the method for CALIBRATION and gives guidance for estimating the uncertainty in measurements performed under conditions different from those during CALIBRATION.

Applications for such measurement are found in diagnostic RADIOLOGY including mammography, COMPUTED TOMOGRAPHY (CT), dental radiology and RADIOSCOPY. This document is not concerned with the safety aspect of such instruments. The requirements for electrical safety applying to them are contained in IEC 61010-1.

2 Normative references

The following documents are referred to in the text in such a way that some or all of their content constitutes requirements of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

IEC 60417, *Graphical symbols for use on equipment*, available at <http://www.graphical-symbols.info/equipment>

IEC 60601-1:2005, *Medical electrical equipment – Part 1: General requirements for basic safety and essential performance*

IEC 60601-1:2005/AMD1:2012

IEC 60601-1:2005/AMD2:2020

IEC TR 60788:1984/2004, ~~Medical radiology – Terminology~~ *Medical electrical equipment – Glossary of defined terms*

IEC 61000-4-2:1995, *Electromagnetic compatibility (EMC) – Part 4-2: Testing and measurement techniques – Electrostatic discharge immunity test*. ~~Basic EMC Publication~~

IEC 61000-4-3:2000, *Electromagnetic compatibility (EMC) – Part 4-3: Testing and measurement techniques – Radiated, radio-frequency, electromagnetic field immunity test*. ~~Basic EMC Publication~~

IEC 61000-4-4:1995, *Electromagnetic compatibility (EMC) – Part 4-4: Testing and measurement techniques – Electrical fast transient/burst immunity test*. ~~Basic EMC Publication~~

IEC 61000-4-5:1995, *Electromagnetic compatibility (EMC) – Part 4-5: Testing and measurement techniques – Surge immunity test*. ~~Basic EMC Publication~~

IEC 61000-4-6:1996, *Electromagnetic compatibility (EMC) – Part 4-6: Testing and measurement techniques – Immunity to conducted disturbances, induced by radio-frequency fields*. ~~Basic EMC Publication~~

IEC 61000-4-11:~~1994~~, *Electromagnetic compatibility (EMC) – Part 4-11: Testing and measurement techniques – Voltage dips, short interruptions and voltage variations immunity tests for equipment with input current up to 16 A per phase*. ~~Basic EMC Publication~~

IEC 61010-1:~~2004~~, *Safety requirements for electrical equipment for measurement, control, and laboratory use – Part 1: General requirements*

IEC 61187:~~1993~~, *Electrical and electronic measuring equipment – Documentation*

~~ISO:1993, International vocabulary of basic and general terms in metrology (ISBN 92-67-01075-1)~~

ISO 7000:~~1989~~2019, *Graphical symbols for use on equipment – Index and synopsis* Registered symbol

3 Terminology Terms and definitions

For the purposes of this document, the terms and definitions given in IEC 60601-1:2005, IEC TR 60788:2004 and the following apply.

~~The definitions given in this standard are generally in agreement with those in IEC 60788 and the ISO International vocabulary of basic and general terms in metrology. Any terms not defined in this subclause have the meanings defined in the above publications or are assumed to be in general scientific usage.~~

ISO and IEC maintain terminological databases for use in standardization at the following addresses:

- IEC Electropedia: available at <http://www.electropedia.org/>
- ISO Online browsing platform: available at <http://www.iso.org/obp>

NOTE 1 An Index of defined terms is to be found at the end of the document.

NOTE 2 A searchable IEC Glossary can be found at std.iec.ch.

3.1

CORRECTION FACTOR

dimensionless multiplier which corrects the INDICATED VALUE of an instrument from its value when operated under particular conditions to its value when operated under stated REFERENCE CONDITIONS

3.2

EFFECTIVE RANGE

range of INDICATED VALUES for which an instrument complies with a stated performance

Note 1 to entry: The maximum (minimum) effective INDICATED VALUE is the highest (lowest) in this range.

3.3

INDICATED VALUE

value of quantity derived from the scale reading of an instrument together with any scale factors indicated on the control panel of the instrument

3.4

INFLUENCE QUANTITY

any external quantity that ~~may~~ can affect the performance of an instrument (e.g., ambient temperature etc.) and any property of the X-RAY EQUIPMENT under test that ~~needs to~~ shall be taken into account in using the instrument for NON-INVASIVE MEASUREMENT of X-RAY TUBE

VOLTAGE (e.g., range of X-RAY TUBE VOLTAGE, ANODE ANGLE, anode material, TOTAL FILTRATION, etc.)

3.5

INSTRUMENT PARAMETER

any internal property of an instrument that ~~may~~ can affect the performance of the instrument

3.6

INTRINSIC ERROR

deviation of the MEASURED VALUE (i.e., the INDICATED VALUE, corrected to REFERENCE CONDITIONS) from the CONVENTIONAL TRUE VALUE under STANDARD TEST CONDITIONS

3.7

INVASIVE MEASUREMENT

measurement of the X-RAY TUBE VOLTAGE by external connection of a suitable meter or a high resistance divider

3.8

LIMITS OF VARIATION

maximum VARIATION of a PERFORMANCE CHARACTERISTIC y , permitted by this document

Note 1 to entry: If the LIMITS OF VARIATION are stated as $\pm L$ % the VARIATION $\Delta y / y$, expressed as a percentage, shall remain in the range from $-L$ % to $+L$ %.

3.9

MAXIMUM PEAK VOLTAGE

maximum value of the X-RAY TUBE VOLTAGE in a specified time interval

Note 1 to entry: The unit of this quantity is the volt (V).

3.10

MEAN PEAK VOLTAGE

mean value of all X-RAY TUBE VOLTAGE peaks during a specified time interval

Note 1 to entry: The unit of this quantity is the volt (V).

3.11

MEASURED VALUE

best estimate of the CONVENTIONAL TRUE VALUE of a quantity, being derived from the INDICATED VALUE of an instrument together with the application of all relevant CORRECTION FACTORS

Note 1 to entry: The CONVENTIONAL TRUE VALUE is usually the value determined by the working standard with which the instrument under test is being compared.

3.12

MINIMUM EFFECTIVE RANGE

smallest permitted range of INDICATED VALUES for which an instrument complies with a stated performance

3.13

NON-INVASIVE MEASUREMENT

measurement of X-RAY TUBE VOLTAGE by analysis of the emitted RADIATION

3.14

PERFORMANCE CHARACTERISTIC

one of the quantities used to define the performance of an instrument (e.g., RESPONSE)

**3.15
VOLTAGE RIPPLE**

VOLTAGE at the X-RAY TUBE, r , expressed as a percentage of the peak voltage, U_{\max} , over a specified time interval

Note 1 to entry: The VOLTAGE RIPPLE is expressed by the formula:

$$r = \frac{U_{\max} - U_{\min}}{U_{\max}} \times 100 \%$$

where U_{\max} is the highest voltage in the interval, and U_{\min} is the lowest voltage in the interval.

**3.16
PRACTICAL PEAK VOLTAGE
PPV**

$$\frac{\int_{U_{\min}}^{U_{\max}} p(U) \times w(U) \times U dU}{\int_{U_{\min}}^{U_{\max}} p(U) \times w(U) dU} \quad \text{with} \quad \int_{U_{\min}}^{U_{\max}} p(U) dU = 1$$

where $p(U)$ is the distribution function for the voltage U and $w(U)$ is a weighting function, U_{\max} is the highest voltage in the interval, and U_{\min} is the lowest voltage in the interval

Note 1 to entry: The unit of the quantity PRACTICAL PEAK VOLTAGE is the volt (V).

Note 2 to entry: Additional information on the PRACTICAL PEAK VOLTAGE, the weighting function $w(U)$ and the distribution function $p(U)$ is provided in Annex B. Using this weighting function $w(U)$ the PRACTICAL PEAK VOLTAGE is defined as the constant potential which produces the same AIR KERMA contrast behind a specified PHANTOM as the non-DC voltage under test.

**3.17
RATED RANGE OF USE**

range of values of an INFLUENCE QUANTITY or INSTRUMENT PARAMETER within which the instrument will operate within the LIMITS OF VARIATION

Note 1 to entry: The limits of rated range are the maximum and minimum RATED values.

Note 2 to entry: The MINIMUM RATED RANGE is the least range of an INFLUENCE QUANTITY or INSTRUMENT PARAMETER within which the instrument shall operate within the specified LIMITS OF VARIATION in order to comply with this document.

**3.18
REFERENCE CONDITION**

condition under which all INFLUENCE QUANTITIES and INSTRUMENT PARAMETERS have their REFERENCE VALUES

**3.19
REFERENCE VALUE**

particular value of an INFLUENCE QUANTITY (or INSTRUMENT PARAMETER) chosen for the purposes of reference i.e., the value of an INFLUENCE QUANTITY (or INSTRUMENT PARAMETER) at which the CORRECTION FACTOR for dependence on that INFLUENCE QUANTITY (or INSTRUMENT PARAMETER) is unity

**3.20
RELATIVE INTRINSIC ERROR**

ratio of the INTRINSIC ERROR to the CONVENTIONAL TRUE VALUE

3.21**RESPONSE**

quotient of the INDICATED VALUE divided by the CONVENTIONAL TRUE VALUE

3.22**STANDARD TEST CONDITION**

condition under which all INFLUENCE QUANTITIES and INSTRUMENT PARAMETERS have their STANDARD TEST VALUES

3.23**STANDARD TEST VALUE**

value or a range of values of an INFLUENCE QUANTITY or INSTRUMENT PARAMETER, which is permitted when carrying out CALIBRATIONS or tests on another INFLUENCE QUANTITY or INSTRUMENT PARAMETER

3.24**VARIATION**

relative difference $\Delta y / y$, between the values of a PERFORMANCE CHARACTERISTIC y , when one INFLUENCE QUANTITY or INSTRUMENT PARAMETER assumes successively two specified values, the other INFLUENCE QUANTITIES and INSTRUMENT PARAMETERS being kept constant at the STANDARD TEST VALUES, unless other values are specified

3.25**X-RAY TUBE VOLTAGE**

potential difference applied to an X-RAY TUBE between the anode and the cathode

Note 1 to entry: The unit of this quantity is the volt (V).

4 General performance requirements for measurement of PRACTICAL PEAK VOLTAGE measurements

4.1 Quantity to be measured

IEC 61676:2023

The quantity to be measured is the PRACTICAL PEAK VOLTAGE.

NOTE Additional quantities ~~may~~ can be displayed.

The MINIMUM EFFECTIVE RANGES of PRACTICAL PEAK VOLTAGE shall be as listed in Table 1 for the relevant X-RAY applications.

Table 1 – Minimum effective ranges

Application	Nominal anode material	MINIMUM EFFECTIVE RANGE
Mammography 20 kV to 50 kV	Mo ^{a)}	24 kV to 35 kV
Diagnostic 40 kV to 150 kV	W	60 kV to 120 kV
CT 80 70 kV to 150 kV	W	100 80 kV to 140 kV
Dental 40 kV to 110 kV	W	60 kV to 90 kV
Fluoroscopic 40 kV to 130 kV	W	60 kV to 120 kV
^{a)} For mammography anode materials other than Mo, the MINIMUM EFFECTIVE RANGE of PPV shall be at least 10 kV.		

4.2 Limits of PERFORMANCE CHARACTERISTICS

4.2.1 Limits

All values of the limits of PERFORMANCE CHARACTERISTICS stated in this subclause do not contain the uncertainty of the test equipment.

4.2.2 Maximum error

4.2.2.1 Maximum RELATIVE INTRINSIC ERROR for voltages above 50 kV

The RELATIVE INTRINSIC ERROR, I , of PRACTICAL PEAK VOLTAGE, \hat{U} , measurements made under STANDARD TEST CONDITIONS, shall not be greater than $\pm 2\%$ over the EFFECTIVE RANGE of voltages. This is expressed by the formula:

$$|I| = \left| \frac{\hat{U}_{\text{meas}} - \hat{U}_{\text{true}}}{\hat{U}_{\text{true}}} \right| \leq 0,02$$

where \hat{U}_{meas} is the MEASURED VALUE of PRACTICAL PEAK VOLTAGE and \hat{U}_{true} is the TRUE VALUE of the PRACTICAL PEAK VOLTAGE. The voltages for the MINIMUM EFFECTIVE RANGE are listed in Table 1.

The compliance test for performance requirement for this subclause is listed under 4.2.2.2.

4.2.2.2 Maximum INTRINSIC ERROR for voltages below 50 kV

The maximum INTRINSIC ERROR, E , of PRACTICAL PEAK VOLTAGE, \hat{U} , measurements made under STANDARD TEST CONDITIONS shall not be greater than ± 1 kV over the EFFECTIVE RANGE of voltages. This is expressed by the formula:

$$|E| = \left| \hat{U}_{\text{meas}} - \hat{U}_{\text{true}} \right| \leq 1,0 \text{ kV}$$

where \hat{U}_{meas} is the MEASURED VALUE of PRACTICAL PEAK VOLTAGE and \hat{U}_{true} is the CONVENTIONAL TRUE VALUE of the PRACTICAL PEAK VOLTAGE. The voltages for the MINIMUM EFFECTIVE RANGE are listed in Table 1.

Compliance with performance requirements 4.2.2.1 and 4.2.2.2 shall be checked by measuring the RELATIVE INTRINSIC ERROR above 50 kV or the INTRINSIC ERROR below 50 kV over the EFFECTIVE RANGE of voltages for each application claimed. STANDARD TEST CONDITIONS are listed in Table 2 for each application. The end points of the EFFECTIVE RANGE ~~must~~ shall be checked. For mammography, the nominal step between measurements shall be no greater than 2 kV. For all other applications the nominal step between measurements shall be no greater than 5 kV for voltages below 100 kV, and no greater than 10 kV for voltages above 100 kV.

If more than one instrument configuration can be utilised to measure a span of voltages, then that span of voltages shall be measured utilising all relevant instrument configurations. As a minimum the end points and enough interim points shall be measured to meet the minimum step requirements given above. An example could be the use of different absorber pairs to provide overlapping voltage spans. In the case of different absorber pairs, if the first measured from 40 kV to 80 kV, and the second from 60 kV to 120 kV, then the overlapping span would be from 60 kV to 80 kV. At a minimum, measurements would be made utilising each absorber pair at 60 kV, 65 kV, 70 kV, 75 kV, and 80 kV.