



# Standard Practice for Expanded Welded and Silver Braze Socket Joints for Pipe and Tube<sup>1</sup>

This standard is issued under the fixed designation F1076; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon ( $\epsilon$ ) indicates an editorial change since the last revision or reapproval.

## 1. Scope\*

1.1 This practice covers expanded welded and silver braze socket joints for use on shipboard piping systems.

1.2 Expanded welded and silver braze socket joints are to be used to join two pipes or tubes having the same NPS (see **Note 1**) without using a fitting or butt weld.

1.3 Braze socket type joints are not intended for use on systems containing flammable or combustible fluids in areas where fire hazards exist or where the service temperature exceeds 425°F (205°C).

1.4 Braze joints depending solely upon a fillet weld rather than primarily upon braze material between pipe/tube and socket are not covered by this practice.

**NOTE 1**—The dimensionless designator nominal pipe size (NPS) has been substituted in this practice for such traditional terms as “nominal diameter,” “size,” “nominal size,” and “iron pipe size.”

1.5 The values stated in inch-pound units are to be regarded as standard. The values given in parentheses are mathematical conversions to SI units that are provided for information only and are not considered standard.

1.6 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety, health, and environmental practices and determine the applicability of regulatory limitations prior to use.*

1.7 *This international standard was developed in accordance with internationally recognized principles on standardization established in the Decision on Principles for the Development of International Standards, Guides and Recommendations issued by the World Trade Organization Technical Barriers to Trade (TBT) Committee.*

<sup>1</sup> This practice is under the jurisdiction of ASTM Committee F25 on Ships and Marine Technology and is the direct responsibility of Subcommittee F25.11 on Machinery and Piping Systems.

Current edition approved Dec. 1, 2019. Published December 2019. Originally approved in 1987. Last previous edition approved in 2015 as F1076 – 87 (2015) <sup>$\epsilon$ 1</sup>. DOI: 10.1520/F1076-19.

## 2. Referenced Documents

### 2.1 ASTM Standards:<sup>2</sup>

- A312/A312M Specification for Seamless, Welded, and Heavily Cold Worked Austenitic Stainless Steel Pipes
- B75/B75M Specification for Seamless Copper Tube
- B88 Specification for Seamless Copper Water Tube
- B466/B466M Specification for Seamless Copper-Nickel Pipe and Tube

### 2.2 Military Standards:<sup>3</sup>

- MIL-P-24691/3 Pipe and Tube, Corrosion-Resistant, Stainless Steel, Seamless or Welded
- MIL-T-16420 Tube, Copper-Nickel Alloy, Seamless and Welded
- MIL-T-24107 Tube, Copper (Seamless)

### 2.3 ASME Standard:<sup>4</sup>

- ASME Boiler and Pressure Vessel Code, Section IX

### 2.4 Federal Standard:<sup>3</sup>

- Code of Federal Regulations, Title 46

### 2.5 NAVSEA Document:<sup>3</sup>

- 0900-LP-001-7000 Fabrication and Inspection of Braze Piping Systems

## 3. Significance and Use

3.1 Expanded welded socket joints may be used with the following pipe and tube:

3.1.1 *Seamless Copper Tube*—2.375-in. (60-mm) outside diameter through 6.625-in. (170-mm) outside diameter.

3.1.2 *Seamless Copper-Nickel Tube*—2.375-in. (60-mm) outside diameter through 6.625-in. (170-mm) outside diameter.

3.1.3 *Seamless Copper Water Tube*—2.125-in. (55-mm) outside diameter through 4.125-in. (105-mm) outside diameter.

3.1.4 *Seamless Stainless Steel Pipe*—2 NPS through 6 NPS, Schedules 5 and 10.

<sup>2</sup> For referenced ASTM standards, visit the ASTM website, [www.astm.org](http://www.astm.org), or contact ASTM Customer Service at [service@astm.org](mailto:service@astm.org). For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

<sup>3</sup> Available from U.S. Government Printing Office, Superintendent of Documents, 732 N. Capitol St., NW, Washington, DC 20401-0001, <http://www.access.gpo.gov>.

<sup>4</sup> Available from American Society of Mechanical Engineers (ASME), ASME International Headquarters, Two Park Ave., New York, NY 10016-5990, <http://www.asme.org>.

\*A Summary of Changes section appears at the end of this standard

3.2 Expanded silver brazed socket joints may be used with the following tube:

3.2.1 *Seamless Copper Tube*—2.375-in. (60-mm) outside diameter through 6.625-in. (170-mm) outside diameter.

3.2.2 *Seamless Copper-Nickel Tube*—2.375-in. (60-mm) outside diameter through 6.625-in. (170-mm) outside diameter.

3.2.3 *Seamless Copper Water Tube*—2.125-in. (55-mm) outside diameter through 4.125-in. (105-mm) outside diameter.

3.3 Expanded welded and silver brazed socket joints may be used where experience or test has demonstrated that the joint is safe and suitable for design and operating conditions, and where adequate provision is made to prevent separation of the joint.

**4. Materials and Manufacture**

4.1 *Welded Socket Joint:*

4.1.1 *Seamless Copper Tube*—Specification **B75/B75M**, UNS Number C12200 and MIL-T-24107, UNS Number C12200, light drawn (see 5.3).

4.1.2 *Seamless Copper-Nickel Tube (90-10)*—Specification **B466/B466M**, UNS Number C70600 and MIL-T-16420, UNS Number C70600, Class 200, annealed.

4.1.3 *Seamless Copper-Nickel Tube (70-30)*—Specification **B466/B466M**, UNS Number C71500 and MIL-T-16420, UNS Number C71500, Class 200, annealed.

4.1.4 *Seamless Copper Water Tube*—Specification **B88**, Type K, UNS Number C71500, drawn (see 5.3).

4.1.5 *Seamless Stainless Steel Pipe*—Specification **A312/A312M**, UNS Number S30400 and S31600, MIL-P-24691/3, UNS Number S30400 and S31600, Schedules 5 and 10.

4.2 *Silver-Brazed Socket Joint:*

4.2.1 *Seamless Copper Tube*—Specification **B75/B75M**, UNS Number C12200 and MIL-T-24107, UNS Number C12200, light drawn (see 5.3).

4.2.2 *Seamless Copper-Nickel Tube (90-10)*—Specification **B466/B466M**, UNS Number C70600 and MIL-T-16420, UNS Number C70600, Class 200, annealed.

4.2.3 *Seamless Copper-Nickel Tube (70-30)*—Specification **B466/B466M**, UNS Number C71500 and MIL-T-16420, UNS Number C71500, Class 200, annealed.

4.2.4 *Seamless Copper Water Tube*—Specification **B88**, Type K, UNS Number C12200, drawn (see 5.3).

**5. Procedure**

5.1 Install no more than two expanded joints in any 36-in. (915-mm) long section of pipe/tube and in no case allow a pipe/tube expanded at both ends in lengths of less than 36 in.

5.2 Fabricate expanded joints on the ends of the pipe/tube by use of an expanding machine.

5.3 Expanded joints shall not be used on Class I piping systems as defined in 46CFR56.04 for United States Coast Guard inspected and certified vessels.


5.4 Perform a minimum of three expansions to ensure the degree of expansion.

5.5 Bevel the unexpanded end of pipe/tube 30 to 40° for copper-nickel alloy and 10 to 20° for stainless steel.

5.6 Clean the pipe/tube ends to be inserted into the silver-brazed expanded pipe/tube socket and the interior of the socket itself to a bright metal before insertion.

5.7 Align pipe/tube ends concentrically as accurately as possible, and preserve this alignment during the welding process.

5.8 Provide a gap of approximately 1/16 in. (1.5 mm) (expanded welded socket joint, Fig. 1) and 1/8 in. (3 mm) (expanded silver-brazed joint, Fig. 2) between the end of the

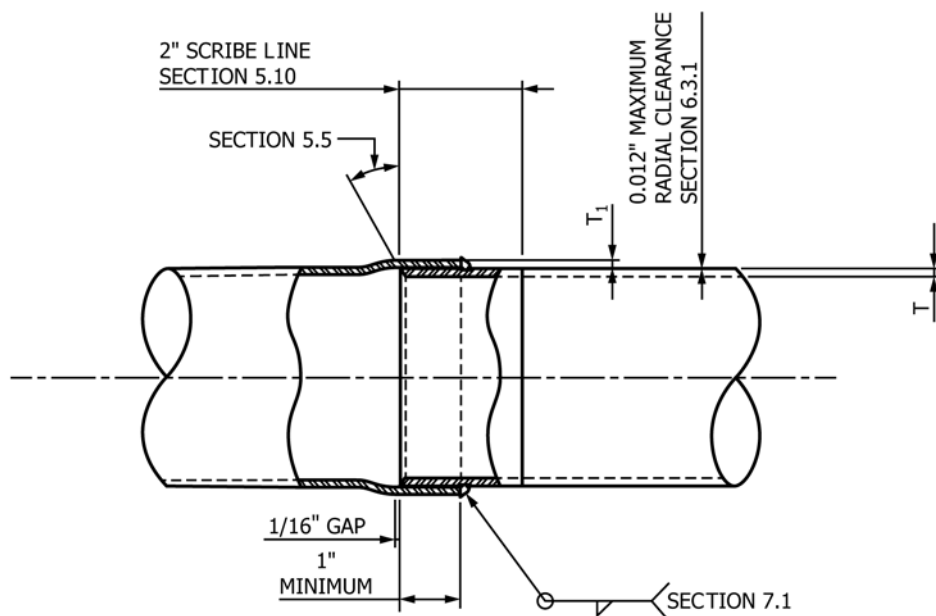

NOTE 1—1 in. = 25.4 mm.

FIG. 1 Expanded Welded Socket Joint