



Designation: **D7698 – 11a D7698 – 19**

Standard Test Method for In-Place Estimation of Density and Water Content of Soil and Aggregate by Correlation with Complex Impedance Method¹

This standard is issued under the fixed designation D7698; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reappraisal. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reappraisal.

1. Scope

1.1 *Purpose and Application*—This test method describes the procedure, equipment, and interpretation methods for estimating in-place soil dry density and water content using a Complex-Impedance Measuring Instrument (CIMI).

1.1.1 This test method describes the procedure, equipment, and interpretation methods for estimating in-place soil dry density and water content using a Complex-Impedance Measuring Instrument (CIMI). The purpose and application of this test method is for testing porous material such as used in roadway base or building foundations that may be deployed in the field at various test sites. The test apparatus includes electrodes that contact the porous material under test and a sensor unit that supplies electromagnetic signals to the porous material. Response signals reveal electrical parameters such as complex impedance which can be equated to material properties such as density and moisture content.

1.1.2 CIMI measurements as described in this Standard Test Method test method are applicable to measurements of compacted soils intended for roads and foundations.

1.1.3 This test method describes the procedure for estimating in-place density and water content of soils and soil-aggregates by use of a CIMI. The electrical properties of the soil are measured using a radio frequency (RF) voltage applied source connected to soil electrical probes driven into the soils and soil-aggregates to be tested, in a prescribed pattern and depth. Certain algorithms of these properties are related to wet density and water content. This correlation between electrical measurements, and density and water content is accomplished using a calibration methodology. In the calibration methodology, density and water content are determined by other ASTM Test Standards that measure soil density and water content, thereafter correlating the corresponding measured electrical properties to the soil physical properties.

1.1.4 The values stated in SI units are to be regarded as standard. The inch-pound units given in parentheses are mathematical conversions which are provided for information purposes only and are not considered standard.

1.1.5 All observed and calculated values shall conform to the guidelines for significant digits and rounding established in Practice D6026 unless superseded by this standard.

1.2 *Units*—The values stated in SI units are to be regarded as standard. The inch-pound units given in parentheses are mathematical conversions which are provided for information purposes only and are not considered standard.

1.2.1 All observed and calculated values shall conform to the guidelines for significant digits and rounding established in Practice D6026 unless superseded by this standard.

1.3 *Generalized Theory*:

1.3.1 Two key electrical properties of soil are conductivity and relative dielectric permittivity which are manifested as a value of complex-impedance that can be determined.

1.3.2 The soil conductivity contributes primarily to the real component of the complex-impedance, and the soil relative dielectric permittivity contributes primarily to the imaginary component of the complex-impedance.

1.3.3 The complex-impedance of soil can be determined by placing two electrodes in the soil to be tested at a known distance apart and a known depth. The application of a known frequency of alternating current to the electrodes enables a measurement of current through the soil, voltage across the electrodes, and the electrical phase difference between the voltage and current waves. Complex-impedance is calculated from these known and measured parameters.

1.3.4 From the determined complex-impedance, an electrical network consisting of a resistor (R) and capacitor (C) connected in parallel are used to represent a model of the soil being tested.

¹ This test method is under the jurisdiction of ASTM Committee D18 on Soil and Rock and is the direct responsibility of Subcommittee D18.08 on Special and Construction Control Tests.

Current edition approved Nov. 1, 2011; Nov. 1, 2019. Published January 2012; December 2019. Originally approved in 2011. Last previous edition approved in 2011 as D7698-11-11a. DOI: 10.1520/D7698-11a; 10.1520/D7698-19.

1.3.5 Relationships can be made between the soil wet density and the magnitude of the complex-impedance, and also between the soil water mass per unit measured, and the quotient of the values of C and R using a Soil Model process.

1.3.6 The Soil Model process results in mathematical relationships between the physical and electrical characteristics of the soil which are used for soil-specific calibration of the CIMI.

1.3.7 Refer to **Appendix X1** for a more detailed explanation of complex-impedance measurement of in-place soil, and its use in field measurements for the estimation of dry density and water content.

1.4 ~~Precautions~~Precautions:

1.4.1 ~~The radio frequencies and low-level RF output power levels of the CIMI method are such that they are harmless according to the Federal Communications Commission (FCC)-harmless.~~

1.4.2 ~~This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use. The SI units presented for apparatus are substitutions of the inch-pound units, other similar SI units should be acceptable providing they meet the technical requirements established by the inch-pound apparatus.~~

1.5 This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety, health, and environmental practices and determine the applicability of regulatory limitations prior to use.

1.6 This international standard was developed in accordance with internationally recognized principles on standardization established in the Decision on Principles for the Development of International Standards, Guides and Recommendations issued by the World Trade Organization Technical Barriers to Trade (TBT) Committee.

2. Referenced Documents

2.1 *ASTM Standards:*²

[D653 Terminology Relating to Soil, Rock, and Contained Fluids](#)

[D698 Test Methods for Laboratory Compaction Characteristics of Soil Using Standard Effort \(12,400 ft-lbf/ft³ \(600 kN-m/m³\)\)](#)

[D1556 Test Method for Density and Unit Weight of Soil in Place by Sand-Cone Method](#)

[D1557 Test Methods for Laboratory Compaction Characteristics of Soil Using Modified Effort \(56,000 ft-lbf/ft³ \(2,700 kN-m/m³\)\)](#)

[D2216 Test Methods for Laboratory Determination of Water \(Moisture\) Content of Soil and Rock by Mass](#)

[D3740 Practice for Minimum Requirements for Agencies Engaged in Testing and/or Inspection of Soil and Rock as Used in Engineering Design and Construction](#)

[D4253 Test Methods for Maximum Index Density and Unit Weight of Soils Using a Vibratory Table](#)

[D4643 Test Method for Determination of Water Content of Soil and Rock by Microwave Oven Heating](#)

[D4718 Practice for Correction of Unit Weight and Water Content for Soils Containing Oversize Particles](#)

[D4944 Test Method for Field Determination of Water \(Moisture\) Content of Soil by the Calcium Carbide Gas Pressure Tester](#)

[D6026 Practice for Using Significant Digits in Geotechnical Data](#)

[D7382 Test Methods for Determination of Maximum Dry Unit Weight and Water Content Range for Effective Compaction of Granular Soils Using a Vibrating Hammer \(Withdrawn 2017\)](#)³

[E691 Practice for Conducting an Interlaboratory Study to Determine the Precision of a Test Method](#)

3. Terminology

3.1 ~~Definitions—Definitions shall be in accordance with the terms and symbols given in~~For definitions of common technical terms used in this standard, refer to Terminology [D653](#).

3.2 *Definitions of Terms Specific to This Standard:*

3.2.1 *complex impedance, n*—the ratio of the phasor equivalent of a steady-state sine-wave or voltage like quantity (driving force) to the phasor equivalent of a steady-state sine-wave current of current like quantity (response)~~(response)~~.⁽⁴⁾~~1~~. In practice, CIMI uses the magnitude of the impedance ratio ($|Z|$) in its calculations.

3.2.2 ~~dielectric properties; relative permittivity, n~~—see the relative dielectric permittivity permittivity of the material relative to that and of dielectric phase-free space.⁵

² For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

³ The last approved version of this historical standard is referenced on www.astm.org.

⁴ The boldface numbers in parentheses refer to a list of references at the end of this standard. Institute of Electrical and Electronics Engineers Standards 100, 1972

⁵ Notwithstanding the statements on precision and bias contained in this test method, the precision of this test method is dependent on the competence of the personnel performing it and the suitability of the equipment and facilities used. Agencies that meet the criteria of Practice [D3740](#) are generally considered capable of competent and objective testing. Users of this test method are cautioned that compliance with Practice [D3740](#) does not in itself ensure reliable results. Reliable testing depends on many factors; Practice [D3740](#) provides a means of evaluating some of those factors. Sears & Zemansky, *University Physics*, 10th Edition

~~3.2.2.1 dielectric phase angle, n —the angular difference in phase between the sinusoidal alternating voltage applied to a dielectric and the component of the resulting alternating current having the same period as the voltage.~~

~~3.2.2.2 relative dielectric permittivity, n —the property that determines the electrostatic energy stored per unit volume for unit potential gradient multiplied by the permittivity of free space (2).~~

~~3.2.3 phase relationship, n —the electrical phase difference between the applied probe-to-probe radio frequency RF voltage, and the resulting soil current.~~

~~3.2.4 probe-to-probe RF voltage, n —the peak value of radio frequency RF voltage measured across two probes that are conducting soil current.~~

~~3.2.5 radio frequency, n —a frequency useful for radio transmission (1).⁴~~

~~3.2.5 soil capacitance, n —the value of the capacitor in an equivalent parallel resistor-capacitor circuit that results from the probe-to-probe voltage, soil current, RF voltage, current in the soil, and resulting phase relationship due to the application of a radio frequency alternating RF voltage source applied to the probes.~~

~~3.2.6 soil current, current, n —the peak value of the radio frequency RF current passing through the soil from one probe electrode to another.~~

~~3.2.7 Soil Model, n —the result of a calibration procedure that establishes a correlating linear function between measured electrical soil properties and measured physical soil properties.~~

~~3.2.8 Soil Model linear correlation function, n —one of the two mathematical expressions that are derived from performing linear regressions on two sets of soil test data; measured physical soil characteristics, and a corresponding set of electrical measurements made on the soil samples.~~

~~3.2.9 soil resistance, n —the value of the resistor in an equivalent parallel resistor-capacitor circuit that results from the probe-to-probe RF voltage, soil current, and resulting phase relationship due to the application of a radio frequency alternating voltage RF source applied to the probes.~~

~~3.2.11 water mass per unit volume, n —the mass of water contained in a volume of soil being measured, and is expressed dimensionally as kg/m^3 .~~

4. Summary of the Test Method

4.1 The test method is a ~~two step~~ two-step process.

4.1.1 A Soil Model that relates impedance measurement to the density and water content of the soil is developed. In this step the electrical measurements are collected at locations that have various water contents and densities typical of the range to be expected. Concurrent with collecting the electrical data, determination of density and water content are performed at the same locations using one or more of the traditional test methods, such as Test Methods **D1556** and **D2216**. The process is repeated over the site sufficiently such that a range of water contents and densities are obtained. The combined data (impedance and density/water content) will generate the correlating linear regression functions of the Soil Model.

4.1.2 Once the Soil Model has been developed the CIMI device is used to make electrical measurements of the soil at locations of unknown density and water content. Using the Soil Model linear correlation functions, the procedure then estimates the values of soil density and water content based on the measured electrical properties.

5. Significance and Use

5.1 CIMI measurements as described in this Standard Test Method are applicable to measurements of compacted soils intended for roads and foundations.

5.2 The test method is a ~~procedure used~~ procedure used for estimating in-place values of density and water content of soils and soil-aggregates based on electrical measurements.

5.3 The test method may be used for quality control and acceptance testing of compacted soil and soil aggregate mixtures as used in construction and also for research and development. The minimal disturbance nature of the methodology allows repetitive measurements in a single test location and statistical analysis of the results.

5.4 Limitations:

5.4.1 This test method provides an overview of the CIMI measurement procedure using a controlling console connected to a soil sensor unit which applies a 3.0 MHz radio frequency RF voltage to an in-place soil via metallic probes that are driven into the soil at a prescribed distance apart. This test method does not discuss the details of the CIMI electronics, computer, or software that utilize on-board algorithms for estimating the soil density and water content

5.4.2 It is difficult to address an infinite variety of soils in this standard. ~~This test method does not address the various types of soils on which the CIMI method may or may not be applicable.~~ However, data presented in **X3.1** provides a list of soil types that are applicable for the CIMI use.

5.4.3 The procedures used to specify how data are collected, recorded, or calculated in this standard are regarded as the industry standard. In addition, they are representative of the significant digits that generally should be retained. The procedures prescribed

in this standard do not consider material variation, purpose for obtaining the data, special purpose studies, or any considerations for the user's objectives; it is common practice to increase or reduce significant digits of reported data to be commensurate with these considerations. It is beyond the scope of this standard to consider significant digits used in analytical methods for engineering design.

NOTE 1—Notwithstanding the statements on precision and bias contained in this test method, the precision of this test method is dependent on the competence of the personnel performing it and the suitability of the equipment and facilities used. Agencies that meet the criteria of Practice **D3740** are generally considered capable of competent and objective testing. Users of this test method are cautioned that compliance with Practice **D3740** does not in itself ensure reliable results. Reliable testing depends on many factors; Practice **D3740** provides a means of evaluating some of those factors.

5.5 All observed and calculated values shall conform to the guidelines for significant digits and rounding established in Practice **D6026**, unless superseded by this test method.

6. Interferences

6.1 Anomalies in the test material with electrical impedance properties significantly different from construction soils and aggregate evaluated during Soil Model development, such as metal objects or organic material, may affect the accuracy of the test method.

6.2 The accuracy of the results obtained by this test method may be influenced by poor contact between the soil electrical probes and the soil being tested. Large air voids, relative to the volume of material being tested, that may be present between soil probes and the surface of the material being tested may cause incorrect density measurements. The shape of the soil electrical probe is important to the quality of the electrical measurements collected by the CIMI.

6.3 When driving the measuring electrical probes, it is critical to the accuracy of the measurement that they make a complete and tight contact with the soil over the entire conical part of the probe.

6.4 If the volume of soil material being tested as defined in **X2.10** has oversize particles or large voids in the electrical field, this may cause errors in measurements of electrical properties. Where lack of uniformity in the soil due to layering, aggregate or voids is suspected, the test site should be excavated and visually examined to determine if the test material is representative of the in-situ material in general and if an oversize correction is required in accordance with Practice **D4718**. Soils must be homogeneous and practically free of rocks that are in excess of five centimeters in diameter (2 in.) and construction debris for the most accurate results.

6.5 Statistical variance may increase for soil material that is significantly drier or wetter than optimum water content (2.5 % over optimum or 6.0 % below optimum) as determined using Test Methods **D698** or **D1557**. Statistical variance may increase for soil material that is compacted to less than 88 % of the maximum dry density as determined using Test Methods **D698** or **D1557**. The CIMI is generally more accurate when the Soil Model range is broader than the range of soil density and water content being tested in the field.

6.6 If temperature measurements are not used, an error may be introduced in the results depending on the value of the difference between the temperature of the soil used for the Soil Model and the unknown in-place soil being measured. All electrical values are equilibrated to $\pm 5.55^{\circ}\text{C}$, 15.5°C (60 °F). The equilibration is necessary because the soil temperature affects the electrical signals that are measured. The operating temperature range where the CIMI has been used globally is for the CIMI is between 1.1°C (34 °F) and 50°C (122 °F).

6.7 This test method applies only to non-frozen soil. The electrical properties of soil change considerably as soil temperature approaches the freezing point of the entrained water.

6.8 The use of electrical probes with different length than those used to make the ~~soil model~~ Soil Model will introduce an error in the interpretation of the data and the estimation of the density of water content of the tested soils.

6.9 The use of a Soil Model that was generated from a different soil than that selected for unknown in-place measurements will result in errors in the estimation of the density and water content of the tested soils.


6.10 Attempts to measure unknown in-place soils with a Soil Model that was generated from a limited range of wet density or water content values, or both, may result in density and water content estimation errors.

6.11 Variation in pore water salinity, soil chemistry, soil mineralogy or other anomalies that causes field-test electronic measurements to be outside the soil model operational range will cause the CIMI to report a warning message. **X2.1** contains additional information regarding variation in electrical measurements and CIMI management techniques.

7. Apparatus

7.1 *Complex-Impedance Measuring Instrument* (See **Fig. 1**)—While exact details of construction of the apparatus and the electric circuits therein may vary, the system shall consist of the following:

7.1.1 *Soil Sensor Unit*—The “Soil Sensor” is a component of the CIMI which electronically combines the ~~Frequency-RF voltage~~ source and the three RF measurement devices. Cables are used to connect the Soil Sensor to the electrical probes.

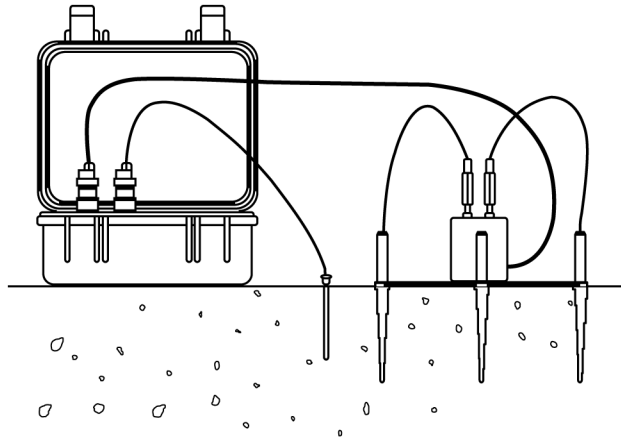

NOTE 1—The wires crossing in the diagram are not touching each other during use to prevent parasitic capacitance.

In the drawing the small probe is the thermistor and the three large probes are three of the four used to collect soil electrical data, the fourth probe is not seen in the section drawing because it is directly behind the center probe.

FIG. 1 Diagram of a GIMI Complex Impedance Measuring Instrument in Use

7.1.1.1 *Radio-Frequency RF Source*—Typically a 3 MHz frequency RF voltage source is applied to the soil under test by probe type electrodes driven into the in-place soil at a prescribed depth and spacing. The radio-frequency current that passes through the soil electrical probes into the soil and the voltage that appears across it measures the RF voltage applied to the soil electrical probes are measured. Additionally the RF current drawn by the soil. Additionally, the electrical phase relationship between the soil current and the probe-to-probe RF voltage is determined.

7.1.1.2 *Ammeter*—Means for measuring the RF soil current.

7.1.1.3 *Voltmeter*—Means for measuring the probe-to-probe RF voltage.

7.1.1.4 *Phase Difference Meter*—Means for measuring the phase difference between the probe-to-probe RF voltage and RF soil current.

7.1.1.5 *Connecting Cables*—For connecting the electrical sensors—soil electrical probes to the display console meter (that is, ammeter, voltmeter, and phase difference meter) to the soil electrical probes and to the display console meter).

7.1.2 *Display Console Unit*

7.2 *Soil Electrical Probes (Four Required, Equally Dimensioned)*—Of electrical conducting material suitable for driving into compacted material, typically constructed of common water hardened drill steel or stainless steel. The soil electrical probes have a conical shape designed to optimize the contact between the electrode and the compacted construction material around the electrode as it is driven in. To further control the contact area of the electrode with the compacted construction material a shoulder is machined at the end of the conical taper that is undercut. When the conical electrode is driven in the compacted construction material to the level where the shoulder is level with the construction material surface, a repeatable surface area of the electrode is in contact with the construction material. The soil electrode achieves good contact with the compacted construction material and allows for consistency in electrical measurements.

7.2.1 The length of soil electrical probes can vary typically having embedment lengths between 101.6 mm (4 in.) and 304.8 mm (12 in.) and diameters between 6.35 mm (1/4 in.) and 12.7 mm (1/2 in.). The bottom diameter of each soil electrical probe is 5 mm (0.2 in.). The top diameter of the embedded length of each soil electrical probe varies between 14 mm (0.56 in.) for the 102 mm (4 in.) embedded length probe and 32 mm (1.25 in.) and 12.7 mm (1/2 in.) for the 305 mm (12 1/2 in.) embedded length probe. During the testing procedure, the soil electrical probe length is selected to best match thickness of the compacted material. Since a portion of the probe must be above the surface to facilitate electrical clip connector, the desired embedment depth must be clearly indicated with a scribed mark or change in geometry. The drawing in Fig. 2 below shows the size and dimensions for the 152 mm (6 in.) electrical probe, the other electrical probes have similar shape and can be reviewed in the manufacturer's catalog.


7.3 A template should be used to place the electrodes as they are driven into the soil. The four probes are driven into the soil at the 0°, 90°, 180°, and 270° in clockwise positions around the periphery of the template.

7.4 *Thermistor* temperature probe that connects to the CIMI for soil temperature measurement, and resulting compensation of calculated electrical soil parameters.

7.5 *Hand Tools*—Hand tools for driving and retrieving the soil electrical probes. A 6- to 10-lb 2.7-kg to 5.4-kg (6-lb to 12-lb) dead blow or brass-faced hammer is used to avoid damaging the steel probes. The soil electrical probes are removed from the soil that has been tested using 30.5 cm (12 in.) channel lock pliers.

7.6 Other components of the system are:

7.6.1 *Safety goggles*, and

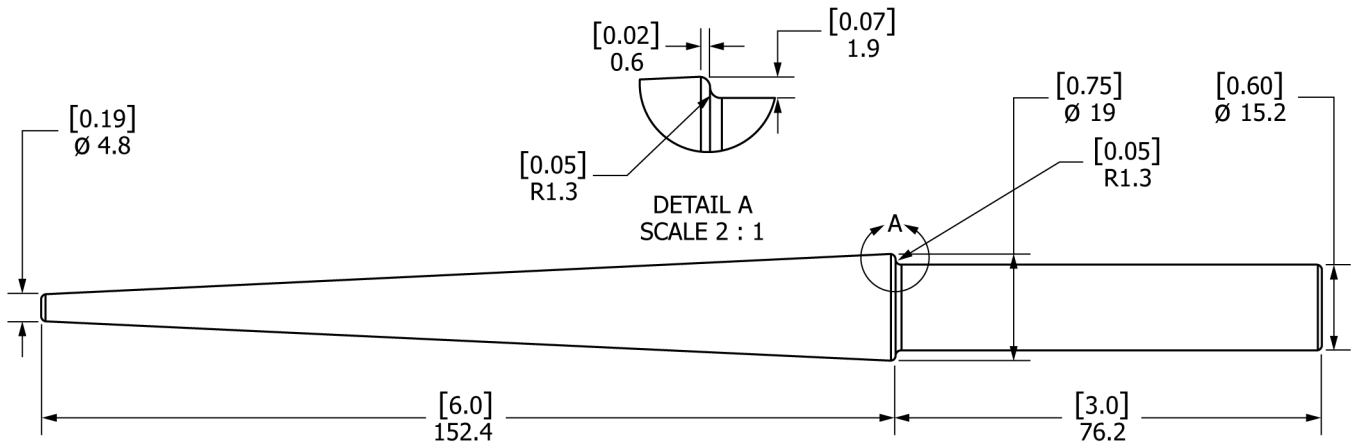

United States Patent Number 7,239,154, July 3, 2007

Dimensions in mm [in]
 Tolerance: ± 0.1 mm [± 0.004 in]
 Material: 0.75 Grade W-1, water-hard. drill rod
 Chamfer as shown: 45 deg., approx. 0.6 mm [0.024 in] on flat (3 places)

FIG. 2 Drawing of a 152.4 mm (6 in.) Soil Electrical Probe

7.6.2 Software with which to download and process the data.

8. Calibration and Standardization

8.1 For a soil type that has not yet been modeled, a Soil Model must be generated. Refer to Section 9 for details on how the testing is performed.

8.2 Determine the test method(s) that will be used in conjunction with developing the Soil Model through calibration. For example, one or more of the test methods cited in 2.1. Assemble the equipment required for each test method.

8.3 Obtain a representative sample of soil from the site where in-place testing is conducted or from the borrow area planned as a source of material. The sample should be of sufficient amount of soil for at least five compaction specimens, typically about 20 Kg (44 lb). For materials with maximum particle size less than 5 cm (No. 4) sieve with a 5-cm screen, kg (44 lb). More material may be required if ancillary testing is planned, such as Atterberg limits, particle size analysis, etc.

8.4 Determine the laboratory compaction characteristics of the material to be tested. Test Methods D698 or D1557 for fine grained soils and soil rock mixtures that exhibit a clear maximum dry density or Test Methods D4253 or D7382 for predominately granular material.

8.5 Determine the depth of investigation required for the job and select the electrical probes with length equal to the depth of investigation. These same length probes must be used for both creating the Soil Model and for testing at the Job Site.

8.6 Select areas on the Job Site where the type of soil is consistent from place to place, and where there are differences in water content and compaction. Special preparation of spots of different densities or water contents should be done the day before, so as to allow stabilization of the soil water content.

8.7 A matrix of six (6) spots should be used during the calibration procedure, consisting of two different soil density conditions and three (3) water content conditions that cover the range that is expected to be measured. The three calibration tests that evaluate high density soil will use test locations that ideally will have soil conditions that are close to the maximum density as determined by Test Methods D1557 or an equivalent method. The range in water content should include low water content, middle range water content, and high water content that is near the optimum water content as determined by Test Methods D1557 and D2216 or equivalent test methods.

8.7.1 A four spot Soil Model matrix will result in the development of a Soil Model with an accuracy that will typically be less than the six-spot matrixes, and a nine-spot soil matrix will only slightly increase the accuracy of the Soil Model over that of the six-spot Soil Model matrixes. The four-spot Soil Model matrixes should have variation of two density conditions and two water content conditions, wherein the high density and high water content should be performed in soil that is near the maximum density and optimum water content as determined by Test Methods D1557 or an equivalent test method. The nine-spot Soil Model should