



Designation: F1800 – 19<sup>ε1</sup>

# Standard Practice for Cyclic Fatigue Testing of Metal Tibial Tray Components of Total Knee Joint Replacements<sup>1</sup>

This standard is issued under the fixed designation F1800; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon ( $\epsilon$ ) indicates an editorial change since the last revision or reapproval.

<sup>ε1</sup> NOTE—Section 8.2 was corrected editorially in January 2020.

## 1. Scope

1.1 This practice covers a procedure for the fatigue testing of metallic tibial trays used in knee joint replacements using a cyclic, constant-amplitude force. It applies to tibial trays that cover both the medial and lateral plateaus of the tibia. This practice may require modifications to accommodate other tibial tray designs.

1.2 This practice is intended to provide useful, consistent, and reproducible information about the fatigue performance of metallic tibial trays with one unsupported condyle. The results are applicable to the laboratory test conditions and may not correlate with *in vivo* performance.

1.3 The values stated in SI units are to be regarded as standard. No other units of measurement are included in this standard.

1.4 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety, health, and environmental practices and determine the applicability of regulatory limitations prior to use.*

1.5 *This international standard was developed in accordance with internationally recognized principles on standardization established in the Decision on Principles for the Development of International Standards, Guides and Recommendations issued by the World Trade Organization Technical Barriers to Trade (TBT) Committee.*

## 2. Referenced Documents

2.1 *ASTM Standards:*<sup>2</sup>

E4 Practices for Force Verification of Testing Machines

E467 Practice for Verification of Constant Amplitude Dynamic Forces in an Axial Fatigue Testing System

E468 Practice for Presentation of Constant Amplitude Fatigue Test Results for Metallic Materials

F2083 Specification for Knee Replacement Prosthesis

## 3. Terminology

3.1 *Definitions of Terms Specific to This Standard:*

3.1.1 *anteroposterior centerline*—line that passes through the center of the tibial tray, parallel to the sagittal plane and perpendicular to the line of load application. For asymmetric tibial tray designs, the appropriate center of the tibial tray shall be determined by the investigator and the rationale reported.

3.1.2 *fixture centerline*—line that passes through the center of the fixture, parallel to the anteroposterior centerline. This line represents the separation between the supported and unsupported portions of the test fixture.

3.1.3 *mediolateral centerline*—line that passes through the center of the tibial tray, parallel to the coronal, or frontal, plane and perpendicular to the line of load application. For asymmetric tibial tray designs, the appropriate center of the tibial tray shall be determined by the investigator and the rationale reported.

3.1.4 *moment arm,  $d_{ap}$* —the perpendicular distance between the mediolateral centerline of the tibia component and the line of load application.

3.1.5 *moment arm,  $d_{ml}$* —the perpendicular distance between the anteroposterior centerline of the tibia component and the line of load application.

## 4. Significance and Use

4.1 This practice can be used to describe the effects of materials, manufacturing, and design variables on the fatigue performance of metallic tibial trays subject to cyclic loading for relatively large numbers of cycles.

4.2 The loading of tibial tray designs *in vivo* will, in general, differ from the loading defined in this practice. The results obtained here cannot be used to directly predict *in-vivo* performance. However, this practice is designed to allow for

<sup>1</sup> This practice is under the jurisdiction of ASTM Committee F04 on Medical and Surgical Materials and Devices and is the direct responsibility of Subcommittee F04.22 on Arthroplasty.

Current edition approved Oct. 1, 2019. Published January 2020. Originally approved in 1997. Last previous edition approved in 2012 as F1800–12. DOI: 10.1520/F1800-19E01.

<sup>2</sup> For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

comparisons between the fatigue performance of different metallic tibial tray designs, when tested under similar conditions.

4.3 In order for fatigue data on tibial trays to be comparable, reproducible, and capable of being correlated among laboratories, it is essential that uniform procedures be established.

**5. Specimen Selection**

5.1 The test component selected shall have the same geometry as the final product, and shall be in finished condition.

**6. Apparatus**

6.1 The tibial tray shall be mounted as a cantilever beam (see Fig. 1 and Fig. 2). Care shall be taken to ensure that the fixation of the tibial tray does not produce abnormal stress concentrations that could change the failure mode of the part. One possible setup involving fixation of the inferior surface and/or clamping of the superior surface is shown in Fig. 1 and Fig. 2. If necessary, bone cement or other high-strength epoxy may be used on the supported aspect of the tibial tray to prevent loosening during the test. Ensure that there is a clearance of at least 5 mm between the undersurface of the loaded compartment on the tibial tray and any part of the fixture.

NOTE 1—The load applicator and the spacer displayed in Fig. 1 and Fig. 2 is an example. Other methods to meet the requirement given by 7.4 might be used.

6.2 The tibial tray shall be positioned such that the antero-posterior centerline and the fixture centerline are aligned with an accuracy of  $\pm 1$  mm in the  $x$  direction and  $\pm 2^\circ$  in the  $x$ - $y$  plane (see Fig. 1 and Fig. 2).

6.3 When the tibial tray design includes a central keel or other prominence, only the medial or lateral half of the keel shall be supported (see 8.3 and Fig. 2).

6.4 A spacer of plastic possessing sufficient stiffness and creep resistance (for example, ultra high molecular weight polyethylene, acetal co-polymer) shall be placed between the tibial tray and the load applicator (see Fig. 3). The spacer shall contain a spherical indentation (or recess) for the spherical indenter. This recess shall be greater than or equal to the

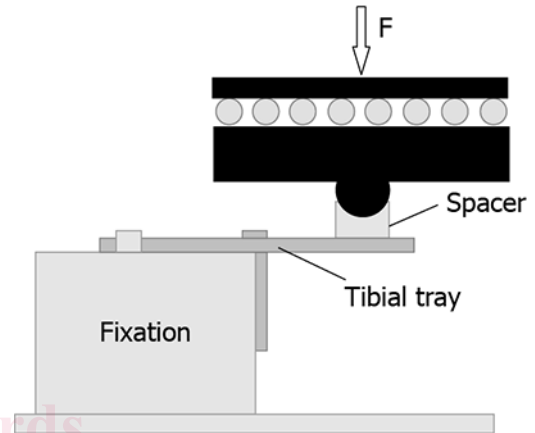
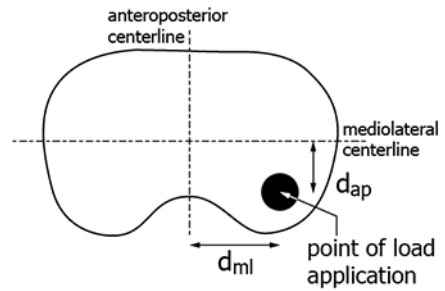


FIG. 2 Schematic of Test Setup With a Central Keel

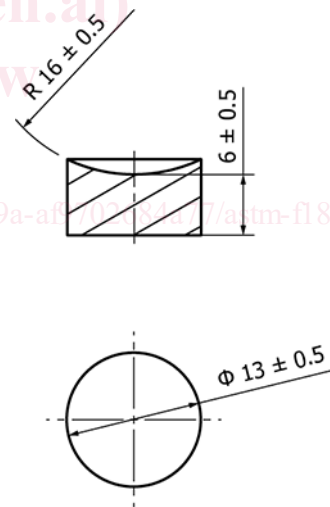


FIG. 3 Recommended Spacer Drawing

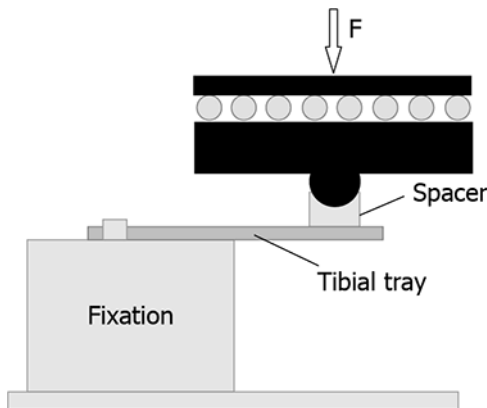


FIG. 1 Schematic of Test Setup Without a Central Keel

diameter of the spherical indenter and is included to minimize the chance of spacer fracture under load. The spacer shall have a minimum thickness of 6 mm, measured at the dome of the sphere. It is recommended that the diameter of the spacer be 13 mm.

NOTE 2—Actual dimensions of the spacer may vary as smaller tibial tray designs may require a smaller diameter disk.

NOTE 3—Metal might be used as the spacer material if the plastic spacer is not capable of transferring the test load.

6.4.1 The spacer shall be placed on the unsupported tibial condyle. The purpose of the spacer is to distribute load to the