



Designation: E1137/E1137M – 08 (Reapproved 2020)

# Standard Specification for Industrial Platinum Resistance Thermometers<sup>1</sup>

This standard is issued under the fixed designation E1137/E1137M; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon ( $\epsilon$ ) indicates an editorial change since the last revision or reapproval.

## 1. Scope

1.1 This specification covers the requirements for metal-sheathed industrial platinum resistance thermometers (PRT's) suitable for direct immersion temperature measurement. It applies to PRT's with an average temperature coefficient of resistance between 0 and 100 °C of 0.385 %/°C and nominal resistance at 0 °C of 100  $\Omega$  or other specified value. This specification covers PRT's suitable for all or part of the temperature range –200 to 650 °C. The resistance-temperature relationship and tolerances are specified as well as physical, performance, and testing requirements.

1.2 The values of temperature in this specification are based on the International Temperature Scale of 1990 (ITS-90).<sup>2</sup>

1.3 The values stated in inch-pound units or SI (metric) units may be regarded separately as standard. The values stated in each system are not exact equivalents, and each system shall be independent of the other.

1.4 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety, health, and environmental practices and determine the applicability of regulatory limitations prior to use.*

1.5 *This international standard was developed in accordance with internationally recognized principles on standardization established in the Decision on Principles for the Development of International Standards, Guides and Recommendations issued by the World Trade Organization Technical Barriers to Trade (TBT) Committee.*

## 2. Referenced Documents

### 2.1 ASTM Standards:<sup>3</sup>

<sup>1</sup> This specification is under the jurisdiction of ASTM Committee E20 on Temperature Measurement and is the direct responsibility of Subcommittee E20.03 on Resistance Thermometers.

Current edition approved May 1, 2020. Published May 2020. Originally approved in 1987. Last previous edition approved in 2014 as E1137/E1137M – 08 (2014). DOI: 10.1520/E1137\_E1137M-08R20.

<sup>2</sup> Preston-Thomas, H., "The International Temperature Scale of 1990 (ITS-90)," *Metrologia*, Vol 27, No. 1, 1990, pp. 3–10, *ibid*, Vol 27, No. 2, 1990, p. 107

<sup>3</sup> For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

[A269 Specification for Seamless and Welded Austenitic Stainless Steel Tubing for General Service](#)

[B167 Specification for Nickel-Chromium-Aluminum Alloys \(UNS N06699\), Nickel-Chromium-Iron Alloys \(UNS N06600, N06601, N06603, N06690, N06693, N06025, N06045, and N06696\), Nickel-Chromium-Cobalt-Molybdenum Alloy \(UNS N06617\), Nickel-Iron-Chromium-Tungsten Alloy \(UNS N06674\), and](#)

[E344 Terminology Relating to Thermometry and Hydrometry](#)

[E644 Test Methods for Testing Industrial Resistance Thermometers](#)

[E1652 Specification for Magnesium Oxide and Aluminum Oxide Powder and Crushable Insulators Used in the Manufacture of Base Metal Thermocouples, Metal-Sheathed Platinum Resistance Thermometers, and Noble Metal Thermocouples](#)

## 3. Terminology

### 3.1 Definitions:

3.1.1 For definitions of terms used in this specification see Terminology [E344](#).

### 3.2 Definitions of Terms Specific to This Standard:

3.2.1 *connecting wire end closure, n*—moisture barrier at the connecting wire end of the sheath.

3.2.1.1 *Discussion*—The closure is intended to provide a seal sufficient to prevent the sensor's insulation resistance from dropping below the minimum requirements.

3.2.2 *connecting wires, n*—wires that run from the element through the connecting wire end closure and external to the sheath.

3.2.3 *excitation, n*—electrical current passing through the element.

3.2.4 *g-level, n*—acceleration of an object relative to the local acceleration of gravity.

3.2.4.1 *Discussion*—For example, a g-level of 5 is equivalent to an acceleration of approximately  $5 \times 9.8 \text{ m/s}^2 = 49.0 \text{ m/s}^2$ .

3.2.5 *minimum immersion length, n*—depth that a thermometer should be immersed, in a uniform temperature environment, such that further immersion does not produce a change in indicated temperature greater than the specified tolerance.

3.2.6 *PRT design, n*—generic term used to differentiate between different PRT construction details, such as element and connecting wire construction, insulation methods, sealing techniques, and mounting methods (for example, spring loaded or direct mounting).

3.2.7 *self-heating, n*—change in temperature of the element caused by the heating effect of the excitation.

3.2.8 *sheath, n*—cylindrical metal tube with an integral welded closure at the end in which the element is located.

4. Significance and Use

4.1 This specification is written to provide common terminology, resistance versus temperature characteristics, accuracy classification, and inspection requirements for a specified configuration of a typical industrial platinum resistance thermometer (PRT).

4.2 This specification may be used as part of the documentation to support negotiations for the purchase and discussion of such thermometers.

5. Classification of Tolerances

5.1 The PRT shall conform to the resistance-temperature relation (see 9.2.1) within the following tolerances:

$$\text{Grade A} = \pm [0.13 + 0.0017 |t|] \text{ } ^\circ\text{C} \quad (1)$$

$$\text{Grade B} = \pm [0.25 + 0.0042 |t|] \text{ } ^\circ\text{C} \quad (2)$$

where:

|t| = value of temperature without regard to sign, °C.

5.1.1 The tolerances are given in Table 1 for a PRT with a nominal resistance of 100 Ω at 0 °C.

6. Ordering Information

6.1 The purchase order documents shall specify the following information to ensure that the PRT is adequately described:

- 6.1.1 The number of this specification,
- 6.1.2 Sheath diameter and overall length (see Fig. 1),
- 6.1.3 Sheath material,
- 6.1.4 Minimum and maximum sensed temperature,
- 6.1.5 Maximum and minimum temperature at connecting wire end closure,

6.1.6 Connection configuration; 2-Wire, 3-Wire, 4-Wire (potentiometric), and compensating loop (4-Wire) (see Fig. 2),

6.1.7 Tolerance, (Grade A, or Grade B),

6.1.8 Nominal resistance at 0 °C (100 Ω unless otherwise specified), and

6.1.9 Serial Number identification requirement (mandatory if an individual calibration or test record will be maintained).

7. Materials and Manufacture

7.1 All materials used shall be in accordance with the following requirements:

7.1.1 *Sheath Materials*—For temperatures not exceeding 480 °C, austenitic stainless steel tubing, conforming to Specification A269. For temperatures not exceeding 650 °C, high-nickel alloy tubing, conforming to Specification B167.

7.1.2 *Sensing Element*—Sensing element shall be platinum.

7.1.3 *Insulation*—The insulating material within the PRT shall be compatible with the temperature range –200 to 650 °C or as specified in 6.1.4. Magnesium oxide (MgO) and aluminum oxide (Al<sub>2</sub>O<sub>3</sub>) powders and crushable insulators conforming to Specification E1652 satisfy this requirement.

7.1.4 *Connecting Wire End Closure Materials*—Closure materials shall provide a barrier against water and other liquids and generally prevent the penetration of water vapor. Any material used shall be compatible with the ambient temperatures specified for the application (see 6.1.5).

7.1.4.1 Typically, epoxy materials are used for ambient temperatures less than 200 °C and moisture impervious ceramic adhesives are used over 200 °C, but the connecting wire end closure shall not be limited to these materials if the end closure meets all other requirements of this specification.

7.1.5 *Connecting Wires*—Typically, materials of connecting wires are: nickel plated copper, nickel, platinum, constantan, or manganin. Individual connecting wires may be comprised of two or more different materials and sizes over their length to accommodate different requirements internal and external to the sensor sheath. Where different materials are used, care must be exercised in their selection to minimize thermoelectrically induced measurement error (see 9.6). Any material used in joining the connecting wires to the PRT element must withstand the maximum operating temperature of the PRT.

8. Other Requirements

8.1 *Pressure*—The PRT shall withstand an external pressure of 21 MPa (3000 psig) and shall be tested in accordance with Test Methods E644 pressure test. The PRT shall remain within the tolerance specified in 5.1.

8.2 *Vibration:*

8.2.1 The PRT shall withstand vibration testing as described in Test Methods E644 using the test parameters in Table 2.

8.2.2 The PRT shall be mounted by installation in the thermowell or by threaded connection to simulate normal mounting procedure as limited by Table 2.

8.2.3 The PRT shall be continuously energized with an oscilloscope-monitored 1.0 mA dc excitation. There shall be no discontinuity of the monitored trace during the test.

TABLE 1 Classification Tolerances<sup>A,B</sup>

Temperature, <i>t</i> , °C	Grade A		Grade B	
	°C	Ω	°C	Ω
–200	0.47	0.20	1.1	0.47
–100	0.30	0.12	0.67	0.27
0	0.13	0.05	0.25	0.10
100	0.30	0.11	0.67	0.25
200	0.47	0.17	1.1	0.40
300	0.64	0.23	1.5	0.53
400	0.81	0.28	1.9	0.66
500	0.98	0.33	2.4	0.78
600	1.15	0.37	2.8	0.89
650	1.24	0.40	3.0	0.94

<sup>A</sup> The table represents values for 3-wire and 4-wire PRT's. Caution must be exercised with 2-wire PRT's because of possible errors caused by connecting wires.

<sup>B</sup> Tabulated values are based on elements of 100.0 Ω (nominal) at 0 °C.

NOTE: EXTERNAL CONNECTING WIRE AND END CLOSURE NEED NOT WITHSTAND MAXIMUM PRT OPERATING TEMPERATURE

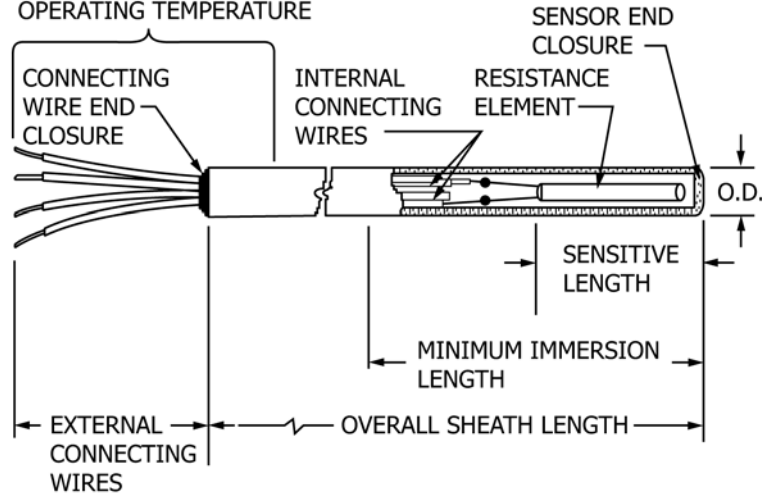


FIG. 1 Typical Industrial Platinum Resistance Thermometer

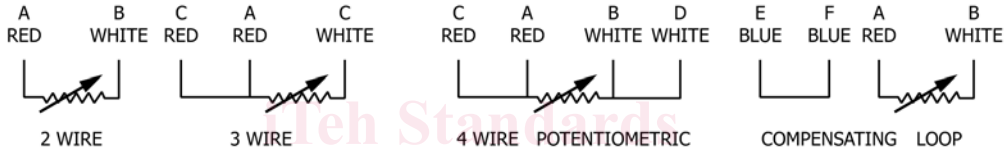


FIG. 2 Connection Configurations

TABLE 2 Vibration Test Parameters

NOTE 1—The values in Table 2 apply to a PRT mounted in a thermowell with nominal diametral clearance of less than 0.25 mm (0.01 in.). If the PRT is not mounted in a thermowell, the values in Table 2 apply to a PRT with an unsupported stem length less than 100 mm (4 in.).

Frequency	5 to 500 Hz
Test Level	1.27 mm (0.05-in.) double amplitude displacement or peak g-level of 3, whichever is less
Resonant Dwell Time	30 min for each resonant point
Cycling Time	3 h per axis less the time spent at resonant dwells at the axis.
Mounting	As normally mounted including the mating thermowell, if applicable.

TABLE 3 Insulation Resistance

Applied dc Voltage, Volts dc		Minimum Insulation Resistance	
min	max	°C	MΩ
10	50	25 ± 5	100
10	50	300 ± 10	10
10	50	650 ± 15	2

8.2.4 After the PRT is tested for vibration the insulation resistance of the PRT shall remain within the tolerance of Table 3 and the resistance at 0 °C within the tolerance specified in 5.1.

8.3 Mechanical Shock:

8.3.1 The PRT shall withstand mechanical shock testing as described in Test Methods E644. The half-sine pulse shall have a peak g-level of 50 and duration of 11 ms.

8.3.2 The PRT shall be continuously energized with an oscilloscope-monitored 1.0 mA dc excitation. There shall be no discontinuity of the monitored trace during the test.

8.3.3 After the PRT is tested for mechanical shock, the insulation resistance of the PRT shall remain within the tolerance of Table 3 and the resistance at 0 °C within the tolerance in 5.1.

8.4 Thermal:

8.4.1 The PRT shall be capable of continuous operation over the specified temperature range (see 6.1).

8.4.2 The connecting wire end closure and external connecting wires need not withstand the entire PRT operating temperature range. As a minimum, these materials must withstand the ambient temperature limits specified for the application (see 6.1.5).

9. Performance

9.1 Excitation:

9.1.1 The PRT must be constructed such that it is usable in ac or dc measurement systems. In ac measuring systems, reactance effects shall be considered.

9.1.2 The PRT shall be capable of operating with continuous excitation of 10 mA. However, excitation of 1 mA or less is

recommended to minimize measurement errors associated with self-heating (see 9.4).

## 9.2 Resistance Versus Temperature Relation:

9.2.1 *Resistance-Temperature Equations*—Within the specified tolerances (see 5.1), the PRT shall have resistance-temperature characteristics defined as follows: for the range  $-200\text{ °C} \leq t < 0\text{ °C}$ :

$$R_t = R_o [1 + At + Bt^2 + C(t - 100)t^3] \Omega \quad (3)$$

for the range  $0\text{ °C} \leq t \leq 650\text{ °C}$ :

$$R_t = R_o [1 + At + Bt^2] \Omega \quad (4)$$

where:

- $t$  = temperature (ITS-90), °C,
- $R_t$  = resistance at temperature ( $t$ ),
- $R_o$  = resistance at  $0\text{ °C}$ ,
- $A$  =  $3.9083 \times 10^{-3}\text{ °C}^{-1}$ ,
- $B$  =  $-5.775 \times 10^{-7}\text{ °C}^{-2}$ , and
- $C$  =  $-4.183 \times 10^{-12}\text{ °C}^{-4}$ .

9.2.2 *Resistance Table*—Resistance values of the PRT versus temperature using the equations of 9.2.1 and  $R_o$  of  $100\ \Omega$  are given in Table 4.

9.2.3 Inverse equations that may be used to compute values of temperature (°C) as a function of resistance are given in Appendix XI.

9.3 *Insulation Resistance*—The insulation resistance between each connecting wire and the sheath shall meet the requirements of Table 3 when tested in accordance with Test Methods E644. The PRT shall be tested with at least the minimum immersion length exposed to the temperature environment.

9.4 *Self-heating*—A power of at least 33 mW shall be required to produce a self-heating of  $1\text{ °C}$  when the PRT is tested in water in accordance with Test Methods E644.

9.5 *Thermal Response Time*—The 63.2 % response time shall not exceed the values in Table 5 when determined in accordance with Test Methods E644. The step change in temperature shall be from  $20 \pm 5\text{ °C}$  air to  $77 \pm 5\text{ °C}$  water flowing at  $0.9 \pm 0.09\text{ m/s}$  ( $3.0 \pm 0.3\text{ ft/s}$ ).

9.6 *Thermoelectric Effect*—When tested in accordance with Test Methods E644 at the upper operating temperature, the PRT shall remain within the tolerances specified in 5.1 with an excitation current of  $1\text{ mA dc} \pm 15\%$ , regardless of polarity.

NOTE 1—Internal and external connecting wire composition, wire inhomogeneity, and temperature gradients within the PRT can be sources for generation of thermoelectric EMF. Some resistance determination error can result from this EMF. The magnitude and sense of this thermoelectric effect error depends on the excitation current, temperature distribution, and construction of the PRT. For a given PRT, the thermoelectric effect can be minimized by using an alternating polarity excitation with a suitable measurement circuitry.

9.7 *Stability*—When tested in accordance with Test Methods E644, the PRT shall remain within the tolerances specified in 5.1 for a four-week test. During this test, the resistance at  $0\text{ °C}$  shall be checked at regular intervals (two times per week).

9.8 *Minimum Immersion Length*—When determined in accordance with Test Methods E644, the PRT minimum immer-

sion length shall be less than 51 mm (2 in.). The limit of uncertainty shall be 0.13 and  $0.25\text{ °C}$  for Grade A and Grade B PRT's respectively.

9.9 *End Seal Integrity*—When tested in accordance with Test Methods E644, the PRT shall meet the minimum insulation resistance value at  $25 \pm 5\text{ °C}$  as specified in Table 3.

## 10. Dimensions, Mass, and Permissible Variations

10.1 A PRT without a process fitting or other means of attachment is shown in Fig. 1.

10.2 PRT's manufactured in accordance with this specification shall be able to pass through the straightness ring gauge with the gauge sizes listed in Table 6.

## 11. Required Tests

11.1 *Qualification Tests*—The PRT shall be subjected to the tests outlined in Table 7 to demonstrate conformance to this specification. The manufacturer shall perform these tests at least one time to qualify the PRT design. Thereafter, it is recommended these tests be used on a periodic basis to verify process control.

11.1.1 *Qualification Test Report*—The manufacturer shall prepare and retain a qualification test report applicable to the PRT design that documents the model number, test procedure (by reference to Test Methods E644 and this specification), and the results obtained.

11.2 *Acceptance Tests*—The manufacturer shall verify that the PRT to be delivered satisfies the following minimum test requirements: resistance at  $0\text{ °C}$  (see 5.1), room temperature insulation resistance (see 9.3), and dimensions (see 10.2).

NOTE 2—The purchaser may perform any of the tests included in Table 7 as a basis for acceptance or rejection.

## 12. Declaration of Conformity

12.1 The manufacturer shall provide a document to the purchaser that states the PRT satisfies the requirements of this specification.

## 13. Product Marking

13.1 Each PRT shall carry a permanent identification marking, which includes, as a minimum, the PRT serial number or date code. A serial number is required if the PRT will be subjected to calibration or testing that requires an individual test record (see 6.1.9). Additional identification including the PRT producer, grade, and this ASTM designation shall be present on the PRT, on a tag attached to the PRT, or on the PRT packaging.

## 14. Packaging

14.1 Each PRT shall be packaged to adequately protect it against handling shock and vibration in transportation and storage.

## 15. Keywords

15.1 ITS-90; metal sheath; platinum resistance thermometer; PRT