



Designation: E592 – 20

# Standard Guide to Obtainable ASTM Equivalent Penetrameter Sensitivity for Film Radiography of Steel Plates ¼ to 2 in. (6 to 51 mm) Thick with X-Rays and 1 to 6 in. (25 to 152 mm) Thick with Cobalt-60<sup>1</sup>

This standard is issued under the fixed designation E592; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reappraisal. A superscript epsilon ( $\epsilon$ ) indicates an editorial change since the last revision or reappraisal.

## 1. Scope\*

1.1 This guide to obtainable equivalent penetrameter sensitivity covers the minimum penetrameter thicknesses for which the image of the 1T and 2T holes is visible for a few practical radiographic conditions using industrial X-ray film. The values represent near optimum sensitivity for flat steel plates. Radiographic conditions that give higher values of scatter buildup from the specimen or backscattered radiation at the image plane will give poorer sensitivity.

1.2 Eight radiographs that illustrate sensitivities obtainable with practical radiographic systems are included as adjuncts to this guide and must be purchased from ASTM.

1.3 *Units*—The values stated in inch-pound units are to be regarded as standard. The values given in parentheses are mathematical conversions to SI units that are provided for information only and are not considered standard.

1.4 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety, health, and environmental practices and determine the applicability of regulatory limitations prior to use.*

1.5 *This international standard was developed in accordance with internationally recognized principles on standardization established in the Decision on Principles for the Development of International Standards, Guides and Recommendations issued by the World Trade Organization Technical Barriers to Trade (TBT) Committee.*

<sup>1</sup> This guide is under the jurisdiction of ASTM Committee E07 on Nondestructive Testing and is the direct responsibility of Subcommittee E07.02 on Reference Radiological Images.

Current edition approved June 1, 2020. Published June 2020. Originally approved in 1977. Last previous edition approved in 2015 as E592 – 15. DOI: 10.1520/E0592-20.

## 2. Referenced Documents

### 2.1 ASTM Standards:<sup>2</sup>

E746 Practice for Determining Relative Image Quality Response of Industrial Radiographic Imaging Systems

E999 Guide for Controlling the Quality of Industrial Radiographic Film Processing

E1025 Practice for Design, Manufacture, and Material Grouping Classification of Hole-Type Image Quality Indicators (IQI) Used for Radiography

E1316 Terminology for Nondestructive Examinations

E1742 Practice for Radiographic Examination

E1735 Practice for Determining Relative Image Quality Response of Industrial Radiographic Imaging Systems from 4 to 25 MeV

E1815 Test Method for Classification of Film Systems for Industrial Radiography

### 2.2 ISO Standard:<sup>3</sup>

ISO 7004 Photography—Industrial Radiographic Films—Determination of ISO Speed, ISO Average Gradient, and ISO Gradients G2 and G4 When Exposed to X- and Gamma-Radiation

### 2.3 Military Standard:<sup>4</sup>

NAVSEA Technical Publication T9074-AS-GIB-010/271 Requirements for Nondestructive Testing Methods

### 2.4 ASTM Adjuncts:<sup>5</sup>

Guide for Equivalent Penetrameter Sensitivity Between X-Rays and Cobalt-60


<sup>2</sup> For referenced ASTM standards, visit the ASTM website, [www.astm.org](http://www.astm.org), or contact ASTM Customer Service at [service@astm.org](mailto:service@astm.org). For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

<sup>3</sup> Available from American National Standards Institute (ANSI), 25 W. 43rd St., 4th Floor, New York, NY 10036, <http://www.ansi.org>.

<sup>4</sup> Available from Naval Sea Systems Command (NAVSEA), 1333 Isaac Hull Avenue, SE, Washington Navy Yard, DC 20376, <https://www.navsea.navy.mil>.

<sup>5</sup> Available from ASTM Headquarters. Order [RRE0592](https://www.astm.org).

\*A Summary of Changes section appears at the end of this standard

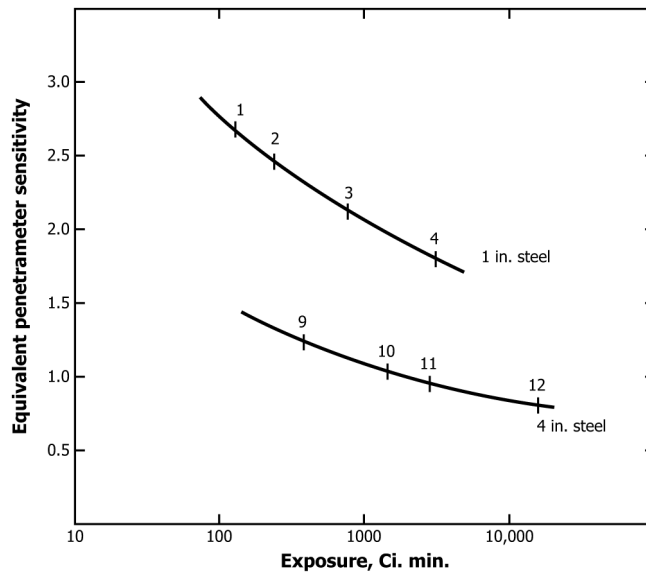

NOTE 1—The demonstration radiograph numbers on curves refer to exposure conditions given in Table 1.

FIG. 1 Obtainable Penetrator Sensitivity for Cobalt-60 Radiography of 1 and 4 in. (25 and 102 mm) Thick Steel at 36 in. (914 mm) Distance

### 3. Terminology

3.1 *Definitions*—For definitions of terms used in this standard, refer to Terminology E1316, Section D.

3.2 *Definitions of Terms Specific to This Standard:*

3.2.1 *demonstration radiograph, n*—radiographs from which data was gathered for Fig. 1 and Fig. 2.

3.2.2 *reference radiograph, n*—the adjunct materials illustrations.

### 4. Significance and Use

4.1 A key consideration with any radiographic system is its contrast resolution and spatial resolution capability (that is, sensitivity). The degree of obtainable sensitivity with a given system is dependent upon several radiographic parameters such as source energy level, film system class, type and thickness of intensifying screens, exposure (density), etc. This guide permits the user to estimate the degree of sensitivity that may be obtained with X-rays and Cobalt-60 gamma rays when using a prescribed set of radiographic parameters. This guide may also be used in conjunction with Practices E746 or E1735 to provide a basis for developing data for evaluation of a user's specific system. This data may assist a user in determining appropriate parameters for obtaining desired degrees of radiographic system sensitivity. An alternate to this approach is the use of those adjunct radiographic illustrations detailed in Section 6.

### 5. Procedure

5.1 *Sensitivity for 1/4 to 2 in. (6 to 51 mm) Thick Steel Using X-Rays:*

5.1.1 The values of sensitivity were determined from a statistical study of visibility of images of penetrator holes. Near 100 % certainty of seeing the image of a hole on any

radiograph was taken as the criterion for determining sensitivity. Most radiographs will show slightly better sensitivity than indicated in Figs. 3-5 because of the statistical nature of recording information from a beam of X-rays, but occasionally, one will not show quite as good sensitivity.

5.1.2 Equivalent Penetrator Sensitivity (EPS) is defined in Eq 1. For a full discussion of EPS see Appendix X1 of Practice E1025.

$$EPS, \% = 70.7 (dT)^{1/2}/t \quad (1)$$

where:


- $d$  = diameter of penetrator hole,
- $T$  = thickness of penetrator, and
- $t$  = specimen thickness.

A clear definition of equivalent penetrator sensitivity has not been established for penetrators less than 10 mils (0.25 mm) thick. For this work, it was calculated as in Eq 1. The change in slope of the steel thickness curves on Fig. 4 and Fig. 5 is a result of the established 10 mil minimum hole diameter in Practice E1025 and Practice E1742, Appendix A1.

5.1.3 Fig. 3 illustrates obtainable equivalent penetrator sensitivity for four X-ray films. The films are identified by reciprocal speed (see Test Method E1815) when exposed in accordance with ISO 7004 in a 200 kV range, and processed in accordance with the manufacturer's recommendations (see Guide E999).


Film Type	Roentgen Speed	ISO Speed	ASTM Class
1	17	1700	none
2	4.0	400	III
3	1.2	120	I
4	0.35	35	Special

5.1.4 The radiographic exposure conditions for reference radiographs 1, 2, 3, and 4 were: 36 in. (914 mm) focus-film

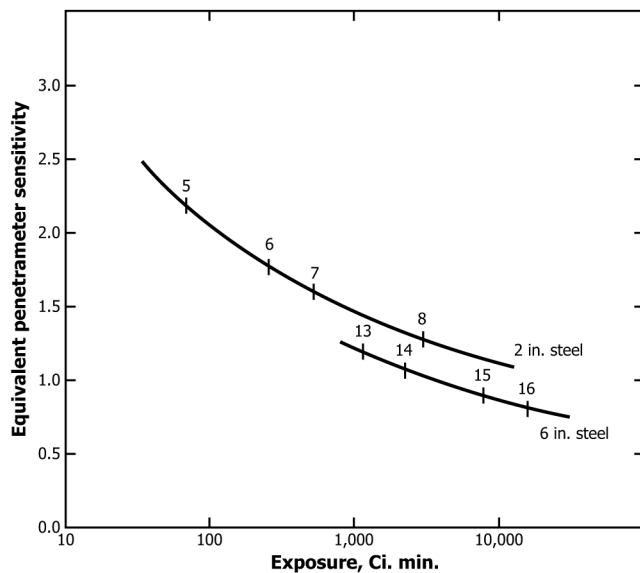

NOTE 1—The demonstration radiograph numbers on curves refer to exposure conditions given in Table 1.

FIG. 2 Obtainable Penetrameter Sensitivity for Cobalt-60 Radiography of 2 and 6 in. (51 and 152 mm) Steel at 36 in. (914 mm) Distance

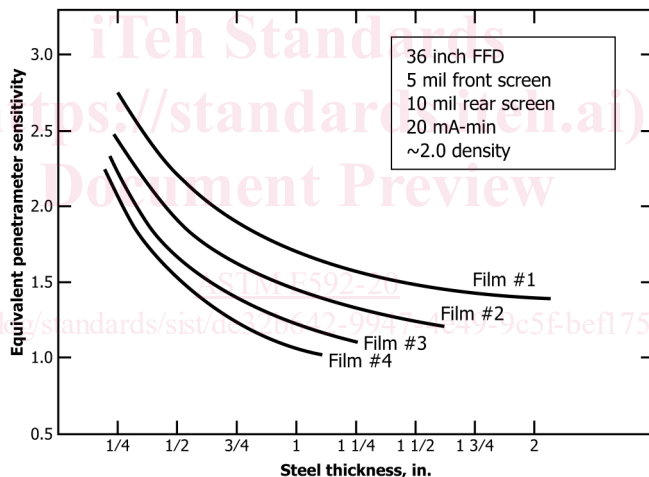

NOTE 1—See 5.1.4 for exposure conditions.

FIG. 3 Obtainable Penetrameter Sensitivity for 1/4 to 2 in. (6 to 51 mm) Thick Steel When Radiographing with X-Rays

distance, 5 mil (0.13 mm) front and 10 mil (0.25 mm) back lead screens, 20 mA-min exposure, and kilovoltage adjusted to give a density of near 2.0. The focal spot size was not recorded with the original data.


5.1.5 Most high-quality industrial X-ray films intended for direct or lead screen exposure, that are exposed and developed accordingly to give these speed values, will provide similar illustrations of sensitivity. Interpolation will give illustrations of sensitivity for speeds obtained with other film systems.

5.1.6 In Fig. 4, the data are presented to show the thinnest penetrameter for which the image of the 2T hole will be visible. The intersection of the line for a particular steel thickness and the line for a given film projected onto the abscissa gives the best obtainable equivalent penetrameter sensitivity. Two different penetrameter markings are displayed in the figure: those for

Practice E1025 and those for Practice E1742, Annex A1 (also NAVSEA Technical Publication T9074-AS-GIB-010/271 and former MIL-STD-453 penetrameter markings). The intersection projected to the left ordinate gives the minimum penetrameter marking (thickness in mils) in accordance with Practice E1025 for which the image of the 2T hole will be visible. The right ordinate gives the minimum penetrameter marking in accordance with Practice E1742, Annex A1, for which the image of the 2T hole will be visible.


5.1.7 Fig. 5 gives the Practice E1025 and Practice E1742, Annex A1 markings for which the image of the 1T hole will be visible.

5.1.8 To take an example, on Fig. 4 the intersection of the curve for 1 in. (25 mm) thick steel and for Film No. 2 shows that the penetrameter sensitivity is 1.45 %. The minimum

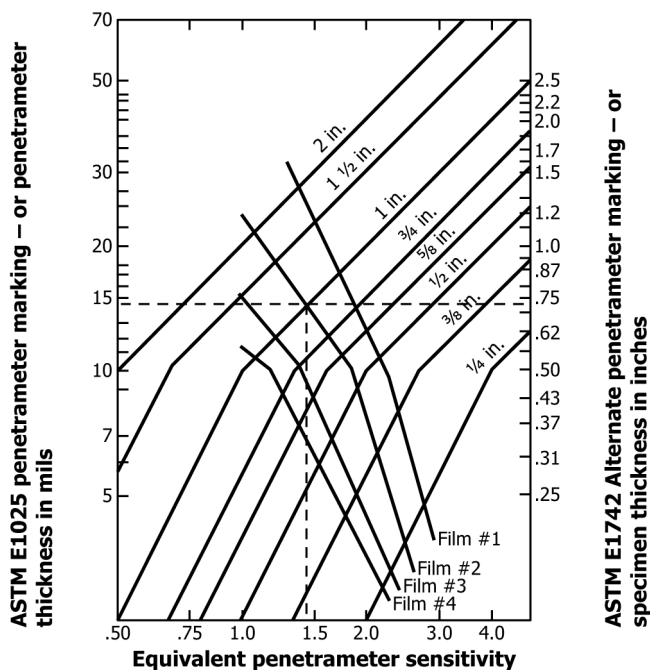

NOTE 1—See 5.1.4 for exposure conditions.

FIG. 4 Penetrator Sensitivity and Minimum Penetrator Markings for Showing the 2T Hole When Radiographing 1/4 to 2 in. (6 to 51 mm) Thick Steel with X-Rays

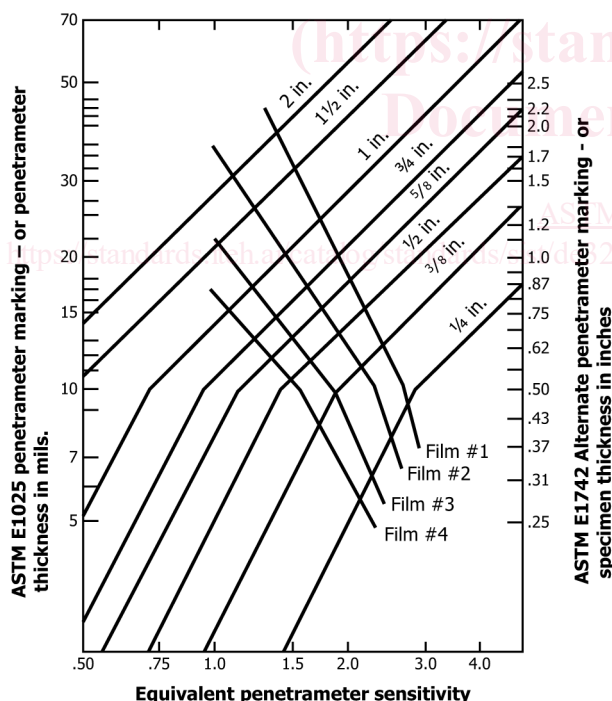

NOTE 1—See 5.1.4 for exposure conditions.

FIG. 5 Penetrator Sensitivity and Minimum Penetrator Markings for Showing the 1T Hole When Radiographing 1/4 to 2 in. (6 to 51 mm) Thick Steel with X-Rays

Practice E1025 penetrator thickness that will show the 2T hole image is 15. The corresponding Practice E1742, Annex A1 marking is 0.75 (see dashed lines). On Fig. 5 the sensitivity is, of course, 1.45 %. The minimum Practice E1025 penetrator

thickness that will show the 1T hole image is ‘22’ and the Practice E1742, Annex A1 specification marking is ‘1.1.’

5.1.9 If radiographs are exposed to a density other than 2 by changing mA·min exposure, but not kilovoltage, the equivalent penetrator sensitivity (EPS) that will be obtained in the density range 1.3 to 4 can be calculated approximately as follows:

$$EPS_D = EPS_2 (2/D)^{1/4} \quad (2)$$

where:

$D$  = density to which the radiograph is exposed,  
 $EPS_2$  = sensitivity for  $D = 2.0$ , and  
 $EPS_D$  = sensitivity for  $D$ .

5.2 Sensitivity for 1 to 6 in. (25 to 152 mm) Thick Steel Using Cobalt-60:

5.2.1 For Cobalt-60 radiography of steel, the variables that affect image quality and that can be controlled are the speed of the film and the recording of scattered radiation relative to the recording of image-forming radiation. The relative recording of scatter (the scatter buildup factor) can be decreased by the use of lead filtration between the specimen and the film or by the use of low-atomic-number metal screens. Either method gives nearly equal improvement in image quality for a given increase in exposure.

5.2.2 Radiographs of flat steel plates were made either with 10 mil (0.25 mm) thick front and back lead or copper screens. A30-Ci source, 4 by 4 mm, was used with a setup designed to give maximum buildup of scatter in the specimen and no backscatter. The source-to-film distance was 36 in. (914 mm). The exposure was adjusted for a density near 2.0.

5.2.3 The four films used are identified by reciprocal roentgen speed when exposed in accordance with ISO 7004 using Cobalt-60 radiation and processed in accordance with the manufacturer’s recommendations.

Film Type	Roentgen Speed	ISO Speed
1	3.5	350
2	0.67	67
3	0.13	13
4	0.04	4

5.2.4 Fig. 1 shows equivalent penetrator sensitivity obtainable for 1 and 4 in. (25 and 102 mm) thick steel as a function of exposure in curie minutes. Fig. 2 shows equivalent penetrator sensitivity obtainable for 2 and 6 in. (51 and 152 mm) thick steel as a function of exposure. The numbers on the curves indicate the various radiographic exposures shown in Table 1.

5.2.5 The films, screens, and exposures used for the radiographs were as specified in Table 1.

6. Descriptions and Suggested Uses of Reference Radiographic Illustrations (See 1.2)

6.1 Eight radiographs were chosen to illustrate sensitivities obtainable with practical radiographic systems. Table 2 lists films and exposure conditions for reference radiograph illustrations Nos. 1 through 6 (for X-ray) and Table 1 lists films and exposure conditions for reference radiograph illustrations Nos. 7 and 8 (for Cobalt-60). The reference radiograph illustrations for Cobalt-60 correspond to demonstration radiographs Nos. 9 and 12 in Table 1 and Fig. 1.