



Designation: G18 – 07 (Reapproved 2020)

Standard Test Method for Joints, Fittings, and Patches in Coated Pipelines¹

This standard is issued under the fixed designation G18; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

1. Scope

1.1 This test method describes determination of the comparative corrosion preventative characteristics of materials used for applications to joints, couplings, irregular fittings, and patched areas in coated pipelines. The test method is applicable to materials whose principal function is to act as barriers between the pipe surface and surrounding soil environment.

1.2 The test method described employs measurements of leakage current, capacitance, and dissipation factor to indicate changes in the insulating effectiveness of joint and patching materials.

1.3 The values stated in SI units are to be regarded as the standard. The values given in parentheses are for information only.

1.4 The values stated in SI units to three significant decimals are to be regarded as the standard. The values given in parentheses are for information only.

1.5 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety, health, and environmental practices and determine the applicability of regulatory limitations prior to use.*

1.6 *This international standard was developed in accordance with internationally recognized principles on standardization established in the Decision on Principles for the Development of International Standards, Guides and Recommendations issued by the World Trade Organization Technical Barriers to Trade (TBT) Committee.*

2. Referenced Documents

2.1 *ASTM Standards:*²

G12 Test Method for Nondestructive Measurement of Film

¹ This test method is under the jurisdiction of ASTM Committee D01 on Paint and Related Coatings, Materials, and Applications and is the direct responsibility of Subcommittee D01.48 on Durability of Pipeline Coating and Linings.

Current edition approved Aug. 1, 2020. Published August 2020. Originally approved in 1971. Last previous edition approved in 2013 as G18 – 07 (2013). DOI: 10.1520/G0018-07R20.

² For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

Thickness of Pipeline Coatings on Steel (Withdrawn 2013)³

3. Summary of Test Method

3.1 The test method consists of an immersion test where coated pipe specimens, each containing a simulated joint, tee, or patched area, are suspended in an electrolyte and placed under cathodic protection by connecting the specimens to the negative (–) terminal of a 6-V d-c power supply (see Fig. 1). An anode, also immersed in the electrolyte and connected to the positive (+) terminal of the power supply, completes the test circuit. Joint or patch performance is followed through periodic determinations of leakage current measured as voltage drops across a calibrated resistor in the anode-to-cathode circuit.

3.2 Capacitance and dissipation factor measurements are used to supplement the periodic leakage current determinations.

4. Significance and Use

4.1 The exposed metal surfaces at joints, fittings, and damaged areas in an otherwise coated pipeline will be subjected to corrosion if allowed to come in contact with the soil environment. The performance of joint and patching materials designed to function as protective coverings will depend upon such factors as the ability of the material to bond to both the pipe coating and exposed metal surfaces, the integrity of the moisture seal at lapped joints, and the water absorption characteristics of the joint material.

4.2 The existence of substantial leakage current through the coating joint, patch, or fitting is reliable evidence that the material has suffered a significant decrease in its performance as a protective barrier. In a similar manner, measured changes in joint capacitance and dissipation factor are useful because they are related to the water absorption rate of the joint material. Water permeating an insulating barrier increases its capacitance and its progress can be measured through the use of a suitable impedance bridge.

³ The last approved version of this historical standard is referenced on www.astm.org.

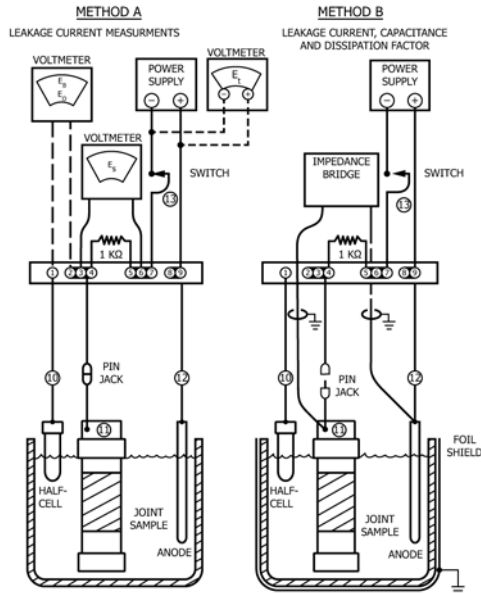



FIG. 1 Test Circuits

5. Apparatus

5.1 Test Vessel, nonconducting, shall be used to contain the test specimens. Dimensions of the vessel shall permit the following requirements:

5.1.1 The test vessel shall be large enough to allow for suspension of the specimens in a vertical position and equidistant from a centrally located anode. The specimens shall not touch either each other, the walls, or bottom of the test vessel.

5.1.2 The test vessel shall be deep enough to allow for immersion of the specimens in the electrolyte to the lower edge of the upper moisture shield (see Fig. 2).

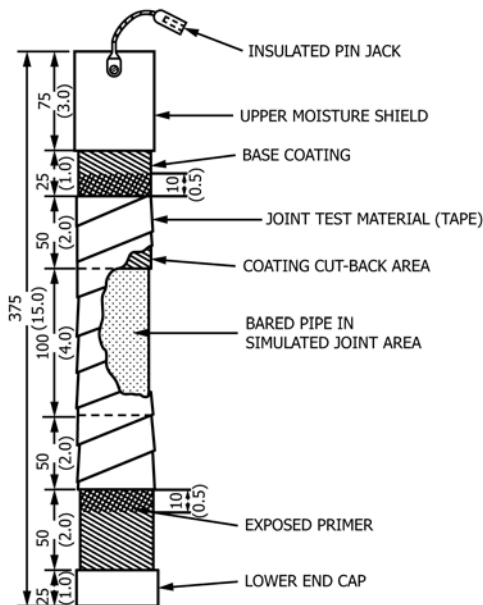

NOTE 1—All dimensions are in millimetres with inches in parentheses.

FIG. 2 Joint Test Specimen

NOTE 1—A commercially available, 42 L (11-gal) waste container of high-density polyethylene can be conveniently used as a test vessel and will accommodate up to six test specimens of a size indicated in 7.2.

5.2 Support Plate, fabricated from a nonconductive material, to suspend the specimens in the test vessel. The support plate shall contain an access hole for the reference electrode. A typical test cell is illustrated in Fig. 3.

5.3 Anode, fabricated from 9.525 mm (0.375-in.) diameter 300 series stainless steel rod, 609.6 mm (24.00 in.) long. Other inert anodes such as carbon or platinum may be used.

5.4 D-C Voltmeter, to serve the dual purpose of (1) measuring leakage current as a potential drop across a 1,000-Ω shunt in the measuring circuit and (2) measuring the potential of the test specimen with reference to a Cu-CuSO₄ half cell. The instrument characteristics for these functions shall be:

5.4.1 Voltage Range—50 μV full scale to 10 V full scale in overlapping 1× and 3× ranges.

5.4.2 Accuracy—±3 percent of full scale on all ranges.

5.4.3 Input Resistance—Greater than 10 MΩ on all ranges.

5.5 Thickness Gage—Measurements of coating thickness will be required for this test. Any instrument suitable for use with Test Method G12 can be used. However, the choice of measuring gage shall be compatible with the joint coating thickness that will be encountered in the test.

5.6 Ohmmeter—Measurements for end-cap integrity shall be made with a suitable ohmmeter capable of reading resistance to an upper limit of 1000 MΩ ± 5 %.

5.7 Reference Electrode—A Cu-CuSO₄ half cell of conventional glass or plastic tube with porous plug construction, but preferably not over 19.05 mm (¾ in.) in diameter, having a potential of -0.316 V with respect to the standard hydrogen electrode.

NOTE 2—A saturated calomel half cell may be used, but measurements made with it shall be converted to the Cu-CuSO₄ reference for reporting

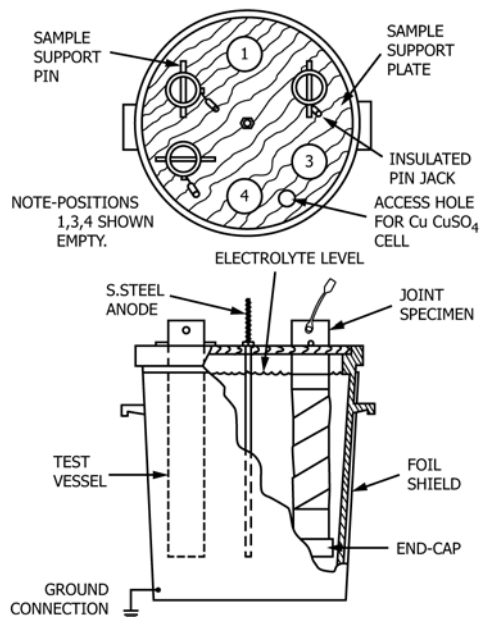


FIG. 3 Joint Test Cell

by adding -0.072 V to the observed reading.

5.8 Voltage Source—A battery or rectifier-type power supply shall be used to maintain a potential difference of 6.0 ± 0.1 V dc between each of the test specimens and the Cu-CuSO₄ half cell. Where multiple specimens are tested, a suitable voltage-dividing circuit will be required for individual control of the voltage applied to each specimen.

5.9 Circuit Wiring from the anode to specimen shall be of No. 18 Awg insulated copper. A switch for disconnecting each specimen from its voltage source shall be included in the circuit. A1000 $\Omega \pm 1$ percent, 1-W (minimum) precision resistor shall be placed in the anode-to-cathode circuit as a shunt for current. A diagram illustrating the test cell wiring appears as **Fig. 1**.

5.10 Capacitance Bridge—Measurements of specimen capacitance and dissipation factor shall be made with a low-voltage a-c, resistive ratio arm-type bridge having the following characteristics:

5.10.1 Oscillator Frequency, 1 kHz ± 2 % tolerance.

5.10.2 Series Capacitance Range, 100 pF to 1100 pF accuracy ± 1 % ± 1 pF, whichever is larger.

5.10.3 Dissipation Factor Range, 0.002 to 1.0 at 1 kHz accuracy ± 5 % or ± 0.001 dissipation, whichever is larger.

5.11 Connectors—Miniature, pin-type, insulated jacks shall be used at the point of connection to each test specimen. The jacks serve two important functions: (1) they permit the disconnection of the specimen from the voltage source when the impedance bridge is in use, and (2) disconnection of the specimen from the test circuit also removes the effect of stray capacitance due to excessive lead length that may introduce error into impedance bridge measurements.

5.12 Foil Shield—As an additional safeguard against stray capacitance effects, wrap the entire test vessel in heavy-gage aluminum foil as shown in **Fig. 3** and ground the shield.

6. Materials

6.1 Electrolyte—The electrolyte shall consist of potable tap water with the addition of 3 weight percent of technical-grade sodium chloride.

6.2 Materials for sealing the ends of the specimens may consist of waxes, epoxies, or other suitable materials. However, they should have a dielectric constant in the range from 2 to 6, and exhibit a low water-absorption rate. It is also important that the end-cap material maintains good adhesion to any coated pipe surfaces throughout the test period.

7. Test Specimen

7.1 The joint specimen shall be prepared from a representative piece of 60.325 mm (2.375 in.) outside diameter, Schedule 40, production-coated pipe.

7.2 Each piece of coated pipe shall be 381 mm (15.0 in.) long and serve as a carrier for the particular joint material to be tested.

7.3 The simulated coating joint shall be made by cleaning away a 101.6 mm (4.0-in.) band of pipe coating starting from a point 203.2 mm (8.0 in.) below the upper end of the pipe. The

coating may be removed by power brushing or any other suitable device that will remove all of the coating in the area indicated and leave a clean metal surface behind.

7.4 The lower end of the test specimen shall be plugged flush with a stopper and sealed or capped with a material meeting the requirements of **6.2**.

7.5 When used, the primer shall be applied to the test specimen in sufficient quantity to coat the test specimen from a point 88.9 mm (3.50 in.) below its upper end and ending at a point 317.5 mm (12.5 in.) from the upper end. This will allow for a 12.7-mm (0.5-in.) band of excess primer beyond each tape margin.

7.6 The joint material to be tested shall be applied to the prepared pipe specimen (using a spiral wrap for tapes) and starting from a point 101.6 mm (4.0 in.) below the upper end of the pipe section and ending at a point 304.8 mm (12.0 in.) from the upper end. The 203.2 mm (8.0 in.) of joint material thus applied should overlap the bared section of pipe by 50.8 mm (2.0 in.) at each end. This distance represents the typical cut-back distance encountered in the field joining, through welding, of coated pipe in 60.325 mm (2.375 in.) outside diameter size. A diagram of the joint specimen appears as **Fig. 2**.

7.7 The manner of applying the joint material shall be done in accordance with the manufacturer's specifications. The supplier of the joint material should specify the desired time interval between the application of the material and the start of the test.

NOTE 3—Materials that are intended for use as a field-applied patch over damaged areas on coated pipelines can be tested using the same procedures, with the patching compound applied, instead, to the bared area of the simulated joint.

7.8 The upper 76.2 mm (3.0 in.) of the completed joint test specimen shall be coated with the material used for the lower end cap. This moisture shield can be conveniently made, in the case of some waxes and epoxies, with several successive brush or dip-applied applications. The thickness of the moisture shield should be approximately 3.175 mm (0.125 in.).

8. Testing Temperature

8.1 Perform all tests at a room temperature of 21 to 25°C (70 to 77°F).

9. Preliminary Test Measurements

9.1 Coating and Joint Thickness—Measure and record the thickness of the base coating which lies exposed at each end of the test joint. Measurements shall be made in accordance with Test Method **G12**. In a like manner, measure and record the average thickness of the joint covering.

10. Procedure for Leakage Current Measurements

10.1 Suspend the joint test specimens in the test vessel, observing the clearances specified in **5.1.1** and **5.1.2**. Fill the vessel with electrolyte, bringing the fluid level up to a point midway between the end cap and the lower edge of the joint material.