



Designation: **D4049 – 16** **D4049 – 20**

Standard Test Method for Determining the Resistance of Lubricating Grease to Water Spray¹

This standard is issued under the fixed designation D4049; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reappraisal. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reappraisal.

1. Scope*

1.1 This test method² covers the ability of a grease to adhere to a metal surface when subjected to a water spray under prescribed laboratory conditions.

1.2 The values stated in SI units are to be regarded as standard.

1.2.1 *Exception*—The values given in parentheses are for information only.

1.3 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety, health, and environmental practices and determine the applicability of regulatory limitations prior to use.*

1.4 *This international standard was developed in accordance with internationally recognized principles on standardization established in the Decision on Principles for the Development of International Standards, Guides and Recommendations issued by the World Trade Organization Technical Barriers to Trade (TBT) Committee.*

2. Referenced Documents

- 2.1 *ASTM Standards:*³
- [D217 Test Methods for Cone Penetration of Lubricating Grease](#)
 - [D1742 Test Method for Oil Separation from Lubricating Grease During Storage](#)
 - [E691 Practice for Conducting an Interlaboratory Study to Determine the Precision of a Test Method](#)

3. Terminology

3.1 *Definitions:*

3.1.1 *lubricating grease, n*—a semi-fluid to solid product of a dispersion of a thickener in a liquid lubricant.

3.1.1.1 *Discussion*—

The dispersion of the thickener forms a two-phase system and immobilizes the liquid lubricant by surface tension and other physical forces. Other ingredients are commonly included to impart special properties. **D217**


¹ This test method is under the jurisdiction of ASTM Committee D02 on Petroleum Products, Liquid Fuels, and Lubricants and is the direct responsibility of Subcommittee D02.G0.06 on Functional Tests - Contamination.

Current edition approved Dec. 1, 2016; Nov. 1, 2020. Published January 2017; November 2020. Originally approved in 1981. Last previous edition approved in 2014 as D4049 – 06 (2011); D4049 – 16. DOI: 10.1520/D4049-16.10.1520/D4049-20.

² The development of this test method is described in Musilli, T. G., “Water Spray-Off Characteristics of Lubricating Grease,” *NLGI Spokesman*, December 1982, pp. 323–326.

³ For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard’s Document Summary page on the ASTM website.

*A Summary of Changes section appears at the end of this standard

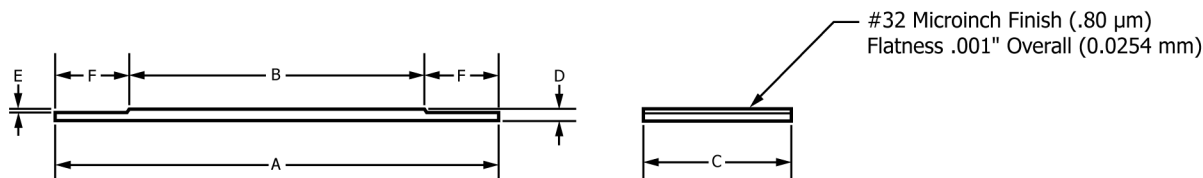

DIMENSIONS

	in.	mm
A Overall panel length	6.0	152.4
B Raised section length	4.0	101.6
C Width	2.000 - 0.002	50.8 - 0.05
D Thickness	$0\frac{3}{16} \pm 0.003$	4.76 ± 0.08
E Reduced section thickness	$\frac{1}{16}$	1.59
F Reduced section length	1.0	25.4

NOTE 1—All tolerances ± 0.03 mm unless otherwise specified.

FIG. 1 Stainless Steel Test Panel

3.1.2 *oil separation, n*—the appearance of a liquid fraction from an otherwise homogeneous lubricating composition. **D1742**

3.1.3 *thickener, n*—*in lubricating grease*, a substance composed of finely divided particles dispersed in a liquid lubricant to form the product's structure.

3.1.3.1 *Discussion*—

The thickeners can be fibers (such as various metallic soaps) or plates or spheres (such as certain non-soap thickeners), which are insoluble or, at most, only very slightly soluble in the liquid lubricant. The general requirements are that the solid particles be extremely small, uniformly dispersed, and capable of forming a relatively stable, gel-like structure with the liquid lubricant. **D217**

4. Summary of Test Method

4.1 The grease to be tested is coated on a stainless steel panel and sprayed with water at the specified test temperature and pressure. The amount of grease remaining on the panel after 5 min \pm 15 s is a measure of the resistance of the grease to water spray.

5. Significance and Use

5.1 This test method is used to evaluate the ability of a grease to adhere to a metal surface when subjected to direct water spray. The results obtained from the use of this test method suggest correlation in operations involving direct water spray impingement such as steel mill roll neck bearing service.⁴ This test method is used for quality control and purchase specifications.

6. Apparatus⁵

6.1 *Stainless Steel Test Panel*, 18-8 (chromium-nickel) stainless steel, as shown in Fig. 1.

6.1.1 *Grease Application Jig*, for applying grease to panel; Fig. 2.


6.2 *Water Spray Apparatus*, as shown in Fig. 3.

6.3 *Spray Nozzle*, as shown in Fig. 4.

6.4 *Thermometer or Thermocouple*—*Thermocouple*, capable of measuring 38 °C \pm 0.5 °C, to determine the temperature of the water spray, positioned to prevent breaking the spray pattern.

⁴ Cichelli, A. E. "Evaluation of Greases for Steel Mill Service," *NLGI Spokesman*, August 1973, and A. E. Cichelli, "Grease Lubrication in Steel Mills with Emphasis on Roll Neck Bearings," *NLGI Spokesman*, April 1980.

⁵ The sole source of supply of the apparatus known to the committee at this time is Koehler Instrument Co., Inc., 1595 Sycamore Ave., Bohemia, NY 11716. If you are aware of alternative suppliers, please provide this information to ASTM International Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee,¹ which you may attend.

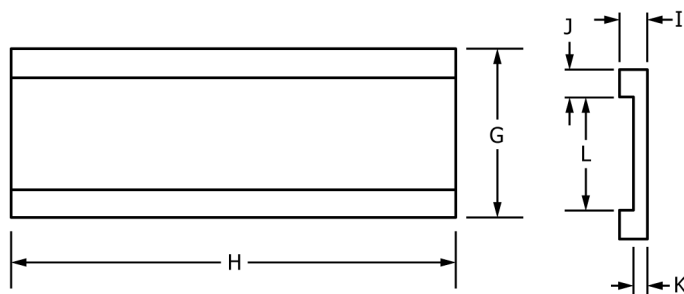

DIMENSIONS

	in.	mm
G Width	3.0	76.2
H Length	8.0	203.2
I Thickness	7/16	11.11
J Raised section width	1/2	12.7
K Reduced section thickness	7/32	5.54
L Reduced section width	2.001 + 0.003	50.83 + 0.5

NOTE 1—All tolerances ± 0.03 mm unless otherwise specified.

FIG. 2 Grease Application Jig

7. Reagents and Materials

7.1 *Purity of Reagents*—Reagent grade chemicals shall be used in all tests. Unless otherwise indicated, it is intended that all reagents shall conform to the specifications of the committee on Analytical Reagents of the American Chemical Society, where such specifications are available.⁶ Other grades may be used, provided it is first ascertained that the reagent is of sufficiently high purity to permit its use without lessening the accuracy of the determination.

7.2 *Mineral Spirits*, reagent grade, minimum purity. (**Warning**—Combustible. Vapor harmful.)

7.3 *n-Heptane*, reagent grade, minimum purity. (**Warning**—Flammable. Harmful if inhaled.)

8. Sampling

8.1 Each test will require a quantity sufficient to cover the steel panel (approximately 4 g to 12 g).

8.2 Supply a 25 g (minimum) representative sample.

8.3 Examine for any indication of nonhomogeneity, such as oil separation, phase changes, or gross contamination. If any abnormal conditions are found, obtain a new sample.

9. Preparation of Apparatus


9.1 Clean the test panel by brushing with mineral spirits. Then rinse with *n*-heptane and air dry. (**Warning**—See 7.2 and 7.3.)

9.2 Clean reservoir by flushing with water and wipe off any residual oil film from the surfaces of the reservoir and from the spray chamber area. Disassemble and clean the spray nozzle, taking care to properly position the vane in the cone body during assembly. This shall be done after each test.

NOTE 1—For proper vane orientation, see Fig. 4.

9.2.1 Visually inspect apparatus prior to each test to ensure cleanliness.

⁶ *Reagent Chemicals, American Chemical Society Specifications, ACS Reagent Chemicals, Specifications and Procedures for Reagents and Standard-Grade Reference Materials*, American Chemical Society, Washington, DC. For suggestions on the testing of reagents not listed by the American Chemical Society, see *Analar Standards for Laboratory Chemicals*, BDH Ltd., Poole, Dorset, U.K., and the *United States Pharmacopeia and National Formulary*, U.S. Pharmacopeial Convention, Inc. (USPC), Rockville, MD.

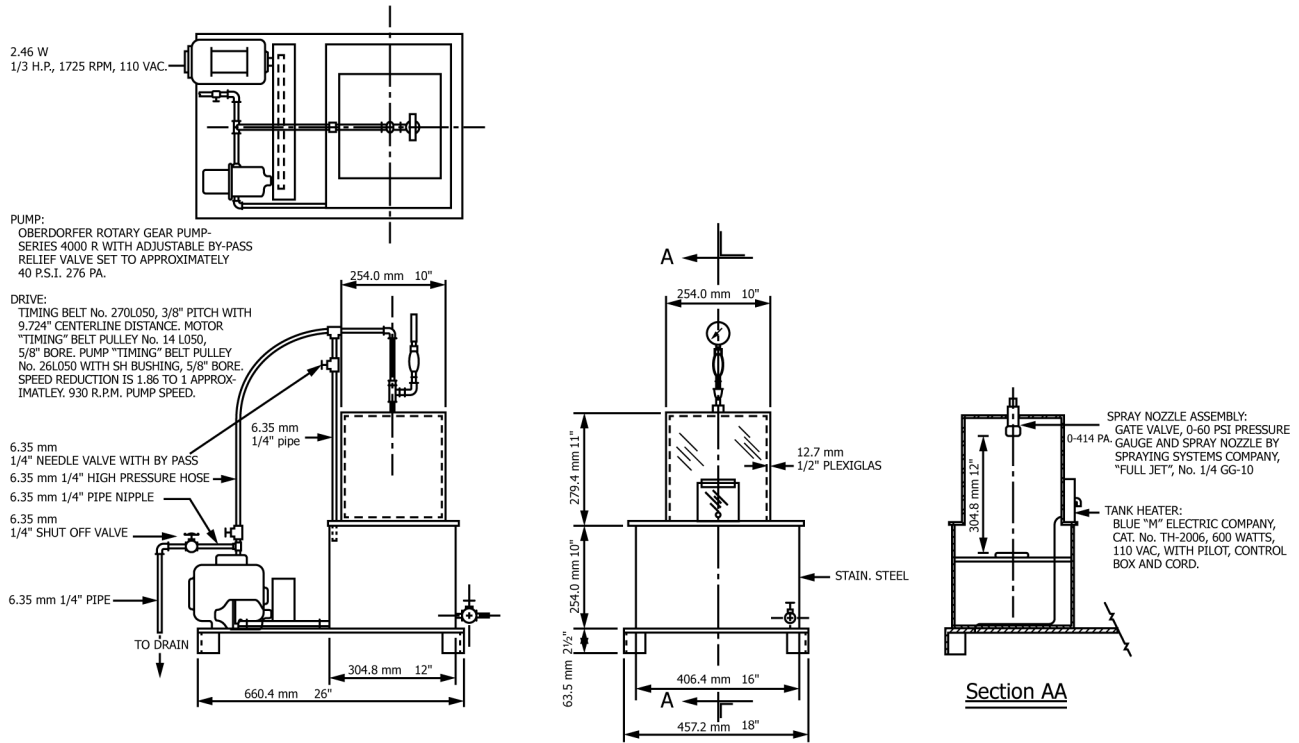

NOTE 1—The bypass valve shall be ahead of the gauge, not between the gauge and nozzle.

FIG. 3 Water Spray Apparatus

10. Procedure

10.1 Weigh a clean test panel to the nearest 0.1 g, and record as W_1 , and then, using the metal jig (as shown in Fig. 2), use a spatula to spread approximately a $0.8 \text{ mm} \pm 0.005 \text{ mm}$ ($1/32 \text{ in.}$) thick film of grease. Clean off any grease beyond the raised section of the panel. Reweigh and record as W_2 .

10.2 Add an adequate amount of tap water to the reservoir and to cover the heater and adjust the water temperature to $38 \text{ }^\circ\text{C} \pm 0.5 \text{ }^\circ\text{C}$ ($100 \text{ }^\circ\text{F} \pm 1 \text{ }^\circ\text{F}$). When the water temperature in the reservoir reaches $38 \text{ }^\circ\text{C} \pm 0.5 \text{ }^\circ\text{C}$ ($100 \text{ }^\circ\text{F} \pm 1 \text{ }^\circ\text{F}$), circulate 2 min to 3 min to attain temperature equilibrium before spraying the panel. Adjust pump pressure to $276 \text{ kPa} \pm 7 \text{ kPa}$ ($40 \text{ psi} \pm 1 \text{ psi}$) using the bypass valve. The bypass valve must be ahead of the gauge, not between the gauge and nozzle. Shut off the motor.

10.3 Insert the panel, making sure the panel is level and centered below the spray nozzle. Start the motor and spray the water on the panel for $5 \text{ min} \pm 15 \text{ s}$.

10.4 Shut off the motor to stop the spray, and remove the panel. Remove the excess grease outside the raised section of panel (area BC, Fig. 1) and along the sides and bottom of the panel. Place the panel in a horizontal position in an oven for $1 \text{ h} \pm 5 \text{ min}$ at $66 \text{ }^\circ\text{C} \pm 1 \text{ }^\circ\text{C}$ ($150 \text{ }^\circ\text{F} \pm 2 \text{ }^\circ\text{F}$).

10.5 Remove the panel from the oven, and allow to cool. Reweigh the panel, and record as W_3 .

11. Calculation

11.1 Calculate the percent spray-off as follows:

$$\% \text{ spray - off} = \left[\frac{(W_2 - W_3)}{(W_2 - W_1)} \right] (100) \quad (1)$$

where:

W_1 = initial mass of clean panel,