



Designation: **E1114—09 (Reapproved 2014) E1114 – 20**

Standard Test Method for Determining the Size of ~~Iridium-192~~ Iridium-192, Cobalt-60, and Selenium-75 Industrial Radiographic Sources¹

This standard is issued under the fixed designation E1114; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

1. Scope

1.1 This test method covers the determination of the size of ~~an Iridium-192 radiographic source.~~ Iridium-192, Cobalt-60, and Selenium-75 radiographic sources. The determination is based upon measurement of the image of the ~~Iridium metal~~ source in a projection radiograph of the source assembly and comparison to the measurement of the image of a reference sample in the same ~~radiograph.~~ radiograph or the source guide tube.

1.2 *Units*—The values stated in either SI units or inch-pound units are to be regarded separately as standard. The values stated in each system ~~may~~ are not ~~be~~ necessarily exact equivalents; therefore, to ensure conformance with the standard, each system shall be used independently of the other. ~~Combining~~ other, and values from the two systems ~~may result in non-conformance with the standard.~~ shall not be combined.

1.3 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety, health, and ~~health~~ environmental practices and determine the applicability of regulatory limitations prior to use.*

1.4 *This international standard was developed in accordance with internationally recognized principles on standardization established in the Decision on Principles for the Development of International Standards, Guides and Recommendations issued by the World Trade Organization Technical Barriers to Trade (TBT) Committee.*

2. Referenced Documents

2.1 ASTM Standards:²

- E999 Guide for Controlling the Quality of Industrial Radiographic Film Processing
- E1316 Terminology for Nondestructive Examinations
- E1815 Test Method for Classification of Film Systems for Industrial Radiography
- E2445 Practice for Performance Evaluation and Long-Term Stability of Computed Radiography Systems
- E2597 Practice for Manufacturing Characterization of Digital Detector Arrays

¹ This test method is under the jurisdiction of ASTM Committee E07 on Nondestructive Testing and is the direct responsibility of Subcommittee E07.01 on Radiology (X and Gamma) Method.

Current edition approved Oct. 1, 2014 Dec. 1, 2020. Published November 2014 February 2021. Originally approved in 1986. Last previous edition approved in 2009 2014 as E1114 – 09¹-(2014). DOI: 10.1520/E1114-09R14-10.1520/E1114-20.

² For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

[E2002 Practice for Determining Total Image Unsharpness and Basic Spatial Resolution in Radiography and Radioscopy](#)

2.2 *Other International Standards:*

[EN 12679:2000](#) [EN 12679:2018](#) [Industrial Radiography—Radiographic Method for the Determination of the Source Size for Radioisotopes](#)³

3. Terminology

3.1 For definitions of terms relating to this test method, refer to Terminology [E1316](#).

4. Significance and Use

4.1 One of the factors affecting the quality of a radiographic image is geometric unsharpness. The degree of geometric unsharpness is dependent upon the size of the source, the distance between the source and the object to be radiographed, and the distance between the object to be radiographed and the film or digital detector. This test method allows the user to determine the size of the source and to use this result to establish source to object and object to film or detector distances appropriate for maintaining the desired degree of geometric unsharpness.

NOTE 1—The European standard CEN EN 12579 describes a simplified procedure for measurement of source sizes of Ir-192, ~~Co-60~~ [Co-60](#), and Se-75. The resulting source size of Ir-192 is comparable to the results obtained by this test method.

5. Apparatus

5.1 *Subject Iridium-192 Source, Subjects are Iridium-192, Cobalt-60, and Selenium-75 Sources* where the source size of which is sizes are to be determined. The appropriate apparatus and equipment for the safe storage, handling, and manipulation of the subject source, such as a radiographic exposure device (also referred to as a gamma ray projector or gamma camera), remote control, source guide tube, and source stop are also required.

5.2 *Reference Sample (see Figs. 1-3)*—The reference sample for film radiography shall be of material which is not radioactive. The recommended material is ~~Iridium~~ Iridium, Cobalt (also steel), or Selenium (also SeO_2), respectively. However, substitutes such as platinum, tungsten, or other material of similar radiopacity may be used. The sample should be of the same geometric shape as the subject source, should be approximately the same size as the subject source, and should be positioned on or within a shim or envelope to simulate the source capsule wall. The resulting radiographic contrast, with reference to adjacent background density of the image of the reference sample, should be approximately the same as that of the subject source. The actual dimensions of the reference sample should be determined to the nearest 0.025 mm (0.001 in.). If digital radiography and image processing is applied with imaging plates or DDAs, the source guide can be used as reference sample for dimensional measurement.

5.3 *X-ray Generator*, capable of producing a radiation intensity (roentgen per hour at one ~~metre~~ metre / 39 in.) at least ten times greater than that produced by the subject source. Examples of typical X-ray generator output requirements that satisfy this criterion are presented in [Table 1](#).

5.4 *Film systems—Systems*—Only film systems having cognizant engineering organization approval or meeting the system class requirements of Test Method [E1815](#), for system classes I, II, or Special, shall be used. Selection of film systems should be determined by such factors as the required radiographic quality level, equipment capability, materials, and so forth. The film system selected shall be capable of demonstrating the required image quality. No intensifying screens shall be used. ~~Radiographic~~ Radiographic films shall be processed in accordance with Guide [E999](#).

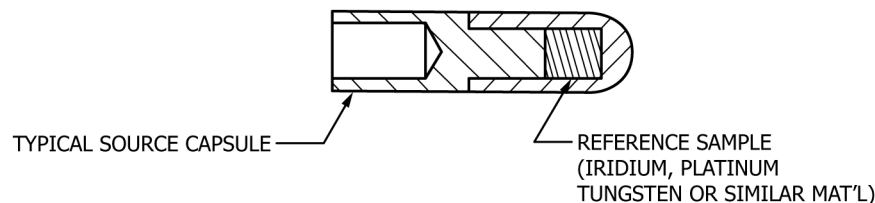


FIG. 1 Reference Sample in Standard Source Encapsulation

³ Available from American National Standards Institute (ANSI), 25 W. 43rd St., 4th Floor, New York, NY 10036, <http://www.ansi.org>.

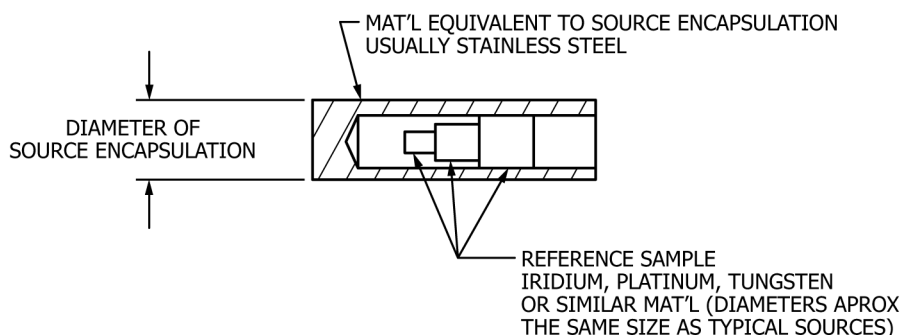


FIG. 2 Alternate Reference Sample Arrangement

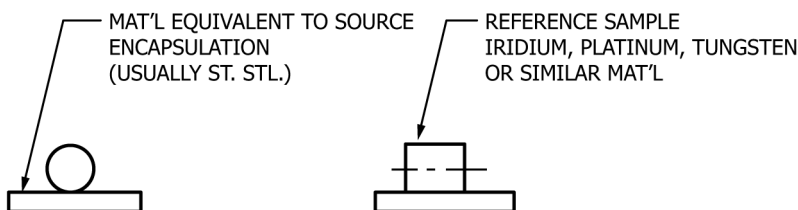


FIG. 3 Alternate Reference Sample Arrangement

TABLE 1 Examples of Typical X-ray Generator Output Requirements for Related Iridium¹⁹² Source Activities

Subject Iridium ¹⁹² Source Radiation		Typical X-ray Generator Output Requirements	
Activity (Curie)	Output (R/h at 1 m)	Potential	Current
30	14.4	160 kV	5 mA
		200 kV	3 mA
100	48.0	160 kV	10 mA
		250 kV	4 mA
200	96.0	160 kV	20 mA
		250 kV	8 mA
		300 kV	6 mA

<https://standards.iteh.ai/catalog/standards/sist/42308df2-43d5-4aac-a1d9-4da483184a23/astm-e1114-20>

5.5 *Image Measurement Apparatus*—This apparatus is used to measure the size of the image of the spot. The apparatus shall be an optical comparator with built-in graticule with 0.1 (see 8.2 mm divisions or 0.001 in. divisions and magnification of 5× to 10× for requirements).

5.6 *Digital Detectors*—Digital detectors, which are either imaging plates or digital detector arrays, may be used as film replacement. The digital detector shall possess a pixel pitch which is at least 40 times smaller than the nominal source size to measure and a basic spatial resolution smaller than 1/20 of the nominal source size. The basic spatial resolution of the detector shall be measured in accordance with Practice E2002 (see an example in 9.2), the procedure of Practice E2597 for DDAs or Practice E2445 for the imaging plate scanner systems or taken from manufacturer statements. In the area of free beam a detector SNR_D > 100 shall be achieved. The measurement procedure of the SNR shall be in accordance with the procedure of Practice E2597 for DDAs or Practice E2445 for the imaging plate scanner system.

5.7 *Evaluation of Digital Images*—Digital images shall be evaluated by an image processing software with contrast, brightness, profile and zoom function. The digital images shall be magnified at the monitor to a degree that allows the image viewing with at least one pixel of the image at one pixel of the monitor.

6. Procedure

6.1 Set up the exposure arrangement as shown in Figs. 4-7. Position the X-ray tube directly over the center of the film or digital detector. The film or detector plane must be normal to the central ray of the X-ray beam. The X-ray spot should be 0.90 m (36

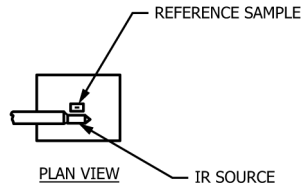
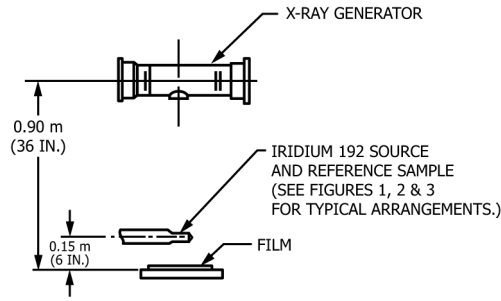


FIG. 4 Typical Exposure Arrangement

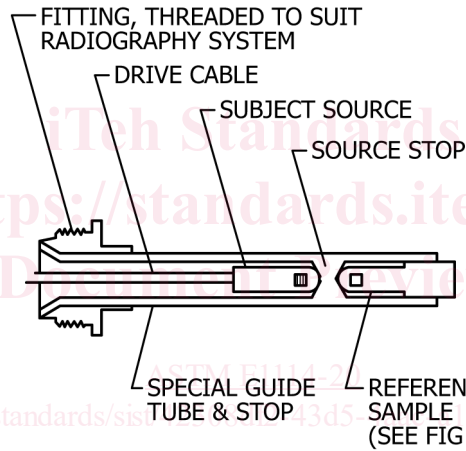


FIG. 5 Typical Arrangement Using a Specially Designed Guide Tube

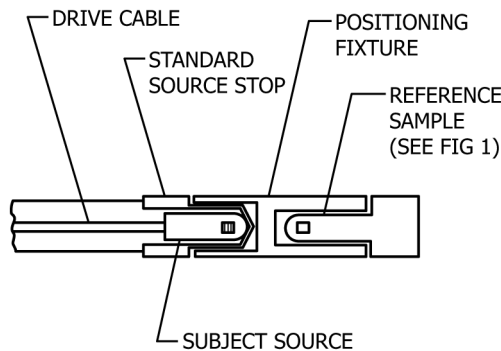


FIG. 6 Typical Arrangement Using a Standard Guide Tube and Special Positioning Fixture

in.) from the film or detector. Position the reference sample and apparatus used to locate the subject source (source stop) as close together as possible and directly over the center of the film or detector. The plane of the source stop and reference sample must be parallel to the film or detector and normal to the central ray of the X-ray beam. The source stop and reference sample should be 0.15 m (6 in.) from the film or detector. The source stop should be connected to the radiographic exposure device by the shortest source guide tube practicable in order to minimize fogging of the film or detector during source transit.

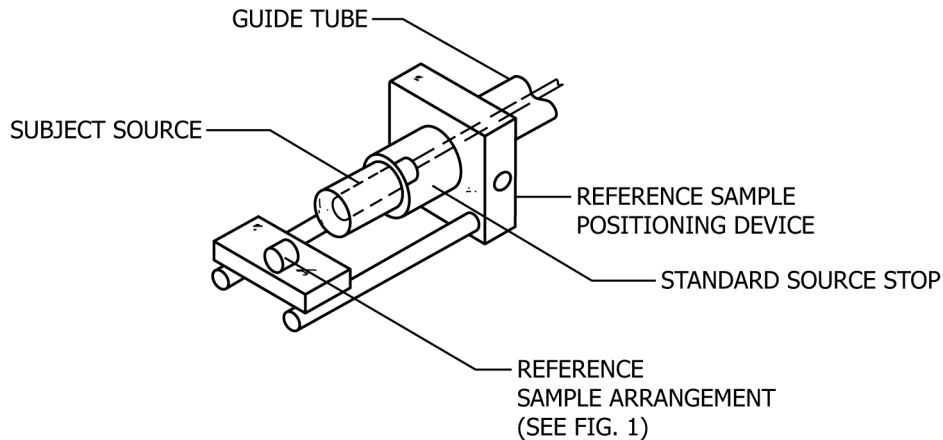


FIG. 7 Typical Arrangement Using Reference Sample Positioning Device

6.2 Place identification markers to be imaged on the film or detector to identify, as a minimum, the identification (serial number) of the subject source, the size of the reference sample, the identification of the organization performing the determination, and the date of the determination. Care should be taken to ensure that the images of the subject source and reference sample will not be superimposed on the image of the identification markers.

6.3 *Exposure*—Select the X-ray tube potential (kV), X-ray tube current (mA), and exposure time such that the density in the image of the envelope surrounding the reference sample does not exceed 3.0 and that the density difference between the image of the reference sample and the image of the envelope surrounding the reference sample is at least 0.10. In digital images, the linear greypixel value difference between the image of the reference sample and the image of the envelope surrounding the reference sample shall be five at least ten times larger than the image noise σ (σ = standard deviation) of the greypixel value fluctuations in an area of homogeneous exposure, measured in a window of at least 20 by 55 pixels in a homogeneous neighborhood area.

NOTE 2—The actual parameters that will produce acceptable results may vary between X-ray units, and trial exposures may be necessary.

6.3.1 Energize the X-ray generator and, at the same time, manipulate the subject source into the exposure position in the source stop. It is important that this be performed as quickly as possible to minimize fogging of the film or detector.

6.3.2 At the conclusion of the exposure time, deenergize the X-ray generator and, at the same time, return the subject source to the proper shielded storage position.

6.3.3 Process the film or read out the digital detector array or scan the imaging plate.

7. Measurement of Source Dimensions

7.1 The source size for a given technique is the maximum projected dimension of the source in the plane perpendicular to a line drawn from the source to the object being radiographed. Therefore, sufficient measurements of the image of the sources must be made to determine the size of the source in any orientation. Subsections 7.2 – 7.5 serve as examples.

7.2 *Uniform Right Circular Cylinder* (see Fig. 8)—Determine the source size of a uniform right circular cylindrical source by measuring the diameter, d , the height, h , and the diagonal, m , as illustrated in Fig. 8 and computing the actual dimensions as described in 8.1. Fig. 8 shows a stack of disks, which is typically used for Ir-192 sources.

7.3 *Sphere* (see Fig. 9)—Determine the size of a spherical source by measuring the diameter, d , as illustrated in Fig. 9 and computing the actual dimension as described in 8.1.

7.4 *Nonuniform Stack of Right Circular Cylinders* (see Fig. 10)—Determine the size of a nonuniform stack of right circular




FIG. 8 Uniform Right Circular Cylinder




FIG. 9 Sphere

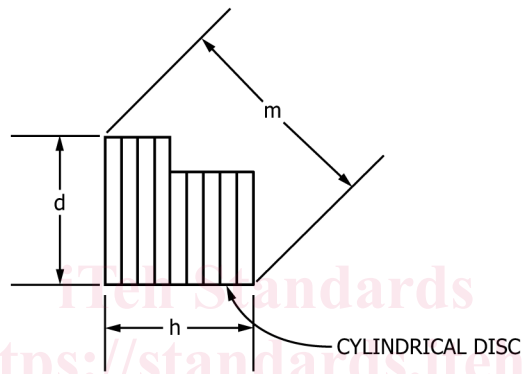


FIG. 10 Nonuniform Cylindrical Stack

cylindrical components of a source by measuring the intrinsic diameter, d , the height, h , and the effective maximum dimension, m , as illustrated in Fig. 10 and computing the actual dimensions as described in 8.1.

7.5 *Separated Stack of Right Circular Cylinders* (see Fig. 11)—Determine the size of a separated stack of right circular cylindrical components of a source by measuring the intrinsic diameter, d , the effective height, h , and the effective maximum dimension, m , as illustrated in Fig. 11 and computing the actual dimensions as described in 8.1.

8. Measurement of Source Dimensions and Evaluation with Film

8.1 When viewing the film radiograph, radiograph, view it with sufficient light intensity for adequate viewing. Using an optical comparator with built-in graticule as described in 5.5, measure the linear dimensions of the image of the spot size of the subject source and the reference sample. Take measurements from the perceptible edges of the image. When performing the physical measurements with the optical comparator, the actual measured values shall be to the nearest graduation on the graticule scale being used.

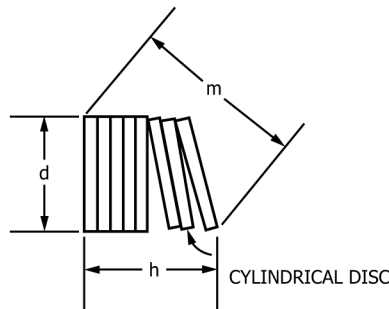


FIG. 11 Separated Cylindrical Stack

7.2 When viewing the digital image, view it in a darkened room and use a bright monitor with at least 250 cd/m². Use the profile function of the image processing software for size measurement in digital images after proper brightness and contrast adjustment.

8.2 The source size for a given technique is the maximum projected dimension of the source in the plane perpendicular to a line drawn film radiograph shall be examined visually on a film illuminator using a magnifying lens with a built-in measurement scale (graticule) with divisions of ≤ 0.1 mm (0.004 in.) for source sizes ≥ 1 mm (0.04 in.) or of ≤ 0.05 mm (0.002 in.) for source sizes < 1 mm (0.04 in.) and an optical magnification between 5 and 10. The magnifying factor, *v*, according to Fig. 4 from the source to the object being radiographed. Therefore, sufficient measurements of the shall be taken into account for calculation of the actual dimension, *d*, from the measured values at film or digitized film. The image of the Iridium must be made to determine the size of the source in any orientation. Sections radiation source shall have sufficient contrast 7.4–7.7 serve as examples: sensitivity to be easily measured.

7.4 *Uniform Right Circular Cylinder* (see Fig. 8) Determine the source size of a uniform right circular cylindrical source by measuring the diameter, *d*, the height, *h*, and the diagonal, *m*, as illustrated in Fig. 8 and computing the actual dimensions as described in 8.1.

7.5 *Sphere* (see Fig. 9) Determine the size of a spherical source by measuring the diameter, *d*, as illustrated in Fig. 9 and computing the actual dimension as described in 8.1.

7.6 *Nonuniform Stack of Right Circular Cylinders* (see Fig. 10) Determine the size of a nonuniform stack of right circular cylindrical components of a source by measuring the intrinsic diameter, *d*, the height, *h*, and the effective maximum dimension, *m*, as illustrated in Fig. 10 and computing the actual dimensions as described in 8.1.

7.7 *Separated Stack of Right Circular Cylinders* (see Fig. 11) Determine the size of a separated stack of right circular cylindrical components of a source by measuring the intrinsic diameter, *d*, the effective height, *h*, and the effective maximum dimension, *m*, as illustrated in Fig. 11 and computing the actual dimensions as described in 8.1.

9. Measurement and Evaluation with Digital Detectors

ASTM E1114-20

9.1 Digital images shall be evaluated by an image processing software with contrast, brightness (window levelling), profile, pixel size calibration, and zoom function. The digital images shall be magnified at the monitor to a degree that allows the image viewing with at least one pixel of the image at one pixel of the monitor.

9.2 Digital images show the gamma source with a certain magnifying factor. It shall be normalized by the magnifying factor for measurement of the source size. The measurement shall consider a known dimension as, for example, the diameter of a reference object (for example, a steel or tungsten cylinder) or the known sample guide tube diameter to determine the overall magnifying factor and the real dimensions of the source (see Section 10). The measurement of the source size shall be performed with a profile function as shown in Fig. 12 to achieve sufficient accuracy.

10. Calculation and Evaluation

10.1 Measure the linear dimension of interest in the subject source image and measure the same linear dimension in the reference sample image (that is, the diameter of each). The actual dimension of the subject source is computed/calculated from the following:

$$a = bc/d$$

$$a = bc/d$$

where:

- a* = actual dimension of the subject source,
- b* = actual dimension of the reference sample,
- c* = measured dimension of the subject source image, and
- d* = measured dimension of the reference sample image.