



Designation: ~~D7110~~–~~20~~ D7110 – 21

Standard Test Method for Determining the Viscosity-Temperature Relationship of Used and Soot-Containing Engine Oils at Low Temperatures¹

This standard is issued under the fixed designation D7110; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reappraisal. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reappraisal.

1. Scope*

1.1 This test method covers how to measure the apparent viscosity of used and soot-containing engine oils at low temperatures.

1.2 A shear rate of approximately 0.2 s^{-1} is produced at shear stresses below 200 Pa. Apparent viscosity is measured continuously as the sample is cooled at a rate of $3 \text{ }^\circ\text{C}$ per hour over the range of $-5 \text{ }^\circ\text{C}$ to $-40 \text{ }^\circ\text{C}$.

1.3 The measurements resulting from this test method are viscosity, the maximum rate of viscosity increase (Gelation Index) and the temperature at which the Gelation Index occurs.

1.4 Applicability to petroleum products other than engine oils has not been determined in preparing this test method.

1.5 The values stated in SI units are to be regarded as standard. No other units of measurement are included in this standard.

1.6 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety, health, and environmental practices and determine the applicability of regulatory limitations prior to use.*

1.7 *This international standard was developed in accordance with internationally recognized principles on standardization established in the Decision on Principles for the Development of International Standards, Guides and Recommendations issued by the World Trade Organization Technical Barriers to Trade (TBT) Committee.*

2. Referenced Documents

2.1 ASTM Standards:²

[D341 Practice for Viscosity-Temperature Equations and Charts for Liquid Petroleum or Hydrocarbon Products](#)

[D3829 Test Method for Predicting the Borderline Pumping Temperature of Engine Oil](#)

[D4684 Test Method for Determination of Yield Stress and Apparent Viscosity of Engine Oils at Low Temperature](#)

[D4057 Practice for Manual Sampling of Petroleum and Petroleum Products](#)

[D5133 Test Method for Low Temperature, Low Shear Rate, Viscosity/Temperature Dependence of Lubricating Oils Using a Temperature-Scanning Technique](#)

[D6299 Practice for Applying Statistical Quality Assurance and Control Charting Techniques to Evaluate Analytical Measurement System Performance](#)

¹ This test method is under the jurisdiction of ASTM Committee D02 on Petroleum Products, Liquid Fuels, and Lubricants and is the direct responsibility of Subcommittee D02.07 on Flow Properties.

Current edition approved June 1, 2020/Jan. 1, 2021. Published June 2020/February 2021. Originally approved in 2005. Last previous edition approved in 2015/2020 as ~~D7110 – 15~~-D7110 – 20. DOI: ~~10.1520/D7110-20-10.1520/D7110-21~~.

² For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

*A Summary of Changes section appears at the end of this standard

3. Terminology

3.1 Definitions:

3.1.1 *apparent viscosity, n*—the viscosity obtained by use of this test method.

3.1.1.1 Discussion—

See 3.1.7 for definition of viscosity and units.

3.1.2 *digital contact thermometer (DCT), n*—an electronic device consisting of a digital display and associated temperature sensing probe.

3.1.2.1 Discussion—

This device consists of a temperature sensor connected to a measuring instrument; this instrument measures the temperature-dependent quantity of the sensor, computes the temperature from the measured quantity, and provides a digital output, or display of the temperature, or both. This device is sometimes referred to as a digital thermometer. This digital output goes to a digital thermometer display and/or recording device that may be internal or external to the device.

3.1.2.2 Discussion—

The devices are often referred to as a “digital thermometers,” however the term includes devices that sense temperature by means other than being in physical contact with the media.

3.1.2.3 Discussion—

PET is an acronym for portable electronic thermometers, a subset of digital contact thermometers (DCT).

3.1.3 *Newtonian oil, n*—an oil or fluid that at a given temperature exhibits a constant viscosity at all shear rates or shear stresses.

3.1.4 *non-Newtonian oil, n*—an oil or fluid that at a given temperature exhibits a viscosity that varies with changing shear stress or shear rate.

3.1.5 *shear rate, n*—velocity gradient perpendicular to the direction of flow.

3.1.5.1 Discussion—

The SI unit for shear rate is the reciprocal second (1/s; also s⁻¹).

3.1.6 *shear stress, n*—force per unit area in the direction of flow.

3.1.6.1 Discussion—

The SI unit for shear stress is the pascal (Pa).

3.1.7 *viscosity, n*—the ratio between the applied shear stress and rate of shear which is sometimes called the coefficient of dynamic viscosity and is a measure of the resistance to flow of the liquid.

3.1.7.1 Discussion—

Mathematically expressed:

$$\text{viscosity} = \text{shear stress/shear rate or, symbolically, } \eta = \tau/\dot{\gamma} \quad (1)$$

in which the symbols in the second portion of Eq 1 are defined by 3.1.5 and 3.1.6. The SI unit for viscosity used herein is millipascal seconds (mPa·s).

3.2 Definitions of Terms Specific to This Standard:

3.2.1 *air-binding oils, n*—those engine oils whose borderline pumping temperatures are determined by a combination of gelation and viscous flow.

3.2.2 *borderline pumping temperature, n*—that temperature at which an engine oil may have such poor flow characteristics that the engine oil pump may not be capable of supplying sufficient lubricant to the engine.

3.2.3 *calibration oil, n*—Newtonian oils developed and used to calibrate the viscometer drive module over the viscosity range required for this test method.

3.2.3.1 Discussion—

These calibration oils are specially blended to give sufficient sensitivity and range for the special viscometer head used.

3.2.4 *computer-programmed automated analysis, n*—use of techniques for acquiring analog data, converting these to digital values and using this information to automatically record and analyze torque output from the viscometer drive module and to render this information into tabular data and plotted relationships.

3.2.4.1 *analog-to-digital (A-D) converter, n*—a device for converting continuously produced electrical signals into discrete numerical values capable of being analyzed by computer technology.

3.2.5 *critical pumpability temperature, n*—the temperature at which an oil reaches a viscosity believed to be critical to limiting pumpability of the oil (see 3.2.6).

3.2.6 *critical pumpability viscosity, n*—that apparent viscosity believed to cause pumpability problems in an engine.

3.2.7 *flow-limited oils, n*—those oils whose borderline pumping temperatures are determined by viscous flow.

3.2.8 *gelation, n*—a rheological condition of an oil characterized by a marked increase in flow resistance over and above the normal exponential increase of viscosity with decreasing temperature, particularly at lower shear stresses and temperatures.

3.2.8.1 *Discussion*—

Gelation has been attributed to a process of nucleation and crystallization of oil components and the consequent formation of a gel-like mass.³

3.2.9 *Gelation Index, n*—the maximum value of the incremental ratio:

$$-\frac{[(\log \log \eta_1) - (\log \log \eta_2)]}{(\log T_1 - \log T_2)} \quad (2)$$

in which η is dynamic viscosity and T is temperature in Kelvin over the temperature range scanned when the incremental decrease in temperature is 1 K.

3.2.9.1 *Discussion*—

The technique of deriving Gelation Index was first developed and practiced⁴ by collecting information from a strip-chart recording and applying the empirical MacCoull-Walther-Wright equation. For further information, see Appendix 1 of Viscosity-Temperature Charts **D341**.

3.2.10 *Gelation Index reference oils, n*—non-Newtonian oils chosen to give certain levels of Gelation Index as a check on instrument performance.

<https://standards.iteh.ai/catalog/standards/sist/43a452c8-f953-4c2b-ace5-26d6556c4758/astm-d7110-21>

3.2.11 *Gelation Index Temperature, n*—the temperature in degrees Celsius at which the Gelation Index occurs.

3.2.12 ~~*pre-treatment sample heating bath, n*—a water or air bath to heat the samples for 1.5 h at 90 °C ± 2 °C before testing.~~

3.2.12 ~~*programmable liquid-cold-cooling bath, n*—a liquid or dry block (referred to as direct cool) bath having a temperature controller capable of being programmed to run the calibration and the analysis portions of the test method.~~ method within the temperature tolerances listed.

3.2.13 ~~*sample preheater, n*—a water bath, air bath or oven, or dry bath (integrated or separate) to heat the samples for 1.5 h at 90 °C ± 2 °C before testing.~~

3.2.14 *temperature controller, n*—a programmable device which, when properly programmed, ramps the temperature upward or downward at a chosen rate or series of steps while simultaneously controlling temperature excursions.

3.2.14.1 *calibration program, n*—a program to run the required series of temperatures at which the torque values necessary to calibrate the viscometer drive module are collected and analyzed.

3.2.14.2 *test program, n*—a program to run the test oil analysis at 3 °C/h temperature decrease.

3.2.14.3 *hold program, n*—a program to reach and hold the programmable ~~liquid-cold-cooling~~ bath at -5 °C.

³ *Symposium on Low Temperature Lubricant Rheology Measurement and Relevance to Engine Operation*, ASTM STP 1143, Ed. Robert B. Rhodes, ASTM, 1992.

⁴ Selby, T. W., "The Use of the Scanning Brookfield Technique to Study the Critical Degree of Gelation of Lubricants at Low Temperatures," SAE Paper 910746, Society of Automotive Engineers, 1991.

3.2.15 *test cell, n*—the combination of the rotor and stator. Critical elements of the test cell are sketched in Fig. 1.

3.2.15.1 *rotor, n*—a titanium rotor sized to give a compromise of sensitivity and range to the determination of viscosity and gelation using this test method.

3.2.15.2 *stator, n*—a precision-bore borosilicate glass tube, to which a measured amount of oil is added for the test and within which the specially-made rotor turns.

3.2.15.2.1 *stator collar, n*—a clamp for the stator which also positions it on the test cell alignment device.

3.2.15.3 *test cell alignment device, n*—a special device used to support the viscometer drive module while maintaining the stator and the rotor coaxial and vertical in regard to the viscometer driveshaft. Later designs admit dry gas into the cell to prevent moisture and frost buildup.

3.2.16 *test oil, n*—any oil for which apparent viscosity is to be determined using the procedure described by this test method.

3.2.17 *viscometer drive module, n*—the rotor drive and torque-sensing component of a rotational viscometer.

3.2.18 *viscometer module support, n*—a part of the test cell alignment device supporting the viscometer drive module.

4. Summary of Test Method

4.1 Used and sooted engine oils are analyzed using a special rotational viscometer with analog or digital output to a computer program. A specially made metal or glass stator/metal rotor cell is attached to the viscometer and subjected to a programmed temperature change for both calibration and sample analysis. Following calibration of the rotor-stator set, an approximately 20 mL test sample of a test lubricating oil is poured into the stator and preheated for 1.5 h to 2.0 h at 90 °C in an oven or water bath, a sample preheater. Shortly after completing the preheating step, the room-temperature rotor is put into the stator containing the heated oil and coupled to a torque-sensing viscometer head using an adapter to automatically center the rotor in the stator during test. A programmable low-temperature cooling bath is used to cool the cell at a specified rate of 3 °C/h from -5 °C to the

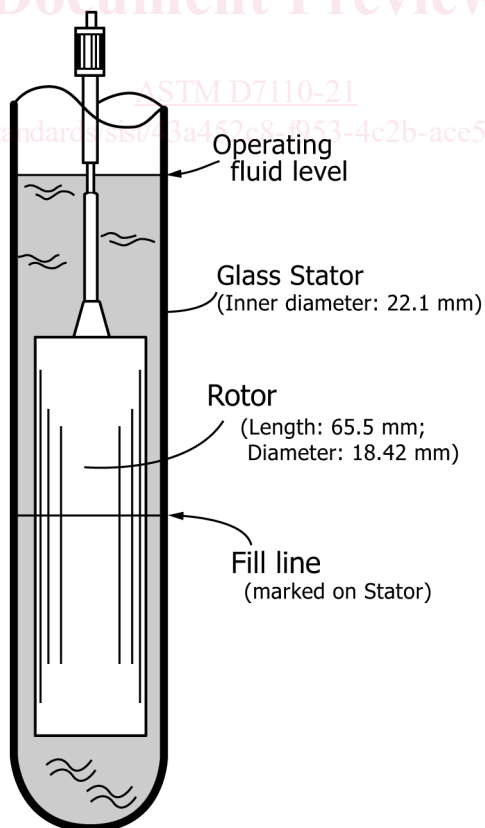


FIG. 1 Test Cell

temperature at which the maximum torque recordable is exceeded when using a speed of 0.3 r/min for the rotor. After the desired information has been collected, the computer program generates the desired viscometric and rheological values from the recorded data.

5. Significance and Use

5.1 Significance of Low Temperature, Low Shear Rate, Engine Oil Rheology—The low-temperature, low-shear viscometric behavior of an engine oil, whether new, used, or sooted, determines whether the oil will flow to the sump inlet screen, then to the oil pump, then to the sites in the engine requiring lubrication in sufficient quantity to prevent engine damage immediately or ultimately after cold temperature starting. Two forms of flow problems have been identified,³ flow-limited and air-binding behavior. The first form of flow restriction, flow-limited behavior, is associated with the oil's viscosity; the second, air-binding behavior, is associated with gelation.

5.2 Significance of the Test Method—The temperature-scanning technique employed by this test method was designed to determine the susceptibility of the engine oil to flow-limited and air-binding response to slow cooling conditions by providing continuous information on the rheological condition of the oil over the temperature range of use.^{3,4,5} In this way, both viscometric and gelation response are obtained in one test.

NOTE 1—This test method is one of three related to pumpability related problems. Measurement of low-temperature viscosity by the two other pumpability test methods, **D3829** and **D4684**, hold the sample in a quiescent state and generate the apparent viscosity of the sample at shear rates ranging up to 15 s⁻¹ and shear stresses up to 525 Pa at a previously selected temperature. Such difference in test parameters (shear rate, shear stress, sample motion, temperature scanning, and so forth) can lead to differences in the measured apparent viscosity among these methods with some test oils, particularly when other rheological factors associated with gelation are present. In addition, the three methods differ considerably in cooling rates.

5.3 Gelation Index and Gelation Index Temperature—This test method has been further developed to yield parameters called the Gelation Index and Gelation Index Temperature. The first parameter is a measure of the maximum rate of torque increase caused by the rheological response of the oil as the oil is cooled slowly. The second parameter is the temperature at which the Gelation Index occurs.

6. Apparatus

6.1 Test Cell—Shown in **Fig. 1**, consisting of a matched rotor and a stator of the following critical dimensions:

6.1.1 Rotor Dimensions—Critical length is 65.5 mm ± 0.1 mm and critical diameter is 18.40 mm ± 0.02 mm.

6.1.2 Stator Dimensions—Critical diameter is 22.05 mm (±0.02 mm) at whatever length will satisfy the immersion depth when the upper oil level is a minimum of 15 mm below the cooling liquid level over the entire temperature range.

6.2 Viscometer Drive Modules—Rotational viscometer drive modules capable of producing an analog signal to an analog-to-digital converter or other analog signal data processor such as a strip-chart recorder.

6.2.1 With the rotor and stator described in **6.1.1** and **6.1.2**, the viscometer drive module must be capable of measuring to at least 90 000 mPa·s (cP).

6.3 Test Cell Alignment Device—Simultaneously maintains a vertical axial alignment and reasonably consistent positioning of the rotor in the stator to give repeatable torque readout from test to test when setting up the apparatus for analysis.

6.3.1 Viscometer Support—Supports the viscometer drive module and aligns it vertically.

6.3.2 Stator Collar—Clamps the stator and supports it when the stator collar is attached to the viscometer support.

6.4 A means of providing a dry gas atmosphere over the top of the test sample is necessary to prevent condensation and freezing of water on the oil surface.

⁵ Shaub, H., "A History of ASTM Accomplishments in Low Temperature Engine Oil Rheology," *Symposium on Low Temperature Lubricant Rheology Measurement and Relevance to Engine Operation, ASTM STP 1143*, Rhodes, R. B., ed., ASTM, 1992, pp. 1-19.

6.5 ~~Programmable Liquid Cooling or Scanning Brookfield Technique (SBT) Direct Cool Bath—Liquid bath capable~~ Capable of running either the calibration or the testing program with temperature control of ± 0.1 °C over the temperature range desired at 3 °C/h.

6.5.1 *Temperature Controller* is set up to operate according to two programs, the calibration program and the test program. At any temperature the controller modulates temperature within 0.1 °C of the desired value.

6.6 *Computer, Analog-to-Digital Converter, and Analysis Program*—Means of receiving data from the viscometer drive module and converting this data into the desired information.

6.7 ~~Sample Pre-treatment Water or Air Bath—Preheater—A programmable water or air bath for both bath, air bath or oven, or dry bath (integrated or separate) for precise control of the test oils at 90 °C \pm 2 °C and during immersion time after the sample reaches pre-treatment temperature. SBT Direct Cool bath can also perform the preheating portion of the test.~~

6.8 ~~Calibrated Liquid-in-Glass or Digital Contact Thermometer, Thermometer—calibrated at 90 °C and reading to ± 0.2 °C.~~ Calibrated liquid-in-glass or digital contact thermometer meeting the following requirements:

6.8.1 *Calibrated Liquid-in-Glass Thermometer*—One calibrated at 90 °C and reading to ± 0.2 °C and another calibrated at -20 °C reading to ± 0.1 °C.

6.8.2 *Digital Contact Thermometer*—A DCT meeting the criteria of [Table 1](#).

7. Materials

7.1 *Calibration Oil*—A Newtonian calibration oil of known dynamic viscosity over a temperature range of -5 °C to -35 °C.

7.2 *Gelation Index Reference Oils, GIR-series, non-Newtonian Reference Oils*, having gelation indices of established values as well as related values for the gelation index temperatures.

ASTM D7110-21

<https://standards.iteh.org/standard/ASTM-D7110-21> **TABLE 1 Digital Contact Thermometer Criteria for the Independent Temperature Indicator** [astm-d7110-21](https://standards.iteh.org/standard/ASTM-D7110-21)

Parameter	Liquid Baths	Dry Baths
Nominal temperature range ^A	-40 °C to 0 °C	
Display resolution, minimum	0.1 °C	
Accuracy, ^B minimum	-40 °C to 0 °C: ± 100 mK (± 0.1 °C)	
Sensor type	PRT	
Immersion depth ^C	114 mm (4.50 in.) minimum by Practice D7962	89 mm (3.50 in.) minimum by Practice D7962
Measurement drift ^D	less than 100 mK (0.1 °C) per year	
Response time ^E	12 s	
Sensor sheath, ^F max diameter	4.77 mm (0.188 in.)	3.18 mm (0.125 in.)
Sensor length, ^G max	25 mm (1.0 in.)	
Temperature calibration data ^H	When the 'range-of-use' is 30° or greater and less than 90° then at least 3 data points are required. When the 'range-of-use' is 90° or greater, then at least 4 data points are required. In all cases the calibration data is to be included in calibration report.	
Temperature calibration report	The DCT shall have a report of temperature calibration traceable to a national calibration or metrology standards body issued by a competent calibration laboratory with demonstrated competency in temperature calibration. An ISO 17025 accredited laboratory with temperature calibration in its accreditation scope would meet this requirement.	

^A A device's minimum and maximum temperature may be different than the values shown provided the calibration requirements are met.

^B Accuracy is the total combined accuracy of the DCT unit, which includes the display, electronics, and sensor probe with correction factors.

^C Minimum probe immersion depth as determined by Practice [D7962](#), or an equivalent procedure, and is to be equal to or less than the value in the table. This is the minimum immersion needed to obtain an accurate temperature measurement. Thus, the actual immersion will likely exceed this minimum.

^D Drift is the difference between the corrected DCT temperature and a reference.

^E *Response Time*—This applies to a Digital Contact Thermometer's (DCT) combined display and sensor system. Conformance with this requirement is to be provided in the manufacturer's or supplier's product documentation. Response time is defined as the time for a DCT to respond to a 63.2 % step change in temperature. The step change begins with the DCT probe at an initial temperature of 20 °C \pm 5 °C in air and the timing begins when it is transferred to water at 77 °C \pm 5 °C which is flowing at 0.9 m/s \pm 0.09 m/s past the sensor, as described in Test Method [E644](#) or an equivalent method. The DCT display refresh rate is to be at intervals of every 3 seconds or less.

^F Sensor sheath is the tube that holds the sensing element. The value is the nominal outside diameter of the sheath segment containing the sensing element.

^G The physical length of the temperature sensing element. Contact the DCT supplier to determine whether this parameter is met, as it will not be accessible to the user.

^H Minimum number of calibration data points used to establish calibration.

7.3 *Finger Cots*, latex, used to close the top of the oil-filled stators when they are in the ~~pre-treatment heating baths, sample preheater~~, particularly if subject to water condensation inside the stator when heated in water baths.

7.4 *Viscometer Heads*, equipped with torque signal output and suitable sensitivity.

7.5 *Temperature-programmable, Low-temperature Bath*.

7.6 *Torque Signal Recorder*—Computer, analog-to-digital converter, and data analysis program.

7.7 *Constant-temperature Oven or Water Bath*, (programmable or non-programmable) for preheating samples.

7.8 *Operator Calibrated, Temperature Measuring Devices*, for 90 °C and –20 °C.

7.9 *Newtonian Calibration Oil*.

7.10 *Source of Dry Air or Nitrogen Gas* and means of gas introduction over top of stator.

8. Sampling

8.1 Approximately a 20 mL sample of test oil is necessary for the test. The sample must be thoroughly shaken so that the sample is homogeneous (see 12.1).

NOTE 2—The submitter of samples should refer to Practice D4057 to be aware of how to properly acquire representative samples of petroleum products.

9. Preparation of Apparatus

9.1 ~~Pre-treatment heating of~~ Pretreat the samples using either a water bath or an oven a preheater.

9.1.1 *Water Baths*—Using boiling distilled water and correcting for barometric pressure (if significant because of altitude of the laboratory), check the calibration of liquid-in-glass or digital contact thermometer used in the ~~pre-treatment water bath sample preheater~~ by appropriate methods.

9.1.1.1 Check the constant temperature of the ~~pre-treatment water bath~~ after ensuring that it is filled with distilled water to a level 20 mm above the oil level in the immersed stators. The temperature should be constant at 90 °C ± 2 °C. Complete this check upon initial set-up or if test results indicate suspicious viscous behavior of the sample. Examples of such behavior might include non-repeatable gelation indices or GI temperature for a given fluid, unexpectedly high or low gelation indices, gelation at an unexpected temperature, or non-repeatable viscosity-temperature curves.

9.1.2 ~~Ovens~~—*Air Baths or Ovens and Separate Dry Block Heaters*—Check the calibration of the temperature sensing device by appropriate methods. The temperature should be constant at 90 °C ± 2 °C. Complete this check upon initial set-up or if test results indicate suspicious viscous behavior of the sample. Examples of such behavior might include non-repeatable gelation indices or GI temperature for a given fluid, unexpectedly high or low gelation indices, gelation at an unexpected temperature, or non-repeatable viscosity-temperature curves.

9.1.2.1 Determine the length of time required to bring the sample up to 90 °C. Use this time interval to establish the length of time the sample is held in the ~~oven before being poured into the stator preheater.~~

NOTE 3—Preheaters integral to the dry block bath and calibrated at –20 °C can reasonably be assumed to hold 90 °C ± 2 °C without additional checks.

9.2 *Preparing Liquid Cold bath—Programmable Cooling Bath*—~~Check the liquid level in the programmable liquid cold bath. Fill bath~~ If using a liquid bath, fill to proper depth according to supplier's instructions at –5 °C.

NOTE 4—To ensure adequate cooling fluid height above the sample, it is advisable to fill the liquid bath at –5 °C to the appropriate level indicated by the manufacturer in the owners' manual to avoid over-filling the bath and to always bring the bath back to this temperature when on stand-by. This keeps