



Designation: F648 – 21

# Standard Specification for Ultra-High-Molecular-Weight Polyethylene Powder and Fabricated Form for Surgical Implants<sup>1</sup>

This standard is issued under the fixed designation F648; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon ( $\epsilon$ ) indicates an editorial change since the last revision or reapproval.

## 1. Scope

1.1 This specification covers ultra-high molecular weight polyethylene powder (UHMWPE) and fabricated forms intended for use in surgical implants.

1.2 The requirements of this specification apply to UHMWPE in two forms. One is virgin polymer powder (Section 4). The second is any form fabricated from this powder from which a finished product is subsequently produced (Section 5). This specification addresses material characteristics and does not apply to the packaged and sterilized finished implant.

1.3 The requirements of this specification do not apply to UHMWPE virgin powder or fabricated forms intentionally crosslinked or blended with other additives, for example, antioxidants.

1.4 The biological response to polyethylene in soft tissue and bone has been well characterized by a history of clinical use (1-3)<sup>2</sup> and by laboratory studies (4-6).

1.5 The values stated in SI units are to be regarded as standard.

1.6 The following precautionary caveat pertains only to the test method portion, Section 7, of this specification: *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety, health, and environmental practices and determine the applicability of regulatory limitations prior to use.*

1.7 *This international standard was developed in accordance with internationally recognized principles on standardization established in the Decision on Principles for the Development of International Standards, Guides and Recommendations issued by the World Trade Organization Technical Barriers to Trade (TBT) Committee.*

<sup>1</sup> This specification is under the jurisdiction of ASTM Committee F04 on Medical and Surgical Materials and Devices and is the direct responsibility of Subcommittee F04.11 on Polymeric Materials.

Current edition approved April 1, 2021. Published April 2021. Originally approved in 1980. Last previous edition approved in 2014 as F648 – 14. DOI: 10.1520/F0648-21.

<sup>2</sup> The boldface numbers in parentheses refer to the list of references at the end of this specification.

## 2. Referenced Documents

### 2.1 ASTM Standards:<sup>3</sup>

- D256 Test Methods for Determining the Izod Pendulum Impact Resistance of Plastics
- D638 Test Method for Tensile Properties of Plastics
- D648 Test Method for Deflection Temperature of Plastics Under Flexural Load in the Edgewise Position
- D790 Test Methods for Flexural Properties of Unreinforced and Reinforced Plastics and Electrical Insulating Materials
- D792 Test Methods for Density and Specific Gravity (Relative Density) of Plastics by Displacement
- D1505 Test Method for Density of Plastics by the Density-Gradient Technique
- D1898 Practice for Sampling of Plastics (Withdrawn 1998)<sup>4</sup>
- D4020 Specification for Ultra-High-Molecular-Weight Polyethylene Molding and Extrusion Materials
- F619 Practice for Extraction of Materials Used in Medical Devices
- F748 Practice for Selecting Generic Biological Test Methods for Materials and Devices
- F749 Practice for Evaluating Material Extracts by Intracutaneous Injection in the Rabbit
- F756 Practice for Assessment of Hemolytic Properties of Materials
- F763 Practice for Short-Term Screening of Implant Materials
- F813 Practice for Direct Contact Cell Culture Evaluation of Materials for Medical Devices
- F895 Test Method for Agar Diffusion Cell Culture Screening for Cytotoxicity
- F981 Practice for Assessment of Compatibility of Biomaterials for Surgical Implants with Respect to Effect of Materials on Muscle and Insertion into Bone

<sup>3</sup> For referenced ASTM standards, visit the ASTM website, [www.astm.org](http://www.astm.org), or contact ASTM Customer Service at [service@astm.org](mailto:service@astm.org). For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

<sup>4</sup> The last approved version of this historical standard is referenced on [www.astm.org](http://www.astm.org).

**F2759** Guide for Assessment of the Ultra-High Molecular Weight Polyethylene (UHMWPE) Used in Orthopedic and Spinal Devices

2.2 ISO Standards:<sup>5</sup>

**ISO 3451-1** Plastics—Determination of Ash, Part 1: General Methods

**ISO 11542/2** Plastics—Ultra-High Molecular Weight Polyethylene (UHMWPE) Moulding and Extrusion Materials—Part 2: Preparation of Test Specimens and Determination

**ISO 9001** Quality Management Systems—Requirements

**ISO 13485** Medical Devices—Quality Management Systems—Requirements for Regulatory Purposes

**3. Terminology**

3.1 *Definitions of Terms Specific to This Standard:*

3.1.1 *fabricated form, n*—any bulk shape of UHMWPE, fabricated from the virgin polymer powder and used during the process of fabricating surgical implants prior to packaging and sterilization.

3.1.1.1 *Discussion*—This form results from the application of heat and pressure to the virgin polymer powder, and the material characteristics of this form are subject to the applicable requirements of this specification. In present practice, this includes ram-extruded bars or molded blocks from which the final product form is machined, or a molded shape which is subsequently trimmed.

3.1.2 *generic property, n*—that property which is determined solely by the chemical composition and structure of the virgin polymer.

3.1.3 *morphology index (MI), n*—ratio of the total number of Type A and Type B indications (see **Annex A2**) to the total surface area examined in cm<sup>2</sup>.

3.1.4 *Type A non-fused flake, n*—a Type A non-fused flake (**A2.4.1** and **Fig. A2.1**) is an indication visible under conditions described in **A2.5.1** that has an essentially complete circumferential black boundary and a white center.

3.1.5 *Type B non-fused flake, n*—a Type B non-fused flake (**A2.4.2** and **Fig. A2.2**) is an indication visible under conditions described in **A2.5.1** that has a partially circumferential black boundary that appears to trace out 50 % to 99 % of a flake’s perimeter.

3.1.6 *virgin polymer powder, n*—form of UHMWPE as obtained from the powder manufacturer and prior to fabrication into a bulk shape.

**4. Virgin UHMWPE Powder Requirements**

4.1 *Generic Properties:*

4.1.1 The virgin polymer shall be a homopolymer of ethylene in accordance with Specification **D4020**.

4.1.2 The resin type and solution viscosity number requirements are listed in **Table 1**.

4.2 *Nongeneric Properties:*

**TABLE 1** Requirements for UHMWPE Powders

Property	Test Method	Requirement		
		Type 1	Type 2	Type 3
Resin Type				
Viscosity Number, mL/g,	ASTM <b>D4020</b> (0.02 %)	2000–3200	>3200	>3200
Elongation Stress, (Minimum)	ASTM <b>D4020</b>	0.20	0.42	0.42
Ash, mg/kg, (Maximum)	ISO 3451-1	125	125	300
Extraneous Matter, No. Particles, (Maximum)	<b>4.2.1</b>	3	3	25
Titanium, mg/kg, (Maximum)	<b>7.1.3.1</b>	40	40	150
Aluminum, mg/kg, (Maximum)	<b>7.1.3.1</b>	20	20	100
Calcium, mg/kg, (Maximum)	<b>7.1.3.1</b>	5	5	50
Chlorine, mg/kg, (Maximum)	<b>7.1.3.2</b>	30	30	90

4.2.1 When a 300 g sample is prepared and viewed in accordance with **7.1.2**, there shall be no more particles of extraneous matter than that specified in **Table 1**.

4.2.2 To promote uniformity between different lots of polymer powder, concentration limits for trace elements have been established and are listed in **Table 1**.

4.2.3 When determined as described in ISO 3451-1, the mean ash of duplicate samples shall not exceed the limits established in **Table 1**.

4.3 *Quality System Requirements:*

4.3.1 The UHMWPE powder as described in the scope of this specification shall be produced in accordance with an ISO 9001 or ISO 13485 certified Quality Management System.

**5. UHMWPE Fabricated Form Requirements**

5.1 *Compositional Requirements:*

5.1.1 No stabilizers, antioxidants, or processing aids are to be added to the virgin polymer powder during manufacture of a fabricated form.

5.1.2 No stabilizers, antioxidants, or processing aids are to be added to the fabricated form during manufacture of the final implant.

5.2 *Physical Requirements:*

5.2.1 *Foreign Matter Requirements:*

5.2.1.1 When 5000 cm<sup>2</sup> is evaluated according to **7.2.2**, there shall be no more than ten particles of extraneous matter visible on the surface when visually inspected by a person with normal or fully corrected vision.

5.2.2 *Morphology Requirements:*

5.2.2.1 When evaluated during the consolidation process validation according to **Annex A2**, the calculated morphology index (MI) and total surface area examined shall be reported. It is not required to evaluate the morphology index during routine monitoring of a validated manufacturing process because alternative test methods in this standard, such as density and the mechanical properties required in **Table 2**, already provide reasonable, redundant assurance of successful consolidation.

5.3 *Mechanical Requirements:*

5.3.1 UHMWPE in fabricated form from which implants will be made (after annealing processes, if appropriate) shall meet the requirements listed in **Table 2**.

5.3.2 The following mechanical tests may be conducted based on agreement between the vendor and purchaser:

5.3.2.1 Deflection temperature, Test Method **D648** (1.8 MPa); and flexural modulus, Test Methods **D790** (secant, 2 % offset).

<sup>5</sup> Available from International Organization for Standardization (ISO), 1, ch. de la Voie-Creuse, CP 56, CH-1211 Geneva 20, Switzerland, <http://www.iso.org>.

**TABLE 2 Requirements for UHMWPE Fabricated Forms**

Property	Test Method	Requirement		
		Type 1	Type 2	Type 3
Resin Type				
Density, kg/m <sup>3</sup>	ASTM <b>D792</b> or <b>D1505</b>	927–944	927–944 <sup>B</sup>	927–944
Tensile Strength, 23 °C, MPa, (Minimum)	ASTM <b>D638</b> , Type IV, 1.5 mm ± 0.5 mm, 5.08 cm/min			
Ultimate Yield		40	40	27
Elongation, %, (Minimum) <sup>A</sup>	ASTM <b>D638</b> , Type IV, 5.08 cm/min	21	19	19
Izod Impact Strength, kJ/m <sup>2</sup> , (Minimum)	<b>Annex A1</b>	380	340	250
		126	73	25

<sup>A</sup> Use an extensometer for measuring strain and calculating percent elongation.

<sup>B</sup> For molded shapes as defined in 3.1.1.1, the density requirement is 925 to 944 for Type 2 resin.

#### 5.4 Quality System Requirements:

5.4.1 The UHMWPE fabricated forms as described in the scope of this specification shall be produced in accordance with an ISO 9001 or ISO 13485 certified Quality Management System.

### 6. Sampling

6.1 Where applicable, the requirements of this specification shall be determined for each lot of powder and fabricated form by sampling sizes and procedures according to Practice **D1898**, or as agreed upon between the purchaser and seller.

### 7. Test Methods

#### 7.1 UHMWPE Powder:

7.1.1 Determine the solution viscosity number in accordance with the method given in Specification **D4020** at a concentration of 0.02 %.

7.1.2 Determine the amount of extraneous matter by the following procedure as agreed upon by the purchaser and seller.

7.1.2.1 A 300 g sample is divided into four 75 g samples. Place a 75 g sample in each of four 1000 mL Erlenmeyer flasks, add 400 mL isopropyl alcohol, shake 5 min, and let settle for 5 min. Count the total number of particles of extraneous matter in the four flasks.

7.1.2.2 Visually examine (with 20/20 corrected vision if necessary) the four flasks and count the total number of particles of extraneous matter.

7.1.3 Determine the following trace element concentrations by the following methods, or by methods agreed upon by the purchaser and seller.

7.1.3.1 The elements Ti, Al, and Ca may be determined by atomic absorption (AA) or emission spectroscopy (ES); inductively coupled plasma mass spectroscopy (ICP/MS); or inductively coupled plasma spectroscopy (ICP).

7.1.3.2 The element chlorine (Cl) may be determined potentiometrically, titrimetrically, by neutron activation analysis, by inductively coupled plasma mass spectroscopy (ICP/MS), or by the oxygen bomb combustion/UV-Vis spectroscopy method.

#### 7.2 UHMWPE Fabricated Form:

7.2.1 The requirement that there will be no addition of any stabilizer, antioxidant, or processing aid during fabrication of the fabricated form shall be met by certification of the fabricator.

7.2.2 Determine the amount of extraneous matter by the following procedure.

7.2.2.1 Prepare a number of test specimens from the fabricated form as agreed upon by the purchaser and seller.

7.2.2.2 Visually examine (with 20/20 corrected vision if necessary) a total area of 5000 cm<sup>2</sup> taken from locations within the fabricated form agreed upon by the purchaser and seller.

7.2.3 Determine the density in accordance with Test Methods **D792** or **D1505**.

7.2.4 Determine specific mechanical properties in accordance with the methods listed in **Table 2**. Mechanical test specimens shall be produced by methods that represent those used to produce the fabricated form.

7.2.5 Unless otherwise specified, the testing described in **Table 2** (except for ash) shall be conducted under standard conditions of 23 ± 2 °C after storage of the test specimens for at least 16 h.

### 8. Biocompatibility

8.1 This material has been shown to produce a well-characterized level of biological response following long-term clinical use in laboratory animals. The results of these studies and the clinical history indicate an acceptable level of biological response in the applications in which the material has been utilized. When new applications of the material, or modification to the material or physical forms of the materials are being contemplated, the recommendations of Practice **F748** should be considered and testing as described in Practices **F619**, **F749**, **F756**, **F763**, **F813**, and **F981** as well as Test Method **F895**.

### 9. Keywords

9.1 fabricated forms; powdered form; ultra-high molecular weight polyethylene

ANNEXES

(Mandatory Information)

A1. IMPACT STRENGTH

A1.1 General Description

A1.1.1 This test method covers the determination of the impact resistance of ultra-high molecular weight polyethylene (UHMWPE) which is extremely impact resistant. When tested according to Test Method D256, Method A, UHMWPE generally gives a non-break type for failure, rendering the test result invalid. This test method specifies the same type of pendulum impact test machine as given in Test Method D256 but introduces a much higher degree of stress concentration into the specimen by double notching with a razor blade. It is advised that the user be familiar with Test Method D256 before attempting to use this test method.

A1.2 Apparatus

A1.2.1 The Izod-type impact machine which conforms to the requirements of Test Method D256, including the calibration and checking methods, shall be used.

A1.3 Test Specimen


A1.3.1 The geometry and dimensions of the specimen are given in Fig. A1.1.

A1.3.2 The specimens shall be made from the fabricated form.

A1.3.3 Each specimen shall be free of twist and shall be bounded by mutually perpendicular pairs of plane parallel surfaces, free from scratches, pits, and sink marks.

A1.4 Notching of Specimens

A1.4.1 In the case of compression molding, the two notches (or width of two notches) shall be perpendicular to the direction of application of molding pressure, if applicable. The impact resistance of a plastic material may be different if the notch is perpendicular to, rather than parallel to, the direction

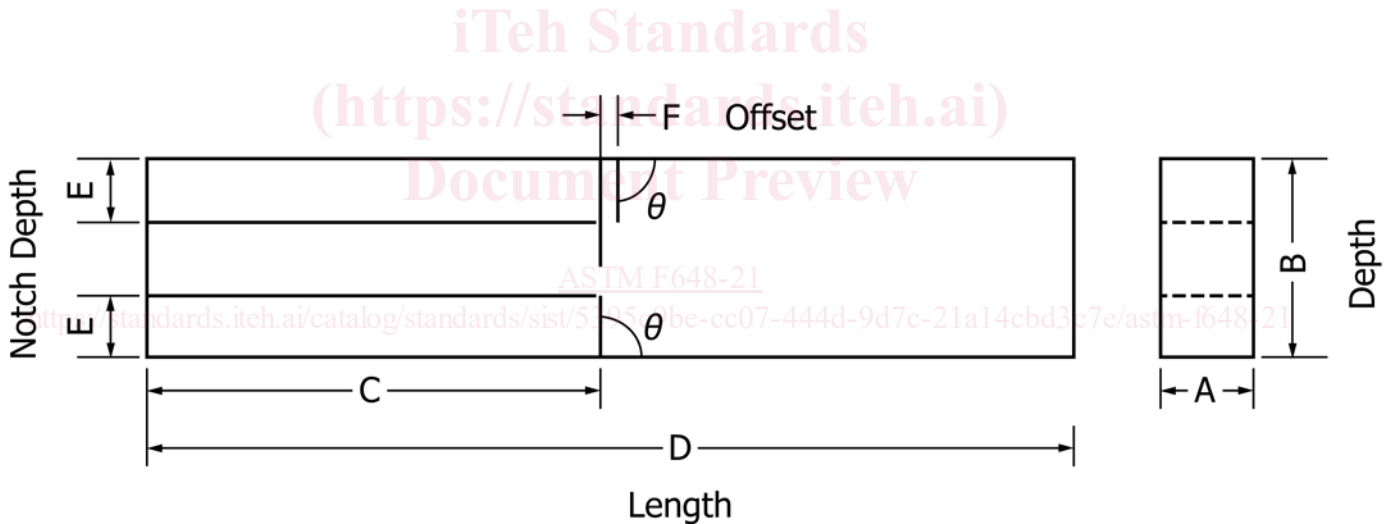

	mm		in.
A	6.35 ± 0.38	A	0.250 ± 0.015
B	12.70 ± 0.10	B	0.500 ± 0.004
C	31.75 ± 0.25	C	1.250 ± 0.010
D	63.50 ± 0.38	D	2.500 ± 0.015
E	4.57 ± 0.08	E	0.180 ± 0.003
F	0.00 ± 0.13	F	0.000 ± 0.005
O	90° ± 2°	O	90° ± 2°

FIG. A1.1 Dimensions of Double-Notched Izod Test Specimen



of molding. The same is true for specimens cut with or across the grain of an anisotropic sheet or plate.

A1.4.2 A  $4.57 \pm 0.076$  mm ( $0.180 \pm 0.003$  in.) deep notch shall be made with a suitable machine by pressing in a 0.25 mm (0.010 in.) thick single-edge razor blade with a  $15^\circ$  included angle at the cutting edge. The notching speed shall be less than 508 mm/min. (20 in./min.). A new blade shall be used after notching 40 specimens.

A1.4.3 The calibration of the notching machine shall be checked by direct measurement of the notch depth, perpendicularity, and offset of the two notches. One of the possible measurement methods is given in A1.8.

**A1.5 Conditioning**

A1.5.1 *Conditioning*—Condition the notched specimens at  $23 \pm 2$  °C ( $73 \pm 4$  °F) for not less than 16 h prior to testing.

A1.5.2 *Test Conditions*—Conduct the test in the standard laboratory atmosphere of  $23 \pm 2$  °C ( $73 \pm 4$  °F).

**A1.6 Procedure**

A1.6.1 At least five and preferably ten individual determinations of impact value shall be made on each sample to be tested under the conditions prescribed.

A1.6.2 Measure the width of each specimen in the area between notches twice with a micrometer to the nearest 0.025 mm (0.001 in.) and record its average width. Carefully measure the distance between the notch roots on the two sides of the specimen. Use of an optical microscope may improve the accuracy of this measurement. Record the average value and multiply this number by the width of the specimen to get the remaining unnotched cross section area, AR. Also record the identifying markings of the specimen.

A1.6.3 Estimate the breaking energy for the specimen and select a pendulum of suitable energy. Start the test with a pendulum of 11 J (8 ft-lb), if no prior test data is available. Use the lightest standard pendulum that is expected to break each specimen in the group with a loss of not more than 85 % of its energy.

A1.6.4 Before testing the specimens, perform the operations on the machine.

A1.6.4.1 With the excess energy indicating pointer in its normal starting position but without a specimen in the vise, release the pendulum from its normal starting position and note the position the pointer attains after the swing as one reading of Factor A.


A1.6.4.2 Without resetting the pointer, raise the pendulum and release again. The pointer should move up the scale an additional amount. Repeat this procedure until a swing causes no additional movement of the pointer and note the final reading as one reading of Factor B.

A1.6.4.3 Repeat the above two operations several times and calculate and record the average A and B readings.

A1.6.5 Position the specimen precisely and rigidly but not too tightly clamped in the vise. The relationship of the vise, specimen, and striking edge of the pendulum to each other is given in Fig. A1.2. Note that the top plane of the vise shall be  $0.13 \pm 0.13$  mm ( $0.005 \pm 0.005$  in.) below the notches.

A1.6.6 Release the pendulum and note and record the excess energy remaining in the pendulum after breaking the specimen.

A1.6.7 From the breaking strength of the specimen and Factors A and B, determine the energy loss of the pendulum due to windage and friction using the correction charts from the commercial testing machine supplier. If these charts are not

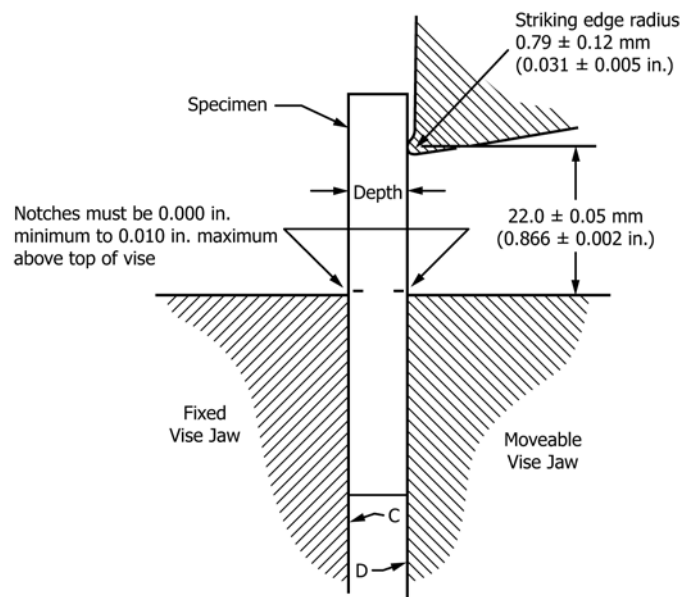

Planes C and D must be parallel to within 0.025 mm (0.001 in.)  
**FIG. A1.2 Relationship of Vise, Specimen, and Striking Edge to Each Other**