



Designation: E2008 – 17 (Reapproved 2021)

Standard Test Methods for Volatility Rate by Thermogravimetry¹

This standard is issued under the fixed designation E2008; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

1. Scope

1.1 These test methods cover procedures for assessing the volatility of solids and liquids at given temperatures using thermogravimetry under prescribed experimental conditions. Results of these test methods are obtained as volatility rates expressed as mass per unit time. Rates ≥ 5 $\mu\text{g}/\text{min}$ are achievable with these test methods.

1.2 Temperatures typical for these test methods are within the range from 25 °C to 500 °C. This temperature range may differ depending upon the instrumentation used.

1.3 These test methods are intended to provide a value for the volatility rate of a sample using a thermogravimetric analysis measurement on a single representative specimen. It is the responsibility of the user of these test methods to determine the need for and the number of repetitive measurements on fresh specimens necessary to satisfy end use requirements.

1.4 The values stated in SI units are to be regarded as standard. No other units of measurement are included in this standard.

1.5 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety, health, and environmental practices and determine the applicability of regulatory limitations prior to use.*

1.6 *This international standard was developed in accordance with internationally recognized principles on standardization established in the Decision on Principles for the Development of International Standards, Guides and Recommendations issued by the World Trade Organization Technical Barriers to Trade (TBT) Committee.*

¹ These test methods are under the jurisdiction of ASTM Committee E37 on Thermal Measurements and are the direct responsibility of Subcommittee E37.01 on Calorimetry and Mass Loss.

Current edition approved July 1, 2021. Published July 2021. Originally approved in 1999. Last previous edition approved in 2017 as E2008 – 17. DOI: 10.1520/E2008-17R21.

2. Referenced Documents

2.1 ASTM Standards:²

E177 Practice for Use of the Terms Precision and Bias in ASTM Test Methods

E473 Terminology Relating to Thermal Analysis and Rheology

E691 Practice for Conducting an Interlaboratory Study to Determine the Precision of a Test Method

E1142 Terminology Relating to Thermophysical Properties

E1582 Test Method for Temperature Calibration of Thermogravimetric Analyzers

E1860 Test Method for Elapsed Time Calibration of Thermal Analyzers

E2040 Test Method for Mass Scale Calibration of Thermogravimetric Analyzers

3. Terminology

3.1 Definitions:

3.1.1 The following terms are applicable to these test methods and can be found in Terminologies E473 and E1142:

3.1.1.1 thermogravimetric analysis (TGA),

3.1.1.2 thermogravimetry (TG), and

3.1.1.3 volatility.

3.2 Definitions of Terms Specific to This Standard:

3.2.1 volatility rate—the rate of conversion of a solid or liquid substance into the vapor state at a given temperature; mass per unit time.

4. Summary of Test Method

4.1 A solid or liquid specimen is confined in an appropriate container with a pinhole opening between 0.33 mm and 0.38 mm. The confined specimen is heated within a thermogravimetric analyzer either to a temperature and held constant at that temperature for a fixed interval of time (Test Method A, Fig. 1) or at a slow constant heating rate between temperature limits (Test Method B, Fig. 2). The mass of the specimen is measured continuously and it or its rate of change is displayed as a function of time or temperature. The volatility rate at any

² For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For Annual Book of ASTM Standards volume information, refer to the standard's Document Summary page on the ASTM website.

water at 323 K; 0.33 mm pinhole; 5.285 mg; nitrogen purge at 100 mL/min

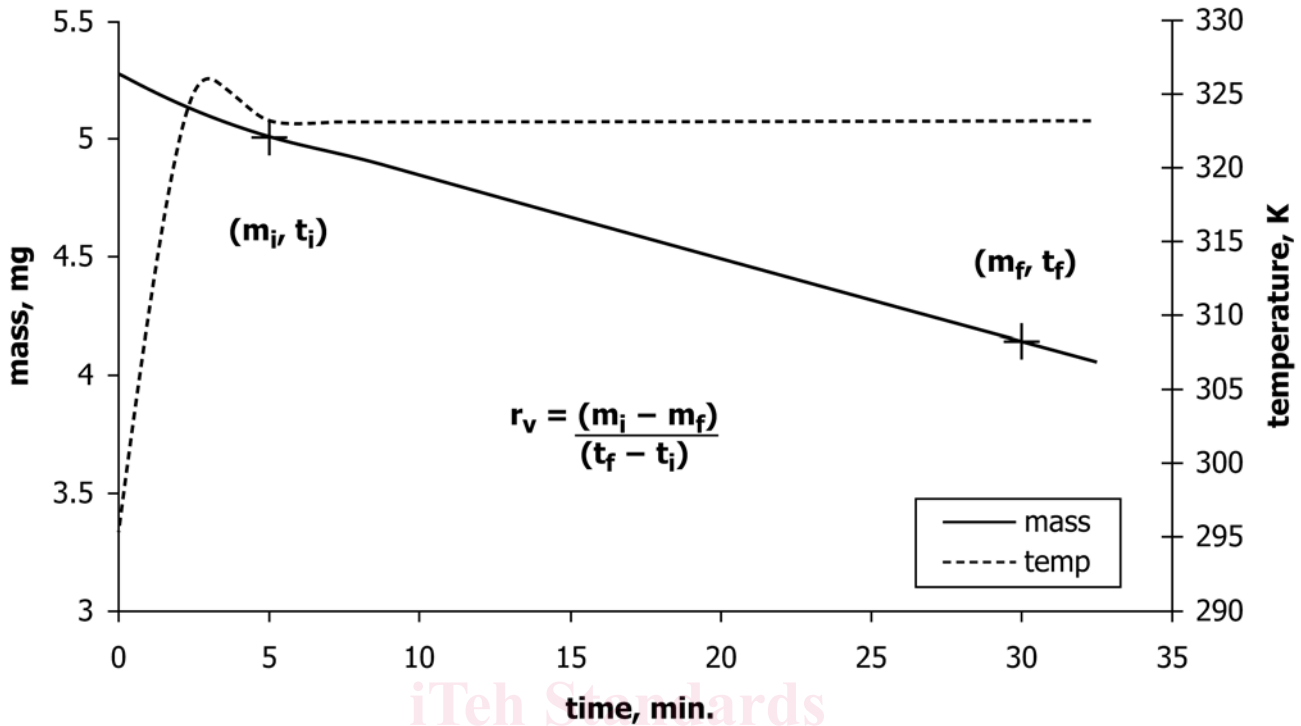


FIG. 1 Test Method A: R_v = Average Volatility Rate

temperature is reported either as the average rate of mass loss per unit time from Test Method A or as the instantaneous rate of mass loss (first derivative) per unit time from Test Method B.

5. Significance and Use

5.1 Volatility of a material is not an equilibrium thermodynamic property but is a characteristic of a material related to a thermodynamic property that is vapor pressure. It is influenced by such factors as surface area, temperature, particle size, and purge gas flow rate; that is, it is diffusion controlled.

5.2 The extent of containment achieved for specimens in these test methods by means of a pinhole opening between 0.33 mm to 0.38 mm allows for measurement circumstances that are relatively insensitive to experimental variables other than temperature. Decreasing the extent of containment by use of pinholes larger than 0.38 mm will increase the magnitude of the observed rate of mass loss but will also reduce the measurement precision by increasing the sensitivity to variations in other experimental variables.

5.3 Results obtained by these test methods are not strictly equivalent to those experienced in processing or handling conditions but may be used to rank materials for their volatility in such circumstances. Therefore, the volatility rates determined by these test methods should be considered as index values only.

5.4 The volatility rate may be used to estimate such quantifiable values as drying interval or the extent of volatile release from a process.

6. Interferences

6.1 Specimens that consist of a mixture of two or more volatile components or that undergo decomposition during this test may exhibit curvature in the mass loss versus time plot of Test Method A (see Fig. 3). In such cases the volatility rate is not constant and shall not be reported as a singular value.

7. Apparatus

7.1 The essential instrumentation required to provide the minimum thermogravimetric analytical capability for these test methods includes:

7.1.1 A *Thermobalance*, composed of:

7.1.1.1 A *Furnace*, to provide uniform controlled heating of a specimen at a constant temperature or at a constant rate within the applicable temperature range of these test methods;

7.1.1.2 A *Temperature Sensor*, to provide an indication of the specimen/furnace temperature to ± 1 K;

7.1.1.3 A continuously recording *Balance*, to measure the specimen mass with a minimum capacity of 100 mg and a sensitivity of ± 10 μ g;

7.1.1.4 A means of sustaining the specimen/container under *atmospheric control* of inert gas (nitrogen, helium, and so forth) of 99.9 % purity at a purge rate of 50 mL/min to 100 mL/min ± 5 %.

7.1.2 A *Temperature Controller*, capable of executing a specific temperature program by operating the furnace between selected temperature limits at a rate of temperature change of 1 K/min to 2 K/min constant to within ± 0.1 K/min or to rapidly heat a specimen at a minimum of 50 K/min to an

water at 2 K/min; 0.38 mm pinhole; 4.762 mg; nitrogen at 100 mL/min

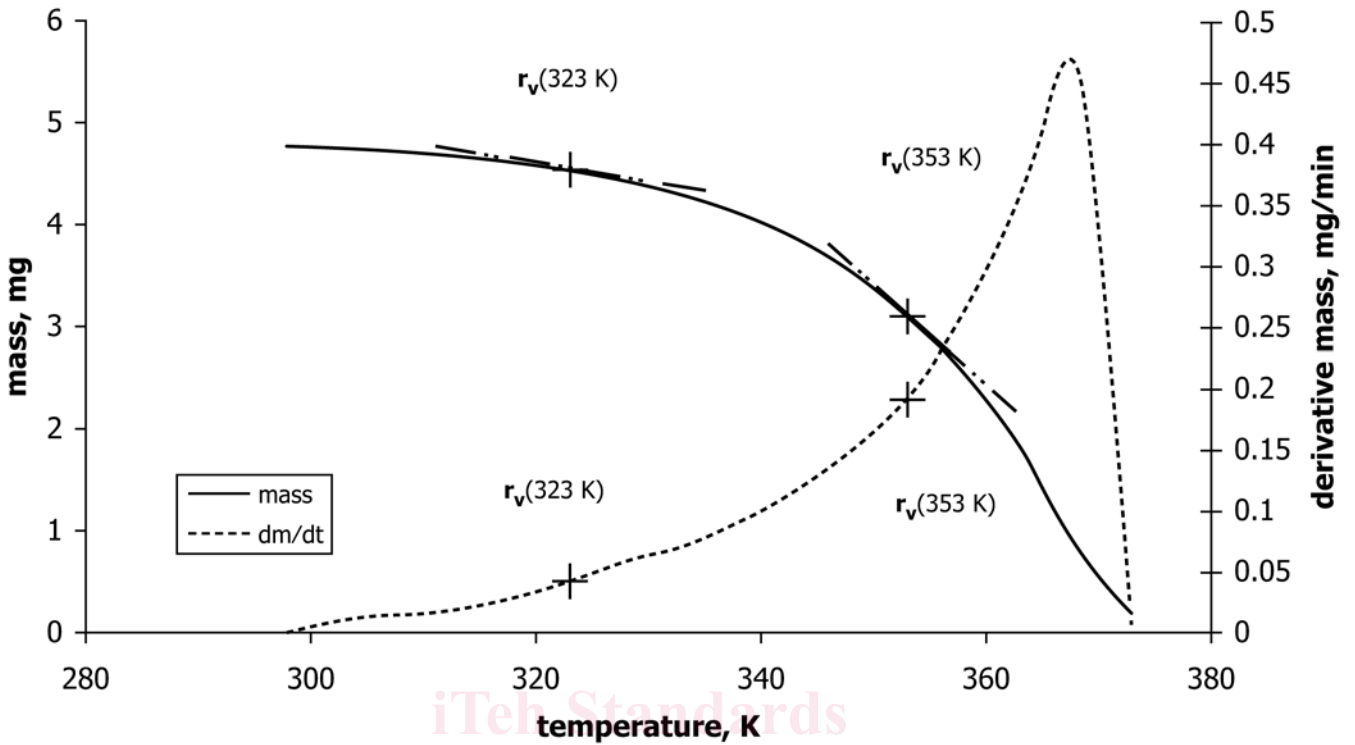


FIG. 2 Test Method B: $R_v =$ Instantaneous Volatility Rate

water/ethanol 50:50; 0.38 mm pinhole; 9.183 mg; nitrogen purge at 100 mL/min

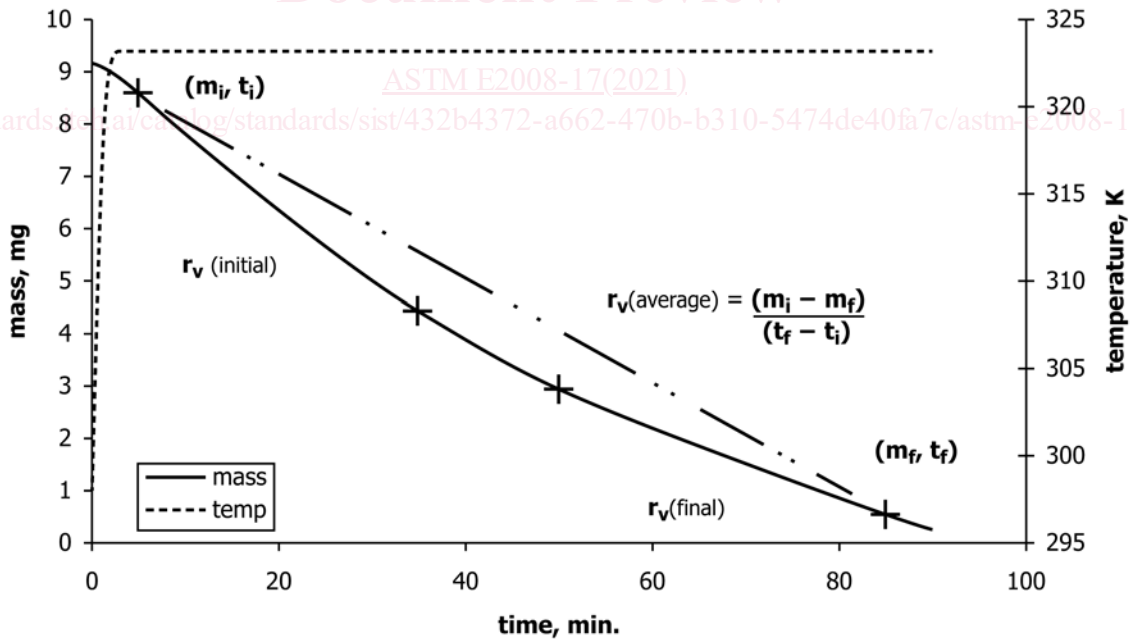


FIG. 3 Test Method A—Two Component Mixture

isothermal temperature that is maintained constant to ± 1 K for a minimum of 30 min.

7.1.3 A Data Collection Device, to provide a means of acquiring, storing, and displaying measured or calculated

signals, or both. The minimum output signals required for thermogravimetry are mass, temperature, and time.

7.1.4 Sealable Containers, (pans, crucibles, and so forth), that are inert to the specimen, that will remain gravimetrically

stable within the temperature limits of these test methods, and that contain a pinhole in the lid of diameter between 0.33 mm and 0.38 mm.³

NOTE 1—The most critical parameters for containers suitable for use with these test methods are the pinhole diameter and the lid thickness. Sealable containers of volumes (25 μL to 50 μL) and wall thicknesses (80 μm to 150 μm) commercially available from Mettler-Toledo, Perkin Elmer Corporation, and TA Instruments, Inc., have been found suitable for this purpose.

7.2 Auxiliary equipment necessary or useful in conducting these test methods includes:

7.2.1 While not required, it is convenient to have a data analysis device that will continuously calculate and display the first derivative of mass with respect to time (in mass/min) capable of detecting 0.05 $\mu\text{g}/\text{min}$.

7.2.2 Device to encapsulate the specimen in sealable containers.

7.2.3 Micropipette or syringe to deliver liquid specimens of 1 μL to 30 μL into the containers.

8. Sampling

8.1 Samples are ordinarily measured as received. If a pretreatment is applied to any specimen, this treatment shall be noted in the report.

8.2 Since the applicable samples may be mixtures or blends, care shall be taken to ensure that the analyzed specimen is representative of the sample from which it is taken. If the sample is liquid, mixing prior to taking the specimen is sufficient to ensure this consideration. If the sample is solid, take several samplings from different areas and either combine into a single specimen or run as a separate specimen with the final analysis representing an average of these determinations. Include the number of determinations in the report.

9. Calibration

9.1 Perform temperature calibration in accordance with Practice E1582 using the same purge gas conditions and container type to be used for the subsequent measurements at a heating rate of 2 K/min. Do not disturb the temperature sensor position after this calibration.

9.2 Perform mass calibration in accordance with Test Method E2040.

9.3 Perform time scale calibration in accordance with Test Method E1860.

10. Procedure

10.1 *Test Method A—Isothermal Test:*

10.1.1 Initiate a purge gas flow through the thermobalance between 50 mL/min to 100 mL/min \pm 5 %.

10.1.2 Equilibrate the furnace, gas purge, and so forth at room temperature, and tare the balance.

NOTE 2—If the balance is tared with the empty crucible and lid in place, then the mass of the test specimen may be recorded directly

10.1.3 Encapsulate a specimen in an appropriate container with the specified pinhole. Specimen sizes between 1 mg and

30 mg are typical for this test method, with the larger mass being used for more volatile specimens. (**Warning**—Volatile materials may pose a respiratory hazard. Avoid unnecessary exposure to vapors.)

10.1.4 Place the encapsulated specimen in the thermogravimetric analyzer, close the furnace, and allow the temperature, purge, and so forth, to become stable within \pm 1 % of settings.

NOTE 3—For highly volatile substances, a significant mass fraction of the specimen could be lost during this period of equilibration. Any large discrepancy between the specimen mass as delivered and subsequently recorded by the thermobalance should be noted in the report.

10.1.5 Heat the specimen rapidly at 50 K/min to the desired isothermal temperature, and thereafter, maintain the isothermal temperature to \pm 1 K for 30 min. Record the specimen mass in mg or μg continually during this heating program versus time. The specimen temperature should be recorded during the heating program.

NOTE 4—If the specimen is exhausted before 30 min have elapsed, it is recommended that the test be repeated with a larger specimen mass. If excessively large specimen mass is required to complete a 30-min test time, a shorter time interval or a lower isothermal temperature may be used and shall be reported.

NOTE 5—The initial rapid heating to the desired isothermal temperature may result in a momentary overshoot in the furnace temperature. Overshoot in itself does not create a measurement question provided the data in 10.1.7 is taken only from the region where the isothermal temperature is stable and provided the entire specimen has not been exhausted.

10.1.6 Restore the furnace to ambient temperature, and remove the specimen container.

10.1.7 Calculate the volatility rate in accordance with 11.2.

10.1.8 Repeat 10.1.2 – 10.1.7 for additional samples.

10.2 *Test Method B—Constant Heating Rate Test:*

10.2.1 Follow the instructions given in 10.1.1 – 10.1.4.

10.2.2 Heat the specimen at a constant heating rate of 2 K/min \pm 0.1 K/min between ambient temperature and the desired limit temperature. Record the specimen mass in mg or μg continually during this heating program versus temperature, and calculate and display the first derivative (with respect to time) of the mass loss in $\mu\text{g}/\text{min}$ during heating.

NOTE 6—If the specimen is exhausted before reaching the desired limit temperature, repeat the test using a larger specimen mass. If excessively large specimen mass is required to reach the limit temperature, it may be necessary to terminate the test at a lower limit temperature, and this shall be noted in the report.

10.2.3 Restore the furnace to ambient temperature, and remove the specimen container.

10.2.4 Calculate the volatility rate in accordance with 11.3.

10.2.5 Repeat 10.2.1 – 10.2.4 for additional samples.

11. Calculation

11.1 Use all available decimals for each value in the calculations. Round the final volatility rate to the nearest 0.1 $\mu\text{g}/\text{min}$.

11.2 Using Test Method A, the volatility rate is obtained from the difference in mass at the initial time and the mass at the final time at the isothermal temperature divided by 30 min (or other elapsed time used, see Fig. 1):

³ See Appendix X1.