

---

# INTERNATIONAL STANDARD



# 4945

---

INTERNATIONAL ORGANIZATION FOR STANDARDIZATION • МЕЖДУНАРОДНАЯ ОРГАНИЗАЦИЯ ПО СТАНДАРТИЗАЦИИ • ORGANISATION INTERNATIONALE DE NORMALISATION

---

## Steel — Determination of nitrogen content — Spectrophotometric method

*Acier — Dosage de l'azote — Méthode spectrophotométrique*

**First edition — 1977-12-15**

Corrected and reprinted —

**iTeh STANDARD PREVIEW**  
**(standards.iteh.ai)**

ISO 4945:1977

<https://standards.iteh.ai/catalog/standards/sist/8997b13d-b12e-4d3b-b50b-0c45ace901bb/iso-4945-1977>

---

UDC 669.14 : 669.786 : 543.42

Ref. No. ISO 4945-1977 (E)

**Descriptors :** steels, chemical analysis, determination of content, nitrogen, spectrophotometric analysis.

Price based on 6 pages

FOREWORD

ISO (the International Organization for Standardization) is a worldwide federation of national standards institutes (ISO member bodies). The work of developing International Standards is carried out through ISO technical committees. Every member body interested in a subject for which a technical committee has been set up has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work.

Draft International Standards adopted by the technical committees are circulated to the member bodies for approval before their acceptance as International Standards by the ISO Council.

International Standard ISO 4945 was developed by Technical Committee ISO/TC 17, *Steel*, and was circulated to the member bodies in March 1976.

It has been approved by the member bodies of the following countries :

ISO 4945:1977		
Australia	India	Portugal
Belgium	Iran	South Africa, Rep. of
Canada	Ireland	Spain
Chile	Italy	Sweden
Czechoslovakia	Korea, Rep. of	Switzerland
Denmark	Mexico	Turkey
Finland	Netherlands	U.S.A.
France	Norway	U.S.S.R.
Germany	Philippines	Yugoslavia
Hungary	Poland	

The member bodies of the following countries expressed disapproval of the document on technical grounds :

Australia  
Japan

# Steel — Determination of nitrogen content — Spectrophotometric method

## 1 SCOPE

This International Standard specifies a spectrophotometric method for the determination of the nitrogen content of non-alloy and low-alloy steels. This method allows the determination only of the nitrogen content which can be converted to an ammonium salt.

## 2 FIELD OF APPLICATION

The method is applicable to non-alloy and low-alloy steels containing between 0,002 % and 0,050 % (m/m) of nitrogen and less than 0,6 % (m/m) of silicon.

## 3 REFERENCE

ISO/R 377, *Selection and preparation of samples and test pieces for wrought steel.*

## 4 PRINCIPLE

Dissolution of a test portion in dilute sulphuric acid.

After concentration, progressive increasing of the temperature to above 300 °C.

Separation of ammonia from the ammonium salt formed, by displacement and distillation in a boiling sodium hydroxide medium and collecting in an acid medium.

At ambient temperature, formation of a blue-coloured complex between the ammonium ions and phenol in the presence of sodium hypochlorite and sodium pentacyanonitrosylferrate(II) (sodium nitroprusside). Spectrophotometric measurement of the complex at a wavelength of about 640 nm.

## 5 REAGENTS

During the analysis, use only reagents of recognized analytical grade.

**5.1 Distilled or de-ionized water**, free from nitrogen compounds, purified by a second passage through ion-exchange resins.

**5.2 Potassium sulphate**, anhydrous ( $K_2SO_4$ ).

**5.3 Sulphuric acid**,  $\rho$  approximately 1,84 g/ml, about 96 % (m/m) solution, free from nitrogen compounds.

**5.4 Sulphuric acid**,  $\rho$  approximately 1,21 g/ml, about 29 % (m/m) solution.

Add in small portions, whilst cooling, 200 ml of sulphuric acid (5.3) to about 700 ml of water (5.1), make up the volume to 1 000 ml with water (5.1) and mix.

**5.5 Sodium hydroxide**, approximately 12 N solution.

Dissolve, with caution, 480 g of sodium hydroxide pellets in 700 ml of water (5.1) contained in a polytetrafluoroethylene beaker. Heat the solution to boiling and boil for 10 min. Cool, make up the volume to 1 000 ml with water (5.1) and mix. Store in a suitable plastics container.

**5.6 Sulphuric acid**, approximately 1 N solution.

Add 30 ml of sulphuric acid (5.3) to about 700 ml of water (5.1); after cooling make up the volume to 1 000 ml with water (5.1) and mix.

**5.7 Sulphuric acid**, approximately 0,04 N solution.

Dilute 40 ml of sulphuric acid solution (5.6) to 1 000 ml with water (5.1) and mix.

**5.8 Sodium hydroxide**, approximately 0,2 N solution.

Dilute 30 ml of a 250 g/l solution of sodium hydroxide with water (5.1), make up the volume to 1 000 ml with water (5.1) and mix.

**5.9 Sodium phenate** solution.

Add, whilst agitating and cooling, 5 g of phenol to a mixture of 10 ml of a 250 g/l solution of sodium hydroxide and 80 ml of water (5.1).

Make up the volume to 100 ml with water (5.1) and mix.

Prepare this solution at the time of use.

**5.10 Disodium hydrogen phosphate**, 0,1 M solution.

Dissolve 36 g of disodium hydrogen phosphate dodecahydrate ( $Na_2HPO_4 \cdot 12H_2O$ ) in water (5.1), make up the volume to 1 000 ml with water (5.1) and mix.

**5.11 Disodium pentacyanonitrosylferrate(II)**, 0,25 g/l solution.

Dissolve 10 g of disodium pentacyanonitrosylferrate(II)

dihydrate (sodium nitroprusside)  $[\text{Na}_2\text{Fe}(\text{CN})_5\text{NO} \cdot 2\text{H}_2\text{O}]$  in water (5.1), make up the volume to 1 000 ml with water (5.1) and mix.

At the moment of use, dilute 25 ml of this solution to 1 000 ml with water (5.1).

**5.12 Sodium hypochlorite**, approximately 0,1 N solution (approximately 0,3 % (m/m) of active chlorine).

Store this solution at a temperature less than 10 °C.

**5.13 Nitrogen**, standard solution corresponding to 0,100 0 g of nitrogen (N) per litre.

Weigh, to the nearest 0,1 mg, 0,471 6 g of dry ammonium sulphate, dissolve in water (5.1) and transfer the solution quantitatively to a 1 000 ml one-mark volumetric flask. Dilute to the mark and mix.

1 ml of this standard solution contains 100 µg of nitrogen (N).

**5.14 Nitrogen**, standard solution corresponding to 0,002 0 g of nitrogen (N) per litre.

Transfer 20,0 ml of the standard nitrogen solution (5.13) to a 1 000 ml one-mark volumetric flask, dilute to the mark with water (5.1) and mix.

1 ml of this standard solution contains 2 µg of nitrogen (N).

Prepare this standard solution at the time of use.

**5.15 Methyl red**, 0,1 g/l solution.

Dissolve 0,1 g of methyl red in water (5.1), make up the volume to 1 000 ml with water (5.1) and mix.

## 6 APPARATUS

Ordinary laboratory apparatus and

**6.1 Semi-micro apparatus for distillation without additional steam** (see figure 1) or

**6.2 Apparatus for distillation under a current of steam** (see figure 2).

**6.3 Spectrophotometer.**

NOTE — All glassware shall be cleaned prior to use in hot sulphuric-chromic acid prepared from pure ingredients and water (5.1).

## 7 SAMPLING

Sampling shall be carried out in accordance with ISO/R 377. For wrought steels not complying with ISO/R 377, the appropriate national standard shall be used.

## 8 PROCEDURE

NOTE — Carry out operations in a well-ventilated room away from all work on nitrogenous products.

### 8.1 Test portion

Weigh, to the nearest 0,001 g, masses of 1 g and 2 g respectively of the test sample, to be treated concurrently.

### 8.2 Blank test

The procedure specified in 8.3 and 8.4 eliminates the incidence of the value of the blank test when the same reagents are used with the two test portions indicated in 8.1.

### 8.3 Determination

#### 8.3.1 Preparation of the test solution

In a 150 ml Kjeldahl flask covered with a watch-glass, dissolve the test portion (8.1) with 30 ml of sulphuric acid solution (5.4). Allow to digest, taking care that the temperature of the liquid does not exceed 90 °C, until the release of hydrogen has definitely ceased.

When the release of hydrogen has ceased, remove the watch-glass and heat until white sulphuric fumes begin to appear.

Then add

- 5 ml of sulphuric acid (5.3) and
- 1 g of potassium sulphate (5.2).

Heat for 2 h at a temperature above 300 °C, in such a way that the mixture remains liquid. Cool, add 10 ml of water (5.1) and heat to dissolve the majority of the sulphates.

#### 8.3.2 Distillation

The distillation may be carried out with or without additional steam.

NOTE — The flasks used in distillation are attacked by the sodium hydroxide solution; change them frequently.

#### 8.3.2.1 DISTILLATION WITHOUT ADDITIONAL STEAM

Use the apparatus shown in figure 1 (6.1).

To collect the distillate, transfer 5 ml of sulphuric acid solution (5.6) to a 100 ml volumetric flask with a ground neck and having a mark at 85 ml. Introduce the tapered tube extension of the condenser into the flask in such a manner that it is immersed in the sulphuric acid solution (5.6).

Pass the test solution (8.3.1) quantitatively into the distillation flask, rinsing with 60 ml of water (5.1), add 50 ml of sodium hydroxide solution (5.5) and rinse the neck of the flask with 30 ml of water (5.1). The final volume of the solution should be approximately 160 to 165 ml. Moisten the ground neck and connect the flask

to the condenser immediately after the addition of the sodium hydroxide solution (5.5).

Now begin the distillation. Distil about 80 ml in 25 min. When the distillation is ended, rinse the immersed tube with water (5.1), collecting the washings in the volumetric flask; make up to volume with water (5.1) and mix. Solutions  $S_1$  for the 1 g test portion and  $S_2$  for the 2 g test portion are obtained. Repeat the same operation (8.3.2.1) for each sample to be analysed, taking care, after each distillation, to rinse the flask with plenty of water, then distilled water and finally the water (5.1).

NOTE — To regulate the boiling during the distillation in the apparatus shown in figure 1, it is as well to add some pieces of porous ceramic. These pieces are previously treated as a test sample and collected up after distillation. They are then washed with sulphuric acid solution (5.6) until neutral, then with water (5.1) and finally dried.

### 8.3.2.2 DISTILLATION UNDER A CURRENT OF STEAM

Use the apparatus shown in figure 2 (6.2).

To collect the distillate, transfer 5 ml of sulphuric acid (5.7) to a beaker of suitable capacity, introduce the tapered tube extension of the condenser into this beaker which has a mark at 85 ml, in such a manner that it is immersed in the 5 ml of sulphuric acid solution (5.7). Pass the test solution (8.3.1) quantitatively into the distillation flask with the aid of the funnel.

Rinse the Kjeldahl flask with 60 ml of water (5.1), add through the funnel 50 ml of sodium hydroxide solution (5.5) and rinse the funnel with 30 ml of water (5.1). The volume of the solution should then be about 160 to 165 ml. The steam generator should be preheated to allow the distillation to commence immediately the sodium hydroxide is introduced.

Distil about 80 ml in 25 min. When the distillation is ended, rinse the immersed tube with water (5.1), collecting the washings in the beaker. Transfer the solution quantitatively to a 100 ml one-mark volumetric flask, make up to volume with water (5.1) and mix. Solutions  $S_1$  for the 1 g test portion and  $S_2$  for the 2 g test portion are obtained. Interrupt the heating of the steam generator and allow to cool; the liquid in the flask syphons into the empty flask. Repeat the same operation for each sample to be analysed.

### 8.3.3 Development of the colour

According to the presumed nitrogen content, take the following aliquots of solutions  $S_1$  and  $S_2$  :

- 10,0 ml for nitrogen contents between 0,020 and 0,050 % (m/m)
- 25,0 ml for nitrogen contents between 0,010 and 0,020 % (m/m)
- 50,0 ml for nitrogen contents between 0,002 and 0,010 % (m/m)

and transfer them respectively into two 100 ml volumetric flasks.

Make up to 50 ml with water (5.1) those volumes less than 50 ml. Add 1 drop of methyl red solution (5.15) and neutralize exactly with sodium hydroxide solution (5.8).

Add with a pipette and in the following order :

- 5,0 ml of sodium phenate solution (5.9)
- 5,0 ml of disodium hydrogen phosphate solution (5.10)
- 10,0 ml of sodium pentacyanonitrosylferrate(II) solution (5.11)
- 5,0 ml of sodium hypochlorite solution (5.12).

Make up the volume to 100 ml with water (5.1) and agitate the flasks in an identical manner by alternately turning them upside down (at least ten times).

Allow the colour to develop in the dark for 1 h at ambient temperature.

NOTE — The aliquots indicated are such that in relation to the nitrogen contents, the quantity of nitrogen in the 100 ml flask used for the spectrophotometric measurement is always between 10 and 50  $\mu\text{g}$  for  $S_1$  and 20 and 100  $\mu\text{g}$  for  $S_2$  : thus, the difference is between 10 and 50  $\mu\text{g}$ .

### 8.3.4 Spectrophotometric measurement

Homogenize the coloured solutions  $S_1$  and  $S_2$  and measure the absorbance of solution  $S_2$  in a 1 cm cell, using the spectrophotometer (6.3) at a wavelength corresponding to the maximum absorption — a maximum which is situated — at about 640 nm — after having adjusted the apparatus to zero absorbance in relation to solution  $S_1$ .

## 8.4 Plotting of the calibration curve

### 8.4.1 Preparation of the standard solutions, related to the spectrophotometric measurement carried out in a 1 cm cell

To a series of six 100 ml volumetric flasks, transfer the quantities of standard nitrogen solution (5.14) indicated in the following table.

Standard nitrogen solution (5.14)	Corresponding mass of nitrogen
ml	$\mu\text{g}$
0 *	0
5,0	10
10,0	20
15,0	30
20,0	40
25,0	50

\* Compensating solution.

Add to each flask 5 ml of sulphuric acid solution (5.7), then add the quantity of water (5.1) necessary to bring the volume to about 50 ml.

Then add 1 drop of methyl red solution (5.15), neutralize exactly with sodium hydroxide solution (5.8) and continue in accordance with the procedure specified in the third paragraph of 8.3.3.

#### 8.4.2 Spectrophotometric measurements

Homogenize the coloured solutions and proceed with the spectrophotometric measurements according to the procedure specified in 8.3.4, after having adjusted the apparatus (6.3) to zero absorbance in relation to the zero term (compensating solution).

#### 8.4.3 Plotting of the calibration graph or calculation of the angular coefficient of the straight line

The absorbance values measured and the masses, in micrograms, of nitrogen indicated permit a calibration graph to be plotted or the angular coefficient of the straight line to be calculated.

The angular coefficient  $a$  of this straight line represents the absorbance of 1  $\mu\text{g}$  of nitrogen in 100 ml.

### 9 EXPRESSION OF RESULTS

The nitrogen (N) content is given, as a percentage by mass, by the formula

$$\frac{D}{a} \times \frac{100}{V} \times \frac{1}{10^6} \times \frac{100}{m}$$

$$= \frac{D}{100 \times a \times V \times m}$$

where

$D$  is the absorbance of the coloured solution corresponding to the 2 g test portion adjusted for the zero of the apparatus in relation to the coloured solution corresponding to the 1 g test portion;

$a$  is the angular coefficient, in reciprocal micrograms, of the straight line established in 8.4.3, relating to an optical path length of 1 cm;

$V$  is the volume, in millilitres, of the aliquots of solutions  $S_1$  and  $S_2$  taken for the coloured reactions;

$m$  is the difference in mass, expressed in grams, between the 1 g and 2 g test portions.

### 10 TEST REPORT

The test report shall include the following particulars :

- the method of analysis used, by reference to this International Standard;
- the results obtained, as well as the form in which they are expressed;
- any particular details which may have been noted during the determination;
- any operations not specified in this International Standard or any optional operations which could have had an influence on the result.

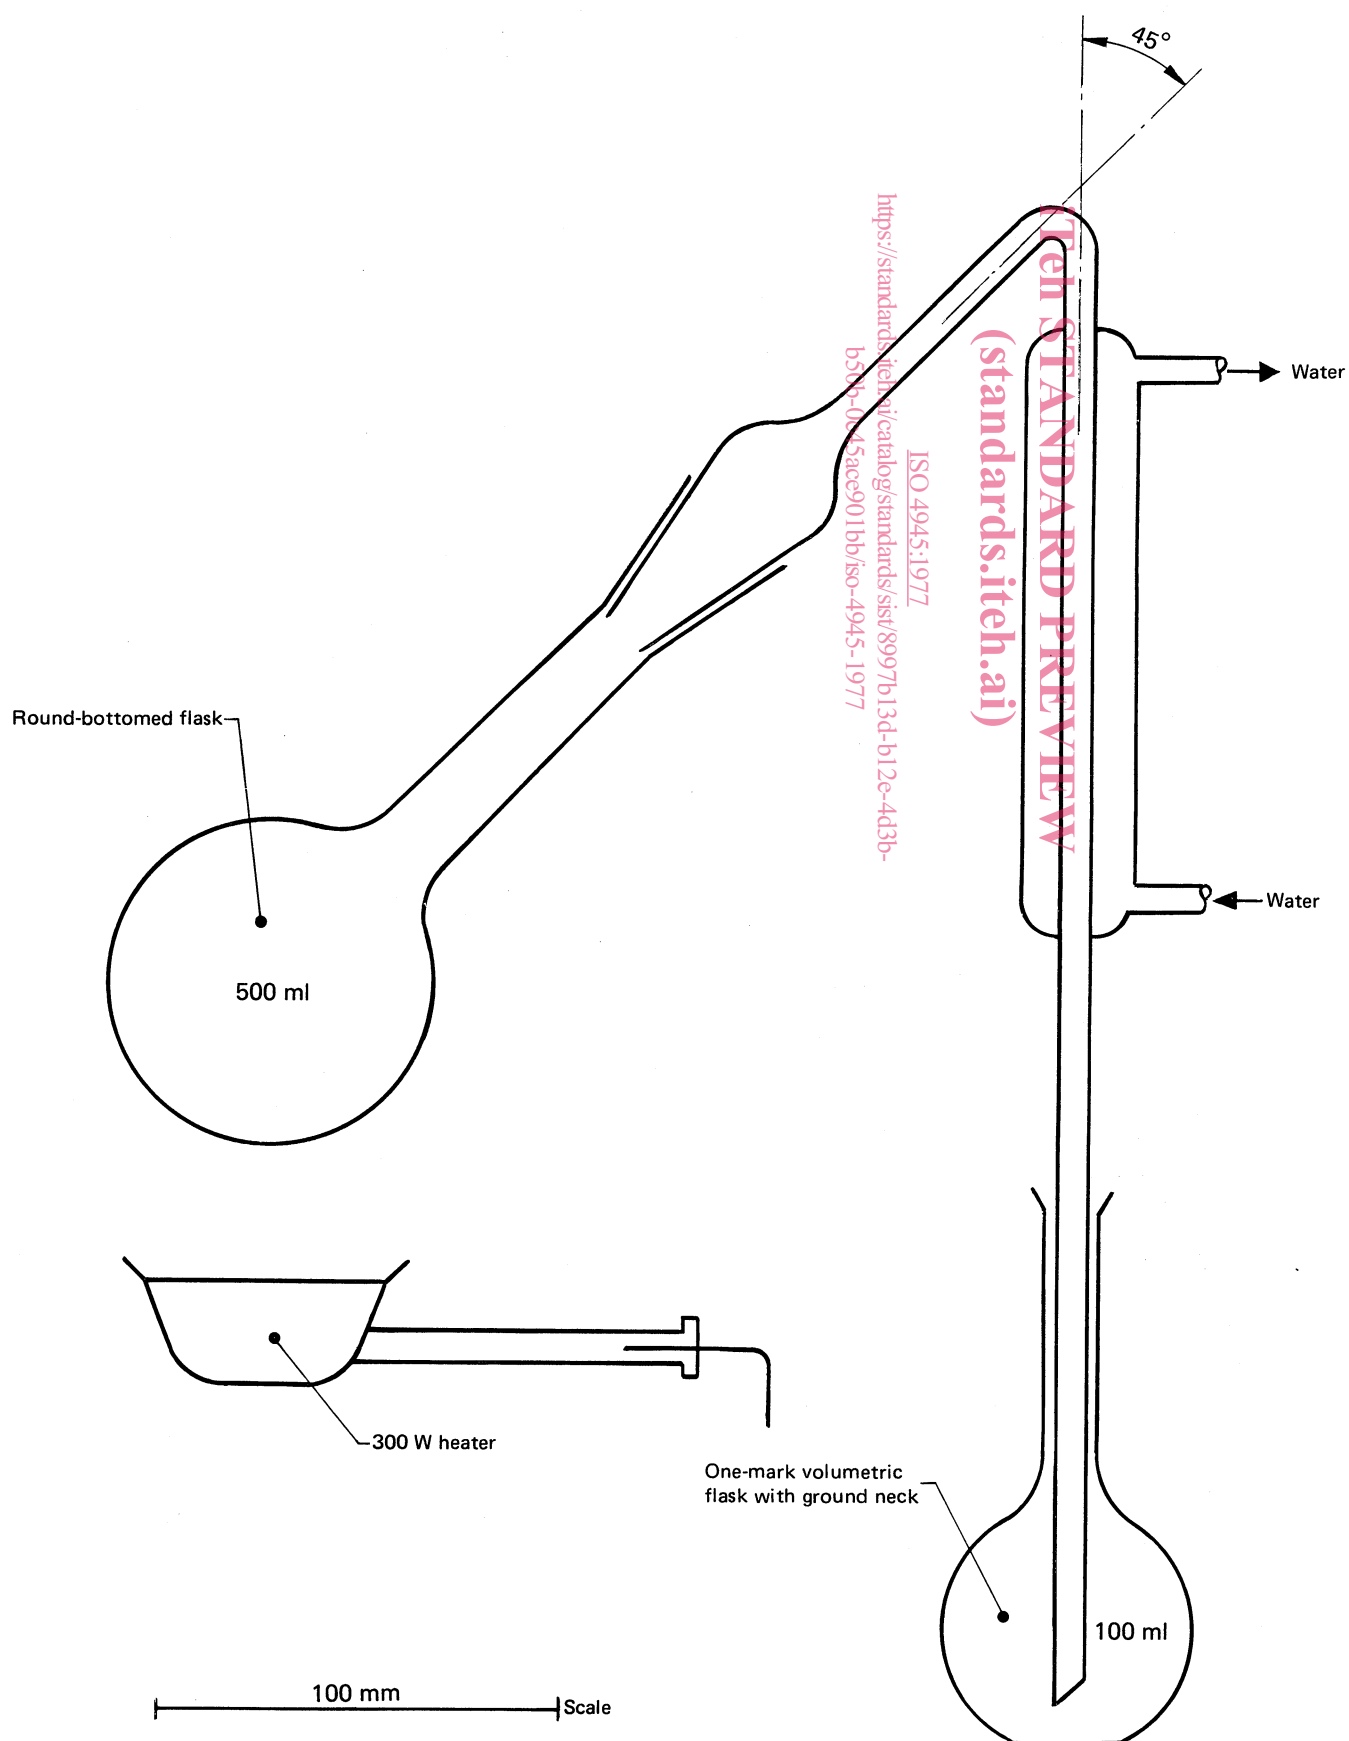


FIGURE 1 — Semi-micro distillation apparatus  
(Method of heating given as example)

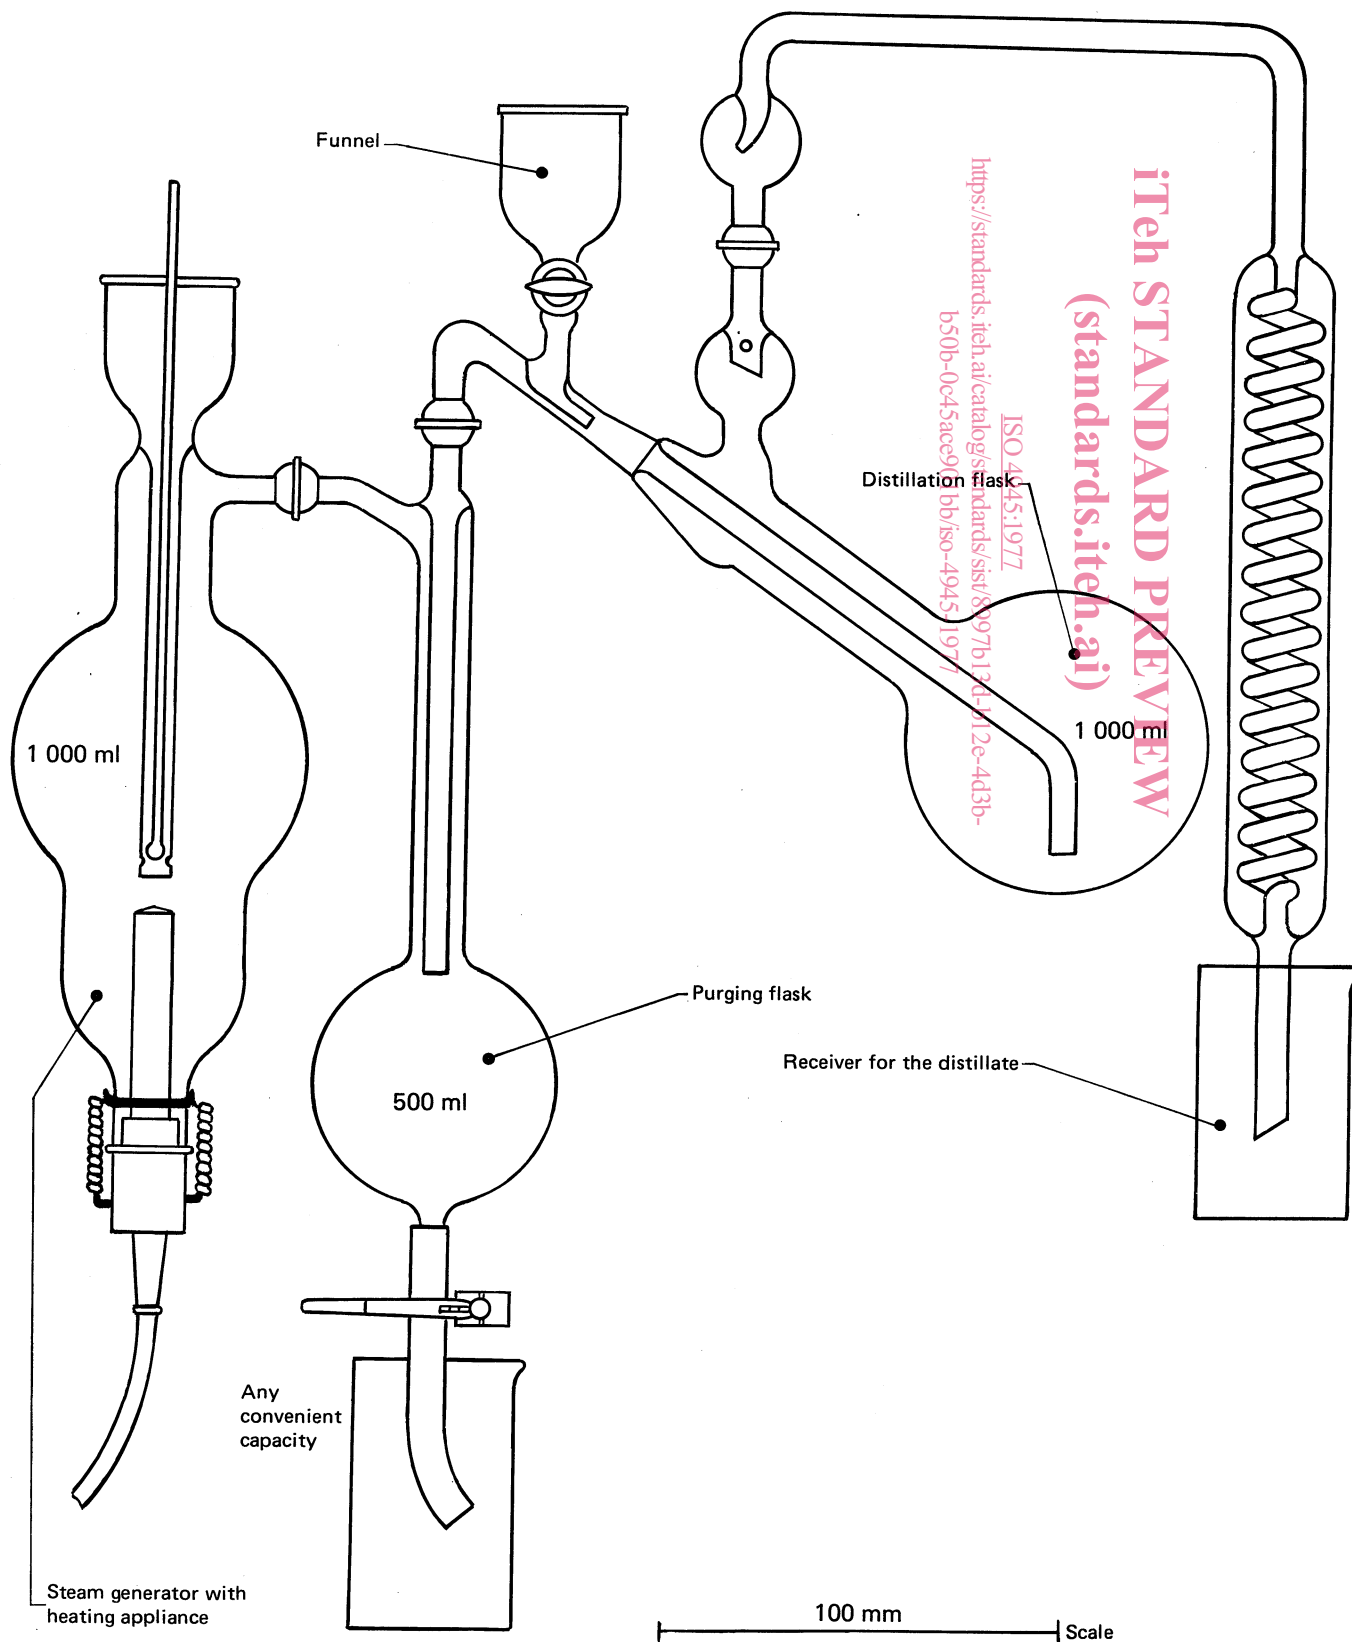


FIGURE 2 — Apparatus for distillation under a current of steam