



## Designation: E2251 – 14 (Reapproved 2021)

# Standard Specification for Liquid-in-Glass ASTM Thermometers with Low-Hazard Precision Liquids<sup>1</sup>

This standard is issued under the fixed designation E2251; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon ( $\epsilon$ ) indicates an editorial change since the last revision or reapproval.

## 1. Scope

1.1 The purpose of this standard is to specify liquid-in-glass ASTM thermometers using low hazard thermometric liquids defined in this standard.

1.2 This standard specifies liquid-in-glass thermometers graduated in degrees Celsius or degrees Fahrenheit that are frequently identified and used in methods under the jurisdiction of the various technical committees within ASTM. The current approved thermometers are listed in [Table 1](#).

1.3 The technical requirements for the thermometric liquids used in the thermometers in [Table 1](#) are specified in [Annex A1](#). Tests for conformity to the technical requirements are also found in [Annex A1](#).

NOTE 1—It has been found by experience that ASTM Thermometers, although developed in general for specific tests, may also be found suitable for other applications, thus precluding the need for new thermometer specifications differing in only minor features. However, it is suggested that technical committees contact E20.05 before choosing a currently designated thermometer for a new method to be sure the thermometer will be suitable for the intended application.

1.4 For full rationale, see [Appendix X1](#).

*1.5 This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety, health, and environmental practices and determine the applicability of regulatory limitations prior to use.*

*1.6 This international standard was developed in accordance with internationally recognized principles on standardization established in the Decision on Principles for the Development of International Standards, Guides and Recommendations issued by the World Trade Organization Technical Barriers to Trade (TBT) Committee.*

<sup>1</sup> This specification is under the jurisdiction of ASTM Committee E20 on Temperature Measurement and is the direct responsibility of Subcommittee E20.05 on Liquid-in-Glass Thermometers and Hydrometers.

Current edition approved Dec. 1, 2021. Published December 2021. Originally approved in 2003. Last previous edition approved in 2014 as E2251 – 14. DOI: 10.1520/E2251-14R21.

## 2. Referenced Documents

2.1 *ASTM Standards:*<sup>2</sup>

E1 Specification for ASTM Liquid-in-Glass Thermometers  
E77 Test Method for Inspection and Verification of Thermometers

E344 Terminology Relating to Thermometry and Hydrometry

E563 Practice for Preparation and Use of an Ice-Point Bath as a Reference Temperature

## 3. Terminology

3.1 *Definitions*—The definitions given in Terminology [E344](#) apply.

3.2 *Definitions of Terms Specific to This Standard:*

3.2.1 *bulb length, n*—the distance from the bottom of the bulb to the junction of the bulb and the stem tubing.

3.2.2 *contraction chamber, n*—an enlargement of the capillary, located below the main scale or between the main scale and the auxiliary scale, that serves to reduce the scale length or to prevent contraction of all the liquid column into the bulb.

3.2.3 *diameter, n*—the largest outside dimension of the glass tubing as measured with a ring gage.

3.2.4 *expansion chamber, n*—an enlargement at the top of the capillary to provide protection against breakage caused by excessive gas pressure.

3.2.5 *faden thermometer, n*—a thermometer with a long, thin bulb used to determine emergent stem temperatures.

3.2.6 *interval error, n*—the deviation of the nominal value of a temperature interval from its true value; either for the total range (total interval) or for a part of the range (partial interval).

3.2.7 *low-hazard liquid, n*—a liquid that is biodegradable, non-hazardous and considered non-toxic in thermometer quantities.

<sup>2</sup> For referenced ASTM standards, visit the ASTM website, [www.astm.org](http://www.astm.org), or contact ASTM Customer Service at [service@astm.org](mailto:service@astm.org). For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.



NOTE 2—It is the responsibility of the manufacturer to determine the suitability of a liquid for this standard. In marking the thermometer with the ASTM designation the manufacturer is confirming that the liquid in the thermometer is non-hazardous as defined by current OSHA (Occupational Safety and Health Administration) standards and non-toxic in thermometer quantities per current definitions of the United States Environmental Protection Agency.

3.2.8 *thermometric liquid, n*—the liquid in a liquid-in-glass thermometer that indicates the value of temperature.

3.2.9 *top of the thermometer, n*—the top of the finished instrument.

3.2.10 *total length, n*—overall length of the finished instrument.

3.3 Other terms may be found in the Terminology sections of Specification E1 and Test Method E77.

## 4. Specifications

4.1 The individual thermometers shall conform to the detailed specifications given in Table 1, the general requirements specified in Sections 5 – 15, and Annex A1 and Annex A2.

NOTE 3—Thermometers manufactured to previous revisions of this standard shall retain the same ASTM status as those meeting current specifications.

NOTE 4—The encapsulation (jacketing) of the glass of liquid-in-glass thermometers with polyflourinated hydrocarbons will change their performance and physical characteristics, including, but not limited to, response time, accuracy, and physical dimensions. Therefore, under no circumstances should an encapsulated or otherwise modified ASTM thermometer be used in performing tests that specify the use of an ASTM thermometer.

## 5. Type

5.1 Each thermometer in Table 1 shall be of the liquid-in-glass type filled with a low hazard thermometric liquid that meets the specifications in Annex A1. The gas filling above the liquid shall be nitrogen or other suitable inert gas. The filling gas shall be chosen to have very low solubility in the thermometric fluid.

## 6. Stem

6.1 *Stem*—The stem shall be made of suitable thermometer tubing and shall have a plain front and enamel back.

6.2 *Top Finish*—The top of all thermometers specified in Table 1 shall have a plain rounded finish, except the following, which shall have the top finish indicated below. Any special top finish shall be included in the total length of the thermometer.

### 6.2.1 *Special Finish:*

6.2.1.1 Any finish suitable for assembly in a standard 304.8-mm (12-in.) non-sparking metal armor with open face; in a cup case assembly; or in a flushing case assembly as defined in standards the thermometers are used in:

Thermometers S58C, S58F, S59C, S59F, S130C, S130F

## 7. Bulb

7.1 The bulb shall be made of glass having a viscosity of at least  $10^{14.6}$  poises at 490°C (914°F) and at least  $10^{13.4}$  poises at 520°C (968°F).

NOTE 5—Thermometers made with bulb glasses having properties close to these minimum requirements should not be subjected to temperatures above 405°C (760°F) or be continuously exposed to temperatures above 370°C (700°F).

## 8. Capillary Clearances

8.1 The following distances between graduations and the bulb, and between graduations and enlargements in the capillary, are minimum limits acceptable for thermometers in this standard.

NOTE 6—In order for a thermometer to be usable over its entire graduated range, graduation marks must not be placed too close to any enlargement in the capillary. Insufficient immersion of the thermometric liquid in the main bulb or capillary enlargement, graduation marks placed over parts of the capillary that have been changed by manufacturing operations, or graduations so close to the top of the thermometer that excessive gas pressure results when the thermometric liquid is raised to this level, may lead to appreciable errors.

8.1.1 A 13-mm length of unchanged capillary between the bulb and the immersion line or lowest graduation, if the graduation is not above 100°C (212°F); a 30-mm length if the graduation is above 100°C (212°F).

8.1.2 A 5-mm length of unchanged capillary between an enlargement and the graduation next below, except at the top of the thermometer.

8.1.3 A 10-mm length of unchanged capillary between an enlargement, other than the bulb, and the immersion line or the graduation next above, if the graduation is not above 100°C (212°F); a 30-mm length if the graduation is above 100°C (212°F).

8.1.4 A 10-mm length of unchanged capillary above the highest graduation, if there is an expansion chamber at the top of the thermometer; a 30-mm length if there is no expansion chamber. For the purposes of this requirement, “an expansion chamber” is interpreted as an enlargement at the top end of the capillary bore that shall have a capacity equivalent to not less than 20 mm of unchanged capillary.

8.2 Due to a change in the methods used for scale placement, it is possible to manufacture thermometers that comply with the specifications given in Table 1, but not meet the requirements for capillary clearances given above. In any case, the distances given in this section are the governing factor. Under no circumstances shall the scales on thermometers be placed closer than these minimum distances.

## 9. Graduations and Inscriptions

9.1 All graduation lines, figures, and letters shall be clearly defined, suitably colored, and permanent. The width and the sharpness of the graduation lines shall be designed in accordance with necessary space between the graduations and the desired accuracy of interpolation. The middle of the graduation line shall be accurately determinable.

9.1.1 A suitably etched thermometer with the etched lines and figures filled with a suitable colorant shall be considered permanently marked provided it passes the test for permanency of pigment in Specification E1.

9.2 *Graduation Lines*—All graduation lines shall be straight, of uniform width, and perpendicular to the axis of the thermometer. The width of the graduation lines shall be as follows:

9.2.1 *Group 1*—Maximum line width 0.10 mm; for thermometers that may read to fractions of a division, often with magnifying aids:

Thermometers S56C, S56F, S62C, S62F, S63C, S63F, S64C, S64F, S65C, S65F, S66C, S66F, S67C, S67F, S91C, S116C, S117C, S120C

9.2.2 *Group 2*—Maximum line width 0.15 mm; for thermometers that may be read to the nearest half division or where the congestion of scale dictates the use of a scale to moderate fineness:

Thermometers S5C, S5F, S12C, S12F, S15C, S15F, S18C, S18F, S22C, S22F

9.2.3 *Group 3*—Maximum line width 0.20 mm; for thermometers with more open scales, usually read to the nearest division, often times under adverse conditions where a bold graduation is therefore desired:

Thermometers S58C, S58F, S59C, S59F, S130C, S130F

9.3 *Immersion Line*—On partial immersion thermometers an immersion line shall be permanently marked on the front of the thermometer at the distance above the bottom of the bulb as specified in **Table 1** within a tolerance of  $\pm 0.5$  mm. The immersion inscription shall be written in capital letters and abbreviated (for example, 76 mm immersion shall be written 76 MM IMM.)

9.4 *Terminal Numbers*—The terminal number shall be in full when there are one or more numbered graduations between it and the next full number. This rule need not necessarily be followed for:

#### 9.4.1 Precision Thermometers:

S65F, S66F, S67C, and S67F

9.5 *Scale Below Zero*—When a scale extends both above and below 0°C or 0°F, the two parts of the scale shall be differentiated by some means. Examples of suitable means are:

9.5.1 Different colorants for the graduations for the two parts of the scale,

9.5.2 Different style of numerical characters for the two parts of the scale, and

9.5.3 Use of minus signs before appropriate numbers below 0°C or 0°F.

### 10. Special Inscription

10.1 The special inscription specified in **Table 1** shall be marked on the thermometer in capital letters and Arabic numbers without the use of periods. Include year of current revision in the ASTM designation (for example ASTM S56C-03).

10.1.1 Each thermometer shall be permanently marked with a unique serial number and the manufacturer's tradename or mark.

10.1.2 Each thermometer shall have the average coefficient of thermal expansion of the liquid permanently marked.

10.1.3 When the length of the thermometer permits, the words "TOTAL IMMERSION" may also be inscribed on the back of thermometers calibrated for total immersion.

### 11. Permanency of Pigment

11.1 The test for permanency of pigment shall be performed on any convenient portion of the scale section of the thermometer. The pigment shall not chalk, burn out, or loosen as a result of this test (see Specification **E1**).

## 12. Bulb Stability

12.1 No test for bulb stability is necessary for any thermometers currently in this standard. However, should there be in the future, the bulb stability test as found in Specification **E1** shall be used.

## 13. Scale Error

13.1 Thermometers shall be verified and calibrated at the temperatures specified in **Table 4**. Partial immersion thermometers shall be calibrated for the emergent stem temperatures specified in **Table 4** using faden thermometers.

13.1.1 At the time of purchase, the scale errors must be within the maximum scale error found in **Table 1**. The indications of many high temperature and fractionally graduated thermometers may change with time and continued use, due to minute changes in bulb volume. Periodic verification of these thermometers either over the entire scale or reverification at the reference temperature (ice point or steam point), in accordance with procedures set forth in Test Method **E77**, is recommended.

13.2 Due to the application requirements for range and construction of the following thermometer(s) do not have reference points such as ice and steam points:

S91C

## 14. Case and Instructions

14.1 Each thermometer shall be supplied in a suitable case on which shall appear the following marking (except when a transparent case is used): the letters "ASTM," the thermometer number (S59C, S59F, etc.), and the temperature range.

14.2 Each thermometer shall be supplied with suitable user instructions. See **Appendix X2** for Sample User Instructions.

## 15. Methods of Verification and Calibration

15.1 Thermometers shall be verified and calibrated at the specified immersion in accordance with Test Method **E77**. For partial immersion thermometers careful consideration to emergent stem temperatures shall be observed.

**TABLE 1 Specification for E2251 ASTM Thermometers**

All dimensions are in millimeters.

See Table 4 for Verification and Calibration Temperatures.

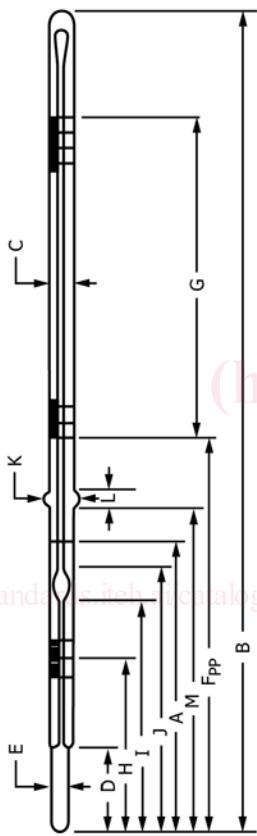


FIG. A. General Reference Figure for **Table 1**  
(Specific figures associated with individual thermometers are found at the end of **Table 1**)

*Explanatory Notes for Table 1 (numbers correspond to those found in **Table 1** of Specification **E1** whenever possible):*

- A* An expansion chamber is provided for relief of gas pressure to avoid distortion of the bulb at higher temperatures. It is not for the purpose of joining thermometric liquid separations and under no circumstances should the thermometer be heated above the highest temperature reading.
- e* The test temperatures shall be indicated by an arrow whether the graduation corresponding to that point is numbered or not.
- m* For kinematic viscosity thermometers, the ice-point reading shall be taken within 1 h after being at the test temperature for not less than 3 min. The ice-point reading shall be expressed to the nearest 0.01°C or 0.02°F and applied as explained in Test Method **E77**, Section 13.

*o* Capillary clearances must conform to Section **8**.

*y* Over any interval of 2°C the change in calibration correction shall not exceed 0.02°C.

*z* Over any interval of 4°F the change in calibration correction shall not exceed 0.05°F.

*AA* Special finish, see **6.2.1**.

*BB* The bulb diameter shall not be more than 0.5 mm greater than the stem.

*FF* For Fahrenheit thermometers, dimension G (length of graduated portion) shall be measured as the length of graduated portion corresponding to the nominal Celsius range.

*oo* Bulb length as necessary for the thermometric liquid and meeting capillary clearances found in Section **8**.

*PP* Distance "F" may be to top temperature for thermometers. See individual thermometer reference figure numbers.

*RR* Contraction chamber necessary for the thermometric liquid and conforming to capillary clearances found in Section **8**.



TABLE 1 Continued

IP No.	ASTM No.	S5C-11	S5F-11 <sup>FF</sup>	S12C-03	S12F-03 <sup>FF</sup>	S15C-11	S15F-11 <sup>FF</sup>	S18C-11	S18F-11 <sup>FF</sup>	S22C-11	S22F-11 <sup>FF</sup>
Name		Cloud and Pour	Density-Wide Range			Low Softening Point		Reid Vapor Point		Oxidation Stability	
Reference Fig. No.		5	2	-20 to 102°C	-5 to 215°F	-2 to +80°C	30 to +180°F	34 to +42°C	94 to +108°F	95 to 103°C	204 to 218°F
Range		-38 to 50°C	-36 to 120°F					37.8°C <sup>G</sup>	100°F <sup>G</sup>	98.9 and 100°C <sup>G</sup>	210°F <sup>G</sup>
For test at										TOTAL	
A Immersion, mm	108										
Graduations:											
Subdivisions		2°F	0.2°C	0.5°F	0.2°C	0.5°F	0.1°C	0.2°F	0.1°C	0.2°F	
Long lines at each		10°F	1°C	1°F	1°C	1°F	0.5°C	1°F	0.5°C	1°F	
Numbers at each		20°F	2°C	5°F	2°C	5°F	1°C	2°F	1°C	2°F	
Scale error, max	0.5°C	0.15°C	0.25°F	0.25°C	0.2°C	0.4°F	0.1°C	0.2°F	0.1°C	0.2°F	
Special inscription											
	ASTM		ASTM					ASTM		ASTM	
	S5C-11 or S5F-11		S12C-03 or S12F-03					S18C-11 or S18F-11		S22C-11 or S22F-11	
	108 MM IMM										
Expansion chamber:											
	70°C <sup>A</sup>	158°F <sup>A</sup>	130°C <sup>A</sup>	266°F <sup>A</sup>	100°C <sup>A</sup>	212°F <sup>A</sup>	70°C <sup>A</sup>	158°F <sup>A</sup>	125°C <sup>A</sup>	257°F <sup>A</sup>	
Permit heating to											
B Total length, mm	254 to 264	435 to 445	395 to 400	395 to 400			295 to 305	295 to 305			
C Stem OD, mm	6.0 to 7.0	6.0 to 8.0	6.0 to 7.0	6.0 to 7.0			6.0 to 7.0	6.0 to 7.0			
D Bulb length, mm	OO	OO	OO	OO			OO	OO			
E Bulb OD, mm											
bulb size [ng]stem size											
not > stem											
Scale location:											
Bottom of bulb to line at											
F Distance, mm	50°C	120°F	102°C	215°F	80°C	180°F	42°C	108°F	103°C	218°F	
G Length of graduated portion, mm	195 to 205	370 to 385	370 to 385	328 to 343	328 to 343	245 to 276°	210 to 222	210 to 222	210 to 222	60 to 90°	
Ice-point scale:											
H Range											
I Bottom of bulb to ice-point, mm											
Contraction chamber:											
J Distance to bottom, min, mm											
K Distance to top, max, mm											
L Stem enlargement:											
M OD, mm											
N Length, mm											
O Distance to bottom, mm											

<sup>A</sup> An expansion chamber is provided for relief of gas pressure to avoid distortion of the bulb at higher temperatures. It is not for the purpose of joining thermometric liquid separations and under no circumstances should the thermometer be heated above the highest temperature reading.

<sup>G</sup> The test temperatures shall be indicated by an arrow whether the graduation corresponding to that point is numbered or not.

<sup>o</sup> Capillary clearances shall conform to Section 8.

<sup>FF</sup> For Fahrenheit thermometers, dimension G (length of graduated portion) shall be measured as the length of graduated portion corresponding to the nominal Celsius range.

<sup>OO</sup> Bulb length as necessary for the thermometric liquid and meeting capillary clearances found in Section 8.

<sup>RR</sup> Contraction chamber necessary for the thermometric liquid and conforming to capillary clearances found in Section 8.



TABLE 1 Continued

IP No.	ASTM No.	S56C-03	S56F-03 <sup>FF</sup>	S58C-11	S58F-11 <sup>FF</sup>	S59C-03	S59F-03 <sup>FF</sup>	S62C-03	S62F-03 <sup>FF</sup>	S63C-03	S63F-03 <sup>FF</sup>
Name Reference Fig. No. Range	Bomb Calorimeter 4 19 to 35°C	66 to 95°F -34 to +49°C	66 to 95°F -30 to +120°F	Tank 2 <sup>AA</sup> 0 to 180°F -18 to 82°C	Tank 2 <sup>AA</sup> 0 to 180°F -18 to 82°C	TOTAL	TOTAL	TOTAL	Precision <sup>2</sup> -36 to 35°F -8 to 32°C	Precision <sup>2</sup> -38 to +2°C -8 to 32°C	Precision <sup>2</sup> -18 to 89°F
For test at											
A Immersion, mm		TOTAL									
Graduations:	0.02°C 0.1°C 0.2°C 0.10°C <sup>y</sup>	0.05°F 0.1 and 0.5°F 1°F 0.20°F <sup>z</sup>	0.5°C 1°C 5°C 0.3°C	1°F 5°F 10°F 0.5°F	0.5°C 1°C 5°C 0.3°C	1°F 5°F 10°F 0.5°F	0.1°C 0.5°C 1°C 0.1°C	0.1°C 0.5°C 2°F 0.1°C	0.2°F 1°F 2°F 0.1°C	0.1°C 0.5°C 1°C 0.1°C	0.2°F 1°F 2°F 0.2°F
Subdivisions: Long lines at each Numbers at each											
Scale error, max											
Special inscription	S56C-03 or S56F-03	ASTM	S58C-11 or S58F-11								
Expansion chamber:											
Permit heating to	45°C <sup>A</sup>	113°F <sup>A</sup>	100°C <sup>A</sup>	212°F <sup>A</sup>	100°C <sup>A</sup>	212°F <sup>A</sup>	100°C <sup>A</sup>	212°F <sup>A</sup>	55°C <sup>A</sup>	131°F <sup>A</sup>	55°C <sup>A</sup>
Total length, mm	610 to 622	300 to 305	300 to 305	300 to 305	300 to 305	300 to 305	300 to 305	300 to 305	401 to 411	401 to 411	401 to 411
Stem OD, mm	7.0 to 8.0 <sup>OO</sup>	6.0 to 7.0 <sup>OO</sup>	6.0 to 7.0 <sup>OO</sup>	6.0 to 7.0 <sup>OO</sup>	6.0 to 7.0 <sup>OO</sup>	6.0 to 7.0 <sup>OO</sup>	6.0 to 7.0 <sup>OO</sup>	6.0 to 7.0 <sup>OO</sup>	7.0 to 8.0 <sup>OO</sup>	7.0 to 8.0 <sup>OO</sup>	7.0 to 8.0 <sup>OO</sup>
Bulb length, mm											
Bulb OD, mm											
Scale location:											
Bottom of bulb to line at	35°C	95°F	49°C <sup>E2</sup>	120°F	82°C	180°F	0°C	32°F	32°C	32°C	89°F
F Distance, mm											
G Length of graduated portion, mm	510 to 550	245 to 260	510 to 550	245 to 260	323 to 385°	165 to 195°	306 to 324	32°F	319 to 344	319 to 344	319 to 344
Ice-point scale:											
H Range											
I Bottom of bulb to ice- point, mm											
J Contraction chamber:											
K Distance to bottom, min, mm											
L Distance to top, max, mm											
M Stem enlargement:											
K OD, mm											
L Length, mm											
M Distance to bottom, mm											

<sup>A</sup> An expansion chamber is provided for relief of gas pressure to avoid distortion of the bulb at higher temperatures. It is not for the purpose of joining thermometric liquid separations and under no circumstances should the thermometer be heated above the highest temperature reading.  
<sup>B</sup> Capillary clearances shall conform to Section 8.  
<sup>y</sup> Over any interval of 2°C the change in calibration correction shall not exceed 0.02°C.  
<sup>z</sup> Over any interval of 4°F the change in calibration correction shall not exceed 0.05°F.  
<sup>AA</sup> Special finish, see 6.2.1.  
<sup>BB</sup> The bulb diameter shall not be more than 0.5 mm greater than the stem.  
<sup>FF</sup> For Fahrenheit thermometers, dimension G (length of graduated portion) shall be measured as the length of graduated portion corresponding to the nominal Celsius range.  
<sup>OO</sup> Bulb length as necessary for the thermometric liquid and meeting capillary clearances found in Section 8.



TABLE 1 Continued

IP No.	ASTM No.	S64C-03	S64F-03 <sup>FF</sup>	S65C-03	S65F-03 <sup>FF</sup>	S66C-03	S66F-03 <sup>FF</sup>	S67C-03	S67F-03 <sup>FF</sup>
Name			Precision 1		Precision 1		Precision 1		Precision 1
Reference Fig. No.		25 to 55°C	77 to 131°F	50 to 80°C	122 to 176°F	75 to 105°C	167 to 221°F	95 to 155°C	203 to 311°F
Range			TOTAL		TOTAL		TOTAL		TOTAL
For test at A									
Immersion, mm				0.1°C	0.2°F	0.1°C	0.2°F	0.2°C	0.5°F
Graduations:				0.5°C	1°F	0.5°C	1°F	1°C	1°F
Subdivisions				1°C	2°F	1°C	2°F	2°C	5°F
Long lines at each				0.1°C	0.2°F	0.1°C	0.2°F	0.2°C	0.5°F
Numbers at each									
Scale error, max									
Special inscription									
Expansion chamber:									
Permit heating to									
B		75°C <sup>A</sup>	167°F <sup>A</sup>	100°C <sup>A</sup>	212°F <sup>A</sup>	125°C <sup>A</sup>	257°F <sup>A</sup>	180°C <sup>A</sup>	355°F <sup>A</sup>
Total length, mm		401 to 411		401 to 411		401 to 411		401 to 411	
C		7.0 to 8.0		7.0 to 8.0		7.0 to 8.0		7.0 to 8.0	
Stem OD, mm		○○		○○		○○		○○	
D									
Bulb OD, mm									
E									
Scale location:									
Bottom of bulb to line at									
F		25°C	77°F	50°C	115 to 135	75°C	115 to 135	95°C	115 to 135
Distance, mm		115 to 135		115 to 135		115 to 135		115 to 135	
G		189 to 229°		189 to 229°		189 to 229°		189 to 229°	
Length of graduated portion, mm									
Ice-point scale:									
H		-0.5 to 0.5°C <sup>O</sup>	31 to 33°F <sup>O</sup>	-0.5 to 0.5°C <sup>O</sup>	31 to 33°F <sup>O</sup>	-0.5 to 0.5°C <sup>O</sup>	31 to 33°F <sup>O</sup>	-1 to +1°C <sup>O</sup>	30 to 34°F <sup>O</sup>
Bottom of bulb to ice-point, mm									
I								○	○
Contraction chamber:									
J								102	102
Distance to bottom, min, mm									
K									
L									
M									
Distance to bottom, mm									

<sup>A</sup> An expansion chamber is provided for relief of gas pressure to avoid distortion of the bulb at higher temperatures. It is not for the purpose of joining thermometric liquid separations and under no circumstances should the thermometer be heated above the highest temperature reading.

<sup>O</sup> Capillary clearances shall conform to Section 8.

<sup>FF</sup> For Fahrenheit thermometers, dimension G (length of graduated portion) shall be measured as the length of graduated portion corresponding to the nominal Celsius range.

<sup>○○</sup> Bulb length as necessary for the thermometric liquid and meeting capillary clearances found in Section 8.