



Designation: E1856 – 13 (Reapproved 2021)

# Standard Guide for Evaluating Computerized Data Acquisition Systems Used to Acquire Data from Universal Testing Machines<sup>1</sup>

This standard is issued under the fixed designation E1856; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon ( $\epsilon$ ) indicates an editorial change since the last revision or reapproval.

## 1. Scope\*

1.1 This guide is intended to assist the user in the evaluation and documentation of computerized data acquisition systems used to acquire data from quasi-static tests, performed on universal testing machines. The report produced will aid in the correct use and calibration of the computerized universal testing machine.

1.2 The values stated in SI units are to be regarded as standard. No other units of measurement are included in this standard.

1.3 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety, health, and environmental practices and determine the applicability of regulatory limitations prior to use.*

1.4 *This international standard was developed in accordance with internationally recognized principles on standardization established in the Decision on Principles for the Development of International Standards, Guides and Recommendations issued by the World Trade Organization Technical Barriers to Trade (TBT) Committee.*

## 2. Referenced Documents

2.1 *ASTM Standards:*<sup>2</sup>

[E4 Practices for Force Calibration and Verification of Testing Machines](#)

[E6 Terminology Relating to Methods of Mechanical Testing](#)  
[E8/E8M Test Methods for Tension Testing of Metallic Materials](#)

[E74 Practices for Calibration and Verification for Force-Measuring Instruments](#)

[E83 Practice for Verification and Classification of Extensometer Systems](#)

[E691 Practice for Conducting an Interlaboratory Study to Determine the Precision of a Test Method](#)

[E1012 Practice for Verification of Testing Frame and Specimen Alignment Under Tensile and Compressive Axial Force Application](#)

## 3. Terminology

3.1 The definitions of mechanical testing terms that appear in Terminology [E6](#) apply to this guide.

3.2 *Definitions:*

3.2.1 *resolution, n*—for a particular measurement device, the smallest change in the quantity being measured that causes a perceptible change in the corresponding indication.

3.2.1.1 *Discussion*—Resolution may depend on the value (magnitude) of the quantity being measured.

3.2.1.2 *Discussion*—For paper charts or analog indicators, the resolution should not be assumed to be better (smaller) than  $1/10$  of the spacing between graduations. For digital devices, the best resolution potentially achievable is the smallest difference between two different readings given by the display.

3.2.1.3 *Discussion*—For both analog and digital devices, the actual resolution can be significantly poorer than described above, due to factors such as noise, friction, etc.

3.3 *Definitions of Terms Specific to This Standard:*

3.3.1 *basic data, n*—the digital equivalents of analog counterparts, such as force and displacement measurements, which under static conditions are traceable to national standards (see [Fig. 1](#)).

3.3.2 *computerized data acquisition system*—a device that collects basic data from a universal testing machine during a test and calculates and presents derived data based on the basic data collected.

3.3.3 *derived data, n*—additional numbers derived from the basic data through computation using software algorithms, such as a peak force or a modulus value.

3.3.4 *data acquisition rate, n*—the rate at which digital samples of each wave-form (that is, force, strain, displacement, and so forth) are acquired, expressed in samples/second.

3.3.5 *transducer-channel bandwidth*—the frequency at which the amplitude response of a transducer channel has

<sup>1</sup> This guide is under the jurisdiction of ASTM Committee [E28](#) on Mechanical Testing and is the direct responsibility of Subcommittee [E28.15](#) on Automated Testing.

Current edition approved Nov. 1, 2021. Published December 2021. Originally approved in 1997. Last previous edition approved in 2013 as E1856–13. DOI: 10.1520/E1856-13R21.

<sup>2</sup> For referenced ASTM standards, visit the ASTM website, [www.astm.org](http://www.astm.org), or contact ASTM Customer Service at [service@astm.org](mailto:service@astm.org). For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

\*A Summary of Changes section appears at the end of this standard

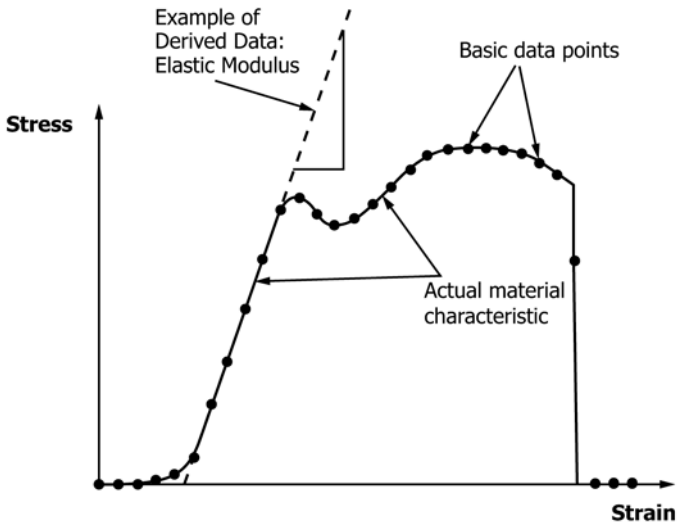


FIG. 1 Basic Data and Derived Data

those tested. Specimen types may be differentiated by material (strength level), size, shape, or test performed.

6.2 Use one of the following procedures to evaluate and document the conformity of the derived data.

6.2.1 Round Robin Procedure:

6.2.1.1 Perform a round robin involving at least two other universal testing machines. The other testing machines need not necessarily be computerized.

NOTE 1—It is preferable to use universal testing machines of varying types so that systemic problems are not masked.

6.2.1.2 If possible, configure the universal testing machines in such a way as to be able to obtain a graphic record of the tests. The graphic record may be generated by analog signal sources, the computerized data acquisition system, or may be generated manually from digital data recorded by the computerized data acquisition system.

6.2.1.3 Ascertain that all readout and recording devices have been calibrated in accordance with Practices E4, E83, or other applicable standards.

6.2.1.4 Test at least five specimens of each specimen type on each machine in conformance with the applicable test methods or established procedures.

NOTE 2—It may be desirable to test many more specimens after an initial screening, particularly if high standard deviations are observed on all machines.

6.2.1.5 Obtain the derived data from the computerized data acquisition system or graphic records of the tests from each machine, or both.

6.2.1.6 From the graphic records obtained, manually calculate the same test results obtained by the computerized data acquisition system.

6.2.1.7 Calculate the average and standard deviation of both the manually calculated results and the derived data obtained by the computerized data acquisition system(s) within each group of five or more specimens.

6.2.1.8 Investigate, identify, and correct, if necessary, the cause of any average results obtained by the computer that differ from the manually obtained average results, or the average results obtained by other testing machines, by more than 2.0 % of the average or more than one standard deviation, whichever is greater. In all cases, use the smallest non-zero standard deviation for evaluations.

6.2.1.9 Investigate, identify, and correct, if necessary, the cause of any standard deviations of the derived data obtained by the computerized data acquisition system that are more than two times the standard deviation obtained manually or by the other machines.

NOTE 3—Differences in averages and standard deviations of these magnitudes are quite often due to variations in the material being tested, and a complete statistical evaluation of the data using methods such as Practice E691 may be necessary.

6.2.2 Single Machine Procedure:

6.2.2.1 This procedure may be used for universal testing machines with the capability of producing graphic records from which derived data can be manually calculated.

6.2.2.2 Configure the testing machine in such a way as to be able to obtain a graphic record of the tests. The graphic record

fallen by 3 dB; that is, the measured signal is in error by about 30 % and the phase shift is 45° or greater.

3.3.5.1 Discussion—The precise amplitude and phase responses vary with the electrical design of the computerized data acquisition system, but the 3 dB bandwidth (expressed in hertz) is a simple single measure of responsiveness (see Fig. 2).

4. Summary of Guide

4.1 Comparative tests are performed to determine if the derived data acquired with a computerized universal testing machine agree with results acquired on the same machine from graphical records or with results acquired on other testing machines to ensure that the materials being tested are correctly characterized.

5. Significance and Use

5.1 This guide is recommended to be used by anyone acquiring data from a universal testing machine using a computerized data acquisition system.

6. Procedure

6.1 Choose at least five different test specimen types that are representative of the specimens commonly tested on the universal testing machine. If the universal testing machine is used to test fewer than five different specimen types, choose all

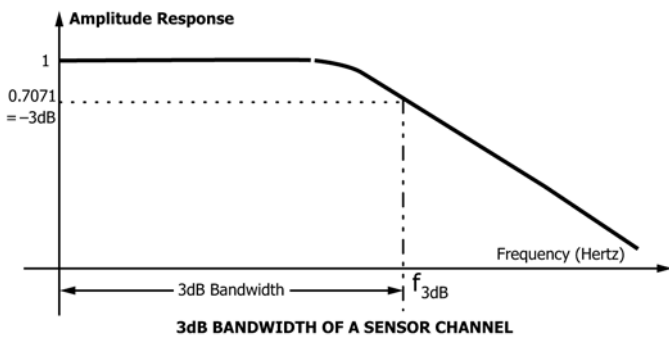


FIG. 2 Bandwidth

may be generated by analog signal sources, the computerized data acquisition system, or may be generated manually from digital data recorded by the computerized data acquisition system.

6.2.2.3 Ascertain that all readout and recording devices used (analog or digital, or both) have been calibrated in accordance with Practices E4, E83, or other applicable standards.

6.2.2.4 Ascertain that all transducers with their readout or recording devices, or both, including the devices producing the graphic record, have the required transducer-channel bandwidth for the tests performed with the machine (see Appendix X2).

6.2.2.5 Test at least five specimens of each specimen type in conformance with the applicable test methods or established procedures, obtaining both a graphic record and derived data from the computerized data acquisition system at the same time.

6.2.2.6 From the graphic record, determine the same test results as are calculated by the computerized data acquisition system.

6.2.2.7 Calculate the average and standard deviation of both the manually calculated results and the derived data obtained by the computerized data acquisition system (derived data) within each group of five specimens.

6.2.2.8 Investigate, identify, and correct, if necessary, the cause of any average derived data obtained by the computerized data acquisition system that differ from the manually obtained average results by more than 2.0 % of the average or more than one standard deviation, whichever is greater. In all cases, use the smallest non-zero standard deviation for evaluations.

6.2.2.9 Investigate, identify, and correct, if necessary, the cause of any standard deviations of the derived data obtained by the computerized data acquisition system that are more than two times the standard deviation of results obtained manually.

## 7. Test Result Evaluation

7.1 A bias in average results between machines or readouts may be due to one or more of the following:

7.1.1 *Calibration Differences*—A bias in all of the force results observed usually indicates a difference in calibration. If maximum forces disagree between the manual and computerized results, it may be due to differences in calibration between parts of the machine (see Appendix X1). If force results are in agreement and stress results vary, the difference may be due to cross-sectional area or other measurements such as span in a flexure test. If maximum force results agree and other force results differ, the difference is probably not due to differences in force calibration.

7.1.2 *Differences in the Speed of Testing*—Depending on the strain-rate sensitivity of the material being tested, a difference in derived data may be observed if there is a difference in the speed of testing. A simple way to check the speed of testing is to measure the elapsed time between two points during the tests.

7.1.3 *Incorrect Inputs to the Computer Algorithms*—If the results calculated by manual methods from the graphic record agree with the other universal testing machines but the derived

data from the computerized data acquisition system disagree, the difference may be due to incorrect inputs to the computer algorithms.

7.1.4 *Algorithms Used*—If the results calculated by manual methods from the graphic record agree with the other machines but the derived data from the computer disagree, the difference may be due to algorithms used by the computerized data acquisition system.

7.1.5 *Algorithms That Are Not Working Properly*—If the results calculated by manual methods from the graphic record agree with the other machines but the derived data from the computerized data acquisition system disagree, the difference may be due to algorithms that are not working properly.

7.1.6 *Ambiguity in the Interpretation of the Test Method*—The writer(s) of the algorithms used, or the user, or both, may be interpreting the test method differently or incorrectly.

7.1.7 *Differences in Gripping and Other Apparatus in Contact with the Specimen*—Differences in gripping and other apparatus in contact with the specimen may cause premature failure of the specimen or act as a heat sink and cause differences in elongation related results.

7.1.8 *Alignment of the Test Piece*—Poor alignment can cause lower-than-normal test results or poorly formed stress-strain curves, or both, in the elastic region of the curve (see Practice E1012).

7.1.9 Insufficient bandwidth in one or more of the transducer channels (see Appendix X2).

NOTE 4—Differences are just as likely to be due to problems with the manually calculated results as they are to problems with the computer generated derived data.

NOTE 5—For additional information, see the appendix on Factors Affecting Tension Test Results in Test Methods E8/E8M.

7.2 A difference in the standard deviation between machines may be due to one or more of the following:

7.2.1 *Differences in Resolution*—Poor resolution can show up in two forms. A standard deviation of zero may indicate poor resolution. Alternatively, if two or more discrete derived data occur with a difference between them that is large relative to the result being measured, poor resolution may be the cause. Example: 206, 206, 210, 206, 210 (see Appendix X3).

7.2.2 *Specimen Dimension Precision*—If derived-data force standard deviations agree and derived-data stress standard deviations differ, the difference is probably due to imprecise measurements of cross sectional area.

7.2.3 *Differences in the Speed of Testing*—Testing at speeds that are too fast may give either high or low standard deviations due to one or more of the transducer-channel bandwidths (see Appendix X2).

7.2.4 *Unstable Control of Test Speed*—Unstable control of the testing machine speed may increase the standard deviation of derived data in strain-rate sensitive materials and cause poorly formed stress-strain curves and measurement errors in extreme cases.

7.2.5 *Electrical Noise Being Picked Up By One or More of the Transducer Channels*—Electrical noise can cause computer algorithms to perform poorly. This may be observed in the graphic record or in the basic data. This problem may be

detected by capturing data at a fixed force or strain. The standard deviation of this data should be comparable to the resolution.

7.2.6 *Differences in Gripping and Other Apparatus in Contact with the Specimen*—Some devices in contact with the specimen may only cause an occasional premature failure. This will show up as a high standard deviation.

7.2.7 *Alignment of the Test Piece*—Poor alignment is often not repeatable and leads to high standard deviations (see Practice E1012).

7.2.8 Insufficient band width in one or more of the transducer channels (see Appendix X2).

## 8. Report

8.1 For each testing machine evaluated, report the following information:

- 8.1.1 Name of reporting agency,
- 8.1.2 Date of report,
- 8.1.3 Complete testing machine description(s) including the serial number(s) of the machine(s), and all instrumentation, and the location(s),
- 8.1.4 Software version(s) identification,
- 8.1.5 Graphic data and manually calculated test results, if available,
  - 8.1.5.1 Computer test report(s),
  - 8.1.5.2 Averages and standard deviations for each test result,

8.1.5.3 Tabulation of the differences observed, and

8.1.6 Name(s) of reporting personnel.

8.2 This report need only be performed once and need not be repeated unless changes are made to the system that would significantly affect the report.

8.2.1 Changes that can significantly affect the results of this report include, but are not limited to:

8.2.1.1 Replacement of any of the electronics in the system with a different type of electronics,

8.2.1.2 Software changes or modifications, and


8.2.1.3 Changes to the computer(s) in the system that affect the processor's speed.

## 9. Precision and Bias

9.1 The precision and bias of this guide for evaluating computerized data acquisition systems on universal testing machines is dependent upon the derived data being determined. Refer to the test method for the derived data being determined such as Test Method E8/E8M for the precision and bias of the derived data.

## 10. Keywords

10.1 algorithm; bandwidth; basic data; computer; data acquisition; data acquisition rate; derived data; resolution; universal testing machine

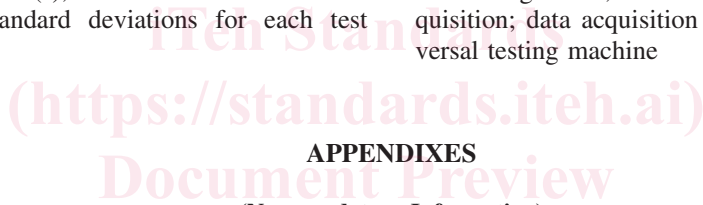

## APPENDIXES

(Nonmandatory Information)

### X1. CALIBRATION CONSIDERATIONS

X1.1 It is important to understand the way(s) in which information is transmitted within the testing system, so that the system is properly calibrated and verified. Information is transmitted either digitally or in an analog fashion between components within a testing system.

X1.1.1 An example of a digital transmission of data within a testing system is the transmission of test results from a computer to a printer. In some cases, a testing machine will digitally transmit force and other data to a computer.

X1.1.2 An example of an analog transmission of data is the electrical signal developed by a force cell that is transmitted to amplifiers in the testing machine, where the signal is converted into engineering units. Another example is a testing machine that transmits a DC voltage proportional to the applied force to an analog X-Y recorder.

X1.2 An analog to digital converter (A/D) converts analog signals to digital signals, and a digital to analog converter (DAC) converts digital signals to analog signals. In modern

testing machines, one or more of these devices are used. Calibration may be required at each point in a system where an A/D or a DAC is used in the transmission of data. The calibration may be on the analog, digital, or on both sides of the converter.

X1.3 In most cases, if devices receive digital signals from a calibrated digital device with no A/Ds or DACs in between (such as printers and monitors) the receiving devices will not require routine calibration and may be replaced without calibration.

X1.4 Determine from electrical schematics or obtain from the manufacturer a block diagram of the testing system that shows, as a minimum, all transducers used and all data output devices. Mark on the diagram all necessary calibration points. During routine verification of the testing machine, use this as a guide to ensure that the system has been verified at all of the necessary places.