



Designation: F3088 – 22

Standard Practice for Use of a Centrifugation Method to Quantify/Study Cell- Material Adhesive Interactions¹

This standard is issued under the fixed designation F3088; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

1. Scope

1.1 This practice covers a centrifugation cell adhesion assay that can be used to detect changes in adhesive characteristics of cells with passage or treatments. This approach measures the force required to detach cells from a substrate. Adhesion, among many variables, may vary due to changes in the phenotype of the cells.

1.2 This practice does not cover methods to verify the uniformity of coating of surfaces, nor does it cover methods for characterizing surfaces.

1.3 The cells may include adult, progenitor, or stem cells from any species. The types of cells may include chondrocytes, fibroblasts, osteoblast, islet cells, or other relevant adherent cell types.

1.4 This practice does not cover methods for isolating or harvesting of cells. This practice does not cover methods to quantitate changes in gene expression, or changes in biomarker type or concentration, as identified by immunostaining. Nor does this practice cover quantitative image analysis techniques.

1.5 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety, health, and environmental practices and determine the applicability of regulatory limitations prior to use.*

1.6 *This international standard was developed in accordance with internationally recognized principles on standardization established in the Decision on Principles for the Development of International Standards, Guides and Recommendations issued by the World Trade Organization Technical Barriers to Trade (TBT) Committee.*

¹ This practice is under the jurisdiction of ASTM Committee F04 on Medical and Surgical Materials and Devices and is the direct responsibility of Subcommittee F04.43 on Cells and Tissue Engineered Constructs for TEMPs.

Current edition approved April 1, 2022. Published May 2022. Originally approved in 2014. Last previous edition approved in 2014 as F3088 – 14. DOI: 10.1520/F3088-22.

2. Referenced Documents

2.1 *ASTM Standards:*²

F2603 Guide for Interpreting Images of Polymeric Tissue Scaffolds

F2664 Guide for Assessing the Attachment of Cells to Biomaterial Surfaces by Physical Methods

F2739 Guide for Quantifying Cell Viability and Related Attributes within Biomaterial Scaffolds

F2944 Practice for Automated Colony Forming Unit (CFU) Assays—Image Acquisition and Analysis Method for Enumerating and Characterizing Cells and Colonies in Culture

F2998 Guide for Using Fluorescence Microscopy to Quantify the Spread Area of Fixed Cells

F3294 Guide for Performing Quantitative Fluorescence Intensity Measurements in Cell-based Assays with Wide-field Epifluorescence Microscopy

3. Summary of Practice

3.1 *Centrifugation Cell Assay on Cell Populations*—A conventional centrifuge can be used to apply a normal or shear force to cells depending on the orientation of the cells with respect to the centrifugal force (**1-3**).³ The centrifugal force that the cells are subject to can be calculated according to the following formula assuming that the plates are 90° (normal) to the spindle of the centrifuge.

$$F_D = (p_{\text{cell}} - p_{\text{medium}})V_{\text{cell}}RCF \quad (1)$$

where:

F_D = detachment force applied per cell,
 V_{cell} = cell volume,

² For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

³ The boldface numbers in parentheses refer to the list of references at the end of this standard.

p_{cell} = density of the cell,
 p_{medium} = the density of the surrounding medium, and
 RCF = Relative Centrifugal Forces = $r\omega^2$, where r = centrifugation radius and ω = centrifugation speed.

See **X1.6** for example of a calculation of “detachment force per cell.”

3.1.1 Such tests are easy to conduct and the results represent a population average. The method can be performed in a moderately outfitted cell biology lab with an inverted microscope or a fluorescence microplate reader and a centrifuge with a microtiter plate holder. Three factors need to be considered when using this methodology: the potential influences of forces applied during the period of spin-up time, the maximum spin speed, and the test duration. The method is only able to correlate with cell detachment with the maximum force applied after the centrifuge has reached its set spin speed. It should also be considered that the maximum force that can be applied is limited by the centrifuge, sample configuration (that is, configuration and type of multi-well plate), and time of centrifugation. In some instances, the cell adhesion strength will be greater than the applied forces. Therefore, for certain cell types that have attached for extended periods of time, the method may not be able to generate forces sufficient to detach these cells.

3.1.2 Cell attachment is a complex, time-dependent process involving significant morphological and structural changes of the cell and deposition of a bed of extracellular matrix and is a function of cellular and substrate parameters. Cell adhesion to a surface depends on a range of biological factors that include culture history, species, the source and origin of the cells, embryological status of the cells (adult, progenitor, stem), histological types of cells (chondrocytes, fibroblasts, osteoblast, islet cells, etc.), purity, passage number, population doublings, and time after trypsinization. The adhesive strength also depends on the chemistry, surface chemistry/topography, and morphology of the underlying surface and adsorbed proteins or engineered ligands and, most importantly, time of adhesion.

4. Significance and Use

4.1 This practice describes a cell adhesion method that can be used to provide a detachment percent at a given RCF for cells that have adhered to a substrate, typically for a short time. The information generated by this practice can be used to obtain a semi-quantitative measurement of the adhesion of cells to either an uncoated or pre-coated substrate, when compared to a reference (adherent) cell type on the same substrate. As described in Reyes and Garcia (2003), it is recommended that the 50 % point be used for either ligand concentration or RCF for the most robust measurement of adhesion strength. The adhesion may vary due to changes in the phenotype of the cells or as a result of the specific properties of the surface. The substrate may include tissue culture-treated polystyrene, biomaterials, or bioactive surfaces. If the substrate is a hydrogel, care must be taken to avoid cohesive failure in the hydrogel (that is, detached cells have pulled away fragments of gel). The coating may consist of (but is not limited to) the following: natural or synthetic

biomaterials, hydrogels, components of extracellular matrix (ECM), ligands, adhesion or bioactive molecules, genes, or gene products. Cell concentration is also critical, as use of too high a concentration of cells may result in cells detaching as a sheet, rather than as individual cells. This centrifugation approach, once validated, may be applicable for quality control (QC) and product development. However, until the method is correlated to other measures of cell attachment, the current method should be run in parallel with other known measures of cell adhesion.

4.2 This practice does not cover methods to quantitate changes in gene expression, or changes in biomarkers, as identified by immunostaining. This practice additionally does not cover quantitative image analysis techniques. In some cases, the change in adhesive properties may reflect on the degree of differentiation or de-differentiation of the cells. However, it is worth noting that adhesive interactions do not necessarily reflect the differentiation state of a particular cell type, although in many instances they do. (See **X1.3** for application to the adhesion of chondrocytes.)

5. Interferences

NOTE 1—The following interferences may result in variable and inconsistent results from this method, and care should be taken to minimize these conditions.

5.1 Cell concentration too high in multi-wells. If the cell concentration is too high, then the cells may detach as a sheet, instead of as individual cells.

5.2 Cells not evenly distributed in wells (that is, clumping).

5.3 Inconsistency in the fluid level within multi-wells. Wells must be completely filled with fluid (4).

5.4 Inconsistency in well coating and blocking protocols. Where possible, a negative substrate control (that is, non-tissue culture-treated polystyrene, or similar control which has been shown to limit cell adhesion) should be included.

5.5 Inconsistency in pipetting forces when washing wells.

5.6 Air bubbles in well prior to, or forming during, centrifugation. The air bubbles can result from improper pipetting of fluid within the wells, or an improper fluid level in the wells prior to sealing the top of the wells with an adhesive cover (that is, “reverse meniscus” not formed in well prior to sealing with acetate sealing tape).

5.7 Incomplete washing of wells to remove loosely adherent or dead cells.

5.8 Crossover of fluorescent signal between adjacent wells in clear or translucent multi-well plates.

5.9 Centrifugation of multiple multi-well plates. A complex stress situation can result from spinning multiple multi-well plates (that is, stacking plates within a plate holder on the centrifuge), depending on the orientation of cells with respect to the centripetal force.

5.10 Photobleaching of fluorescence stain. Photobleaching may be reduced by limiting the exposure of the stained cells to room light or ultraviolet light.

5.11 Long cell adhesion times and variations in adhesive proteins. Use of long exposure times and/or specific ECM or protein may require adjustment of the protocol to optimize cell detachment conditions. Since detachment forces with this method are low, well spread, or strongly attached cells may not be detached by this method (5).

6. Apparatus

- 6.1 *Humidified CO₂ Incubator.*
- 6.2 *Rocker for Isolated Cells.*
- 6.3 *Hemocytometer.*
- 6.4 *Centrifuge.*
- 6.5 *Plate Adapters for Centrifuging Multi-Well Plates.*
- 6.6 *Multi-Well Pipetter.*
- 6.7 *Inverted Microscope, equipped with bright field/phase contrast, as well as fluorescence optics.*
- 6.8 *Microplate Reader.*
- 6.9 *Image Acquisition and Image Analysis Software (that is, Zeiss AxioVision Software, Image J, or equivalent).*

7. Reagents and Materials

- 7.1 *Cell Type, for adhesion assay, as well as control cell type (if applicable). A positive control cell type should consistently exhibit greater than 50 % adhesion on a given substrate, at a given RCF. Similarly, a negative control cell type should consistently exhibit less than 50 % adhesion on a given substrate at a given RCF.*
- 7.2 *Proteins, Extracellular Matrix Components, Genes or Gene Products or Biomaterials, for pre-coating wells of multi-well plates.*
- 7.3 *Medium, appropriate for either the cell type of interest or the control cell type, with or without the addition of antibiotic/antimycotic solution. Care should be taken to limit/avoid carryover of serum contents and adhesive proteins from media. Additionally, the trypsin protocol (trypsin concentration and trypsinization times) should be optimized.*
- 7.4 *Trypan Blue, or equivalent (cell viability).*
- 7.5 *Multi-Well Plates (96 well).*

7.6 *Dulbecco's Phosphate Buffered Saline (without calcium and magnesium), (D-PBS).*

7.7 *Fluorescence Stain.*

7.8 *Acetate Sealing Tape, or equivalent (to seal top of multi-well plate).*

7.9 *Aluminum Foil (to cover multi-well plate during incubation).*

8. Hazards

- 8.1 *Hoechst 33342 fluorescence stain (possible carcinogen).*
- 8.2 *Trypan blue dye (possible carcinogen).*

9. Calibration and Standardization

9.1 *Calibration of Image System*—Any inverted microscope system equipped with appropriate image capture device and image analysis software may be used for the assay. For the purposes of illustration in this standard, we refer to a Zeiss AxioVert inverted microscope equipped with an Axio Cam digital camera for image capture and AxioVision software for data collection/analysis.

9.1.1 Using an inverted microscope, 5 × 5 digital tiled images (tiled overlap 10 %, total tiled image area = 3.177 mm²) are captured for each of the three wells prior to centrifugation (pre-spin). Approximately 2400 to 3600 cells (800 to 1200 cells/well × 3 wells) are counted per sample.

10. Procedure

10.1 *Centrifugation Cell Adhesion Method*—A schematic of the method is shown in Fig. 1. The method was modified from the method of Reyes and Garcia (2003) (2).

10.1.1 Wells of a 96 multi-well plate are passively coated with protein or matrix protein. The coating concentration will depend on the ECM protein. The incubation time and incubation temperature (for example, room temperature versus 4 °C versus 37 °C) will vary with the substrate. In the example of fibronectin, the wells are passively coated for 30 min to 1 h at room temperature.

10.1.2 *Optimization of Multi-Well Plate Coating*—The following procedure is suggested to obtain the optimal well-coating concentration and time of incubation for the coating.

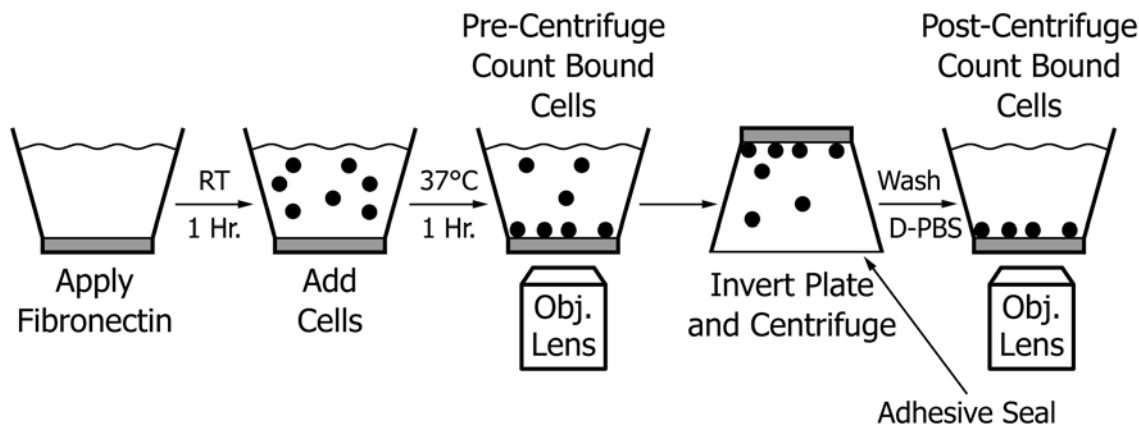


FIG. 1 Schematic of Centrifugation Cell Adhesion Assay

First, a series of test runs of the method should be performed where a broad concentration range (including a no-coating, zero concentration, control) of the desired coating substrate are coated on separate wells of the multi-well plate for various time periods at the appropriate temperature/relative humidity. Note that depending on the specific coating or intended outcome of the adhesion method, it may be appropriate to compare multi-well plates with and without “tissue culture treatment.” A statistically significant number of replicates should be run to allow appropriate statistical analysis of the data. The data from the initial (broad concentration) test run will provide data to re-run the adhesion method using a more restrictive range for the coating concentration and for the time of incubation. Appropriate statistical analyses should be performed on the data. If an even more specific coating concentration is desired, then the procedure can be repeated using data from the second set of test runs. If desired, incubation times for the coating may also be varied. The procedure shall be repeated for each new coating material to optimize the coating concentration and the time of incubation for the coating.

10.1.3 Remove excess coating solution from the wells. A blocking step, using heat-denatured serum albumin, is recommended if sub-saturating protein densities are used. The blocking is usually performed prior to protein absorption. Follow by three washes in D-PBS.

10.1.4 Harvest cells and assess for viability using an appropriate method, such as the trypan blue dye exclusion method, and a hemocytometer. As the harvesting procedure very likely influences the cell adhesive process, care should be taken when performing procedures such as trypsinization to use the lowest concentration of trypsin/ethylenediamine tetra acetic acid (EDTA) for the shortest time possible. In addition, to limit potential effects on cell attachment strength, care should be taken to minimize the processing time, during which time the cells are outside of their optimum incubation/adhesion temperature/CO₂ conditions. For additional information on quantitating cell viability within biomaterial scaffolds and enumerating and characterizing cells and colonies in culture, we recommend consulting Guide F2739 and Practice F2944, respectively.

10.1.5 Dilute cells to a suggested cell concentration of 5×10^3 to 1×10^4 (per well in a 96-well plate) in appropriate medium for test cells or control cells in medium which has been pre-mixed with the desired fluorescence stain. The desired stain concentration (percentage stain to total volume) will vary with the specific stain employed. But as an example, with Hoechst stain, the recommended mix is 10 % of the volume.

10.1.6 Add cells to the wells and incubate at 37 °C at 95 % air/5 % CO₂/90 % R.H. (relative humidity), covered in aluminum foil to prevent photobleaching. The time required for adhesion varies significantly across cell type, ECM, and surface. Also, cell seeding in the presence of serum-containing medium affects adhesion time. Replicate samples in sufficient number of the 96 wells should be run to obtain statistical significance. It is recommended that an additional well be used to adjust the microscope parameters, such as exposure time, etc. Discard measurements from this additional well. For

additional information on assessing the attachment of cells to biomaterial surfaces by physical methods, see Guide F2664.

10.1.7 It is recommended that an inverted microscope be used to capture at least 5×5 digital tiled images (fluorescence) for each of the wells prior to centrifugation (pre-spin). Alternatively, the use of a fluorescence dye (that is, Calcein AM) and a microplate reader may be used before and after spinning instead of microscope imaging, followed by image processing. This alternate method may also minimize exposure that could cause photobleaching (2). Microscope imaging may still be required if further information on individual cell morphology or patterns of cell adhesion on a particular substrate is required.

10.1.8 *Determination of the Appropriate RCF for a Particular Cell Type and Substrate*—The following procedure is suggested to obtain the optimal relative centrifugal force (RCF) for a particular cell line seeded on a particular coating-substrate. First, a series of test runs of the method should be performed using multiple replicate test multi-well plates, incorporating a range of RCF values, such as 10 to $50 \times g$, 100 to $250 \times g$, and $350 \times g$ or above; where g = acceleration due to gravity. Data obtained from these test runs should be analyzed to determine the lowest RCF that results in approximately 50 % detachment of the cells from the treated surface. Appropriate viability, biochemical, histochemical, or mechanical testing should be performed on the cells following centrifugation at the selected RCF to determine if the centrifugation adhesion method has resulted in adverse changes in these properties for the cells. Note that the optimization of the RCF must be performed on each cell type or cell line. Depending on the cell type, the procedure may need to be repeated at different passages of the cells. Optimization of the RCF shall be performed for each substrate coating.

10.1.9 Before centrifugation, the wells are filled with D-PBS (at room temperature) to form a “reverse meniscus,” purged of air bubbles and covered with acetate sealing tape and immediately centrifuged.

10.1.10 Centrifuge the plates (upside down) at the pre-optimized RCF for 5 min at 22 °C.

10.1.11 Following centrifugation, discard acetate sealing tape and remove the supernatant from the wells. Wash one time with D-PBS. Fill wells with 100 μ L D-PBS. If possible, it is recommended to use a motorized pipetter set at low speed to have reproducible washing forces.

10.1.12 Capture fluorescent tiled digital images (suggested at least 5×5 matrices or appropriate for the cell line) (Guides F2998 and F3294) for each of the wells after centrifugation (post-spin).

10.1.13 Appendix X1.3 provides an example of the application of the protocol for the cell adhesion centrifugation assay with primary bovine chondrocytes. The purpose of this application is to determine the increase in cell adhesion of chondrocytes with serial passage number.

11. Calculation or Interpretation of Results

11.1 *Determination of Cell Number Pre- and Post-Spin:*

11.1.1 Tiled images for each of the wells are “stitched” together using the image analysis software. Subsequently, an

automated cell counting routine (such as Zeiss AxioVision, or any equivalent image analysis software) is used to count the number of fluorescently labeled nuclei.

11.1.2 Divide the post-spin cell count by the pre-spin count and multiply by 100 to determine the percent adhesion. As described in Reyes and Garcia (2003) (2), it is recommended to use the 50 % point for either ligand concentration or RCF for the most robust measurement of adhesion strength. For additional information on interpreting images of polymeric tissue scaffolds, see Guide F2603.

11.2 The centrifugation cell adhesion assay compares the adhesion of cells pre-centrifugation to the adhesion of the cells post-centrifugation at known RCFs. Results of a typical centrifugation assay (for chondrocytes) run at both 120 g and 350 g are shown in Fig. 2.

12. Precision and Bias

12.1 *Precision*—It is not possible to specify the precision of the procedure in this practice because of the wide variance in cell source and the specific tissue material to be used as a substrate for the test.

12.2 *Bias*—No information can be presented on the bias of the procedure in the Standard Practice F3088 for Use of a Centrifugation Method to Quantify/Study Cell-Material Adhesive Interactions because no material and/or cell source having an accepted reference value are available.

13. Keywords

13.1 cell adhesion assay; centrifugation; chondrocytes; monolayer culture; serial passage; tissue culture-treated polystyrene

iTeh Standards
(<https://standards.itih.ai>)
Document Preview

[ASTM F3088-22](#)

<https://standards.itih.ai/catalog/standards/sist/ed05cf48-b192-4378-8215-e29e2125589c/astm-f3088-22>