



Designation: D5449/D5449M – 22

Standard Test Method for Transverse Compressive Properties of Hoop Wound Polymer Matrix Composite Cylinders¹

This standard is issued under the fixed designation D5449/D5449M; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

This standard has been approved for use by agencies of the U.S. Department of Defense.

1. Scope

1.1 This test method determines the transverse compressive properties of wound polymer matrix composites reinforced by high-modulus continuous fibers. It describes testing of hoop wound (90°) cylinders in axial compression for determination of transverse compressive properties.

1.2 The technical content of this test method has been stable since 1993 without significant objection from its stakeholders. As there is limited technical support for the maintenance of this test method, changes since that date have been limited to items required to retain consistency with other ASTM D30 Committee standards, including editorial changes and incorporation of updated guidance on specimen preconditioning and environmental testing. The test method, therefore, should not be considered to include any significant changes in approach and practice since 1993. Future maintenance of the test method will only be in response to specific requests and performed only as technical support allows.

1.3 *Units*—The values stated in either SI units or inch-pound units are to be regarded separately as standard. The values stated in each system are not necessarily exact equivalents; therefore, to ensure conformance with the standard, each system shall be used independently of the other, and values from the two systems shall not be combined.

1.3.1 Within the text, the inch-pound units are shown in brackets.

1.4 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety, health, and environmental practices and determine the applicability of regulatory limitations prior to use.*

1.5 *This international standard was developed in accordance with internationally recognized principles on standardization established in the Decision on Principles for the*

Development of International Standards, Guides and Recommendations issued by the World Trade Organization Technical Barriers to Trade (TBT) Committee.

2. Referenced Documents

2.1 ASTM Standards:²

- D792 Test Methods for Density and Specific Gravity (Relative Density) of Plastics by Displacement
- D883 Terminology Relating to Plastics
- D2584 Test Method for Ignition Loss of Cured Reinforced Resins
- D2734 Test Methods for Void Content of Reinforced Plastics
- D3171 Test Methods for Constituent Content of Composite Materials
- D3878 Terminology for Composite Materials
- D5229/D5229M Test Method for Moisture Absorption Properties and Equilibrium Conditioning of Polymer Matrix Composite Materials
- D5448/D5448M Test Method for Inplane Shear Properties of Hoop Wound Polymer Matrix Composite Cylinders
- D5450/D5450M Test Method for Transverse Tensile Properties of Hoop Wound Polymer Matrix Composite Cylinders
- E4 Practices for Force Calibration and Verification of Testing Machines
- E6 Terminology Relating to Methods of Mechanical Testing
- E11 Specification for Woven Wire Test Sieve Cloth and Test Sieves
- E122 Practice for Calculating Sample Size to Estimate, With Specified Precision, the Average for a Characteristic of a Lot or Process
- E132 Test Method for Poisson's Ratio at Room Temperature
- E177 Practice for Use of the Terms Precision and Bias in ASTM Test Methods
- E251 Test Methods for Performance Characteristics of Metallic Bonded Resistance Strain Gages

¹ This test method is under the jurisdiction of ASTM Committee D30 on Composite Materials and is the direct responsibility of Subcommittee D30.04 on Lamina and Laminate Test Methods.

Current edition approved May 1, 2022. Published May 2022. Originally approved in 1993. Last previous edition approved in 2016 as D5449/D5449M – 16. DOI: 10.1520/D5449_D5449M-22.

² For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

E456 Terminology Relating to Quality and Statistics
 E691 Practice for Conducting an Interlaboratory Study to Determine the Precision of a Test Method
 E1237 Guide for Installing Bonded Resistance Strain Gages

3. Terminology

3.1 *Definitions*—Terminology D3878 defines terms relating to high-modulus fibers and their composites. Terminology D883 defines terms relating to plastics. Terminology E6 defines terms relating to mechanical testing. Terminology E456 and Practice E177 defines terms relating to statistics. In the event of a conflict between terms, Terminology D3878 shall have precedence over other standards.

NOTE 1—If the term represents a physical quantity, its analytical dimensions are stated immediately following the term (or letter symbol) in fundamental dimension form, using the following ASTM standard symbology for fundamental dimensions, shown within square brackets: $[M]$ for mass, $[L]$ for length, $[T]$ for time, $[\theta]$ for thermodynamic temperature, and $[nd]$ for non-dimensional quantities. Use of these symbols is restricted to analytical dimensions when used with square brackets, as the symbols may have other definitions when used without the brackets.

3.2 Definitions of Terms Specific to This Standard:³

3.2.1 *hoop wound, n*—a winding of a cylindrical component in which the filaments are circumferentially oriented.

3.2.2 *specimen, n*—a single part cut from a winding; each winding may yield several specimens.

3.2.3 *transverse compressive modulus, E_{22} [$ML^{-1}T^{-2}$]*, *n*—the compressive elastic modulus of a unidirectional material in the direction perpendicular to the reinforcing fibers.

3.2.4 *transverse compressive strain at failure, ϵ_{22}^{uc} [nd]*, *n*—the value of strain, perpendicular to the reinforcing fibers in a unidirectional material, at failure when a compressive force is applied in the direction perpendicular to the reinforcing fibers.

3.2.5 *transverse compressive strength, σ_{22}^{uc} [$ML^{-1}T^{-2}$]*, *n*—the strength of a unidirectional material when a compressive force is applied in the direction perpendicular to the reinforcing fibers.

3.2.6 *winding, n*—an entire part completed by one winding operation and then cured.

4. Summary of Test Method

4.1 A thin-walled hoop wound cylinder nominally 100 mm [4 in.] in diameter and 140 mm [5½ in.] in length is bonded into two end fixtures. The specimen fixture assembly is mounted in the testing machine and monotonically loaded in compression while recording force. The transverse compressive strength can be determined from the maximum force carried before failure. If the cylinder strain is monitored with strain gages then the stress-strain response, the compressive strain at failure, transverse compression modulus of elasticity, and Poisson's ratio can be derived.

³ If the term represents a physical quantity, its analytical dimensions are stated immediately following the term (or letter symbol) in fundamental dimension form, using the following ASTM standard symbology for fundamental dimensions, shown within square brackets: $[M]$ for mass, $[L]$ for length, $[T]$ for time, $[\theta]$ for thermodynamic temperature, and $[nd]$ for nondimensional quantities. Use of these symbols is restricted to analytical dimensions when used with square brackets, as the symbols may have other definitions when used without the brackets.

5. Significance and Use

5.1 This test method is designed to produce transverse compressive property data for material specifications, research and development, quality assurance, and structural design and analysis. Factors that influence the transverse compressive response and should therefore be reported are: material, method of material preparation, specimen preparation, specimen conditioning, environment of testing, specimen alignment and gripping, speed of testing, void content, and fiber volume fraction. Properties in the test direction that may be obtained from this test method are:

- 5.1.1 Transverse compressive strength, σ_{22}^{uc} ,
- 5.1.2 Transverse compressive strain at failure, ϵ_{22}^{uc} ,
- 5.1.3 Transverse compressive modulus of elasticity, E_{22} , and
- 5.1.4 Poisson's ratio, γ_{21} .

6. Interference

6.1 *Material and Specimen Preparation*—Poor material fabrication practices, lack of control of fiber alignment, and damage induced by improper specimen machining are known causes of high material data scatter in composites.

6.2 *Bonding Specimens to Test Fixtures*—A high percentage of failures in or near the bond between the test specimen and the test fixture, especially when combined with high material data scatter, is an indicator of specimen bonding problems. Specimen to fixture bonding is discussed in 11.5.

6.3 *System Alignment*—Excessive bending may cause premature failure, as well as highly inaccurate modulus of elasticity determination. Every effort should be made to eliminate excess bending from the test system. Bending may occur as a result of misaligned grips, misaligned specimens in the test fixtures, or from departures of the specimens from tolerance requirements. The alignment should always be checked as discussed in 13.2.

7. Apparatus

7.1 *Micrometers and Calipers*—A micrometer with a 4 to 8 mm [0.16 to 0.32 in.] nominal diameter ball-interface or a flat anvil interface shall be used to measure the specimen wall thickness, inner diameter, and outer diameter. A ball interface is recommended for these measurements when at least one surface is irregular (for example, a coarse peel ply surface, which is neither smooth nor flat). A micrometer or caliper with a flat anvil interface shall be used for measuring the overall specimen length, the gage length (the free length between the fixtures), and other machined surface dimensions. The use of alternative measurement devices is permitted if specified (or agreed to) by the test requestor and reported by the testing laboratory. The accuracy of the instruments shall be suitable for reading to within 1 % of the sample dimensions. For typical specimen geometries, an instrument with an accuracy of ± 0.0025 mm [± 0.0001 in.] is adequate for wall thickness measurements, while an instrument with an accuracy of ± 0.025 mm [± 0.001 in.] is adequate for measurement of the inner diameter, outer diameter, overall specimen length, gage length, and other machined surface dimensions.

7.2 *Compression Fixture*—The compression fixture consists of a steel outer shell and insert. An assembly drawing for these components and the test fixture is shown in Fig. 1.

7.2.1 *Outer Shell*—The outer shell (SI units Fig. 2, English units Fig. 3) is circular with a concentric circular hollow in one face, a groove along the diameter of the other face, and a center hole through the thickness. Along the diameter perpendicular to the groove, three pairs of small eccentric holes are placed at three radial distances. The two outer pairs of holes are threaded. Four additional threaded holes are placed at the same radial distance as the innermost set of holes at 90° intervals starting 45° from the diameter that passes through the center groove.

7.2.2 *Insert*—The fixture insert is circular with a center hole through the thickness (SI units Fig. 4, English units Fig. 5). Two sets of holes are placed along a concentric centerline. These holes align with the innermost set of holes in the outer shell. The set of four holes at 90° intervals are counterbored. The insert is fastened inside the hollow of the outer shell to form the concentric groove used to put the specimen in the fixture (Fig. 1).

7.2.3 The outer shell and insert for the compression fixture are the same outer shell and insert used for the fixtures in standard test methods D5448/D5448M and D5450/D5450M.

7.3 *Testing Machine*, comprised of the following:

7.3.1 *Fixed Member*—A fixed or essentially stationary member.

7.3.2 *Movable Member*.

7.3.3 *Steel Platens*, two, flat, one of which connects to the force-sensing device and the other at the opposite end of the assembled test fixture. At least one (preferably both) of these platens is coupled to the test machine with a swivel joint, that is, a hemispherical ball on the machine that fits into a hemispherical recess on one or both of the platens.

7.3.4 *Drive Mechanism*, for imparting to the movable member a uniform controlled velocity with respect to the fixed member, this velocity to be regulated as specified in 11.6.

7.3.5 *Force Indicator*—A suitable force-indicating mechanism capable of showing the total compressive force carried by

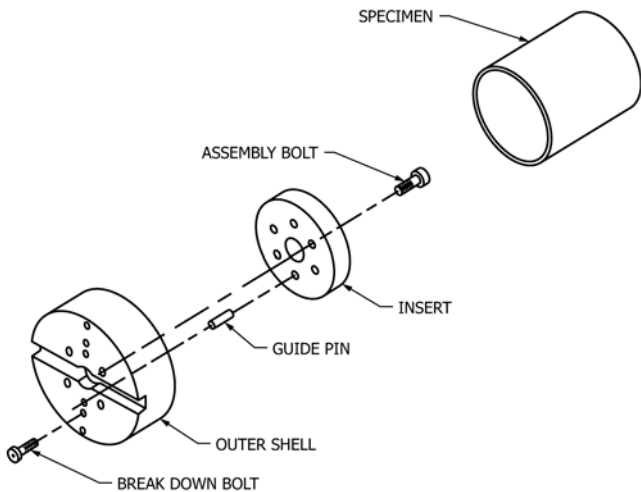


FIG. 1 Assembly Drawing for the Compression Fixture and Specimen

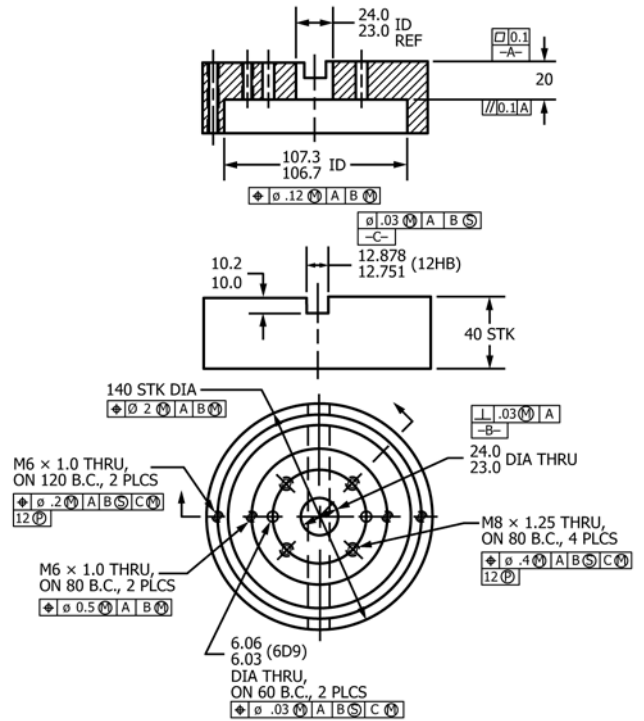


FIG. 2 The Outer Shell of the Compression Fixture in Metric Units

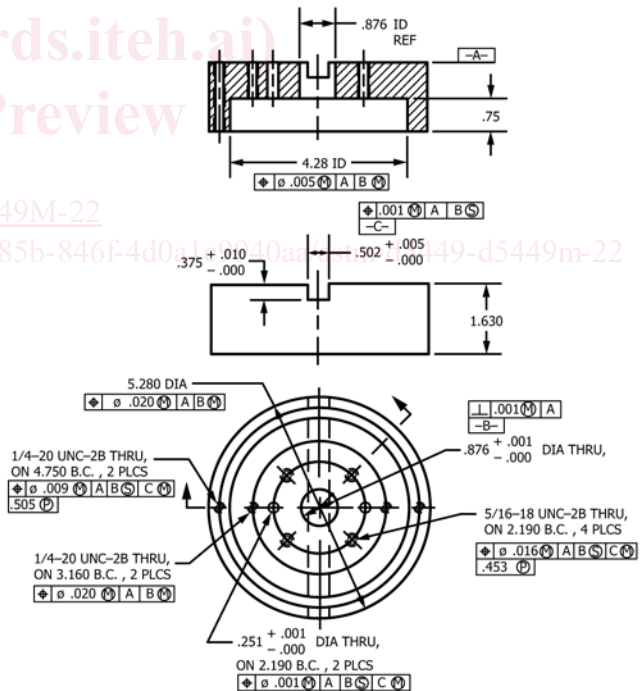


FIG. 3 The Outer Shell of the Compression Fixture in English Units

the test specimen. This mechanism shall be essentially free of inertia-lag at the specified rate of testing and shall indicate the force within an accuracy of $\pm 1\%$ of the actual value, or better. The accuracy of the testing machine shall be verified in accordance with Practice E4.

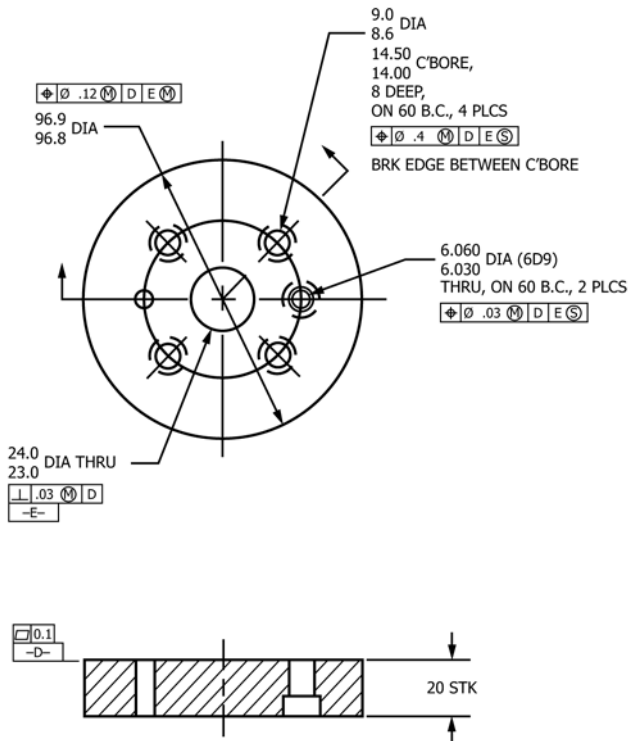


FIG. 4 The Insert of the Compression Fixture in Metric Units

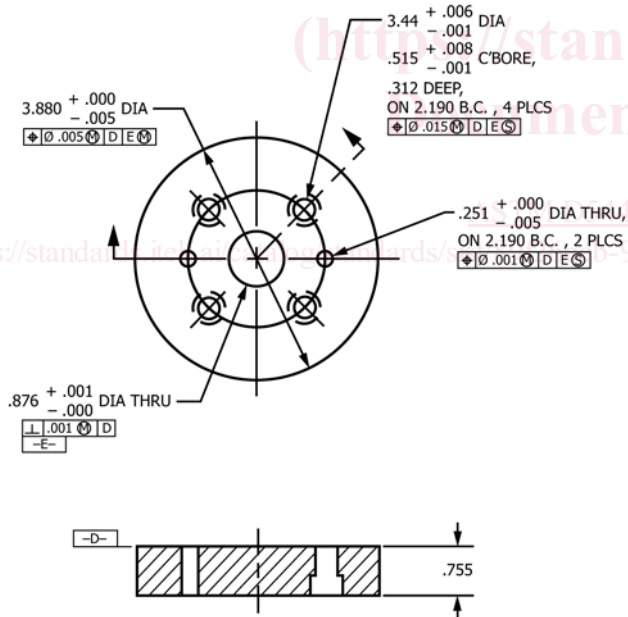


FIG. 5 The Insert of the Compression Fixture in English Units

specimen shall be instrumented to measure strain in both the axial and circumferential direction to determine Poisson's ratio. Strain gage rosettes (0°/45°/90°) shall be used to correct for gage misalignment. Gage calibration certification shall comply with Test Method E251. Some guidelines on the use of strain gages on composites are presented as follows. A general reference on the subject is Tuttle and Brinson.⁴

7.4.1 *Surface Preparation*—The surface preparation of fiber-reinforced composites discussed in Guide E1237 can penetrate the matrix material and cause damage to the reinforcing fibers, resulting in improper specimen failures. Reinforcing fibers should not be exposed or damaged during the surface preparation process. The strain gage manufacturer should be consulted regarding surface preparation guidelines and recommended bonding agents for composites, pending the development of a set of standard practices for strain gage installation surface preparation of fiber-reinforced composite materials.

7.4.2 *Gage Resistance*—Consideration should be given to the selection of gages having larger resistance to reduce heating effects on low-conductivity materials. Resistances of 350 Ω or higher are preferred. Additional considerations should be given to the use of the minimum possible gage excitation voltage consistent with the desired accuracy (1 to 2 V is recommended) to reduce further the power consumed by the gage. Heating of the specimen by the gage may affect the performance of the material directly, or it may affect the indicated strain as a result of a difference between the gage temperature compensation factor and the coefficient of thermal expansion of the specimen material.

7.4.3 *Temperature Considerations*—Consideration of some form of temperature compensation is recommended, even when testing at standard laboratory atmosphere. Temperature compensation is required when testing in nonambient temperature environments.

7.4.4 *Transverse Sensitivity*—Consideration should be given to the transverse sensitivity of the selected strain gage. The strain gage manufacturer should be consulted for recommendations on transverse sensitivity corrections and effects on composites. This is particularly important for a transversely mounted gage used to determine Poisson's ratio.

7.5 *Conditioning Chamber*—When conditioning materials at non-laboratory environments, a temperature/vapor-level controlled environment conditioning chamber is required that shall be capable of maintaining the required temperature to within ±3 °C [±5 °F] and the required relative humidity level to within ±3 % RH. Chamber conditions shall be monitored either on an automated continuous basis or on a manual basis at regular intervals.

7.6 *Environmental Test Chamber*—An environmental test chamber is required for testing environments other than ambient testing laboratory conditions. This chamber shall be capable of maintaining the gage section of the test specimen at the required test environment during the mechanical test. The

7.3.6 *Construction Materials*—The fixed member, movable member, platens, drive mechanism, and fixtures shall be constructed of such materials and in such proportions that the total longitudinal deformation of the system contributed by these parts is minimized.

7.4 *Strain-Indicating Device*—Force versus strain data shall be determined by means of bonded resistance strain gages. Each strain gage shall be 6.3 mm [0.25 in.] in length. The

⁴ Tuttle, M. E., and Brinson, H. F., "Resistance Foil Strain Gauge Technology as Applied to Composite Materials," *Experimental Mechanics*, Vol 24, No. 1, March 1984, pp. 54–64; errata noted in Vol 26, No. 2, January 1986, pp. 153–154.

test temperature shall be maintained within $\pm 3\text{ }^{\circ}\text{C}$ [$\pm 5\text{ }^{\circ}\text{F}$] of the required temperature, and the relative humidity level shall be maintained to within $\pm 3\%$ RH of the required humidity level.

8. Sampling and Test Specimens

8.1 *Sampling*—At least five specimens per test condition should be tested unless valid results can be gained through the use of fewer specimens, such as in the case of a designed experiment. For statistically significant data, the procedures outlined in Practice E122 should be consulted. The method of sampling shall be reported.

NOTE 2—If specimens are to undergo environmental conditioning to equilibrium, and are of such type or geometry that the weight change of the material cannot be properly measured by weighing the specimen itself, then another traveler of the same nominal thickness and appropriate size shall be used to determine when equilibrium has been reached for the specimens being conditioned.

8.2 *Geometry*—The test specimen shall be as shown in Fig. 6. The length of all specimens shall be 140 mm [5.5 in.]. This will provide a 102 mm [4.0 in.] gage length. The inner diameter of all specimens shall be $100 \pm 4\text{ mm}$ [$4.000 \pm 0.015\text{ in.}$]. Specimens may be fabricated on a tapered mandrel yielding a maximum taper over the specimen length of 0.0005 mm/mm [in./in.] on the diameter. The specimens shall have a nominal wall thickness of 2 mm [0.08 in.], the actual thickness to be specified by the winding parameters and shall be maintained as the test specimen is wound and cured.

8.3 *Winding*—All specimens shall be hoop wound (approximately 90°) with a single tow and with enough layers to meet the thickness criterion described above.

8.4 Unless otherwise directed, determine specific gravity and reinforcement and void volume percentages for each

winding. The material used for the determination of these properties should be extracted from the center of the winding if multiple specimens are extracted from one winding or from one of the ends of the winding if only one specimen is extracted from the winding. Determine and report specific gravity and density in accordance with Test Methods D792. Determine and report volume percent of the constituents by one of the matrix digestion procedures of Test Method D3171, or, for certain reinforcement materials such as glass and ceramics, by the matrix burn-off technique of Test Method D2584. The void content equations of Test Methods D2734 are applicable to both Test Method D2584 and the matrix digestion procedures.

8.5 *Labeling*—Label the specimens so that they will be distinct from each other and traceable back to the raw material, and will neither influence the test nor be affected by it.

9. Calibration


9.1 The accuracy of all measurement equipment shall have certified calibrations which are current at the time of use of the equipment.

10. Conditioning

10.1 The recommended pre-test condition is effective moisture equilibrium at a specific relative humidity as established by Test Method D5229/D5229M; however, if the test requestor does not explicitly specify a pre-test conditioning environment, no conditioning is required and the test specimens may be tested as prepared.

NOTE 3—The term moisture, as used in Test Method D5229/D5229M, includes not only the vapor of a liquid and its condensate, but the liquid itself in large quantities, as for immersion.

<https://standards.iteh.ai/catalog/standards/sist/89f26ecb-90c3-485b-846f-4d0a1c9940aa/astm-d5449-d5449m-22>

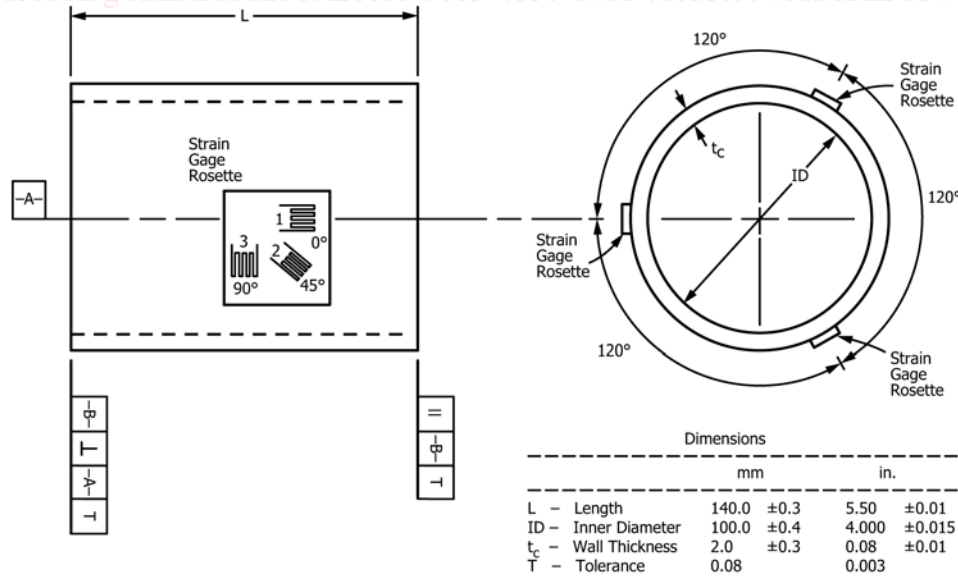

- Notes: 1. Tube may be fabricated on a tapered mandrel with maximum taper of 0.0005 in/in (0.0005 mm/mm) on the diameter.
 2. Actual measure of inner diameter will depend on specimen placement along tapered mandrel during fabrication.

FIG. 6 Test Specimen Shown with Strain Gage Configuration

10.2 The pre-test specimen conditioning process, to include specified environmental exposure levels and resulting moisture content, shall be reported with the test data.

10.3 If no explicit conditioning process is performed, the specimen conditioning process shall be reported as “unconditioned” and the moisture content as “unknown.”

11. Procedure

11.1 Parameters to Be Specified Before Test:

11.1.1 The sampling method, specimen geometry, and test parameters used to determine density and reinforcement volume.

11.1.2 The compression specimen sampling method.

11.1.3 The environmental conditioning test parameters.

11.1.4 The compression property and data reporting format desired.

NOTE 4—Specific material property, accuracy, and data reporting requirements should be determined before test for proper selection of instrumentation and data recording equipment. Estimates of operating stress and strain levels should also be made to aid in transducer selection, calibration of equipment, and determination of equipment settings.

11.2 General Instructions:

11.2.1 Any deviation from this test method shall be reported.

11.2.2 Following any conditioning, but before the testing, measure and report the specimen’s outer diameter (OD), inner diameter (ID), and length. The specimens are measured by first marking two randomly selected locations within the middle two thirds of the specimen’s length. At each of the points, average four measurements of the outer diameter on an axis that passes through the point and then repeat the procedure on an axis perpendicular to the initial axis. Repeat the procedure for the inner diameter using the same axes. Subtract the average inner diameter from the average outer diameter and divide the remainder by 2. This value will be used as the composite wall thickness, t_c . Also, obtain four length measurements, made at 90° intervals around the specimen circumference, and compute their average. This value will be used as the specimen length.

11.3 *Strain Gage Installation*—Attach strain gages to the center of the specimen’s gage section. Three strain gage rosettes (oriented as 0°/45°/90° where 0° is parallel to the specimen axis), mounted 120° around the specimen’s outer circumference from each other as shown in Fig. 6, are recommended to ascertain that only compressive loading is being applied. Noncompressive loading may be detected if the strain measured on one of the rosettes is greatly different from the strain on one or both of the other rosettes. For an accurate assessment of Poisson’s ratio, strain gages may be optionally attached to the inside of the specimen, directly opposite the gages on the outside, to measure circumferential strain.

11.4 *Fixture Assembly*—Assembly of the compression fixture is illustrated in Fig. 1. Place two guide pins into the guide pin holes of the insert such that approximately half of the pins length is protruding from the insert. Place the insert inside the concentric hollow of the outer shell such that the protruding

guide pins enter the outer shell guide pin holes. Secure the insert to the outer shell using four assembly bolts.

11.5 *Securing Specimens*—Secure the test specimen within two fixtures, as shown in Fig. 7, by filling the fixture’s cavities with potting material and inserting the specimen ends firmly to the bottom of the cavities while allowing the potting material to form a bead (Note 5). Cure in accordance with the manufacturer’s specifications, but the cure temperature should not jeopardize the specimen. Obtain four measurements of the free length between the fixtures, made at 90° intervals around the specimen/fixture circumference, and compute their average. This value will be used as the gage length.

NOTE 5—The potting material should be selected so that it can be cured at a temperature, T_c , no greater than 28 °C [50 °F] lower than the glass transition temperature T_g of the specimen, $T_c < T_g - 28$ °C [$T_c < T_g - 50$ °F]. It is helpful if the potting material can be removed without a great deal of difficulty upon completion of the test. A potting material should be selected to have properties sufficient to avoid failure of the potting material and failure of the specimen near the potting material during the test.

11.6 *Speed of Testing*—Speed of testing should be set to effect a nearly constant strain rate in the gage section. If strain control is not available on the testing machine, this may be approximated by repeated monitoring and adjusting of the rate of force application to maintain a nearly constant strain rate, as measured by strain transducer response versus time. The strain rate should be selected so as to produce failure within 1 to 10 min. If the ultimate strain of the material cannot be reasonably estimated, initial trials should be conducted using standard speeds until the ultimate strain of the material and the compliance of the system are known, and the strain rate can be adjusted. The suggested standard speeds are:

11.6.1 *Strain Control Machines*—A standard strain rate of 0.0125 min⁻¹.

11.6.2 *Constant Crosshead Speed Machine*—A standard crosshead displacement of 1.3 mm [0.05 in.] per min.

NOTE 6—Use of a fixed crosshead speed in testing machine systems with a high compliance will result in a strain rate that is much lower than required.

11.7 *Test Environment*—The specimen shall be conditioned to the desired moisture profile and tested under the same

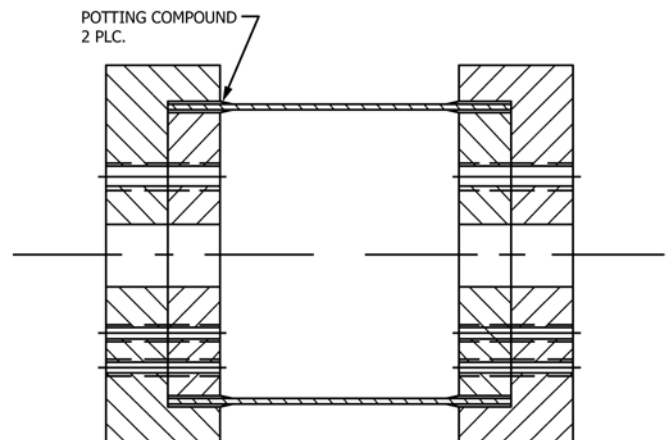


FIG. 7 Illustration of the Assembled Compression Fixture and Specimen

conditioning fluid exposure level. However, cases such as elevated temperature testing of a moist specimen place unrealistic requirements on the capabilities of common testing machine environmental chambers. In such cases, the mechanical test environment may need to be modified, for example, by testing at elevated temperature with no fluid exposure control, but with a specified limit on time to failure from withdrawal from the conditioning chamber. Modifications to the test environment shall be recorded.

NOTE 7—When testing a conditioned specimen at elevated temperature with no fluid exposure control, the percentage moisture loss of the specimen prior to test completion may be estimated by placing a conditioned traveler of known weight within the test chamber at the same time the specimen is placed in the chamber. The traveler should be configured to mimic the specimen, such that moisture evaporation is comparable to that of the test specimen. Upon completion of the test, the traveler is removed from the chamber, weighed, and the percentage weight calculated and reported.

11.7.1 If the testing area environment is different than the specimen conditioning environment, then the specimens shall be stored in the conditioned environment until the test time.

11.8 *Data Recording Instrumentation*—Attach the data recording instrumentation to the strain gages on the specimen and to the load cell.

11.9 *Loading*—Apply force to the specimen at the specified rate until failure, while recording data.

11.10 *Data Recording*—Record force versus strain continuously or at frequent regular intervals; for this test method, a sampling rate of 2 to 3 data recordings per second, and a target minimum of 100 data points per test are recommended. If the specimen is to be failed, record the maximum force, the failure force, and the strain at, or as near as possible to, where the force drops off significantly. A 10 % drop off in force is typically considered significant.

11.11 *Failure Mode*—Record the mode and location of failure of the specimen. Choose, if possible, a standard description from the sketches of common test failure modes which are shown in Fig. 8. Failure in a specimen occurring within one specimen thickness of the bond between the specimen and the test fixture is considered a Grip (GR) failure. Grip failure is typically precipitated by an anomalous condition; therefore, the grip failure mode is considered inappropriate.

11.12 *Fixture Disassembly*—This is only an advised procedure for disassembling the test fixture. Cut each end of the specimen at the base of the fixture. Remove the four assembly bolts from the insert. Place the outer shell and insert assembly

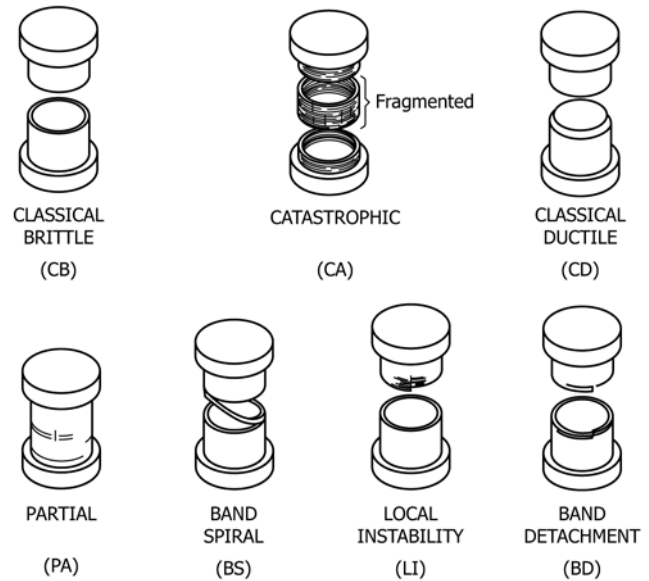


FIG. 8 Failure Modes for Hoop Wound Tubes in Compression

into an oven at a temperature that will degrade the potting compound. After a sufficient period of time, remove the fixtures from the oven and allow them to cool. Insert two break down bolts into the outer shell (see Fig. 1). Turn break down bolts to force insert out of the concentric circular hollow of the outer shell. Remove guide pins from the insert and outer shell. Wire brush the insert and outer shell to remove specimen debris.

12. Validation

12.1 Values for ultimate properties shall not be calculated for any specimen that breaks at some obvious flaw, unless such flaw constitutes a variable being studied. Retests shall be performed for any specimen on which values are not calculated.

12.2 A significant fraction of failures in a sample population occurring within one specimen thickness of the bond between the specimen and test fixture shall be cause to reexamine the means of force introduction into the material. Factors considered should include alignment of the specimen in the fixture, alignment of the fixtures in the grips, and material used to bond the specimen to the fixture.

13. Calculation

13.1 *Transverse Sensitivity Correction*—Correct the strain gage readings for transverse sensitivity separately for each rosette.

$$\epsilon_1^i = \frac{\epsilon_1^i (1 - \nu_o K_{t_1}) - K_{t_1} \epsilon_3^i (1 - \nu_o K_{t_3})}{1 - K_{t_1} K_{t_3}} \quad (1)$$

$$\epsilon_2^i = \frac{\epsilon_2^i (1 - \nu_o K_{t_2})}{1 - K_{t_2}} - \frac{K_{t_2} [\epsilon_1^i (1 - \nu_o K_{t_1}) (1 - K_{t_3}) + \epsilon_3^i (1 - \nu_o K_{t_3}) (1 - K_{t_1})]}{(1 - K_{t_1} K_{t_3}) (1 - K_{t_2})} \quad (2)$$