



Designation: C1022 – 17 (Reapproved 2022)

Standard Test Methods for Chemical and Atomic Absorption Analysis of Uranium-Ore Concentrate¹

This standard is issued under the fixed designation C1022; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

1. Scope

1.1 These test methods cover procedures for the chemical and atomic absorption analysis of uranium-ore concentrates to determine compliance with the requirements prescribed in Specification C967.

1.2 The analytical procedures appear in the following order:

	Sections
Uranium by Ferrous Sulfate Reduction—Potassium Dichromate Titrimetry	9
Nitric Acid-Insoluble Uranium	10 to 18
Extractable Organic Material	19 to 26
Determination of Arsenic	27
Carbonate by CO ₂ Gravimetry	28 to 34
Fluoride by Ion-Selective Electrode	35 to 42
Halides by Volhard Titration	43 to 50
Phosphorus by Spectrophotometry	52 to 60
Determination of Silicon	61
Determination of Thorium	62
Calcium, Iron, Magnesium, Molybdenum, Titanium, and Vanadium by Atomic Absorption Spectrophotometry	63 to 72
Potassium and Sodium by Atomic Absorption Spectrophotometry	73 to 82
Boron by Spectrophotometry	83 to 92

1.3 The values stated in SI units are to be regarded as standard. The values given in parentheses are for information only.

1.4 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety, health, and environmental practices and determine the applicability of regulatory limitations prior to use.* A specific precautionary statement is given in Section 7.

1.5 *This international standard was developed in accordance with internationally recognized principles on standardization established in the Decision on Principles for the Development of International Standards, Guides and Recommendations issued by the World Trade Organization Technical Barriers to Trade (TBT) Committee.*

¹ These test methods are under the jurisdiction of ASTM Committee C26 on Nuclear Fuel Cycle and are the direct responsibility of Subcommittee C26.05 on Methods of Test.

Current edition approved July 1, 2022. Published July 2022. Originally approved in 1984. Last previous edition approved in 2017 as C1022 – 17. DOI: 10.1520/C1022-17R22.

2. Referenced Documents

2.1 ASTM Standards:²

- C761 Test Methods for Chemical, Mass Spectrometric, Spectrochemical, Nuclear, and Radiochemical Analysis of Uranium Hexafluoride
- C859 Terminology Relating to Nuclear Materials
- C967 Specification for Uranium Ore Concentrate
- C1110 Test Method for Determining Elements in Waste Streams by Inductively Coupled Plasma-Atomic Emission Spectroscopy (Withdrawn 2014)³
- C1219 Test Methods for Arsenic in Uranium Hexafluoride (Withdrawn 2015)³
- C1254 Test Method for Determination of Uranium in Mineral Acids by X-Ray Fluorescence
- C1267 Test Method for Uranium by Iron (II) Reduction in Phosphoric Acid Followed by Chromium (VI) Titration in the Presence of Vanadium
- C1287 Test Method for Determination of Impurities in Nuclear Grade Uranium Compounds by Inductively Coupled Plasma Mass Spectrometry
- C1347 Practice for Preparation and Dissolution of Uranium Materials for Analysis
- C1843 Test Method for Determining Moisture Content in Uranium-Ore Concentrate
- D1193 Specification for Reagent Water
- E60 Practice for Analysis of Metals, Ores, and Related Materials by Spectrophotometry

3. Terminology

3.1 *Definitions*—For definitions of terms used in these test methods, refer to Terminology C859.

4. Significance and Use

4.1 The test methods in this standard are designed to show whether a given material meets the specifications prescribed in Specification C967.

² For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

³ The last approved version of this historical standard is referenced on www.astm.org.

4.2 Because of the variability of matrices of uranium-ore concentrate and the limited availability of suitable reference or calibration materials, the precision and bias of these test methods should be established by each individual laboratory that will use them. The precision and bias statements given for each test method are those reported by various laboratories and can be used as a guideline.

4.3 Instrumental test methods such as X-ray fluorescence and emission spectroscopy can be used for the determination of some impurities where such equipment is available.

5. Interferences

5.1 Interferences are identified in the individual test methods.

5.2 Ore concentrates are of a very variable nature; therefore, all interferences are very difficult to predict. The individual user should verify the applicability of each procedure for specific ore concentrates.

6. Reagents

6.1 *Purity of Reagents*—Reagent grade chemicals shall be used in all tests. Unless otherwise indicated, it is intended that all reagents shall conform to the specifications of the Committee on Analytical Reagents of the American Chemical Society, where such specifications are available.⁴ Other grades may be used, provided it is first ascertained that the reagent is of sufficiently high purity to permit its use without lessening the accuracy of the determination.

6.2 *Purity of Water*—Unless otherwise indicated, references to water shall be understood to mean reagent water conforming to type I water in Specification D1193.

7. Precautions

7.1 Proper precautions should be taken to prevent inhalation or ingestion of uranium during sample preparation and any subsequent sample analysis.

7.2 Hydrofluoric acid is a highly corrosive acid that can severely burn skin, eyes, and mucous membranes. Hydrofluoric acid differs from other acids because the fluoride ion readily penetrates the skin, causing destruction of deep tissue layers. Unlike other acids that are rapidly neutralized, hydrofluoric acid reactions with tissue may continue for days if left untreated. Familiarization and compliance with the Safety Data Sheet is essential.

7.3 Chloroform is a dangerous chemical causing acute toxicity with repeated inhalation, dermal, or oral exposure. Many health hazards are associated with exposure to chloroform including its potential to cause cancer. Familiarization and compliance with the Safety Data Sheet is essential.

⁴ ACS Reagent Chemicals, Specifications and Procedures for Reagents and Standard-Grade Reference Materials, American Chemical Society, Washington, DC. For suggestions on the testing of reagents not listed by the American Chemical Society, see *Analar Standards for Laboratory Chemicals*, BDH Ltd., Poole, Dorset, U.K., and the *United States Pharmacopeia and National Formulary*, U.S. Pharmacopeial Convention, Inc. (USPC), Rockville, MD.

8. Sampling

8.1 Collect samples in accordance with Specification C967.

8.2 Special requirements for subsampling are given in the individual test methods.

URANIUM BY FERROUS SULFATE REDUCTION—POTASSIUM DICHROMATE TITRIMETRY

9. Scope

9.1 This test method covers the determination of uranium in uranium-ore concentrates. This test method was discontinued in January 2002 and replaced with Test Method C1267.

9.2 The uranium content of the sample may also be determined using Test Method C1254. The user's laboratory must establish and document method performance.

NOTE 1—Dissolution of UOC samples may be achieved using the techniques or combination of techniques described in Practice C1347. The laboratory must validate the performance of Practice C1347 using characterized UOC samples. If Practice C1347 methods are not suitable for UOC sample dissolution, the user may establish and document applicable dissolution methods.

NITRIC ACID-INSOLUBLE URANIUM

10. Scope

10.1 This test method covers the determination of that quantity of uranium in uranium-ore concentrate that is not soluble in nitric acid.

11. Summary of Test Method

11.1 A sample of ore concentrate is digested in 10 M nitric acid at 95 °C to 100 °C for 1 h. The slurry is filtered and the residue washed with 1 M nitric acid until the filtrate gives a negative test for uranium. The washed residue is then dried and ignited at 1000 °C ± 25 °C for 1 h. The uranium content is determined on the ignited residue by spectrophotometry.

12. Interference

12.1 At the specification limit for nitric acid insoluble uranium usually established for uranium-ore concentrates, interference effects are insignificant.

13. Apparatus

13.1 *Digestion Flask*, 500 mL, with side entry tube and attached reservoir.

13.2 *Stirring Apparatus*, with sleeve-type stirrer.

13.3 *Heating Mantle*, 250 W, controlled by a variable transformer.

13.4 *Büchner Funnel*.

13.5 *Porcelain Crucibles*, 40 mL.

13.6 *Muffle Furnace*.

13.7 *Filter Paper*, ashless of medium porosity, and a medium flow rate with a particle retention of 8 µm has been found to be suitable.

13.8 *Spectrophotometer*, with 1 cm cells that are in accordance with Practice E60.

14. Reagents

14.1 *Nitric Acid (10 M)*—Dilute 62.5 mL of HNO₃ (sp gr 1.42) to 100 mL with distilled water.

14.2 *Nitric Acid (1 M)*—Dilute 62.5 mL of HNO₃ (sp gr 1.42) to 1 L with distilled water.

14.3 *Sodium Hydroxide (100 g/L)*—Dissolve 10 g of NaOH in 100 mL of water.

14.4 *Hydrogen Peroxide (H₂O₂, 30 %)*.

14.5 *Hydrochloric Acid (HCl, sp gr 1.19)*.

14.6 *Hydrofluoric Acid (HF, 48 %)*.

14.7 *Sulfuric Acid (9 M)*—Add 500 mL H₂SO₄ (sp gr 1.84) to 500 mL of iced water with constant stirring. Cool and dilute to 1 L with water.

15. Procedure

15.1 Weigh a 50.0 g ± 0.1 g sample directly into the digestion flask.

15.2 Place the flask in the heating mantle and adjust the support ring so that the joints of the flask and sleeve stirrer are engaged, and the stirrer blades turn freely but just clear the bottom of the flask.

15.3 Transfer 95 mL of 10 M nitric acid to a 250 mL beaker and heat between 95 °C to 100 °C.

15.4 Slowly transfer the heated nitric acid solution to the digestion flask through the entry side tube with the stirrer turning.

NOTE 2—The stirrer is started before the acid is added to prevent material from sticking to the flask.

15.5 Adjust the thermometer so that the bulb of the thermometer is immersed in the stirring slurry, but adequately clears the turning stirrer blades.

15.6 Quickly bring the sample to 97 °C and digest between 95 °C to 100 °C for 1 h while stirring. (Measure the 1-h digestion time after the temperature of the slurry has reached 97 °C.)

15.7 Turn off the variable transformer, but allow the stirrer to continue turning.

15.8 Remove the thermometer and carefully rinse with water all slurry that adheres to it.

15.9 Wipe the immersed portion of the thermometer with one fourth of a circle of filter paper and transfer the paper to a prepared Büchner funnel fitted with a filter paper.

15.10 Add 10 mL of paper pulp to the slurry and continue stirring for about 5 min.

15.11 Turn off the stirrer, then lower the flask and mantle.

15.12 Carefully wash the slurry that adheres to the stirrer shaft and blades into the flask with water.

15.13 Wipe the shaft and blades with one fourth of a circle of filter paper and transfer the filter paper to the Büchner funnel.

15.14 Filter the slurry through the Büchner funnel and wash contents of the flask into the funnel.

15.15 Wash the residue with 1 M nitric acid until a 10 mL portion of the filtrate shows no detectable yellow color when made basic with sodium hydroxide and after a few drops of H₂O₂ (30 %) have been added as a color developer.

15.16 Wash the residue several times with water after a negative test is obtained.

15.17 Draw air through the filter until the residue and filter pad are dry.

15.18 Scrape the residue and paper into a preignited (1000 °C) tared 40 mL crucible, place on a hot plate and slowly char off the organic material.

15.19 Ignite the residue for 1 h at 1000 °C in a muffle furnace.

15.20 Cool the crucible in a desiccator and weigh.

15.21 Calculate the percentage of solids in accordance with 17.1. If the percentage of solids (insoluble residue) is greater than 0.1 %, grind and mix the residue and determine the total milligrams of uranium in the residue by the photometric procedure in 16.1 – 16.10.

16. Photometric Procedure for Uranium

16.1 Transfer the ground, blended residue from 15.20 to a 100 mL beaker.

16.2 Add 10 mL of water and 10 mL of HCl (sp gr 1.19), cover, and boil for 10 min.

16.3 Add 5 mL of HNO₃ (sp gr 1.42) and boil until fuming of NO₂ ceases. Remove cover glass.

16.4 Add 5 mL of 9M H₂SO₄ and 2 mL of HF (48 %), then heat to dryness on the hotplate. Bake to fume off remaining H₂SO₄ and cool.

16.5 Wash down sides of beaker with water and add 5 mL of HNO₃.

16.6 Cover with a watchglass and digest for approximately 10 min near the boiling point.

16.7 Quantitatively transfer the solution to a 250 mL volumetric flask. Add 25 mL of NaOH solution and a few drops of H₂O₂. Make up to mark with water and mix.

NOTE 3—The solution must be basic for yellow sodium peruranate color to develop.

16.8 Measure the absorbance of the solution in a spectrophotometer at 425 nm in a 1 cm cell using a blank as reference. The blank is prepared by diluting 25 mL of a 100 g/L NaOH solution, plus a few drops of H₂O₂, to 250 mL with water.

16.9 Prepare a calibration curve covering the range from 0 mg to 50 mg of uranium from aliquots of a standard uranium solution. Proceed as in 16.5 – 16.8. Plot the milligrams of uranium against absorbance readings.

16.10 Determine the total milligrams of uranium in the sample solution from the calibration curve.

NOTE 4—If the sample solution falls outside the calibration range, dilute a portion with the reference-blank solution and read again.

17. Calculation

17.1 Calculate the percentage of insoluble residue, R , present as follows:

$$R = \frac{R_w \times 100}{S_w} \quad (1)$$

where:

R_w = weight of residue (see 15.20), g, and
 S_w = weight of samples, g.

17.2 If the insoluble residue exceeds 0.1 %, calculate the percentage of nitric acid-insoluble uranium, U_N , and present as follows:

$$U_N = \frac{U}{S_w \times 10} \quad (2)$$

where:

U = uranium content calculated in 16.10, mg, and
 S_w = weight of sample, g.

17.3 Calculate the percentage of nitric acid-insoluble uranium, U_u , on a uranium basis as follows:

$$U_u = \frac{U_N \times 100}{U_s} \quad (3)$$

where:

U_N = nitric acid-insoluble residue present (see 17.2), %, and
 U_s = uranium in sample, %.

18. Precision and Bias

18.1 *Precision*—A relative standard deviation for this test method has been reported as 10 % at the 0.2 % HNO₃ insoluble uranium level (see 4.2).

18.2 *Bias*—For information on the bias of this test method see 4.2.

EXTRACTABLE ORGANIC MATERIAL

19. Scope

19.1 This test method is used to determine the extractable organic material in uranium-ore concentrates. It is recognized that certain water-soluble organic materials, such as flocculant agents, are not measured by this test method.

20. Summary of Test Method

20.1 This test method consists of a dual extraction using *n*-hexane on the solid uranium-ore concentrate sample and chloroform on a subsequent nitric acid solution of the sample. Each of the extractants is evaporated to measure the amount of organic material extracted.

21. Interferences

21.1 At the specification limit for extractable organic material established for uranium-ore concentrations, and within the scope of this test method, interferences are insignificant.

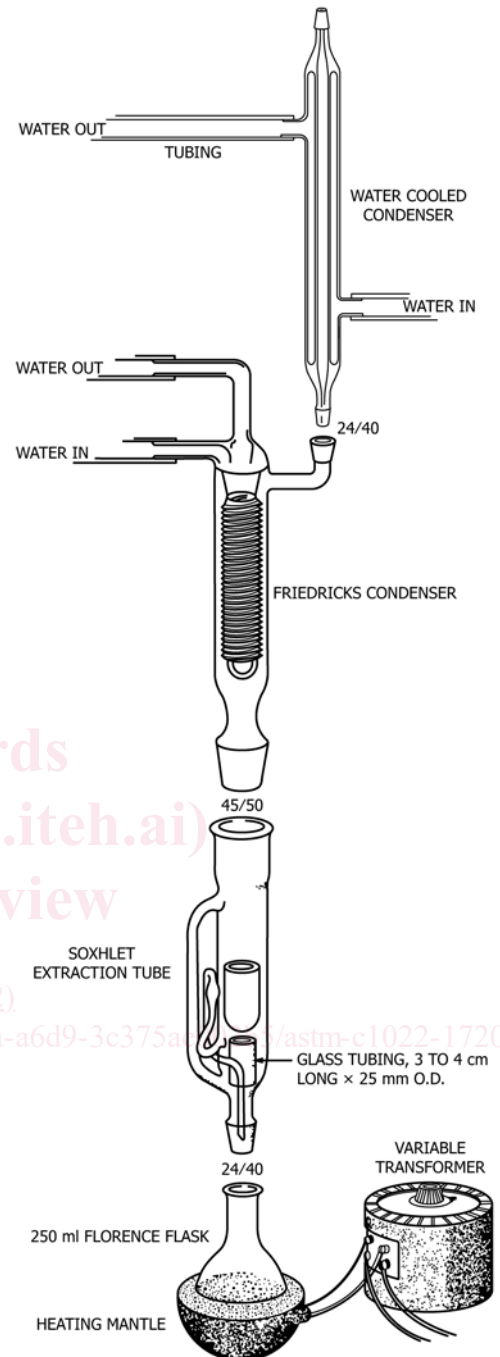


FIG. 1 Hexane Extraction Unit

22. Apparatus

22.1 *Soxhlet Extraction Apparatus*—The *n*-hexane extraction is done in a Soxhlet extraction apparatus. Construct as follows (see Fig. 1):

22.1.1 Modify a medium Soxhlet extraction tube so that the sidearm siphon is about 2 cm high, therefore, reducing the volume of solvent needed. Insert a 3 cm to 4 cm long, 25 mm outside diameter glass tube upright into the extraction tube in such a manner that an extraction thimble may be placed on it.

22.1.2 Connect a 250 mL Florence flask, that has a 24/40 ground-glass joint on the lower end to the top of the extraction tube. A 250 mL heating mantle connected to a 7.5 A variable transformer shall be used to heat this.

22.1.3 Connect a Friedrichs condenser, that has a 45/50 ground-glass joint on the lower end, to the top of the extraction tube. Turn this side of the condenser upward, and fuse the outer member of a 24/40 ground-glass joint to it.

22.1.4 Connect a Graham condenser, that has a 24/40 ground-glass joint on the lower end, to the modified sidearm of the Friedrichs condenser. Unless the relative humidity is low, insulate the Graham condenser to prevent the condensation of water on the outside surface that might seep through the joint to the Friedrichs condenser. Foam insulation 1 cm thick may be used for this purpose. The Graham condenser is cooled with cold water from a water bath cooler, and may be required when *n*-hexane is used for the extraction.

22.2 *Heat gun* (hot-air electric dryer), may be used to evaporate the solvent in procedure 24.6 or 24.15.

22.3 *Extraction Thimbles*, with 33 mm I.D., length 94 mm, and 1.5 mm thick has been found to be suitable.

22.4 *Phase Separator Paper*, treated with silicon and about 90 mm in diameter.

23. Reagents

23.1 *n*-hexane—Whenever a new supply is used, it should be checked for nonvolatile residue. Evaporate 100.0 mL just to dryness in a weighted platinum dish, cool to room temperature, and reweigh the dish. If there is any residue, either make the appropriate blank correction or distill the solvent before use to remove the nonvolatile impurities.

23.2 *Nitric Acid (1 + 1)*—Mix equal volumes of concentrated (sp gr 1.42) reagent grade HNO₃ and water.

23.3 *Chloroform*—Whenever a new supply of chloroform is to be used, it should be checked for nonvolatile residue as described in 23.1.

24. Procedure

24.1 Weigh 50.0 g of well-mixed, undried uranium-concentrate sample and transfer to an extraction thimble while tapping the thimble on a table top to compact and level the sample.

24.2 Place a plug of glass wool in the thimble above the sample. Support the thimble on the glass tube in the Soxhlet extraction tube so that when solvent condenses on the lower tip of the Friedrichs condenser, it will drop into the thimble.

24.3 Connect the extraction tube to the bottom of the Friedrichs condenser that is in series with the Graham condenser. Turn on the tap water coolant to the condensers.

NOTE 5—Tap water may be used in cooling both condensers if the amount of reagent lost during the refluxing (see 24.5) is not greater than 10 % of the volume added in 24.4. If the tap water is too warm, then the Graham condenser must be cooled by the refrigerated water cooler, or an ice-cooled condenser may be used in place of the Graham condenser.

24.4 Add a piece of sintered glass or several glass boiling beads and then 120 mL to 125 mL *n*-hexane to the 250 mL Florence flask. Attach the flask to the Soxhlet extraction tube.

24.5 Place the heating mantle below the Florence flask, connect to the variable transformer set at 55 V to 60 V, and allow the reagent to reflux rapidly for 3 ½ to 4 h.

24.6 Pour the refluxed reagent into a weighed (W_1 in grams) platinum dish, and evaporate in a hood. An infrared lamp or hot air stream from a heat gun may be used.

NOTE 6—Exercise care in this evaporation. If a heat source is used, adjust the rate of heat input and velocity of air across the dish so that no sample will be mechanically lost. If a heat gun is used, the amount and temperature of the air directed against the sample are especially critical because the high rate of evaporation is likely to lower the temperature of the solution to the point where water will condense in the dish.

24.7 Allow the dish to come to room temperature while tilting and rotating it to spread the last few drops of solvent uniformly over the bottom.

NOTE 7—Do not allow the temperature of the dish to go below the dewpoint.

24.8 Weigh in open air at intervals on an analytical balance, recording the weight of the dish 5 min after the rate of loss has decreased to 0.5 mg/min.

NOTE 8—This weight is in grams as W_2 .

24.9 Add a plastic-covered magnetic stirring bar and 100 mL of (1 + 1) nitric acid to a 400 mL beaker.

24.10 While magnetically stirring the acid, cautiously add the extracted sample from the extraction thimble. Stir until the sample is dissolved or until it is apparent that practically no more sample will dissolve.

24.11 Cool to about room temperature and transfer to a 500 mL separatory funnel. Add 100.0 mL of chloroform, stopper tightly, and shake as vigorously as possible for 60 s.

24.12 Allow the phases to separate.

NOTE 9—If emulsions form, transfer to centrifuge tubes and centrifuge to separate the phases.

24.13 Drain off the lower phase. If the lower phase is the chloroform layer, filter through a phase-separator filter paper into a graduated cylinder or narrow-neck flask. If the lower phase is the aqueous phase, drain and discard. Then filter the upper phase through a phase-separator filter paper into a graduated cylinder or narrow-neck flask.

24.14 Transfer 50.0 mL of the filtered chloroform into an ignited (900 °C) platinum dish.

24.15 Place the platinum dish in a hood and evaporate until about 1 mL of chloroform remains. This evaporation may be done as described in 24.6.

24.16 Allow the dish to cool to room temperature while tilting and rotating it to spread the last few drops uniformly over the bottom.

24.17 Weigh in open air on a recording balance or at intervals on an analytical balance, recording the weight of the dish 5 min after the rate of weight loss has decreased to 0.5 mg/min.

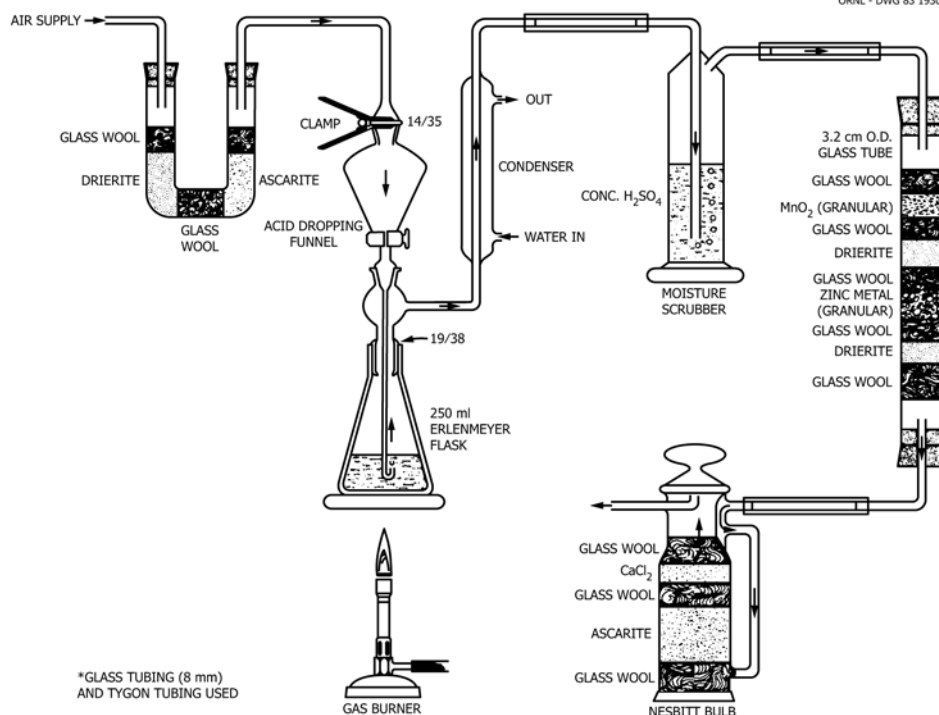


FIG. 2 Carbonate Apparatus

NOTE 10—This weight is in grams as W_3 .

24.18 Ignite the platinum dish at 900 °C for a minimum of 30 min, cool to room temperature, and weigh.

NOTE 11—This weight is in grams as W_4 .

25. Calculation

25.1 Calculate the percentage of extractable organic material, O_m , as follows:

$$O_m = \frac{100 [(W_2 - W_1) + 2 (W_3 - W_4)]}{S_w} \quad (4)$$

where:

- W_2 = weight of platinum dish in 24.8, g,
- W_1 = weight of platinum dish in 24.6, g,
- W_3 = weight of platinum dish in 24.17, g,
- W_4 = weight of platinum dish in 24.18, g, and
- S_w = weight of sample.

26. Precision and Bias

26.1 *Precision*—A relative standard deviation for this test method has been reported as 18 % at the 0.1 % extractable organic level (see 4.2).

26.2 *Bias*—For information on the bias of this test method see 4.2.

DETERMINATION OF ARSENIC

27. Scope

27.1 The determination of Arsenic by diethyldithiocarbamate photometric method has been discontinued. Interested persons can obtain a copy in the C1022 – 02 version. A copy of

the C1022 – 02 version can be obtained by visiting www.astm.org and entering C1022 – 02 into the search.

27.2 With appropriate sample preparation, Atomic Absorption Spectrometry as described in Test Methods C1219 may be used for arsenic determination.

27.3 As an alternative and with appropriate sample preparation, ICP-MS as described in Test Method C1287 may be used for arsenic determination.

CARBONATE BY CO₂ GRAVIMETRY

28. Scope

28.1 This test method covers the determination of 0.1 % to 3 % carbonate in uranium-ore concentrate.


28.2 The concentration range can be extended by taking smaller sample weights.

29. Summary of Test Method

29.1 The carbonate in the sample is decomposed with hydrochloric acid and evolved as carbon dioxide. The incoming air is dried and the CO₂ is removed by passing it through NaOH and anhydrous calcium sulfate (CaSO₄). The evolved gases are scrubbed in H₂SO₄ to remove moisture and passed through a tower of manganese dioxide and zinc metal to remove any SO₂ or H₂S formed. The evolved gas is then absorbed by NaOH in a Nesbitt bulb and determined gravimetrically (1).

30. Apparatus

30.1 *Carbonate Apparatus*, (see Fig. 2).

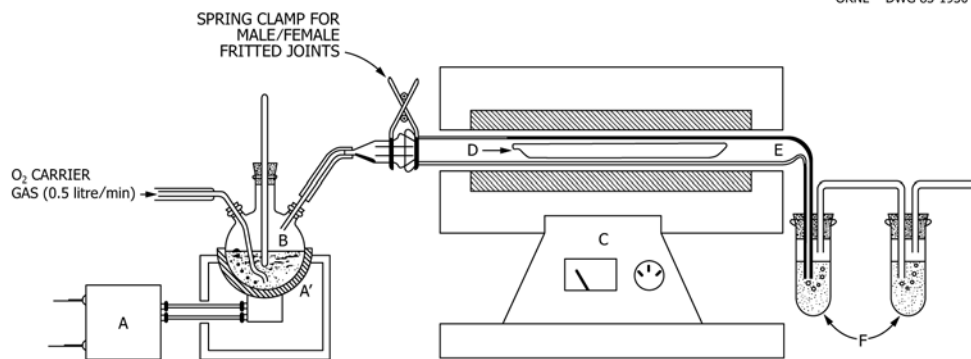

A, A'—Heating jacket controlled by variable transformer. Nominal temperature 80 °C to 85 °C for water.
 B—One-liter three-necked with gas diffuser and thermometer 0 °C to 110 °C. Water used meeting specification D1193.
 C—Tube furnace, controlled by variable transformer with thermocouple. Operating temperature 850 °C ± 25 °C.
 D—Sample boat.
 E—Pyrohydrolytic tube.
 F—Collection system; 10 mL of 0.2 N sodium hydroxide in first tube, 10 mL to 15 mL of water in second tube.

FIG. 3 Pyrohydrolysis Apparatus

31. Reagents

- 31.1 Sodium Hydroxide Coated Non-Fibrous Silicate.
- 31.2 Anhydrous Calcium Sulfate.
- 31.3 Glass Wool.
- 31.4 Manganese Dioxide, granular.
- 31.5 Zinc Metal, granular.
- 31.6 Sulfuric Acid (H₂SO₄, sp gr 1.84).
- 31.7 Hydrochloric Acid (5.5 M)—Dilute 50 mL of HCl (sp gr 1.19) to 100 mL with water.

32. Procedure

32.1 Weigh a sample (maximum of 5 g) to the nearest 0.01 g. The sample should contain approximately 20 mg CO₂. Transfer to an Erlenmeyer flask and add enough water to cover the inlet tube.

32.2 Attach the Nesbitt bulb, open the stopper and pass air through the apparatus for 10 to 15 min at the rate of 2 to 3 bubbles/s.

32.2.1 Measure the flow rate at the H₂SO₄ moisture trap.

32.3 Remove the Nesbitt bulb without altering the air flow. Close the stopper and weigh the bulb to nearest 0.1 mg.

32.4 Open the stopper of the bulb and replace it on the apparatus.

32.5 Evaluate the type of uranium ore concentrate.

32.5.1 If the UOC was produced as any type other than uranium peroxide, then place 25 mL of 5.5 M HCl in the dropping funnel and force it into the flask by replacing the air inlet tube.

32.5.2 If the uranium-ore concentrate was produced as a uranium peroxide, replace 25 mL of 5.5 M HCl with 25 mL of 5.5 M H₂SO₄ to prevent the release of chlorine.

32.6 Heat the Erlenmeyer flask with a small burner until the acid boils and adjust the burner to maintain gentle boiling.

32.7 Boil for 15 min, then shut off the flame.

32.8 Continue to pass air through the apparatus for an additional 10 min.

32.9 Remove the Nesbitt bulb and close the stopper immediately.

32.10 Reweigh the Nesbitt bulb to the nearest 0.1 mg.

32.11 Remove the Erlenmeyer flask from the apparatus while air is still flowing. Leave the air on until the flask is removed to prevent suck-back of the H₂SO₄.

32.12 Repeat the procedure in 32.1 – 32.10, without a sample, to obtain a blank.

33. Calculation

33.1 Calculate the percentage of carbonate, C_a, for the sample and the blank as follows:

$$C_a = \frac{136.36 (B - C)}{A} \quad (5)$$

where:

- A = sample weight, g, (step 32.1),
- B = weight of Nesbitt bulb after absorption of CO₂, g, (step 32.10), and
- C = weight of Nesbitt bulb before absorption of CO₂, g (step 32.3).

33.2 Correct the percentage of CO₃ obtained on the sample for a blank.

33.3 Calculate the weight percentage of carbonate, C_u, on a uranium basis as follows:

$$C_u = \frac{C_c \times 100}{U} \quad (6)$$

where:

- C_c = corrected percentage of carbonate in the sample (see 33.2), and