



Designation: **E363—16 E363 – 22**

## Standard Test Methods for Chemical Analysis of Chromium and Ferrochromium<sup>1</sup>

This standard is issued under the fixed designation E363; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon ( $\epsilon$ ) indicates an editorial change since the last revision or reapproval.

### 1. Scope

1.1 These test methods cover the chemical analysis of chromium and ferrochromium having chemical compositions within the following limits:

Element	Composition, %
Aluminum	0.25 max
Antimony	0.005 max
Arsenic	0.005 max
Bismuth	0.005 max
Boron	0.005 max
Carbon	9.00 max
Chromium	51.0 to 99.5
Chromium	51.0 to 75
Cobalt	0.10 max
Columbium	0.05 max
Copper	0.05 max
Lead	0.005 max
Manganese	0.75 max
Molybdenum	0.05 max
Nickel	0.50 max
Nitrogen	6.00 max
Phosphorus	0.03 max
Silicon	12.00 max
Silver	0.005 max
Sulfur	0.07 max
Tantalum	0.05 max
Tin	0.005 max
Titanium	0.50 max
Vanadium	0.50 max
Zinc	0.005 max
Zirconium	0.05 max

1.2 The analytical procedures appear in the following order:

<sup>1</sup> These test methods are under the jurisdiction of ASTM Committee E01 on Analytical Chemistry for Metals, Ores, and Related Materials and are the direct responsibility of Subcommittee E01.01 on Iron, Steel, and Ferroalloys.

Current edition approved May 1, 2016; Nov. 1, 2022. Published June 2016; November 2022. Originally approved in 1970. Last previous edition approved in 2009 as E363 – 09:16. DOI: [10.1520/E0363-16](https://doi.org/10.1520/E0363-16); [10.1520/E0363-22](https://doi.org/10.1520/E0363-22).

Arsenic by the Molybdenum Blue Spectrophotometric Test Method [0.001 % to 0.005 %]	Sections 10 – 20
Lead by the Dithizone Spectrophotometric Test Method [0.001 % to 0.05 %]	21 – 31
Chromium by the Sodium Peroxide Fusion-Titrimetric Test Method [50 % to 75 %]	32 – 38

1.3 **Units**—The values stated in SI units are to be regarded as standard. No other units of measurement are included in this standard.

1.4 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of whoever uses the user of this standard to consult and establish appropriate safety, health, and environmental practices and determine the applicability of regulatory limitations prior to use.* Specific hazard statements are given in Section 6 and in special “Warning” paragraphs throughout these test methods.

1.5 *This international standard was developed in accordance with internationally recognized principles on standardization established in the Decision on Principles for the Development of International Standards, Guides and Recommendations issued by the World Trade Organization Technical Barriers to Trade (TBT) Committee.*

## 2. Referenced Documents

### 2.1 ASTM Standards:<sup>2</sup>

[A101 Specification for Ferrochromium](#)

[A481 Specification for Chromium Metal](#)

[D1193 Specification for Reagent Water](#)

[E29 Practice for Using Significant Digits in Test Data to Determine Conformance with Specifications](#)

[E32 Practices for Sampling Ferroalloys and Steel Additives for Determination of Chemical Composition](#)

[E50 Practices for Apparatus, Reagents, and Safety Considerations for Chemical Analysis of Metals, Ores, and Related Materials](#)

[E60 Practice for Analysis of Metals, Ores, and Related Materials by Spectrophotometry](#)

[E135 Terminology Relating to Analytical Chemistry for Metals, Ores, and Related Materials](#)

[E173 Practice for Conducting Interlaboratory Studies of Methods for Chemical Analysis of Metals](#) (Withdrawn 1997)<sup>3</sup>

[E1601 Practice for Conducting an Interlaboratory Study to Evaluate the Performance of an Analytical Method](#)

[ASTM E363-22](#)

## 3. Terminology [standards.iteh.ai/catalog/standards/sist/acc9249b-109a-47ca-8042-19ea9deb855f/astm-e363-22](https://standards.iteh.ai/catalog/standards/sist/acc9249b-109a-47ca-8042-19ea9deb855f/astm-e363-22)

3.1 For definition of terms used in this test method, refer to Terminology [E135](#).

## 4. Significance and Use

4.1 These test methods for the chemical analysis of chromium metal and ferrochromium alloy are primarily intended to test such materials for compliance with compositional specifications such as Specifications [A101](#) and [A481](#). It is assumed that all who use these test methods will be trained analysts capable of performing common laboratory procedures skillfully and safely. It is expected that work will be performed in a properly equipped laboratory.

## 5. Apparatus, Reagents, and Spectrophotometric Practice

5.1 Apparatus, standard solutions, and other reagents required for each determination are listed in separate sections preceding the procedure. Spectrophotometers shall conform to the requirements prescribed in Practice [E60](#). (Note 1) (See [5.1.1](#).)

**Note 1**—In these methods, cells utilized to contain the reference material and sample solutions in spectrophotometers are referred to as “absorption cells.” The radiant energy passed through the cells can be measured as absorbance or transmittance. These methods refer to absorbance measurements. Refer to Practices [E60](#) for details.

<sup>2</sup> For referenced ASTM standards, visit the ASTM website, [www.astm.org](http://www.astm.org), or contact ASTM Customer Service at [service@astm.org](mailto:service@astm.org). For *Annual Book of ASTM Standards* volume information, refer to the standard’s Document Summary page on the ASTM website.

<sup>3</sup> The last approved version of this historical standard is referenced on [www.astm.org](http://www.astm.org).

5.1.1 In these methods, cells utilized to contain the reference material and sample solutions in spectrophotometers are referred to as “absorption cells.” The radiant energy passed through the cells can be measured as absorbance or transmittance. These methods refer to absorbance measurements. Refer to Practice E60 for details.

5.2 Spectrophotometric practices prescribed in these test methods shall conform to Practice E60.

5.3 *Purity of Water*—Unless otherwise indicated, references to water shall be understood to mean reagent water conforming to Type I or Type II of Specification D1193. Type III or Type IV may be used if they effect no measurable change in the blank or sample.

5.4 *Purity of Reagents*—Reagent grade chemicals shall be used in all tests. Unless otherwise indicated, it is intended that all reagents conform to the specifications of the Committee on Analytical Reagents of the American Chemical Society where such specifications are available.<sup>4</sup> Other grades may be used, provided it is first ascertained that the reagent is of sufficiently high purity to permit its use without lessening the accuracy of the determination.

## 6. Hazards

6.1 For precautions to be observed in the use of certain reagents in these test methods, refer to Practices E50.

6.2 Specific hazard statements are given in 27.1, ~~27.6~~27.7, and 36.2.

## 7. Sampling

7.1 For procedures to sample the material, and particle size requirements of the sample, refer to Practices E32.

## 8. Rounding Calculated Values

8.1 Calculated values shall be rounded to the desired number of places. Rounding of test results obtained using this test method shall be performed as directed in the Practice E29 Rounding Procedure of Practice, Rounding Method, unless E29 an alternative rounding method is specified by the customer or applicable material specification.

## 9. Interlaboratory Studies

9.1 These test methods have been evaluated in accordance with Practice E173, unless otherwise noted in the precision Precision and bias Bias section. Practice E173 has been replaced by Practice E1601. The Reproducibility  $R_2$  corresponds to the Reproducibility Index R of Practice E1601. The Repeatability  $R_1$  of Practice E173 corresponds to the Repeatability Index r of Practice E1601.

# ARSENIC BY THE MOLYBDENUM BLUE SPECTROPHOTOMETRIC TEST METHOD

## 10. Scope

10.1 This test method covers the determination of arsenic in chromium and ferrochromium in compositions from 0.001 % to 0.005 %.

## 11. Summary of Method

11.1 Arsenic is first separated by distillation as the trivalent chloride. Ammonium molybdate is added to form arsenomolybdate, which is then reduced by hydrazine sulfate to form the molybdenum blue complex. Spectrophotometric absorbance measurement is made at ~~850 nm~~850 nm.

<sup>4</sup> *Reagent Chemicals, American Chemical Society Specifications*, American Chemical Society, Washington, DC., [www.acs.org](http://www.acs.org). For suggestions on the testing of reagents not listed by the American Chemical Society, see the *United States Pharmacopeia and National Formulary*, U.S. Pharmacopeial Convention, Inc. (USPC), Rockville, MD, [www.usp.org](http://www.usp.org).

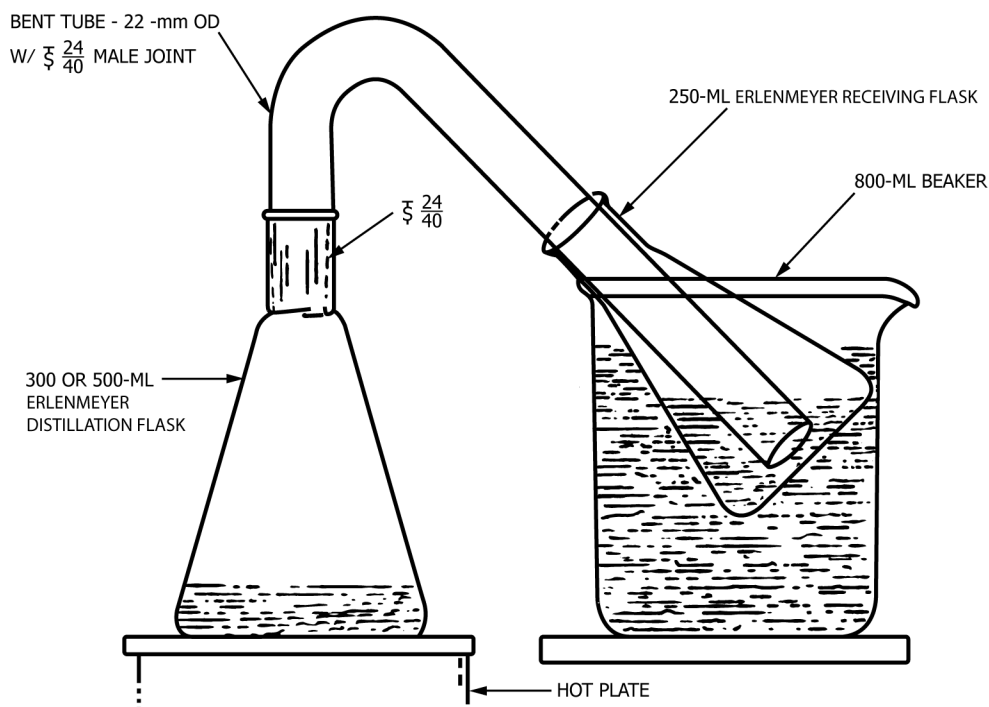


FIG. 1 Arsenic Distillation Apparatus

## 12. Concentration Range

12.1 The recommended concentration range is 0.01 mg to 0.15 mg of arsenic per 50 mL of solution using a 1-cm cell. (See Note 1.)

NOTE 1—This test method has been written for cells having a 1-cm light path. Cells having other dimensions may be used, provided suitable adjustments can be made in the amount of sample and reagents used.

## 13. Stability of Color

13.1 The color is stable for at least 2 h.

## 14. Interferences

14.1 The elements ordinarily present do not interfere if their compositions are under the maximum limits shown in 1.1.

## 15. Apparatus

15.1 Distillation Apparatus, Distillation Apparatus, Fig. 1.

15.2 Zirconium Crucibles, Zirconium Crucibles, 30-mL 30 mL capacity.

## 16. Reagents

16.1 Ammonium Bromide ( $\text{NH}_4\text{Br}$ ).

16.2 Ammonium Molybdate Solution (10 g/L)—Dissolve 2.5 g of ammonium heptamolybdate tetrahydrate ( $(\text{NH}_4)_6\text{Mo}_7\text{O}_{24} \cdot 4\text{H}_2\text{O}$ ) in 40 mL of warm water. Add 128 mL of  $\text{H}_2\text{SO}_4$  (1 + 3), dilute to 250 mL, and mix.

16.3 *Ammonium Molybdate-Hydrazine Sulfate Solution*—Dilute ~~100 mL~~ 100 mL of ammonium molybdate solution to ~~900 mL~~, add ~~10 mL~~ 900 mL, add 10 mL of hydrazine sulfate solution, dilute to ~~1 L~~, 1 L, and mix. Do not use a solution that has stood more than ~~1 h~~ 1 h.

16.4 *Arsenic, Standard Solution A* (~~1 mL = 0.10 mg As~~)—Transfer ~~0.1320 g~~ (~~1 mL = 0.10 mg As~~)—Transfer 0.1320 g of arsenic trioxide ( $\text{As}_2\text{O}_3$ ) to a ~~1 L~~ 1 L volumetric flask, dissolve in ~~100 mL~~ 100 mL of HCl, cool, dilute to volume, and mix.

16.5 *Arsenic, Standard Solution B* (~~1 mL = 0.01 mg As~~)—Using (~~1 mL = 0.01 mg As~~)—Using a pipet, transfer ~~100 mL~~ 100 mL of arsenic solution A (~~1 mL = 0.10 mg As~~) (~~1 mL = 0.10 mg As~~) to a ~~1 L~~ 1 L volumetric flask, dilute to volume, and mix.

16.6 *Hydrazine Sulfate* ( $(\text{NH}_2)_2\cdot\text{H}_2\text{SO}_4$ ).

16.7 *Hydrazine Sulfate Solution* (~~1.5 (1.5 g/g/L)~~)—Dissolve ~~1.5 g/L~~)—Dissolve 1.5 g of hydrazine sulfate ( $(\text{NH}_2)_2\cdot\text{H}_2\text{SO}_4$ ) in water, dilute to ~~1 L~~, 1 L, and mix. Do not use a solution that has stood more than 1 day.

16.8 *Sodium Carbonate* ( $\text{Na}_2\text{CO}_3$ ).

16.9 *Sodium Peroxide* ( $\text{Na}_2\text{O}_2$ ).

## 17. Preparation of Calibration Curve

17.1 *Calibration Solutions:*

17.1.1 Using pipets, transfer (~~1, 2, 5, 10, and 15~~) ~~mL~~ 15 mL of arsenic Solution B (~~1 mL = 0.01 mg As~~) to ~~125 mL~~ (~~1 mL = 0.01 mg As~~) to 125 mL Erlenmeyer flasks.

17.1.2 Add ~~10 mL~~ 10 mL of  $\text{HNO}_3$  and evaporate the solution to dryness on a hot plate. Bake for ~~30 min~~ 30 min at  $150\text{ }^\circ\text{C}$  to  $180\text{ }^\circ\text{C}$ . Remove from the hot plate. Add ~~45~~ Add 45 mL of ammonium molybdate-hydrazine sulfate solution to each flask, warm gently to dissolve the residue, and transfer the solution to a ~~50 mL~~ 50 mL volumetric flask. Proceed as directed in **17.3**.

17.2 *Reference Solution*—Transfer ~~10 mL~~ 10 mL of  $\text{HNO}_3$  to a ~~125 mL~~ 125 mL Erlenmeyer flask and proceed as directed in **17.1.2**.

17.3 *Color Development*—Heat the flask in a boiling water bath for ~~15 min~~ 15 min. Remove the flask, cool to room temperature, dilute to volume with ammonium molybdate-hydrazine sulfate solution, and mix.

17.4 *Spectrophotometry:*

17.4.1 *Multiple-Cell Spectrophotometer*—Measure the cell correction using absorption cells with a ~~1 cm~~ 1 cm light path and a light band centered at ~~850 nm~~ 850 nm. Using the test cell, take the spectrophotometric absorbance readings of the calibration solutions.

17.4.2 *Single-Cell Spectrophotometer*—Transfer a suitable portion of the reference solution to an absorption cell with a ~~1 cm~~ 1 cm light path and adjust the spectrophotometer to the initial setting, using a light band centered at ~~850 nm~~ 850 nm. While maintaining this adjustment, take the spectrophotometric absorbance readings of the calibration solutions.

17.5 *Calibration Curve*—Plot the net spectrophotometric absorbance readings of the calibration solutions against milligrams of arsenic per ~~50 mL~~ 50 mL of solution. Follow the instrument manufacturer's instructions for generating the calibration curve.

## 18. Procedure

18.1 *Test Solution:*

18.1.1 Select and weigh a sample to the nearest ~~0.2 mg~~ 0.2 mg as follows:

As, %	Sample Weight, g
As, %	Sample Mass, g
0.001 to 0.015	0.500
0.01 to 0.04	0.250
0.035 to 0.10	0.125

18.1.1.1 Transfer the sample to a ~~30-mL~~30 mL zirconium crucible containing 10 g of Na<sub>2</sub>O<sub>2</sub> and 1 g of Na<sub>2</sub>CO<sub>3</sub> if ferrochromium, or 8 g of Na<sub>2</sub>O<sub>2</sub> plus 2 g of Na<sub>2</sub>CO<sub>3</sub> if chromium metal.

18.1.2 Mix thoroughly with a metal spatula. Fuse carefully over a free flame by holding the crucible with a pair of tongs and slowly revolving it around the outer edge of the flame until the contents have completely melted; raise the temperature gradually to avoid spattering. When the contents are molten, give the crucible a rotary motion to ~~stir up~~ dissolve any ~~unattached~~ undissolved particles of the alloy adhering to the bottom or sides. Finally, increase the temperature until the crucible is bright red for ~~1 min.~~ 1 min. Cool the crucible to room temperature. Transfer the crucible to an ~~800-mL~~800 mL beaker containing ~~60 mL~~ 60 mL of H<sub>2</sub>SO<sub>4</sub> (1 + 1) and ~~200 mL~~ 200 mL of water. Dissolve the melt; remove and rinse the crucible.

18.1.3 If manganese dioxide is present, add H<sub>2</sub>SO<sub>4</sub> drop-wise until the solution clears.

18.1.4 Heat to boiling, and cool. While stirring vigorously, add NH<sub>4</sub>OH until the solution is alkaline to litmus, and then add ~~3 mL~~ to ~~5 mL~~ 3 mL to 5 mL in excess. Heat to boiling, remove from the heat, and allow the precipitate to settle. Filter on a coarse filter paper and wash five times with hot water. Discard the filtrate. Remove the filter paper, carefully open it, and place it on the inside wall of the original ~~800-mL~~800 mL beaker. Wash the precipitate from the paper using a fine stream of water. Pass ~~25 mL~~ 25 mL of HNO<sub>3</sub> (1 + 1) over the paper, and wash well with water but do not exceed a total volume of ~~40 mL~~ 40 mL. Discard the paper. Warm gently until the precipitate dissolves.

18.1.5 Transfer the solution to the distillation flask, add ~~1 g~~ 1 g of NH<sub>4</sub>Br and ~~0.75 g~~ 0.75 g of hydrazine sulfate. Add ~~20 mL~~ 20 mL of HNO<sub>3</sub> (1 + 1) to the receiving flask, and place the flask in an ~~800-mL~~800 mL beaker containing cold water. Assemble the apparatus (Fig. 1), heat the distillation flask, and distill into the receiving flask.

18.1.6 Distill until the volume is reduced to ~~10 mL~~ 10 mL or until oxides of nitrogen are noted in the distillation flask. Remove the distillation flask from the heat source. Place the receiving flask on a hot plate and evaporate the solution to dryness. Bake for ~~30 min~~ 30 min at 150 °C to 180 °C. Add ~~45 mL~~ 45 mL of ammonium molybdate-hydrazine sulfate solution to the flask, warm gently to dissolve the residue, and transfer the solution to a ~~50 mL~~ 50 mL volumetric flask. Proceed as directed in 18.3.

18.2 *Reference Solution*—Carry a reagent blank through the entire procedure using the same amounts of all reagents with the sample omitted. Proceed as directed in 18.3.

18.3 *Color Development*—Proceed as directed in 17.3.

18.4 *Spectrophotometry*—Take the spectrophotometric absorbance reading of the test solution as directed in 17.4.

## 19. Calculation

19.1 Convert the net spectrophotometric absorbance reading of the test solution to milligrams of arsenic by means of the calibration curve. Calculate the percentage of arsenic as follows:

$$\text{Arsenic, \%} = A/(B \times 10) \quad (1)$$

where:

*A* = milligrams of arsenic found in 50 mL of final test solution, and  
*B* = grams of sample represented in 50 mL of final test solution.

$\frac{A}{B}$  = milligrams of arsenic found in 50 mL of final test solution, and  
 $\frac{A}{B}$  = grams of sample represented in 50 mL of final test solution.

## 20. Precision and Bias

20.1 *Precision*—Nine laboratories cooperated in testing this test method and obtained the data summarized in Table 1. Samples

**TABLE 1 Statistical Information—Arsenic**

Ferroalloy Type	As Found, %	Repeatability ( $R_1$ , Practice <b>E173</b> )	Reproducibility ( $R_2$ , Practice <b>E173</b> )
1. 70Cr-1Si-5C	0.0015	0.0001	0.0005

with arsenic compositions near the upper limit of the scope were not available for testing. The user is cautioned to verify, by the use of reference materials, if available, that the precision and bias of this test method is adequate for the contemplated use.

20.2 Bias—No information on the bias of this is known because at the time of the interlaboratory study, suitable reference materials were not available or were not tested. The user of this method is encouraged to employ accepted reference materials, if available, to determine the presence or absence of bias.

## LEAD BY THE DITHIZONE SPECTROPHOTOMETRIC TEST METHOD

### 21. Scope

21.1 This test method covers the determination of lead in chromium and ferrochromium in compositions from 0.001 % to 0.05 %.

### 22. Summary of Test Method

22.1 After dissolution of the sample, lead is precipitated with  $\text{NH}_4\text{OH}$ . Interfering metals are complexed with sodium citrate and sodium cyanide, and the lead dithizone complex is extracted with chloroform. Spectrophotometric absorbance measurement is made at ~~520 nm~~ 520 nm.

### 23. Concentration Range

23.1 The recommended concentration range is from ~~0.001 mg to 0.025 mg~~ 0.001 mg to 0.025 mg of lead per ~~10 mL~~ 10 mL of solution, using a ~~1-cm~~ 1 cm cell.

**Note 3**—This test method has been written for cells having a 1-cm light path. Cells having other dimensions may be used, provided suitable adjustments can be made in the amounts of sample and reagents used.

### 24. Stability of Color

24.1 The color is quite stable if the solution is protected against evaporation and decomposition of chloroform. Because of the volatility of the solvent, it is advisable to make all readings promptly. The color develops almost immediately.

### 25. Interferences

25.1 The elements ordinarily present do not interfere if their compositions are under the maximum limits shown in 1.1. If more than 0.005 % bismuth is present, it must be removed as directed in 28.3.3 to avoid high results for lead.

### 26. Apparatus

26.1 *Glassware*—Use only borosilicate beakers, covers, and funnels. Wash all glassware with hot  $\text{HNO}_3$  (1 + 1) and reserve for this determination only. Before using separatory funnels, rinse them with dithizone solution and then with water. Store all reagents in glass-stoppered borosilicate bottles which have been previously washed with hot  $\text{HNO}_3$  (1 + 1) and rinsed with distilled water.

26.2 *pH Meter*—A pH meter for measurements to within  $\pm 0.10$  pH  $\pm 0.10$  pH units is required.

### 27. Reagents

27.1 *Chloroform* ( $\text{CHCl}_3$ )—(**Warning**—Chloroform is highly toxic and must be used in a well-ventilated hood. Consult the Safety Data Sheet or other source of data prior to use. Refer to the Hazards Section of Practices **E50**.)