



Designation: E363 – 23

# Standard Test Methods for Chemical Analysis of Chromium and Ferrochromium<sup>1</sup>

This standard is issued under the fixed designation E363; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon ( $\epsilon$ ) indicates an editorial change since the last revision or reapproval.

## 1. Scope

1.1 These test methods cover the chemical analysis of chromium and ferrochromium having chemical compositions within the following limits:

Element	Composition, %
Aluminum	0.25 max
Antimony	0.005 max
Arsenic	0.005 max
Bismuth	0.005 max
Boron	0.005 max
Carbon	9.00 max
Chromium	51.0 to 99.5
Cobalt	0.10 max
Columbium	0.05 max
Copper	0.05 max
Lead	0.005 max
Manganese	0.75 max
Molybdenum	0.05 max
Nickel	0.50 max
Nitrogen	6.00 max
Phosphorus	0.03 max
Silicon	12.00 max
Silver	0.005 max
Sulfur	0.07 max
Tantalum	0.05 max
Tin	0.005 max
Titanium	0.50 max
Vanadium	0.50 max
Zinc	0.005 max
Zirconium	0.05 max

1.2 The analytical procedures appear in the following order:

	Sections
Arsenic by the Molybdenum Blue Spectrophotometric Test Method [0.001 % to 0.005 %]	10 – 20
Lead by the Dithizone Spectrophotometric Test Method [0.001 % to 0.05 %]	21 – 31
Chromium by the Sodium Peroxide Fusion-Titrimetric Test Method [50.0 % to 99.5 %]	32 – 38

1.3 *Units*—The values stated in SI units are to be regarded as standard. No other units of measurement are included in this standard.

1.4 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the*

<sup>1</sup> These test methods are under the jurisdiction of ASTM Committee E01 on Analytical Chemistry for Metals, Ores, and Related Materials and are the direct responsibility of Subcommittee E01.01 on Iron, Steel, and Ferroalloys.

Current edition approved July 1, 2023. Published July 2023. Originally approved in 1970. Last previous edition approved in 2022 as E363 – 22. DOI: 10.1520/E0363-23.

*responsibility of the user of this standard to establish appropriate safety, health, and environmental practices and determine the applicability of regulatory limitations prior to use. Specific hazard statements are given in Section 6 and in special “Warning” paragraphs throughout these test methods.*

1.5 *This international standard was developed in accordance with internationally recognized principles on standardization established in the Decision on Principles for the Development of International Standards, Guides and Recommendations issued by the World Trade Organization Technical Barriers to Trade (TBT) Committee.*

## 2. Referenced Documents

### 2.1 ASTM Standards:<sup>2</sup>

- A101 Specification for Ferrochromium
- A481 Specification for Chromium Metal
- D1193 Specification for Reagent Water
- E29 Practice for Using Significant Digits in Test Data to Determine Conformance with Specifications
- E32 Practices for Sampling Ferroalloys and Steel Additives for Determination of Chemical Composition
- E50 Practices for Apparatus, Reagents, and Safety Considerations for Chemical Analysis of Metals, Ores, and Related Materials
- E60 Practice for Analysis of Metals, Ores, and Related Materials by Spectrophotometry
- E135 Terminology Relating to Analytical Chemistry for Metals, Ores, and Related Materials
- E173 Practice for Conducting Interlaboratory Studies of Methods for Chemical Analysis of Metals (Withdrawn 1997)<sup>3</sup>
- E1601 Practice for Conducting an Interlaboratory Study to Evaluate the Performance of an Analytical Method

## 3. Terminology

3.1 For definition of terms used in this test method, refer to Terminology E135.

<sup>2</sup> For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard’s Document Summary page on the ASTM website.

<sup>3</sup> The last approved version of this historical standard is referenced on www.astm.org.

#### 4. Significance and Use

4.1 These test methods for the chemical analysis of chromium metal and ferrochromium alloy are primarily intended to test such materials for compliance with compositional specifications such as Specifications **A101** and **A481**. It is assumed that all who use these test methods will be trained analysts capable of performing common laboratory procedures skillfully and safely. It is expected that work will be performed in a properly equipped laboratory.

#### 5. Apparatus, Reagents, and Spectrophotometric Practice

5.1 Apparatus, standard solutions, and other reagents required for each determination are listed in separate sections preceding the procedure. Spectrophotometers shall conform to the requirements prescribed in Practice **E60**. (See **5.1.1**.)

5.1.1 In these methods, cells utilized to contain the reference material and sample solutions in spectrophotometers are referred to as “absorption cells.” The radiant energy passed through the cells can be measured as absorbance or transmittance. These methods refer to absorbance measurements. Refer to Practice **E60** for details.

5.2 Spectrophotometric practices prescribed in these test methods shall conform to Practice **E60**.

5.3 *Purity of Water*—Unless otherwise indicated, references to water shall be understood to mean reagent water conforming to Type I or Type II of Specification **D1193**. Type III or Type IV may be used if they effect no measurable change in the blank or sample.

5.4 *Purity of Reagents*—Reagent grade chemicals shall be used in all tests. Unless otherwise indicated, it is intended that all reagents conform to the specifications of the Committee on Analytical Reagents of the American Chemical Society where such specifications are available.<sup>4</sup> Other grades may be used, provided it is first ascertained that the reagent is of sufficiently high purity to permit its use without lessening the accuracy of the determination.

#### 6. Hazards

6.1 For precautions to be observed in the use of certain reagents in these test methods, refer to Practices **E50**.

6.2 Specific hazard statements are given in **27.1**, **27.7**, and **36.2**.

#### 7. Sampling

7.1 For procedures to sample the material, and particle size requirements of the sample, refer to Practices **E32**.

#### 8. Rounding Calculated Values

8.1 Rounding of test results obtained using this test method shall be performed as directed in Practice **E29**, Rounding

Method, unless an alternative rounding method is specified by the customer or applicable material specification.

#### 9. Interlaboratory Studies

9.1 These test methods have been evaluated in accordance with Practice **E173**, unless otherwise noted in the Precision and Bias section. Practice **E173** has been replaced by Practice **E1601**. The Reproducibility  $R_2$  corresponds to the Reproducibility Index  $R$  of Practice **E1601**. The Repeatability  $R_1$  of Practice **E173** corresponds to the Repeatability Index  $r$  of Practice **E1601**.

### ARSENIC BY THE MOLYBDENUM BLUE SPECTROPHOTOMETRIC TEST METHOD

#### 10. Scope

10.1 This test method covers the determination of arsenic in chromium and ferrochromium in compositions from 0.001 % to 0.005 %.

#### 11. Summary of Method

11.1 Arsenic is first separated by distillation as the trivalent chloride. Ammonium molybdate is added to form arsenomolybdate, which is then reduced by hydrazine sulfate to form the molybdenum blue complex. Spectrophotometric absorbance measurement is made at 850 nm.

#### 12. Concentration Range

12.1 The recommended concentration range is 0.01 mg to 0.15 mg of arsenic per 50 mL of solution using a 1 cm cell. (See **Note 1**.)

**NOTE 1**—This test method has been written for cells having a 1 cm light path. Cells having other dimensions may be used, provided suitable adjustments can be made in the amount of sample and reagents used.

#### 13. Stability of Color

13.1 The color is stable for at least 2 h.

#### 14. Interferences

14.1 The elements ordinarily present do not interfere if their compositions are under the maximum limits shown in **1.1**.

#### 15. Apparatus

15.1 *Distillation Apparatus*, **Fig. 1**.

15.2 *Zirconium Crucibles*, 30 mL capacity.

#### 16. Reagents

16.1 *Ammonium Bromide* ( $\text{NH}_4\text{Br}$ ).

16.2 *Ammonium Molybdate Solution* (10 g/L)—Dissolve 2.5 g of ammonium heptamolybdate tetrahydrate ( $(\text{NH}_4)_6\text{Mo}_7\text{O}_{24} \cdot 4\text{H}_2\text{O}$ ) in 40 mL of warm water. Add 128 mL of  $\text{H}_2\text{SO}_4$  (1 + 3), dilute to 250 mL, and mix.

16.3 *Ammonium Molybdate-Hydrazine Sulfate Solution*—Dilute 100 mL of ammonium molybdate solution to 900 mL, add 10 mL of hydrazine sulfate solution, dilute to 1 L, and mix. Do not use a solution that has stood more than 1 h.

<sup>4</sup> *Reagent Chemicals, American Chemical Society Specifications*, American Chemical Society, Washington, DC., [www.acs.org](http://www.acs.org). For suggestions on the testing of reagents not listed by the American Chemical Society, see the *United States Pharmacopeia and National Formulary*, U.S. Pharmacopeial Convention, Inc. (USPC), Rockville, MD, [www.usp.org](http://www.usp.org).

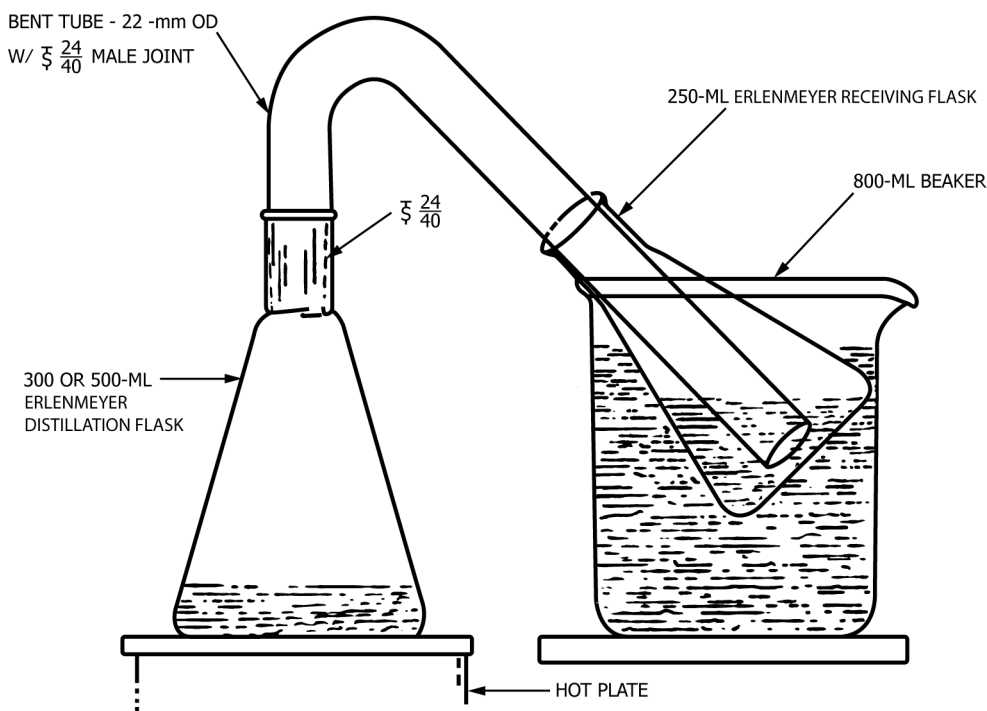


FIG. 1 Arsenic Distillation Apparatus

iTeh Standards

16.4 *Arsenic, Standard Solution A* (1 mL = 0.10 mg As)—Transfer 0.1320 g of arsenic trioxide ( $\text{As}_2\text{O}_3$ ) to a 1 L volumetric flask, dissolve in 100 mL of HCl, cool, dilute to volume, and mix.

16.5 *Arsenic, Standard Solution B* (1 mL = 0.01 mg As)—Using a pipet, transfer 100 mL of arsenic solution A (1 mL = 0.10 mg As) to a 1 L volumetric flask, dilute to volume, and mix.

16.6 *Hydrazine Sulfate* ( $(\text{NH}_2)_2\cdot\text{H}_2\text{SO}_4$ ).

16.7 *Hydrazine Sulfate Solution* (1.5 g/L)—Dissolve 1.5 g of hydrazine sulfate ( $(\text{NH}_2)_2\cdot\text{H}_2\text{SO}_4$ ) in water, dilute to 1 L, and mix. Do not use a solution that has stood more than 1 day.

16.8 *Sodium Carbonate* ( $\text{Na}_2\text{CO}_3$ ).

16.9 *Sodium Peroxide* ( $\text{Na}_2\text{O}_2$ ).

## 17. Preparation of Calibration Curve

### 17.1 Calibration Solutions:

17.1.1 Using pipets, transfer (1, 2, 5, 10, and 15) mL of arsenic Solution B (1 mL = 0.01 mg As) to 125 mL Erlenmeyer flasks.

17.1.2 Add 10 mL of  $\text{HNO}_3$  and evaporate the solution to dryness on a hot plate. Bake for 30 min at 150 °C to 180 °C. Remove from the hot plate. Add 45 mL of ammonium molybdate-hydrazine sulfate solution to each flask, warm gently to dissolve the residue, and transfer the solution to a 50 mL volumetric flask. Proceed as directed in 17.3.

17.2 *Reference Solution*—Transfer 10 mL of  $\text{HNO}_3$  to a 125 mL Erlenmeyer flask and proceed as directed in 17.1.2.

17.3 *Color Development*—Heat the flask in a boiling water bath for 15 min. Remove the flask, cool to room temperature, dilute to volume with ammonium molybdate-hydrazine sulfate solution, and mix.

### 17.4 Spectrophotometry:

17.4.1 *Multiple-Cell Spectrophotometer*—Measure the cell correction using absorption cells with a 1 cm light path and a light band centered at 850 nm. Using the test cell, take the spectrophotometric absorbance readings of the calibration solutions.

17.4.2 *Single-Cell Spectrophotometer*—Transfer a suitable portion of the reference solution to an absorption cell with a 1 cm light path and adjust the spectrophotometer to the initial setting, using a light band centered at 850 nm. While maintaining this adjustment, take the spectrophotometric absorbance readings of the calibration solutions.

17.5 *Calibration Curve*—Plot the net spectrophotometric absorbance readings of the calibration solutions against milligrams of arsenic per 50 mL of solution. Follow the instrument manufacturer's instructions for generating the calibration curve.

## 18. Procedure

### 18.1 Test Solution:

18.1.1 Select and weigh a sample to the nearest 0.2 mg as follows:

As, %	Sample Mass, g
0.001 to 0.015	0.500
0.01 to 0.04	0.250
0.035 to 0.10	0.125

18.1.1.1 Transfer the sample to a 30 mL zirconium crucible containing 10 g of Na<sub>2</sub>O<sub>2</sub> and 1 g of Na<sub>2</sub>CO<sub>3</sub> if ferrochromium, or 8 g of Na<sub>2</sub>O<sub>2</sub> plus 2 g of Na<sub>2</sub>CO<sub>3</sub> if chromium metal.

18.1.2 Mix thoroughly with a metal spatula. Fuse carefully over a free flame by holding the crucible with a pair of tongs and slowly revolving it around the outer edge of the flame until the contents have completely melted; raise the temperature gradually to avoid spattering. When the contents are molten, give the crucible a rotary motion to dissolve any undissolved particles of the alloy adhering to the bottom or sides. Finally, increase the temperature until the crucible is bright red for 1 min. Cool the crucible to room temperature. Transfer the crucible to an 800 mL beaker containing 60 mL of H<sub>2</sub>SO<sub>4</sub> (1 + 1) and 200 mL of water. Dissolve the melt; remove and rinse the crucible.

18.1.3 If manganese dioxide is present, add H<sub>2</sub>SO<sub>4</sub> dropwise until the solution clears.

18.1.4 Heat to boiling, and cool. While stirring vigorously, add NH<sub>4</sub>OH until the solution is alkaline to litmus, and then add 3 mL to 5 mL in excess. Heat to boiling, remove from the heat, and allow the precipitate to settle. Filter on a coarse filter paper and wash five times with hot water. Discard the filtrate. Remove the filter paper, carefully open it, and place it on the inside wall of the original 800 mL beaker. Wash the precipitate from the paper using a fine stream of water. Pass 25 mL of HNO<sub>3</sub> (1 + 1) over the paper, and wash well with water but do not exceed a total volume of 40 mL. Discard the paper. Warm gently until the precipitate dissolves.

18.1.5 Transfer the solution to the distillation flask, add 1 g of NH<sub>4</sub>Br and 0.75 g of hydrazine sulfate. Add 20 mL of HNO<sub>3</sub> (1 + 1) to the receiving flask, and place the flask in an 800 mL beaker containing cold water. Assemble the apparatus (Fig. 1), heat the distillation flask, and distill into the receiving flask.

18.1.6 Distill until the volume is reduced to 10 mL or until oxides of nitrogen are noted in the distillation flask. Remove the distillation flask from the heat source. Place the receiving flask on a hot plate and evaporate the solution to dryness. Bake for 30 min at 150 °C to 180 °C. Add 45 mL of ammonium molybdate-hydrazine sulfate solution to the flask, warm gently to dissolve the residue, and transfer the solution to a 50 mL volumetric flask. Proceed as directed in 18.3.

18.2 *Reference Solution*—Carry a reagent blank through the entire procedure using the same amounts of all reagents with the sample omitted. Proceed as directed in 18.3.

18.3 *Color Development*—Proceed as directed in 17.3.

18.4 *Spectrophotometry*—Take the spectrophotometric absorbance reading of the test solution as directed in 17.4.

## 19. Calculation

19.1 Convert the net spectrophotometric absorbance reading of the test solution to milligrams of arsenic by means of the calibration curve. Calculate the percentage of arsenic as follows:

$$\text{Arsenic, \%} = A/(B \times 10) \quad (1)$$

**TABLE 1 Statistical Information—Arsenic**

Ferroalloy Type	As Found, %	Repeatability ( <i>R</i> <sub>1</sub> , Practice E173)	Reproducibility ( <i>R</i> <sub>2</sub> , Practice E173)
1. 70Cr-1Si-5C	0.0015	0.0001	0.0005

where:

*A* = milligrams of arsenic found in 50 mL of final test solution,

*B* = grams of sample represented in 50 mL of final test solution, and

10 = conversion factor from mg to percent.

## 20. Precision and Bias

20.1 *Precision*—Nine laboratories cooperated in testing this test method and obtained the data summarized in Table 1. Samples with arsenic compositions near the upper limit of the scope were not available for testing. The user is cautioned to verify, by the use of reference materials, if available, that the precision of this test method is adequate for the contemplated use.

20.2 *Bias*—No information on the bias of this is known because at the time of the interlaboratory study, suitable reference materials were not available or were not tested. The user of this method is encouraged to employ accepted reference materials, if available, to determine the presence or absence of bias.

## LEAD BY THE DITHIZONE SPECTROPHOTOMETRIC TEST METHOD

### 21. Scope

21.1 This test method covers the determination of lead in chromium and ferrochromium in compositions from 0.001 % to 0.05 %.

### 22. Summary of Test Method

22.1 After dissolution of the sample, lead is precipitated with NH<sub>4</sub>OH. Interfering metals are complexed with sodium citrate and sodium cyanide, and the lead dithizone complex is extracted with chloroform. Spectrophotometric absorbance measurement is made at 520 nm.

### 23. Concentration Range

23.1 The recommended concentration range is from 0.001 mg to 0.025 mg of lead per 10 mL of solution, using a 1 cm cell.

### 24. Stability of Color

24.1 The color is quite stable if the solution is protected against evaporation and decomposition of chloroform. Because of the volatility of the solvent, it is advisable to make all readings promptly. The color develops almost immediately.

### 25. Interferences

25.1 The elements ordinarily present do not interfere if their compositions are under the maximum limits shown in 1.1. If



more than 0.005 % bismuth is present, it must be removed as directed in 28.3.3 to avoid high results for lead.

## 26. Apparatus

26.1 *Glassware*—Use only borosilicate beakers, covers, and funnels. Wash all glassware with hot  $\text{HNO}_3$  (1 + 1) and reserve for this determination only. Before using separatory funnels, rinse them with dithizone solution and then with water. Store all reagents in glass-stoppered borosilicate bottles which have been previously washed with hot  $\text{HNO}_3$  (1 + 1) and rinsed with distilled water.

26.2 *pH Meter*—A pH meter for measurements to within  $\pm 0.10$  pH units is required.

## 27. Reagents

27.1 *Chloroform* ( $\text{CHCl}_3$ )—(**Warning**—Chloroform is highly toxic and must be used in a well-ventilated hood. Consult the Safety Data Sheet or other source of data prior to use. Refer to the Hazards Section of Practices E50.)

27.2 *Dithizone Solution* (0.04 g/L in chloroform)—Dissolve 0.02 g of dithizone (diphenylthiocarbazone) in 80 mL of  $\text{CHCl}_3$  in a 500 mL conical separatory funnel, add 100 mL of cold water and 10 mL of  $\text{NH}_4\text{OH}$ , stopper, and shake vigorously for 1 min to 2 min. Draw off the  $\text{CHCl}_3$  layer and discard. Wash the aqueous layer with 5 mL of  $\text{CHCl}_3$  and discard the latter. Add  $\text{HCl}$  (1 + 9) to the aqueous layer until it is just acidic to litmus paper, cool, and extract with three 50 mL portions of  $\text{CHCl}_3$ . Combine the  $\text{CHCl}_3$  extracts, wash several times with water until the aqueous phase does not give an acid test with pH paper, and discard the aqueous layer. Dilute the  $\text{CHCl}_3$  layer to 500 mL with  $\text{CHCl}_3$  and store in an amber glass bottle preferably in a refrigerator.

27.3 *Hydroxylamine Hydrochloride Solution* (10 g/L)—Dissolve 0.5 g of hydroxylamine hydrochloride ( $\text{NH}_2\text{OH}\cdot\text{HCl}$ ) in 50 mL of water. Prepare fresh as needed.

27.4 *Iron Solution*—Dissolve 1 g of iron (lead content 0.001 % maximum) in 10 mL of  $\text{HCl}$  (1 + 1) and 10 mL of  $\text{HNO}_3$ . Add 10 mL of  $\text{HClO}_4$ , heat to strong fumes, cool, and dilute to 100 mL.

27.5 *Lead Standard Solution* (1 mL = 0.001 mg Pb)—Dissolve 0.2000 g of lead (purity 99.9 % minimum) in 20 mL of  $\text{HNO}_3$  (1 + 1), and heat moderately to expel oxides of nitrogen. Cool, transfer to a 1 L volumetric flask, dilute to volume, and mix. Using a pipet, transfer 5 mL of this solution to a 1 L volumetric flask, dilute to volume, and mix.

27.6 *Sodium Citrate Solution*—Dissolve 30 g of sodium citrate dihydrate in 100 mL of distilled water. Add  $\text{NH}_4\text{OH}$  until the pH is between 9.5 and 10.0. Add 10 mL of  $\text{CHCl}_3$  and 1 mL of dithizone solution, and shake. If the  $\text{CHCl}_3$  solution is red or gray, add a few drops more of the dithizone solution and shake again. Repeat until the color becomes green. Discard the organic layer and re-extract with a 10 mL portion of fresh  $\text{CHCl}_3$ . If the color becomes green, draw off the organic phase and then extract several more times with  $\text{CHCl}_3$  until the aqueous phase is colorless and the  $\text{CHCl}_3$  phase is almost colorless or very light green.

27.7 *Sodium Cyanide Solution* (300 g/L)—Dissolve 60 g of sodium cyanide ( $\text{NaCN}$ ) in 200 mL of water. Store in a polyethylene bottle. (**Warning**—The preparation, storage, use, and disposal of  $\text{NaCN}$  solutions requires special care and attention. Avoid any possibility of inhalation, ingestion, or skin contact with the compound, its solutions, or its vapors. Work only in a well-ventilated hood. Refer to the Hazards Section of Practices E50.)

NOTE 2—Because of the strongly alkaline properties of  $\text{NaCN}$  solutions, contact with borosilicate glass may result in contamination of the reagent.

27.8 *Sodium Sulfite Solution* (Saturated)—Prepare a saturated solution of sodium sulfite ( $\text{Na}_2\text{SO}_3$ ).

27.9 *Wash Solution*—Add 10 mL of  $\text{NH}_4\text{OH}$ , 40 mL of  $\text{Na}_2\text{SO}_3$  solution, and 20 mL of  $\text{NaCN}$  solution (**Warning**—See 27.7.) to 100 mL of water, and dilute to 1 L with water (Note 2).

## 28. Preparation of Calibration Curve

28.1 *Calibration Solutions*—Using pipets, transfer (1, 5, 10, 15, 20, and 25) mL of Standard Lead Solution (1 mL = 0.001 mg Pb) to 250 mL beakers and add enough water to make a total volume of approximately 25 mL. Proceed as directed in 28.3.

28.2 *Reference Solution*—Add 25 mL of water to a 250 mL beaker. Proceed as directed in 28.3.

### 28.3 Color Development:

28.3.1 In a well-ventilated hood, add 10 mL of sodium citrate solution, 10 mL of  $\text{Na}_2\text{SO}_3$  solution, and 10 mL of  $\text{NaCN}$  solution (**Warning**—See 27.7.), heat at 80 °C for 3 min, and cool. Using a pH meter, adjust the pH to  $10.5 \pm 0.2$  with  $\text{NH}_4\text{OH}$  (1 + 1) or  $\text{HCl}$  (1 + 1) as required. Cool to 10 °C and transfer to a 125 mL conical separatory funnel with a minimum of washing.

28.3.2 Using a pipet, transfer 10 mL of dithizone solution to the funnel, shake vigorously for 1 min, and allow the layers to separate. Draw off the lower  $\text{CHCl}_3$  layer into a second 125 mL separatory funnel containing 50 mL of wash solution. Shake for 30 s, allow the layers to separate, and drain off the lower  $\text{CHCl}_3$  layer into a third 125 mL separatory funnel containing 50 mL of wash solution. Shake for 30 s and allow the layers to separate thoroughly. Eliminate water droplets in the  $\text{CHCl}_3$  solution by transferring this solution to a clean, dry test tube before transferring to the absorption cell.

28.3.3 If more than 0.005 % bismuth is present in the sample, the  $\text{CHCl}_3$  layer should be back-washed with a solution of hydroxylamine hydrochloride (10 g/L) adjusted to a pH of 3.0.

### 28.4 Spectrophotometry:

28.4.1 *Multiple-Cell Spectrophotometer*—Measure the cell correction using the reference solution (28.2) in absorption cells with a 1 cm light path and using a light band centered at 520 nm. Using the test cell, take spectrophotometric absorbance readings of the calibration solutions versus the reference solution (28.2).

28.4.2 *Single-Cell Spectrophotometer*—Transfer a suitable portion of the reference solution (28.2) to an absorption cell