

INTERNATIONAL STANDARD

NORME INTERNATIONALE

INTERNATIONAL SPECIAL COMMITTEE ON RADIO INTERFERENCE
COMITÉ INTERNATIONAL SPÉCIAL DES PERTURBATIONS RADIOÉLECTRIQUES

**Specification for radio disturbance and immunity measuring apparatus and methods –
Part 1-1: Radio disturbance and immunity measuring apparatus – Measuring apparatus**

**Spécifications des méthodes et des appareils de mesure des perturbations radioélectriques et de l'immunité aux perturbations radioélectriques –
Partie 1-1: Appareils de mesure des perturbations radioélectriques et de l'immunité aux perturbations radioélectriques – Appareils de mesure**



THIS PUBLICATION IS COPYRIGHT PROTECTED

Copyright © 2007 IEC, Geneva, Switzerland

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either IEC or IEC's member National Committee in the country of the requester.

If you have any questions about IEC copyright or have an enquiry about obtaining additional rights to this publication, please contact the address below or your local IEC member National Committee for further information.

Droits de reproduction réservés. Sauf indication contraire, aucune partie de cette publication ne peut être reproduite ni utilisée sous quelque forme que ce soit et par aucun procédé, électronique ou mécanique, y compris la photocopie et les microfilms, sans l'accord écrit de la CEI ou du Comité national de la CEI du pays du demandeur.

Si vous avez des questions sur le copyright de la CEI ou si vous désirez obtenir des droits supplémentaires sur cette publication, utilisez les coordonnées ci-après ou contactez le Comité national de la CEI de votre pays de résidence.

IEC Central Office
3, rue de Varembe
CH-1211 Geneva 20
Switzerland
Email: inmail@iec.ch
Web: www.iec.ch

About the IEC

The International Electrotechnical Commission (IEC) is the leading global organization that prepares and publishes International Standards for all electrical, electronic and related technologies.

About IEC publications

The technical content of IEC publications is kept under constant review by the IEC. Please make sure that you have the latest edition, a corrigenda or an amendment might have been published.

- Catalogue of IEC publications: www.iec.ch/searchpub

The IEC on-line Catalogue enables you to search by a variety of criteria (reference number, text, technical committee,...). It also gives information on projects, withdrawn and replaced publications.

- IEC Just Published: www.iec.ch/online_news/justpub

Stay up to date on all new IEC publications. Just Published details twice a month all new publications released. Available on-line and also by email.

- Electropedia: www.electropedia.org

The world's leading online dictionary of electronic and electrical terms containing more than 20 000 terms and definitions in English and French, with equivalent terms in additional languages. Also known as the International Electrotechnical Vocabulary online.

- Customer Service Centre: www.iec.ch/webstore/custserv

If you wish to give us your feedback on this publication or need further assistance, please visit the Customer Service Centre FAQ or contact us:

Email: csc@iec.ch
Tel.: +41 22 919 02 11
Fax: +41 22 919 03 00

A propos de la CEI

La Commission Electrotechnique internationale (CEI) est la première organisation mondiale qui élabore et publie des normes internationales pour tout ce qui a trait à l'électricité, à l'électronique et aux technologies apparentées.

A propos des publications CEI

Le contenu technique des publications de la CEI est constamment revu. Veuillez vous assurer que vous possédez l'édition la plus récente, un corrigendum ou amendement peut avoir été publié.

- Catalogue des publications de la CEI: www.iec.ch/searchpub/cur_fut-f.htm

Le Catalogue en-ligne de la CEI vous permet d'effectuer des recherches en utilisant différents critères (numéro de référence, texte, comité d'études,...). Il donne aussi des informations sur les projets et les publications retirées ou remplacées.

- Just Published CEI: www.iec.ch/online_news/justpub

Restez informé sur les nouvelles publications de la CEI. Just Published détaille deux fois par mois les nouvelles publications parues. Disponible en-ligne et aussi par email.

- Electropedia: www.electropedia.org

Le premier dictionnaire en ligne au monde de termes électroniques et électriques. Il contient plus de 20 000 termes et définitions en anglais et en français, ainsi que les termes équivalents dans les langues additionnelles. Egalement appelé Vocabulaire Electrotechnique International en ligne.

- Service Clients: www.iec.ch/webstore/custserv/custserv_entry-f.htm

Si vous désirez nous donner des commentaires sur cette publication ou si vous avez des questions, visitez le FAQ du Service clients ou contactez-nous:

Email: csc@iec.ch
Tél.: +41 22 919 02 11
Fax: +41 22 919 03 00

INTERNATIONAL STANDARD

NORME INTERNATIONALE

INTERNATIONAL SPECIAL COMMITTEE ON RADIO INTERFERENCE
COMITÉ INTERNATIONAL SPÉCIAL DES PERTURBATIONS RADIOÉLECTRIQUES

**Specification for radio disturbance and immunity measuring apparatus and methods –
Part 1-1: Radio disturbance and immunity measuring apparatus – Measuring apparatus**

**Spécifications des méthodes et des appareils de mesure des perturbations radioélectriques et de l'immunité aux perturbations radioélectriques –
Partie 1-1: Appareils de mesure des perturbations radioélectriques et de l'immunité aux perturbations radioélectriques – Appareils de mesure**

INTERNATIONAL
ELECTROTECHNICAL
COMMISSION

COMMISSION
ELECTROTECHNIQUE
INTERNATIONALE

PRICE CODE
CODE PRIX

CR

CONTENTS

FOREWORD.....	4
1 Scope.....	6
2 Normative references	6
3 Terms and definitions	7
4 Quasi-peak measuring receivers for the frequency range 9 kHz to 1 000 MHz.....	9
5 Measuring receivers with peak detector for the frequency range 9 kHz to 18 GHz	22
6 Measuring receivers with average detector for the frequency range 9 kHz to 18 GHz.....	26
7 Measuring receivers with rms-average detector for the frequency range 9 kHz to 18 GHz.....	30
8 Measuring receivers for the frequency range 1 GHz to 18 GHz with amplitude probability distribution (APD) measuring function	35
9 Disturbance analyzers	36
Annex A (normative) Determination of response to repeated pulses of quasi-peak and rms-average measuring receivers	45
Annex B (normative) Determination of pulse generator spectrum	50
Annex C (normative) Accurate measurements of the output of nanosecond pulse generators	52
Annex D (normative) Influence of the quasi-peak measuring receiver characteristics on its pulse response	54
Annex E (normative) Response of average and peak measuring receivers	55
Annex F (normative) Performance check of the exceptions from the definitions of a click according to 4.2.3 of CISPR 14-1.....	64
Annex G (informative) Rationale for the specifications of the APD measuring function.....	71
Bibliography.....	74
Figure 1 – Pulse response curves	14
Figure 2 – Limits of overall selectivity	18
Figure 3 – Arrangement for testing intermodulation effects	19
Figure 4 – Block diagram of an average detector.....	29
Figure 5 – Response of the meter simulating network to an intermittent narrowband signal	29
Figure 6 – Example of a disturbance analyzer.....	38
Figure 7 – A graphical presentation of test signals used in the test of the analyzer for the performance check against the definition of a click according to Table 14.....	39
Figure 8 – Limits for the overall selectivity – pass band (Band E).....	25
Figure E.1 – Correction factor for estimating the ratio B_{imp}/B_6 for other tuned circuits.....	56
Figure E.2 – Pulse rectification coefficient P	58
Figure E.3 – Example (spectrum) of a pulse-modulated signal with a pulse width of 200 ns.....	60

Figure E.4 – Pulse-modulated RF signal applied to a measuring receiver	61
Figure E.5 – Filtering with a B_{imp} much smaller than the prf	61
Figure E.6– Filtering with a B_{imp} much wider than the prf.....	61
Figure E.7 – Calculation of the impulse bandwidth	62
Figure E.8 – Example of a normalized linear selectivity function.	63
Figure F.1 – A graphical presentation of the test signals used for the performance check of the analyzer with the additional requirements according to Table F.1.....	70
Figure G.1 – Block diagram of APD measurement circuit without A/D converter.....	72
Figure G.2 – Block diagram of APD measurement circuit with A/D converter.....	72
Figure G.3 – Example of display of APD measurement	73
Table 1 – Fundamental characteristics of quasi-peak receivers.....	10
Table 2 – Test pulse characteristics for quasi-peak measuring receivers	11
Table 3 – Pulse response of quasi-peak receivers	15
Table 4 – Bandwidth characteristics for intermodulation test of quasi-peak measuring receivers.....	20
Table 5 – VSWR requirements for receiver input impedance.....	22
Table 6 – Bandwidth requirements.....	22
Table 7 – Relative pulse response of peak and quasi-peak measuring receivers for the same bandwidth (frequency range 9 kHz to 1 000 MHz).....	24
Table 8 – Bandwidth requirements.....	26
Table 9 – Relative pulse response of average and quasi-peak measuring receivers for the same bandwidth (frequency range 9 kHz to 1 GHz).....	27
Table 10 – Maximum reading of average measuring receivers for a pulse-modulated sine-wave input in comparison with the response to a continuous sine-wave having the same amplitude.....	29
Table 14 – Disturbance analyzer performance test – Test signals used for the check against the definition of a click	40
Table 15 – VSWR requirements of input impedance.....	31
Table 16 – Bandwidth requirements.....	31
Table 17 – Minimum pulse repetition rate without overload	32
Table 18 – Relative pulse response of rms-average and quasi-peak measuring receivers.....	33
Table 19 – Pulse response of rms-average receiver.....	33
Table 20 – Maximum reading of rms-average measuring receivers for a pulse- modulated sine-wave input in comparison with the response to a continuous sine-wave having the same amplitude	34
Table B.1 – Pulse generator characteristics	50
Table E.1 – Carrier level for pulse-modulated signal of 1,4 nVs	59
Table F.1 – Disturbance analyzer test signals	65

INTERNATIONAL ELECTROTECHNICAL COMMISSION
INTERNATIONAL SPECIAL COMMITTEE ON RADIO INTERFERENCE

**SPECIFICATION FOR RADIO DISTURBANCE AND IMMUNITY
MEASURING APPARATUS AND METHODS –**

**Part 1-1: Radio disturbance and immunity measuring apparatus –
Measuring apparatus**

FOREWORD

- 1) The International Electrotechnical Commission (IEC) is a worldwide organization for standardization comprising all national electrotechnical committees (IEC National Committees). The object of IEC is to promote international co-operation on all questions concerning standardization in the electrical and electronic fields. To this end and in addition to other activities, IEC publishes International Standards, Technical Specifications, Technical Reports, Publicly Available Specifications (PAS) and Guides (hereafter referred to as "IEC Publication(s)"). Their preparation is entrusted to technical committees; any IEC National Committee interested in the subject dealt with may participate in this preparatory work. International, governmental and non-governmental organizations liaising with the IEC also participate in this preparation. IEC collaborates closely with the International Organization for Standardization (ISO) in accordance with conditions determined by agreement between the two organizations.
- 2) The formal decisions or agreements of IEC on technical matters express, as nearly as possible, an international consensus of opinion on the relevant subjects since each technical committee has representation from all interested IEC National Committees.
- 3) IEC Publications have the form of recommendations for international use and are accepted by IEC National Committees in that sense. While all reasonable efforts are made to ensure that the technical content of IEC Publications is accurate, IEC cannot be held responsible for the way in which they are used or for any misinterpretation by any end user.
- 4) In order to promote international uniformity, IEC National Committees undertake to apply IEC Publications transparently to the maximum extent possible in their national and regional publications. Any divergence between any IEC Publication and the corresponding national or regional publication shall be clearly indicated in the latter.
- 5) IEC provides no marking procedure to indicate its approval and cannot be rendered responsible for any equipment declared to be in conformity with an IEC Publication.
- 6) All users should ensure that they have the latest edition of this publication.
- 7) No liability shall attach to IEC or its directors, employees, servants or agents including individual experts and members of its technical committees and IEC National Committees for any personal injury, property damage or other damage of any nature whatsoever, whether direct or indirect, or for costs (including legal fees) and expenses arising out of the publication, use of, or reliance upon, this IEC Publication or any other IEC Publications.
- 8) Attention is drawn to the Normative references cited in this publication. Use of the referenced publications is indispensable for the correct application of this publication.
- 9) Attention is drawn to the possibility that some of the elements of this IEC Publication may be the subject of patent rights. IEC shall not be held responsible for identifying any or all such patent rights.

International Standard CISPR 16-1-1 has been prepared by CISPR subcommittee A: Radio interference measurements and statistical methods.

This consolidated version of CISPR 16-1-1 consists of the second edition (2006) [documents CISPR/A/642/FDIS and CISPR/A/651/RVD], its amendment 1 (2006) [documents CISPR/A/647/CDV and CISPR/A/686/RVC] and its amendment 2 (2007) [documents CISPR/A/737/FDIS and CISPR/A/751/RVD].

The technical content is therefore identical to the base edition and its amendments and has been prepared for user convenience.

It bears the edition number 2.2.

A vertical line in the margin shows where the base publication has been modified by amendments 1 and 2.

This publication has been drafted in accordance with the ISO/IEC Directives, Part 2.

The CISPR 16 series, published under the general title *Specification for radio disturbance and immunity measuring apparatus and methods*, consists of Parts 1, 2, 3 and 4, each of which is further subdivided into parts:

- measurement instrumentation specifications are given in the five parts of CISPR 16-1;
- methods of measurement are covered in the four parts of CISPR 16-2;
- various reports with further information and background on CISPR and radio disturbances in general are given in CISPR 16-3;
- information related to uncertainties, statistics and limit modelling is contained in CISPR 16-4.

CISPR 16-1 consists of the following parts, under the general title *Specification for radio disturbance and immunity measuring apparatus and methods – Radio disturbance and immunity measuring apparatus*:

- Part 1-1: Measuring apparatus
- Part 1-2: Ancillary equipment – Conducted disturbances
- Part 1-3: Ancillary equipment – Disturbance power
- Part 1-4: Ancillary equipment – Radiated disturbances
- Part 1-5: Antenna calibration test sites for 30 MHz to 1 000 MHz

The committee has decided that the contents of the base publication and its amendments will remain unchanged until the maintenance result date indicated on the IEC web site under "<http://webstore.iec.ch>" in the data related to the specific publication. At this date, the publication will be

- reconfirmed,
- withdrawn,
- replaced by a revised edition, or
- amended.

SPECIFICATION FOR RADIO DISTURBANCE AND IMMUNITY MEASURING APPARATUS AND METHODS –

Part 1-1: Radio disturbance and immunity measuring apparatus – Measuring apparatus

1 Scope

This part of CISPR 16 is designated a basic standard, which specifies the characteristics and performance of equipment for the measurement of radio disturbance voltages, currents and fields in the frequency range 9 kHz to 18 GHz. In addition, requirements are specified for specialized equipment for discontinuous disturbance measurements. The requirements include the measurement of broadband and narrowband types of radio disturbance.

The receiver types covered include the following:

- a) the quasi-peak measuring receiver,
- b) the peak measuring receiver,
- c) the average measuring receiver,
- d) the rms-average measuring receiver.

The requirements of this publication shall be complied with at all frequencies and for all levels of radio disturbance voltages, currents, power or field strengths within the CISPR indicating range of the measuring equipment.

Methods of measurement are covered in Part 2, and further information on radio disturbance is given in Part 3 of CISPR 16. Uncertainties, statistics and limit modelling are covered in Part 4 of CISPR 16.

2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

IEC 60050-161:1990, *International Electrotechnical Vocabulary (IEV) – Chapter 161: Electromagnetic compatibility*

Amendment 1 (1997)

Amendment 2 (1998)

CISPR 11:2003, *Industrial, scientific and medical (ISM) radio-frequency equipment – Electromagnetic disturbance characteristics – Limits and methods of measurement*

CISPR 14-1:2005, *Electromagnetic compatibility – Requirements for household appliances, electric tools and similar apparatus – Part 1: Emission*

CISPR 16-3:2003, *Specification for radio disturbance and Immunity measuring apparatus and methods – Part 3: CISPR technical reports*

BIPM / IEC / IFCC / ISO / IUPAC / IUPAP / OIML:1993, *International vocabulary of basic and general terms in metrology*

3 Terms and definitions

For the purpose of this document, the following definitions apply. Also see IEC 60050(161) and the *International vocabulary of basic and general terms in metrology*.

3.1 bandwidth

B_n

the width of the overall selectivity curve of the receiver between two points at a stated attenuation, below the midband response. The bandwidth is represented by the symbol B_n , where n is the stated attenuation in decibels.

3.2 impulse bandwidth

B_{imp}

$$B_{\text{imp}} = A(t)_{\text{max}} / (2 G_0 \times IS)$$

where

$A(t)_{\text{max}}$ is the peak of the envelope at the IF output of the receiver with an impulse area IS applied at the receiver input;

G_0 is the gain of the circuit at the centre frequency.

Specifically for two critically-coupled tuned transformers,

$$B_{\text{imp}} = 1,05 \times B_6 = 1,31 \times B_3$$

where

B_6 and B_3 are respectively the bandwidths at the -6 dB and -3 dB points (see Clause A.2 for further information).

3.3 impulse area

IS

the impulse area (sometimes called impulse strength, IS) is the voltage-time area of a pulse defined by the integral:

$$IS = \int_{-\infty}^{+\infty} V(t) dt \text{ (expressed in } \mu\text{Vs or dB}(\mu\text{Vs))}$$

NOTE Spectral density (D) is related to impulse area and expressed in $\mu\text{V/MHz}$ or $\text{dB}(\mu\text{V/MHz})$. For rectangular impulses of pulse duration T at frequencies $f \ll 1/T$, the relationship $D (\mu\text{V/MHz}) = \sqrt{2} \times 10^6 IS (\mu\text{Vs})$ applies.

3.4 electrical charge time constant

T_c

the time needed after the instantaneous application of a constant sine-wave voltage to the stage immediately preceding the input of the detector for the output voltage of the detector to reach 63 % of its final value

NOTE This time constant is determined as follows: A sine-wave signal of constant amplitude and having a frequency equal to the mid-band frequency of the i.f. amplifier is applied to the input of the stage immediately preceding the detector. The indication, D , of an instrument having no inertia (e.g., a cathode-ray oscilloscope) connected to a terminal in the d.c. amplifier circuit so as not to affect the behaviour of the detector, is noted. The level of the signal is chosen such that the response of the stages concerned remains within the linear operating range. A sine-wave signal of this level, applied for a limited time only and having a wave train of rectangular envelope is gated such that the deflection registered is 0,63 D . The duration of this signal is equal to the charge time of the detector.

3.5 electrical discharge time constant

T_D
the time needed after the instantaneous removal of a constant sine-wave voltage applied to the stage immediately preceding the input of the detector for the output of the detector to fall to 37 % of its initial value

NOTE The method of measurement is analogous to that for the charge time constant, but instead of a signal being applied for a limited time, the signal is interrupted for a definite time. The time taken for the deflection to fall to 0,37 D is the discharge time constant of the detector.

3.6 mechanical time constant of a critically damped indicating instrument

T_M

$$T_M = T_L / 2\pi$$

where

T_L is the period of free oscillation of the instrument with all damping removed.

NOTE 1 For a critically damped instrument, the equation of motion of the system may be written as:

$$T_M^2 (d^2\alpha / dt^2) + 2T_M (d\alpha / dt) + \alpha = ki$$

where

α is the deflection;

i is the current through the instrument;

k is a constant.

It can be deduced from this relation that this time constant is also equal to the duration of a rectangular pulse (of constant amplitude) that produces a deflection equal to 35 % of the steady deflection produced by a continuous current having the same amplitude as that of the rectangular pulse.

NOTE 2 The methods of measurement and adjustment are deduced from one of the following:

- The period of free oscillation having been adjusted to $2\pi T_M$, damping is added so that $\alpha T = 0,35\alpha_{\max}$.
- When the period of oscillation cannot be measured, the damping is adjusted to be just below critical such that the overshoot is not greater than 5 % and the moment of inertia of the movement is such that $\alpha T = 0,35\alpha_{\max}$.

<https://standards.iteh.ai/en/standards/iec/5337a05f4-b1d6-4d09-a228-9343e02cf441/cispr-16-1-1-2006>

3.7 overload factor

the ratio of the level that corresponds to the range of practical linear function of a circuit (or a group of circuits) to the level that corresponds to full-scale deflection of the indicating instrument

The maximum level at which the steady-state response of a circuit (or group of circuits) does not depart by more than 1 dB from ideal linearity defines the range of practical linear function of the circuit (or group of circuits).

3.8 symmetric voltage

in a two-wire circuit, such as a single-phase mains supply, the symmetric voltage is the radio-frequency disturbance voltage appearing between the two wires. This is sometimes called the differential mode voltage. If V_a is the vector voltage between one of the mains terminals and earth and V_b is the vector voltage between the other mains terminal and earth, the symmetric voltage is the vector difference ($V_a - V_b$)

3.9 CISPR indicating range

it is the range specified by the manufacturer which gives the maximum and the minimum meter indications within which the receiver meets the requirements of this section of CISPR 16

3.10

weighting (of e.g. impulsive disturbance)

the pulse-repetition-frequency (PRF) dependent conversion (mostly reduction) of a peak-detected impulse voltage level to an indication that corresponds to the interference effect on radio reception

- For the analogue receiver, the psychophysical annoyance of the interference is a subjective quantity (audible or visual, usually not a certain number of misunderstandings of a spoken text).
- For the digital receiver, the interference effect is an objective quantity that may be defined by the critical bit error ratio (BER) (or bit error probability (BEP)) for which perfect error correction can still occur or by another, objective and reproducible parameter.

3.10.1

weighting characteristic

the peak voltage level as a function of PRF for a constant effect on a specific radiocommunication system, i.e., the disturbance is weighted by the radiocommunication system itself

3.10.2

weighting function or weighting curve

the relationship between input peak voltage level and PRF for constant level indication of a measuring receiver with a weighting detector, i.e. the curve of response of a measuring receiver to repeated pulses

3.10.3

weighting factor

the value in dB of the weighting function relative to a reference PRF or relative to the peak value

3.10.4

weighting detector

detector which provides an agreed weighting function

3.10.5

weighted disturbance measurement

measurement of disturbance using a weighting detector

4 Quasi-peak measuring receivers for the frequency range 9 kHz to 1 000 MHz

The receiver specification depends on the frequency of operation. There is one receiver specification covering the frequency range 9 kHz to 150 kHz (band A), one covering 150 kHz to 30 MHz (band B), one covering 30 MHz to 300 MHz (band C), and one covering 300 MHz to 1 000 MHz (band D).

4.1 Input impedance

The input circuit of measuring receivers shall be unbalanced. For receiver control settings within the CISPR indicating range, the input impedance shall be nominally 50 Ω with a v.s.w.r. not to exceed 2,0 to 1 when the RF attenuation is 0 and 1,2 to 1 when the RF attenuation is 10 dB or greater.

Symmetric input impedance in the frequency range 9 kHz to 30 MHz: to permit symmetrical measurements a balanced input transformer is used. The preferred input impedance for the frequency range 9 kHz to 150 kHz is 600 Ω . This symmetric input impedance may be incorporated either in the relevant symmetrical artificial network necessary to couple to the receiver or optionally in the measuring receiver.

4.2 Fundamental characteristics

The responses to pulses as specified in 4.4 are calculated on the basis of the measuring receivers having the following fundamental characteristics.

Table 1 – Fundamental characteristics of quasi-peak receivers

Characteristics	Frequency band		
	Band A 9 kHz to 150 kHz	Band B 0,15 MHz to 30 MHz	Bands C and D 30 MHz to 1 000 MHz
Bandwidth at the -6 dB points, B ₆ in kHz	0,20	9	120
Detector electrical charge time constant, in ms	45	1	1
Detector electrical discharge time constant, in ms	500	160	550
Mechanical time constant of critically damped indicating instrument, in ms	160	160	100
Overload factor of circuits preceding the detector, in dB	24	30	43,5
Overload factor of the d.c. amplifier between detector and indicating instrument, in dB	6	12	6

NOTE 1 The definition of mechanical time constant (see 3.6) assumes that the indicating instrument is linear, i.e., equal increments of current produce equal increments of deflection. An indicating instrument having a different relation between current and deflection may be used provided that the instrument satisfies the requirements of this subclause. In an electronic instrument, the mechanical time-constant may be simulated by a circuit.

NOTE 2 No tolerance is given for the electrical and mechanical constants. The actual values used in a specific receiver will be determined by the design to meet the requirements in 4.4

4.3 Sine-wave voltage accuracy

The accuracy of measurement of sine-wave voltages shall be better than ±2 dB when supplied with a sine-wave signal at 50 Ω resistance source impedance.

4.4 Response to pulses

NOTE Annexes B and C describe methods for determining the output characteristics of a pulse generator for use in testing the requirements of this subclause.

4.4.1 Amplitude relationship (absolute calibration)


The response of the measuring receiver to pulses of impulse area of a) μVs (microvolt second) e.m.f. at 50 Ω source impedance, having a uniform spectrum up to at least b) MHz, repeated at a frequency of c) Hz shall, for all frequencies of tuning, be equal to the response to an unmodulated sine-wave signal at the tuned frequency having an e.m.f. of r.m.s. value 2 mV (66 dB(μV)). The source impedances of the pulse generator and the signal generator shall both be the same. A tolerance of ±1,5 dB shall be permitted on the sine-wave voltage level.

Table 2 – Test pulse characteristics for quasi-peak measuring receivers


Frequency range	a) μ Vs	b) MHz	c) Hz
9 kHz to 150 kHz	13,5	0,15	25
0,15 MHz to 30 MHz	0,316	30	100
30 MHz to 300 MHz	0,044	300	100
300 MHz to 1 000 MHz	0,044	1 000	100

4.4.2 Variation with repetition frequency (relative calibration)

The response of the measuring receiver to repeated pulses shall be such that for a constant indication on the measuring receiver, the relationship between amplitude and repetition frequency is in accordance with Figures 1a, 1b or 1c.

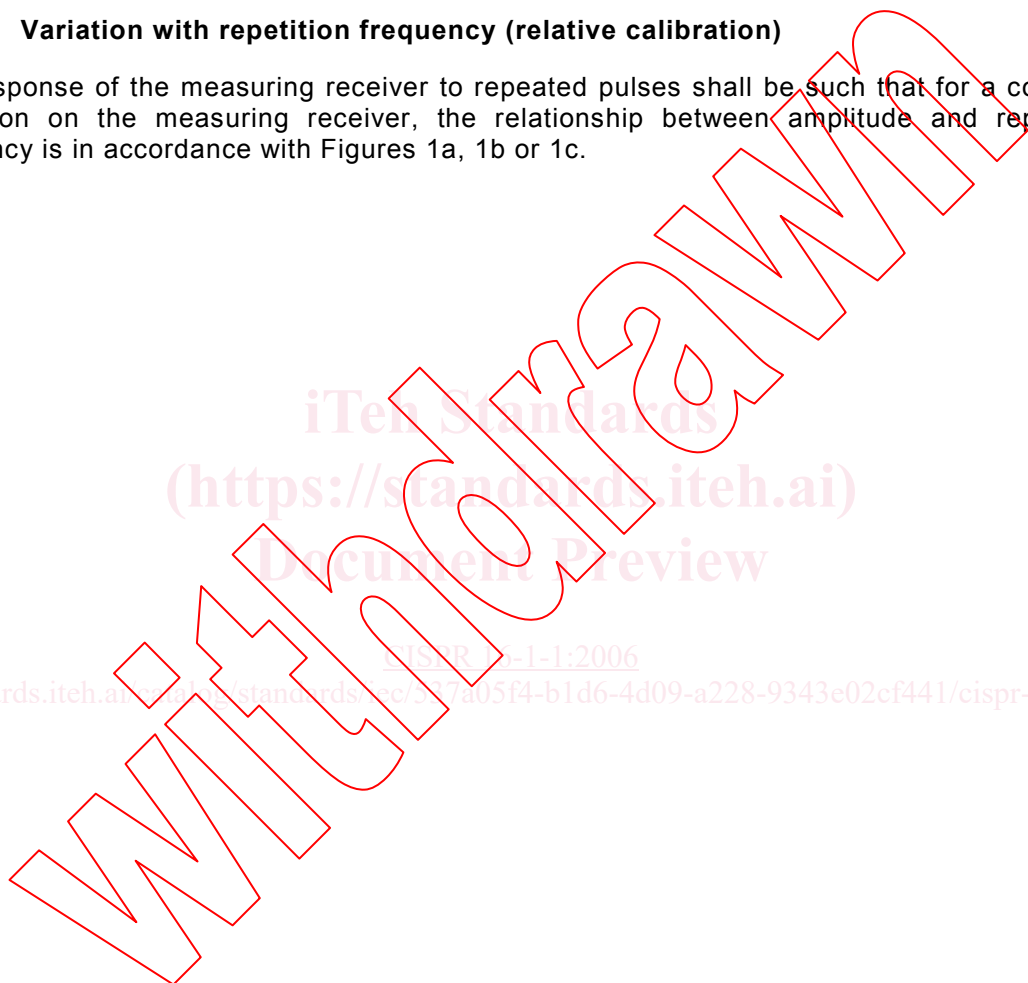

iTech Standards
(<https://standards.iteh.ai>)
Document Preview

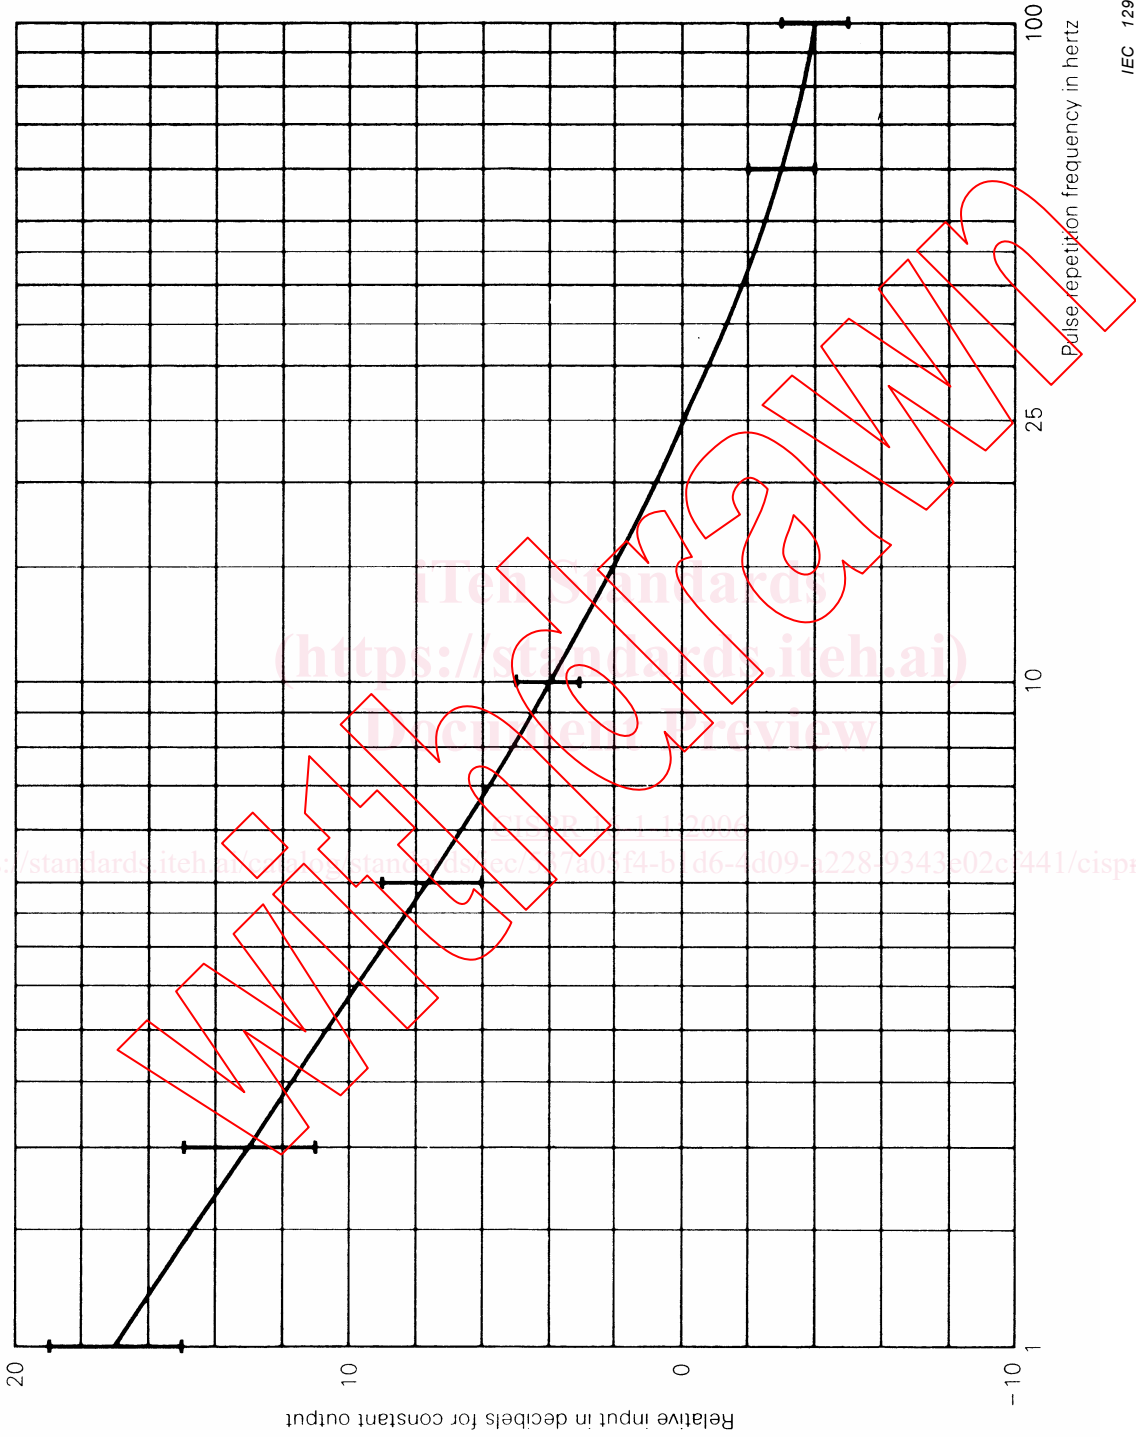

IEC 1290/99

Figure 1a – Pulse response curve (Band A)