

Multimedia systems and equipment - Colour measurement and management - Part 5: Equipment using plasma display panels (IEC 61966-5:2000)

Multimedia systems and equipment - Colour measurement and management -- Part 5: Equipment using plasma display panels

Multimediasysteme und -geräte - Farbmessung und Farbmanagement -- Teil 5: Geräte mit Plasma-Anzeigen

Systèmes et appareils multimédia - Mesure et gestion de la couleur -- Partie 5: Appareils utilisant des afficheurs à plasma

<https://standards.iteh.ai/catalog/standards/sist/58875c5d-274e-454d-bea4-fde1a58da475/sist-en-61966-5-2003>

Ta slovenski standard je istoveten z: EN 61966-5:2001

ICS:

17.180.20	Barve in merjenje svetlobe	Colours and measurement of light
33.160.60	Multimedia systems and teleconferencing equipment	

SIST EN 61966-5:2003

en

iTeh STANDARD PREVIEW
(standards.iteh.ai)

SIST EN 61966-5:2003

<https://standards.iteh.ai/catalog/standards/sist/58875c5d-274e-454d-bea4-fde1a58da475/sist-en-61966-5-2003>

EUROPEAN STANDARD

EN 61966-5

NORME EUROPÉENNE

EUROPÄISCHE NORM

January 2001

ICS 33.160.60;35.180;31.120

English version

**Multimedia systems and equipment -
Colour measurement and management
Part 5: Equipment using plasma display panels
(IEC 61966-5:2000)**

Systèmes et appareils multimédia -
Mesure et gestion de la couleur
Partie 5: Appareils utilisant des afficheurs
à plasma
(CEI 61966-5:2000)

Multimediasysteme und -geräte -
Farbmessung und Farbmanagement
Teil 5: Geräte mit Plasma-Anzeigen
(IEC 61966-5:2000)

iTeh STANDARD PREVIEW
(standards.iteh.ai)

SIST EN 61966-5:2003

This European Standard was approved by CENELEC on 2000-11-01. CENELEC members are bound to comply with the CEN/CENELEC Internal Regulations which stipulate the conditions for giving this European Standard the status of a national standard without any alteration.

Up-to-date lists and bibliographical references concerning such national standards may be obtained on application to the Central Secretariat or to any CENELEC member.

This European Standard exists in three official versions (English, French, German). A version in any other language made by translation under the responsibility of a CENELEC member into its own language and notified to the Central Secretariat has the same status as the official versions.

CENELEC members are the national electrotechnical committees of Austria, Belgium, Czech Republic, Denmark, Finland, France, Germany, Greece, Iceland, Ireland, Italy, Luxembourg, Netherlands, Norway, Portugal, Spain, Sweden, Switzerland and United Kingdom.

CENELEC

European Committee for Electrotechnical Standardization
Comité Européen de Normalisation Electrotechnique
Europäisches Komitee für Elektrotechnische Normung

Central Secretariat: rue de Stassart 35, B - 1050 Brussels

Foreword

The text of document 100/148/FDIS, future edition 1 of IEC 61966-5, prepared by IEC TC 100, Audio, video and multimedia systems and equipment, was submitted to the IEC-CENELEC parallel vote and was approved by CENELEC as EN 61966-5 on 2000-11-01.

The following dates were fixed:

- latest date by which the EN has to be implemented
at national level by publication of an identical
national standard or by endorsement (dop) 2001-08-01
- latest date by which the national standards conflicting
with the EN have to be withdrawn (dow) 2003-11-01

Annexes designated "normative" are part of the body of the standard.
Annexes designated "informative" are given for information only.
In this standard, annex ZA is normative and annex A is informative.
Annex ZA has been added by CENELEC.

iTeh STANDARD PREVIEW (standards.iteh.ai)

Endorsement notice

The text of the International Standard IEC 61966-5:2000 was approved by CENELEC as a European Standard without any modification.

[SIST EN 61966-5:2003](https://standards.iteh.ai/catalog/standards/sist/58875c5d-274e-454d-bea4-fde1a58da475/sist-en-61966-5-2003)

<https://standards.iteh.ai/catalog/standards/sist/58875c5d-274e-454d-bea4-fde1a58da475/sist-en-61966-5-2003>

CONTENTS

Clause	Page
1 Scope	5
2 Normative references.....	5
3 Terms and definitions	6
4 Letters and symbols.....	7
5 Conditions	7
5.1 Environmental conditions.....	7
5.2 Conditions of measurements.....	8
5.3 Input digital data.....	9
6 Measurement equipment.....	10
6.1 Spectroradiometer	10
6.2 Colorimeter.....	10
7 Spectral characteristics and intensity of the primaries and white.....	11
7.1 Characteristics to be measured	11
7.2 Measurement conditions.....	11
7.3 Method of measurement.....	11
7.4 Presentation of results.....	12
8 Basic colorimetric characteristics.....	12
8.1 Characteristics to be measured	12
8.2 Method of calculation.....	13
8.3 Presentation of results.....	14
9 Tone characteristics.....	14
9.1 Characteristics to be measured	14
9.2 Measurement conditions.....	14
9.3 Method of measurement	15
9.4 Presentation of results.....	16
10 Inter-channel dependency.....	18
10.1 Characteristics to be measured	18
10.2 Measurement conditions.....	18
10.3 Method of measurement	19
10.4 Presentation of results.....	20
11 Spatial non-uniformity.....	22
11.1 Characteristics to be measured	22
11.2 Measurement conditions.....	22
11.3 Method of measurement	22
11.4 Presentation of results.....	23
12 Temporal stability	24
12.1 Short-term stability	24
12.1.1 Characteristics to be measured.....	24
12.1.2 Measurement conditions	24
12.1.3 Method of measurement	24
12.1.4 Presentation of results	25

Clause	Page
12.2 Mid-term stability	26
12.2.1 Characteristics to be measured	26
12.2.2 Measurement conditions	26
12.2.3 Method of measurement	26
12.2.4 Presentation of results	26
13 Surface reflection.....	27
13.1 Characteristics to be measured	27
13.2 Measurement conditions	27
13.3 Method of measurement	28
13.4 Presentation of results	28
14 Display area ratio characteristics	29
14.1 Characteristics to be measured	29
14.2 Measurement conditions	29
14.3 Method of measurement	29
14.4 Presentation of results	30
Annex A (informative) External colour control for colour management in open systems	31
Annex ZA (informative) Normative references to international publications with their corresponding European publications.....	36
Bibliography.....	35
Figure 1 – Equipment arrangement for non-contact measurements	8
Figure 2 – Equipment arrangement for contact measurements	8
Figure 3 – Size of a colour patch	9
Figure 4 – An example of the spectral radiance distributions $r(\lambda)$, $g(\lambda)$, $b(\lambda)$	12
Figure 5 – Measured points and interpolated curves	16
Figure 6 – Measurement points for spatial non-uniformity.....	22
Figure 7 – Example plots for short-term stability.....	25
Figure 8 – Example plots for mid-term stability.....	27
Figure 9 – Equipment arrangement	28
Figure 10 – Specification of a white patch	29
Figure 11 – Example plots for the display area ratio characteristics.....	30
Figure A.1 – Comparison between additive colour model and measured tristimulus values in linear and log-log plots	32
Figure A.2 – An example result of the backward transformation approximating the input data RGB for desired displayed colours in $X' Y' Z'$	34
Table 1 – Input data for peak primaries and peak white.....	11
Table 2 – Example of reporting form for colours in maximum excitations.....	12
Table 3 – Example of reporting form	14
Table 4 – An example set of basic normalized data for tone characteristics	17
Table 5 – Digital inputs to generate colour patches for measurement of inter-channel dependency.....	19
Table 6 – Example of normalized tristimulus values (the matrix A).....	21
Table 7 – Example of reporting form	24
Table 8 – Example of reporting form	28

MULTIMEDIA SYSTEMS AND EQUIPMENT – COLOUR MEASUREMENT AND MANAGEMENT – Part 5: Equipment using plasma display panels

1 Scope

A series of methods and parameters for colour measurements and management for use in multimedia systems and equipment is applicable to the assessment of colour production and reproduction. This part of IEC 61966 deals with equipment using plasma display panels (PDP) to display colour images for use in multimedia applications.

The methods of measurement standardized in this part of IEC 61966 are designed to make possible the objective performance assessment and characterization of colour reproduction of PDP displays which accept red – green – blue analogue or digital signals from electrical input terminals and output colour images on PDP display screens. For PDP displays to which analogue signals are applicable, the corresponding digital signals are taken into account. The measured results are intended to be used for the purpose of equipment specific colour control in order to attain colour management in open multimedia systems.

This part of IEC 61966 defines input test signals, measurement conditions, methods of measurement and reporting of the measured data, so as to make possible the colour management and comprehensive comparison of the results of measurements.

Colour control within equipment is outside the scope of this part of IEC 61966. It does not specify limiting values for various parameters.

2 Normative references

The following normative documents contain provisions which, through reference in this text, constitute provisions of this part of 61966. For dated references, subsequent amendments to, or revisions of, any of these publications do not apply. However, parties to agreements based on this part of 61966 are encouraged to investigate the possibility of applying the most recent editions of the normative documents indicated below. For undated references, the latest edition of the normative document referred to applies. Members of IEC and ISO maintain registers of currently valid International Standards.

IEC 60050-845:1987, *International Electrotechnical Vocabulary (IEV) – Chapter 845: Lighting*
CIE 17.4: 1987, *International Lighting Vocabulary* (joint IEC/CIE publication)

IEC 61966-3:2000, *Multimedia systems and equipment – Colour measurement and management – Part 3: Equipment using cathode ray tubes*

ISO 5-4:1995, *Photography – Density measurements – Part 4: Geometric conditions for reflection density*

ISO 9241-8:1997, *Ergonomic requirements for office work with visual display terminals (VDTs) – Part 8: Requirements for displayed colours*

ISO/CIE 10526:1999, *CIE standard illuminants for colorimetry*

ISO/CIE 10527:1991, *CIE standard colorimetric observers*

CIE 15.2:1986, *Colorimetry*

3 Terms and definitions

For the purpose of this part of IEC 61966, the definitions of IEC 60050-845/CIE 17.4, as well as the following definitions, apply.

3.1

background

image on a screen of the PDP display other than the interested area of a colour patch

3.2

colour control

effort to convert equipment dependent colour image data to equipment independent data for a specific colour space including tone characteristics

3.3

colour patch, test area

square colour image on a screen of the PDP display subject to be measured for colour reproduction, in which input data for the red, green and blue channels are kept constant within the image area

3.4

CRT

colorimetrically well-controlled equipment using cathode ray tubes to present colour images with digital inputs for reference

3.5

PDP display

any multimedia equipment using plasma display panels to present colour images

3.6

effective screen height

vertical dimension of the effective screen area

3.7

effective screen area

area where a picture can be produced

3.8

normalized (image) signal

input signal normalized by its full scale value, whose level is of interest in calculation and evaluation of colour control function within PDP display, see also equation (1)

3.9

uncertainty (of measurement)

parameter, associated with the result of a measurement, that characterizes the dispersion of the values that could reasonably be attributed to the particular quantity subject to measurement

See also [16] ¹⁾.

¹⁾ Figures in square brackets refer to the bibliography.

4 Letters and symbols

The notations consistently adopted in this part of IEC 61966 are summarized below.

A	display area ratio
N	number of bits in digital data for each channel
M	maximum integer for non-negative N -bit system; $M = 2^{N-1}$
D_R	digital data applied to red channel
D_G	digital data applied to green channel
D_B	digital data applied to blue channel
R	normalized input level to red channel
G	normalized input level to green channel
B	normalized input level to blue channel
X	one of measured raw data using spectroradiometers and colorimeters corresponding to tristimulus values
Y	one of measured raw data using spectroradiometers and colorimeters corresponding to tristimulus values in candela per square metre
Z	one of measured raw data using spectroradiometers and colorimeters corresponding to tristimulus values
R'	linearized data for red channel taking into account the tone characteristics of the channel
G'	linearized data for green channel taking into account the tone characteristics of the channel
B'	linearized data for blue channel taking into account the tone characteristics of the channel
X'	one of the tristimulus values normalized by Y_n (candela per square metre) for peak white
Y'	one of the tristimulus values normalized by Y_n (candela per square metre) for peak white
Z'	one of the tristimulus values normalized by Y_n (candela per square metre) for peak white

5 Conditions

5.1 Environmental conditions

All measurements specified in this standard shall be carried out in a dark room. Particular attention should be paid to reflected illumination caused by the ambient objects (desktop, wall, etc.) and to direct illumination from light-emitting indicators of measuring instruments.

A 1 h warm-up time should precede the measurements in 7.2, 9.2, 10.2, 11.2 and 14.2, if not specified by the manufacturer of the equipment.

The mains voltage and frequency shall be at the rated values specified by the manufacturer of a PDP display. When the mains voltage fluctuates, a regulated power supply should be used to maintain the supply voltage within $\pm 5\%$ of the rated value.

Other environmental conditions such as room temperature and relative humidity shall be reported together with the results of the measurements.

If additional environmental conditions are described in the manufacturer's specifications, these should also be taken into account.

Conditions of measurements


Contrast, brightness and additional adjustments shall be set to the preset positions specified by the manufacturer of the PDP display under measurement. When the adjustment is set to a position other than the preset, the position or corresponding value should be reported with the results of the measurements.

The equipment arrangement for non-contact measurements should be as shown in figure 1. It incorporates a spectroradiometer or a non-contact colorimeter, depending on the characteristics to be measured. The instrument optical axis should be normal to the centre of the surface of the PDP display.

The distance d between the faceplate of the PDP display and the measuring instrument shall be $4h$ or larger, where h is the effective screen height of the display.

NOTE 1 It is recommended to take precautions so that the measurement is not influenced by vibration and that there are no missing picture elements within the field of view of the measuring instrument.

NOTE 2 The measurement area in the colour patch should include more than 500 picture elements.

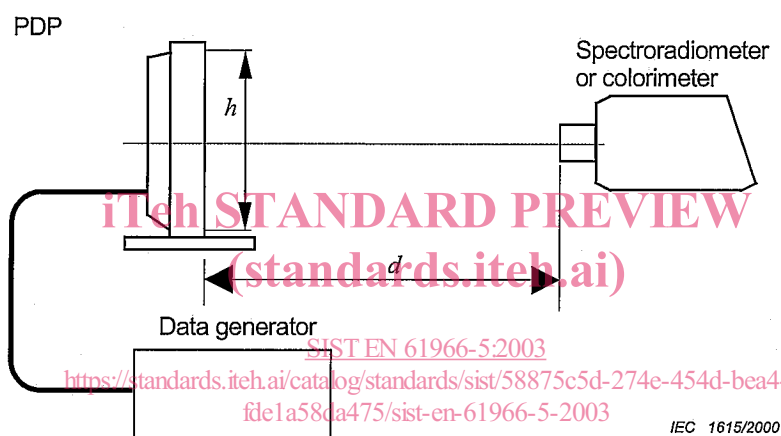

h the effective screen height

Figure 1 – Equipment arrangement for non-contact measurements

The equipment arrangement for contact measurements should be as shown in figure 2, where a measurement probe is placed on the faceplate of the PDP display.


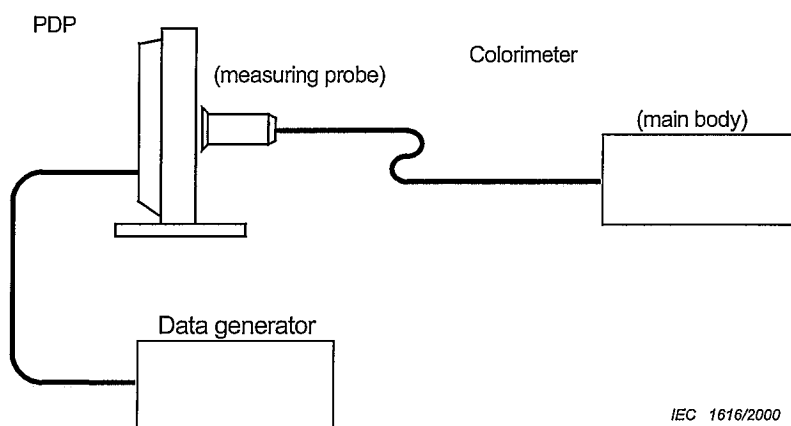


Figure 2 – Equipment arrangement for contact measurements

Test signals applied to red, green and blue channels shall result in a colour patch of the size shown in figure 3 on the PDP display. The positioning of the colour patch shall be referred to by the centre as in figure 3. The background shall be black, unless otherwise specified.

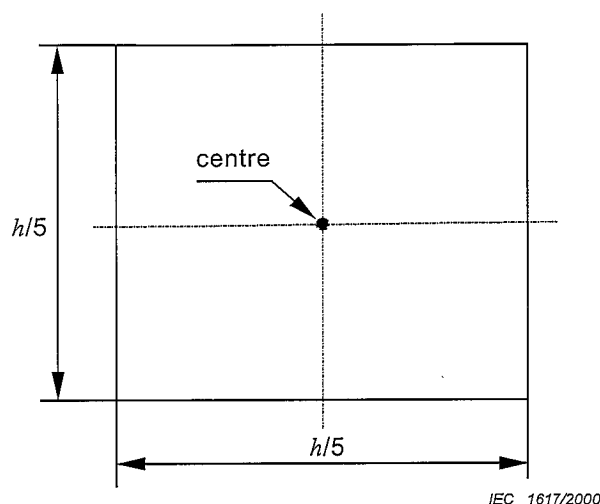

h the effective screen height

Figure 3 – Size of a colour patch

The area for measurement shall be circular, centred on the colour patch, with a diameter between $0,05 h$ and $0,15 h$.

SIST EN 61966-5:2003

5.2 Input digital data

The relationship between input digital data, D_R, D_G, D_B , of N bits and corresponding normalized signal level for calculation shall be

$$\begin{aligned} R_i &= \frac{D_{R_i}}{2^N - 1} \\ G_i &= \frac{D_{G_i}}{2^N - 1} \\ B_i &= \frac{D_{B_i}}{2^N - 1} \end{aligned} \quad (1)$$

where an index i denotes the i -th measurement step.

NOTE When the input signal is applicable in analogue voltage, the signal level normalized by the maximum input voltage should correspond to the signal level for each step defined in equation (1).

6 Measurement equipment

6.1 Spectroradiometer

A spectroradiometer with the following specifications should be used for the measurements:

- | | | |
|----|------------------------|---|
| a) | wavelength range | including 380 nm to 780 nm |
| b) | field of view | between 0,1° and 2,0° |
| c) | wavelength uncertainty | less than 0,5 nm throughout the wavelength range |
| d) | scanning interval | 5 nm or less |
| e) | bandpass | 5 nm or less |
| f) | repeatability | 0,001 in x, y and 0,5 % in luminance (cd/m ²) |
| g) | uncertainty | 0,005 in x, y for red, green, blue and white of a CRT and 4 % in luminance (cd/m ²) for white of the CRT that has a definite x, y and luminance value |

The (x, y) is the CIE 1931 chromaticity coordinate specified in CIE 15.2.

NOTE 1 Periodic calibration should be done with a standard source of known spectral power distribution.

NOTE 2 Further technical details of the design, characterization, and calibration of spectroradiometers can be found in CIE 63 [17] and JIS Z 8724 [7].

NOTE 3 The standard CRT is referred to because no standard PDP displays exist at the time of publication of this part of IEC 61966. When it is available, the standard CRT should be replaced by the standard PDP display.

If the spectroradiometer used for measurements does not meet the above specifications, the model name and specification of the equipment shall be reported together with the results of measurements.

[SIST EN 61966-5:2003](https://standards.iteh.ai/catalog/standards/sist/58875c5d-274e-454d-bea4-fde1a58da475/sist-en-61966-5-2003)

6.2 Colorimeter

The colorimeter should have the following specifications:

- | | | |
|----|----------------------------------|---|
| a) | measurement area (contact type) | 0,05 h to 0,15 h , where h is the effective screen height of the PDP display |
| b) | field of view (non-contact type) | any value between 0,1° and 2,0° |
| c) | spectral responsivity | compliant to the CIE 2-degree colour matching functions as defined in ISO/CIE 10527 |
| d) | repeatability | 0,001 in x, y and 0,5 % for luminance |
| e) | uncertainty | 0,005 in x, y for red, green, blue and white of the CRT and 4 % in luminance (cd/m ²) for white of the CRT that has a definite x, y and luminance value |

The (x, y) is the CIE 1931 chromaticity coordinate defined in CIE 15.2.

NOTE 1 If the original uncertainty of the colorimeter does not meet this recommendation, correction methods are available to improve the accuracy for the PDP display measurement. (See [5], [6] and [11].)

NOTE 2 The instrument should be calibrated periodically to assure the uncertainty recommendation given in item e) above.

NOTE 3 The standard CRT is referred to because no standard PDP displays exist at the time of publication of this part of IEC 61966. When it is available, the standard CRT should be replaced by the standard PDP display.