

International Standard



6999

INTERNATIONAL ORGANIZATION FOR STANDARDIZATION • МЕЖДУНАРОДНАЯ ОРГАНИЗАЦИЯ ПО СТАНДАРТИЗАЦИИ • ORGANISATION INTERNATIONALE DE NORMALISATION

Carbonaceous materials for the production of aluminium — Pitch for electrodes — Determination of density — Pyknometric method

Produits carbonés utilisés pour la production de l'aluminium — Brai pour électrodes — Détermination de la masse volumique — Méthode pycnométrique

First edition — 1983-12-15

ISO 6999:1983
<https://standards.iteh.ai/catalog/standards/sist/af1598ec-ddeb-462a-9777-9f32b35b8632/iso-6999-1983>

UDC 665.777 : 669.713 : 531.754.4

Ref. No. ISO 6999-1983 (E)

Descriptors : aluminium, production, pitch (materials), electrodes, tests, determination, density (mass/volume), pyknometric analysis, test equipment.

Price based on 3 pages

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of developing International Standards is carried out through ISO technical committees. Every member body interested in a subject for which a technical committee has been authorized has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work.

Draft International Standards adopted by the technical committees are circulated to the member bodies for approval before their acceptance as International Standards by the ISO Council.

International Standard ISO 6999 was developed by Technical Committee ISO/TC 47, *Chemistry*, and was circulated to the member bodies in July 1982.

It has been approved by the member bodies of the following countries:

Australia
Austria
Belgium
Canada
China
Czechoslovakia
Egypt, Arab Rep. of
France
Germany, F.R.

Hungary
India
Italy
Korea, Rep. of
Netherlands
New Zealand
Nigeria
Portugal
Romania

South Africa, Rep. of
Spain
Sweden
Switzerland
Thailand
USA
USSR

The member body of the following country expressed disapproval of the document on technical grounds:

United Kingdom

Carbonaceous materials for the production of aluminium — Pitch for electrodes — Determination of density — Pyknometric method

0 Introduction

The density of pitch used for preparation of electrodes for the production of aluminium is a property which gives a guide to its consistency of quality. Knowledge of this parameter is essential for optimum use of pitch.

1 Scope and field of application

This International Standard specifies a pyknometric method for determination of density of pitch used for preparation of electrodes for use in the aluminium industry.

2 References

ISO 3507, *Pyknometers*.

ISO 5725, *Precision of test methods — Determination of repeatability and reproducibility by inter-laboratory tests*.

ISO 6257, *Carbonaceous materials used in the production of aluminium — Pitch for electrodes — Sampling*.

3 Principle

Measurement, by a pyknometric method, of the density of pitch at 25 °C, after degassing under vacuum.

4 Reagents and materials

During the determination, use only reagents of recognized analytical grade and distilled water or water of equivalent purity.

4.1 Ethanol, 95 % (V/V).

4.2 Acetone.

4.3 Non-ionic wetting agent, 0,1 % (m/m) aqueous solution.

5 Apparatus

Ordinary laboratory material and

5.1 Pyknometer, Gay-Lussac, type 3, capacity 25 ml (see ISO 3507).

5.2 Vacuum pump, fitted with safety valve and filter, capacity about 1 m³/h, capable of producing a residual pressure of 33 mbar.

5.3 Airtight container, to hold the pyknometer (5.1) capable of being maintained under vacuum during the determination and fitted with a suitable separating funnel.

WARNING — When under vacuum, place behind a suitable safety screen.

A typical assembled apparatus is shown in the figure.

5.4 Electric oven, capable of being controlled at 120 ± 2 °C.

5.5 Water bath, capable of being controlled at 25 ± 0,05 °C.

6 Sampling

Sampling shall be carried out according to the method specified in ISO 6257.

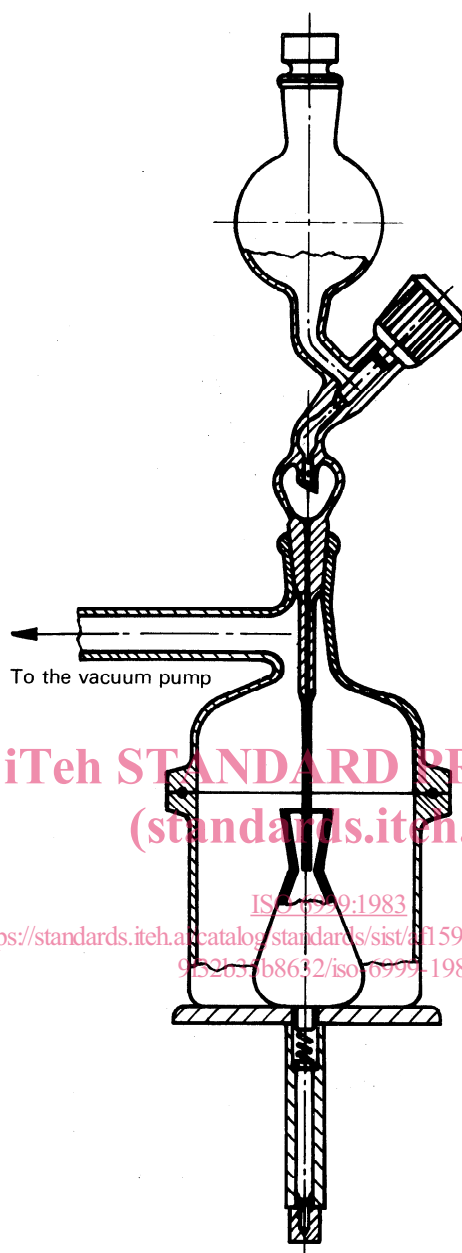


Figure — Typical apparatus for pycnometric determination of density

7 Procedure

7.1 Calibration of the pycnometer

Commercial pycnometers are usually calibrated at 20 °C whereas the present determination is carried out at 25 °C. It is therefore necessary to calibrate the pycnometer at this latter temperature.

7.1.1 Determination of the mass of the pycnometer

WARNING — Sulpho-chromic mixture causes severe burns, is carcinogenic and in contact with combustible material, may cause fire. Avoid contact with eyes, skin and clothing. Do not breathe vapour. Wear protective clothing and goggles when using this material.

Wash the pycnometer (5.1) with a warm sulpho-chromic mixture, taking all necessary precautions. Wash carefully first with tap water then with distilled water, then with the ethanol (4.1) and finally with the acetone (4.2). Dry the pycnometer in an air stream and weigh to the nearest 0,000 1 g (m_0).

7.1.2 Determination of the volume of the pycnometer

Fill the pycnometer with distilled water at a temperature of 23 to 24 °C, insert its stopper, making sure that water escapes through the orifice in the stopper, and wipe the pycnometer with filter paper.

Place the filled pycnometer in the water bath (5.5), controlled at $25 \pm 0,05$ °C, and allow it to reach thermal equilibrium at this temperature. Level off the water to the top of the stopper.

Remove the pycnometer from the water bath, cool slightly with the acetone (4.2) and wipe carefully with filter paper.

Weigh the filled pycnometer to the nearest 0,000 1 g (m_1).

The volume V , in millilitres, of the pycnometer is given by the formula

$$\frac{m_1 - m_0}{0,997\ 05}$$

where

m_0 is the mass, in grams, of the dry, empty pycnometer;

m_1 is the mass, in grams, of the pycnometer filled with water;

0,997 05 is the density of water, in grams per millilitre, at 25 °C.

NOTES

1 The volume V of the pycnometer is rounded off to 0,000 1 ml. The calibration should be repeated every 3 months; the mass m_0 should remain constant to 0,001 g.

2 It is essential that the volume of the pycnometer be determined several times on different days, to eliminate the effect of outside influences as well as the small differences in regulation of the water bath. The volume V should represent the mean of 8 to 10 determinations.

pycnometer and continue the determination according to the conditions specified in 7.1.2, starting from the paragraph: "Place the filled pycnometer in the water bath..."

Weigh the filled pycnometer to the nearest 0,000 1 g (m_3).

8 Expression of results

8.1 Calculations

The density of the pitch, expressed in grams per millilitre, is given by the formula

$$\rho = \frac{m_2}{V - \frac{m_3 - (m_2 + m_0)}{0,997\ 05}}$$

where

m_0 is the mass, in grams, of the dry, empty pycnometer;

m_2 is the mass, in grams, of the test portion (7.2.1);

m_3 is the mass, in grams, of the pycnometer containing the test portion and water;

0,997 05 is the density of the wetting agent solution (4.3), practically equal to that of the water.

7.2 Determination of density

7.2.1 Test portion

Weigh to the nearest 0,000 1 g, $5 \pm 0,1$ g of the laboratory sample (clause 6) with a particle size between 1 and 2 mm (m_2) into the dry, empty pycnometer, prepared according to 7.1.1.

7.2.2 Determination

Fill the separating funnel fitted to the airtight container (5.3), with the wetting solution (4.3). Place the unstoppered pycnometer containing the test portion (7.2.1) in the container and, with the stopcock of the separating funnel closed, run the vacuum pump (5.2) for about 5 min until a residual pressure of 33 to 35 mbar is obtained.

Slowly open the stopcock of the separating funnel and allow the wetting agent solution to fall, drop by drop, until about 20 ml have been added to the pycnometer. Close the stopcock. Maintain the vacuum until any air bubbles in the pycnometer have disappeared. Restore the pressure within the container to ambient level, open the container, remove the pycnometer and fill it completely with the wetting agent solution. Close the

8.2 Precision (see ISO 5725, sub-clause 3.1)

Standard deviation of repeatability: 0,004 g/ml.

Standard deviation of reproducibility: 0,006 g/ml.

Results rounded off to the third place of decimals.

8.3 Checking the determination

Systematic errors can be checked by carrying out determinations on reference materials from time to time.

9 Test report

The test report shall include the following particulars:

- an identification of the sample;
- the reference of the method used;
- the results and the method of expression used;
- any unusual features noted during the determination;
- any operations not included in this International Standard or in the International Standards to which reference is made, or regarded as optional.

iTeh STANDARD PREVIEW

(standards.iteh.ai)

This page intentionally left blank

ISO 6999:1983

<https://standards.iteh.ai/catalog/standards/sist/af1598ec-ddeb-462a-9777-9f32b35b8632/iso-6999-1983>

iTeh STANDARD PREVIEW
(standards.iteh.ai)

This page intentionally left blank

ISO 6999:1983

<https://standards.iteh.ai/catalog/standards/sist/af1598ec-ddeb-462a-9777-9f32b35b8632/iso-6999-1983>

iTeh STANDARD PREVIEW

(standards.iteh.ai)

This page intentionally left blank

ISO 6999:1983

<https://standards.iteh.ai/catalog/standards/sist/af1598ec-ddeb-462a-9777-9f32b35b8632/iso-6999-1983>