

# INTERNATIONAL STANDARD

# ISO 7492

Second edition  
1997-02-15

---

---

## Dental explorers

*Sondes exploratrices dentaires*

**iTeh STANDARD PREVIEW**  
**(standards.iteh.ai)**

[ISO 7492:1997](#)

<https://standards.iteh.ai/catalog/standards/sist/911db431-f823-457c-b955-d183d1a49533/iso-7492-1997>



Reference number  
ISO 7492:1997(E)

## Contents

<b>1 Scope</b> .....	<b>1</b>
<b>2 Normative references</b> .....	<b>1</b>
<b>3 Definitions</b> .....	<b>1</b>
<b>4 Material</b> .....	<b>1</b>
<b>4.1 Material of the working end</b> .....	<b>1</b>
<b>4.2 Material of the handle</b> .....	<b>2</b>
<b>5 Requirements</b> .....	<b>2</b>
<b>5.1 Surface finish</b> .....	<b>2</b>
<b>5.2 Vickers hardness and tensile strength of the working end</b> .....	<b>2</b>
<b>5.3 Resistance against corrosion</b> .....	<b>2</b>
<b>5.4 Resistance against thermal exposure</b> .....	<b>2</b>
<b>5.5 Union of working end and handle</b> .....	<b>2</b>
<b>5.6 Marking</b> .....	<b>3</b>
<b>6 Form and dimensions</b> .....	<b>3</b>
<b>7 Test methods</b> .....	<b>3</b>
<b>7.1 Visual inspection</b> .....	<b>3</b>
<b>7.2 Tests for heat and corrosion resistance</b> .....	<b>3</b>
<b>7.3 Test for union of working end and handle</b> .....	<b>4</b>
<b>Annex A (informative) Measurement of dimensions</b> .....	<b>7</b>
<b>Annex B (informative) Vickers hardness testing</b> .....	<b>9</b>
<b>Annex C (informative) Tensile load test</b> .....	<b>11</b>
<b>Annex D (informative) Torque test</b> .....	<b>12</b>
<b>Annex E (informative) Designation and marking</b> .....	<b>15</b>

ITeH STANDARD PREVIEW  
(standards.iteh.ai)

<https://standards.iteh.ai/catalog/standards/sist/911fdb431-f823-457c-b955-d183d1a49533/iso-7492-1997>  
ISO 7492:1997

© ISO 1997

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from the publisher.

International Organization for Standardization  
Case postale 56 • CH-1211 Genève 20 • Switzerland  
Internet central@iso.ch  
X.400 c=ch; a=400net; p=iso; o=isocs; s=central

Printed in Switzerland

## Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

International Standard ISO 7492 was prepared by Technical Committee ISO/TC 106, *Dentistry*, Subcommittee SC 4, *Dental instruments*.

This second edition cancels and replaces the first edition (ISO 7492:1983), of which it constitutes a technical revision.

Annexes A to E of this International Standard are for information only.

## iTeh STANDARD PREVIEW (standards.iteh.ai)

[ISO 7492:1997](https://standards.iteh.ai/catalog/standards/sist/911db431-f823-457c-b955-d183d1a49533/iso-7492-1997)

<https://standards.iteh.ai/catalog/standards/sist/911db431-f823-457c-b955-d183d1a49533/iso-7492-1997>

**iTeh STANDARD PREVIEW**  
This page intentionally left blank  
**(standards.iteh.ai)**

ISO 7492:1997

<https://standards.iteh.ai/catalog/standards/sist/911db431-f823-457c-b955-d183d1a49533/iso-7492-1997>

# Dental explorers

## 1 Scope

This International Standard specifies the dimensions and performance requirements for dental explorers.

## 2 Normative references

The following standards contain provisions which, through reference in this text, constitute provisions of this International Standard. At the time of publication, the editions indicated were valid. All standards are subject to revision, and parties to agreements based on this International Standard are encouraged to investigate the possibility of applying the most recent editions of the standards indicated below. Members of IEC and ISO maintain registers of currently valid International Standards.

ISO 1942-3:1989, *Dental vocabulary – Part 3: Dental instruments*.

ISO 6507-1:—<sup>1)</sup>, *Metallic materials – Vickers hardness test – Part 1: Test method*.

ISO 7153-1:1991, *Instruments for surgery – Metallic materials – Part 1: Stainless steel*.

ISO 13402:1995, *Surgical and dental hand instruments – Determination of resistance against autoclaving, corrosion and thermal exposure*.

## 3 Definitions

For the purposes of this International Standard, the definition for the term “dental explorer” stated in ISO 1942–3 applies.

## 4 Material

### 4.1 Material of the working end

Working ends shall be made of austenitic or martensitic stainless steel in accordance with ISO 7153-1.

NOTE — Other materials may also be used, provided that the instruments made therefrom meet the requirements of clause 5.

---

1) To be published. (Revision of ISO 6507-1:1982, ISO 6507-2:1983, ISO 6507-3:1989, ISO 409-1:1982, ISO 409-2:1983 and ISO/DIS 409-3)

## 4.2 Material of the handle

The material of the handle, selected at the discretion of the manufacturer, shall meet the requirements of clause 5.

## 5 Requirements

### 5.1 Surface finish

#### 5.1.1 All surfaces

All dental explorer surfaces shall be visibly free from pores, crevices, grinding marks, residual scale, acid, greases and residual grinding and polishing materials.

Tests shall be carried out in accordance with 7.1.

#### 5.1.2 Satin finish

The satin finish shall be both uniform and smooth, and it shall reduce glare.

#### 5.1.3 Mirror finish

The mirror finish shall be obtained by grinding to remove all surface imperfections and by polishing to remove grind marks, resulting in a highly reflective surface.

### 5.2 Vickers hardness and tensile strength of the working end

The Vickers hardness of the finished instrument when tested in accordance with ISO 6507-1, shall be:

Martensitic stainless steel	500 HV1 to 650 HV1
Cobalt-based alloys	min. 480 HV1
Austenitic stainless steel	min. 500 HV1 or min. 1 700 MN·mm <sup>-2</sup> tensile strength

Annexes B and C describe methods for the measurement of Vickers hardness and tensile strength, respectively.

### 5.3 Resistance against corrosion

When the dental explorer is tested in accordance with 7.2.1 or 7.2.2 and 7.1, there shall be no visible signs of corrosion.

With the exception of serrated martensitic stainless steel handles, any blemish shall be considered as evidence of corrosion.

### 5.4 Resistance against thermal exposure

When the dental explorer is tested in accordance with 7.2.3, there shall be no alteration in physical appearance; the hardness value (or, in the case of austenitic stainless steel, tensile strength) shall remain within the specified limits.

Annexes B and C describe methods for the measurement of Vickers hardness and tensile strength, respectively.

### 5.5 Union of working end and handle

The union between the working end and the handle of the instrument, which has previously been subjected to the tests according to 7.2.1 and 7.2.2, shall not become loosened under tensile load when tested in accordance with 7.3.1 and under torque when tested in accordance with 7.3.2.

## 5.6 Marking

The instruments shall be marked in a manner chosen at the discretion of the manufacturer. Annex E provides details of a proposed method for instrument designation (see also table 2) and it is recommended that manufacturers mark their packaging and catalogues in the proposed manner.

## 6 Form and dimensions

The explorers shall have one of the forms A to H shown in figure 1 and the dimensions, measured in accordance with table 1, as shown in table 2. All linear dimensions shall be expressed in millimetres and all angular dimensions shall be expressed in degrees.

Annex A provides details of one method of measurement applicable to most types of dental instrument.

The maximum overall length, irrespective of the form of the instrument, shall be 178 mm.

**Table 1 — Measurement of dental explorer dimensions (see figure 1)**

Symbol	Meaning	Points of measurement
$b_3$	Blade length	distance from the extreme tip of the blade, parallel to the centreline of the blade, to the blade/shank interface
$h_1$	Blade height	distance from the datum point, at right angles to the centreline of the instrument, to the farthest extremity of the blade
$h_2$	Shank height	distance from the datum point, at right angles to the centreline of the instrument, to the farthest external surface of the first bend of the shank
$r_1$	Radius of blade	radius of curvature of the inside of the blade
$\alpha$	Blade angle	angle between the centreline of the blade and the centreline of the instrument
$\beta$	Offset angle	angle between the centreline of the shank and a line, parallel to the centreline of the instrument, forming a tangent with the first bend of the instrument

## 7 Test methods

### 7.1 Visual inspection

Visually inspect, without magnification and at normal visual acuity, the surfaces to determine compliance with the requirements.

### 7.2 Tests for heat and corrosion resistance

Carry out the autoclave test (7.2.1) or the boiling water test (7.2.2) and the thermal test (7.2.3), in one continuous operation for five cycles. After completion of the tests, the instrument(s) shall be rubbed vigorously with a cloth to remove blemishes.

#### 7.2.1 Autoclave test

The autoclave test shall be carried out as specified in ISO 13402.

### 7.2.2 Boiling water test

The boiling water test shall be carried out as specified in ISO 13402.

### 7.2.3 Thermal test

The thermal test shall be carried out as specified in ISO 13402.

## 7.3 Test for union of working end and handle

### 7.3.1 Under tensile load

Subject the union between the working end and handle to a tensile force of 600 N, applied in the direction parallel to the centreline of the handle, for a duration of 5 s.

Annex C describes a suitable test procedure.

### 7.3.2 Under torque

Subject the union between the working end and handle to a torque of 45 N·cm for a duration of 5 s.

Annex D describes a suitable test procedure.

**iTeh STANDARD PREVIEW**  
**(standards.iteh.ai)**

[ISO 7492:1997](https://standards.iteh.ai/catalog/standards/sist/911db431-f823-457c-b955-d183d1a49533/iso-7492-1997)

<https://standards.iteh.ai/catalog/standards/sist/911db431-f823-457c-b955-d183d1a49533/iso-7492-1997>



Table 2 — Dental explorers – Dimensions

Linear dimensions in millimetres  
Angular dimensions in degrees

Form (designation)	Dimensions					
	$r_1$	$b_3$ $\pm 0,5$	$\alpha$ $\pm 5^\circ$	$h_1$ $\pm 0,5$	$h_2$ $\pm 0,5$	$\beta$ $\pm 5^\circ$
A (= 010)						
011	4	—	85°	4,2	3,8	—
012	4	—	90°	4,2	3,8	—
B (= 020)						
021	6	—	85°	2,5	7,5	—
022	6	—	90°	1,5	9,0	—
C (= 030)						
031	2	—	85°	10,0	3,0	—
032	2,5	—	86°	8,2	4,1	—
033	2	—	80°	9,0	3,0	—
D (= 040)						
041	2	—	60°	9,0	3,0	—
042	2,5	—	62°	7,2	3,2	—
E (= 050)						
051	—	—	67°	6,0	—	—
052	—	—	80°	4,5	—	—
F (= 060)						
061	—	—	67°	11,5	—	—
062	—	—	80°	12,0	—	—
G (= 070)						
071	2	2	125°	5,0	4,0	38°
H (= 080)						
081	11	—	45°	11	—	—
082	11	—	35°	6	—	—
083	11	—	25°	4	—	—

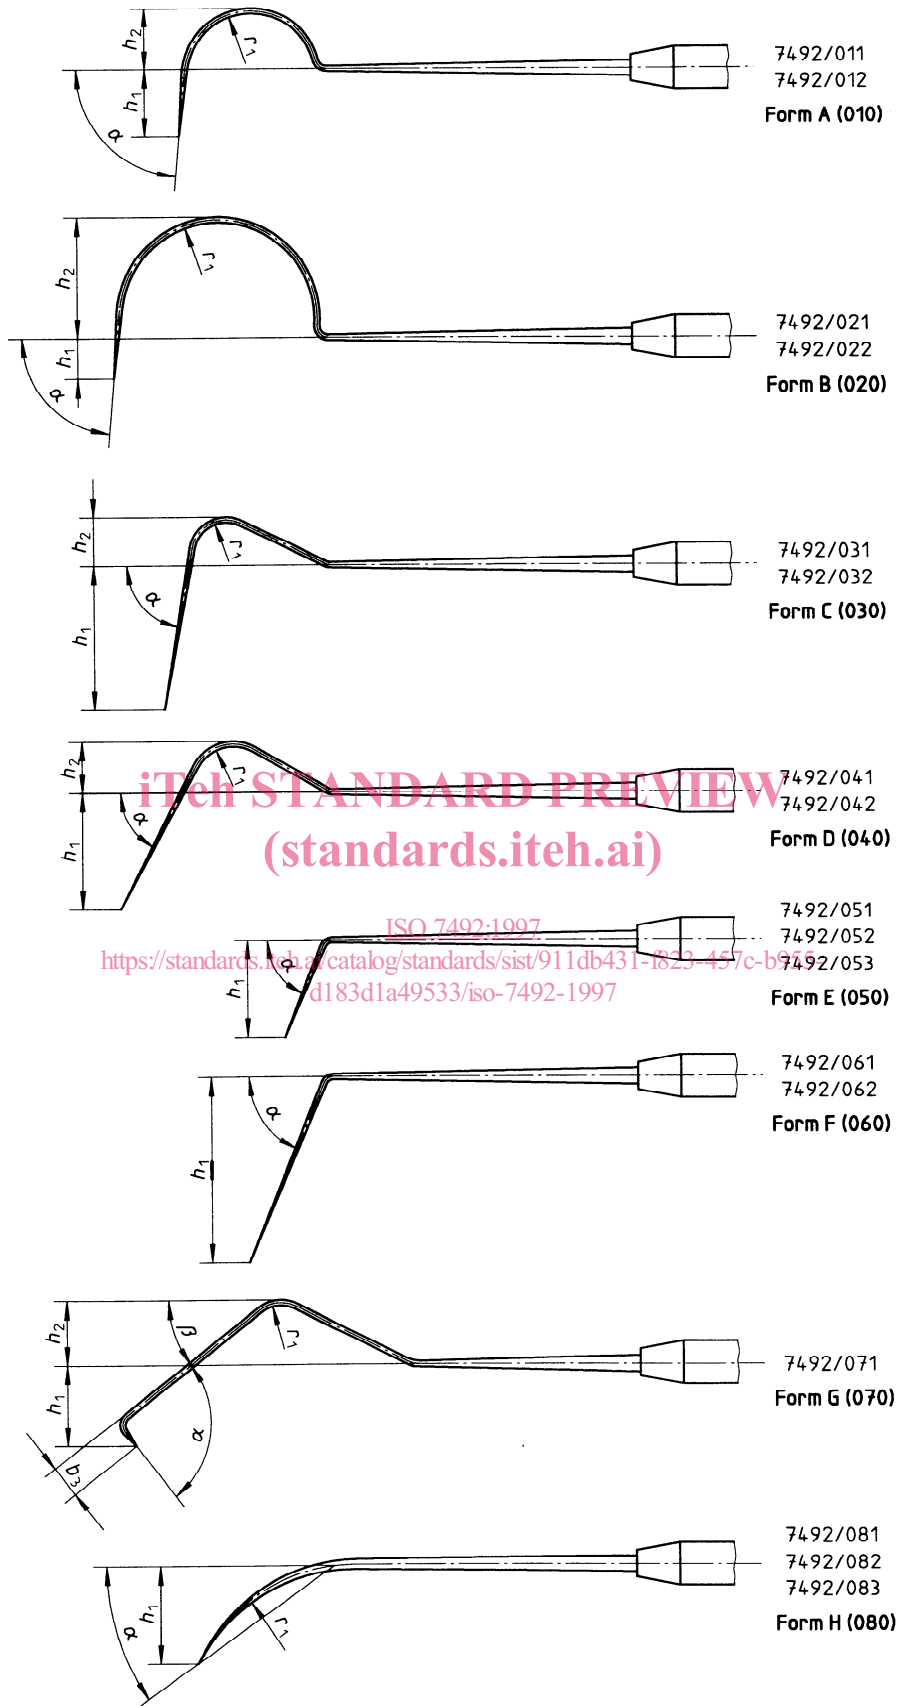


Figure 1 — Forms of dental explorer

## Annex A (informative)

### Measurement of dimensions

#### A.1 General

This method of measurement is applicable to most types of dental hand instrument and is based on the use of an optical projector. Dimensions are measured parallel, and at right angles, to the centreline of the instrument and are constructed from a datum point at its working end. Although this is the preferred method, it is by no means the only technique available.

#### A.2 Apparatus

**A.2.1 Optical projector** (shadowgraph) fitted with 10 × magnifying lens and micrometer stage.

**A.2.2 Glass specimen slide and plasticine**, or

**A.2.3 Mechanical holding device** (e.g. light machine vice), or

**A.2.4 V-block.**

[ISO 7492:1997](https://standards.iteh.ai/catalog/standards/sist/911db431-f823-457c-b955-d183d1a49533/iso-7492-1997)

<https://standards.iteh.ai/catalog/standards/sist/911db431-f823-457c-b955-d183d1a49533/iso-7492-1997>

#### A.3 Procedure

##### A.3.1 Preparation for measurement

**A.3.1.1** Support or hold the dental instrument using one of the devices in A.2.2, A.2.3 or A.2.4.

**A.3.1.2** Place the supported instrument on the micrometer stage of the projector (A.2.1) and ensure that the following requirements are met:

- a) the working end of the instrument projects beyond the holding device;
- b) the instrument is securely held;
- c) there is an unobstructed view of the working end.

**A.3.1.3** Ensure that the dental instrument is parallel to the micrometer stage by focusing on, and traversing the length of, the handle. If the handle remains in focus over the traversed distance, then the instrument is ready for measurement.

If the handle does not remain in focus, repeat A.3.1.2 and A.3.1.3 until the handle remains in focus through the field of traverse.

**A.3.1.4** Align the centreline of the dental instrument with the vertical or horizontal cross-wires on the projector screen.