

# INTERNATIONAL STANDARD

**Ultrasonics – Hydrophones –  
Part 1: Measurement and characterization of medical ultrasonic fields up to  
40 MHz**

Itch Standards  
(<https://standards.itech.ai>)  
Document Preview

IEC 62127-1:2007

<https://standards.itech.ai/standards/iec/436ad83f-e73e-40e4-b170-f507c6dd5d94/iec-62127-1-2007>

Withhold





## THIS PUBLICATION IS COPYRIGHT PROTECTED

Copyright © 2007 IEC, Geneva, Switzerland

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either IEC or IEC's member National Committee in the country of the requester.

If you have any questions about IEC copyright or have an enquiry about obtaining additional rights to this publication, please contact the address below or your local IEC member National Committee for further information.

IEC Central Office  
3, rue de Varembe  
CH-1211 Geneva 20  
Switzerland  
Email: [inmail@iec.ch](mailto:inmail@iec.ch)  
Web: [www.iec.ch](http://www.iec.ch)

### About the IEC

The International Electrotechnical Commission (IEC) is the leading global organization that prepares and publishes International Standards for all electrical, electronic and related technologies.

### About IEC publications

The technical content of IEC publications is kept under constant review by the IEC. Please make sure that you have the latest edition, a corrigenda or an amendment might have been published.

- Catalogue of IEC publications: [www.iec.ch/searchpub](http://www.iec.ch/searchpub)

The IEC on-line Catalogue enables you to search by a variety of criteria (reference number, text, technical committee,...). It also gives information on projects, withdrawn and replaced publications.

- IEC Just Published: [www.iec.ch/online\\_news/justpub](http://www.iec.ch/online_news/justpub)

Stay up to date on all new IEC publications. Just Published details twice a month all new publications released. Available on-line and also by email.

- Electropedia: [www.electropedia.org](http://www.electropedia.org)

The world's leading online dictionary of electronic and electrical terms containing more than 20 000 terms and definitions in English and French, with equivalent terms in additional languages. Also known as the International Electrotechnical Vocabulary online.


- Customer Service Centre: [www.iec.ch/webstore/custserv](http://www.iec.ch/webstore/custserv)

If you wish to give us your feedback on this publication or need further assistance, please visit the Customer Service Centre FAQ or contact us:

Email: [csc@iec.ch](mailto:csc@iec.ch)

Tel.: +41 22 919 02 11

Fax: +41 22 919 03 00

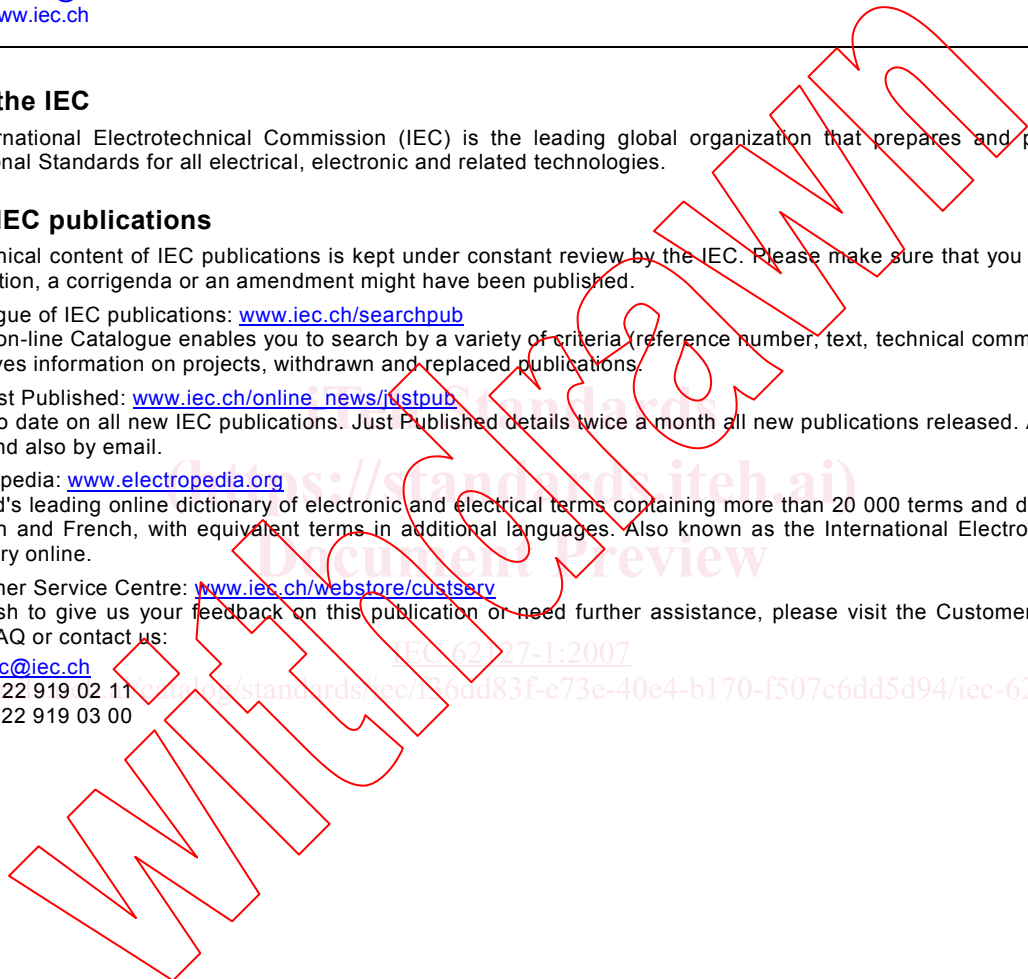

<https://standards.iteh.ai/>  
IEC 62127-1:2007  
<https://standards.iec.org/66dd83f-e73e-40e4-b170-f507c6dd5d94/iec-62127-1-2007>

# INTERNATIONAL STANDARD

---

**Ultrasonics – Hydrophones –  
Part 1: Measurement and characterization of medical ultrasonic fields up to  
40 MHz**

Document Preview  
<https://standards.iteh.ai/>

IEC 62127-1:2007

<https://standards.iteh.ai/en/standards/iec/136ad83f-e73e-40e4-b170-f507c6dd5d94/iec-62127-1-2007>

INTERNATIONAL  
ELECTROTECHNICAL  
COMMISSION

PRICE CODE **XC**

## CONTENTS

FOREWORD.....	5
INTRODUCTION.....	7
1 Scope and object.....	8
2 Normative references .....	8
3 Terms, definitions and symbols .....	9
4 List of symbols .....	24
5 Measurement requirements .....	26
5.1 Requirements for hydrophones and amplifiers.....	26
5.1.1 Introduction .....	26
5.1.2 General .....	26
5.1.3 Sensitivity of a hydrophone.....	26
5.1.4 Directional response of a hydrophone.....	26
5.1.5 Effective hydrophone radius .....	27
5.1.6 Choice of the size of a hydrophone active element.....	27
5.1.7 Bandwidth .....	28
5.1.8 Linearity .....	28
5.1.9 Hydrophone signal amplifier.....	29
5.1.10 Hydrophone cable length and amplifiers.....	29
5.2 Requirements for positioning and water baths .....	29
5.2.1 General.....	29
5.2.2 Positioning systems.....	30
5.2.3 Water bath.....	31
5.3 Requirements for data acquisition and analysis systems .....	32
5.4 Recommendations for ultrasonic equipment being characterized .....	32
6 Measurement procedure.....	32
6.1 General.....	32
6.2 Preparation and alignment.....	33
6.2.1 Preparation.....	33
6.2.2 Aligning an ultrasonic transducer and a hydrophone.....	33
6.3 Measurement .....	33
6.4 Analysis .....	33
6.4.1 Corrections for restricted bandwidth and spatial resolution .....	33
6.4.2 Uncertainties .....	33
7 Beam characterization .....	34
7.1 General.....	34
7.2 Primary pressure parameters .....	35
7.2.1 General .....	35
7.2.2 Peak-compressional acoustic pressure and peak-rarefactional acoustic pressure .....	36
7.2.3 Spatial-peak rms acoustic pressure .....	36
7.2.4 Non-linear propagation parameter .....	36
7.2.5 Intensity parameters using instantaneous acoustic pressure.....	37
7.2.6 Intensity parameters using pulse-pressure-squared integral .....	37
7.2.7 Derived ultrasonic power .....	39
8 Requirements for specific ultrasonic fields.....	40

8.1	General .....	40
8.2	Diagnostic fields .....	40
8.2.1	Simplified procedures and guidelines .....	40
8.2.2	Pulsed wave diagnostic equipment .....	41
8.2.3	Continuous wave diagnostic equipment .....	41
8.3	Therapy fields .....	42
8.3.1	Physiotherapy equipment .....	42
8.3.2	Hyperthermia .....	42
8.4	Surgical fields .....	42
8.4.1	Lithotripters and pressure pulse sources for other therapeutic purposes .....	42
8.4.2	Low frequency surgical applications .....	43
8.5	Fields from other medical applications .....	43
9	Compliance statement .....	43
9.1	General .....	43
9.2	Maximum probable values .....	43
9.3	Sampling .....	44
Annex A (informative)	General rationale .....	45
Annex B (informative)	Hydrophones and positioning .....	47
Annex C (informative)	Acoustic pressure and intensity .....	53
Annex D (informative)	Voltage to pressure conversion .....	55
Annex E (informative)	Correction for spatial averaging .....	60
Annex F (informative)	Acoustic output parameters for multi-mode medical ultrasonic fields in the absence of scan-frame synchronization .....	62
Annex G (informative)	Propagation medium and degassing .....	68
Annex H (informative)	Specific ultrasonic fields .....	69
Annex I (informative)	Assessment of uncertainty in the acoustic quantities obtained by hydrophone measurements .....	72
Annex J (informative)	Transducer and hydrophone positioning systems .....	74
Annex K (informative)	Beamwidth midpoint method .....	75
Bibliography	.....	76
Figure 1	– Schematic diagram of the different planes and lines in an ultrasonic field (see also IEC 61828) .....	11
Figure 2	– Schematic diagram of the method of determining pulse duration .....	35
Figure D.1	– A flow diagram of the hydrophone deconvolution process .....	56
Figure D.2	– Example of waveform deconvolution .....	59
Figure J.1	– Schematic diagram of the ultrasonic transducer and hydrophone degrees of freedom .....	74
Table 1	– Acoustic parameters appropriate to various types of medical ultrasonic equipment .....	34
Table B.1	– Typical specification data for hydrophones, in this case given at 1 MHz .....	52
Table C.1	– Properties of distilled or de-ionized water as a function of temperature .....	54
Table D.1	– Method of conversion from a double- to a single-sided spectrum .....	57

Table D.2 – Method of conversion from a single- to a double-sided spectrum ..... 58  
Table F.1 – Main parameters defined in IEC standards ..... 63  
Table F.2 – List of parameters that are to be used or are to be deleted ..... 64  
Table K.1 – dB beamwidth levels for determining midpoints ..... 75

Withdrawing

iTeh Standards  
(<https://standards.iteh.ai>)  
Document Preview

IEC 62127-1:2007

<https://standards.iteh.ai/catalog/standards/iec/436ad83f-e73e-40e4-b170-f507c6dd5d94/iec-62127-1-2007>

## INTERNATIONAL ELECTROTECHNICAL COMMISSION

## ULTRASONICS – HYDROPHONES –

**Part 1: Measurement and characterization of medical ultrasonic fields up to 40 MHz**

## FOREWORD

- 1) The International Electrotechnical Commission (IEC) is a worldwide organization for standardization comprising all national electrotechnical committees (IEC National Committees). The object of IEC is to promote international co-operation on all questions concerning standardization in the electrical and electronic fields. To this end and in addition to other activities, IEC publishes International Standards, Technical Specifications, Technical Reports, Publicly Available Specifications (PAS) and Guides (hereafter referred to as "IEC Publication(s)"). Their preparation is entrusted to technical committees; any IEC National Committee interested in the subject dealt with may participate in this preparatory work. International, governmental and non-governmental organizations liaising with the IEC also participate in this preparation. IEC collaborates closely with the International Organization for Standardization (ISO) in accordance with conditions determined by agreement between the two organizations.
- 2) The formal decisions or agreements of IEC on technical matters express, as nearly as possible, an international consensus of opinion on the relevant subjects since each technical committee has representation from all interested IEC National Committees.
- 3) IEC Publications have the form of recommendations for international use and are accepted by IEC National Committees in that sense. While all reasonable efforts are made to ensure that the technical content of IEC Publications is accurate, IEC cannot be held responsible for the way in which they are used or for any misinterpretation by any end user.
- 4) In order to promote international uniformity, IEC National Committees undertake to apply IEC Publications transparently to the maximum extent possible in their national and regional publications. Any divergence between any IEC Publication and the corresponding national or regional publication shall be clearly indicated in the latter.
- 5) IEC provides no marking procedure to indicate its approval and cannot be rendered responsible for any equipment declared to be in conformity with an IEC Publication.
- 6) All users should ensure that they have the latest edition of this publication.
- 7) No liability shall attach to IEC or its directors, employees, servants or agents including individual experts and members of its technical committees and IEC National Committees for any personal injury, property damage or other damage of any nature whatsoever, whether direct or indirect, or for costs (including legal fees) and expenses arising out of the publication, use of, or reliance upon, this IEC Publication or any other IEC Publications.
- 8) Attention is drawn to the Normative references cited in this publication. Use of the referenced publications is indispensable for the correct application of this publication.
- 9) Attention is drawn to the possibility that some of the elements of this IEC Publication may be the subject of patent rights. IEC shall not be held responsible for identifying any or all such patent rights.

International Standard IEC 62127-1 has been prepared by IEC technical committee 87: Ultrasonics.

IEC 62127-1, IEC 62127-2 and IEC 62127-3 are being published simultaneously. Together these cancel and replace IEC 60866:1987, IEC 61101:1991, IEC 61102:1991, IEC 61220:1993 and IEC 62092:2001.

The text of this standard is based on the following documents:

Enquiry draft	Report on voting
87/352/CDV	87/371/RVC

Full information on the voting for the approval of this standard can be found in the report on voting indicated in the above table.

This publication has been drafted in accordance with the ISO/IEC Directives, Part 2.

A list of all parts of IEC 62127 series, published under the general title *Ultrasonics – Hydrophones*, can be found on the IEC website.

NOTE Words in **bold** in the text are defined in Clause 3.

The committee has decided that the contents of this publication will remain unchanged until the maintenance result date indicated on the IEC website under "<http://webstore.iec.ch>" in the data related to the specific publication. At this date, the publication will be

- reconfirmed;
- withdrawn;
- replaced by a revised edition; or
- amended.

A bilingual version of this publication may be issued at a later date.

The contents of the corrigendum of August 2008 have been included in this copy.

Withdawn

iTech Standards  
(<https://standards.itih.ai>)  
Document Preview

IEC 62127-1:2007

<https://standards.itih.ai/standards/iec/136ad83f-e73e-40e4-b170-f507c6dd5d94/iec-62127-1-2007>



## INTRODUCTION

The main purpose of this part of IEC 62127 is to define various acoustic parameters that can be used to specify and characterize ultrasonic fields propagating in liquids, and, in particular, water, using hydrophones. Measurement procedures are outlined that may be used to determine these parameters. Specific device related measurement standards, for example IEC 61689, IEC 61157, IEC 61847 or IEC 62359, can refer to this standard for appropriate acoustic parameters.

The philosophy behind this standard is the specification of the acoustic field in terms of acoustic pressure parameters, acoustic pressure being the primary measurement quantity when piezoelectric hydrophones are used to characterize the field. Of course, if other measurement devices come into use in the future, a new standard with additional definitions and procedures will be necessary. Examples of such devices would be thermistors, thermocouples or optical hydrophones.

Intensity parameters are specified in this standard, but these are regarded as derived quantities that are meaningful only under certain assumptions related to the ultrasonic field being measured.

iTech Standards  
(<https://standards.iteh.ai>)  
Document Preview

<https://standards.iteh.ai/standards/iec/62127-1-2007>

<https://standards.iteh.ai/standards/iec/62127-1-2007>

## ULTRASONICS – HYDROPHONES –

### Part 1: Measurement and characterization of medical ultrasonic fields up to 40 MHz

#### 1 Scope and object

This part of IEC 62127 specifies methods of use of calibrated hydrophones for the measurement in liquids of acoustic fields generated by ultrasonic medical equipment operating in the frequency range up to 40 MHz.

The objectives of this standard are:

- to define a group of acoustic parameters that can be measured on a physically sound basis;
- to define a second group of parameters that can be derived under certain assumptions from these measurements, and called derived intensity parameters;
- to define a measurement procedure that may be used for the determination of acoustic pressure parameters;
- to define the conditions under which the measurements of acoustic parameters can be made in the frequency range up to 40 MHz using calibrated hydrophones;
- to define procedures for correcting, for limitations caused by the use of hydrophones with finite bandwidth and finite active element size

NOTE 1 Throughout this standard, SI units are used. In the specification of certain parameters, such as beam areas and intensities, it may be convenient to use decimal multiples or submultiples. For example beam area may be specified in  $\text{cm}^2$  and intensities in  $\text{W}/\text{cm}^2$  or  $\text{mW}/\text{cm}^2$ .

NOTE 2 The hydrophone as defined may be of a piezoelectric or an optic type. The introduction however implies that optical hydrophones are not covered.

#### 2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

IEC 60050-801:1994, *International Electrotechnical Vocabulary – Chapter 801: Acoustics and electroacoustics*

IEC 60565, *Underwater acoustics – Hydrophones – Calibration in the frequency range 0,01 Hz to 1 MHz*

IEC/TR 60854:1986, *Methods of measuring the performance of ultrasonic pulse-echo diagnostic equipment*

IEC 61689, *Ultrasonics – Physiotherapy systems – Performance requirements and methods of measurement in the frequency range 0,5 MHz to 5 MHz*

IEC 61828, *Ultrasonics – Focusing transducers – Definitions and measurement methods for the transmitted fields*

IEC 61846, *Ultrasonics – Pressure pulse lithotripters – Characteristics of fields*

IEC 61847, *Ultrasonics – Surgical systems – Measurement and declaration of the basic output characteristics*

IEC 62127-2, *Ultrasonics – Hydrophones – Part 2: Calibration for ultrasonic fields up to 40 MHz*

IEC 62127-3, *Ultrasonics – Hydrophones – Part 3: Properties of hydrophones for ultrasonic fields up to 40 MHz*

ISO 16269-6:2005, *Statistical interpretation of data – Part 6: Determination of statistical tolerance intervals*

ISO, *Guide to the expression of uncertainty in measurement*. Geneva, Switzerland: International Organization for Standardization (ISO), 1995

NOTE The following standards rely on the proper use of this document.

IEC 61157, *Standard means for the reporting of the acoustic output of medical diagnostic ultrasonic equipment*

IEC 62359, *Ultrasonics – Field characterization – Test methods for the determination of thermal and mechanical indices related to medical diagnostic ultrasonic fields*

IEC 61847, *Ultrasonics – Surgical systems – Measurement and declaration of the basic output characteristics*.

### 3 Terms, definitions and symbols

For the purposes of this document, the terms and definitions given in IEC 62127-2, IEC 62127-3 and the following apply. It also includes definitions related to subjects in this document to be used in particular medical ultrasound device standards.

#### 3.1

##### **acoustic pulse waveform**

temporal waveform of the instantaneous acoustic pressure at a specified position in an acoustic field and displayed over a period sufficiently long to include all significant acoustic information in a single pulse or tone-burst, or one or more cycles in a continuous wave

NOTE 1 Temporal waveform is a representation (e.g. oscilloscope presentation or equation) of the **instantaneous acoustic pressure**.

NOTE 2 Definition adopted from IEC 60469-1.

#### 3.2

##### **acoustic repetition period**

###### **arp**

**pulse repetition period** for non-automatic scanning systems and the **scan repetition period** for automatic scanning systems, equal to the time interval between corresponding points of consecutive cycles for continuous wave systems

NOTE The **acoustic repetition period** is expressed in seconds (s).

#### 3.3

##### **acoustic frequency**

##### **acoustic-working frequency**

frequency of an acoustic signal based on the observation of the output of a **hydrophone** placed in an acoustic field at the position corresponding to the **spatial-peak temporal-peak acoustic pressure**

NOTE 1 The signal is analysed using either the **zero-crossing acoustic-working frequency** technique or a spectrum analysis method. Acoustic-working frequencies are defined in 3.3.1 and 3.3.2.

NOTE 2 In a number of cases the present definition is not very helpful or convenient, especially for **broadband transducers**. In that case, a full description of the frequency spectrum should be given in order to enable any frequency-dependent correction to the signal.

NOTE 3 **Acoustic frequency** is expressed in hertz (Hz).

**3.3.1  
zero-crossing acoustic-working frequency**

$f_{awf}$   
this is determined according to the procedure specified in IEC/TR 60854

NOTE This frequency is intended for continuous wave systems only.

**3.3.2  
arithmetic-mean acoustic-working frequency**

$f_{awf}$   
arithmetic mean of the most widely separated frequencies  $f_1$  and  $f_2$ , within the range of three times  $f_1$ , at which the magnitude of the acoustic pressure spectrum is 3 dB below the peak magnitude

NOTE 1 This frequency is intended for pulse-wave systems only.

NOTE 2 It is assumed that  $f_1 < f_2$ .

**3.3.3  
peak pulse acoustic frequency**

$f_p$   
arithmetic-mean acoustic-working frequency of the pulse with the largest peak negative acoustic pressure measured at the point of maximum peak negative acoustic pressure

NOTE **Peak pulse acoustic frequency** is expressed in hertz (Hz).

**3.3.4  
time average acoustic frequency**

$f_t$   
arithmetic-mean acoustic-working frequency of the time averaged acoustic pressure spectrum of the acoustic signal measured at the point of maximum **temporal average intensity**

NOTE **Time average acoustic frequency** is expressed in hertz (Hz).

**3.4  
azimuth axis**

axis formed by the junction of the **azimuth plane** and the **source aperture plane** (measurement) or **transducer aperture plane** (design)

NOTE 1 Definition adopted from IEC 61828:2001.

NOTE 2 See Figure 1.



### 3.6

#### **bandwidth**

##### **BW**

difference in the most widely separated frequencies  $f_1$  and  $f_2$  at which the magnitude of the acoustic pressure spectrum becomes 3 dB below the peak magnitude, at a specified point in the acoustic field

NOTE **Bandwidth** is expressed in hertz (Hz).

### 3.7

#### **beam area**

##### **A<sub>b</sub>**

area in a specified plane perpendicular to the **beam axis** consisting of all points at which the **pulse-pressure-squared integral** is greater than a specified fraction of the maximum value of the **pulse-pressure-squared integral** in that plane

NOTE 1 If the position of the plane is not specified, it is the plane passing through the point corresponding to the **spatial-peak temporal-peak acoustic pressure** in the whole acoustic field.

NOTE 2 In a number of cases, the term **pulse-pressure-squared integral** is replaced everywhere in the above definition by any linearly related quantity, for example

- a) in the case of a continuous wave signal the term **pulse-pressure-squared integral** is replaced by mean square acoustic pressure as defined in IEC 61689,
- b) in cases where signal synchronisation with the scanframe is not available the term **pulse-pressure-squared integral** may be replaced by **temporal average intensity**

NOTE 3 Some specified levels are 0,25 and 0,01 for the -6 dB and -20 dB beam areas, respectively.

NOTE 4 Beam area is expressed in metres squared (m<sup>2</sup>).

NOTE 5 Definition is modified compared to that used in IEC 61828:2001.

### 3.8

#### **beam axis**

straight line that passes through the **beam centrepoints** of two planes perpendicular to the line which connects the point of maximal **pulse-pressure-squared integral** with the centre of the **external transducer aperture**

NOTE 1 The location of the first plane is the location of the plane containing the maximum **pulse-pressure-squared integral** or, alternatively, is one containing a single main lobe which is in the focal Fraunhofer zone. The location of the second plane is as far as is practicable from the first plane and parallel to the first with the same two orthogonal scan lines (x and y axes) used for the first plane.

NOTE 2 In a number of cases, the term **pulse-pressure-squared integral** is replaced in the above definition by any linearly related quantity, for example

- a) in the case of a continuous wave signal the term **pulse-pressure-squared integral** is replaced by mean square acoustic pressure as defined in IEC 61689,
- b) in cases where signal synchronisation with the scanframe is not available the term **pulse-pressure-squared integral** may be replaced by **temporal average intensity**.

NOTE 3 See Figure 1.

NOTE 4 Definition is modified compared to that used in IEC 61828:2001.

### 3.9

#### **beam centrepoint**

position determined by the intersection of two lines passing through the **beamwidth midpoints** of two orthogonal planes, xz and yz

NOTE Definition adopted from IEC 61828:2001.

### 3.10

#### **beamwidth midpoint**

linear average of the location of the centres of **beamwidths** in a plane