

INTERNATIONAL STANDARD

NORME INTERNATIONALE



**Medical electrical equipment –
Part 2-21: Particular requirements for the basic safety and essential performance
of infant radiant warmers**

**Appareils électromédicaux –
Partie 2-21: Exigences particulières pour la sécurité de base et les performances
essentielles des incubateurs radiants pour nouveau-nés**

<https://standards.iteh.ai/catalog/standards/iec/0dc2dc36-9107-4d0c-bf74-3059509ca35c/iec-60601-2-21-2009>



THIS PUBLICATION IS COPYRIGHT PROTECTED

Copyright © 2016 IEC, Geneva, Switzerland

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either IEC or IEC's member National Committee in the country of the requester. If you have any questions about IEC copyright or have an enquiry about obtaining additional rights to this publication, please contact the address below or your local IEC member National Committee for further information.

Droits de reproduction réservés. Sauf indication contraire, aucune partie de cette publication ne peut être reproduite ni utilisée sous quelque forme que ce soit et par aucun procédé, électronique ou mécanique, y compris la photocopie et les microfilms, sans l'accord écrit de l'IEC ou du Comité national de l'IEC du pays du demandeur. Si vous avez des questions sur le copyright de l'IEC ou si vous désirez obtenir des droits supplémentaires sur cette publication, utilisez les coordonnées ci-après ou contactez le Comité national de l'IEC de votre pays de résidence.

IEC Central Office
3, rue de Varembe
CH-1211 Geneva 20
Switzerland

Tel.: +41 22 919 02 11
Fax: +41 22 919 03 00
info@iec.ch
www.iec.ch

About the IEC

The International Electrotechnical Commission (IEC) is the leading global organization that prepares and publishes International Standards for all electrical, electronic and related technologies.

About IEC publications

The technical content of IEC publications is kept under constant review by the IEC. Please make sure that you have the latest edition, a corrigenda or an amendment might have been published.

IEC Catalogue - webstore.iec.ch/catalogue

The stand-alone application for consulting the entire bibliographical information on IEC International Standards, Technical Specifications, Technical Reports and other documents. Available for PC, Mac OS, Android Tablets and iPad.

IEC publications search - www.iec.ch/searchpub

The advanced search enables to find IEC publications by a variety of criteria (reference number, text, technical committee,...). It also gives information on projects, replaced and withdrawn publications.

IEC Just Published - webstore.iec.ch/justpublished

Stay up to date on all new IEC publications. Just Published details all new publications released. Available online and also once a month by email.

Electropedia - www.electropedia.org

The world's leading online dictionary of electronic and electrical terms containing 20 000 terms and definitions in English and French, with equivalent terms in 15 additional languages. Also known as the International Electrotechnical Vocabulary (IEV) online.

IEC Glossary - std.iec.ch/glossary

65 000 electrotechnical terminology entries in English and French extracted from the Terms and Definitions clause of IEC publications issued since 2002. Some entries have been collected from earlier publications of IEC TC 37, 77, 86 and CISPR.

IEC Customer Service Centre - webstore.iec.ch/csc

If you wish to give us your feedback on this publication or need further assistance, please contact the Customer Service Centre: csc@iec.ch.

A propos de l'IEC

La Commission Electrotechnique Internationale (IEC) est la première organisation mondiale qui élabore et publie des Normes internationales pour tout ce qui a trait à l'électricité, à l'électronique et aux technologies apparentées.

A propos des publications IEC

Le contenu technique des publications IEC est constamment revu. Veuillez vous assurer que vous possédez l'édition la plus récente, un corrigendum ou amendement peut avoir été publié.

Catalogue IEC - webstore.iec.ch/catalogue

Application autonome pour consulter tous les renseignements bibliographiques sur les Normes internationales, Spécifications techniques, Rapports techniques et autres documents de l'IEC. Disponible pour PC, Mac OS, tablettes Android et iPad.

Recherche de publications IEC - www.iec.ch/searchpub

La recherche avancée permet de trouver des publications IEC en utilisant différents critères (numéro de référence, texte, comité d'études,...). Elle donne aussi des informations sur les projets et les publications remplacées ou retirées.

IEC Just Published - webstore.iec.ch/justpublished

Restez informé sur les nouvelles publications IEC. Just Published détaille les nouvelles publications parues. Disponible en ligne et aussi une fois par mois par email.

Electropedia - www.electropedia.org

Le premier dictionnaire en ligne de termes électroniques et électriques. Il contient 20 000 termes et définitions en anglais et en français, ainsi que les termes équivalents dans 15 langues additionnelles. Egalement appelé Vocabulaire Electrotechnique International (IEV) en ligne.

Glossaire IEC - std.iec.ch/glossary

65 000 entrées terminologiques électrotechniques, en anglais et en français, extraites des articles Termes et Définitions des publications IEC parues depuis 2002. Plus certaines entrées antérieures extraites des publications des CE 37, 77, 86 et CISPR de l'IEC.

Service Clients - webstore.iec.ch/csc

Si vous désirez nous donner des commentaires sur cette publication ou si vous avez des questions contactez-nous: csc@iec.ch.

INTERNATIONAL STANDARD

NORME INTERNATIONALE



**Medical electrical equipment –
Part 2-21: Particular requirements for the basic safety and essential
performance of infant radiant warmers**

**Appareils électromédicaux –
Partie 2-21: Exigences particulières pour la sécurité de base et les
performances essentielles des incubateurs radiants pour nouveau-nés**

<https://standards.iteh.ai/catalog/standards/iec/0dc2dc36-9107-4d0c-bf74-3059509ca35c/iec-60601-2-21-2009>

INTERNATIONAL
ELECTROTECHNICAL
COMMISSION

COMMISSION
ELECTROTECHNIQUE
INTERNATIONALE

ICS 11.040.10

ISBN 978-2-8322-3377-1

**Warning! Make sure that you obtained this publication from an authorized distributor.
Attention! Veuillez vous assurer que vous avez obtenu cette publication via un distributeur agréé.**

REDLINE VERSION

VERSION REDLINE



**Medical electrical equipment –
Part 2-21: Particular requirements for the basic safety and essential performance
of infant radiant warmers**

**Appareils électromédicaux –
Partie 2-21: Exigences particulières pour la sécurité de base et les performances
essentielles des incubateurs radiants pour nouveau-nés**

<https://standards.iteh.ai/catalog/standards/iec/0dc2dc36-9107-4d0c-bf74-3059509ca35c/iec-60601-2-21-2009>

CONTENTS

FOREWORD.....	3
INTRODUCTION.....	6
201.1 Scope, object and related standards	7
201.2 Normative references	9
201.3 Terms and definitions	9
201.4 General requirements	11
201.5 General requirements for testing of ME EQUIPMENT.....	12
201.6 Classification of ME EQUIPMENT and ME SYSTEMS	12
201.7 ME EQUIPMENT identification, marking and documents.....	12
201.8 Protection against electrical HAZARDS from ME EQUIPMENT.....	14
201.9 Protection against MECHANICAL HAZARDS of ME EQUIPMENT and ME SYSTEMS.....	14
201.10 Protection against unwanted and excessive radiation HAZARDS.....	16
201.11 Protection against excessive temperatures and other HAZARDS.....	16
201.12 Accuracy of controls and instruments and protection against hazardous outputs.....	17
201.13 HAZARDOUS SITUATIONS and fault conditions.....	21
201.14 PROGRAMMABLE ELECTRICAL MEDICAL SYSTEMS (PEMS)	21
201.15 Construction of ME EQUIPMENT.....	21
201.16 ME SYSTEMS	23
201.17 Electromagnetic compatibility of ME EQUIPMENT and ME SYSTEMS.....	23
202 Electromagnetic compatibility – Requirements and tests	23
210 Requirements for the development of physiologic closed loop controllers.....	23
Annexes	24
Annex AA (informative) Particular guidance and rationale	25
Bibliography	34
Index of defined terms used in this particular standard	36
Figure 201.101 – Layout of TEST DEVICES.....	10
Figure 201.102 – TEST DEVICE	11
Figure AA.1 – Illustration of the main requirements of this standard	25
Table 201.101 – Additional ESSENTIAL PERFORMANCE requirements.....	12

INTERNATIONAL ELECTROTECHNICAL COMMISSION

MEDICAL ELECTRICAL EQUIPMENT –

Part 2-21: Particular requirements for the basic safety and essential performance of infant radiant warmers

FOREWORD

- 1) The International Electrotechnical Commission (IEC) is a worldwide organization for standardization comprising all national electrotechnical committees (IEC National Committees). The object of IEC is to promote international co-operation on all questions concerning standardization in the electrical and electronic fields. To this end and in addition to other activities, IEC publishes International Standards, Technical Specifications, Technical Reports, Publicly Available Specifications (PAS) and Guides (hereafter referred to as "IEC Publication(s)"). Their preparation is entrusted to technical committees; any IEC National Committee interested in the subject dealt with may participate in this preparatory work. International, governmental and non-governmental organizations liaising with the IEC also participate in this preparation. IEC collaborates closely with the International Organization for Standardization (ISO) in accordance with conditions determined by agreement between the two organizations.
- 2) The formal decisions or agreements of IEC on technical matters express, as nearly as possible, an international consensus of opinion on the relevant subjects since each technical committee has representation from all interested IEC National Committees.
- 3) IEC Publications have the form of recommendations for international use and are accepted by IEC National Committees in that sense. While all reasonable efforts are made to ensure that the technical content of IEC Publications is accurate, IEC cannot be held responsible for the way in which they are used or for any misinterpretation by any end user.
- 4) In order to promote international uniformity, IEC National Committees undertake to apply IEC Publications transparently to the maximum extent possible in their national and regional publications. Any divergence between any IEC Publication and the corresponding national or regional publication shall be clearly indicated in the latter.
- 5) IEC provides no marking procedure to indicate its approval and cannot be rendered responsible for any equipment declared to be in conformity with an IEC Publication.
- 6) All users should ensure that they have the latest edition of this publication.
- 7) No liability shall attach to IEC or its directors, employees, servants or agents including individual experts and members of its technical committees and IEC National Committees for any personal injury, property damage or other damage of any nature whatsoever, whether direct or indirect, or for costs (including legal fees) and expenses arising out of the publication, use of, or reliance upon, this IEC Publication or any other IEC Publications.
- 8) Attention is drawn to the normative references cited in this publication. Use of the referenced publications is indispensable for the correct application of this publication.
- 9) Attention is drawn to the possibility that some of the elements of this IEC Publication may be the subject of patent rights. IEC shall not be held responsible for identifying any or all such patent rights.

This consolidated version of the official IEC Standard and its amendment has been prepared for user convenience.

IEC 60601-2-21 edition 2.1 contains the second edition (2009-02) [documents 62D/735/FDIS and 62D/762/RVD], its corrigendum 1 (2013-02) and its amendment 1 (2016-04) [documents 62D/1326/FDIS and 62D/1347/RVD].

In this Redline version, a vertical line in the margin shows where the technical content is modified by amendment 1. Additions are in green text, deletions are in strikethrough red text. A separate Final version with all changes accepted is available in this publication.

International standard IEC 60601-2-21 has been prepared by subcommittee 62D: Electromedical equipment, of IEC technical committee 62: Electrical equipment in medical practice.

This second edition cancels and replaces the first edition published in 1994 and its Amendment 1 (1996). This edition constitutes a technical revision. This edition of IEC 60601-2-21 was revised to structurally align with the 2005 edition of IEC 60601-1.

This publication has been drafted in accordance with the ISO/IEC Directives, Part 2.

In this standard, the following print types are used:

- Requirements and definitions: roman type.
- *Test specifications: italic type.*
- Informative material appearing outside of tables, such as notes, examples and references: in smaller type. Normative text of tables is also in a smaller type.
- TERMS DEFINED IN CLAUSE 3 OF THE GENERAL STANDARD, IN THIS PARTICULAR STANDARD OR AS NOTED: SMALL CAPITALS.

In referring to the structure of this standard, the term

- “clause” means one of the seventeen numbered divisions within the table of contents, inclusive of all subdivisions (e.g. Clause 7 includes subclauses 7.1, 7.2, etc.);
- “subclause” means a numbered subdivision of a clause (e.g. 7.1, 7.2 and 7.2.1 are all subclauses of Clause 7).

References to clauses within this standard are preceded by the term “Clause” followed by the clause number. References to subclauses within this particular standard are by number only.

In this standard, the conjunctive “or” is used as an “inclusive or” so a statement is true if any combination of the conditions is true.

The verbal forms used in this standard conform to usage described in Annex H of the ISO/IEC Directives, Part 2. For the purposes of this standard, the auxiliary verb:

- “shall” means that compliance with a requirement or a test is mandatory for compliance with this standard;
- “should” means that compliance with a requirement or a test is recommended but is not mandatory for compliance with this standard;
- “may” is used to describe a permissible way to achieve compliance with a requirement or test.

An asterisk (*) as the first character of a title or at the beginning of a paragraph or table title indicates that there is guidance or rationale related to that item in Annex AA.

A list of all parts of the IEC 60601 series, published under the general title *Medical electrical equipment*, can be found on the IEC website.

The committee has decided that the contents of the base publication and its amendment will remain unchanged until the stability date indicated on the IEC web site under "<http://webstore.iec.ch>" in the data related to the specific publication. At this date, the publication will be

- reconfirmed,
- withdrawn,
- replaced by a revised edition, or
- amended.

IMPORTANT – The 'colour inside' logo on the cover page of this publication indicates that it contains colours which are considered to be useful for the correct understanding of its contents. Users should therefore print this document using a colour printer.

iTech Standards
(<https://standards.iteh.ai>)
Document Preview

<https://standards.iteh.ai/csi/standards/iec/0dc2dc36-9107-4d0c-bf74-3059509ca35c/iec-60601-2-21-2009>

INTRODUCTION

The minimum safety requirements specified in this particular standard are considered to provide for a practical degree of safety in the operation of INFANT RADIANT WARMER equipment.

This particular standard amends and supplements IEC 60601-1:~~2005~~, *Medical electrical equipment – Part 1: General requirements for basic safety and essential performance*, hereinafter referred to as the general standard.

The requirements are followed by specifications for the relevant tests.

A general guidance and rationale for the requirements of this particular standard are given in Annex AA.

It is considered that knowledge of the reasons for these requirements will not only facilitate the proper application of this particular standard but will, in due course, expedite any revision necessitated by changes in clinical practice or as a result of developments in technology. However, this annex does not form part of the requirements of this standard.

iTech Standards
(<https://standards.iteh.ai>)
Document Preview

IEC 60601-2-21:2009

<https://standards.iteh.ai/catalog/standards/iec/0dc2dc36-9107-4d0c-bf74-3059509ca35c/iec-60601-2-21-2009>

WITHDRAWN

MEDICAL ELECTRICAL EQUIPMENT –

Part 2-21: Particular requirements for the basic safety and essential performance of infant radiant warmers

201.1 Scope, object and related standards

Clause 1 of the general standard¹⁾ applies, except as follows:

201.1.1 Scope

Replacement:

This International Standard applies to the BASIC SAFETY and ESSENTIAL PERFORMANCE of INFANT RADIANT WARMERS as defined in 201.3.204, also referred to as ME EQUIPMENT.

If a clause or subclause is specifically intended to be applicable to ME EQUIPMENT only, or to ME SYSTEMS only, the title and content of that clause or subclause will say so. If that is not the case, the clause or subclause applies both to ME EQUIPMENT and to ME SYSTEMS, as relevant.

HAZARDS inherent in the intended physiological function of ME EQUIPMENT or ME SYSTEMS within the scope of this standard are not covered by specific requirements in this standard except in 7.2.13 and 8.4.1 of the general standard.

NOTE See also 4.2 of the general standard.

This particular standard specifies the safety requirements for INFANT RADIANT WARMERS, but alternate methods of compliance with a specific clause, by demonstrating equivalent safety, will not be judged as non-compliant, if the MANUFACTURER has demonstrated in his RISK MANAGEMENT FILE that the RISK presented by the HAZARD has been found to be of an acceptable level when weighed against the benefit of treatment from the device.

This particular standard does not apply to:

- devices supplying heat via BLANKETS, PADS or MATTRESSES in medical use; for information see IEC 80601-2-35;
- INFANT INCUBATORS; for information see IEC 60601-2-19;
- INFANT TRANSPORT INCUBATORS, for information see IEC 60601-2-20;
- INFANT PHOTOTHERAPY EQUIPMENT, for information see IEC 60601-2-50.

201.1.2 Object

Replacement:

The object of this particular standard is to establish particular BASIC SAFETY and ESSENTIAL PERFORMANCE requirements for INFANT RADIANT WARMERS as defined in 201.3.204, which minimize HAZARDS to PATIENT and OPERATOR, and to specify tests by which compliance with the requirements can be verified.

¹⁾ The general standard is IEC 60601-1:2005, *Medical electrical equipment – Part 1: General requirements for basic safety and essential performance.*

201.1.3 * Collateral standards

Addition:

This particular standard refers to those applicable collateral standards that are listed in Clause 2 of the general standard and Clause 2 of this particular standard.

IEC 60601-1-2 ~~and IEC 60601-1-10~~ applies as modified in Clauses 202 ~~and 210~~ respectively. IEC 60601-1-3 and IEC 60601-1-10 do not apply. All other published collateral standards in the IEC 60601-1 series apply as published.

201.1.4 * Particular standards

Replacement:

In the IEC 60601 series, particular standards may modify, replace or delete requirements contained in the general standard and collateral standards as appropriate for the particular ME EQUIPMENT under consideration, and may add other BASIC SAFETY AND ESSENTIAL PERFORMANCE requirements.

A requirement of a particular standard takes priority over the general standard.

For brevity, IEC 60601-1 is referred to in this particular standard as the general standard. Collateral standards are referred to by their document number.

The numbering of clauses and subclauses of this particular standard corresponds to that of the general standard with the prefix "201" (e.g. 201.1 in this standard addresses the content of Clause 1 of the general standard) or applicable collateral standard with the prefix "20x" where x is the final digit(s) of the collateral standard document number (e.g. 202.4 in this particular standard addresses the content of Clause 4 of the 60601-1-2 collateral standard, 203.4 in this particular standard addresses the content of Clause 4 of the 60601-1-3 collateral standard, etc.). The changes to the text of the general standard are specified by the use of the following words:

"Replacement" means that the clause or subclause of the general standard or applicable collateral standard is replaced completely by the text of this particular standard.

"Addition" means that the text of this particular standard is additional to the requirements of the general standard or applicable collateral standard.

"Amendment" means that the clause or subclause of the general standard or applicable collateral standard is amended as indicated by the text of this particular standard.

Subclauses, figures or tables which are additional to those of the general standard are numbered starting from 201.101. However, due to the fact that definitions in the general standard are numbered 3.1 through 3.139, additional definitions in this standard are numbered beginning from 201.3.201. Additional annexes are lettered AA, BB, etc., and additional items aa), bb), etc.

Subclauses, figures or tables which are additional to those of a collateral standard are numbered starting from 20x, where "x" is the number of the collateral standard, e.g. 202 for IEC 60601-1-2, 203 for IEC 60601-1-3, etc.

The term "this standard" is used to make reference to the general standard, any applicable collateral standards and this particular standard taken together.

Where there is no corresponding clause or subclause in this particular standard, the clause or subclause of the general standard or applicable collateral standard, although possibly not

relevant, applies without modification; where it is intended that any part of the general standard or applicable collateral standard, although possibly relevant, is not to be applied, a statement to that effect is given in this particular standard.

SKIN TEMPERATURE SENSORS which are applied to operate a BABY CONTROLLED RADIANT WARMER including the displayed value are considered to be not a CLINICAL THERMOMETER in the sense of the particular standard ISO 80601-2-56.

201.2 Normative references

Clause 2 of the general standard applies, except as follows:

Amendment:

IEC 60601-1-2:~~2007~~, *Medical electrical equipment – Part 1-2: General requirements for basic safety and essential performance – Collateral standard: Electromagnetic compatibility – Requirements and tests*

Addition:

~~IEC 60601-1-10:2007, Medical electrical equipment – Part 1-10: General requirements for basic safety and essential performance – Collateral Standard: Requirements for the development of physiologic closed-loop controllers~~

NOTE Informative references are listed in the bibliography beginning on page 34.

201.3 Terms and definitions

For the purposes of this document, the terms and definitions given in the general standard apply, except as follows:

NOTE An index of defined terms is found beginning on page 36.

Addition:

201.3.201

BABY CONTROLLED RADIANT WARMER

mode of operation in which the power output varies automatically in order to maintain the temperature as measured by a SKIN TEMPERATURE SENSOR according to the CONTROL TEMPERATURE set by the OPERATOR

~~NOTE An INFANT RADIANT WARMER operating as a BABY CONTROLLED RADIANT WARMER is a PHYSIOLOGIC CLOSED-LOOP CONTROLLER as defined in IEC 60601-1-10.~~

201.3.202

CONTROL TEMPERATURE

temperature selected at the temperature control

201.3.203

INFANT

PATIENT up to 3 months and with a weight of less than 10 kg

201.3.204

INFANT RADIANT WARMER

electrically powered device with a radiant heating source intended to maintain the thermal balance of an INFANT by direct radiation of energy in the infrared region of the electromagnetic spectrum

201.3.205

MANUAL MODE


mode of operation in which the heater output is either at a fixed level or a proportion of its maximum output set by the OPERATOR

201.3.206

MID-POINT AVERAGE TEMPERATURE

T_M

TEST DEVICE AVERAGE TEMPERATURE of the TEST DEVICE positioned at the mid-point of the INFANT RADIANT WARMER mattress (See Figure 201.101)

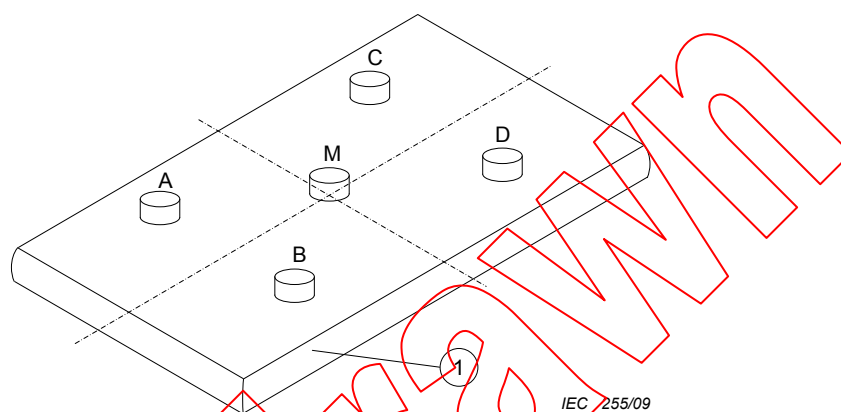

Key

1 = Mattress

Figure 201.101 – Layout of TEST DEVICES

201.3.207

PREWARM MODE

mode of operation in which the heater output is maintained at a preset level (set by the MANUFACTURER) for the purpose of pre-warming the INFANT RADIANT WARMER and maintaining the level of warmth of the INFANT RADIANT WARMER prior to an INFANT being placed on the device

201.3.208

SKIN TEMPERATURE SENSOR

sensing device intended to measure the INFANT'S SKIN TEMPERATURE

201.3.209

STEADY TEMPERATURE CONDITION

condition which is reached when the temperature, measured at the centre of the TEST DEVICE positioned on the mid-point of the INFANT RADIANT WARMER mattress, does not vary by more than 1 °C over a period of 1 h

201.3.210

TEST DEVICE

totally matt blackened disc used as a reproducible receiver of radiant energy during testing of the INFANT RADIANT WARMER (see Figure 201.102)