



Designation: C 133 – 97

Standard Test Methods for Cold Crushing Strength and Modulus of Rupture of Refractories¹

This standard is issued under the fixed designation C 133; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

This standard has been approved for use by agencies of the Department of Defense.

ϵ^1 NOTE—Approved actions inadvertently omitted were added editorially January 22, 1997.

1. Scope

1.1 These test methods cover the determination of the cold crushing strength and the modulus of rupture (MOR) of dried or fired refractory shapes of all types.

1.2 The test methods appear in the following sections:

Test Method	Sections
Cold Crushing Strength	4 to 9
Modulus of Rupture	10 to 15

1.3 The values stated in inch-pound units are to be regarded as the standard. The values given in parentheses are for information only.

1.4 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

2. Referenced Documents

2.1 *ASTM Standards:*

C 862 Practice for Preparing Refractory Concrete Specimens by Casting²

C 1054 Practice for Pressing and Drying Refractory Plastic and Ramming Mix Specimens²

E 4 Practices for Force Verification of Testing Machines³

3. Significance and Use

3.1 The cold strength of a refractory material is an indication of its suitability for use in refractory construction. (It is not a measure of performance at elevated temperatures.)

3.2 These test methods are for determining the room temperature flexural strength in 3-point bending (cold modulus of rupture) or compressive strength (cold crushing strength), or both, for all refractory products.

3.3 Considerable care must be used to compare the results of different determinations of the cold crushing strength or modulus of rupture. The specimen size and shape, the nature of the specimen faces (that is, as-formed, sawed, or ground), the orientation of those faces during testing, the loading geometry, and the rate of load application, may all significantly affect the numerical results obtained. Comparisons of the results between different determinations should not be made if one or more of these parameters differ between the two determinations.

3.4 The relative ratio of the largest grain size to the smallest specimen dimension may significantly affect the numerical results. For example, smaller, cut specimens containing large grains may present different results than the bricks from which they were cut. Under no circumstances should 6- by 1- by 1-in. (152- by 25- by 25-mm) specimens be prepared and tested for materials containing grains with a maximum grain dimension exceeding 0.25 in. (6.4 mm).

3.5 This test method is useful for research and development, engineering application and design, manufacturing process control, and for developing purchasing specifications.

COLD CRUSHING STRENGTH

4. Apparatus

4.1 *Testing Machine*—Any form of standard mechanical or hydraulic compression testing machine conforming to the requirements of Practices E 4 may be used.

NOTE 1—For low-strength materials (such as insulating bricks or castables), a sensitivity of 20 lbf (67 kN) or less is required. The use of a hydraulic testing machine is also preferred over the mechanical type for these materials.

4.2 *Spherical Bearing Block*—The plane surface of the spherical bearing block (see Fig. 1) shall have an area which is equal to or greater than the cross section of the test specimen.

5. Test Specimens

5.1 *Brick and Shapes (bulk density greater than 100 lb/ft³ (1.60 g/cm³))*—The test specimens shall be 2-in. (51-mm) cubes or cylinders, 2 in. (51 mm) in diameter by 2 in. (51 mm) high. The height should be parallel to the original direction of

¹ These test methods are under the jurisdiction of ASTM Committee C-8 on Refractories and are the direct responsibility of Subcommittee C08.01 on Strength.

Current edition approved Jan. 22, 1997. Published March 1997. Originally published as C 133 – 37 T. Last previous edition C 133 – 96.

² *Annual Book of ASTM Standards*, Vol 15.01.

³ *Annual Book of ASTM Standards*, Vol 03.01.

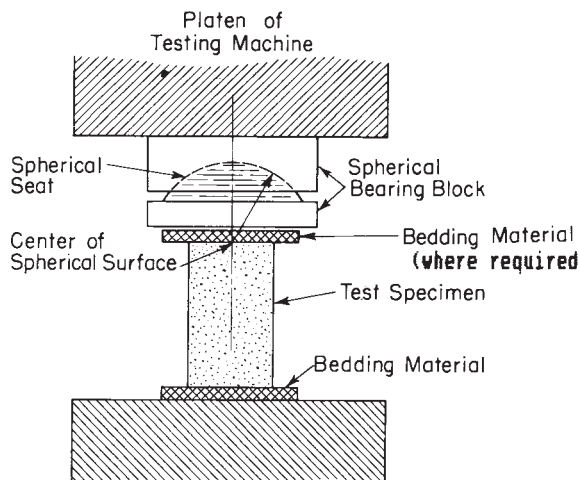


FIG. 1 Recommended Design for Crushing Test Assembly, Including Bearing Block

pressing of the brick or shape. In the case of special shapes, only one specimen shall be cut from a single shape and as many of the original surfaces as possible shall be preserved. In preparing specimens from irregular or large refractory shapes, any method involving the use of abrasives, such as a high-speed abrasion wheel, core drill, or rubbing bed, that will produce a specimen with approximately plane and parallel sides without weakening the structure of the specimen may be used.

5.2 *Insulating Brick or Shapes* (typical bulk density of 100 lb/ft³ (1.60 g/cm³), or greater than 45 % total porosity, or both)—The test specimens shall be 4½ by 4½ by 2½ or 3 in. (114 by 114 by 64 or 76 mm), each taken from a different brick. It is permissible to prepare these specimens from the half-brick resulting from the modulus of rupture test (see Sections 10-15). The selected compression test section shall be free of cracks, chipped surfaces, and other obvious defects. The test surfaces shall be approximately parallel planes.

5.3 *Castable Refractories*—The test specimens shall be 2- by 2- by 2-in. (51- by 51- by 51-mm) cubes or cylinders 2 in. (51 mm) in diameter by 2 in. (51 mm) high, prepared by casting or gunning. It is permissible to prepare one specimen from each 9- by 2- by 2-in. (230- by 51- by 51-mm) bar after the modulus of rupture test (see Sections 10-15). The selected compression test section shall be free of cracks, chipped surfaces, and other obvious defects. The loaded surfaces shall be approximately parallel planes. All samples must be dried at 220 to 230°F (105 to 110°C) for 18 h (overnight). Upon removal from the oven, allow the sample to cool naturally until cool to the touch. Complete testing within 2 h of removal from the drying oven. (See Practices C 862 and C 1054.)

6. Procedure

6.1 At least five specimens from an equivalent number of refractory shapes compose a sample.

NOTE 2—For relatively weak specimens like insulating castables or insulating firebricks, a minimum sample size of ten specimens is preferred.

6.2 *Brick and Shapes*—Place a cellulose fiber wall board (for example, Masonite⁴) 0.25 in. (6.4 mm) in thickness and extending 0.5 in. (12.7 mm) or more beyond the edges of the loaded faces of the specimen. Apply the load parallel to the direction in which the brick was originally pressed.

6.3 *Regular and High Strength Castables*—Place a cellulose fiber wall board 0.25 in. (6.4 mm) in thickness and extending 0.5 in. (12.7 mm) or more beyond the edges of the loaded faces of the specimen. Apply the load on the 2- by 2-in. (51- by 51-mm) or 2-in. (51-mm) diameter face and perpendicular to the depth of the specimen as originally cast or gunned.

6.4 *Insulating Brick or Shapes*—Apply the load directly to the 4½- by 4½-in. (114- by 114-mm) surface of the test specimen.

6.5 *Insulating Castables* (typical bulk density of 100 lb/ft³ (1.60 g/cm³), or greater than 45 % total porosity, or both)—Apply the load directly to the 2- by 2-in. (51- by 51-mm) face and perpendicular to the depth of the specimen as originally cast or gunned.

6.6 Use the bearing block on top of the test specimen, and position it so that the center of the sphere is in alignment with the vertical axis of the specimen (see Fig. 1). Keep the spherical bearing block thoroughly lubricated to ensure accurate adjustment which may be made by hand under a small initial load for each specimen.

NOTE 3—The spherical bearing block may not be necessary on test machines having mechanical linkages which ensure that the stress applied is colinear with the axis of the specimen.

6.7 For *dense* refractories with sufficient strength to require greater than about 3 min per test, initial loading to one-half of the anticipated failure load may be accomplished at any convenient rate exceeding the specified rate. Subsequently, each specimen shall be crushed with a compressive load applied at the standard rates specified in Table 1. The rates shall not vary by more than ±10 % of the specified rate for the type of refractory being tested.

6.8 When using a mechanical testing machine, keep the balance beam in a constantly floating position.

6.9 Specimens are loaded, as specified, to failure. Failure is defined as the collapse of the specimen (failure to support the load), or the reduction of the specimen height to 90 % of its original value. The maximum applied load is recorded.

7. Calculation

7.1 Calculate the cold crushing strength using Eq 1:

$$S = W/A \quad (1)$$

⁴ Masonite has been found satisfactory for this purpose.

TABLE 1 Standard Loading Rates for Cold Crushing Strength

Refractory Type	Size, in. (mm)	Loaded Cross Section, in. (mm)	Loaded Area, in. ² (mm ²)	Stress Rate, lbf/in. ² /min (MPa/min)	Loading Rate, lbf/min (kN/min)	Strain Rate, ^A in./min (mm/min)
<i>Refractory Brick and Shapes</i>						
Density >100 lb/ft ³ (>1.60 gm/cm ³), or <45 % true porosity, or both (Includes regular or high strength castables and fired plastic or rammed refractories)	2 × 2 × 2	2 × 2	4	1750 ^B	7000 ^B	0.05 ^B
	(51 × 51 × 51)	(51 × 51)	(2601)	(12)	(31.2)	(1.3)
	2 diameter × 2	2, diameter	3.14	1750 ^B	5500 ^B	0.05 ^B
	(51 diameter × 51)	(51, diameter)	(2027)	(12)	(24.3)	(1.3)
<i>Insulating Refractories</i>						
Density <100 lb/ft ³ (<1.60 gm/cm ³), or >45 % true porosity, or both (Includes dried, unfired plastic or rammed refractories)	4.5 × 4.5 × 2.5 ^{C,D}	4.5 × 4.5	20.25	435	8809	0.05
	(114 × 114 × 64)	(114 × 114)	(13 064)	(3)	(39)	(1.3)
	4.5 × 4.5 × 3 ^{CD}	4.5 × 4.5	20.25	435	8809	0.05
	(114 × 114 × 76)	(114 × 114)	(13 064)	(3)	(39)	(1.3)
	2 × 2 × 2 ^{D,E}	2 × 2	4	435	1740	0.05
	(51 × 51 × 51)	(51 × 51)	(2601)	(3)	(7.80)	(1.3)
	2 diameter × 2 ^E	2, diameter	3.14	435	1367	0.05
	(51 diameter × 51)	(51, diameter)	(2027)	(3)	(6.08)	(1.3)

^AWhere possible, loading at a constant stress rate is preferable to constant strain rate loading.

^BFor *dense* refractory brick and shapes requiring more than a 3-min test duration, specimens may be loaded to one half of the anticipated fracture strength at any convenient rate exceeding that specified.

^CThese sizes are preferred for insulating firebricks.

^DThese pieces may be cut from broken halves of MOR specimens.

^EThese sizes are preferred for insulating castables.

where:

- S = cold crushing strength, lbf/in.² (MPa),
- W = total maximum load indicated by the testing machine, lbf (N), and
- A = average of the areas of the top and bottom of the specimen perpendicular to the line of application of the load, in.² (mm²).

8. Report

8.1 Report the following:

8.1.1 Designation of the materials tested (that is, manufacturer, brand, description, lot number, etc.);

8.1.2 Specimen configuration, including size, shape, location in the original brick or shape, the character of the faces (that is, cut, drilled, as-pressed, as-cast, etc.), and the specimen orientation during testing;

8.1.3 Pretreatment, if any, given to the test pieces (for example, curing, firing, coking, etc.);

8.1.4 Number of specimens in a sample;

8.1.5 Individual specimen dimensions, the maximum applied load, and the calculated cold crushing strength for each specimen (see 7.1);

8.1.6 Mean cold crushing strength and standard deviation for each sample.

9. Precision and Bias

9.1 *Precision*—The precision of this test method is currently being investigated.

9.2 *Bias*—No justifiable statement can be made on the bias of the test method for measuring the cold crushing strength of refractories, because the value of cold crushing strength can be defined only in terms of a test method.

MODULUS OF RUPTURE

10. Apparatus

10.1 *Testing Machine*—Any form of standard mechanical or hydraulic compression testing machine conforming to the requirements of Practices E 4 may be used.

NOTE 4—Properly calibrated portable apparatus may be used.

10.2 *Bearing Surfaces*, that shall have a radius of curvature of $\frac{5}{8}$ in. (16 mm) or be cylindrical pieces $1\frac{1}{4}$ -in. (32-mm) in diameter. For 6- by 1- by 1-in. (152- by 25- by 25-mm) specimens, the radius of curvature shall be $\frac{3}{16}$ in. (5 mm) or cylindrical pieces $\frac{3}{8}$ in. (10 mm) in diameter. All such bearing surfaces shall be straight and of a length at least equal to the width of the test specimen. The supporting members for the lower bearing surfaces shall be constructed so as to provide a means for the alignment of the bearing surfaces with the under surface of the test specimen because the test brick may have a longitudinal twist. Apparatus of the design shown in Fig. 2 is recommended, although other types may be used, provided they conform to these requirements. A satisfactory alternative design is shown in Fig. 3.

11. Test Specimens

11.1 *Brick and Shapes (bulk density greater than 100 lb/ft³ (1.60 g/cm³)*—The preferred test specimens shall be standard 9- by 4½- by 2½- or 3-in. (228- by 114- by 64- or 76-mm) bricks, or specimens of equivalent size ground or cut from refractory shapes. In the case of special shapes, only one specimen shall be cut from a single shape. As many original surfaces as possible shall be preserved. Where brick sizes are impossible or impracticable, alternative specimen sizes of 9 by 2 by 2 in. (228 by 51 by 51 mm) or 6 by 1 by 1 in. (152 by 25 by 25 mm) may be prepared. In preparing specimens from irregular or larger shapes, any method involving the use of abrasives, such as a high-speed abrasion wheel or rubbing bed,