

# INTERNATIONAL STANDARD

**ISO  
8638**

First edition  
1989-09-15

---

---

## Extracorporeal blood circuit for haemodialysers, haemofilters and haemoconcentrators

*Circuit sanguin extracorporel pour les hémodialyseurs, les hémofiltres  
et les hémococoncentrateurs*

iTeh STANDARD PREVIEW  
(standards.iteh.ai)

ISO 8638:1989

<https://standards.iteh.ai/catalog/standards/sist/bd7c6db9-df3a-4119-9f28-325cbf23f3d5/iso-8638-1989>



Reference number  
ISO 8638 : 1989 (E)

## Contents

	Page
Foreword .....	iii
Introduction .....	iv
1 Scope .....	1
2 Normative references .....	1
3 Definitions .....	1
4 Requirements .....	1
5 Test methods .....	5
6 Packaging, marking and accompanying documentation .....	7

**ITeH STANDARD PREVIEW**  
**(standards.iteh.ai)**

ISO 8638:1989

<https://standards.iteh.ai/catalog/standards/sist/bd7c6db9-df3a-4119-9f28-325cbf23f3d5/iso-8638-1989>

© ISO 1989

All rights reserved. No part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from the publisher.

International Organization for Standardization  
Case postale 56 • CH-1211 Genève 20 • Switzerland

Printed in Switzerland

## Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

Draft International Standards adopted by the technical committees are circulated to the member bodies for approval before their acceptance as International Standards by the ISO Council. They are approved in accordance with ISO procedures requiring at least 75 % approval by the member bodies voting.

International Standard ISO 8638 was prepared by Technical Committee ISO/TC 150, *Implants for surgery*.

<https://standards.iteh.ai/catalog/standards/sist/bd7c6db9-df3a-4119-9f28-325cbf23f3d5/iso-8638-1989>

## Introduction

This International Standard is concerned with the extracorporeal circuit manufactured for single use and intended for use in conjunction with haemodialysers, haemofilters or haemoconcentrators. The requirements specified in this International Standard for the extracorporeal circuit will help to ensure safety and satisfactory function.

It was not found practicable to specify materials of construction nor to give test methods for biocompatibility, validation of sterility, non-pyrogenicity and certain performance characteristics of the extracorporeal circuit. This International Standard therefore requires only that materials will have been tested and that the methods and results are made available upon request.

The specifications for physical characteristics have been limited to those deemed necessary for safe and effective function of the device. A design standard is required for connectors to the blood ports of the haemodialyser, haemofilter or haemoconcentrator and to the blood access device to ensure the compatibility of the circuit and the corresponding device. These design and dimension specifications have been selected to minimize the risk of leakage of blood and the ingress of air. Connectors with either fixed or loose locking shells are permitted.

Attention is drawn to the work of Sub-committee 62D, *Electromedical equipment*, of the International Electrotechnical Commission (IEC) regarding the electrotechnical aspects of dialysis systems. There is no IEC publication dealing with haemofiltration or haemoconcentration systems.

This International Standard reflects the consensus of physicians, manufacturers and other interested parties for devices that are approved for clinical use. Conformance with the standard is voluntary and it does not supersede any national regulation.

# Extracorporeal blood circuit for haemodialysers, haemofilters and haemoconcentrators

## 1 Scope

This International Standard specifies requirements for the extracorporeal blood circuit for single use which is to be used in conjunction with haemodialysers, haemofilters and haemoconcentrators.

Materials of construction and test methods for biocompatibility, validation of sterility, non-pyrogenicity and some performance characteristics are not specified; the rationale for these omissions is given in the Introduction.

This International Standard applies to the blood tubing and integral accessory tubing, including fluid and infusion tubings and tubing for attaching the extracorporeal blood circuit to pressure monitors.

This International Standard does not apply to haemodialysers, haemofilters, haemoconcentrators, vascular access devices, blood pumps, pressure monitors of the extracorporeal blood circuit, air detection devices, haemodialysis systems to prepare, maintain and monitor the dialysing fluid, and hardware used to perform haemofiltration or haemoconcentration.

NOTE — Requirements for haemodialysers, haemofilters and haemoconcentrators are specified in ISO 8637.

## 2 Normative references

The following standards contain provisions which, through reference in this text, constitute provisions of this International Standard. At the time of publication, the editions indicated were valid. All standards are subject to revision, and parties to agreements based on this International Standard are encouraged to investigate the possibility of applying the most recent editions of the standards indicated below. Members of IEC and ISO maintain registers of currently valid International Standards.

ISO 472: 1979, *Plastics — Vocabulary*.

ISO 594-2 — 1), *Conical fittings with a 6 % (Luer) taper for syringes, needles and certain other medical equipment — Part 2: Lock fittings*.

ISO 8637 : 1989, *Haemodialysers, haemofilters and haemoconcentrators*.

## 3 Definitions

For the purposes of this International Standard the following definitions apply.

**3.1 arterial blood circuit:** Portion of the extracorporeal blood pathway from the vascular access device of the patient to the blood inlet of the haemodialyser, haemofilter or haemoconcentrator.

**3.2 non-pyrogenic:** Free of pyrogenic materials within the limit of error of test methods for such determinations, as defined by the national regulatory agency of the country in which the device is to be marketed or, where available, an International Standard, and maintained in that state by suitable protection.

**3.3 pump segment:** Portion of the extracorporeal blood circuit that is acted upon by the blood pump.

**3.4 sterile:** Free from all living organisms within the limits of validation tests for sterility and maintained in that state by suitable protection.

**3.5 venous blood circuit:** Extracorporeal blood circuit from the outlet of the haemodialyser, haemofilter or haemoconcentrator, returning blood to the vascular access device of the patient.

## 4 Requirements

### 4.1 Good manufacturing practice

The extracorporeal circuit shall be manufactured in a clean environment and the fluid pathways shall be free of visible foreign material.

NOTE — Attention is drawn to the need to establish whether codes for good manufacturing practice exist in the country in which the device is produced and, if applicable, in the countries in which the device is to be marketed.

Testing shall be carried out in accordance with 5.1.

### 4.2 Toxicology and biological compatibility

Samples of the device shall be tested for freedom from toxicity using, if available, the method specified in the relevant national standard and the results of such tests shall indicate freedom from biological hazard. If requested, details of the test method

1) To be published.

and the results shall be made available by the manufacturer of the device.

NOTE — Attention is drawn to the need to establish whether national regulations or national standards governing toxicology and biocompatibility testing exist in the country in which the device is produced and, if applicable, in the countries in which the device is to be marketed.

Testing shall be carried out in accordance with 5.2.

### 4.3 Sterility

The fluid pathways of the device shall be supplied sterile.

NOTE — Attention is drawn to the need to establish whether national regulations or national standards governing sterility testing exist in the country in which the device is produced and, if applicable, in the countries in which the device is to be marketed.

Testing shall be carried out in accordance with 5.3.

### 4.4 Pyrogenicity

The blood pathway(s) of the device shall be non-pyrogenic. If requested, details of the test method(s) and the results shall be made available by the manufacturer of the device.

NOTE — Attention is drawn to the need to establish whether national regulations or national standards governing pyrogen testing exist in the country in which the device is produced and, if applicable, in the countries in which the device is to be marketed.

Testing shall be carried out in accordance with 5.4.

### 4.5 Residues from sterilization

After sterilization by the procedure recommended by the manufacturer, the device shall be tested for freedom from toxic residues that have adverse chemical, physical or biological effects on the blood or that result in release of clinically significant amounts of potentially toxic substances into the blood. If requested, details of the test methods and the results shall be made available by the manufacturer of the device.

NOTE — Attention is drawn to the need to establish whether national regulations or national standards governing testing for residues from sterilization exist in the country in which the device is produced and, if applicable, in the countries in which the device is to be marketed.

Testing shall be carried out in accordance with 5.5.

### 4.6 Mechanical characteristics

#### 4.6.1 Structural integrity

Samples of the extracorporeal circuit shall be capable of withstanding

- a) a pressure above atmospheric pressure at sea level that is 1,5 times the manufacturer's specified maximum pressure, and
- b) a pressure 200 mmHg below atmospheric pressure (at sea level).

The pump segment shall be capable of withstanding a minimum of 24 h of use under worst-case conditions.

Testing shall be carried out in accordance with 5.6.1.

#### 4.6.2 Connectors to haemodialyser, haemofilter or haemoconcentrator

The dimensions of the fitting for connection to the haemodialyser, haemofilter or haemoconcentrator shall be as given in figures 1 to 3.

The dimensions shall be checked in accordance with 5.6.2.

#### 4.6.3 Connector to vascular access device

The fitting for connecting the extracorporeal circuit to a vascular access device shall be a male 6 % (Luer) taper lock fitting; this fitting shall be in accordance with ISO 594-2.

The fitting shall be checked in accordance with 5.6.3.

#### 4.6.4 Connectors to ancillary components

All parts of the extracorporeal circuit intended for use with ancillary components, such as heparin lines and pressure transducer lines, shall terminate in a female 6 % (Luer) taper lock fitting; this fitting shall be in accordance with ISO 594-2.

The fittings shall be checked in accordance with 5.6.4.

#### 4.6.5 Access ports

Where injection ports are incorporated into the extracorporeal circuit, they shall be capable of withstanding, without leakage, puncture by needle having at least an internal diameter of 0,8 mm (21 gauge). The injection ports shall be designed so as to minimize the risk of the needle piercing the tube completely and causing injury.

Testing shall be carried out in accordance with 5.6.5.

#### 4.6.6 Colour coding

If the arterial extracorporeal blood circuit differs from the venous extracorporeal blood circuit, the arterial circuit shall be colour-coded **red** and the venous circuit shall be colour-coded **blue**. The coding shall be prominently displayed within 100 mm of the end of the tubing.

The colour coding shall be checked in accordance with 5.6.6.

### 4.7 Physical characteristics

#### 4.7.1 Volume

The volume of the blood pathway of the venous and arterial extracorporeal circuits shall be equal to the manufacturer's stated values  $\pm 20$  %.

Testing shall be in accordance with 5.7.1.

#### 4.7.2 Pump segment

The length and internal diameter of the pump segment shall be equal to the manufacturer's stated values  $\pm 5$  %.

The dimensions shall be checked in accordance with 5.7.2.

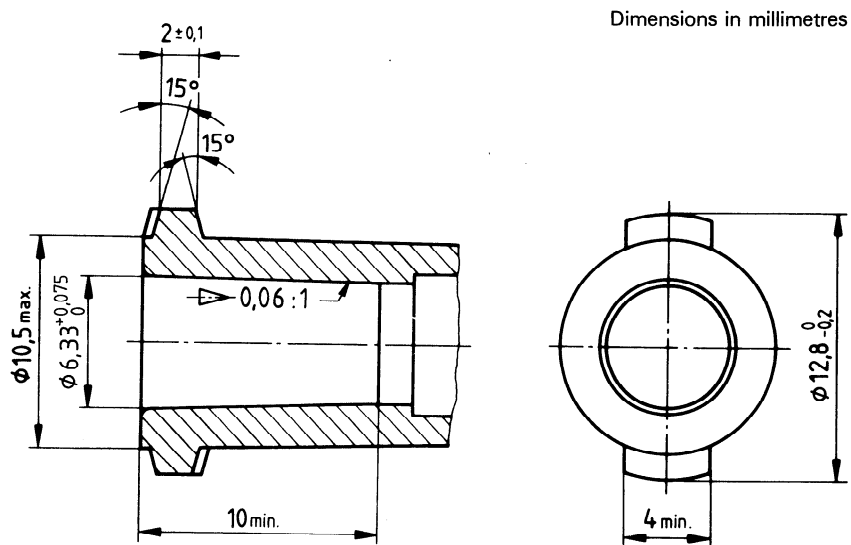


Figure 1 – Main fitting dimensions of extracorporeal circuit connector to blood ports of haemodialyser, haemofilter or haemoconcentrator



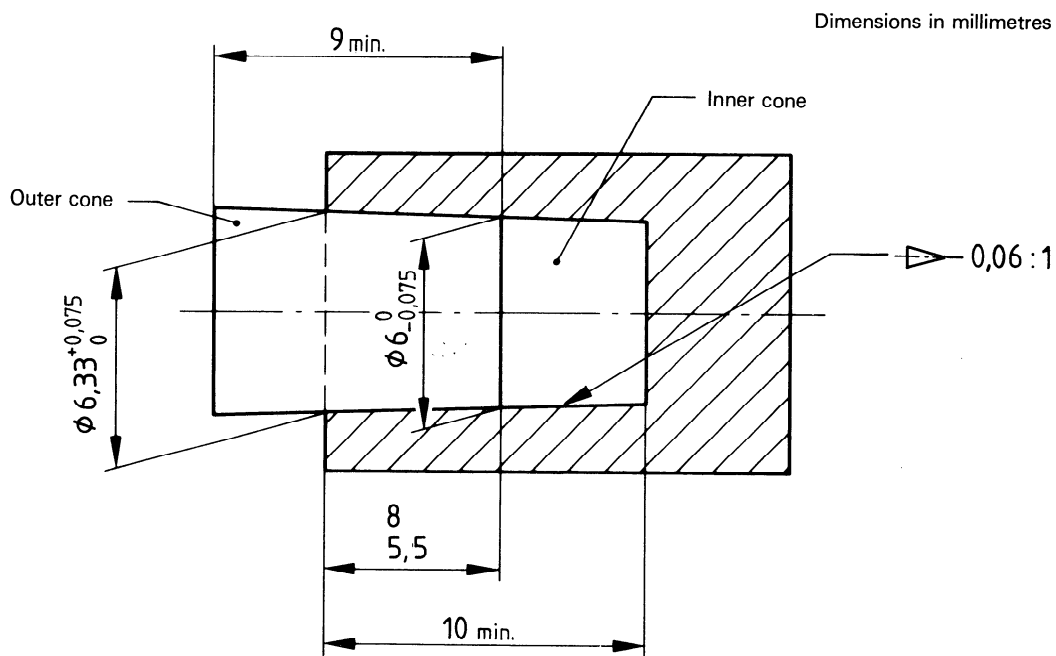


Figure 2 – Length of engagement of male and female cones of blood inlet and outlet connectors

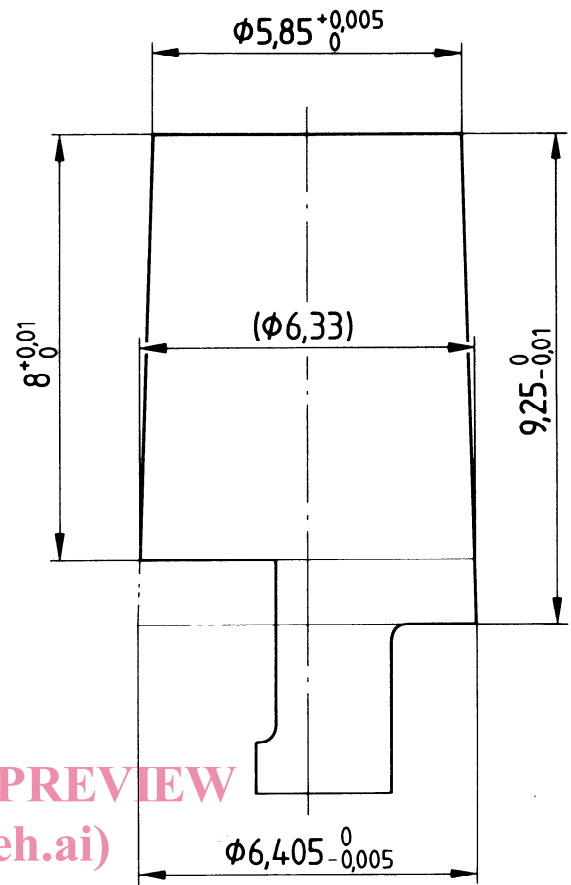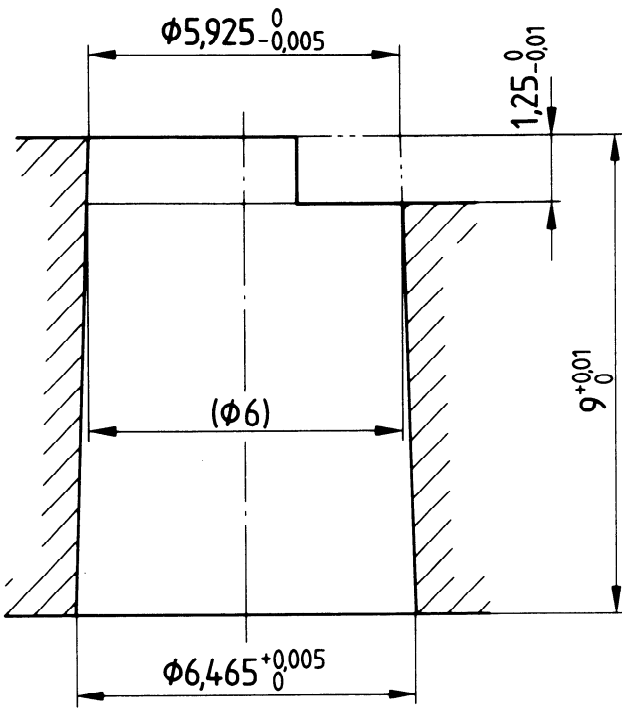

iTeh STANDARD PREVIEW  
(standards.iteh.ai)

ISO 8638:1989

<https://standards.iteh.ai/catalog/standards/sist/bd7c6db9-d3a-4119-9f28-325cbf23f3d5/iso-8638-1989>


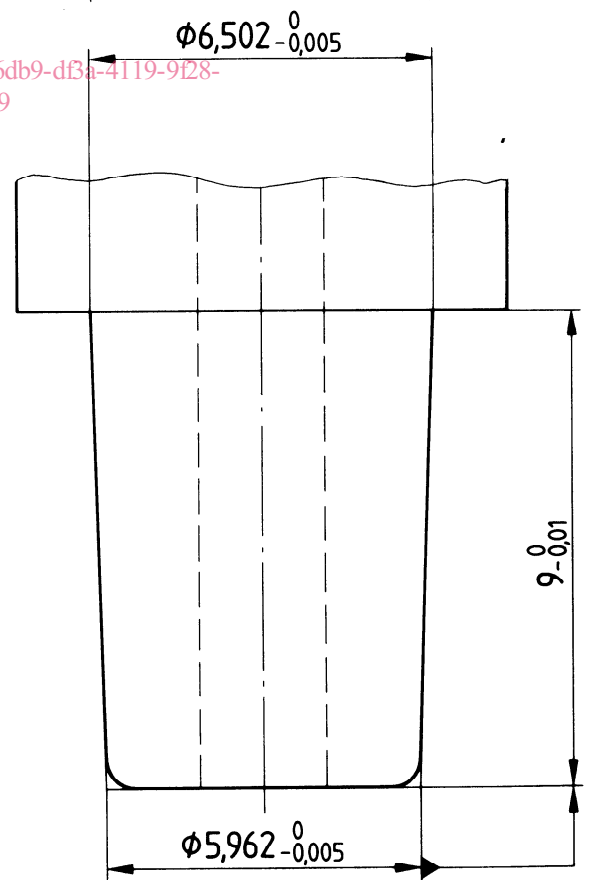


Figure 3 — Details of 6 % taper test fitting for connector to haemodialyser, haemofilter or haemoconcentrator blood port

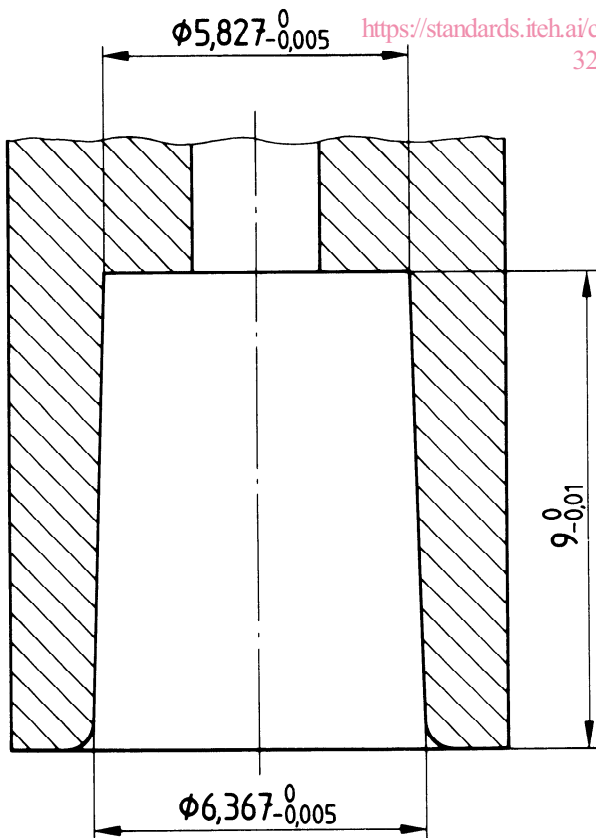

## 5 Test methods

### 5.1 Good manufacturing practice

Compliance with the requirement specified in 4.1 shall be determined by inspection.

### 5.2 Toxicology and biological compatibility

The toxicology and biological compatibility of materials (of a device) which will come into contact with biological fluids shall be determined on samples of each new type of device prior to its marketing or after any change in the materials of construction of that type of device or after any change in the method of sterilization.

NOTE — Testing should be carried out using the method(s) specified in appropriate national regulations or national standards.

### 5.3 Sterility

The sterilization process shall be validated on samples of the finished device prior to marketing a new type of device, and, thereafter, the sterilization process shall be monitored for each batch.

### 5.4 Pyrogenicity

Testing for pyrogens shall be carried out on samples of each new type of device prior to marketing, and, thereafter, the manufacturer shall perform pyrogen testing at intervals shown to ensure non-pyrogenicity of the device.

### 5.5 Residues from sterilization

Samples of the finished device shall be tested for potentially toxic residues by recognized toxicological methods prior to marketing a new type of device, and, thereafter, the manufacturer shall test for toxic residues at intervals shown to ensure the safety of the device and after any change of materials of construction.

### 5.6 Mechanical characteristics

#### 5.6.1 Structural integrity and access port leakage

The test described shall be carried out prior to marketing a new type of device; it is not intended to be a quality control test.

##### 5.6.1.1 Principle

Subjection of the extracorporeal circuit to simulated use during which the access port is punctured. Subjection of the extracorporeal circuit to the specified pressures (see 4.6.1) above and below atmospheric pressure at sea level. Observation for leaks.

##### 5.6.1.2 Reagents

**5.6.1.2.1 Anticoagulated bovine or human plasma**, with a protein mass concentration of  $60 \text{ g/l} \pm 5 \text{ g/l}$  for the perfusate during simulated use.

**5.6.1.2.2 Distilled water, freshly boiled**, for the subatmospheric test.

##### 5.6.1.3 Apparatus

**5.6.1.3.1 Blood pump**, as recommended by the manufacturer, or, if the manufacturer does not recommend a blood pump, **an adjustable double roller blood pump** as commonly used for clinical haemodialysis, haemofiltration or haemoconcentration. The rollers shall be just occlusive at the test pressure. Each roller shall be occlusive at the beginning, the middle and the end of the stroke.

**5.6.1.3.2 Stainless steel or plastic vessel** for the perfusate.

**5.6.1.3.3 Heating device**, capable of maintaining the perfusate at  $37 \text{ }^\circ\text{C} \pm 1 \text{ }^\circ\text{C}$ .

**5.6.1.3.4 Jig**, for puncturing the access port at the same location.

**5.6.1.3.5 Needle**, having the largest internal diameter recommended by the manufacturer or having an internal diameter of 0.8 mm (21 gauge), whichever is the larger.

**5.6.1.3.6 Open or occluded steel reference connectors**, as appropriate (the connectors for the blood access and ancillary tubing), which comply with the requirements specified in ISO 594-2. See figure 3.

**5.6.1.3.7 Blood port**, complying with the requirements specified in clause 4.6.3 of ISO 8637 : 1989.

**5.6.1.3.8 Tubing**, to be attached to the blood port (unless it is occluded), and to the connectors to the blood access connector and to the ancillary tubing connector (5.6.1.3.6) that can withstand the test conditions.

**5.6.1.3.9 Pressurized air source**, capable of maintaining the extracorporeal circuit at the specified pressure above atmospheric pressure.

**5.6.1.3.10 Suction device**, capable of maintaining the specified pressure below atmospheric pressure.

**5.6.1.3.11 Pressure gauges**, accurate to  $\pm 10 \text{ mmHg}$ .

**5.6.1.3.12 Vessel**, filled with water, that will accommodate the extracorporeal circuit during the subatmospheric pressure test.

#### 5.6.1.4 Sampling and preparation of test samples

A statistically significant sample of extracorporeal circuits drawn at random from the manufacturer's production which have passed all safety and quality control measures, where applicable, shall be used.

iTeh STANDARD PREVIEW  
(standards.iteh.ai)  
ISO 8638:1989  
<https://standards.iteh.ai/catalog/standards/sist/bd7c6db9-d3a-4119-9d28-325cbf23bd5/iso-8638-1989>