



Standard Practice for Testing Fixed-Wavelength Photometric Detectors Used in Liquid Chromatography¹

This standard is issued under the fixed designation E 685; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

1. Scope

1.1 This practice is intended to serve as a guide for the testing of the performance of a photometric detector (PD) used as the detection component of a liquid-chromatographic (LC) system operating at one or more fixed wavelengths in the range 210 to 800 nm. Measurements are made at 254 nm, if possible, and are optional at other wavelengths.

1.2 This practice is intended to describe the performance of the detector both independently of the chromatographic system (static conditions) and with flowing solvent (dynamic conditions).

1.3 For general liquid chromatographic procedures, consult Refs (1-9).²

1.4 For general information concerning the principles, construction, operation, and evaluation of liquid-chromatography detectors, see Refs (10 and 11) in addition to the sections devoted to detectors in Refs (1-7).

1.5 The values stated in SI units are to be regarded as standard.

1.6 *This standard does not purport to address all of the safety problems, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

2. Referenced Documents

2.1 ASTM Standards:

E 275 Practice for Describing and Measuring Performance of Ultraviolet, Visible, and Near-Infrared Spectrophotometers³

E 682 Practice for Liquid Chromatography Terms and Relationships⁴

3. Terminology

3.1 Definitions:

¹ This practice is under the jurisdiction of ASTM Committee E13 on Molecular Spectroscopy and is the direct responsibility of Subcommittee E13.19 on Chromatography.

Current edition approved Feb. 15, 1993. Published April 1993. Originally published as E 685 – 79. Last previous edition E 685 – 79.

² The boldface numbers in parentheses refer to the list of references at the end of this practice.

³ *Annual Book of ASTM Standards*, Vol 14.02.

⁴ *Annual Book of ASTM Standards*, Vol 03.06.

3.1.1 *absorbance calibration*—the procedure that verifies that the absorbance scale is correct within $\pm 5\%$.

3.1.2 *drift*—the average slope of the noise envelope expressed in absorbance units per hour (AU/h) as measured over a period of 1 h.

3.1.3 *dynamic*—under conditions of a flow rate of 1.0 mL/min.

3.1.4 *linear range—of a PD*, the range of concentrations of a test substance in a mobile phase over which the response of the detector is constant to within 5% as determined from the linearity plot specified below and illustrated in Fig. 1. The linear range should be expressed as the ratio of the highest concentration to the minimum detectable concentration or the lowest linear concentration, whichever is greatest.

3.1.5 *long-term noise*—the maximum amplitude in AU for all random variations of detector signal of frequencies between 6 and 60 cycles per hour (0.1 and 1.0 cycles per min).

3.1.5.1 *Discussion*—It represents noise that can be mistaken for a late-eluting peak. This noise corresponds to the observed noise only and may not always be present.

3.1.6 *minimum detectability—of a PD*, that concentration of a specific solute in a specific solvent that results in a detector response corresponding to twice the static short-term noise.

3.1.7 *response time (speed of output)—the detector*, the time required for the detector output to change from 10% to 90% of the new equilibrium value when the composition of the mobile phase is changed in a stepwise manner, within the linear range of the detector.

3.1.7.1 *Discussion*—Because the detector volume is very small and the transport rate is not diffusion dependent, the response time is generally fast enough to be unimportant. It is generally comparable to the response time of the recorder and dependent on the response time of the detector electrometer and on the recorder amplifier. Factors that affect the observed response time include the true detector response time, electronic filtering, and system band-broadening.

3.1.8 *short-term noise*—the maximum amplitude, peak to peak, in AU for all random variations of the detector signal of a frequency greater than one cycle per minute.

3.1.8.1 *Discussion*—It determines the smallest signal detectable by a PD, limits the precision attainable in quantitation of trace-level samples, and sets the lower limit on linearity. This noise corresponds to the observed noise only.

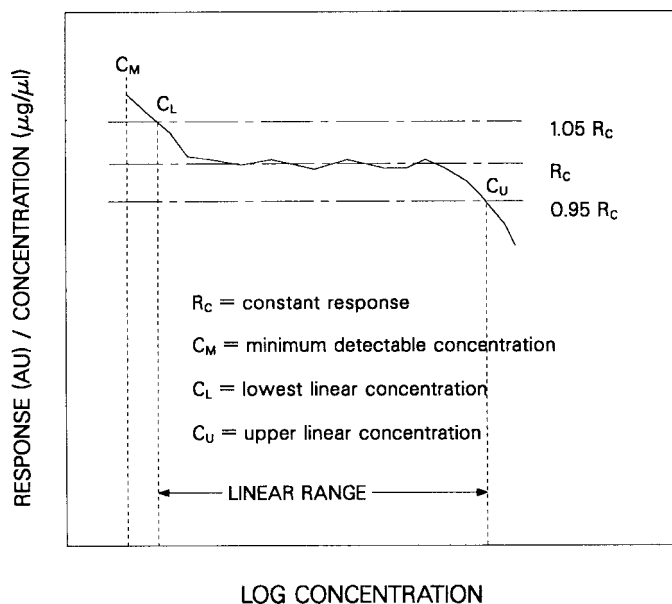


FIG. 1 Example of a Linearity Plot for a Photometric Detector

3.1.9 *static*—under conditions of no flow.

4. Significance and Use

4.1 Although it is possible to observe and measure each of the several characteristics of a detector under different and unique conditions, it is the intent of this practice that a complete set of detector specifications should be obtained *under the same operating conditions*. It should also be noted that to completely specify a detector's capability, its performance should be measured at several sets of conditions within the useful range of the detector. The terms and tests described in this practice are sufficiently general that they may be used regardless of the ultimate operating parameters.

4.2 Linearity and response time of the recorder or other readout device used should be such that they do not distort or otherwise interfere with the performance of the detector. This requires adjusting the gain, damping, and calibration in accordance with the manufacturer's directions. If additional electronic filters or amplifiers are used between the detector and the final readout device, their characteristics should also first be established.

5. Noise and Drift

5.1 *Test Conditions*—Pure, degassed methanol of suitable grade⁵ shall be used in the sample cell. Air or nitrogen shall be used in the reference cell if there is one. Nitrogen is preferred where the presence of high-voltage equipment makes it likely that there is ozone in the air. Protect the entire system from temperature fluctuations because these will lead to detectable drift.

5.1.1 The detector should be located at the test site and turned on at least 24 h before the start of testing. Insufficient warm-up may result in drift in excess of the actual value for the detector.

⁵ Distilled-in-glass or liquid-chromatography grade. Complete freedom from particles may require filtration, for example, through a 0.45-μm membrane filter.

5.2 Methods of Measurement:

5.2.1 Connect a suitable device (Note 1) between the pump and the detector to provide at least 75 kPa (500 psi) back pressure at 1.0 mL/min flow of methanol. Connect a short length (about 100 mm) of 0.25-mm (0.01-in.) internal-diameter stainless steel tubing to the outlet tube of the detector to retard bubble formation. Connect the recorder to the proper detector output channels.

NOTE 1—Suggested devices include (a) 2 to 4 m of 0.1-mm (0.004-in.) internal-diameter stainless steel tubing, (b) about 250 mm of 0.25 to 0.5-mm (0.01 to 0.02-in.) internal-diameter stainless steel tubing crimped with pliers or cutters, or (c) a constant back-pressure valve located between the pump and the injector.

5.2.2 Repeatedly rinse the reservoir and chromatographic system, including the detector, with degassed methanol to remove from the system all other solvents, any soluble material, and any entrained gasses. Fill the reservoir with methanol and pump this solvent through the system for at least 30 min to complete the system cleanup.

5.2.3 Air or nitrogen is used in the reference cell, if any. Ensure that the cell is clean, free of dust, and completely dry.

5.2.4 To perform the static test, cease pumping and allow the chromatographic system to stabilize for at least 1 h at room temperature without flow. Set the attenuator at maximum sensitivity (lowest attenuation), that is, the setting for the smallest value of absorbance units full-scale (AUFS). Adjust the response time as close as possible to 2 s for a PD that has a variable response time (Note 2). Record the response time used. Adjust the detector output to near midscale on the readout device. Record at least 1 h of detector signal under these conditions, during which time the ambient temperature should not change by more than 2°C.

NOTE 2—Time constant is converted to response time by multiplying by the factor 2.2. The effect of electronic filtering on observed noise may be studied by repeating the noise measurements for a series of response-time settings.

5.2.5 Draw pairs of parallel lines, each pair corresponding to between 0.5 and 1 min in length, to form an envelope of *all* observed random variations over any 15-min period (see Fig. 2). Draw the parallel lines in such a way as to minimize the distance between them. Measure the vertical distance, in AU, between the lines. Calculate the average value over all the segments. Divide this value by the cell length in centimetres to obtain the *static short-term noise*.

5.2.6 Now mark the center of each segment over the 15-min period of the static short-term noise measurement. Draw a series of parallel lines encompassing these centers, each pair corresponding to 10 min in length, and choose that pair of lines whose vertical distance apart is greatest (see Fig. 2). Divide this distance in AU by the cell length in centimetres to obtain the *static long-term noise*.

5.2.7 Draw the pair of parallel lines that minimizes the vertical distance separating these lines over the 1 h of measurement (see Fig. 2). The slope of either line is the *static drift* expressed in AU/h.

5.2.8 Set the pump to deliver 1.0 mL/min under the same conditions of tubing, solvent, and temperature as in 5.2.1 through 5.2.3. Allow 15 min for the system to stabilize. Record

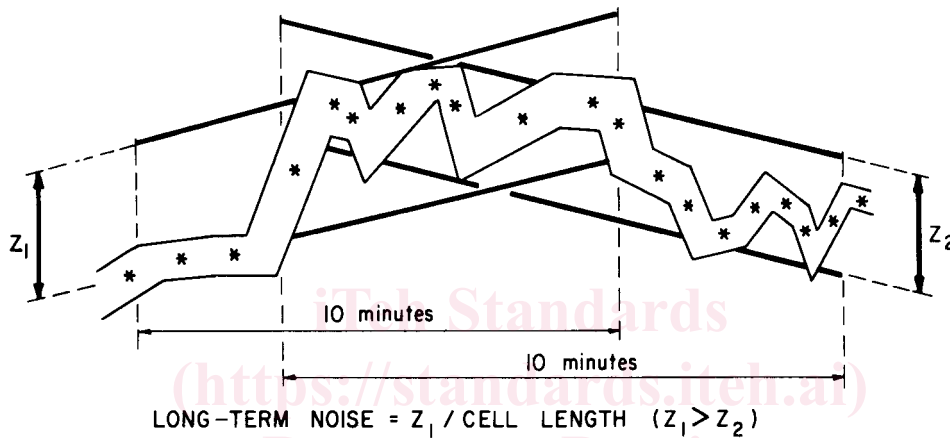
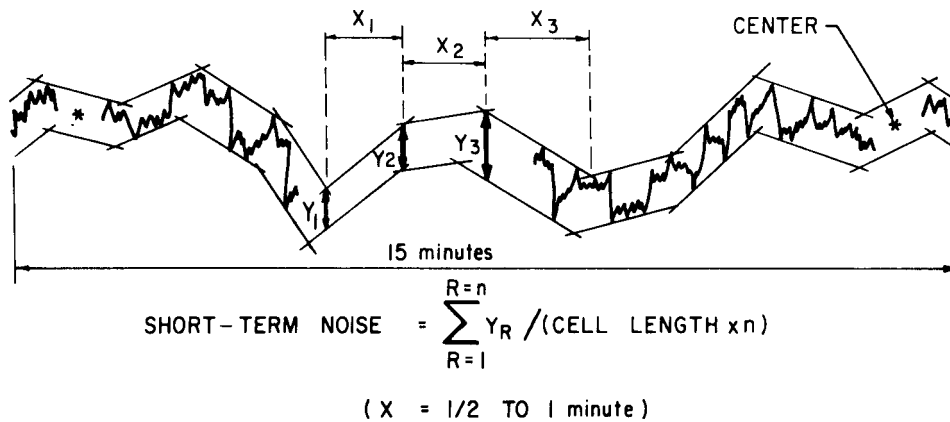


FIG. 2 Example for the Measurement of the Noise and Drift of a PD (Chart Recorder Output).

at least 1 h of signal under these flowing conditions, during which time the ambient temperature should not change by more than 2°C.

5.2.9 Draw pairs of parallel lines, measure the vertical distances, and calculate the *dynamic short-term noise* following the procedure of 5.2.5.

5.2.10 Make the measurement for the *dynamic long-term noise* following the procedure outlined in 5.2.6.

5.2.11 Draw the pair of parallel lines as directed in 5.2.7. The slope of these lines is the *dynamic drift*.

5.2.12 The actual noise of the system may be larger or smaller than the observed values, depending upon the method

of data collection, or signal monitoring of the detector, since observed noise is a function of the frequency, speed of response, and bandwidth of the readout device.

6. Minimum Detectability, Linear Range, and Calibration

6.1 *Methods of Measurement*—For the determination of the linear range of a PD, (12) for a specific substance, the response to that test substance must be determined. The following procedure is designed to provide a worst-case procedure.

6.1.1 Dissolve in methanol a suitable compound with an ultraviolet spectral absorbance that changes rapidly at the