



Standard Test Method for Potential Alkali-Silica Reactivity of Aggregates (Chemical Method)¹

This standard is issued under the fixed designation C 289; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

This standard has been approved for use by agencies of the Department of Defense.

1. Scope

1.1 This test method covers chemical determination of the potential reactivity of an aggregate with alkalies in portland-cement concrete as indicated by the amount of reaction during 24 h at 80°C between 1 *N* sodium hydroxide solution and aggregate that has been crushed and sieved to pass a 300- μm sieve and be retained on a 150- μm sieve.

1.2 The values stated in SI units are to be regarded as standard.

1.3 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.* A specific precautionary statement is given in 5.7.1.

2. Referenced Documents

2.1 ASTM Standards:

- C 114 Test Methods for Chemical Analysis of Hydraulic Cement²
- C 227 Test Method for Potential Alkali Reactivity of Cement-Aggregate Combinations (Mortar-Bar Method)³
- C 295 Guide for Petrographic Examination of Aggregates for Concrete³
- C 1005 Specification for Weights and Weighing Devices for Use in Physical Testing of Hydraulic Cements²
- D 1193 Specification for Reagent Water⁴
- D 1248 Specification for Polyethylene Plastics Molding and Extrusion Materials⁵
- E 11 Specification for Wire-Cloth Sieves for Testing Purposes⁶
- E 60 Practice for Photometric and Spectrophotometric Methods for Chemical Analysis of Metals⁷

¹ This test method is under the jurisdiction of ASTM Committee C-9 on Concrete and Concrete Aggregates and is the direct responsibility of Subcommittee C09.26 on Chemical Reactions of Materials.

Current edition approved April 15, 1994. Published August 1994. Originally published as C 289 – 52. Last previous edition C 289 – 87.

² *Annual Book of ASTM Standards*, Vol 04.01.

³ *Annual Book of ASTM Standards*, Vol 04.02.

⁴ *Annual Book of ASTM Standards*, Vol 11.01.

⁵ *Annual Book of ASTM Standards*, Vol 08.01.

⁶ *Annual Book of ASTM Standards*, Vol 14.02.

⁷ *Annual Book of ASTM Standards*, Vol 03.05.

2.2 American Chemical Society Documents: Reagent Chemicals, American Chemical Society Specifications

NOTE 1—For suggestions on the testing of reagents not listed by the American Chemical Society, see “Reagent Chemicals and Standards,” by Joseph Rosin, D. Van Nostrand Co., Inc., New York, NY, and the “United States Pharmacopeia.”

3. Significance and Use

3.1 This test method may be used in combination with other methods to evaluate the potential reactivity of siliceous aggregate with alkalies in portland-cement concrete. Reactions between a sodium hydroxide solution and siliceous aggregate have been shown to correlate with the performance of the aggregate in concrete structures and should be used where new aggregate sources are being evaluated or alkali-silica reactivity is anticipated.

3.2 The results from this test method can be obtained quickly, and, while not completely reliable in all cases, they provide useful data that may show the need for obtaining additional information through Test Method C 227 and Guide C 295.

4. Apparatus


4.1 *Scales*—The scales and weights used for weighing materials shall conform to the requirements prescribed in Test Method C 1005.

4.2 *Balances*—The analytical balance and weights used for determining dissolved silica by the gravimetric method shall conform to the requirements prescribed in Test Methods C 114.

4.3 *Crushing and Grinding Equipment*—A small jaw crusher and disk pulverizer or other suitable equipment capable of crushing and grinding approximately 4 kg of aggregate to pass a 300- μm sieve.

4.4 *Sieves*—300- μm and 150- μm square-hole, woven wire-cloth sieves conforming to Specification E 11.

4.5 *Containers*—Reaction containers of 50 to 75-mL capacity, made of corrosion-resistant steel or other corrosion-resistant material, and fitted with airtight covers. A container that has been found suitable is shown in Fig. 1. Other containers, made of corrosion-resistant material such as polyethylene, may be suitable. Such suitability can be demonstrated by a change in the alkalinity of the sodium hydroxide solution

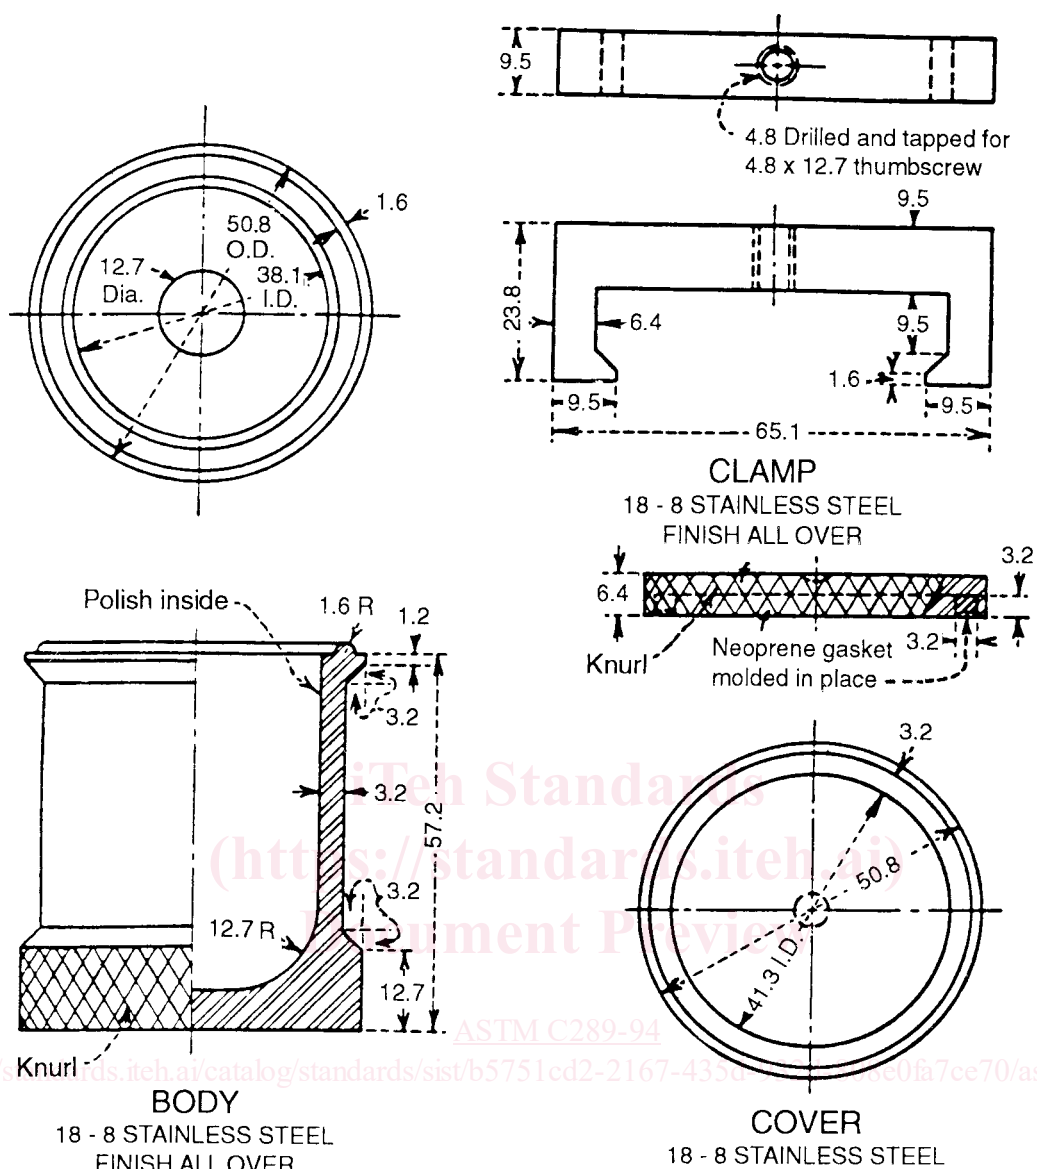

NOTE 1—All dimensions are in mm.

FIG. 1 Reaction Container

(R_c , Section on Reduction in Alkalinity) when used alone as a blank in the container in question, of less than 10 mmol/L.

4.6 *Constant-Temperature Bath*—A liquid bath capable of maintaining a temperature of $80 \pm 1^\circ\text{C}$ for 24 h.

4.7 *Spectrophotometer or Photometer*—A spectrophotometer or photoelectric photometer capable of measuring the transmission of light at a constant wavelength of approximately 410 nm (See Practice E 60).

4.8 *Glassware*—All glass apparatus and vessels should be carefully selected to meet the particular requirements for each operation. Standard volumetric flasks, burets, and pipets should be of precision grade.

5. Reagents

5.1 *Purity of Reagents*—Reagent grade chemicals shall be used in all tests. Unless otherwise indicated, all reagents shall

conform to the specifications of the Committee on Analytical Reagents of the American Chemical Society, where such specifications are available. Other grades may be used, provided it is first ascertained that the reagent is of sufficiently high purity to permit its use without lessening the accuracy of the determination.

5.2 *Purity of Water*—Unless otherwise indicated, references to water shall be understood to mean reagent water conforming to Type IV of Specification D 1193.

5.3 *Ammonium Molybdate Solution*—Dissolve 10 g of ammonium molybdate ($(\text{NH}_4)_6 \text{Mo}_7\text{O}_{24} \cdot 4\text{H}_2\text{O}$) in 100 mL of water. If the solution is not clear, filter through a fine-texture paper. Store the solution in a polyethylene container (Note 2).

5.4 *Hydrochloric Acid (1.19 kg/L)*—Concentrated hydrochloric acid (HCl). Store the solution in a chemically resistant

glass or suitable plastic container (Note 2).

5.5 *Hydrochloric Acid, Standard* (0.05 *N*)—Prepare approximately 0.05 *N* HCl and standardize to ± 0.0001 *N*. Store the solution in a chemically resistant glass or suitable plastic container (Note 2).

5.6 *Hydrochloric Acid* (1 + 1)—Mix equal volumes of concentrated HCl (1.19 kg/L) and water. Store the solution in a chemically resistant glass or suitable plastic container (Note 2).

5.7 *Hydrofluoric Acid* (approximately 50 % HF)—Concentrated hydrofluoric acid. Store in a polyethylene bottle (Note 2).

5.7.1 **Precaution**—Before using HF, review (1) the safety precautions for using HF, (2) first aid for burns, and (3) the emergency response to spills, as described in the manufacturer's Material Safety Data Sheet or other reliable safety literature. HF can cause very severe burns and injury to unprotected skin and eyes. Suitable personal protective equipment should always be used. These should include full-face shields, rubber aprons, and gloves impervious to HF. Gloves should be checked periodically for pin holes.

5.8 *Oxalic Acid Solution*—Dissolve 10 g of oxalic acid dihydrate in 100 mL of water. Store the solution in a chemically resistant glass or suitable plastic container (Note 2).

5.9 *Phenolphthalein Indicator Solution*—Dissolve 1 g of phenolphthalein in 100 mL of ethanol (1 + 1). Store the solution in a chemically resistant glass or suitable plastic container (Note 2).

5.10 *Silica Standard Solution*—Prepare a standard silica solution containing approximately 10 mmol of silica (SiO_2)/L by dissolving sodium metasilicate in water. Store the solution in a polyethylene bottle. Use a 100-mL aliquot of the solution to determine its SiO_2 content by the procedure described in 8.1.1-8.2.1. Do not use a standard silica solution older than 1 year, since dissolved ionic silica in such a solution slowly polymerizes, causing spuriously low photometric readings (Note 2).

5.11 *Sodium Hydroxide, Standard Solution* (1.000 ± 0.010 *N*)—Prepare a 1.000 ± 0.010 *N* sodium hydroxide (NaOH) solution and standardize to ± 0.001 *N*. Store the solution in a polyethylene bottle (Note 2). Protect the dry reagent and solution from contamination by carbon dioxide.

5.12 *Sulfuric Acid* (sp gr 1.84)—Concentrated sulfuric acid (H_2SO_4). Store the solution in a chemically resistant glass container (Note 2).

NOTE 2—In selecting the container, take care to ensure that the reagent will not be modified by reaction with the material composing the container, including pigments or other additives, or by transpiration of phases through the walls of the container. Containers with wall thickness not less than 0.51 mm and composed of high-density polyethylene meeting the requirements of Specification D 1248, for materials of Type III, Class A, are suitable.

6. Selection and Preparation of Test Samples

6.1 The test can be used for either fine or coarse aggregate, and when the fine and coarse aggregate are of the same material it can be used for the total aggregate.

6.2 The test sample shall be prepared from a representative portion of the aggregate by crushing so as to pass a 300- μm sieve, according to the following procedure (Note 3): Reduce

the coarse aggregate to pass a 4.75-mm sieve by means of a small jaw crusher. Sieve the crushed coarse aggregate and likewise the sand to recover the 150- μm particles. Discard the material passing the 150- μm sieve. Reduce the material retained on the 300- μm sieve by repeated passes through a disk-type pulverizer, with sieving after each pass. The separation of the plates shall be about 3 mm for the first pass and shall be progressively diminished until all the material passes the 300- μm sieve. Every effort shall be made to reduce as much as possible the proportion of fines passing the 150- μm sieve.

NOTE 3—It is recommended that each size fraction of coarse aggregate be separately processed according to 6.2, and that the 300- μm to 150- μm material obtained from each size fraction be combined in the proportions in which those fractions are to be used in the concrete. It is recommended that, wherever possible, the sand be screened and the several size fractions recombined in the proportions to be used in the concrete, prior to processing according to 6.2.

6.3 To ensure that all material finer than the 150- μm sieve has been removed, wash the sample over a 150- μm sieve. Do not wash more than 100 g over a 203-mm diameter sieve at one time. Dry the washed sample at $105 \pm 5^\circ\text{C}$ for 20 ± 4 h. Cool the sample and again sieve on the 150- μm sieve. If inspection of the sample indicates the presence of silty or clayey coatings on particles, repeat the washing and drying procedure, and sieve as before over the 150- μm sieve. Reserve the portion retained on the 150- μm sieve for the test sample.

7. Reaction Procedure

7.1 Weigh out three representative 25.00 ± 0.05 -g portions of the dry 150- μm to 300- μm test sample prepared in accordance with Section 6. Place one portion in each of the three of the reaction containers, and add by means of a pipet, 25 mL of the 1.000 *N* NaOH solution. To a fourth reaction container, by means of a pipet, add 25 mL of the same NaOH solution to serve as a blank. Seal the four containers and gently swirl them to liberate trapped air.

7.2 Immediately after the containers have been sealed, place them in a liquid bath maintained at $80 \pm 1.0^\circ\text{C}$. After $24 \pm \frac{1}{4}$ h, remove the containers from the bath and cool them, for 15 ± 2 min, under running tap water having a temperature below 30°C .

7.3 Immediately after the containers have been cooled, open them and filter the solution from the aggregate residue. Use a porcelain Gooch crucible (Note 4) with a disk of rapid, analytical-grade filter paper cut to fit the bottom of the crucible, setting the crucible in a rubber crucible holder in a funnel. Place a dry test tube, 35 to 50-mL capacity, in the filter flask to collect the filtrate, and seat the funnel in the neck of the filter flask. With the aspirator in operation or the vacuum line open, decant a small quantity of the solution onto the filter paper so it will seat properly in the crucible. Without stirring the contents of the container, decant the remaining free liquid into the crucible. When the decantation of the liquid has been completed, discontinue the vacuum and transfer the solids remaining in the container to the crucible and pack in place with the aid of a stainless-steel spatula. Then apply and adjust the vacuum to approximately 51 kPa. Continue the filtration until further filtration yields filtrate at the approximate rate of 1 drop every 10 s; reserve the filtrate for further tests. Record