



Designation: F 2183 – 02

# Standard Test Method for Small Punch Testing of Ultra-High Molecular Weight Polyethylene Used in Surgical Implants<sup>1</sup>

This standard is issued under the fixed designation F 2183; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon ( $\epsilon$ ) indicates an editorial change since the last revision or reapproval.

## 1. Scope

1.1 This test method covers the determination of mechanical behavior of ultra-high molecular weight polyethylene (UHMWPE) by small punch testing of miniature disk specimens (0.5 mm in thickness and 6.4 mm in diameter). The test method has been established for characterizing UHMWPE surgical materials after ram extrusion or compression molding (1,2)<sup>2</sup>; for evaluating as-manufactured implants after radiation crosslinking and sterilization (3,4); as well as for testing of implants that have been retrieved (explanted) from the human body (5,6).

1.2 The parameters of the small punch test, namely the peak load, ultimate displacement, ultimate load, and work to failure, provide metrics of the yielding, ultimate strength, ductility, and toughness of UHMWPE under multiaxial loading conditions. Because the mechanical behavior of UHMWPE is different when loaded under uniaxial and multiaxial loading conditions (3), the small punch test provides a complementary mechanical testing technique to the uniaxial tensile testing specified for medical grade UHMWPE by Specification F 648.

1.3 In addition to its use as a research tool in implant retrieval analysis, the small punch test can be used as a laboratory screening test to evaluate new UHMWPE materials, such as those created by gamma or electron beam irradiation (1). The test method is also well suited for characterization of UHMWPE before and after accelerated aging (for example, Guide F 2003), and in that regard it can provide ranking of the mechanical degradation of different UHMWPE samples after oxidative degradation (4,7).

1.4 The small punch test has been applied to other polymers, including polymethyl methacrylate (PMMA) bone cement, polyacetal, and high density polyethylene (HDPE) (8,9). However, the small punch testing of polymers other than UHMWPE is beyond the scope of this standard.

1.5 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appro-*

*priate safety and health practices and determine the applicability of regulatory limitations prior to use.*

## 2. Referenced Documents

### 2.1 ASTM Standards:

- D 695 Method for Compressive Properties of Rigid Plastics<sup>3</sup>
- D 883 Terminology Relating to Plastics<sup>3</sup>
- E 4 Practices for Force Verification of Testing Machines<sup>4</sup>
- E 83 Practice for Verification and Classification of Extensometers<sup>4</sup>
- F 648 Specification of Ultra-High Molecular Weight Polyethylene Powder and Fabricated Forms for Surgical Implants<sup>5</sup>
- F 1714 Guide for Gravimetric Wear Assessment of Prosthetic Hip Designs in Simulator Devices<sup>5</sup>
- F 1715 Guide for Wear Assessment of Prosthetic Knee Designs in Simulator Devices<sup>5</sup>
- F 2003 Guide for Accelerated Aging of Ultra-High Molecular Weight Polyethylene<sup>5</sup>
- F 2102 Guide for Evaluating the Extent of Oxidation in Ultra-High-Molecular-Weight Polyethylene Fabricated Forms Intended for Surgical Implants<sup>5</sup>

## 3. Terminology

3.1 *Definitions*—The features of a typical small punch test load versus displacement curve for UHMWPE are illustrated in Fig. 1.

3.1.1 *peak load*—an initial local maximum in the load versus displacement curve (Fig. 1). In certain radiation crosslinked UHMWPE materials, the load versus displacement curve increases monotonically and a shoulder, rather than an initial peak load, may be observed.

3.1.2 *small punch test*—a test wherein the specimen is of miniature size relative to conventional mechanical test specimens, is disk-shaped, and is loaded axisymmetrically in bending by a hemispherical-head punch.

3.1.3 *ultimate displacement*—the displacement at rupture (failure) of the specimen (Fig. 1).

<sup>1</sup> This test method is under the jurisdiction of ASTM Committee F04 on Medical and Surgical Materials and Devices and is the direct responsibility of Subcommittee F04.15 on Materials Test Methods.

Current edition approved April 10, 2002. Published June 2002.

<sup>2</sup> The boldface numbers in parentheses refer to the list of references at the end of this standard.

<sup>3</sup> *Annual Book of ASTM Standards*, Vol 08.01.

<sup>4</sup> *Annual Book of ASTM Standards*, Vol 03.01.

<sup>5</sup> *Annual Book of ASTM Standards*, Vol 13.01.

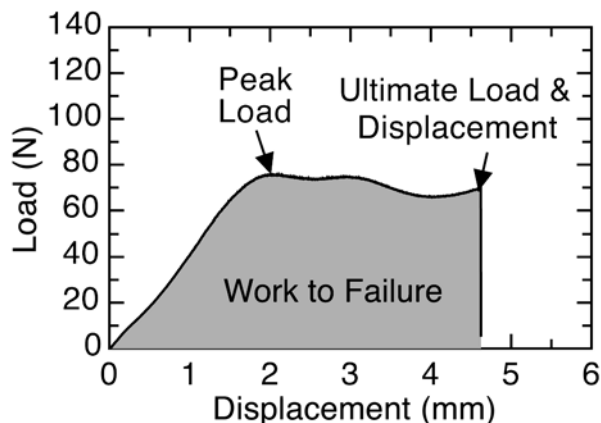


FIG. 1 Features of the Small Punch Test Load Versus Displacement Curve for Unirradiated UHMWPE, Including the Peak Load, Ultimate Load and Displacement, and Work to Failure

3.1.4 *ultimate load*—the load at rupture (failure) of the specimen (Fig. 1).

3.1.5 *work to failure*—the area under the load versus displacement curve (Fig. 1).

#### 4. Significance and Use

4.1 Miniature specimen testing techniques are used to characterize the mechanical behavior of UHMWPE stock materials and surgical implants after manufacture, sterilization, shelf aging, radiation crosslinking, thermal treatment, and implantation (1). Furthermore, experimental UHMWPE materials can be evaluated after accelerated aging and hip or knee wear simulation. Consequently, the small punch test makes it possible to examine relationships between wear performance and mechanical behavior of UHMWPE. This test method can also be used to rank the mechanical behavior of UHMWPE relative to a reference control material (such as the NIST Ultra-High Molecular Weight Polyethylene Reference Material #8456).

4.2 Small punch testing results may vary with specimen preparation and with the speed and environment of testing. Consequently, where precise comparative results are desired, these factors must be carefully controlled.

#### 5. Apparatus

5.1 *Small Punch Test Apparatus*<sup>6</sup>—A system consisting of a hemispherical head punch, a die, and a guide for the punch, as shown in Fig. 2. The parts shall be fabricated from a hardened steel.

5.1.1 *Guide*—The function of the guide is to align the punch relative to the specimen, which rests in a disk-shaped recess. The inner diameter of the guide bore shall be  $0.1010 + 0.0002/-0.0000$  in. ( $2.565 + 0.005/-0.000$  mm), and the specimen recess shall be  $0.0200 + 0.0004/-0.0000$  in. ( $0.508 + 0.010/-0.000$  mm) in depth and  $0.2520 \pm 0.0005$  in. ( $6.401 \pm 0.013$  mm) in diameter.

<sup>6</sup> Small punch testers suitable for use and meeting the requirements of this test method are available from Exponent, Inc., 2300 Chestnut St., Suite 150, Philadelphia, PA, 19103.

5.1.2 *Die*—The function of the die is to constrain the sample during testing. The inner diameter of the die bore shall be  $0.1500 \pm 0.0005$  in. ( $3.810 \pm 0.013$  mm).

5.1.3 *Punch*—The hemispherical head punch shall have a diameter of 0.1000 in. (2.540 mm), with a tolerance of  $+0.0000/-0.0002$  in. ( $+0.000/-0.005$  mm).

5.2 *Testing Machine*—Any suitable testing machine as described in Method D 695, consisting of a drive mechanism and a load indicator. The load indicator shall have a full range of 250 N (56.2 lbs). The accuracy of the machine shall be verified at least once per year, as specified by Method D 695 and Practice E 4.

5.3 *Compressometer*—This instrument, described in Section 5.2 from Method D 695, can be used to determine the distance between the die and the punch during the test. If the actuator displacement of the testing machine can be shown to determine punch displacement within 1 % of the value measured by a suitably calibrated compressometer (as defined in Practice E 83), actuator displacement shall be used as reference.

5.4 *Compression Platen*—The punch shall rest on a compression platen or tool for applying the load to the punch.

5.5 *Micrometers*—Suitable micrometers, reading to 0.0001 in. (0.0025 mm), shall be used to record the diameter and thickness of the specimens.

5.6 *Thermometer*—A suitable thermometer or thermocouple, reading to 0.1°C, shall be used to record the test temperature within the range 20 to 24°C.

#### 6. Test Specimens

6.1 As the test results are known to be sensitive to preparation technique, the specimens described in 6.2 and 6.3 shall be used. The specimens may be prepared by machining operations from materials in sheet, rod, plate, or implant form. All machining operations shall be done carefully so that smooth surfaces result. Great care shall be taken in machining the faces so that smooth, parallel surfaces result.

NOTE 1—Although specimen fabrication methods other than machining (for example, microtoming) may be used, the use of alternate specimen