

# INTERNATIONAL STANDARD

**ISO  
9832**

First edition  
1992-12-15

---

---

## **Animal and vegetable fats and oils — Determination of residual technical hexane content**

**iTeh STANDARD PREVIEW**

*Corps gras d'origines animale et végétale — Dosage de l'hexane  
technique résiduel*

ISO 9832:1992

<https://standards.iteh.ai/catalog/standards/sist/691ab039-d04b-42ed-8436-325ace0c4394/iso-9832-1992>



Reference number  
ISO 9832:1992(E)

## Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

International Standard ISO 9832 was prepared by Technical Committee ISO/TC 34, *Agricultural food products*, Sub-Committee SC 11, *Animal and vegetable fats and oils*.

[ISO 9832:1992](https://standards.iteh.ai/catalog/standards/sist/691ab039-d04b-42ed-8436-325ace0c4394/iso-9832-1992)

<https://standards.iteh.ai/catalog/standards/sist/691ab039-d04b-42ed-8436-325ace0c4394/iso-9832-1992>

© ISO 1992

All rights reserved. No part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from the publisher.

International Organization for Standardization

Case Postale 56 • CH-1211 Genève 20 • Switzerland

Printed in Switzerland

# Animal and vegetable fats and oils — Determination of residual technical hexane content

## 1 Scope

This International Standard specifies a method for the determination of the residual technical hexane content of animal and vegetable fats and oils (referred to as fats hereinafter).

The method is suitable for the determination of hexane contents between 10 mg and 1 500 mg per kilogram of fat.

The method is not applicable to marine oils.

## 2 Normative reference

The following standard contains provisions which, through reference in this text, constitute provisions of this International Standard. At the time of publication, the edition indicated was valid. All standards are subject to revision, and parties to agreements based on this International Standard are encouraged to investigate the possibility of applying the most recent edition of the standard indicated below. Members of IEC and ISO maintain registers of currently valid International Standards.

ISO 661:1989, *Animal and vegetable fats and oils — Preparation of test sample.*

## 3 Definition

For the purposes of this International Standard, the following definition applies.

**3.1 residual technical hexane content:** Content of volatile hydrocarbons such as those remaining in fats following processing involving the use of hydrocarbon solvents, when determined by the method specified in this International Standard.

The content is expressed as milligrams of hexane per kilogram of sample.

## 4 Principle

Desorption of volatile hydrocarbons by heating at 80 °C in a closed vessel after addition of an internal standard. Determination of the particular volatile hydrocarbons content of the headspace by gas chromatography using packed or capillary columns.

## 5 Reagents

All reagents shall be of recognized analytical grade unless otherwise stated.

**5.1 Technical hexane,** with a composition similar to that of hexane used in industrial processing, or, if this is not available, *n*-hexane.

NOTE 1 It is recommended that technical hexane be used for the calibration. This reagent usually has an *n*-hexane content of 50 % (*m/m*) and consists mainly of C<sub>6</sub> isomers but may include C<sub>5</sub> and C<sub>7</sub> hydrocarbons.

**5.2 Internal standard,** *n*-heptane.

If this is not available, cyclohexane may be used, provided that the solvent (5.1) used for the extraction or calibration has a negligible content of cyclohexane and/or *n*-heptane or components with similar retention times.

**5.3 Carrier gas,** e.g. hydrogen, nitrogen or helium, etc., thoroughly dried and with an oxygen content of less than 10 mg/kg.

**5.4 Auxiliary gases,** hydrogen (99,9 % pure, free from organic impurities) and air (free from organic impurities).

**5.5 Calibration fat,** freshly refined and deodorized vegetable fat, the technical hexane content of which is negligible.

NOTE 2 This material should be free from peroxides or other components likely to decompose with the formation

of volatile material which could be confused with hydrocarbons during the test.

## 6 Apparatus

Usual laboratory equipment and, in particular, the following.

**6.1 Septum vials**, of 20 ml capacity.

**6.2 Septa**, inert to fats and solvents, made of a material such as butyl rubber or red rubber free from hydrocarbon solvent residues, and of a suitable quality that they will not swell under the conditions of use, **aluminium caps** suitable for use with the vials (6.1) and **crimping pliers**.

**6.3 Tongs**, suitable for holding the vials (6.1).

**6.4 Syringes**, of 10 µl capacity, used only for the analysis of residual technical hexane. They shall not be cleaned with hydrocarbon solvent.

**6.5 Syringes**, of 1 µl capacity, used only for the analysis of residual technical hexane. They shall not be cleaned with hydrocarbon solvent.

**6.6 Syringes**, of 1 000 µl capacity, gas-tight, used only for the analysis of residual technical hexane. They shall not be cleaned with hydrocarbon solvent.

**6.7 Gas chromatograph**, with a flame ionization detector and an integrator and/or recorder, equipped with either

- a) a packed glass column, 2 m to 4 m long and of internal diameter 3,2 mm approximately, packed with an acid-washed and silanized diatomaceous earth support of particle size 150 µm to 180 µm (Chromosorb P NAW 60-80 mesh<sup>1)</sup> is suitable), and coated with 10 % squalane or any other phase permitting the chromatographic separation required, or
- b) a glass capillary column, approximately 30 m long and of 0,3 mm internal diameter, coated with methylpolysiloxane of film thickness 0,2 µm.

The injector and detector temperature shall be set at 100 °C and the oven temperature at 50 °C.

If a capillary column [see b)] is used, the apparatus shall have a 1/100 split injection system.

NOTE 3 For analyses in series, a headspace gas chromatograph with automatic sample injection and tem-

pering bath has been shown to be satisfactory. In this case, manual injection is not necessary.

**6.8 Heating bath**, equipped with clamps for holding septum vials, regulated thermostatically at 80 °C ± 2 °C.

NOTE 4 For continuous operation, glycerol is recommended as the heating medium.

**6.9 Shaking machine**

## 7 Sampling

It is important that the laboratory receive a sample which is truly representative and has not been damaged or changed during transport and storage.

Sampling is not part of the method specified in this International Standard. A recommended sampling method is given in ISO 5555.<sup>2)</sup>

It is essential that the sample be protected from gain or loss of solvent residues.

## 8 Preparation of test sample

Prepare the test sample in accordance with ISO 661, taking care to prevent gain or loss of solvent.

## 9 Procedure

### 9.1 Calibration

**9.1.1** Weigh, to the nearest 0,01 g, 5 g of calibration fat (5.5) into each of seven vials (6.1). Close each vial with a septum and a cap (6.2).

To six of the seven vials (6.1) add, using a syringe (6.4 or 6.5), the quantity of solvent (5.1) specified in table 1 to obtain the concentrations indicated. Do not add solvent to the seventh vial.

Shake vigorously, in the shaking machine (6.9) for 1 h at room temperature, the six vials to which solvent was added.

**9.1.2** At the end of this time add, by means of a syringe (6.4), 5 µl ± 0,1 µl of internal standard (5.2) to each of the seven vials through the septum.

NOTE 5 For hexane contents between 10 mg/kg and 20 mg/kg, it is preferable to add 2 µl of internal standard (5.2).

1) Chromosorb P NAW 60-80 is an example of a suitable product available commercially. This information is given for the convenience of users of this International Standard and does not constitute an endorsement by ISO of this product.

2) ISO 5555:1991, *Animal and vegetable fats and oils — Sampling*.

Table 1 — Hexane content in the calibration samples

Volume of solvent (5.1) added μl	Hexane content (mg/kg) when using	
	technical hexane	<i>n</i> -hexane
0,5	67	66
1	134	132
2	268	264
4	536	528
7	938	924
10	1 340	1 320

Mix the contents vigorously by hand for about 1 min by moving the vial with a circular motion in a horizontal plane in such a way that the fat does not touch the septum. If this happens, reject the vial and start again with a further portion of calibration fat.

NOTE 6 If there is fat on the septum it will contaminate the needle when the headspace gas is sampled and the contaminant may be transferred to the column; it is particularly important that such contamination be avoided when using capillary columns.

At intervals of about 15 min (i.e. the retention time of the internal standard), place one vial at a time up to its neck in the heating bath (6.8) set at 80 °C to allow equilibrium between the fat and the gaseous phase to be reached.

**9.1.3** From each vial which has been in the heating bath for 60 min ± 1 min, take (without removing it from the bath) 1 000 μl of the gaseous phase by means of a syringe (6.6) warmed to 60 °C. Immediately inject into the gas chromatograph the gaseous phase so removed.

**9.1.4** From the chromatogram corresponding to the vial to which no solvent was added, calculate the hexane content  $A_c$ , expressed as a percentage of the total peak areas.

**9.1.5** From each of the chromatograms corresponding to each of the vials to which solvent was added, calculate the calibration factor  $F$  using the formula

$$F = \frac{w_h \times A_{is}}{(A_t - A_c - A_{is}) \times w_{is}}$$

where

$A_c$  is the hexane content calculated in 9.1.4;

$A_{is}$  is the content of the internal standard in the calibration fat (5.5) with added solvent,

expressed as a percentage of the total peak areas;

$A_t$  is the total hydrocarbons content, including the internal standard, in the calibration fat (5.5) with added solvent, expressed as a percentage of the total peak areas;

$w_h$  is the content of the solvent (5.1) in the calibration fat (5.5) with added solvent, expressed in milligrams per kilogram;

$w_{is}$  is the content of the internal standard in the calibration fat (5.5) with added solvent, expressed in milligrams per kilogram, i.e. 680 for *n*-heptane or 780 for cyclohexane.

NOTE 7 If only 2 μl of internal standard was added in 9.1.2,  $w_{is}$  is equal to 272 for *n*-heptane or 312 for cyclohexane.

Express the result to the third decimal place.

The calibration factors of the six calibration samples should be approximately equal. Calculate the arithmetic mean value  $\bar{F}$ , which should be about 0,45 for heptane. The factor  $\bar{F}$  so evaluated can be used for determining hexane contents of less than 60 mg/kg. If the value of  $F$  found for the vial containing 0,5 μl of solvent (5.1) is significantly below the mean value  $\bar{F}$ , this deviation is probably due to the difficulty of introducing exactly 0,5 μl and this determination shall be eliminated or repeated.

The mean calibration factor for cyclohexane is normally about 0,57, whilst it is about 0,45 for *n*-heptane.

## 9.2 Determination

**9.2.1** Weigh, to the nearest 0,01 g, a test portion of 5 g of the test sample (clause 8) into a vial (6.1) as quickly as possible. Close immediately with a septum and a cap (6.2).

**9.2.2** Inject 5 µl of the internal standard (5.2) through the septum by means of a syringe (6.4). Mix the contents vigorously by hand for about 1 min by moving the vial with a circular motion in a horizontal plane in such a way that the fat does not touch the septum. If this happens, reject the vial and start again with a further test portion. (See note 6 in 9.1.2). Place the vial up to its neck in the heating bath (6.8) set at 80 °C for 60 min ± 1 min.

**9.2.3** Then take 1 000 µl from the gaseous phase by means of a syringe (6.6) warmed to 60 °C, without removing the vial from the heating bath. Immediately inject into the gas chromatograph the gaseous phase so removed.

**9.2.4** Determine the residual technical hexane content of the sample from the chromatogram (see the example given in figure 1), measuring those peaks identified as being from hexane and not from decomposition products.

**9.3 Number of determinations**

Carry out the determination on two test portions from the same test sample in rapid succession.

**10 Expression of results**


The residual technical hexane content of the sample, *w*, in milligrams per kilogram, is given by the formula

$$w = \frac{(A'_t - A'_{is}) \times \bar{F} \times w'_{is}}{A'_{is}}$$

where

- A'\_{is}* is the content of the internal standard in the sample, expressed as a percentage of the total peak areas;
- A'\_t* is the total hydrocarbons content, including the internal standard, of the sample, expressed as a percentage of the total peak areas;
- $\bar{F}$  is the mean calibration factor determined in 9.1.5;
- w'\_{is}* is the content of the internal standard in the sample, expressed in milligrams per kilogram, i.e. 680 for *n*-heptane or 780 for cyclohexane.

Take as the final result the arithmetic mean of the two determinations (9.3) provided that the repeatability requirement (11.2) is met. If the repeatability requirement is not met, disregard the results and carry out two new determinations on test portions taken from the same test sample.

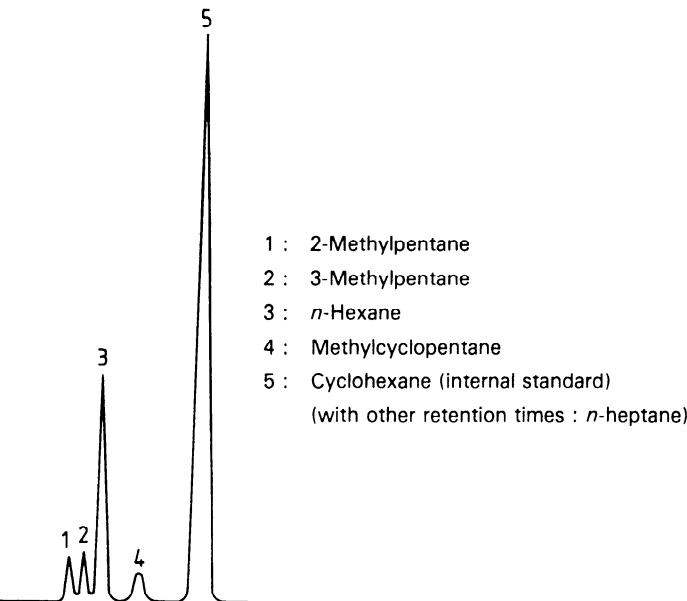

**Figure 1 — Example of a gas chromatogram of hexane hydrocarbons**

## 11 Precision

### 11.1 Results of inter-laboratory test

An inter-laboratory test, carried out at the international level in 1985 by the International Union of Analytical Chemistry (IUPAC), in which each laboratory carried out duplicate determinations, gave the statistical results (evaluated in accordance with ISO 5725<sup>3)</sup> shown in table 2.

### 11.2 Repeatability

When the values of two independent single test results, obtained using the same method on identical test material in the same laboratory by the same operator using the same equipment within a short interval of time, lie within the range of the mean values cited in table 2, the absolute difference between the two test results obtained should not be greater than the repeatability limit  $r$  reduced by linear interpolation from the data given in table 2.

NOTE 8 It should be noted that the reproducibility values  $R$  cited in table 2 apply in the particular case when the results of single determinations obtained by two laboratories are being compared. When following the method described and it is desired to compare the final results (which have

been derived from the means of duplicate determinations) obtained by two laboratories, the values for  $R$  should be converted to the 95 % probability critical difference values,  $CrD_{95}$ , applicable to the means of two determinations using the following formula:

$$CrD_{95} = \sqrt{(R^2 - r^2)/2}$$

## 12 Test report

The test report shall specify

- the method in accordance with which sampling was carried out (if known),
- the method used,
- the test result(s) obtained, and
- if the repeatability has been checked, the final quoted result obtained.

It shall also mention all operating details not specified in this International Standard, or regarded as optional, together with details of any incidents which may have influenced the results.

The test report shall include all information necessary for the complete identification of the sample.

Table 2 — Statistical results of the inter-laboratory test

Sample <sup>1)</sup>	1	2	3	4
Number of laboratories	16	16	11	11
Number of laboratories retained after elimination of outliers	16	16	9	10
Mean residual technical hexane content (mg/kg)	2,95	13,7	104	1 048
Repeatability standard deviation, $s_r$ (mg/kg)	0,65	1,70	7,6	71,5
Coefficient of variation of repeatability (%)	22,4	12,2	7,3	6,8
Repeatability, $r = 2,83 s_r$ (mg/kg)	1,8	4,8	21	202
Reproducibility standard deviation, $s_R$ (mg/kg)	2,6	4,1	28,4	293
Coefficient of variation of reproducibility (%)	89	30	27	28
Reproducibility, $R = 2,83 s_R$ (mg/kg)	7,4	12	80	829

NOTE — The data given for sample 1 are included despite being outside the scope of this International Standard.

- 1) Sample 1: Fresh edible peanut oil + 3,3 ppm technical hexane  
 Sample 2: Fresh peanut oil after storage + 13,2 ppm technical hexane  
 Sample 3: Crude rapeseed oil (pressed) + 100 ppm technical hexane  
 Sample 4: Crude rapeseed oil (pressed) + 1 000 ppm technical hexane

3) ISO 5725:1986, *Precision of test methods — Determination of repeatability and reproducibility for a standard test method by inter-laboratory tests.*

**iTeh STANDARD PREVIEW**  
**(standards.iteh.ai)**

ISO 9832:1992

<https://standards.iteh.ai/catalog/standards/sist/691ab039-d04b-42ed-8436-325ace0c4394/iso-9832-1992>

---

---

**UDC 665.2/.3:543.544:547.216**

**Descriptors:** agricultural products, food products, animal fats, vegetable fats, animal oils, vegetable oils, determination of content, hexane, chromatographic analysis.

Price based on 5 pages

---

---