

INTERNATIONAL
STANDARD

ISO
12644

First edition
1996-12-01

**Graphic technology — Determination of
rheological properties of paste inks and
vehicles by the falling rod viscometer**

iTeh STANDARD PREVIEW

(standards.iteh.ai)

*Technologie graphique — Détermination des caractéristiques rhéologiques
des encres et excipients projetés, à l'aide d'un viscosimètre à tige
tombante*

[ISO 12644:1996](#)

<https://standards.iteh.ai/catalog/standards/sist/b79957d1-fcd4-4c2b-83f8-1ffc4a56cb77/iso-12644-1996>



Reference number
ISO 12644:1996(E)

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

International Standard ISO 12644 was prepared by Technical Committee ISO/TC 130, *Graphic technology*.

Annex A forms an integral part of this International Standard.

iTeh STANDARD PREVIEW
(standards.iteh.ai)
<https://standards.iteh.ai/catalog/standards/sist/b79957d1-fcd4-4c2b-83f8-1ffc4a56cb77/iso-12644-1996>

Graphic technology — Determination of rheological properties of paste inks and vehicles by the falling rod viscometer

1 Scope

This International Standard specifies the procedure for determining the viscosity and yield value of paste inks and vehicles which are unreactive under normal room conditions.

It is applicable to inks in the apparent viscosity range of 2 Pa · s to 200 Pa · s.

iTeh STANDARD PREVIEW
(standards.iteh.ai)

2 Definitions

For the purposes of this International Standard, the following definitions apply.

2.1 viscosity: Measure of the internal friction of a liquid in motion. The viscosity is generally defined as the ratio of the shear stress (2.2) to the shear rate (2.3).

$$\eta = \frac{\sigma}{\dot{\gamma}} \quad \dots (1)$$

2.2 shear stress, σ : Force per area in a direction parallel to the applied force. Unit: Pa.

NOTES

1 For the falling rod viscometer, the shear stress is proportional to the total weight of the rod and the weight loads in accordance with the equation

$$\sigma = \frac{W}{A} = \frac{mg}{2\pi rl} \quad \dots (2)$$

where (see figures 1 and 2)

- σ is the shear stress;
- W is the total weight of the rod and the weight loads;
- A is the apparent shearing area;
- g is the gravitational acceleration;
- m is the total mass;
- r is the radius of the rod;
- l is the length of the aperture.

2 The shearing length of the aperture of a falling rod viscometer usually contains both a tapered and a parallel section; therefore, it is understood that A is not the true shearing area but an apparent shearing area.

2.3 shear rate, γ : Velocity gradient through a stressed liquid in a direction perpendicular to the shearing area. Unit: s^{-1} .

NOTE — For the falling rod viscometer, γ is inversely proportional to all fall time according to the equation

$$\gamma = \frac{L}{r \cdot \ln(R/r) \cdot t} \quad \dots (3)$$

where

- γ is the shear rate;
- L is the falling distance of the rod;
- r is the radius of the rod;
- R is the radius of the aperture;
- t is the fall time.

If the ratio of the radii of the rod and aperture is close to unity, the term may be simplified to

$$\gamma = \frac{L}{st} \quad \dots (4)$$

where s is the thickness of the ink in the nip determined by the difference between radii of the aperture and of the rod.

2.4 apparent viscosity, η_a : Ratio of the shear stress σ to the shear rate γ for a given shear stress or shear rate. Unit: $Pa \cdot s$.

2.5 Newtonian liquid: Liquid whose shear stress is proportional to shear rate.

2.6 non-Newtonian liquid: Liquid whose shear stress is not proportional to shear rate.

NOTES

- 1 There are two types of non-Newtonian liquids: With shear thickening liquids, the viscosity increases with shear rate; with shear thinning liquids, the viscosity decreases with shear rate.
- 2 If the viscosity of a liquid decreases with application of steady mechanical stress from a value at the state of rest to a final value and increases again if the stress ceases, the liquid is called thixotropic.

2.7 flow curve: Graph of the shear stress σ as a function of the shear rate γ or vice versa.

2.8 Casson model (see A.1): Flow model which assumes a non-linear increase of shear stress σ with increasing shear rate γ . A minimum stress σ_0 is required to initiate flow.

2.9 Bingham model (see A.2): Flow model which assumes a linear increase of the shear stress σ with increasing shear rate γ . A minimum stress σ_0 is required to initiate flow.

2.10 Power Law model (see A.3): Flow model which assumes an increase of the shear stress σ of a liquid proportional to the N th power of the shear rate γ .

2.11 yield stress, σ_0 : Minimum stress required to initiate flow of a liquid. Unit: 1 Pa.

2.12 pseudo yield stress, σ_y : Shear stress at a defined low shear rate when applying the Power Law model, typically to $2,5 s^{-1}$.

2.13 reference temperature: Temperature (25 °C) for which all results are reported. Unit: °C.

NOTE — Measurements made at temperatures different from this temperature are corrected (see 6.2.2).

2.14 test temperature: Actual temperature of the aperture ring during measurements. Unit: °C.

2.15 shortness ratio: Ratio of yield stress or pseudo yield stress to the apparent viscosity. Unit: 1 s⁻¹.

3 Test method

3.1 Principle

The principle of this test is the measurement of the relative velocity between a vertical rod and an aperture ring. The bottom of the rod is inserted into the aperture. The gap is filled with the test fluid, which is sheared when the rod falls.

By loading the rod with different load weights, different shear rates are obtained. By applying linear regression methods to the measured fall times as a function of load weight, the viscosity and the yield stress can be calculated.

3.2 Apparatus

iTeh STANDARD PREVIEW
(standards.iteh.ai)

3.2.1 Falling rod viscometer


The viscometer consists of

- a cylindrical rod (figure 1) made from metal or any other hard material. In order to obtain comparable values for shear stress and resulting shear rate the mass of the steel rod should be (132 ± 1) g.
- a metal ring (figure 2) with a defined cylindrical or conical aperture. The ring is fixed on a support and should be temperature controlled. Since the diameter of rod and aperture are critical they are manufactured within low tolerances. These dimensions shall be supplied by the manufacturer. To minimize possible gap differences, only matching sets of rod and aperture ring shall be used.
- load weights to be loaded on top of the rod. Series of load weights are combined to sets. Sets of load weights with the following masses should be used:

A:	5 000,	4 000,	3 000,	2 000,	1 000
B:	3 000,	2 000,	1 500,	500	
C:	1 500,	1 000,	800,	500	
D:	800,	600,	400,	200	
E:	400,	300,	200,	100	
F:	200,	100,	50,	0	

The tolerance for the masses of load weights shall be ± 0,2 g;

- a designated measuring distance marked on the strut. The tolerance shall be ± 0,2 mm. Sensors may be placed at the marks.
- a levelling device.
- a timing device. The tolerance shall be ± 0,1 s (should be ± 0,01 s).

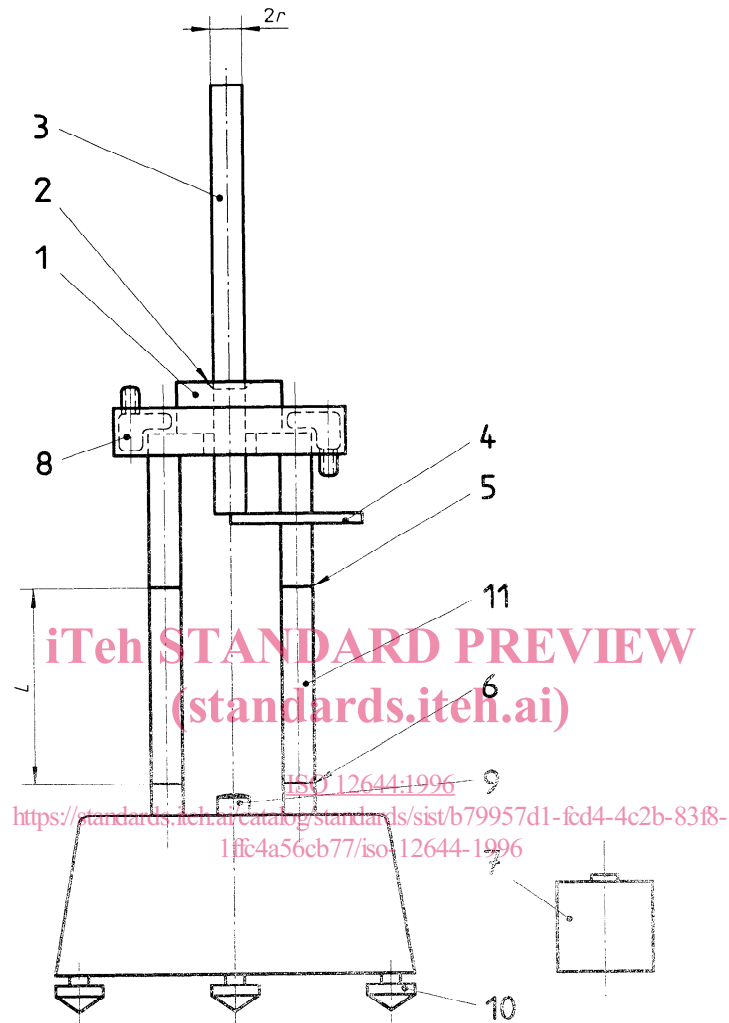

Key

- | | | | |
|---|--------------------------------|-----|------------------------------|
| 1 | Ring | 9 | Level |
| 2 | Aperture | 10 | Horizontally adjusting screw |
| 3 | Rod | 11 | Strut |
| 4 | Support | r | Radius of the rod |
| 5 | Measuring distance, upper mark | R | Radius of the aperture |
| 6 | Measuring distance, lower mark | l | Length of the aperture |
| 7 | Weight | L | Measuring distance |
| 8 | Water jacket | | |

Figure 1 — Falling rod viscometer

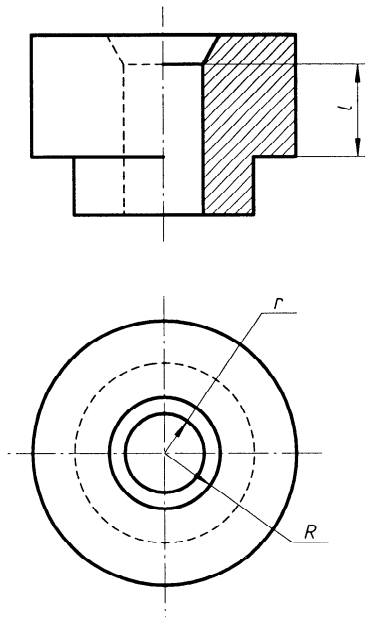


Figure 2 — Aperture ring

3.2.2 Temperature control

Means shall be provided for measurement and control of the test temperature.

3.2.3 Others

Non-scratching spatulas. <https://standards.iteh.ai/catalog/standards/sist/b79957d1-fcd4-4c2b-83f8-1ffc4a56cb77/iso-12644-1996>
 Standard viscosity oils (at least 2) for calibration.

NOTE — The viscosity of the standard viscosity oils shall be in the same range as that of the test samples. The viscosity of these oils shall be traceable to a standards institution. An internal standard may be used for comparative studies only.

3.3 Ambient temperature control

The test shall be carried out under controlled ambient temperature. This can be achieved either by placing the viscometer in a thermostatically controlled cabinet or by working under constant room temperature.

If working in a cabinet, the inner temperature should not vary from the test temperature by more than $\pm 0,5$ °C. For room conditioning, a difference of ± 2 °C to the test temperature is allowed. The standard reference temperature shall be $(25 \pm 0,2)$ °C.

3.4 Preparation for testing

Prior to use, the test sample (about 5 g) shall be kneaded by a spatula and equilibrated to test temperature. The sample shall be homogeneous and not contain any coarse particles.

The proper set of load weights is selected according to the expected results.

NOTE — The fall time with the highest load weight should normally be in the range 4 s to 10 s. For heat-set printing inks it may be desirable to use a shorter fall time for the highest weight.

An amount of the test sample sufficient to coat the rod and aperture is applied to the lower part of the rod. By turning the rod, the sample is distributed uniformly. Running a single pass with the highest weight load, the rod and the aperture ring are wetted by the liquid. The rod is inserted into the aperture and rests on the support before the test run is started.

3.5 Test procedure

The sample is tested with the selected series of load weights in descending order. The fall time shall not exceed 60 s. After each run, the rod is scraped with the spatula and the liquid which was scraped off is reapplied on the lower part of the rod. During the test, additional liquid shall not be added.

At the beginning and at the end of the test, the temperature of the sample is checked.

For highly thixotropic samples, it may be necessary to make a dummy run first.

3.6 Cleaning

After the test, the instrument shall be cleaned immediately with a lint-free wiper and a suitable solvent.

4 Calibration

When installing the viscometer, locate the instrument on a sturdy bench in a draught-free environment. Use the levelling device to obtain proper vertical alignment. The timing device and the distance between the two sensors are calibrated during initial installation. The timing device should be recalibrated regularly.

The calibration shall be performed by testing the standard viscosity oils according to the procedure described in 3.5.

4.1 Calibration for the Casson and Bingham models (see A.1 and A.2)

Assuming that the standard viscosity oils are strictly Newtonian, the calculation is as follows:

From (1), (2) and (4) follows:

$$\eta = \frac{\sigma}{\gamma} = \frac{mg}{2\pi rl} \times \frac{st}{L} \quad \dots (5)$$

where

- η is the viscosity;
- σ is the shear stress;
- γ is the shear rate;
- m is the mass;
- g is the gravitational acceleration;
- r is the radius of the rod;
- l is the length of the aperture;
- s is the thickness of the ink in the nip;
- t is the fall time;
- L is the measuring distance.

Fixed parameters and constants are combined as device factors α and β

$$\alpha = \frac{L}{s} \quad \dots (6)$$

and

$$\beta = \frac{g}{2\pi r l} \quad \dots (7)$$

The unit of α is 1 and the unit of β is Pa/kg.

Since the shear rate

$$\gamma = \frac{\alpha}{t} \quad \dots (8)$$

and shear stress

$$\sigma = \beta m \quad \dots (9)$$

the viscosity of a Newtonian fluid can be calculated from the slope of a plot of γ versus σ for different masses. The measured viscosity is the reciprocal slope of the linear regression line.

If a certain set of rod and aperture ring shows viscosity variations of > 20 % from the specifications of the standard viscosity oil it shall be discarded. Smaller differences are compensated by using a correction factor Φ :

$$\Phi = \eta_{\text{true}} / \eta_{\text{measured}} \quad \dots (10)$$

The correction factor Φ is specific for a single set of rod and aperture. It is recommended that a calibrated set of aperture and rod be kept as an internal standard. [ISO 12644:1996](https://standards.iteh.ai/catalog/standards/sist/b79957d1-fcd4-4c2b-83f8-1ffc4a56cb77/iso-12644-1996)

<https://standards.iteh.ai/catalog/standards/sist/b79957d1-fcd4-4c2b-83f8-1ffc4a56cb77/iso-12644-1996>

4.2 Calibration for the Power Law model

For determination of the device factor β (stress constant) defined in equation (7) it is necessary to measure the radius r of the rod and the length l of the aperture. Both dimensions shall be measured to 0,01 mm. Given these data the device factor β is calculated according to equation (7).

The value of the device factor α defined in equation (6) shall be computed from fall time runs of the standard viscosity oils. For that purpose, measurements shall be taken with at least two such oils, covering the viscosity range of interest, and at least four fall times. The known viscosity of the oils is divided by the fall time t for each weight load with the mass m and this quotient is plotted versus the mass for each standard viscosity oil. According to equation (11), the slope of the regression line is the quotient β/α of the two device factors.

$$\frac{\eta_{\text{std}}}{t} = \frac{\beta}{\alpha} m \quad \dots (11)$$

where

η_{std} is the viscosity of the standard viscosity oil;

t is the fall time;

m is the mass of the weight load.

Having calculated β from the geometric dimensions of rod and aperture according to the above method, α can easily be calculated. With the device factors α and β determined, values for the shear rate γ and shear stress σ can be calculated from the fall time t and the mass m used as shown in equations (8) and (9).