
Kava - Ugotavljanje vsebnosti kofeina - Metoda z uporabo tekočinske kromatografije

Coffee -- Determination of caffeine content -- Method using high-performance liquid chromatography

iTeh STANDARD PREVIEW

Café -- Détermination de la teneur en caféine -- Méthode par chromatographie liquide à haute performance

Ta slovenski standard je istoveten z: ISO 10095:1992

ICS:

67.140.20 Kava in kavni nadomestki Coffee and coffee substitutes

SIST ISO 10095:1995**en**

iTeh STANDARD PREVIEW
(standards.iteh.ai)

SIST ISO 10095:1995

<https://standards.iteh.ai/catalog/standards/sist/4b61fd48-b086-4183-a332-ff207fb393f5/sist-iso-10095-1995>

INTERNATIONAL STANDARD

ISO
10095

First edition
1992-01-15

Coffee — Determination of caffeine content — Method using high-performance liquid chromatography

iTeh STANDARD PREVIEW

(standards.iteh.ai)

*Café — Détermination de la teneur en caféine — Méthode par
chromatographie liquide à haute performance*

SIST ISO 10095:1995

[https://standards.iteh.ai/catalog/standards/sist/4b61fd48-b086-4183-a332-
ff207fb393f5/sist-iso-10095-1995](https://standards.iteh.ai/catalog/standards/sist/4b61fd48-b086-4183-a332-ff207fb393f5/sist-iso-10095-1995)



Reference number
ISO 10095:1992(E)

ISO 10095:1992(E)**Foreword**

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

International Standard ISO 10095 was prepared by Technical Committee ISO/TC 34, *Agricultural food products*, Sub-Committee SC 15, *Coffee*.

Annex A of this International Standard is for information only.

© ISO 1992

All rights reserved. No part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from the publisher.

International Organization for Standardization
Case Postale 56 • CH-1211 Genève 20 • Switzerland

Printed in Switzerland

Coffee — Determination of caffeine content — Method using high-performance liquid chromatography

1 Scope

This International Standard specifies a method for the determination of caffeine content by high-performance liquid chromatography (HPLC) of regular and decaffeinated green and roasted coffee beans and of regular and decaffeinated coffee extract powder.

NOTE 1 The reference method for determination of the caffeine content, using ultraviolet absorption spectrometry, is given in ISO 4052:1983, *Coffee — Determination of caffeine content (Reference method)*.

2 Normative references

The following standards contain provisions which, through reference in this text, constitute provisions of this International Standard. At the time of publication, the editions indicated were valid. All standards are subject to revision, and parties to agreements based on this International Standard are encouraged to investigate the possibility of applying the most recent editions of the standards indicated below. Members of IEC and ISO maintain registers of currently valid International Standards.

ISO 1447:1978, *Green coffee — Determination of moisture content (Routine method)*.

ISO 3726:1983, *Instant coffee — Determination of loss in mass at 70 °C under reduced pressure*.

ISO 6673:1983, *Green coffee — Determination of loss in mass at 105 °C*.

3 Principle

Extraction of the caffeine from a test portion with water at 90 °C in the presence of magnesium oxide. Filtration and then purification of an aliquot portion

on a silica microcolumn modified with phenyl groups.

Determination of the caffeine content by HPLC with ultraviolet detection.

4 Reagents

Use only reagents of recognized analytical grade, unless otherwise specified, and distilled or demineralized water or water of equivalent purity.

4.1 **Methanol**, HPLC grade.

4.2 **Ammonia solution** (0,3 mol/l)/**methanol**, 90 + 10 mixture by volume.

4.3 **Elution solvent**, for purification column, methanol/water/acetic acid, 75 + 25 + 1 mixture by volume.

4.4 **Mobile phase**, methanol/water, 30 + 70 mixture by volume.

Put 600 ml of methanol (4.1) into a 2 l one-mark volumetric flask and make up to the mark with water. Mix and then filter the mixture through a filter of 0,45 µm pore size (5.7).

NOTE 2 By adjusting the methanol concentration, the retention time of caffeine can be modified so as to optimize the HPLC separation.

4.5 **Ethanol/water**, 1 + 4 solution by volume.

4.6 **Magnesium oxide**¹⁾.

4.7 **Caffeine, stock solution**, corresponding to 0,5 g of caffeine per litre.

Weigh, to the nearest 0,1 mg, 125 mg of caffeine into

1) Merck 5867 is an example of a suitable product available commercially. This information is given for the convenience of users of this International Standard and does not constitute an endorsement by ISO of this product.

ISO 10095:1992(E)

a 250 ml volumetric flask made of amber glass. Add sufficient ethanol/water (4.5) to half-fill the flask. Dissolve the caffeine and then make up to the mark with the same ethanol/water mixture.

This solution can be stored for 1 month in a refrigerator.

4.8 Caffeine, standard solutions.

4.8.1 standard solution A, corresponding to 0,010 g of caffeine per litre, to be used for the decaffeinated product.

Allow the stock solution (4.7) to warm up to room temperature. Using a pipette (5.12), transfer 2 ml of this solution to a 100 ml one-mark volumetric flask. Make up to the mark with water and mix.

Prepare this solution on the day of use.

4.8.2 Standard solution B, corresponding to 0,05 g of caffeine per litre, to be used for regular products.

Allow the stock solution (4.7) to warm up to room temperature. Using a pipette (5.12), transfer 5 ml of this solution to a 50 ml one-mark volumetric flask. Make up to the mark with water and mix.

5 Apparatus

Usual laboratory apparatus and, in particular, the following.

5.1 High-performance liquid chromatograph, equipped with an ultraviolet detector, allowing measurements to be made at between 254 nm and 280 nm, and a chart recorder. A wavelength close to 280 nm is preferred since the maximum absorption by caffeine is at 272 nm.

5.2 Chromatographic column for HPLC, type C₁₈, preferably with spherical particles and having an efficiency of at least 5 000 theoretical plates.²⁾

The theoretical plate number N of a column can be calculated as follows, from the shape of the peak obtained by injection of the pure caffeine standard solution (4.8):

2) Spherisorb 5 ODS, Spherisorb 10 ODS, Nucleosil 5 C₁₈, Nucleosil 7 C₁₈, Nucleosil 10 C₁₈, Zorbax BP C₁₈, Hypersil ODS, CP-Spher C₁₈, Bondapak C₁₈, Supelcosil L C₁₈ and Partisphere C₁₈ are examples of suitable products available commercially. This information is given for the convenience of users of this International Standard and does not constitute an endorsement by ISO of these products.

In this International Standard, the chromatographic conditions and the composition of the mobile phase (4.4) specified are suitable for a Partisphere C₁₈ Cartridge column of dimensions 110 mm x 4,6 mm, filled in a Whatman HPLC Cartridge system. If other types of column are used, an alternative mobile phase and chromatographic conditions may be necessary.

3) The 3 ml Baker SPE column, modified with phenyl groups in reversed phase, is an example of a suitable product available commercially. This information is given for the convenience of users of this International Standard and does not constitute an endorsement by ISO of this product.

$$N = 5,54 \left(\frac{t}{w_{0,5}} \right)^2$$

where

t is the retention time of the peak;

$w_{0,5}$ is the peak width at half-height.

5.3 Purification column, for reversed-phase chromatography, of 3 ml capacity, filled with silica modified with phenyl groups, the particles of which have an average size of 40 µm.³⁾

5.4 Coffee mill, suitable for milling roasted coffee beans.

5.5 Grinder with clogged wheel, with a cooling jacket, or **analytical grinder**, with blades and a cooling jacket, or any other grinder suitable for grinding green coffee beans.

5.6 Sieve, of woven wire cloth, with an aperture size of 630 µm.

5.7 Filters, of 0,45 µm pore size.

5.8 Water-bath, capable of operating at 90 °C ± 1 °C with continuous stirring.

5.9 Analytical balance, capable of weighing to the nearest 0,000 1 g

5.10 Bottle, of 250 ml capacity, fitted with a screw cap.

5.11 One-mark volumetric flasks, of 10 ml, 50 ml, 100 ml, 250 ml and 2 l capacity.

5.12 Pipettes, of 2,0 ml, 5,0 ml and 10,0 ml capacity.

6 Sampling

Sampling of green coffee in bags should have been carried out in accordance with ISO 4072.

Sampling of instant coffee in cases with liners should have been carried out in accordance with ISO 6670.

7 Preparation of the test sample

If necessary, grind the sample using the apparatus specified in 5.4 or 5.5, as appropriate, until it passes through the sieve (5.6).

8 Procedure

8.1 Determination of dry matter content

Calculate the dry matter content from the moisture content determined on a portion of the test sample (clause 7) in accordance with

- ISO 1447 or ISO 6673 for green coffee,
- ISO 3726 for instant coffee, or
- a corresponding future International Standard for other types of coffee and coffee-derived products.

8.2 Test portion

8.2.1 Regular and decaffeinated green or roasted coffee

Weigh, to the nearest 0,000 1 g, 1 g of the test sample (clause 7).

8.2.2 Regular and decaffeinated coffee extract powder

Weigh, to the nearest 0,000 1 g, 0,5 g of the test sample (clause 7).

8.3 Extraction of caffeine

8.3.1 Put the test portion (8.2.1 or 8.2.2) into the 250 ml bottle (5.10). Add $4 \text{ g} \pm 0,5 \text{ g}$ of magnesium oxide (4.6) and 100 g of water. Weigh the flask and its contents to the nearest 0,1 g.

8.3.2 Stopper the bottle and mix the contents. Place the bottle plus contents in a water-bath (5.8) and heat to 90 °C, under continuous stirring, for 20 min.

Cool the bottle plus contents and weigh again to the nearest 0,1 g. The mass of the cooled bottle plus contents shall be equal to the mass determined in 8.3.1.

8.3.3 If the masses differ, carry out another extraction (8.3.1 and 8.3.2) using another test portion.

8.3.4 Leave the solution to stand. Remove a portion of the solution and filter it through the filter (5.7).

8.4 Purification of the solution

Before any separation of the solution occurs, activate the purification column (5.3).

8.4.1 Preparation of the purification column

Set up the purification column as shown in figure 1.

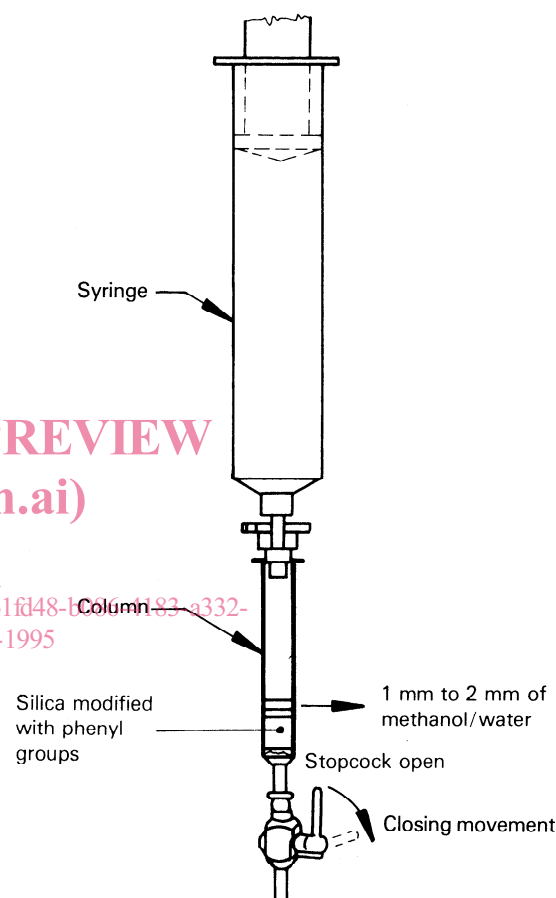


Figure 1 — Preparation of the purification column

Open the stopcock and rinse the column with 5 ml of the methanol (4.1), adjusting the stopcock to achieve a dropwise flow. When 1 mm to 2 mm of the methanol remains above the surface of the silica, close the stopcock. Add 5 ml of water, open the stopcock and close it again when 1 mm to 2 mm of water remains above the silica surface.

Do not allow the column to dry out, otherwise the preparation shall be repeated.

8.4.2 Absorption of caffeine

Using a pipette, introduce into the column either

ISO 10095:1992(E)

- a) 2,0 ml of the filtered solution obtained in 8.3.3 in the case of regular coffee or coffee extract, or
- b) 10,0 ml of the filtered solution obtained in 8.3.4 in the case of decaffeinated coffee or decaffeinated coffee extract.

Adjust the stopcock to allow the solution to flow dropwise. Close the stopcock when the surface of the solution falls just below the surface of the silica.

8.4.3 Removal of unwanted compounds

Open the stopcock and add 2,5 ml of the ammonia solution/methanol mixture (4.2). Close the stopcock when the surface of this mixture falls just below the surface of the silica. Add a further 2,5 ml of the mixture (4.2) and allow it to flow completely through the column. Blow about 20 ml of air through the column in order to remove as much as possible of the mixture (4.2).

NOTE 3 The column may become dry at this stage of the procedure.

8.4.4 Elution of caffeine

Place a 10 ml one-mark volumetric flask (5.11) under the column. Open the stopcock and add 7,5 ml of the elution solvent (4.3), adjusting the stopcock to achieve a dropwise flow. Allow the elution solvent to flow completely into the volumetric flask. Make up to the mark with water and mix the contents.

NOTE 4 The purification column can be regenerated with methanol as indicated in 8.4.1. It may be used at most ten times for purification purposes.

8.5 HPLC analysis

8.5.1 Adjustment of the apparatus

Set up the chromatograph (5.1) and adjust it as follows:

- flow-rate of the mobile phase (4.4): 0,5 ml/min to 1,5 ml/min, depending on the column used (see 5.2)
- temperature of the column (5.2): 40 °C

NOTE 5 The peak separation can also be improved by raising the temperature of the column, but this should not exceed 60 °C.

8.5.2 Analysis

Once the flow-rate of the mobile phase (4.4) and the temperature are stable, inject into the column 10 µl of the test solution obtained in 8.4.4 and then an

equal volume of the standard caffeine solution (4.8.1 or 4.8.2).

NOTE 6 In normal procedures Beer's law is obeyed for caffeine concentrations up to 0,025 0 g/l. This level is higher than the caffeine concentrations used in this test method. If, however, this should not be the case due to instrumentation deviations, a calibration curve for the extinction—caffeine concentration should be made.

9 Expression of results

The caffeine content of the sample, expressed in grams per 100 g of the dry matter content, is as follows.

9.1 For regular roasted or green coffee and instant coffee powder:

$$\frac{A_x}{A_c} \times c_1 \times \frac{10 \times 100}{2 \times m_0 \times 1\,000} \times \frac{100}{RS} \times 100$$

where

A_x is the area of the caffeine peak obtained with the test solution;

A_c is the area of the caffeine peak obtained with the standard caffeine solution;

c_1 is the concentration of the standard caffeine solution (4.8.2), in grams per litre;

m_0 is the mass of the test portion, in grams;

RS is the dry matter content, as a percentage by mass, of the sample (see 8.1).

9.2 For decaffeinated roasted or green coffee and decaffeinated coffee powder:

$$\frac{A_x}{A_c} \times c_2 \times \frac{10 \times 100}{10 \times m_0 \times 1\,000} \times \frac{100}{RS} \times 100$$

where

c_2 is the concentration of the standard caffeine solution (4.8.1), in grams per litre.

10 Precision

10.1 Results of inter-laboratory test

An inter-laboratory test was carried out at the international level in 1987 by ISO/TC 34/SC 15, *Coffee*, in which 18 laboratories participated. The repeatability and reproducibility values shown in table 1 were obtained. The sample plan and procedures followed in this inter-laboratory plan were in accordance with the split-level design as outlined in ISO 5725.

Table 1 — Repeatability and reproducibility values

Sample	Caffeine content g/100 g of coffee	Repeatability g caffeine/100 g of coffee	Reproducibility g caffeine/100 g of coffee
Roasted coffee beans	≈ 2	0,07	0,34
	≈ 1	0,04	0,12
Decaffeinated roasted coffee beans	$< 0,1$	0,01	0,02
Instant coffee	≈ 4	0,09	0,36
Decaffeinated instant coffee	$< 0,3$	0,02	0,03

10.2 Repeatability

The absolute difference between two single test results, obtained using the same method on identical test material in the same laboratory by the same operator using the same equipment within a short interval of time, should not exceed the value given in table 1.

10.3 Reproducibility

The absolute difference between two single test results, obtained using the same method on identical test material in different laboratories with different

operators using different equipment, should not exceed the value given in table 1.

11 Test report

The test report shall specify the method used and the results obtained. It shall also mention all operating details not specified in this International Standard, or regarded as optional, together with details of any incidents which may have influenced the results.

The test report shall include all information necessary for the complete identification of the sample.

<https://standards.iteh.ai/catalog/standards/sist/4b61fd48-b086-4183-a332-f207fb393f5/sist-iso-10095-1995>