

# INTERNATIONAL STANDARD

## NORME INTERNATIONALE

**Superconductivity –**  
**Part 11: Residual resistance ratio measurement – Residual resistance ratio of**  
**Nb<sub>3</sub>Sn composite superconductors**

**Supraconductivité –**  
**Partie 11: Mesure du rapport de résistance résiduelle – Rapport de résistance**  
**résiduelle des supraconducteurs composites de Nb<sub>3</sub>Sn**



## THIS PUBLICATION IS COPYRIGHT PROTECTED

Copyright © 2011 IEC, Geneva, Switzerland

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either IEC or IEC's member National Committee in the country of the requester.

If you have any questions about IEC copyright or have an enquiry about obtaining additional rights to this publication, please contact the address below or your local IEC member National Committee for further information.

Droits de reproduction réservés. Sauf indication contraire, aucune partie de cette publication ne peut être reproduite ni utilisée sous quelque forme que ce soit et par aucun procédé, électronique ou mécanique, y compris la photocopie et les microfilms, sans l'accord écrit de la CEI ou du Comité national de la CEI du pays du demandeur.

Si vous avez des questions sur le copyright de la CEI ou si vous désirez obtenir des droits supplémentaires sur cette publication, utilisez les coordonnées ci-après ou contactez le Comité national de la CEI de votre pays de résidence.

IEC Central Office  
3, rue de Varembe  
CH-1211 Geneva 20  
Switzerland  
Email: [inmail@iec.ch](mailto:inmail@iec.ch)  
Web: [www.iec.ch](http://www.iec.ch)

### About the IEC

The International Electrotechnical Commission (IEC) is the leading global organization that prepares and publishes International Standards for all electrical, electronic and related technologies.

### About IEC publications

The technical content of IEC publications is kept under constant review by the IEC. Please make sure that you have the latest edition, a corrigenda or an amendment might have been published.

- Catalogue of IEC publications: [www.iec.ch/searchpub](http://www.iec.ch/searchpub)

The IEC on-line Catalogue enables you to search by a variety of criteria (reference number, text, technical committee,...). It also gives information on projects, withdrawn and replaced publications.

- IEC Just Published: [www.iec.ch/online\\_news/justpub](http://www.iec.ch/online_news/justpub)

Stay up to date on all new IEC publications. Just Published details twice a month all new publications released. Available on-line and also by email.

- Electropedia: [www.electropedia.org](http://www.electropedia.org)

The world's leading online dictionary of electronic and electrical terms containing more than 20 000 terms and definitions in English and French, with equivalent terms in additional languages. Also known as the International Electrotechnical Vocabulary online.

- Customer Service Centre: [www.iec.ch/webstore/custserv](http://www.iec.ch/webstore/custserv)

If you wish to give us your feedback on this publication or need further assistance, please visit the Customer Service Centre FAQ or contact us:

Email: [csc@iec.ch](mailto:csc@iec.ch)  
Tel.: +41 22 919 02 11  
Fax: +41 22 919 03 00

### A propos de la CEI

La Commission Electrotechnique internationale (CEI) est la première organisation mondiale qui élabore et publie des normes internationales pour tout ce qui a trait à l'électricité, à l'électronique et aux technologies apparentées.

### A propos des publications CEI

Le contenu technique des publications de la CEI est constamment revu. Veuillez vous assurer que vous possédez l'édition la plus récente, un corrigendum ou amendement peut avoir été publié.

- Catalogue des publications de la CEI: [www.iec.ch/searchpub/cur\\_fut-f.htm](http://www.iec.ch/searchpub/cur_fut-f.htm)

Le Catalogue en-ligne de la CEI vous permet d'effectuer des recherches en utilisant différents critères (numéro de référence, texte, comité d'études,...). Il donne aussi des informations sur les projets et les publications retirées ou remplacées.

- Just Published CEI: [www.iec.ch/online\\_news/justpub](http://www.iec.ch/online_news/justpub)

Restez informé sur les nouvelles publications de la CEI. Just Published détaille deux fois par mois les nouvelles publications parues. Disponible en-ligne et aussi par email.

- Electropedia: [www.electropedia.org](http://www.electropedia.org)

Le premier dictionnaire en ligne au monde de termes électroniques et électriques. Il contient plus de 20 000 termes et définitions en anglais et en français, ainsi que les termes équivalents dans les langues additionnelles. Egalement appelé Vocabulaire Electrotechnique International en ligne.

- Service Clients: [www.iec.ch/webstore/custserv/custserv\\_entry-f.htm](http://www.iec.ch/webstore/custserv/custserv_entry-f.htm)

Si vous désirez nous donner des commentaires sur cette publication ou si vous avez des questions, visitez le FAQ du Service clients ou contactez-nous:

Email: [csc@iec.ch](mailto:csc@iec.ch)  
Tél.: +41 22 919 02 11  
Fax: +41 22 919 03 00

# INTERNATIONAL STANDARD

## NORME INTERNATIONALE

**Superconductivity –**  
**Part 11: Residual resistance ratio measurement – Residual resistance ratio of**  
**Nb<sub>3</sub>Sn composite superconductors**

**Supraconductivité –**  
**Partie 11: Mesure du rapport de résistance résiduelle – Rapport de résistance**  
**résiduelle des supraconducteurs composites de Nb<sub>3</sub>Sn**

INTERNATIONAL  
ELECTROTECHNICAL  
COMMISSION

COMMISSION  
ELECTROTECHNIQUE  
INTERNATIONALE

PRICE CODE  
CODE PRIX

S

## CONTENTS

FOREWORD.....	3
INTRODUCTION.....	5
1 Scope.....	6
2 Normative references.....	6
3 Terms and definitions.....	6
4 Requirements.....	7
5 Apparatus.....	7
5.1 Material of measuring base plate.....	7
5.2 Length of the measuring base plate.....	7
5.3 Cryostat for the resistance, $R_2$ , measurement.....	7
6 Specimen preparation.....	8
7 Data acquisition and analysis.....	8
7.1 Resistance ( $R_1$ ) at room temperature.....	8
7.2 Resistance ( $R_2$ ) just above the superconducting transition.....	8
7.3 Residual resistance ratio ( $RRR$ ).....	10
8 Uncertainty and stability of the test method.....	11
8.1 Temperature.....	11
8.2 Voltage measurement.....	11
8.3 Current.....	11
8.4 Dimension.....	11
9 Test report.....	11
9.1 $RRR$ value.....	11
9.2 Specimen.....	11
9.3 Test conditions.....	12
Annex A (informative) Additional information relating to the measurement of $RRR$ .....	13
Annex B (informative) Uncertainty considerations.....	15
Annex C (informative) Uncertainty evaluation in test method of $RRR$ for $Nb_3Sn$ .....	19
Figure 1 – Relationship between temperature and resistance.....	7
Figure 2 – Voltage ( $U$ ) versus temperature ( $T$ ) curves and definitions of each voltage.....	9
Table B.1 – Output signals from two nominally identical extensometers.....	16
Table B.2 – Mean values of two output signals.....	16
Table B.3 – Experimental standard deviations of two output signals.....	16
Table B.4 – Standard uncertainties of two output signals.....	17
Table B.5 – Coefficient of variations of two output signals.....	17
Table C.1 – Uncertainty of each measurement.....	20
Table C.2 – Obtained values of $R_1$ , $R_2$ and $RRR$ for three $Nb_3Sn$ samples.....	21

## INTERNATIONAL ELECTROTECHNICAL COMMISSION

## SUPERCONDUCTIVITY –

**Part 11: Residual resistance ratio measurement –  
Residual resistance ratio of Nb<sub>3</sub>Sn composite superconductors**

## FOREWORD

- 1) The International Electrotechnical Commission (IEC) is a worldwide organization for standardization comprising all national electrotechnical committees (IEC National Committees). The object of IEC is to promote international co-operation on all questions concerning standardization in the electrical and electronic fields. To this end and in addition to other activities, IEC publishes International Standards, Technical Specifications, Technical Reports, Publicly Available Specifications (PAS) and Guides (hereafter referred to as "IEC Publication(s)"). Their preparation is entrusted to technical committees; any IEC National Committee interested in the subject dealt with may participate in this preparatory work. International, governmental and non-governmental organizations liaising with the IEC also participate in this preparation. IEC collaborates closely with the International Organization for Standardization (ISO) in accordance with conditions determined by agreement between the two organizations.
- 2) The formal decisions or agreements of IEC on technical matters express, as nearly as possible, an international consensus of opinion on the relevant subjects since each technical committee has representation from all interested IEC National Committees.
- 3) IEC Publications have the form of recommendations for international use and are accepted by IEC National Committees in that sense. While all reasonable efforts are made to ensure that the technical content of IEC Publications is accurate, IEC cannot be held responsible for the way in which they are used or for any misinterpretation by any end user.
- 4) In order to promote international uniformity, IEC National Committees undertake to apply IEC Publications transparently to the maximum extent possible in their national and regional publications. Any divergence between any IEC Publication and the corresponding national or regional publication shall be clearly indicated in the latter.
- 5) IEC itself does not provide any attestation of conformity. Independent certification bodies provide conformity assessment services and, in some areas, access to IEC marks of conformity. IEC is not responsible for any services carried out by independent certification bodies.
- 6) All users should ensure that they have the latest edition of this publication.
- 7) No liability shall attach to IEC or its directors, employees, servants or agents including individual experts and members of its technical committees and IEC National Committees for any personal injury, property damage or other damage of any nature whatsoever, whether direct or indirect, or for costs (including legal fees) and expenses arising out of the publication, use of, or reliance upon, this IEC Publication or any other IEC Publications.
- 8) Attention is drawn to the Normative references cited in this publication. Use of the referenced publications is indispensable for the correct application of this publication.
- 9) Attention is drawn to the possibility that some of the elements of this IEC Publication may be the subject of patent rights. IEC shall not be held responsible for identifying any or all such patent rights.

International Standard IEC 61788-11 has been prepared by IEC Technical Committee 90: Superconductivity.

This second edition cancels and replaces the first edition published in 2003. It constitutes a technical revision. The main revisions are the addition of two new annexes, "Uncertainty considerations" (Annex B) and "Uncertainty evaluation in test method of RRR for Nb<sub>3</sub>Sn" (Annex C).

The text of this standard is based on the following documents:

FDIS	Report on voting
90/268/FDIS	90/279/RVD

Full information on the voting for the approval of this standard can be found in the report on voting indicated in the above table.

This publication has been drafted in accordance with the ISO/IEC Directives, Part 2.

A list of all parts of the IEC 61788 series, published under the general title Superconductivity, can be found on the IEC website.

The committee has decided that the contents of this publication will remain unchanged until the stability date indicated on the IEC web site under "<http://webstore.iec.ch>" in the data related to the specific publication. At this date, the publication will be

- reconfirmed,
- withdrawn,
- replaced by a revised edition, or
- amended.

iTeh STANDARD PREVIEW  
(standards.iteh.ai)

[IEC 61788-11:2011](https://standards.iteh.ai/standards/iec-61788-11-2011)

<https://standards.iteh.ai/standards/iec-61788-11-2011>

Withdrawing

## INTRODUCTION

Copper or aluminium is used as stabilizer material in multifilamentary Nb<sub>3</sub>Sn superconductors and works as an electrical shunt when the superconductivity is interrupted. It also contributes to recovery of the superconductivity by conducting the heat generated in the superconductor to the surrounding coolant. The resistivity of copper used in the composite superconductor in the cryogenic temperature region is an important quantity which influences the stability of the superconductor. The residual resistance ratio is defined as a ratio of the resistance of the superconductor at room temperature to that just above the superconducting transition.

In this International Standard, the test method for the residual resistance ratio of Nb<sub>3</sub>Sn composite superconductors is described. The curve method is employed for the measurement of the resistance just above the superconducting transition. Other methods are described in Clause A.3.

iTeh STANDARD PREVIEW  
(standards.iteh.ai)

IEC 61788-11:2011

<https://standards.iteh.ai/catalog/standards/sist/56449c47-b055-4750-bc3e-b8a06549c30d/iec-61788-11-2011>

Withstand

## SUPERCONDUCTIVITY –

### Part 11: Residual resistance ratio measurement – Residual resistance ratio of Nb<sub>3</sub>Sn composite superconductors

#### 1 Scope

This part of IEC 61788 covers a test method for the determination of the residual resistance ratio (*RRR*) of Nb<sub>3</sub>Sn composite superconductors. This method is intended for use with superconductor specimens that have a monolithic structure with rectangular or round cross-section, *RRR* less than 350 and cross-sectional area less than 3 mm<sup>2</sup>, and have received a reaction heat-treatment. Ideally, it is intended that the specimens be as straight as possible; however, this is not always the case, thus care must be taken to measure the specimen in its as received condition. All measurements are done without an applied magnetic field.

The method described in the body of this standard is the “reference” method and optional acquisition methods are outlined in Clause A.3.

#### 2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

IEC 60050-815, *International Electrotechnical Vocabulary – Part 815: Superconductivity*

<https://standards.iteh.ai/standards/iec/60050-815/iec-60050-815-2011>

#### 3 Terms and definitions

For the purposes of this document, the terms and definitions given in IEC 60050-815 and the following apply.

##### 3.1

##### **residual resistance ratio** ***RRR***


the ratio of resistance at room temperature to the resistance just above the superconducting transition

NOTE In this standard for Nb<sub>3</sub>Sn composite superconductors, the room temperature is defined as 293 K (20 °C), and the residual resistance ratio is obtained in Equation (1) below, where the resistance (*R*<sub>1</sub>) at 293 K is divided by the resistance (*R*<sub>2</sub>) just above the superconducting transition.

$$RRR = \frac{R_1}{R_2} \quad (1)$$

Figure 1 shows schematically a resistance versus temperature curve acquired on a specimen while measuring cryogenic resistance. Draw a line in Figure 1 where the resistance sharply increases (a), and draw also a line in Figure 1 where the resistance increases gradually (b) with temperature. The value of resistance at the intersection of these two lines at  $T=T_c^*$ , A, is defined as resistance (*R*<sub>2</sub>) just above the superconducting transition.



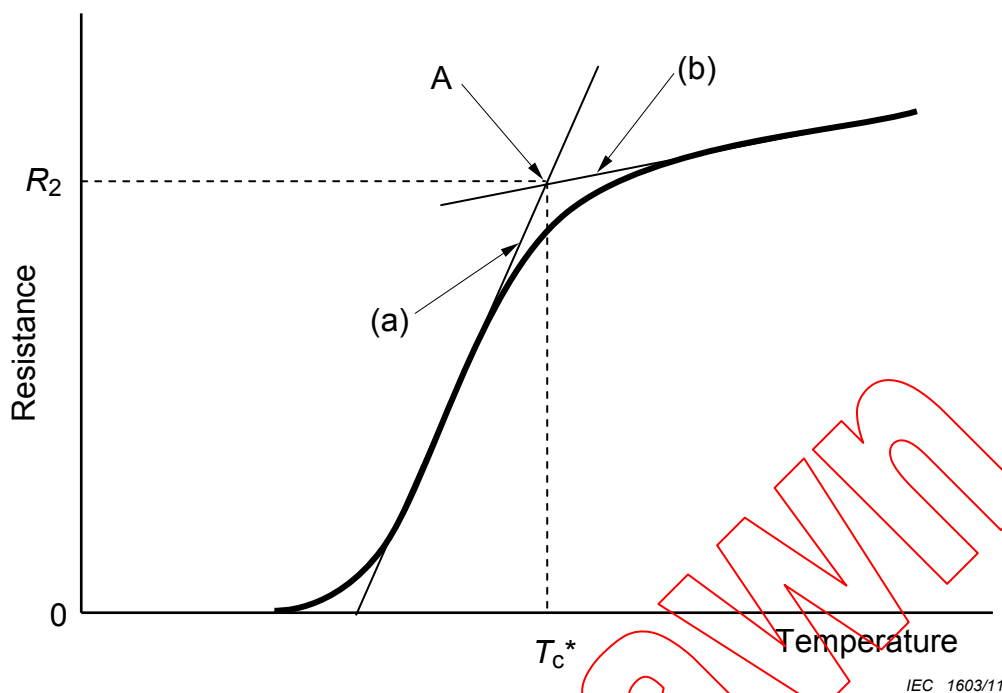

Temperature  $T_c^*$  is that at the intersection point.

**Figure 1 – Relationship between temperature and resistance**

## 4 Requirements

The resistance measurement both at room and cryogenic temperatures shall be performed with the four-terminal technique.

The target relative combined standard uncertainty of this method is defined as an expanded uncertainty ( $k = 2$ ) not to exceed 10 % based on the coefficient of variation (COV) of 5 % in the intercomparison test (see Clause C.2).

## 5 Apparatus

### 5.1 Material of measuring base plate

Material of the measuring base plate shall be copper, aluminum, silver or the like whose thermal conductivity is equal to or better than 100 W/(m·K) at liquid helium temperature (4,2 K). The surface of the material shall be covered with an insulating layer (tape or a layer made of polyethylene terephthalate, polyester, polytetrafluoroethylene, etc.) whose thickness is 0,1 mm or less.

### 5.2 Length of the measuring base plate

The measuring base plate shall be at least 30 mm long in one dimension.

### 5.3 Cryostat for the resistance, $R_2$ , measurement

The cryostat shall include a specimen support structure and a liquid helium reservoir for the resistance,  $R_2$ , measurement. The specimen support structure shall allow the specimen, which is mounted on a measurement base plate, to be lowered and raised into and out of a liquid helium bath. In addition, the specimen support structure shall be made so that a current

can flow through the specimen and the resulting voltage generated along the specimen can be measured.

## 6 Specimen preparation

The test specimen shall have no joints or splices, and shall be 30 mm or longer. The distance between two voltage taps ( $L$ ) shall be 25 mm or longer. A thermometer for measuring cryogenic temperature shall be attached near the specimen.

Some mechanical method shall be used to hold the specimen against the insulated layer of the measurement base plate. Special care shall be taken during instrumentation and installation of the specimen on the measurement base plate so that no excessive force, which may cause undesired bending strain or tensile strain, shall be applied to the specimen.

The specimen shall be instrumented with current contacts near each end of the specimen and a pair of voltage contacts over a central portion of the specimen. The specimen shall be mounted on a measurement base plate for these measurements. Both resistance measurements,  $R_1$  and  $R_2$ , shall be made on the same specimen and the same mounting.

## 7 Data acquisition and analysis

### 7.1 Resistance ( $R_1$ ) at room temperature

The mounted specimen shall be measured at room temperature ( $T_m$  (K)), where  $T_m$  satisfies the following condition  $273 \leq T_m \leq 308$ . A specimen current ( $I_1$  (A)) shall be applied so that the current density is in the range of 0,1 A/mm<sup>2</sup> to 1 A/mm<sup>2</sup> based on the total wire cross-sectional area, and the resulting voltage ( $U_1$  (V)),  $I_1$  and  $T_m$  shall be recorded.

Equation (2) below shall be used to calculate the resistance ( $R_m$ ) at room temperature. The resistance ( $R_1$ ) at 293 K shall be calculated using equation (3) for a wire with Cu stabilizer. The value of  $R_1$  shall be set equal to  $R_m$ , without any temperature correction, for wires that do not contain a pure Cu component.

$$R_m = \frac{U_1}{I_1} \quad (2)$$

$$R_1 = \frac{R_m}{[1 + 0,00393 \cdot (T_m - 293)]} \quad (3)$$


### 7.2 Resistance ( $R_2$ ) just above the superconducting transition

**7.2.1** The specimen, which is still mounted as it was for the room temperature measurement, shall be placed in the cryostat for electrical measurement specified under 5.3. Alternate cryostats that employ a heating element to sweep the specimen temperature are described in Clause A.2.

**7.2.2** The specimen shall be slowly lowered into the liquid helium bath and cooled to liquid helium temperature over a time period of at least 5 min.

**7.2.3** During the acquisition phases of the low-temperature  $R_2$  measurements, a specimen current ( $I_2$ ) shall be applied so that the current density is in the range of 0,1 A/mm<sup>2</sup> to 10 A/mm<sup>2</sup> based on the total wire cross-sectional area and the resulting voltage ( $U$ (V)),  $I_2$ (A), and specimen temperature ( $T$  (K)) shall be recorded. In order to keep the ratio of signal to noise high enough, the measurement shall be carried out under the condition that the

absolute value of resulting voltage above the superconducting transition exceeds  $10 \mu\text{V}$ . An illustration of the data to be acquired and its analysis is shown in Figure 2.

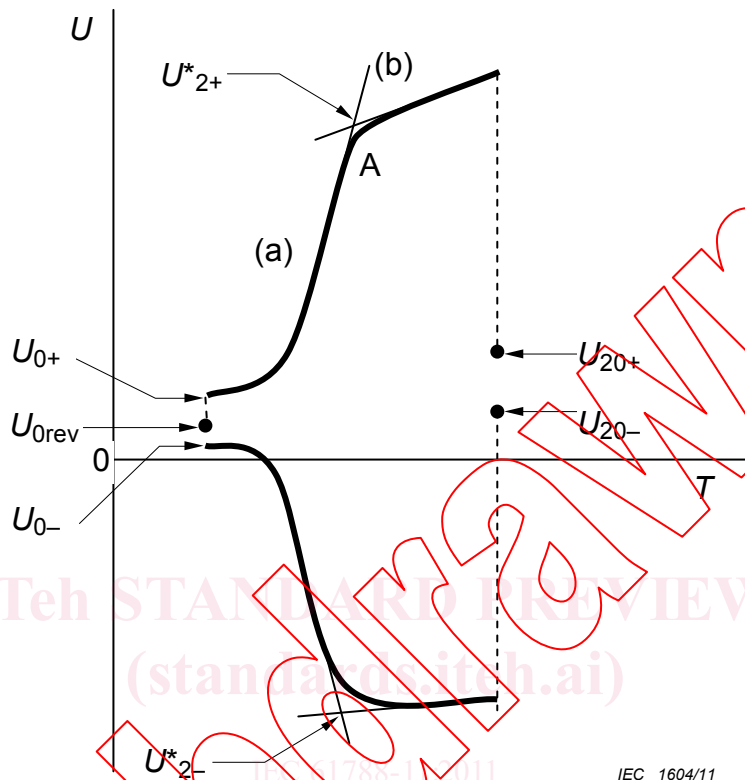

**Figure 2 – Voltage ( $U$ ) versus temperature ( $T$ ) curves and definitions of each voltage**

Voltages with subscripts + and - are those obtained in the first and second measurements under positive and negative currents, respectively, and  $U_{20+}$  and  $U_{20-}$  are those obtained at zero current. For clarity,  $U_{0rev}$  is not shown coincident with  $U_{0-}$ . Voltages  $U_{2+}^*$  and  $U_{2-}^*$  with asterisk are those at the intersection points.

**7.2.4** When the specimen is in superconducting state and test current ( $I_2$ ) is applied, two voltages shall be measured nearly simultaneously:  $U_{0+}$  (the initial voltage recorded with a positive current polarity) and  $U_{0rev}$  (the voltage recorded during a brief change in applied current polarity). A valid  $R_2$  measurement requires that excessive interfering voltages are not present and that the specimen is initially in the superconducting state. Thus, the following condition shall be met for a valid measurement:

$$\frac{|U_{0+} - U_{0rev}|}{\bar{U}_2} < 1\% \quad (4)$$

where  $\bar{U}_2$  is the average voltage for the specimen in the normal state at cryogenic temperature, which is defined in 7.2.10.

**7.2.5** The specimen shall be gradually warmed so that it changes to the normal state completely. When the cryostat for the resistance measurement specified under 5.3 is used, this can be achieved simply by raising the specimen to an appropriate position above the liquid helium level.

**7.2.6** The specimen voltage versus temperature curve shall be acquired with the rate of temperature increase maintained between 0,1 K/min and 10 K/min.

**7.2.7** The voltage versus temperature curve shall continue to be recorded during the transition into the normal state, up to a temperature somewhat less than 25 K. Then, the specimen current shall be decreased to zero and the corresponding voltage,  $U_{20+}$ , shall be recorded at a temperature below 25 K.

**7.2.8** The specimen shall then be slowly lowered into the liquid helium bath and cooled to the same temperature, within  $\pm 1$  K, where the initial voltage signal  $U_{0+}$  was recorded. A specimen current,  $I_2$ , with the same magnitude but negative polarity (polarity opposite that used for the initial curve) shall be applied and the voltage  $U_{0-}$  shall be recorded at this temperature. The procedural steps 7.2.5 to 7.2.7 shall be repeated to record the voltage versus temperature curve with this negative current. In addition, the recording of  $U_{20-}$  shall be made at the same temperature, within  $\pm 1$  K, where  $U_{20+}$  was recorded.

**7.2.9** Each of the two voltages versus temperature curves shall be analyzed by drawing a line (a) through the data where the absolute value of voltage sharply increases with temperature (see Figure 2) and drawing a second line (b) through the data above the transition where the voltage is raised gradually and almost linearly with temperature increase.  $U_{2+}^*$  and  $U_{2-}^*$  in Figure 2 shall be determined at the intersection of these two lines for the positive and negative polarity curves respectively.

**7.2.10** The corrected voltages,  $U_{2+}$  and  $U_{2-}$ , shall be calculated using the following equations,  $U_{2+} = U_{2+}^* - U_{0+}$  and  $U_{2-} = U_{2-}^* - U_{0-}$ . The average voltage,  $\bar{U}_2$ , shall be defined as

$$\bar{U}_2 = \frac{|U_{2+} - U_{2-}|}{2} \quad (5)$$

**7.2.11** A valid  $R_2$  measurement requires that the shift of thermoelectric voltage be within acceptable limits during the measurements of the  $U_{2+}$  and  $U_{2-}$ . Thus, the following condition shall be met for a valid measurement,

$$\frac{|\Delta_+ - \Delta_-|}{U_2} < 3\% \quad (6)$$

where  $\Delta_+$  and  $\Delta_-$  are defined as  $\Delta_+ = U_{20+} - U_{0+}$  and  $\Delta_- = U_{20-} - U_{0-}$ . If the  $R_2$  measurement does not meet the validity requirements in 7.2.4 and this subclause, then improvement steps either in hardware or experimental operation shall be taken to meet these requirements before results are reported.

**7.2.12** Equation (7) shall be used to calculate the measured resistance ( $R_2$ ) just above the superconducting transition.

$$R_2 = \frac{\bar{U}_2}{I_2} \quad (7)$$

### 7.3 Residual resistance ratio (RRR)

The RRR shall be calculated using Equation (1).

## 8 Uncertainty and stability of the test method

### 8.1 Temperature

The room temperature shall be determined with a standard uncertainty not to exceed 0,6 K, while holding the specimen, which is mounted on the measuring base plate, at room temperature.

### 8.2 Voltage measurement

For the resistance measurement, the voltage signal shall be measured with a relative standard uncertainty not to exceed 0,5 %.

### 8.3 Current

When the current is directly applied to the specimen with a programmable DC current source, the specimen test current shall be determined with a standard uncertainty not to exceed 0,3 %.

When the specimen test current is determined from a voltage-current characteristic of a standard resistor by the four-terminal technique, the standard resistor, with a relative combined standard uncertainty not to exceed 0,3 %, shall be used.

The fluctuation of d.c. specimen test current, provided by a d.c. power supply, shall be less than 0,5 % during every resistance measurement.

### 8.4 Dimension

The distance along the specimen between the two voltage taps, ( $L$ ), shall be determined with a relative combined standard uncertainty not to exceed 5 %.

## 9 Test report

### 9.1 *RRR* value

The obtained *RRR* value shall be reported as

$$RRR(1 \pm U_{re}) \quad (n = \dots), \quad (8)$$

where  $U_{re} = 2u_r$  ( $k = 2$ ) is the expanded relative uncertainty with  $u_r$  denoting the uncertainty,  $k$  is a coverage factor and  $n$  is the sampling number. It is desired that  $n$  be larger than 4 so that the normal distribution can be assumed for the estimation of the standard deviation. If  $n$  is not sufficiently large, a square distribution shall be assumed. In case of  $n = 1$  the analytic method described in Annex C shall be used with  $b/R_2 = 1,46 \times 10^{-2}$  estimated from the intercomparison test.

### 9.2 Specimen

The test report for the result of the measurements shall also include the following items, if known:

- a) manufacturer;
- b) classification and/or symbol;
- c) shape and area of the cross-section;
- d) dimensions of the cross-sectional area;
- e) number of filaments;