

IEC 60601-2-52
(First edition – 2009)

Medical electrical equipment –

Part 2-52: Particular requirements for the basic safety and essential performance of medical beds

CEI 60601-2-52
(Première édition – 2009)

Appareils électromédicaux –

Partie 2-52: Exigences particulières de sécurité de base et de performances essentielles des lits médicaux

CORRIGENDUM 1

201.9.1.101 *Protection against PATIENT entrapment in non-moving parts

Replace the first sentence directly below Figure 201.107:

Only applies when the area C above is < 60 mm.

by

* Only applies when the area C above is < 60 mm.

Replace the first sentence directly below Figure 201.108:

Only applies when the area C above is < 60 mm.

<https://standards.iteh.ai/catalog/standards/iec/e184297a-93ec-4266-8c99-cc075d316e5f/iec-60601-2-52-2009-cor1-2010>


by

* Only applies when the area C above is < 60 mm.

201.15.4.6.2 * Limitation of movement

Angle “ α ” is missing in Figures 201.119a 201.119b, 201.119c and 201.119d.

Replace Figure 201.119a by:

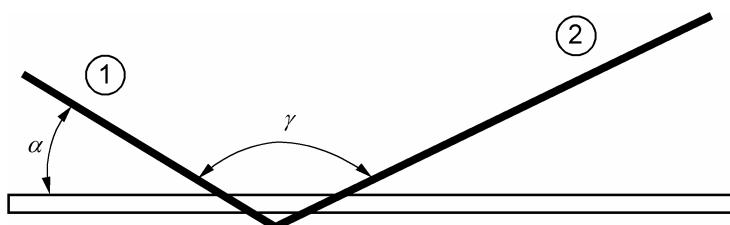

201.9.1.101 *Protection contre un piégeage du PATIENT dans les parties non mobiles

Remplacer le premier alinéa directement en dessous de la Figure 201.107:

Ne s'applique que lorsque la zone C ci-dessus est < 60 mm.

par

* Ne s'applique que lorsque la zone C ci-dessus est < 60 mm.

Replace the first sentence directly below Figure 201.108:

Ne s'applique que lorsque la zone C ci-dessus est < 60 mm.

par

* Ne s'applique que lorsque la zone C ci-dessus est < 60 mm.

201.15.4.6.2 *Limitation du mouvement

L'angle “ α ” manque dans les Figures 201.119a, 201.119b, 201.119c et 201.119d.

Remplacer la Figure 201.119a par: