



Designation: C 698 – 98

## Standard Test Methods for Chemical, Mass Spectrometric, and Spectrochemical Analysis of Nuclear-Grade Mixed Oxides ((U, Pu)O<sub>2</sub>)<sup>1</sup>

This standard is issued under the fixed designation C 698; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ε) indicates an editorial change since the last revision or reapproval.

### 1. Scope

1.1 These test methods cover procedures for the chemical, mass spectrometric, and spectrochemical analysis of nuclear-grade mixed oxides, (U, Pu)O<sub>2</sub>, powders and pellets to determine compliance with specifications.

1.2 The analytical procedures appear in the following order:

	Sections
Uranium by Controlled-Potential Coulometry	2
Plutonium by Controlled-Potential Coulometry	2
Plutonium by Amperometric Titration with Iron (II)	2
Nitrogen by Distillation Spectrophotometry Using Nessler Reagent	7 to 14
Carbon (Total) by Direct Combustion-Thermal Conductivity	15 to 26
Total Chlorine and Fluorine by Pyrohydrolysis	27 to 34
Sulfur by Distillation-Spectrophotometry	35 to 43
Moisture by the Coulometric, Electrolytic Moisture Analyzer	44 to 51
Isotopic Composition by Mass Spectrometry	3
Rare Earths by Copper Spark Spectroscopy	52 to 59
Trace Impurities by Carrier Distillation Spectroscopy	60 to 69
Impurities by Spark-Source Mass Spectrography	70 to 76
Total Gas in Reactor-Grade Mixed Dioxide Pellets	77 to 84
Tungsten by Dithiol-Spectrophotometry	85 to 93
Rare Earth Elements by Spectroscopy	94 to 97
Plutonium-238 Isotopic Abundance by Alpha Spectrometry	98 to 105
Americium-241 in Plutonium by Gamma-Ray Spectrometry	
Uranium and Plutonium Isotopic Analysis by Mass Spectrometry	106 to 114
Oxygen-to-Metal Atom Ratio by Gravimetry	115 to 123

1.3 This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use. (For specific safeguard and safety precaution statements, see Sections 11, 20, 64, and 120 and 110.6.1.)

### 2. Referenced Documents

#### 2.1 ASTM Standards:

C 697 Test Methods for Chemical, Mass Spectrometric, and Spectrochemical Analysis of Nuclear-Grade Plutonium

<sup>1</sup> These test methods are under the jurisdiction of ASTM Committee C-26 on Nuclear Fuel Cycle and are the direct responsibility of Subcommittee C26.05 on Methods of Test.

Current edition approved Feb. 10, 1998. Published June 1998. Originally published as C698 – 72. Last previous edition C698 – 92.

<sup>2</sup> Discontinued as of Nov. 15, 1992.

<sup>3</sup> Discontinued as of May 30, 1980.

Dioxide Powders and Pellets<sup>4</sup>

C 833 Specification for Sintered (Uranium-Plutonium) Dioxide Pellets<sup>4</sup>

C 852 Guide for Design Criteria for Plutonium Gloveboxes  
C 1009 Guide for Establishing a Quality Assurance Program for Analytical Chemistry Laboratories Within the Nuclear Industry

C 1068 Guide for Qualification of Measurement Methods by a Laboratory Within the Nuclear Industry  
C 1108 Test Method for Plutonium by Controlled-Potential Coulometry

C 1128 Guide for Preparation of Working Reference Materials for Use in the Analysis of Nuclear Fuel Cycle Materials

C 1156 Guide for Establishing Calibration for a Measurement Method Used to Analyze Nuclear Fuel Cycle Materials

C 1165 Test Method for Determining Plutonium by Controlled-Potential Coulometry in H<sub>2</sub>SO<sub>4</sub> at a Platinum Working Electrode<sup>4</sup>

C 1168 Practice for Preparation and Dissolution of Plutonium Materials for Analysis

C 1204 Test Method for Uranium in the Presence of Plutonium by Iron (II) Reduction in Phosphoric Acid Followed by Chromium (VI) Titration<sup>4</sup>

C 1206 Test Method for Plutonium by Iron (II)/Chromium (VI) Amperometric Titration<sup>4</sup>

C 1210 Guide for Establishing a Measurement System Quality Control Program for Analytical Chemistry Laboratories Within the Nuclear Industry

C 1268 Test Method for Quantitative Determination of Americium 241 in Plutonium by Gamma-Ray Spectrometry

C 1297 Guide for Qualification of Laboratory Analysts for the Analysis of Nuclear Fuel Cycle Materials

D 1193 Specification for Reagent Water<sup>5</sup>

E 60 Practice for Photometric and Spectrophotometric Methods for Chemical Analysis of Metals<sup>6</sup>

E 115 Practices for Photographic Processing in Optical

<sup>4</sup> Annual Book of ASTM Standards, Vol 12.01.

<sup>5</sup> Annual Book of ASTM Standards, Vol 11.01.

<sup>6</sup> Annual Book of ASTM Standards, Vol 03.05.



Emission Spectrographic Analysis<sup>6</sup>  
E 116 Practice for Photographic Photometry in Spectrochemical Analysis<sup>6</sup>

### 3. Significance and Use

3.1 Mixed oxide, a mixture of uranium and plutonium oxides, is used as a nuclear-reactor fuel in the form of pellets. The plutonium content may be up to 10 weight %, and the diluent uranium may be of any <sup>235</sup>U enrichment. In order to be suitable for use as a nuclear fuel, the material must meet certain criteria for combined uranium and plutonium content, effective fissile content, and impurity content as described in Specification C 833.

3.1.1 The material is assayed for uranium and plutonium to determine whether the plutonium content is as specified by the purchaser, and whether the material contains the minimum combined uranium and plutonium contents specified on a dry weight basis.

3.1.2 Determination of the isotopic content of the plutonium and uranium in the mixed oxide is made to establish whether the effective fissile content is in compliance with the purchaser's specifications.

3.1.3 Impurity content is determined to ensure that the maximum concentration limit of certain impurity elements is not exceeded. Determination of impurities is also required for calculation of the equivalent boron content (EBC).

### 4. Reagents

4.1 *Purity of Reagents*—Reagent grade chemicals shall be used in all tests. Unless otherwise indicated, it is intended that all reagents shall conform to the specifications of the Committee on Analytical Reagents of the American Chemical Society, where such specifications are available.<sup>7</sup> Other grades may be used, provided it is first ascertained that the reagent is of sufficiently high purity to permit its use without lessening the accuracy of the determination.

4.2 *Purity of Water*— Unless otherwise indicated, references to water shall be understood to mean reagent water conforming to Specification D 1193.

### 5. Safety Precautions

5.1 Since plutonium- and uranium-bearing materials are radioactive and toxic, adequate laboratory facilities, gloved boxes, fume hoods, etc., along with safe techniques must be used in handling samples containing these materials. A detailed discussion of all the precautions necessary is beyond the scope of these test methods; however, personnel who handle these materials should be familiar with such safe handling practices as are given in Guide C 852 and in Refs (1) through (3).<sup>8</sup>

5.2 *Committee C-26 Safeguards Statement*.<sup>9</sup>

<sup>7</sup> "Reagent Chemicals, American Chemical Society Specifications," Am. Chem. Soc., Washington, DC. For suggestions on the testing of reagents not listed by the American Chemical Society, see "Reagent Chemicals and Standards," by Joseph Rosin, D. Van Nostrand Co., Inc., New York, NY, and the "United States Pharmacopeia."

<sup>8</sup> The boldface numbers in parentheses refer to the list of references at the end of these test methods.

<sup>9</sup> Based upon Committee C-26 Safeguards Matrix (C 1009, C 1068, C 1128, C 1156, C 1210, C 1297).

5.2.1 The materials [nuclear grade mixed oxides (U, Pu)O<sub>2</sub> powders and pellets] to which these test methods apply are subject to nuclear safeguards regulations governing their possession and use. The following analytical procedures in these test methods have been designated as technically acceptable for generating safeguards accountability measurement data: Uranium by Controlled Potential Coulometry; Plutonium by Controlled-Potential Coulometry; Plutonium by Amperometric Titration with Iron(II); Plutonium-238 Isotopic Abundance by Alpha Spectrometry; and Uranium and Plutonium Isotopic Analysis by Mass Spectrometry.

5.2.2 When used in conjunction with appropriate certified reference materials (CRMs), these procedures can demonstrate traceability to the national measurements base. However, adherence to these procedures does not automatically guarantee regulatory acceptance of the resulting safeguards measurements. It remains the sole responsibility of the user of these test methods to assure that its application to safeguards has the approval of the proper regulatory authorities.

### 6. Sampling and Dissolution

6.1 Criteria for sampling this material are given in Specification C 833.

6.2 Samples can be dissolved using the appropriate dissolution techniques described in Practice C 1168.

#### URANIUM IN THE PRESENCE OF PLUTONIUM BY POTENTIOMETRIC TITRATION

(This test method was discontinued in 1992 and replaced by Test Method C 1204.)

#### PLUTONIUM BY CONTROLLED POTENTIAL COULOMETRY

(This test method was discontinued in 1992 and replaced by Test Method C 1165.)

#### PLUTONIUM BY CONTROLLED-POTENTIAL COULOMETRY

(With appropriate sample preparation, controlled-potential coulometric measurement as described in Test Method C 1108 may be used for plutonium determination.)

#### PLUTONIUM BY AMPEROMETRIC TITRATION WITH IRON(II)

(This test method was discontinued in 1992 and replaced by Test Method C 1206.)

#### NITROGEN BY DISTILLATION SPECTROPHOTOMETRY USING NESSLER REAGENT

### 7. Scope

7.1 This test method covers the determination of 5 to 100 µg/g of nitride nitrogen in mixtures of plutonium and uranium oxides in either pellet or powder form.

### 8. Summary of Test Method

8.1 The sample is dissolved in hydrochloric acid by the sealed tube test method or by phosphoric acid-hydrofluoric

acid solution, after which the solution is made basic with sodium hydroxide and nitrogen is separated as ammonia by steam distillation. Nessler reagent is added to the distillate to form the yellow ammonium complex and the absorbance of the solution is measured at approximately 430 nm (4, 5).

## 9. Apparatus

- 9.1 *Distillation Apparatus* (see Fig. 1).
- 9.2 *Spectrophotometer*, visible-range.

## 10. Reagents

- 10.1 *Ammonium Chloride* ( $\text{NH}_4\text{Cl}$ )—Dry the salt for 2 h at 110 to 120°C.
- 10.2 *Boric Acid Solution* (40 g/litre)—Dissolve 40 g of boric acid ( $\text{H}_3\text{BO}_3$ ) in 800 mL of hot water. Cool to approximately 20°C and dilute to 1 L.
- 10.3 *Hydrochloric Acid* (sp gr 1.19)—Concentrated hydrochloric acid (HCl).
- 10.4 *Hydrofluoric Acid* (sp gr 1.15)—Concentrated hydrofluoric acid (HF).
- 10.5 *Nessler Reagent*—To prepare, dissolve 50 g of potassium iodide (KI) in a minimum of cold ammonia-free water, approximately 35 mL. Add a saturated solution of mercuric chloride ( $\text{HgCl}_2$ , 22 g/350 mL) slowly until the first slight precipitate of red mercuric iodide persists. Add 400 mL of 9 N sodium hydroxide (NaOH) and dilute to 1 L with water. Mix, and allow the solution to stand overnight. Decant the supernatant liquid and store in a brown bottle.
- 10.6 *Nitrogen, Standard Solution* (1 mL = 0.01 mg N)—Dissolve 3.819 g of  $\text{NH}_4\text{Cl}$  in water and dilute to 1 L. Transfer 10 mL of this solution to a 1-L volumetric flask and dilute to volume with ammonia-free water.
- 10.7 *Sodium Hydroxide* (9 N)—Dissolve 360 g of sodium hydroxide (NaOH) in ammonia-free water and dilute to 1 L.
- 10.8 *Sodium Hydroxide Solution*—(50%)—Dissolve NaOH in an equal weight of ammonia-free water.
- 10.9 *Water, Ammonia-Free*—To prepare, pass distilled water through a mixed-bed resin demineralizer and store in a tightly stoppered chemical-resistant glass bottle.

## 11. Precautions

11.1 The use of ammonia or other volatile nitrogenous compounds in the vicinity can lead to serious error. The following precautionary measures should be taken: (1) Clean all glassware and rinse with ammonia-free water immediately

prior to use, and (2) avoid contamination of the atmosphere in the vicinity of the test by ammonia or other volatile nitrogenous compounds.

## 12. Procedure

### 12.1 *Dissolution of Sample:*

12.1.1 Transfer a weighed sample, in the range from 1.0 to 1.5 g, to a 50-mL beaker.

NOTE 1—Pellet samples should be crushed to a particle size of 1 mm or less with a diamond mortar.

12.1.2 To the sample add 5 mL of HCl (sp gr 1.19) and 3 drops of HF (sp gr 1.15). Heat to put the sample into solution.

NOTE 2—Concentrated phosphoric acid or mixtures of phosphoric acid and hydrofluoric acids or of phosphoric and sulfuric acids may be used for the dissolution of mixed oxide samples. Such acids may require a purification step in order to reduce the nitrogen blank before being used in this procedure.

### 12.2 *Distillation:*

12.2.1 Quantitatively transfer the sample solution to the distilling flask of the apparatus. Add 20 mL of ammonia-free water and then clamp the flask into place on the distillation apparatus (see Fig. 2).

12.2.2 Turn on the steam generator but do not close with the stopper.

12.2.3 Add 5 mL of boric acid solution (4 %) to a 50-mL graduated flask and position this trap so that the condenser tip is below the surface of the boric acid solution.

12.2.4 Transfer 20 mL of NaOH solution (50 %) to the funnel in the distillation head.

12.2.5 When the water begins to boil in the steam generator, replace the stopper and slowly open the stopcock on the distilling flask to allow the NaOH solution to run into the sample solution.

NOTE 3—The NaOH solution must be added slowly to avoid a violent reaction which may lead to loss of sample.

12.2.6 Steam distill until 25 mL of distillate has collected in the trap.

12.2.7 Remove the trap containing the distillate from the distillation apparatus, and remove the stopper from the steam generator.

12.2.8 Transfer the cooled distillate to a 50-mL volumetric flask.

12.2.9 Prepare a reagent blank solution by following steps 12.1.1 through 12.2.8.

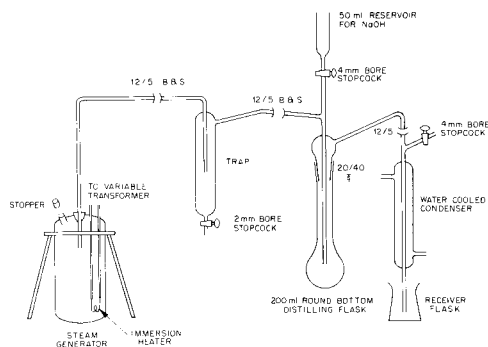


FIG. 1 Distillation Apparatus

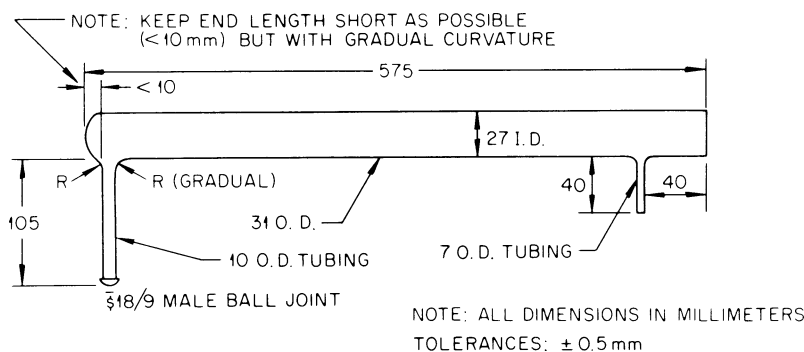


FIG. 2 Quartz Reaction Tube

### 12.3 Measurement of Nitrogen:

12.3.1 Add 1.0 mL of Nessler reagent to each of the distillates collected in 12.2.8 and 12.2.9. Dilute to volume with ammonia-free water, mix, and let stand for 10 min.

12.3.2 Measure the absorbance of the solutions at 430 nm in a 1-cm cell. Use water as the reference.

### 12.4 Calibration Curve:

12.4.1 Add 0, 5, 10, 25, 100, and 150 µg of nitrogen from the nitrogen standard solution to separate distilling flasks. Then, add 5 mL of HCl and 3 drops of HF plus 20 mL of ammonia-free water to each flask.

12.4.2 Process each solution by the procedure in 12.2 through 12.3 (omit step 12.2.9).

12.4.3 Correct for the reagent blank reading and plot the absorbance of each standard against micrograms of nitrogen per 50 mL of solution.

### 13. Calculation

13.1 From the calibration chart, read the micrograms of nitrogen corresponding to the absorbance of the sample solution.

13.2 Calculate the nitrogen content of the sample as follows:

$$N, \mu\text{g/g} = (A - B)/W \quad (1)$$

where:

A = micrograms of nitrogen from sample plus reagents,

B = micrograms of nitrogen in blank, and

W = grams of sample.

### 14. Precision and Bias

14.1 The estimated relative standard deviation for a single measurement by this test method is 20 % for 3 µg of nitrogen and 3 % for 50 to 90 µg of nitrogen.

## CARBON (TOTAL) BY DIRECT COMBUSTION-THERMAL CONDUCTIVITY

### 15. Scope

15.1 This test method covers the determination of 10 to 200 µg of residual carbon in nuclear grade mixed oxides, (U,Pu)O<sub>2</sub>.

### 16. Summary of Test Method

16.1 Powdered samples are covered and mixed with an accelerator in carbon-free crucibles and burned with oxygen in

an induction heating furnace. Traces of sulfur compounds and water vapor are removed from the combustion products by a purification train and the resultant carbon monoxide is converted to carbon dioxide. The purified carbon dioxide is trapped on a molecular sieve, eluted therefrom with a stream of helium upon application to heat to the trap, and passed through a thermal conductivity cell. The amount of carbon present, being a function of the integrated change in the current of the detector cell, is read directly from a calibrated-digital voltmeter or strip-chart recorder.

### 17. Interferences

17.1 There are no known interferences not eliminated by the purification system.

### 18. Apparatus

18.1 *Commercial Combustion Apparatus*, suitable for the carbon determination, is often modified to facilitate maintenance and operation within the glove box which is required for all work with plutonium materials.

18.2 *Combustion Apparatus*,<sup>10</sup> consisting of an induction furnace, suitable for operation at 1600°C, a catalytic furnace, a purification train, a carbon dioxide trap, thermal conductivity cell with appropriate readout equipment, and a regulated supply of oxygen and helium.

18.3 *Combustion Tubes*— Quartz combustion tubes with integral baffle shall be used.

18.4 *Crucibles*—Expendable alumina or similar refractory crucibles shall be used. The use of crucible covers is optional. Satisfactory operation with covers must be established by analysis of standards. Crucibles and covers (if used) must be ignited at a temperature of 1000°C or higher for a time sufficient to produce constant blank values.

18.5 *Accelerators*— Granular tin, copper, iron, and copper oxide accelerators shall be used to obtain satisfactory results. The criterion for satisfactory results is the absence of significant additional carbon release upon recombustion of the specimen.

18.6 *Catalytic Furnace and Tube*—This unit, which is used to ensure complete conversion of CO to CO<sub>2</sub>, consists of a tube containing copper oxide and maintained at a temperature of 300°C by a small furnace.

<sup>10</sup> A Leco Low Carbon Analyzer, sold by Laboratory Equipment Co., St. Joseph, MI, or equivalent, has been found satisfactory for this purpose.



18.7 *Carbon Dioxide Purifiers*—The purifiers that follow the combustion tube must remove finely divided solid metallic oxides and oxides of sulfur and selenium, dry the gases before they enter the CO<sub>2</sub> trap, and protect the absorber from outside effects. Finely divided solid metal oxides are removed from the gases during their passage through the quartz wool. The SO<sub>2</sub> given off by materials containing sulfur is removed by MnO<sub>2</sub> and any water vapor is absorbed in a tube containing Mg(ClO<sub>4</sub>)<sub>2</sub>. Hot copper oxide converts carbon monoxide to carbon dioxide. Additional components in the purification train may be required when materials containing very high amounts of sulfur or of halides are being analyzed. The materials used in the purification train must be checked frequently to ensure that their absorbing capacity has not been exhausted.

18.8 *Vibratory Sample Pulverizer Apparatus*,<sup>11</sup> capable of reducing ceramic materials to a – 100-mesh powder. A stainless steel capsule and mixing ball must be used, in order to reduce contamination of the sample with carbon.

## 19. Reagents and Materials

19.1 *Quartz Wool*, used as a dust trap at the top of the combustion tube.

19.2 *Sulfuric Acid (H<sub>2</sub>SO<sub>4</sub>, sp gr 1.84)*, used in the oxygen purification train.

19.3 *Standard Materials*—National Institute for Standards and Technology (NIST) SRMs 131c (0.0029 % carbon) and 336 (0.567 % carbon) or their replacements.

## 20. Safety Precautions

20.1 *Samples Containing Plutonium*—Due to the extreme toxicity of plutonium and the certainty that some plutonium will become airborne during the analytical operations, it is mandatory to perform all operations within an approved glove box fitted with off-gas filters capable of sustained operation with dust-laden atmospheres.

20.2 *Samples Containing Uranium*—Natural or depleted uranium presents a somewhat less serious toxicological hazard than plutonium, but operations should be conducted in a fume hood with adequate ventilation, as a minimum precaution.

## 21. Sampling and Preparation

21.1 *Sample Size*—The normal size for mixed oxide [(U,Pu)O<sub>2</sub>] fuel materials shall be 1 g. If necessary, this amount shall be altered as required to contain less than 200 µg of carbon.

21.2 *Sample Preparation*—Pellet or particulate samples shall be reduced to approximately – 100-mesh powder prior to the weighing of the specimens. Exposure of the powdered sample to atmospheric carbon dioxide should be minimized by storage of the powder in a closed vial.

## 22. Preparation of Apparatus

22.1 *Analysis System Purge*—After having properly set the operating controls of the instrument system, condition the apparatus by combustion of several blanks prepared with the

sample crucible and accelerator in the amount to be used with the test specimen analyses. Successive blank values should approach a constant value, allowing for normal statistical fluctuations. The instrument should be adjusted for a 2-min combustion period.

## 23. Calibration

23.1 *Preparation of Standards for Combustion*—Mix a weighed portion of an accelerator and a weighed portion of approximately 1 g of NIST 131c Low-Carbon Steel in each of the three sample crucibles. Repeat with NIST SRM 336 (Note 4), using approximately 30 to 40 mg.

NOTE 4—The NIST SRM 336 steel is assigned a carbon content of 0.567 % (5670 µg/g). Therefore, amounts ranging up to approximately 40 mg are used for standardization. Weigh the steel into a tared container (a small nickel sample boat if convenient), obtaining the mass to the nearest 0.01 mg. Transfer the chips to a 30-mm square of aluminum foil (previously acetone washed), and fold the foil into a wrapper with the aid of stainless steel tongs and spatulas. The foil should not be touched by the hands. Place the wrapped standard in a numbered glass sample vial and transfer to the analyzer glove box.

23.2 *Combustion of Standards*—Load and combust the standards and record the results. Adjust the calibration controls in such a way as to produce the correct readout value on the direct readout meter. Combust additional standards as required to produce the correct direct readout. As an alternative, consider the readout digits as arbitrary numbers and prepare a calibration curve of known micrograms of carbon versus readout value. A strip chart recorder connected to present the integrated value of the carbon dioxide response signal is helpful in detecting and correcting for analyzer drift and noise.

## 24. Procedure

24.1 Pulverize the pellet samples for 15 s in the stainless steel capsule of the sample pulverizer.

24.2 Weigh a sample crucible containing the required amount of accelerator to the nearest 0.01 g.

24.3 Transfer the sample powder, not to exceed 1 g or of such size as to give not more than 200 µg of carbon, to the crucible. Weigh the crucible and contents to the nearest 0.01 g and find the specimen mass by difference.

24.4 Mix the specimen powder and the accelerator with a stainless steel spatula.

24.5 Load the sample crucible into the furnace and combust the specimen for 2 min.

24.6 Remove the sample crucible and examine it for evidence of incomplete combustion. The crucible contents should be a uniform fused mass.

## 25. Calculation

25.1 Calculate the concentration of carbon in the sample by dividing the net micrograms of carbon found by the sample mass expressed in grams as follows:

$$C, \mu\text{g/g} = (C_s - C_b/W) \quad (2)$$

where:

$C_s$  = carbon in sample and reagents, µg,  
 $C_b$  = carbon in reagent blank, µg, and  
 $W$  = grams of mixed oxide sample.

<sup>11</sup> Wig-L-Bug, sold by Spex Industries Inc., Scotch Plains, NJ, has been found satisfactory for this purpose.

## 26. Precision and Bias

26.1 *Precision*—The average standard deviation for a single measurement from the results of six laboratories is on the order of  $10\mu\text{ g}$  carbon/g of sample.

26.2 *Bias*—The results obtained by six laboratories participating in a recent comparative analytical program averaged 85 % of the expected  $100\mu\text{ g/g}$  of carbon in the sample. The incomplete recovery is thought to represent a lack of experience on the part of two laboratories inasmuch as 95 to 100 % recovery was obtained by three of the participating laboratories.

## TOTAL CHLORINE AND FLUORINE BY PYROHYDROLYSIS

### 27. Scope

27.1 This test method is applicable to the determination of 5 to  $100\mu\text{ g/g}$  of chlorine and 1 to  $100\mu\text{ g/g}$  of fluorine in 1-g samples of nuclear-grade mixed oxides, (U, Pu) $\text{O}_2$ .

### 28. Summary of Test Method

28.1 A 1 to 2-g sample of the mixed oxide is pyrohydrolyzed at  $950^\circ\text{ C}$  with a stream of moist air or oxygen. The halogens are volatilized as acids during the pyrohydrolysis and are trapped as chloride and fluoride in a buffered solution. Several procedures are outlined for the measurement of chloride and fluoride in the resultant condensate. Chloride is measured by spectrophotometry, microtitrimetry, or with ion-selective electrodes and fluoride with ion-selective electrodes or spectrophotometry (6–9).

### 29. Interferences

29.1 Bromide, iodide, cyanide, sulfide, and thiocyanate, if present in the condensate, would interfere with the spectrophotometric and microtitrimetric measurement of chloride. Bromide, iodide, sulfide, and cyanide interfere in the measurement of chloride with ion-selective electrodes, but have very little effect upon the measurement of fluoride with selective electrodes.

### 30.

Apparatus (See Fig. 3 and Fig. 2)

30.1 *Gas-Flow Regulator*—A flowmeter and a rate controller are required to adjust the flow of sparge gas between 1 to 3 L/min.

30.2 *Hot Plate*—A heater used to keep the water bubbler temperature between  $50$  and  $90^\circ\text{ C}$  is required.

30.3 *Furnace*—A tube furnace is required that is capable of maintaining a temperature from  $900$  to  $1000^\circ\text{ C}$ . The bore of the furnace should be about  $32\text{ mm}$  ( $1\frac{1}{4}\text{ in.}$ ) in diameter and about  $305\text{ mm}$  ( $12\text{ in.}$ ) in length.

30.4 *Reactor Tube*, made from fused-silica or platinum. The delivery tube should be a part of the exit end of the reactor tube and be within  $51\text{ mm}$  ( $2\text{ in.}$ ) of the furnace. (See Fig. 3 for proper tube positioning.)

30.5 *Combustion Boats*, made from fused-silica or platinum. A boat about  $102\text{ mm}$  ( $4\text{ in.}$ ) long is made by cutting lengthwise a  $20\text{-mm}$  diameter silica tube and flattening one end to provide a handle. A fused-silica inner sleeve for the reactor tube can facilitate the movement of the boat into the tube, prevent spillage, and thus prolong the life of the combustion tube.

30.6 *Collection Vessel*—A plastic graduate or beaker designed to maintain most of the scrubber solution above the tip of the delivery tube is required.

30.7 *Automatic Chloride Titrator*.<sup>12</sup>

30.8 *Ion-selective Electrodes*, chloride and fluoride.

30.9 *Reference Electrode*—Use a double-junction type such as mercuric sulfate, sleeve-junction type electrode. Do not use a calomel electrode.

30.10 *Spectrophotometer*—Ultraviolet to visible range and absorption cells. For a discussion on spectrophotometers and their use see Practice E 60.

30.11 *Meter, pH*, with expanded scale with a sensitivity of  $1\text{ mV}$ .

### 31. Reagents

31.1 *Accelerator* ( $\text{U}_3\text{O}_8$ )—Halogen free  $\text{U}_3\text{O}_8$  powder used as a flux to enhance the release of chloride and fluoride.

31.2 *Air or Oxygen*, compressed.

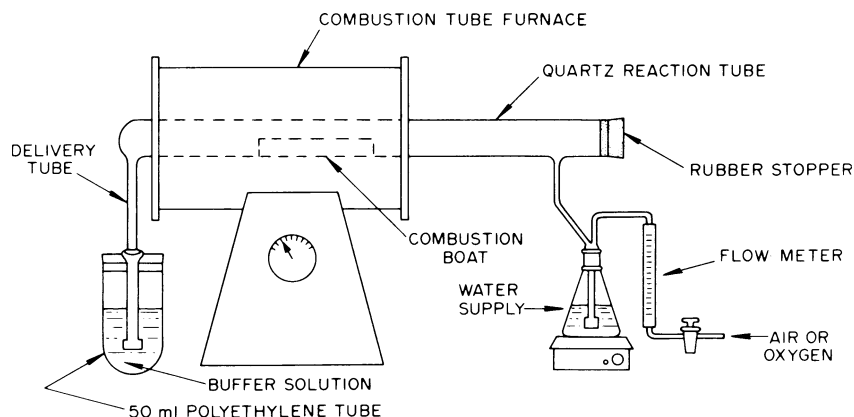


FIG. 3 Pyrohydrolysis Apparatus

<sup>12</sup> A Cotlov Titrator, sold by American Instrument Co., Silver Spring, MD, or by Buchler Instruments, Inc., Fort Lee, NJ, or equivalent, has been found satisfactory for this purpose.

31.3 *Buffer Solution (0.001 N Acetic Acid, 0.001 N Potassium Acetate)*—Prepare by adding 50  $\mu\text{L}$  of glacial acetic acid ( $\text{CH}_3\text{CO}_2\text{H}$ , sp gr 1.05) and 0.10 g of potassium acetate ( $\text{KC}_2\text{H}_3\text{O}_2$ ) to 1 L of water.

31.4 *Chloride Standard Solution (1 mL = 1 mg Cl)*—Dissolve 1.65 g of sodium chloride ( $\text{NaCl}$ ) in water and dilute to 1 L.

31.5 *Chloride Standard Solution (1 mL = 5  $\mu\text{g}$  Cl)*—Prepare by diluting 5 mL of chloride solution (1 mL = 1 mg Cl) to 1 L with water.

31.6 *Ferric Ammonium Sulfate (0.25 M in 9 M Nitric Acid)*—Dissolve 12 g of  $\text{FeNH}_4(\text{SO}_4)_2 \cdot 12 \text{H}_2\text{O}$  in 58 mL of concentrated nitric acid ( $\text{HNO}_3$ , sp gr 1.42) and dilute to 100 mL with water.

31.7 *Fluoride, Standard Solution (1 mL = 1 mg F)*—Dissolve 2.21 g of sodium fluoride ( $\text{NaF}$ ) in water and dilute to 1 L.

31.8 *Fluoride, Standard Solution (1 mL = 10  $\mu\text{g}$  F)*—Dilute 10 mL of fluoride solution (1 mL = 1 mg F) to 1 L with water.

31.9 *Gelatin Solution*—Add 6.2 g of dry gelatin mixture (60 parts of dry gelatin + 1 part of thymol blue + 1 part of thymol) to 1 L of hot water and heat while stirring until the solution is clear.

31.10 *Lanthanum-Alizarin Complexone*—Dissolve 0.048 g of alizarin complexone (3-aminomethylalizarin-*N,N*-diacetic acid) in 100  $\mu\text{L}$  of concentrated ammonium hydroxide, 1 mL of an ammonium acetate solution ( $\text{NH}_4\text{C}_2\text{H}_3\text{O}_2$ , 20 mass %), and 5 mL of water. Filter the solution through high grade, rapid filter paper. Wash the paper with a small volume of water and add 8.2 g of anhydrous sodium acetate ( $\text{NaC}_2\text{H}_3\text{O}_2$ ) and 6 mL of  $\text{CH}_3\text{CO}_2\text{H}$  (sp gr 1.05) to the filtrate. Add 100 mL of acetone while swirling the filtrate. Add 0.040 g of lanthanum oxide ( $\text{La}_2\text{O}_3$ ) dissolved in 2.5 mL of warm 2 N HCl. Mix the two solutions and dilute to 200 mL. After 30 min readjust the solution volume.<sup>13</sup>

NOTE 5—A 0.1-g/L solution of Amadac-F is prepared by dissolving 100 mg of the reagent in water and diluting with isopropyl alcohol to obtain a 60 % alcoholic medium.

31.11 *Mercuric Thiocyanate Solution*—Prepare a saturated solution by adding 0.3 g of mercuric thiocyanate [ $\text{Hg}(\text{SCN})_2$ ] to 100 mL of ethanol (95 %). Shake the mixture thoroughly for maximum dissolution of the solid. Filter the solution.

31.12 *Nitric Acid-Acetic Acid Solution (1 N nitric acid and 4 N acetic acid)*—Prepare by adding 64 mL of nitric acid ( $\text{HNO}_3$ , sp gr 1.42) to a 1-L volumetric flask which contains 500 mL of water. Swirl the solution in the flask and add 230 mL of  $\text{CH}_3\text{CO}_2\text{H}$  (sp gr 1.05). Dilute the solution with water to 1 L.

## 32. Pyrohydrolysis Procedure

32.1 Prepare the pyrohydrolysis apparatus for use as follows:

32.1.1 Regulate the gas flow between 1 and 3 L/min.

32.1.2 Adjust the temperature of the hot plate to heat the water to approximately 90° C.

32.1.3 Adjust the temperature of the furnace to  $950 \pm 50^\circ \text{C}$ .

32.1.4 Add 15 mL of buffer solution to the collection vessel and place around the delivery tube.

32.2 Weigh accurately 1 to 2 g of the powdered mixed oxide and transfer to a combustion boat. If an accelerator,  $\text{U}_3\text{O}_8$ , is used, mix 4 g with the sample before loading the powdered mixed oxide into the boat.

32.3 Place the boat containing the sample into the reactor tube and quickly close the tube. The boat should be in the middle of the furnace.

32.4 Allow the pyrohydrolysis to proceed for at least 30 min.

32.5 Remove the collection vessel and wash down the delivery tube with some buffer solution. Dilute the solution to 25 mL with the acetate buffer. Determine the chloride and fluoride by one or more of the measurement procedures covered in Section 60.

32.6 Remove the boat from the reactor tube and dispose of the sample residue.

32.7 Run a pyrohydrolysis blank with halogen-free  $\text{U}_3\text{O}_8$  by following the procedure in 32.3 through 32.6.

## 33. Measurement of Chloride and Fluoride

33.1 *Determination of Chloride by Spectrophotometry:*

33.1.1 Prepare a calibration curve by adding 0, 1, 2, 5, and 10 mL of chloride standard solution (1 mL = 5  $\mu\text{g}$  Cl) to separate 25-mL flasks. Dilute each to 20 mL with the buffer solution, add 2 mL of ferric ammonium sulfate solution and 2 mL of mercuric thiocyanate reagent. Mix the solution and dilute to 25 mL with water. Mix the solutions again and allow them to stand 10 min. Transfer some of the solution from the flask to a 1-cm absorption cell and read the absorbance at 460 nm using water as the reference liquid. Plot the micrograms of chloride per 25 mL versus the absorbance reading.

33.1.2 To determine the chloride in the pyrohydrolysis condensate transfer 15 mL of buffer solution to a 25-mL volumetric flask. Add 2 mL of ferric ammonium sulfate solution and 2 mL of mercuric thiocyanate solution. Mix the solutions, dilute to volume with water, and mix again. Allow the solution to stand 10 min. Transfer some of the solution from the flask to a 1-cm absorption cell and read the absorbance at 460 nm versus water as the reference. Read the micrograms of chloride present from the calibration curve.

NOTE 6—A calibration curve can be prepared by drying measured aliquots of a standard chloride solution on some halogen-free  $\text{U}_3\text{O}_8$  and proceeding through pyrohydrolysis steps.

33.1.3 Calculate the chlorine as follows:

$$\text{Cl, } \mu\text{g/g} = [(A - B)/W](V_1/V_2) \quad (3)$$

where:

*A* = micrograms of chlorine in aliquot measured,

*B* = micrograms of chlorine in blank,

*W* = grams of mixed oxide pyrohydrolyzed,

*V*<sub>1</sub> = millilitres of scrub solution, and

*V*<sub>2</sub> = aliquot in millilitres of scrub solution analyzed.

33.2 *Determination of Chloride by Amperometric Microtitrimetry:*

<sup>13</sup> The reagent is available commercially under the name Amadac-F.



33.2.1 Calibrate the titrimeter by adding 5 mL of buffer solution, 1 mL of nitric acid-acetic acid solution, and 2 drops of the gelatin solution to a titration cell. Pipet 50  $\mu\text{L}$  of the chloride standard solution (1 mL = 1 mg Cl) into the titration cell. Place the cell on the chloride titrator and follow the manufacturer's suggested sequence of operations for titrating chloride. Record the time required to titrate 50  $\mu\text{g}$ . Run a reagent blank titration.

NOTE 7—The chloride analyzer generates silver ions which react to precipitate the chloride ion. The instrument uses an amperometric end point to obtain an automatic shut-off of the generating current at a pre-set increment of indicator current. Since the rate of generating silver ion is constant, the amount of chloride precipitated is proportional to the time required for the titration.

33.2.2 Determine the chloride in the pyrohydrolysis scrub solution by adding 5 mL to a titration cell which contains 1 mL of the nitric acid-acetic acid solution and 2 drops of the gelatin solution.

33.2.3 Place the cell in position on the titrator. Start the titrator and record the time required to titrate the chloride present.

33.2.4 Calculate the chlorine as follows:

$$\text{Cl, } \mu\text{g/g} = V_1 F (T_s - T_B) / V_2 W \quad (4)$$

where:

- $V_1$  = volume of scrub solutions = 25,
- $V_2$  = aliquot, in millilitres, of scrub solution analyzed,
- $F$  = micrograms of Cl standard titrated/titration time of standard – titration time of blank or
- $F = 50 / (T_{\text{Cl}} - T_B)$ ,
- $T_s$  = titration time to titrate sample and blank,
- $T_{\text{Cl}}$  = titration time to titrate 50  $\mu\text{g}$  Cl and blank,
- $T_B$  = titration time to titrate reagent blank, and
- $W$  = grams of mixed oxide pyrohydrolyzed.

33.3 *Determination of Chloride and Fluoride With Ion-Selective Electrodes:*

33.3.1 Preparation of the calibration curves requires the assembly of the meter and the ion-selective electrode with a suitable reference electrode. From these standards take the millivolt readings for each ion-selective electrode and plot on semi-log paper the halogen content per 25 mL *versus* millivolts. Prepare a series of standards in acetate buffer solution by pipeting aliquots of the halogen standards into separate 25-mL flasks ranging in concentrations as follows:

- chloride 10 to 100  $\mu\text{g}/25$  mL
- fluoride 5 to 100  $\mu\text{g}/25$  mL

33.3.2 Determine the chloride and fluoride in the scrub solution from the pyrohydrolysis by using the appropriate ion-selective electrode. Record the micrograms of chloride or fluoride from the calibration curve and calculate the halide as follows:

$$\text{Cl or F, } \mu\text{g/g} = (H_s - H_b) / W \quad (5)$$

where:

- $H_s$  = micrograms of halide in aliquot of scrub solution plus blank,
- $H_b$  = micrograms of halide in pyrohydrolysis blank, and
- $W$  = grams of sample.

33.4 *Determination of Fluoride by Spectrophotometry:*

33.4.1 Prepare a calibration curve by adding to separate 10-mL flasks 0, 50, 100, 200, 500, and 1000  $\mu\text{L}$  of fluoride standard solution (1 mL = 10  $\mu\text{g}$  F). Add 2.0 mL of lanthanum-alizarin complexone solution and dilute to volume with water. Mix and let stand 1 h. Read the absorbance at 622 nm *versus* the reagent blank. Plot the micrograms of fluoride per 10 mL *versus* the absorbance reading.

33.4.2 Measure the fluoride in the pyrohydrolysis scrub solution by pipeting 5 mL into a 10-mL volumetric flask. Add 2.0 mL of lanthanum-alizarin complexone and dilute to volume. Mix and let stand 1 h. Read the absorbance at 622 nm *versus* a reagent blank and obtain the fluoride content from the calibration curve.

33.4.3 Calculate the fluorine concentration in the mixed oxide sample as follows:

$$\text{F, } \mu\text{g/g} = [(F_s - F_b) / W] \times (V_1 / V_2) \quad (6)$$

where:

- $F_s$  = fluorine in aliquot of scrub solution plus the blank,  $\mu\text{g}$ ,
- $F_b$  = fluorine in pyrohydrolysis blank,  $\mu\text{g}$ ,
- $V_1$  = total volume of the scrub solution, mL,
- $V_2$  = aliquot of scrub solution analyzed, mL, and
- $W$  = grams of mixed oxide sample.

## 34. Precision and Bias

34.1 The relative standard deviations for the measurements of fluorine are approximately 7 % for the 5 to 50- $\mu\text{g/g}$  range and 10 % for the 1 to 5- $\mu\text{g/g}$  range. The relative standard deviations for the measurements of chlorine vary from 5 % at the 5 to 50- $\mu\text{g/g}$  level and up to 10 % below the 5- $\mu\text{g/g}$  range.

## SULFUR BY DISTILLATION-SPECTROPHOTOMETRY

### 35. Scope

35.1 This test method covers the determination of sulfur in the concentration range from 10 to 600  $\mu\text{g/g}$  for samples of nuclear-grade uranium and plutonium mixed oxides, (U, Pu) $\text{O}_2$ .

### 36. Summary of Test Method

36.1 Sulfur is measured spectrophotometrically as Lauth's Violet following its separation by distillation as hydrogen sulfide (10). Higher oxidation states of sulfur are reduced to sulfide by a hypophosphorous-hydriodic acid mixture, the hydrogen sulfide is distilled into zinc acetate, and *p*-phenylenediamine and ferric chloride are added to form Lauth's Violet. The quantity of sulfur is calculated from the measured absorbance at 595 nm and the absorbance per microgram of sulfur obtained for calibration materials having known sulfur contents. The relative standard deviation ranges from 12 to 3 % for the concentration range from 10 to 600  $\mu\text{g}$  of sulfur per gram of sample.

### 37. Interference

37.1 None of the impurity elements interfere when present in amounts up to twice their specification limits for uranium and plutonium mixed oxides.



### 38. Apparatus

- 38.1 *Boiling Flask*, adapted with a gas inlet line and fitted with a water-cooled condenser and delivery tube.
- 38.2 *Spectrophotometer*, with matched 1-cm cells.
- 38.3 *Sulfur Distillation Apparatus*—see Fig. 4.

### 39. Reagents

- 39.1 *Argon Gas*, cylinder.
- 39.2 *Ferric Chloride Solution*, 2 % ferric chloride ( $\text{FeCl}_3$ ) in 6 M HCl.
- 39.3 *Formic Acid*, redistilled.
- 39.4 *Hydriodic-Hypophosphorous Acid Reducing Mixture*—Mix 400 mL of 47 % hydriodic acid (HI) with 200 mL of hypophosphorous acid ( $\text{H}_3\text{PO}_2$ ) (31 %) and boil under reflux for 30 min with a continuous argon sparge. Test for the sulfur content by analyzing a 15-mL aliquot as described in the procedure. Reboil if necessary to reduce the sulfur content to below 1  $\mu\text{g/mL}$ .
- 39.5 *Hydrochloric Acid (0.6 M)*—Dilute 10 mL of 12 M hydrochloric acid (HCl) to 200 mL with water.
- 39.6 *Hydrochloric Acid (3 M)*—Dilute 50 mL of 12 M HCl to 200 mL with water.
- 39.7 *Hydrochloric Acid (6 M)*—Dilute 100 mL of 12 M HCl to 200 mL with water.
- 39.8 *Hydrochloric Acid (12 M)*—Analyze an aliquot of HCl (sp gr 1.19) for sulfur content. Use only a reagent in which the sulfur content is less than 1  $\mu\text{g}/10\text{ mL}$  and prepare the diluted acids with this reagent.
- 39.9 *Hydrofluoric Acid (HF)*, (sp gr 1.15)—Concentrated hydrofluoric acid (HF).
- 39.10 *Hydroxylamine Hydrochloride* ( $\text{NH}_2\text{OH}\cdot\text{HCl}$ ), 20 % aqueous solution.
- 39.11 *Nitric Acid ( $\text{HNO}_3$ ) (15.6 M)*, 70 %.
- 39.12 *p-Phenylenediamine (1 %)*—Dissolve 1 g of p-phenylenediamine in 100 mL of 0.6 M HCl.
- 39.13 *Silver Nitrate* ( $\text{AgNO}_3$ ), 1 % aqueous solution.

39.14 *Sulfur Calibration Solution (1 mL = 5  $\mu\text{g S}$ )*—Dissolve 2.717 g of dry potassium sulfate ( $\text{K}_2\text{SO}_4$ ) in water and dilute to 1 L. Dilute 2.00 mL to 200 mL with water.

39.15 *Zinc Acetate Solution (4 %)*—Dissolve 20 g of zinc acetate [ $\text{Zn}(\text{C}_2\text{H}_3\text{O}_2)_2$ ] in 500 mL of water and filter.

### 40. Calibration

- 40.1 Use aliquots of standard sulfur solution (1 mL = 5  $\mu\text{g S}$ ) to test the test method and check the apparatus. Ideally, blends of oxides and sulfur (20 to 600  $\mu\text{g S/g}$ ) should be analyzed to simulate actual sample conditions.
- 40.2 Prepare a calibration curve of absorbance versus sulfur (using aliquots of the sulfur standard solution) covering a concentration range from 5  $\mu\text{g}$  to 50  $\mu\text{g}/50\text{ mL}$ .

### 41. Procedure

- 41.1 Pulverize mixed oxide pellets in a mixer-mill with a tungsten carbide container and a tungsten carbide ball.
- 41.2 Transfer a sample, weighed to  $\pm 0.2\text{ mg}$ , to a 20-mL beaker or a 30-mL platinum dish. Use a 0.5-g sample when the expected level of sulfur is 100  $\mu\text{g/g}$  or less.
- 41.3 Add 5 mL of 15.6 M  $\text{HNO}_3$  and 3 to 4 drops of 28 M HF and heat the solution below its boiling point. Watch glasses or platinum lids are recommended to avoid spattering.
- 41.4 Add additional amounts of  $\text{HNO}_3$  and HF acids until the sample dissolves (see Note 8).
- NOTE 8—The sealed-tube technique described in USAEC Document LA-4622, 1971, p. 5, is an alternative test method which may be used to advantage for the dissolution of some samples.
- 41.5 Evaporate the solution just to dryness, but do not fume intensely to dryness.
- 41.6 Dropwise add 0.5 mL of formic acid. Heat the solution at moderate heat until the vigorous reaction subsides and gases are no longer evolved.

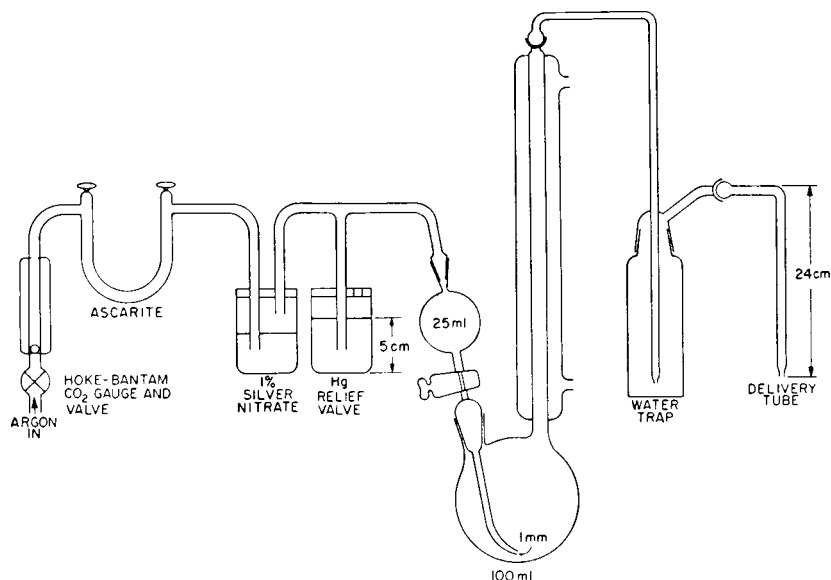


FIG. 4 Sulfur Distillation Apparatus

NOTE 9—The reduction of  $\text{HNO}_3$  by formic acid is vigorous. Keep the dish or beaker covered with a watch glass between additions of formic acid.

41.7 Rinse the cover glass with water. Add 0.5 mL of formic acid and slowly evaporate the rinse and sample solution to dryness.

NOTE 10—Nitrate must be completely removed because it reacts explosively with the reducing acid.

41.8 Dissolve the residue in a minimum volume of 3 M HCl and dilute to approximately 5 mL with water. Heat to just below the boiling point and add 20 drops of hydroxylamine solution (Pu-III, blue, is formed).

41.9 Add 30 mL of water to the trap of the distillation apparatus (Fig. 5) and insert the trap tube.

41.10 Pipet 10.0 mL of 4 % zinc acetate solution into a 50-mL glass-stoppered graduated cylinder, dilute to 35 mL with water, and position the cylinder so the end of the delivery tube is immersed in the solution.

41.11 Transfer the sample solution (41.8) with a minimum of water rinses to the distillation flask and insert the reducing-acid delivery tube.

41.12 Add 15 mL of the reducing acid mixture and 10 mL of 12 M HCl to the delivery bulb. Insert the argon sweep gas tube and start the flow of the reducing acid mixture to the distillation flask.

41.13 Adjust the flow rate of argon to 100  $\text{cm}^3/\text{min}$ ; then turn on the heating mantle and boil the solution for 35 min.

41.14 Disconnect the distillate delivery tube, and rinse it with 2.00 mL of 3 M HCl followed by approximately 2 mL of water, collecting these rinses in the zinc acetate solution. Rinse zinc sulfide (ZnS) formed inside the tube into the zinc acetate solution.

41.15 Pipet 1.00 mL of 1 % *p*-phenylenediamine into the solution and mix rapidly by swirling. Pipet 1.00 mL of 2 % ferric chloride solution and again mix rapidly.

NOTE 11—Rapid mixing after each reagent addition prevents formation of a brown reduction product that interferes with the spectrophotometric measurement.

41.16 Dilute to 50 mL with water, stopper the cylinder, mix the solution, and let stand 1 h.

41.17 Measure the absorbance within 10 min at a wavelength of 595 nm versus a reagent reference.

## 42. Calculation

42.1 Calculate the sulfur content as follows:

$$S, \mu\text{g/g} = (S - B)/W \quad (7)$$

where:

- $S$  = micrograms of sulfur in sample,
- $B$  = micrograms of sulfur in blank, and
- $W$  = grams of sample.

## 43. Precision and Bias

43.1 The relative standard deviations in 0.1-g samples are 6 to 3 % for the range from 50 to 600  $\mu\text{g/g}$  and in 0.5-g samples are 12 to 5 % for the range from 10 to 20  $\mu\text{g/g}$ .

## MOISTURE BY THE COULOMETRIC, ELECTROLYTIC MOISTURE ANALYZER


### 44. Scope

44.1 This test method covers the determination of moisture in nuclear-grade mixed oxides of uranium and plutonium (U,Pu) $\text{O}_2$ . Detection limits are as low as 10  $\mu\text{g}$ .

### 45. Summary of Test Method

45.1 The sample is heated in an oven (up to 400°C) to drive off any water. The moisture is carried from the oven into the electrolytic cell by a flowing stream of *dry* nitrogen. Two parallel platinum wires wound in a helix are attached to the inner surface of the tube, the wall of which is evenly coated with phosphorous pentoxide (a strong desiccant that becomes electrically conductive when wet). A potential applied to the wires produces a measurable electrolysis current when moisture wets the desiccant. Electrolysis of the water continuously regenerates the cell enabling it to accept additional water.

45.2 Precautions must be taken to prevent interference from the following sources: Hydrogen fluoride will cause permanent damage to the cell and sample system and should not be run under any conditions. Corrosive acidic gases such as chlorine and hydrogen chloride will corrode the instrument. Entrained liquids and solids can cause cell failure and should be prevented from entering the gas stream. Ammonia and other basic materials react with the acidic cell coating and render the cell unresponsive. Hydrogen, and to a lesser extent, oxygen or air, may cause a high reading due to recombination in the cell, or in the case of hydrogen due to reaction with oxide coating of the sample boat to produce water. Alcohols and glycols, particularly the more volatile ones, respond like water and therefore must not be present.

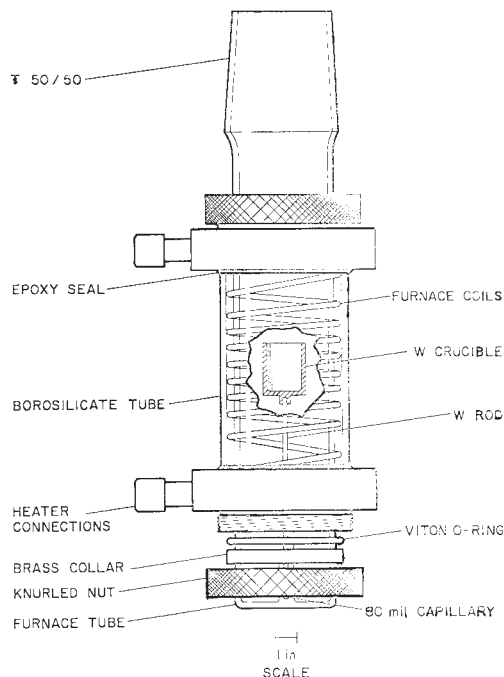

**FIG. 5 Induction Furnace**



C 698

## 46. Apparatus

46.1 *Moisture Analyzer*,<sup>14</sup> for solids, with a quartz-glass oven, capable of being heated from ambient temperatures to 1000°C. The assembly is to include an electrolytic cell, flow meter, range from 30 to 140 cm<sup>3</sup>/min of air, and a dryer assembly.

46.2 *Balance*,<sup>15</sup> for weighing samples in the range from 1 to 100 mg.

46.3 *Nitrogen Gas Cylinder*, with a pressure regulator, a flowmeter, and a drying tower.

## 47. Reagents

47.1 *Barium Chloride Dihydrate* (BaCl<sub>2</sub>·2 H<sub>2</sub>O).

## 48. Operation

48.1 Turn the main power switch ON.

48.2 Adjust nitrogen gas pressure to 41.4 kPa (6 psi) and the flow rate to 50 mL/min measured at the exit of the apparatus.

48.3 Weigh the sample into a small, dry aluminum boat (Note 12) and insert it into the instrument oven as follows.

NOTE 12—For samples that have been reduced in a hydrogen atmosphere and thus contain excess hydrogen, the use of a platinum boat in place of the aluminum tube and nickel boat will minimize any interference due to the hydrogen.

48.4 Open the top of the analyzer and remove the TFE-fluorocarbon plug. Do not touch with gloves.

48.5 With forceps pull the nickel boat one third of the way out of the tube and place the aluminum boat and sample inside the nickel boat. Then reposition the nickel boat near the center of the heating coils.

48.6 Replace the TFE-fluorocarbon plug and close the lid of the analyzer.

48.7 Reset the counter to 0 µg.

48.8 Set the timer at 1 h.

48.9 Set the temperature at 400° C. This will activate the analyzer and start the heating cycle.

48.10 When the preset temperature has been reached and the counter ceases counting, record the reading, *S*.

## 49. Standardization

49.1 Determine the blank by processing dry, empty aluminum boats in accordance with 48.4 through 48.10 until constant values are obtained.

49.2 Weigh and analyze replicate 5-mg samples of BaCl<sub>2</sub>·2 H<sub>2</sub>O until consistent results are obtained. Sodium tungstate dihydrate (NaWO<sub>4</sub>·2 H<sub>2</sub>O) may also be used for calibration.

## 50. Calculation

50.1 Calculate the moisture recovery, *Z*, for the standard as follows:

$$Z = (A - B) / 147.2Y \quad (8)$$

<sup>14</sup> A CEC Solids Moisture Analyzer of Type 26-321A-MA, available from DuPont Instruments, Inc., S. Shamrock Ave., Monrovia, CA 91016, or equivalent, has been found satisfactory.

<sup>15</sup> A Cahn Electrobalance, or equivalent, available from Cahn Div., Ventrone Instruments Corp., Paramount, CA, has been found satisfactory.

where:

*A* = micrograms of moisture on counter when standard is tested,

*B* = micrograms of moisture on counter from blank, and

*Y* = milligrams of BaCl<sub>2</sub>·2 H<sub>2</sub>O. Each milligram of BaCl<sub>2</sub>·2 H<sub>2</sub>O contains 112.2 µg of water.

50.2 Calculate the moisture in the sample as follows:

$$\text{Moisture, } \mu\text{g/g} = (S - B) / WZ \quad (9)$$

where:

*S* = micrograms of moisture on counter when sample is tested,

*B* = micrograms of moisture on counter from blank,

*W* = grams of sample, and

*Z* = recovery of moisture from standard.

## 51. Precision and Bias

51.1 The relative standard deviation for moisture in a concentration range of 100 µg/g is approximately 2 % but increases to 10 % at the 20 µg/g level.

## ISOTOPIC COMPOSITION BY MASS SPECTROMETRY

(This test method was discontinued in 1980 and replaced by Sections 106 to 114.)

## RARE EARTHS BY COPPER SPARK SPECTROSCOPY

## 52. Scope

52.1 This test method covers the determination of rare earths in uranium-plutonium dioxide over the range from 10 to 200 µg/g.

## 53. Summary of Test Method

53.1 The general principles of emission spectrographic analysis are given in an ASTM publication (11). Determination of rare earth content requires their separation from uranium and plutonium by solvent extraction followed by copper-spark spectrographic measurement (12, 13).

## 54. Apparatus

54.1 *Spectrograph*— Commercially available equipment with reciprocal dispersion of approximately 2.5 Å/mm (second order). A direct-reading spectrograph of comparable quality may be substituted for the equipment listed, in which case the directions given by the manufacturer should be followed rather than those given in the succeeding steps of this procedure. The excitation stand must be mounted in a glove box. Power controls must be able to supply the conditions called for in 57.4.

54.2 *Microdensitometer* with a precision of ±1.0 % for transmittances between 5 and 90 %.

54.3 *Electrodes*—Electrolytic copper, 6.4 mm (¼ in.) in diameter by 38.1 mm (1.5 in.) long.

54.4 *Magnetic Stirrer*.