



SLOVENSKI STANDARD SIST EN ISO 6507-2:1998

01-junij-1998

Kovinski materiali - Preskus trdote po Vickersu - 2. del: Preverjanje naprav za preskušanje (ISO 6507-2:1997)

Metallic materials - Vickers hardness test - Part 2: Verification of testing machines (ISO 6507-2:1997)

Metallische Werkstoffe - Härteprüfung nach Vickers - Teil 2: Prüfung der Prüfmaschinen (ISO 6507-2:1997)

Matériaux métalliques - Essai de dureté Vickers - Partie 2: Vérification des machines d'essai (ISO 6507-2:1997)

iTeh STANDARD PREVIEW
(standards.iteh.ai)
<https://standards.iteh.ai/catalog/standards/sist/b91de086-7b12-45e1-a3ca-ccc4993234fb/sist-en-iso-6507-2-1998>

Ta slovenski standard je istoveten z: EN ISO 6507-2:1997

ICS:

77.040.10 Mehansko preskušanje kovin Mechanical testing of metals

SIST EN ISO 6507-2:1998

en

iTeh STANDARD PREVIEW
(standards.iteh.ai)

[SIST EN ISO 6507-2:1998](#)

<https://standards.iteh.ai/catalog/standards/sist/b91de086-7b12-45e1-a3ca-ccc499323f4b/sist-en-iso-6507-2-1998>

EUROPEAN STANDARD
NORME EUROPÉENNE
EUROPÄISCHE NORM

EN ISO 6507-2

November 1997

ICS 77.040.10

Descriptors: see ISO document

English version

Metallic materials - Vickers hardness test - Part 2: Verification of testing machines (ISO 6507-2:1997)

Matériaux métalliques - Essai de dureté Vickers - Partie 2:
Vérification des machines d'essai (ISO 6507-2:1997)

This European Standard was approved by CEN on 22 October 1997.

CEN members are bound to comply with the CEN/CENELEC Internal Regulations which stipulate the conditions for giving this European Standard the status of a national standard without any alteration. Up-to-date lists and bibliographical references concerning such national standards may be obtained on application to the Central Secretariat or to any CEN member.

This European Standard exists in three official versions (English, French, German). A version in any other language made by translation under the responsibility of a CEN member into its own language and notified to the Central Secretariat has the same status as the official versions.

CEN members are the national standards bodies of Austria, Belgium, Czech Republic, Denmark, Finland, France, Germany, Greece, Iceland, Ireland, Italy, Luxembourg, Netherlands, Norway, Portugal, Spain, Sweden, Switzerland and United Kingdom.

[SIST EN ISO 6507-2:1998](https://standards.iteh.ai/catalog/standards/sist/b91de086-7b12-45e1-a3ca-ccc499323f4b/sist-en-iso-6507-2-1998)

<https://standards.iteh.ai/catalog/standards/sist/b91de086-7b12-45e1-a3ca-ccc499323f4b/sist-en-iso-6507-2-1998>



EUROPEAN COMMITTEE FOR STANDARDIZATION
COMITÉ EUROPÉEN DE NORMALISATION
EUROPÄISCHES KOMITEE FÜR NORMUNG

Central Secretariat: rue de Stassart, 36 B-1050 Brussels

Foreword

The text of the International Standard ISO 6507-2:1997 has been prepared by Technical Committee ISO/TC 164 "Mechanical testing of metals" in collaboration with Technical Committee ECISS/TC 1 "Steels - Mechanical and physical tests", the secretariat of which is held by AFNOR.

This European Standard shall be given the status of a national standard, either by publication of an identical text or by endorsement, at the latest by May 1998, and conflicting national standards shall be withdrawn at the latest by May 1998.

According to the CEN/CENELEC Internal Regulations, the national standards organizations of the following countries are bound to implement this European Standard: Austria, Belgium, Czech Republic, Denmark, Finland, France, Germany, Greece, Iceland, Ireland, Italy, Luxembourg, Netherlands, Norway, Portugal, Spain, Sweden, Switzerland and the United Kingdom.

Endorsement notice

The text of the International Standard ISO 6507-2:1997 was approved by CEN as a European Standard without any modification.

iTeh STANDARD PREVIEW
(standards.iteh.ai)

[SIST EN ISO 6507-2:1998](https://standards.iteh.ai/catalog/standards/sist/b91de086-7b12-45e1-a3ca-ccc499323f4b/sist-en-iso-6507-2-1998)

<https://standards.iteh.ai/catalog/standards/sist/b91de086-7b12-45e1-a3ca-ccc499323f4b/sist-en-iso-6507-2-1998>



INTERNATIONAL STANDARD

ISO
6507-2

Second edition
1997-11-15

Metallic materials — Vickers hardness test —

Part 2: Verification of testing machines

*Matériaux métalliques — Essai de dureté Vickers —
Partie 2: Vérification des machines d'essai*
(standards.iteh.ai)

[SIST EN ISO 6507-2:1998](https://standards.iteh.ai/catalog/standards/sist/b91de086-7b12-45e1-a3ca-ccc499323f4b/sist-en-iso-6507-2-1998)

<https://standards.iteh.ai/catalog/standards/sist/b91de086-7b12-45e1-a3ca-ccc499323f4b/sist-en-iso-6507-2-1998>



Reference number
ISO 6507-2:1997(E)

ISO 6507-2:1997(E)

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

International Standard ISO 6507-2 was prepared by Technical Committee ISO/TC 164, *Mechanical testing of metals*, Subcommittee SC 3, *Hardness testing*.

This second edition of ISO 6507-2 cancels and replaces ISO 146:1984 and ISO 146-2:1993 as follows:

- Combination of the two different International Standards for the verification of the hardness testing machines (ISO 146:1989 and ISO 146-2:1993) into this part of ISO 6507.
- Addition of a new table (table 3) for the estimation capability and the maximum permissible error of the measuring device.
- Changing of the values for the repeatability of the hardness testing machine in table 4.
- Addition of a new clause 6 concerning the intervals between the verifications.
- Addition of a new annex A "Example of a method for an indirect verification of the measuring device" (using a reference indentation).
- Addition of a new annex B "Notes on diamond indenters".

ISO 6507 consists of the following parts, under the general title *Metallic materials — Vickers hardness test*:

- *Part 1: Test method*
- *Part 2: Verification of testing machines*
- *Part 3: Calibration of reference blocks*

Annexes A and B of this part of ISO 6507 are for information only.

© ISO 1997

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from the publisher.

International Organization for Standardization
Case postale 56 • CH-1211 Genève 20 • Switzerland
Internet central@iso.ch
X.400 c=ch; a=400net; p=iso; o=isocs; s=central

Printed in Switzerland

Metallic materials — Vickers hardness test —

Part 2: Verification of testing machines

1 Scope

This part of ISO 6507 specifies a method of verification of testing machines for determining Vickers hardness in accordance with ISO 6507-1.

It describes a direct verification method for checking the main functions of the machine, and an indirect verification method suitable for the overall checking of the machine. The indirect verification method may be used on its own for periodic routine checking of the machine in service.

If a testing machine is also to be used for other methods of hardness testing, it is essential that it is verified independently for each method.

Portable hardness testing machines shall comply with all the requirements of this part of ISO 6507, but the word "relocation" in 6.1a) does not apply.

The force values in this part of ISO 6507 were calculated from kilogram force values. They were introduced before the SI-system was adopted. It was decided to keep the values based on the old units for this edition, but for the next revision it will be necessary to consider the advantage of introducing rounded values of test force and the consequence on the hardness scales.

2 Normative references

The following standards contain provisions which, through reference in this text, constitute provisions of this part of ISO 6507. At the time of publication, the editions indicated were valid. All standards are subject to revision, and parties to agreements based on this part of ISO 6507 are encouraged to investigate the possibility of applying the most recent editions of the standards indicated below. Members of IEC and ISO maintain registers of currently valid International Standards.

ISO 376:—¹⁾, *Metallic materials — Calibration of force-proving instruments used for the verification of uniaxial testing machines.*

ISO 3878:1983, *Hardmetals — Vickers hardness test.*

ISO 6507-1:1997, *Metallic materials — Vickers hardness test — Part 1: Test method.*

ISO 6507-3:1997, *Metallic materials — Vickers hardness test — Part 3: Calibration of reference blocks.*

1) To be published. (Revision of ISO 376:1987)

3 General conditions

Before a Vickers hardness testing machine is verified, it shall be checked to ensure that

- a) the machine is properly set up;
- b) the plunger holding the indenter is capable of sliding in its guide;
- c) the indenter-holder is firmly mounted in the plunger;
- d) the test force can be applied and removed without shock or vibration and in such a manner that the readings are not influenced;
- e) if the measuring device is integral with the machine
 - 1) the change from removing the test force to measuring mode does not influence the readings,
 - 2) illumination does not affect the readings,
 - 3) the centre of the indentation is in the centre of the field of view, if necessary.

The illumination device of the measuring microscope shall produce uniform lighting of the whole observed field and maximum contrast between the indentation and the surrounding surface.

4 Direct verification

Direct verification should be carried out at a temperature of (23 ± 5) °C. If the verification is made outside this temperature range, this shall be reported in the verification report.

The instruments used for verification shall have a certified traceability using the International System of Units (SI).

[SIST EN ISO 6507-2:1998](https://standards.iteh.ai/catalog/standards/sist/b91de086-7b12-45e1-a3ca-ccc499323f4b/sist-en-iso-6507-2-1998)

Direct verification involves <https://standards.iteh.ai/catalog/standards/sist/b91de086-7b12-45e1-a3ca-ccc499323f4b/sist-en-iso-6507-2-1998>

- a) verification of the test force;
- b) verification of the indenter;
- c) verification of the measuring device;
- d) verification of the testing cycle.

4.1 Verification of the test force

4.1.1 Each test force used within the working range of the testing machine shall be measured. Whenever applicable, this shall be done at not less than three positions of the plunger uniformly spaced throughout its range of movement during testing.

4.1.2 The test force shall be measured by one of the following two methods:

- a) by means of an elastic proving device in accordance with ISO 376, class 1,
- b) by balancing against a force, accurate to $\pm 0,2$ %, applied by means of standardized masses with mechanical advantage.

4.1.3 Three readings shall be taken for each test force at each position of the plunger. Immediately before each reading is taken, the plunger shall have been moved in the same direction as during testing.

4.1.4 Each measurement for the force shall be within the tolerances of the nominal value of the test force, as given in table 1.

Table 1

Ranges of test force, F N	Tolerances %
$F \geq 1,961$	$\pm 1,0$
$0,098\ 07 \leq F < 1,961$	$\pm 1,5$

4.2 Verification of the indenter

4.2.1 The four faces of the square-based diamond pyramid shall be polished and free from surface defects.

4.2.2 The verification of the shape of the indenter can be made by direct measurement or by measurement of its projection on a screen.

4.2.3 The angle between the opposite faces at the vertex of the diamond pyramid shall be $136^\circ \pm 0,5^\circ$ (see figure 1).

4.2.4 The angle between the axis of the diamond pyramid and the axis of the indenter-holder (normal to the seating surface) shall be less than $0,5^\circ$. The four faces shall meet in a point; the maximum permissible length of the line of conjunction between opposite faces is given in table 2 (see also figure 2).

Independent of the intervals between the direct verifications of the testing machines, the indenter shall be verified at intervals not exceeding two years.

<https://standards.iteh.ai/catalog/standards/sist/b91de086-7b12-45e1-a3ca-ccc499323f4b/sist-en-iso-6507-2-1998>

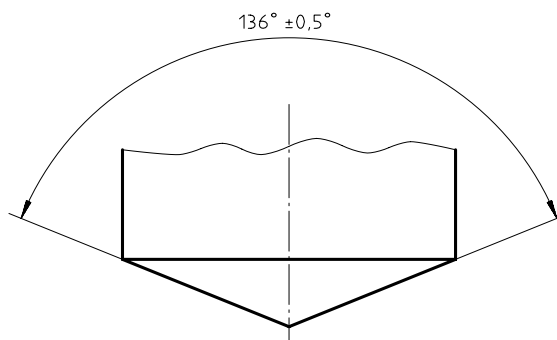


Figure 1 — Angle of the diamond pyramid