



Standard Test Method for Thermal Diffusivity of Carbon and Graphite by a Thermal Pulse Method¹

This standard is issued under the fixed designation C 714; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

1. Scope

1.1 This test method covers the determination of the thermal diffusivity of carbons and graphite to $\pm 5\%$ at temperatures up to 500°C. It requires only a small easily fabricated specimen. Thermal diffusivity values in the range from 0.04 to 2.0 cm²/s are readily measurable by this test method; however, for the reason outlined in Section 5, for materials outside this range this test method may require modification.

1.2 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

2. Summary of Test Method

2.1 A high-intensity short-duration thermal pulse from a flash lamp is absorbed on the front surface of a specimen; and the rear surface temperature change as a function of time is observed on an oscilloscope. The pulse raises the average temperature of the specimen only a few degrees above its initial value. The ambient temperature of the specimen is controlled by a furnace or cryostat. Thermal diffusivity is calculated from the specimen thickness and the time required for the temperature of the back surface to rise to one half of its maximum value (1).²

2.2 The critical factors in this test method are:

2.2.1 $\tau/t_{1/2}$ must be 0.02 or less. τ is the pulse time as defined in Fig. 1 and $t_{1/2}$ is the time for the rear surface temperature to rise to one half of its maximum value (see Fig. 2).

2.2.2 Heat losses from the specimen via radiation, convection, or conduction to the specimen holder must be small. Whether or not this condition is violated can be determined experimentally from the oscilloscope trace, an example of which is shown in Fig. 2. If $\Delta T(10 t_{1/2})/\Delta T(t_{1/2}) > 1.98$, the heat losses are assumed to be zero.

2.2.3 The oscilloscope trace must be such that ΔT_{\max} , $\Delta T(10 t_{1/2})$, and $t_{1/2}$ can be determined to $\pm 2\%$.

2.2.4 The other conditions are less critical, and the experimenter is left to his discretion.

3. Significance and Use

3.1 Sulfur, even in very low concentrations, is of concern in a nuclear reactor because of potential corrosion of metallic components. This test method has the sensitivity to analyze very low sulfur contents in graphite using very small samples.

3.2 This test method can be used to characterize graphite for design purposes.

4. Apparatus

4.1 The essential features of the apparatus are shown in Fig. 3. The window may be any material that is transparent to the flash source. The specimen holder should be a ceramic or other material whose thermal conductivity is low relative to that of the sample.

4.2 *Thermocouple*, used to monitor the transient temperature response of the rear surface of the specimen. The wire ends should be prepared to minimize heat losses from the specimen to the thermocouple wires (that is, by grinding to points or clipping) and attached in a manner that prevents penetration into the specimen. They are separated by about 1 mm so that the electrical circuit of the thermocouple is completed through the specimen.

4.3 *Oscilloscope*, with calibrated sweep speeds that can be varied from 0.1 ms/cm to 0.5 s/cm or more. The vertical amplifier section of the oscilloscope should have a frequency response in the range from 0.06 to 10 kHz to be perfectly insensitive to frequency in the range of interest described in Section 5. A minimum vertical deflection sensitivity of 1 C/cm is recommended. The cathode-ray tube should have a usable viewing area of at least 40 by 100 mm. A camera is used to photograph the oscilloscope trace.

4.4 *Flash Tube*—The experimenter has considerable latitude in his choice of flash tube. A typical 1000-J unit raises the specimen temperature from 1 to 3°C. The power supply for such a unit might consist of a 125- μ F capacitor bank charged to 4000 V; discharge time would be about 1 ms. Either an external

¹ This test method is under the jurisdiction of ASTM Committee D02 on Petroleum Products and Lubricants and is the direct responsibility of Subcommittee D02.F on Manufactured Carbon and Graphite Products.

Current edition approved July 26, 1985. Published September 1985. Originally published as C 714 – 72. Last previous edition C 714 – 72.

² The boldface numbers in parentheses refer to the list of references at the end of this test method.

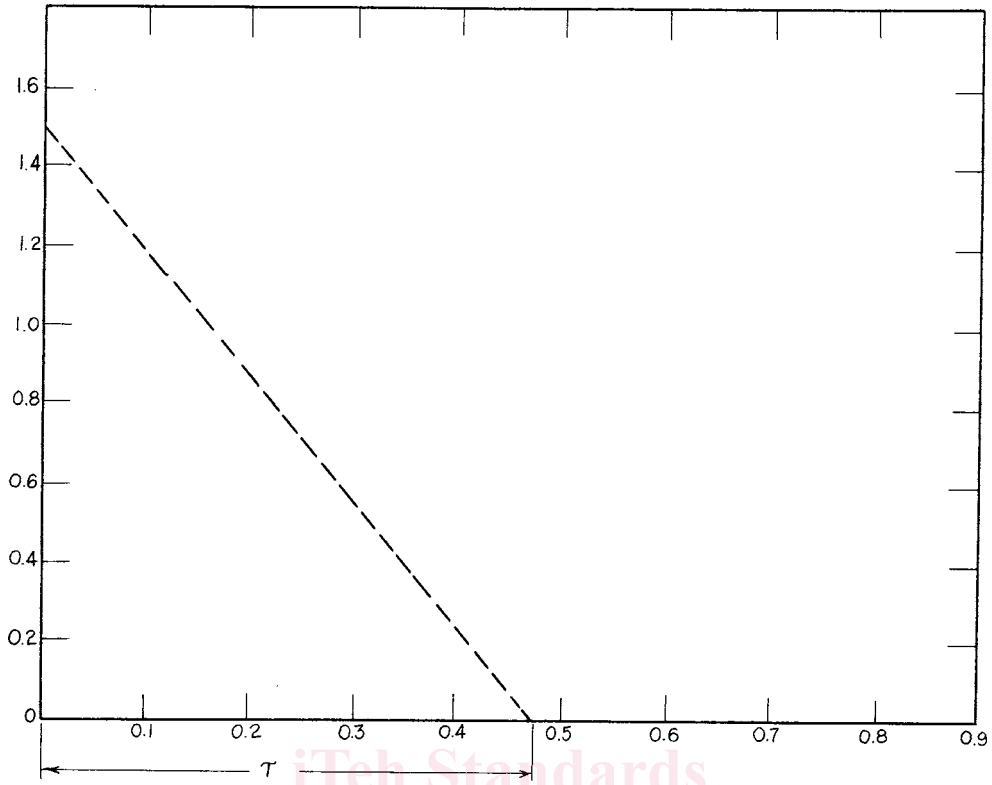


FIG. 1 Flash Tube Response

iteh Standards
 (https://standards.iteh.ai)
 Document Preview

ASTM C714-85(2000)

https://standards.iteh.ai/catalog/standards/sist/7454b87-160-4c6c-a605-d04106e63109/astm-c714-852000

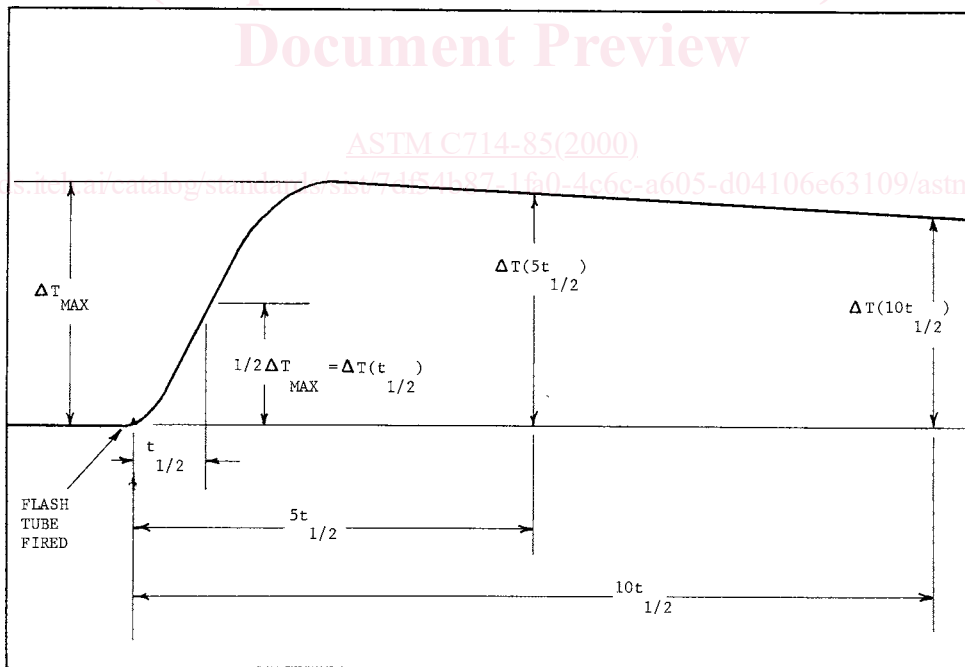


FIG. 2 Example of Oscilloscope Trace Showing Parameters Used to Calculate Thermal Diffusivity