

INTERNATIONAL STANDARD

NORME INTERNATIONALE



Medical electrical equipment –

Part 2-71: Particular requirements for the basic safety and essential performance of functional near-infrared spectroscopy (NIRS) equipment

Appareils électromédicaux – [IEC 80601-2-71:2015](https://standards.iteh.ai/catalog/standards/sist/60c6e697-3bb7-4e0c-8877-e0c6e6973bb7/iec-80601-2-71-2015)

Partie 2-71: Exigences particulières pour la sécurité de base et les performances essentielles des appareils de spectroscopie dans le proche infrarouge (NIRS) fonctionnelle



THIS PUBLICATION IS COPYRIGHT PROTECTED

Copyright © 2015 IEC, Geneva, Switzerland

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either IEC or IEC's member National Committee in the country of the requester. If you have any questions about IEC copyright or have an enquiry about obtaining additional rights to this publication, please contact the address below or your local IEC member National Committee for further information.

Droits de reproduction réservés. Sauf indication contraire, aucune partie de cette publication ne peut être reproduite ni utilisée sous quelque forme que ce soit et par aucun procédé, électronique ou mécanique, y compris la photocopie et les microfilms, sans l'accord écrit de l'IEC ou du Comité national de l'IEC du pays du demandeur. Si vous avez des questions sur le copyright de l'IEC ou si vous désirez obtenir des droits supplémentaires sur cette publication, utilisez les coordonnées ci-après ou contactez le Comité national de l'IEC de votre pays de résidence.

IEC Central Office
3, rue de Varembe
CH-1211 Geneva 20
Switzerland

Tel.: +41 22 919 02 11
info@iec.ch
www.iec.ch

About the IEC

The International Electrotechnical Commission (IEC) is the leading global organization that prepares and publishes International Standards for all electrical, electronic and related technologies.

About IEC publications

The technical content of IEC publications is kept under constant review by the IEC. Please make sure that you have the latest edition, a corrigenda or an amendment might have been published.

IEC Catalogue - webstore.iec.ch/catalogue

The stand-alone application for consulting the entire bibliographical information on IEC International Standards, Technical Specifications, Technical Reports and other documents. Available for PC, Mac OS, Android Tablets and iPad.

IEC publications search - webstore.iec.ch/advsearchform

The advanced search enables to find IEC publications by a variety of criteria (reference number, text, technical committee,...). It also gives information on projects, replaced and withdrawn publications.

IEC Just Published - webstore.iec.ch/justpublished

Stay up to date on all new IEC publications. Just Published details all new publications released. Available online and also once a month by email.

Electropedia - www.electropedia.org

The world's leading online dictionary of electronic and electrical terms containing 21 000 terms and definitions in English and French, with equivalent terms in 16 additional languages. Also known as the International Electrotechnical Vocabulary (IEV) online.

IEC Glossary - std.iec.ch/glossary

67 000 electrotechnical terminology entries in English and French extracted from the Terms and Definitions clause of IEC publications issued since 2002. Some entries have been collected from earlier publications of IEC TC 37, 77, 86 and CISPR 71-2015

IEC Customer Service Centre - webstore.iec.ch/csc

If you wish to give us your feedback on this publication or need further assistance, please contact the Customer Service Centre: sales@iec.ch.

A propos de l'IEC

La Commission Electrotechnique Internationale (IEC) est la première organisation mondiale qui élabore et publie des Normes internationales pour tout ce qui a trait à l'électricité, à l'électronique et aux technologies apparentées.

A propos des publications IEC

Le contenu technique des publications IEC est constamment revu. Veuillez vous assurer que vous possédez l'édition la plus récente, un corrigendum ou amendement peut avoir été publié.

Catalogue IEC - webstore.iec.ch/catalogue

Application autonome pour consulter tous les renseignements bibliographiques sur les Normes internationales, Spécifications techniques, Rapports techniques et autres documents de l'IEC. Disponible pour PC, Mac OS, tablettes Android et iPad.

Recherche de publications IEC - webstore.iec.ch/advsearchform

La recherche avancée permet de trouver des publications IEC en utilisant différents critères (numéro de référence, texte, comité d'études,...). Elle donne aussi des informations sur les projets et les publications remplacées ou retirées.

IEC Just Published - webstore.iec.ch/justpublished

Restez informé sur les nouvelles publications IEC. Just Published détaille les nouvelles publications parues. Disponible en ligne et aussi une fois par mois par email.

Electropedia - www.electropedia.org

Le premier dictionnaire en ligne de termes électroniques et électriques. Il contient 21 000 termes et définitions en anglais et en français, ainsi que les termes équivalents dans 16 langues additionnelles. Egalement appelé Vocabulaire Electrotechnique International (IEV) en ligne.

Glossaire IEC - std.iec.ch/glossary

67 000 entrées terminologiques électrotechniques, en anglais et en français, extraites des articles Termes et Définitions des publications IEC parues depuis 2002. Plus certaines entrées antérieures extraites des publications des CE 37, 77, 86 et CISPR de l'IEC.

Service Clients - webstore.iec.ch/csc

Si vous désirez nous donner des commentaires sur cette publication ou si vous avez des questions contactez-nous: sales@iec.ch.



IEC 80601-2-71

Edition 1.0 2015-06

INTERNATIONAL STANDARD

NORME INTERNATIONALE



Medical electrical equipment –
Part 2-71: Particular requirements for the basic safety and essential
performance of functional near-infrared spectroscopy (NIRS) equipment

Appareils électromédicaux –
Partie 2-71: Exigences particulières pour la sécurité de base et les
performances essentielles des appareils de spectroscopie dans le proche
infrarouge (NIRS) fonctionnelle

INTERNATIONAL
ELECTROTECHNICAL
COMMISSION

COMMISSION
ELECTROTECHNIQUE
INTERNATIONALE

ICS 11.040.55

ISBN 978-2-8322-6318-1

Warning! Make sure that you obtained this publication from an authorized distributor.
Attention! Veuillez vous assurer que vous avez obtenu cette publication via un distributeur agréé.

CONTENTS

FOREWORD.....	4
INTRODUCTION.....	6
201.1 Scope, object and related standards	7
201.2 Normative references.....	9
201.3 Terms and definitions.....	9
201.4 General requirements	12
201.5 General requirements for testing ME EQUIPMENT	12
201.6 Classification of ME EQUIPMENT and ME SYSTEMS	12
201.7 ME EQUIPMENT identification, marking and documents	12
201.8 Protection against electrical HAZARDS from ME EQUIPMENT.....	12
201.9 Protection against mechanical HAZARDS of ME EQUIPMENT and ME SYSTEMS	13
201.10 Protection against unwanted and excessive radiation HAZARDS	13
201.11 Protection against excessive temperatures and other hazards	13
201.12 ACCURACY of controls and instruments and protection against hazardous outputs	13
201.13 HAZARDOUS SITUATIONS and fault conditions for ME EQUIPMENT	21
201.14 PROGRAMMABLE ELECTRICAL MEDICAL SYSTEMS (PEMS).....	21
201.15 Construction of ME EQUIPMENT	21
201.16 ME SYSTEMS	21
201.17 Electromagnetic compatibility of ME EQUIPMENT and ME SYSTEMS	21
Annexes	22
Annex C (informative) Guide to marking and labelling requirements for ME EQUIPMENT and ME SYSTEMS.....	22
Annex AA (informative) Particular guidance and rationale.....	23
Annex BB (normative) Evaluating ME EQUIPMENT performance using the FUNCTIONAL NIRS PHANTOM.....	25
Annex CC (informative) Reference to the essential principles	34
Bibliography.....	36
Index of defined terms	37
Figure 201.101 – FULL WIDTH AT HALF MAXIMUM of spectral power distribution	10
Figure 201.102 – Measurement of AVERAGE OPTICAL POWER	14
Figure 201.103 – Measurement of PEAK WAVELENGTH and FWHM.....	15
Figure 201.104 – Measurement of signal stability.....	16
Figure 201.105 – Measurement of RESPONSE TIME	17
Figure 201.106 – Rise time and fall time in RESPONSE TIME	18
Figure 201.107 – Measurement of signal-to-noise ratio.....	19
Figure 201.108 – Measurement of SIGNAL CROSS-TALK.....	21
Figure 201.BB.1 – The FUNCTIONAL NIRS PHANTOM in two states with different detected light intensities.....	28
Figure BB.2 – FUNCTIONAL NIRS PHANTOM measurement using the reference system.....	29
Figure BB.3 – FUNCTIONAL NIRS PHANTOM measurement using the ME EQUIPMENT to be evaluated.....	29

Figure BB.4 – Schematic for measurement of OPTICAL LOSS	32
Table 201.101 – Performance tests employing the FUNCTIONAL NIRS PHANTOM or attenuator and the required OPTICAL LOSS.....	13
Table 201.C.101 – Marking on the outside of FUNCTIONAL NIRS EQUIPMENT or their parts.....	22
Table 201.C.102 – ACCOMPANYING DOCUMENTS, instructions for use of FUNCTIONAL NIRS EQUIPMENT	22
Table CC.1 – Correspondence between this particular standard and the essential principles	34

iTeh STANDARD PREVIEW **(standards.iteh.ai)**

[IEC 80601-2-71:2015](https://standards.iteh.ai/catalog/standards/sist/ac26ba99-bc9a-4f1c-8877-e0c6e6973bb/iec-80601-2-71-2015)

<https://standards.iteh.ai/catalog/standards/sist/ac26ba99-bc9a-4f1c-8877-e0c6e6973bb/iec-80601-2-71-2015>

INTERNATIONAL ELECTROTECHNICAL COMMISSION

MEDICAL ELECTRICAL EQUIPMENT –

Part 2-71: Particular requirements for the basic safety and essential performance of functional near-infrared spectroscopy (NIRS) equipment

FOREWORD

- 1) The International Electrotechnical Commission (IEC) is a worldwide organization for standardization comprising all national electrotechnical committees (IEC National Committees). The object of IEC is to promote international co-operation on all questions concerning standardization in the electrical and electronic fields. To this end and in addition to other activities, IEC publishes International Standards, Technical Specifications, Technical Reports, Publicly Available Specifications (PAS) and Guides (hereafter referred to as "IEC Publication(s)"). Their preparation is entrusted to technical committees; any IEC National Committee interested in the subject dealt with may participate in this preparatory work. International, governmental and non-governmental organizations liaising with the IEC also participate in this preparation. IEC collaborates closely with the International Organization for Standardization (ISO) in accordance with conditions determined by agreement between the two organizations.
- 2) The formal decisions or agreements of IEC on technical matters express, as nearly as possible, an international consensus of opinion on the relevant subjects since each technical committee has representation from all interested IEC National Committees.
- 3) IEC Publications have the form of recommendations for international use and are accepted by IEC National Committees in that sense. While all reasonable efforts are made to ensure that the technical content of IEC Publications is accurate, IEC cannot be held responsible for the way in which they are used or for any misinterpretation by any end user.
- 4) In order to promote international uniformity, IEC National Committees undertake to apply IEC Publications transparently to the maximum extent possible in their national and regional publications. Any divergence between any IEC Publication and the corresponding national or regional publication shall be clearly indicated in the latter.
- 5) IEC itself does not provide any attestation of conformity. Independent certification bodies provide conformity assessment services and, in some areas, access to IEC marks of conformity. IEC is not responsible for any services carried out by independent certification bodies.
- 6) All users should ensure that they have the latest edition of this publication.
- 7) No liability shall attach to IEC or its directors, employees, servants or agents including individual experts and members of its technical committees and IEC National Committees for any personal injury, property damage or other damage of any nature whatsoever, whether direct or indirect, or for costs (including legal fees) and expenses arising out of the publication, use of, or reliance upon, this IEC Publication or any other IEC Publications.
- 8) Attention is drawn to the Normative references cited in this publication. Use of the referenced publications is indispensable for the correct application of this publication.
- 9) Attention is drawn to the possibility that some of the elements of this IEC Publication may be the subject of patent rights. IEC shall not be held responsible for identifying any or all such patent rights.

International standard IEC 80601-2-71 has been prepared by a Joint Working Group of IEC subcommittee 62D: Electromedical equipment, of IEC technical committee 62: Electrical equipment in medical practice and ISO subcommittee SC3: Lung ventilators and related equipment, of ISO technical committee 121: Anaesthetic and respiratory equipment.

This publication is published as a double logo standard.

This bilingual version (2018-11) corresponds to the monolingual English version, published in 2015-06.

The text of this particular standard is based on the following documents:

FDIS	Report on voting
62D/1238/FDIS	62D/1261/RVD

Full information on the voting for the approval of this standard can be found in the report on voting indicated in the above table. In ISO, the standard has been approved by 14 P-members out of 14 having cast a vote.

The French version of this standard has not been voted upon.

This publication has been drafted in accordance with the ISO/IEC Directives, Part 2.

In this standard, the following print types are used:

- Requirements and definitions: roman type.
- *Test specifications: italic type.*
- Informative material appearing outside of tables, such as notes, examples and references: in smaller type. Normative text of tables is also in a smaller type.
- TERMS DEFINED IN CLAUSE 3 OF THE GENERAL STANDARD, IN THIS PARTICULAR STANDARD OR AS NOTED: SMALL CAPITALS.

In referring to the structure of this standard, the term

- “clause” means one of the seventeen numbered divisions within the table of contents, inclusive of all subdivisions (e.g. Clause 7 includes subclauses 7.1, 7.2, etc.);
- “subclause” means a numbered subdivision of a clause (e.g. 7.1, 7.2 and 7.2.1 are all subclauses of Clause 7).

References to clauses within this standard are preceded by the term “Clause” followed by the clause number. References to subclauses within this particular standard are by number only.

In this standard, the conjunctive “or” is used as an “inclusive or” so a statement is true if any combination of the conditions is true.

[IEC 80601-2-71:2015](https://standards.iteh.ai/catalog/standards/sist/ac26ba99-bc9a-4f1c-8877-c0cc09150612/iec-80601-2-71-2015)

<https://standards.iteh.ai/catalog/standards/sist/ac26ba99-bc9a-4f1c-8877-c0cc09150612/iec-80601-2-71-2015>

The verbal forms used in this standard conform to usage described in Annex H of the ISO/IEC Directives, Part 2. For the purposes of this standard, the auxiliary verb:

- “shall” means that compliance with a requirement or a test is mandatory for compliance with this standard;
- “should” means that compliance with a requirement or a test is recommended but is not mandatory for compliance with this standard;
- “may” is used to describe a permissible way to achieve compliance with a requirement or test.

An asterisk (*) as the first character of a title or at the beginning of a paragraph or table title indicates that there is guidance or rationale related to that item in Annex AA.

A list of all parts of the IEC 60601 series, published under the general title *Medical electrical equipment*, can be found on the IEC website.

The committee has decided that the contents of this publication will remain unchanged until the stability date indicated on the IEC web site under “<http://webstore.iec.ch>” in the data related to the specific publication. At this date, the publication will be

- reconfirmed,
- withdrawn,
- replaced by a revised edition, or
- amended.

NOTE The attention of National Committees and Member Bodies is drawn to the fact that equipment manufacturers and testing organizations may need a transitional period following publication of a new, amended or revised IEC or ISO publication in which to make products in accordance with the new requirements and to equip themselves for conducting new or revised tests. It is the recommendation of the committees that the content of this publication be adopted for implementation nationally not earlier than 3 years from the date of publication.

INTRODUCTION

The minimum safety requirements specified in this particular standard are considered to provide for a practical degree of safety in the operation of FUNCTIONAL NIRS EQUIPMENT.

The requirements are followed by specifications for the relevant tests.

A "Particular guidance and rationale" text giving some explanatory notes, where appropriate, about the more important requirements is included in Annex AA. It is considered that knowledge of the reasons for these requirements will not only facilitate the proper application of the standard but will, in due course, expedite any revision necessitated by changes in clinical practice or as a result of developments in technology. However, this annex does not form part of the requirements of this standard.

iTeh STANDARD PREVIEW
(standards.iteh.ai)

[IEC 80601-2-71:2015](https://standards.iteh.ai/catalog/standards/sist/ac26ba99-bc9a-4f1c-8877-e0c6e6973bb/iec-80601-2-71-2015)

<https://standards.iteh.ai/catalog/standards/sist/ac26ba99-bc9a-4f1c-8877-e0c6e6973bb/iec-80601-2-71-2015>

MEDICAL ELECTRICAL EQUIPMENT –

Part 2-71: Particular requirements for the basic safety and essential performance of functional near-infrared spectroscopy (NIRS) equipment

201.1 Scope, object and related standards

Clause 1 of the general standard¹ applies, except as follows:

201.1.1 Scope

Replacement:

This International standard applies to the BASIC SAFETY and ESSENTIAL PERFORMANCE of FUNCTIONAL NIRS EQUIPMENT intended to be used by themselves, or as a part of an ME SYSTEM, for the production of FUNCTIONAL NIRS EQUIPMENT output for adjunctive diagnostic purposes, hereinafter referred to as ME EQUIPMENT.

Not included within the scope of this particular standard are:

- a) the part of ME EQUIPMENT, if provided, that measures oxygen saturation of the haemoglobin in the micro vessels (capillaries, arterioles and venules);
- b) near-infrared spectroscopy (NIRS) tissue oximeter equipment, which is not intended for obtaining FUNCTIONAL NIRS EQUIPMENT output;
- c) PULSE OXIMETER EQUIPMENT, which is not intended for obtaining FUNCTIONAL NIRS EQUIPMENT output. The requirements for PULSE OXIMETER EQUIPMENT are found in ISO 80601-2-61.
- d) frequency-domain and time-domain equipment for functional near-infrared spectroscopy, which may require different test procedures than defined herein.
- e) FUNCTIONAL NEAR-INFRARED SPECTROSCOPY EQUIPMENT which measure changes in the concentration of chromophores other than oxy- and deoxy-haemoglobin, which may require different test procedures than defined herein.

201.1.2 OBJECT

Replacement:

The object of this particular standard is to establish particular BASIC SAFETY and ESSENTIAL PERFORMANCE requirements for FUNCTIONAL NIRS EQUIPMENT as defined in 201.3.205.

201.1.3 Collateral standards

Addition:

This particular standard refers to those applicable collateral standards that are listed in Clause 2 of the general standard and Clause 201.2 of this particular standard.

¹ The general standard is IEC 60601-1:2005 + IEC 60601-1:2005/AMD1:2012, *Medical electrical equipment – Part 1: General requirements for basic safety and essential performance*.

IEC 60601-1-3 and IEC 60601-1-10² do not apply. All other published collateral standards in the IEC 60601-1 series apply as published.

201.1.4 Particular standards

Replacement:

In the IEC 60601 series, particular standards may modify, replace or delete requirements contained in the general standard or collateral standards as appropriate for the particular ME EQUIPMENT under consideration, and may add other BASIC SAFETY and ESSENTIAL PERFORMANCE requirements.

A requirement of a particular standard takes priority over the general standard.

For brevity, IEC 60601-1:2005 + IEC 60601-1:2005/AMD1:2012 is referred to in this particular standard as the general standard. Collateral standards are referred to by their document number.

The numbering of clauses and subclauses of this particular standard corresponds to that of the general standard with the prefix “201” (e.g. 201.1 in this standard addresses the content of Clause 1 of the general standard) or applicable collateral standard with the prefix “20x” where x is the final digit(s) of the collateral standard document number (e.g. 202.4 in this particular standard addresses the content of Clause 4 of the IEC 60601-1-2 collateral standard, 203.4 in this particular standard addresses the content of Clause 6 of the IEC 60601-1-3 collateral standard, etc.). The changes to the text of the general standard are specified by the use of the following words:

"Replacement" means that the clause or subclause of the general standard or applicable collateral standard is replaced completely by the text of this particular standard.

"Addition" means that the text of this particular standard is additional to the requirements of the general standard or applicable collateral standard.

"Amendment" means that the clause or subclause of the general standard or applicable collateral standard is amended as indicated by the text of this particular standard.

Subclauses, figures or tables which are additional to those of the general standard are numbered starting from 201.101. However due to the fact that definitions in the general standard are numbered 3.1 through 3.139, additional definitions in this standard are numbered beginning from 201.3.201. Additional annexes are lettered AA, BB, etc., and additional items aa), bb), etc.

Subclauses, figures or tables which are additional to those of a collateral standard are numbered starting from 20x, where “x” is the number of the collateral standard, e.g. 202 for IEC 60601-1-2, 203 for IEC 60601-1-3, etc.

The term "this standard" is used to make reference to the general standard, any applicable collateral standards and this particular standard taken together.

Where there is no corresponding clause or subclause in this particular standard, the clause or subclause of the general standard or applicable collateral standard, although possibly not relevant, applies without modification; where it is intended that any part of the general standard or applicable collateral standard, although possibly relevant, is not to be applied, a statement to that effect is given in this particular standard.

² IEC 60601-1-10, *Medical electrical equipment – Part 1-10: General requirements for basic safety and essential performance – Collateral Standard: Requirements for the development of physiologic closed-loop controllers.*

201.2 Normative references

Clause 2 of the general standard applies, except as follows:

Replacement:

IEC 60601-1-6, *Medical electrical equipment – Part 1-6: General requirements for basic safety and essential performance – Collateral standard: Usability*

IEC 60825-1:2014, *Safety of laser products – Part 1: Equipment classification and requirements*

Addition:

IEC 60601-1, *Medical electrical equipment – Part 1: General requirements for basic safety and essential performance*

ISO 80601-2-61, *Medical electrical equipment – Part 2-61: Particular requirements for the basic safety and essential performance of pulse oximeter equipment*

ISO/TR 16142:2006, *Medical devices – Guidance on the selection of standards in support of recognized essential principles of safety and performance of medical devices*

iTeh STANDARD PREVIEW
(standards.iteh.ai)

201.3 Terms and definitions

For the purposes of this document, the terms and definitions given in IEC 60601-1, IEC 60601-1-6, ISO/TR 16142:2006 and IEC 60825-1:2014 and the following apply.

<https://standards.iteh.ai/catalog/standards/sist/ac26ba99-bc9a-4flc-8877-e0c6e697Bbb/iec-80601-2-71-2015>

Addition:

201.3.201

AVERAGE OPTICAL POWER

temporal average power of continuous light or repeated light pulses from each discrete wavelength, from the EMITTER PROBE connected to the FUNCTIONAL NIRS MONITOR

201.3.202

DETECTOR PROBE

part of the FUNCTIONAL NIRS EQUIPMENT which detects light from the living tissue that forms part of the APPLIED PART

201.3.203

EMITTER PROBE

part of the FUNCTIONAL NIRS EQUIPMENT which emits light to the living tissue that forms part of the APPLIED PART

201.3.204

FWHM

FULL WIDTH AT HALF MAXIMUM OF SPECTRAL POWER DISTRIBUTION

difference of the wavelength between the two points whose corresponding power values are equal and 3 dB lower than the values at each PEAK WAVELENGTH

Note 1 to entry: FWHM is the measurement of spectral power distribution illuminated from the EMITTER PROBE connected to the FUNCTIONAL NIRS MONITOR. Figure 201.101 provides a visual representation. If there are more than two wavelengths where power value is 3 dB lower than the values at each PEAK WAVELENGTH, FWHM shall be calculated from the difference between minimum and maximum wavelengths.

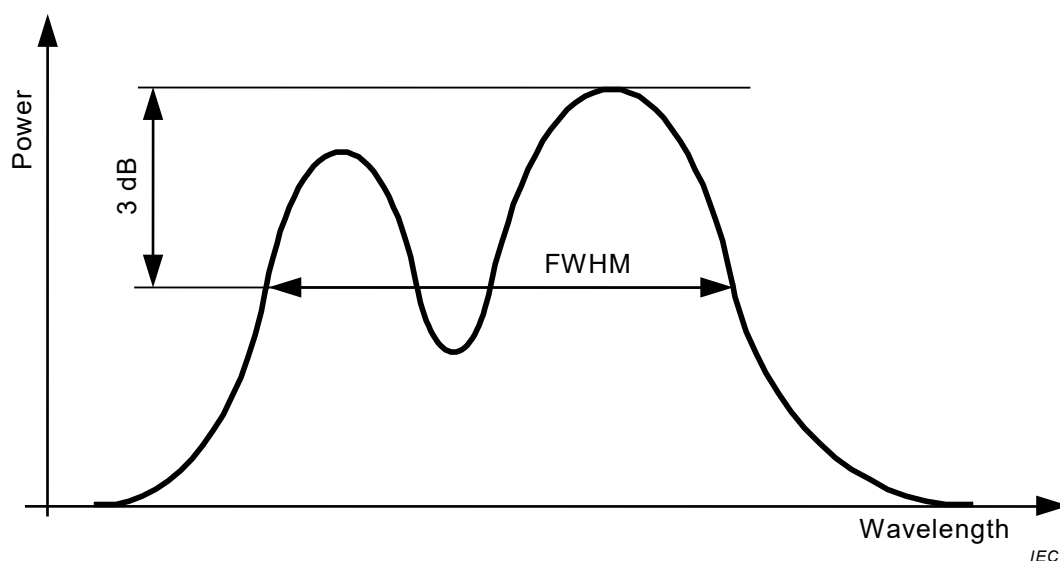


Figure 201.101 – FULL WIDTH AT HALF MAXIMUM of spectral power distribution

201.3.205

FUNCTIONAL NIRS EQUIPMENT

FUNCTIONAL NEAR-INFRARED SPECTROSCOPY EQUIPMENT

ME EQUIPMENT that measures PATHLENGTH-DEPENDENT HAEMOGLOBIN CHANGE in living tissue by illuminating tissue and detecting changes in the infrared and visible light intensity diffusively reflected from the tissue

<https://standards.iteh.ai/catalog/standards/sist/ac26ba99-bc9a-4f1c-8877-e0c6e6973bb/iec-80601-2-71-2015>

201.3.206

FUNCTIONAL NIRS MONITOR

FUNCTIONAL NEAR-INFRARED SPECTROSCOPY MONITOR

part of the FUNCTIONAL NIRS EQUIPMENT that encompasses the electronics, display and operator-equipment interface excluding the EMITTER PROBE and DETECTOR PROBE

201.3.207

FUNCTIONAL NIRS PHANTOM

apparatus that simulates a PATHLENGTH-DEPENDENT HAEMOGLOBIN CHANGE by giving the ME EQUIPMENT a specified known change in OPTICAL LOSS to evaluate the difference between the measured value of the pseudo PATHLENGTH-DEPENDENT HAEMOGLOBIN CHANGE and the reference value calculated from the attenuation change

Note 1 to entry: The FUNCTIONAL NIRS PHANTOM plays a role in determining the performance of FUNCTIONAL NIRS EQUIPMENT, especially PATHLENGTH-DEPENDENT HAEMOGLOBIN CHANGE measurement. A description of the function and specifications regarding the manufacturing of the FUNCTIONAL NIRS PHANTOM is found in Annex BB.

Note 2 to entry: A FUNCTIONAL NIRS PHANTOM is developed during design and is used at the time of inspection in manufacturing or after being placed into service.

201.3.208

MEASUREMENT CHANNEL

combination of an EMITTER PROBE and a DETECTOR PROBE that provide an output

201.3.209

OPTICAL LOSS

ratio of the total optical power exiting the FUNCTIONAL NIRS PHANTOM or attenuator through a specified aperture, to the optical power emitted by the EMITTER PROBE connected to the FUNCTIONAL NIRS MONITOR

Note 1 to entry: The OPTICAL LOSS is denoted in dB. X dB OPTICAL LOSS is equivalent to $10^{-X/10}$.

Note 2 to entry: The optical power exiting the EMITTER PROBE and the FUNCTIONAL NIRS PHANTOM can be measured with an optical power meter.

Note 3 to entry: For details of the measurement of the OPTICAL LOSS refer to Annex BB.3.2

201.3.210

PATHLENGTH-DEPENDENT DEOXYHAEMOGLOBIN CHANGE

value calculated from the received signals of the ME EQUIPMENT given by the multivariate modified Beer-Lambert law whose equation is shown in Annex BB.2 and which is equal to the product of the change in the concentration of deoxyhaemoglobin and the mean optical pathlength

201.3.211

PATHLENGTH-DEPENDENT HAEMOGLOBIN CHANGE

$\Delta c \cdot L$

collective term which signifies the product of apparent haemoglobin concentration change and the mean optical pathlength inclusive of two chromophores (oxyhaemoglobin and deoxyhaemoglobin), as well as total haemoglobin change

Note 1 to entry: The calculation of the PATHLENGTH-DEPENDENT HAEMOGLOBIN CHANGE from measured changes in attenuation is described in Annex BB.2.

201.3.212

PATHLENGTH-DEPENDENT OXYHAEMOGLOBIN CHANGE

value calculated from the received signal of the ME EQUIPMENT given by the multivariate modified Beer-Lambert law, equal to the apparent value of the product of the change in concentration of oxyhaemoglobin and the mean optical pathlength

Note 1 to entry: Oxyhaemoglobin is the haemoglobin bonded with oxygen molecules.

201.3.213

PATHLENGTH-DEPENDENT TOTAL HAEMOGLOBIN CHANGE

value calculated as a sum of PATHLENGTH-DEPENDENT OXYHAEMOGLOBIN CHANGE and PATHLENGTH-DEPENDENT DEOXYHAEMOGLOBIN CHANGE

201.3.214

PEAK WAVELENGTH

wavelength where the power is the largest in the spectral power distribution for each of the distinct NOMINAL wavelengths in the light radiated from the EMITTER PROBE

201.3.215

RESPONSE TIME

time required for the step response of the ME EQUIPMENT to move from its specified percentage of the final steady-state value to the other specified percentage

Note 1 to entry: RESPONSE TIME is conventionally denoted by the rise time or fall time that represents the interval between the times corresponding to 10 % and 90 % of the step response amplitude during the transition. See also 201.12.1.101.7 and Figure 201.106.

201.3.216

SIGNAL CROSS-TALK

signal contamination or interference from the other MEASUREMENT CHANNEL(s) to the relevant channel in multiple channel equipment

201.4 General requirements

Clause 4 of the general standard applies, except as follows:

201.4.3 ESSENTIAL PERFORMANCE

Addition:

For the purposes of this standard, FUNCTIONAL NIRS EQUIPMENT is considered not to have ESSENTIAL PERFORMANCE. Notwithstanding this fact, when this standard refers to ESSENTIAL PERFORMANCE as an acceptance criterion, the AVERAGE OPTICAL POWER shall be evaluated. Subclause 201.12.1.101.2 indicates a method of evaluating AVERAGE OPTICAL POWER as acceptance criterion following specific tests required by this standard.

201.5 General requirements for testing ME EQUIPMENT

Clause 5 of the general standard applies.

201.6 Classification of ME EQUIPMENT and ME SYSTEMS

Clause 6 of the general standard applies.

201.7 ME EQUIPMENT identification, marking and documents

Clause 7 of the general standard applies, except as follows:

201.7.2 Marking on the outside of ME EQUIPMENT or ME EQUIPMENT parts

Additional subclause:

201.7.2.101 Additional requirements for marking on the outside of ME EQUIPMENT or ME EQUIPMENT parts

The marking on the ME EQUIPMENT shall be clearly legible and shall include its classification as specified in Clause 7 of IEC 60825-1:2014.

201.7.9 ACCOMPANYING DOCUMENTS

Additional subclause:

201.7.9.2.101 Additional requirements for instructions for use

The performances specified in 201.12.1.101 shall be disclosed in the instructions for use.

201.8 Protection against electrical HAZARDS from ME EQUIPMENT

Clause 8 of the general standard applies, except as follows:

201.8.3 Classification of APPLIED PARTS

Additional subclause:

201.8.3.101 Additional requirements for classification of APPLIED PARTS

APPLIED PARTS of FUNCTIONAL NIRS EQUIPMENT shall be TYPE BF or TYPE CF APPLIED PARTS.

Compliance is checked by inspection.

201.9 Protection against mechanical HAZARDS of ME EQUIPMENT and ME SYSTEMS

Clause 9 of the general standard applies.

201.10 Protection against unwanted and excessive radiation HAZARDS

Clause 10 of the general standard applies.

201.11 Protection against excessive temperatures and other hazards

Clause 11 of the general standard applies.

201.12 ACCURACY of controls and instruments and protection against hazardous outputs

Clause 12 of the general standard applies, except as follows:

201.12.1 Accuracy of controls and instruments

Additional subclauses:

201.12.1.101 Performance of FUNCTIONAL NIRS EQUIPMENT**201.12.1.101.1 General**

In the following performance test items, if there are multiple EMITTER PROBES and DETECTOR PROBES, combinations of EMITTER PROBES and DETECTOR PROBES should be selected according to RISK MANAGEMENT defined by each MANUFACTURER. The selected combinations shall be recorded.

The FUNCTIONAL NIRS PHANTOM and the attenuator consisting of scattering and absorbing materials with the required OPTICAL LOSS shall be used for testing the performance of FUNCTIONAL NIRS EQUIPMENT as shown in Table 201.101.

Table 201.101 – Performance tests employing the FUNCTIONAL NIRS PHANTOM or attenuator and the required OPTICAL LOSS

Performance	FUNCTIONAL NIRS PHANTOM	Attenuator	OPTICAL LOSS
PATHLENGTH-DEPENDENT HAEMOGLOBIN CHANGE	✓		State A: > 40 dB, state B: 3 dB to 4 dB larger than in state A
Signal stability		✓	> 40 dB
RESPONSE TIME	✓		State A: > 40 dB, state B: 3 dB to 4 dB larger than in state A
Signal-to-noise ratio	✓		State A: > 60 dB, state B: 3 dB to 4 dB larger than in state A