



Designation: D 852 – 02

Standard Test Method for Solidification Point of Benzene¹

This standard is issued under the fixed designation D 852; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reappraisal. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reappraisal.

1. Scope *

1.1 This test method covers the determination of the solidification point of benzene.

1.2 In determining the conformance of the test results using this method to applicable specifications, results shall be rounded off in accordance with the rounding-off method of Practice E 29.

1.3 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.* For specific hazard statements, see Section 7.

2. Referenced Documents

2.1 ASTM Standards:

D 1015 Test Method for Freezing Points of High-Purity Hydrocarbons²

D 1016 Test Method for Purity of Hydrocarbons from Freezing Points²

D 1193 Specification for Reagent Water³

D 3437 Practice for Sampling and Handling Liquid Cyclic Products⁴

E 1 Specification for ASTM Thermometers⁵

E 29 Practice for Using Significant Digits in Test Data to Determine Conformance with Specifications⁶

E 691 Practice for Conducting an Interlaboratory Study to Determine the Precision of a Test Method⁶

2.2 Other Document:

OSHA Regulations, 29CFR, paragraphs 1910.1000 and 1910.1200⁷

3. Terminology

3.1 Definitions:

3.1.1 *solidification point*—an empirical constant defined as the temperature at which the liquid phase of a substance is in approximate equilibrium with a relatively small portion of the solid phase.

3.1.1.1 *Discussion*—Solidification point is distinguished from freezing point which is described in Test Method D 1015. An interpretation of mol percent purity in terms of freezing point is given in Test Method D 1016.

4. Summary of Test Method

4.1 Solidification point is measured by noting the maximum temperature reached during a controlled cooling cycle after the appearance of a solid phase.

5. Significance and Use

5.1 This test method may be used as a criteria for determining the purity of benzene. The closer the solidification point reaches that of pure benzene, the purer the sample.

6. Apparatus

6.1 Benzene Container (Air Jacketed):

6.1.1 *Inner Container*, a test tube 15 mm in outside diameter and 125 mm in length.

6.1.2 *Air Jacket*, a standard test tube 25 mm in outside diameter and 150 mm in length.

6.1.3 *Insulation*—Dry absorbent cotton or glass wool.

6.2 *Benzene Container (thick walled)*, a glass test tube 18 mm in outside diameter, 14 mm in inside diameter and 150 mm in length. The thick walled tube is only compatible with the thermistor.

6.3 *Ice Bath*, a 1-L beaker, or similar suitable container, having an effective depth of at least 127 mm and filled with chipped or shaved ice.

¹ This test method is under the jurisdiction of ASTM Committee D16 on Aromatic Hydrocarbons and Related Chemicals and is the direct responsibility of Subcommittee D16.01 on Benzene, Toluene, Xylenes, Cyclohexane, and Their Derivatives.

Current edition approved Aug. 10, 2002. Published October 2002. Originally published as D 852 – 45. Last previous edition D 852 – 00^{ε1}.

² *Annual Book of ASTM Standards*, Vol 05.01.

³ *Annual Book of ASTM Standards*, Vol 11.01.

⁴ *Annual Book of ASTM Standards*, Vol 06.04.

⁵ *Annual Book of ASTM Standards*, Vol 14.03.

⁶ *Annual Book of ASTM Standards*, Vol 14.02.

⁷ Available from U.S. Government Printing Office Superintendent of Documents, 732 N. Capitol St., NW, Mail Stop: SDE, Washington, DC 20401.

*A Summary of Changes section appears at the end of this standard.

6.4 *Stirrer*, consisting of a 1-mm wire (copper or stainless steel) or a 2-mm glass rod with one end bent into a circular form at right angles to the shaft so that it will move freely in the annular space between the thermometer stem and the wall of the smaller test tube.

6.5 *Temperature Measurement Device*, either device described below has been found satisfactory.

6.5.1 *Thermometer*, an ASTM Benzene Freezing Point Thermometer having a range from 4.0 to 6.0°C and conforming to the requirements for Thermometer 112C as prescribed in Specification E 1.

6.5.2 *Thermistor*, Type CSP with accuracy of 0.01° C with a nominal resistance at 2500 s at 25°C. The thermistor shall be equipped with an ohm meter capable of reading resistance to the nearest 0.1 s.

6.6 *Stirring Apparatus (Optional)*, the apparatus illustrated in Fig. 1 has been demonstrated to be an acceptable replacement for manually stirring the benzene solution.

7. Hazards

7.1 Consult the latest OSHA regulations, supplier’s Material Safety Data Sheets, and local regulations for all materials used in this test method.

8. Sampling

8.1 Sample the material in accordance with Practice D 3437.

9. Preparation of Apparatus

9.1 Fit the benzene container with a two-hole stopper. Through one hole insert the temperature measurement device. The thermometer should be inserted up to the 4.0°C mark. The thermistor should be inserted so as to contact the benzene solution. Through the other hole insert the shaft of the stirrer.

9.2 If using the benzene container (air jacketed), place a 1/8-in. (3.2-mm) layer of dry absorbent cotton or glass wool in the bottom of the larger test tube and insert the inner container

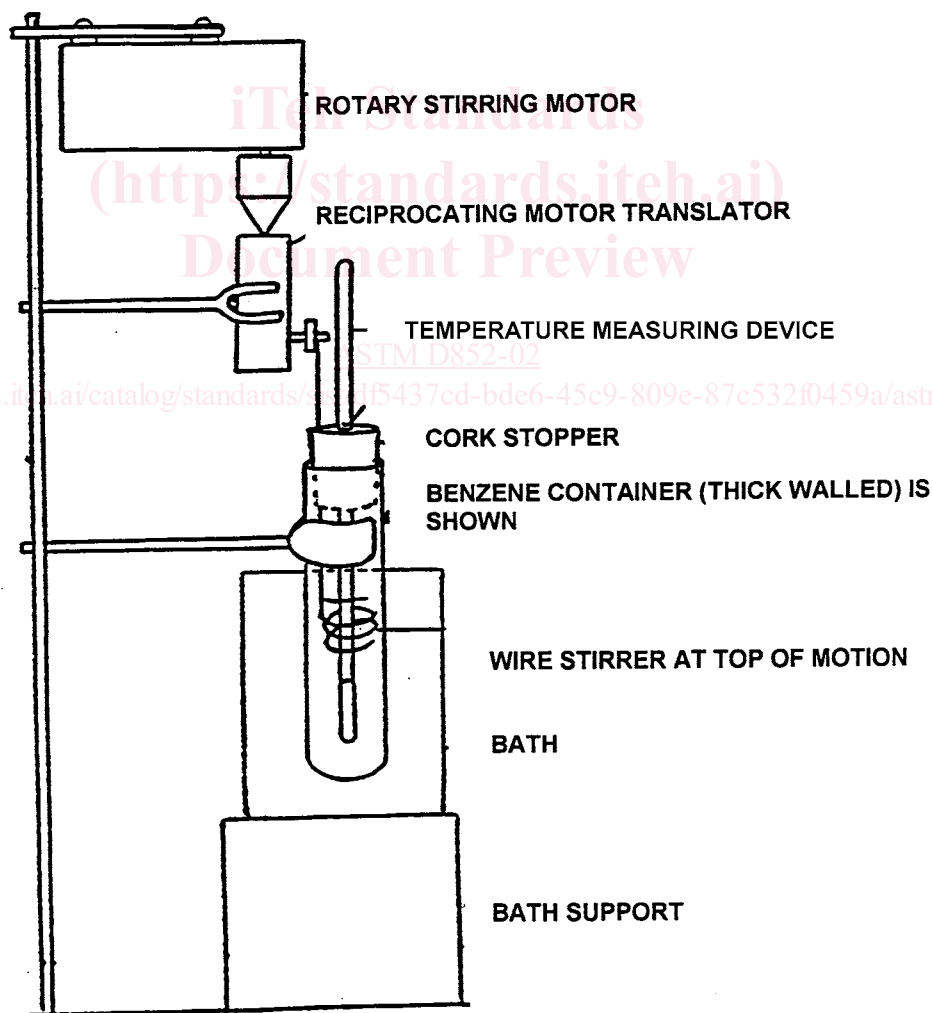


FIG. 1 Benzene Solidification Point Apparatus Set Up