



SLOVENSKI STANDARD

SIST ISO 10705-2:2000

01-december-2000

**Kakovost vode - Ugotavljanje prisotnosti in števila bakteriofagov - 2. del:
Ugotavljanje števila somatskih kolifagov**

Water quality -- Detection and enumeration of bacteriophages -- Part 2: Enumeration of somatic coliphages

iTeh STANDARD PREVIEW

Qualité de l'eau -- Détection et dénombrement des bactériophages -- Partie 2:
Dénombrement des coliphages somatiques

[SIST ISO 10705-2:2000](https://standards.iteh.ai/catalog/standards/sist/190ad9fd-ecc7-4cc3-b2a1-cc6897b2b167/sist-iso-10705-2-2000)

Ta slovenski standard je istoveten z: ISO 10705-2:2000

ICS:

07.100.20 Mikrobiologija vode Microbiology of water

SIST ISO 10705-2:2000

en

iTeh STANDARD PREVIEW
(standards.iteh.ai)

SIST ISO 10705-2:2000

<https://standards.iteh.ai/catalog/standards/sist/190ad9fd-ecc7-4cc3-b2a1-cc6897b2b167/sist-iso-10705-2-2000>

INTERNATIONAL
STANDARD

ISO
10705-2

First edition
2000-04-01

**Water quality — Detection and enumeration
of bacteriophages —**

**Part 2:
Enumeration of somatic coliphages**

*Qualité de l'eau — Détection et dénombrement des bactériophages —
Partie 2: Dénombrement des coliphages somatiques*
(standards.iteh.ai)

[SIST ISO 10705-2:2000](https://standards.iteh.ai/catalog/standards/sist/190ad9fd-ccc7-4cc3-b2a1-cc6897b2b167/sist-iso-10705-2-2000)

[https://standards.iteh.ai/catalog/standards/sist/190ad9fd-ccc7-4cc3-b2a1-
cc6897b2b167/sist-iso-10705-2-2000](https://standards.iteh.ai/catalog/standards/sist/190ad9fd-ccc7-4cc3-b2a1-cc6897b2b167/sist-iso-10705-2-2000)



Reference number
ISO 10705-2:2000(E)

© ISO 2000

ISO 10705-2:2000(E)**PDF disclaimer**

This PDF file may contain embedded typefaces. In accordance with Adobe's licensing policy, this file may be printed or viewed but shall not be edited unless the typefaces which are embedded are licensed to and installed on the computer performing the editing. In downloading this file, parties accept therein the responsibility of not infringing Adobe's licensing policy. The ISO Central Secretariat accepts no liability in this area.

Adobe is a trademark of Adobe Systems Incorporated.

Details of the software products used to create this PDF file can be found in the General Info relative to the file; the PDF-creation parameters were optimized for printing. Every care has been taken to ensure that the file is suitable for use by ISO member bodies. In the unlikely event that a problem relating to it is found, please inform the Central Secretariat at the address given below.

iTeh STANDARD PREVIEW (standards.iteh.ai)

[SIST ISO 10705-2:2000](https://standards.iteh.ai/catalog/standards/sist/190ad9fd-ecc7-4cc3-b2a1-cc6897b2b167/sist-iso-10705-2-2000)

<https://standards.iteh.ai/catalog/standards/sist/190ad9fd-ecc7-4cc3-b2a1-cc6897b2b167/sist-iso-10705-2-2000>

© ISO 2000

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Case postale 56 • CH-1211 Geneva 20
Tel. + 41 22 749 01 11
Fax + 41 22 734 10 79
E-mail copyright@iso.ch
Web www.iso.ch

Printed in Switzerland

Contents

	Page
1	Scope 1
2	Normative references 1
3	Terms and definitions 1
4	Safety precautions..... 2
5	Principle..... 2
6	Diluent, culture media and reagents..... 2
6.1	Basic materials..... 2
6.2	Diluent..... 2
7	Apparatus and glassware 2
8	Microbiological reference cultures 4
9	Sampling..... 4
10	Preparation of test material 5
10.1	Culturing and maintenance of host strains 5
10.2	Calibration of absorbance measurements for counts of viable microorganisms 6
11	Procedure 6
11.1	Preparation of inoculum cultures 6
11.2	Standard procedure..... 7
11.3	Method for samples with high bacterial background flora 7
11.4	Samples with low phage counts 7
11.5	Presence/absence test 8
11.6	Quality assurance..... 8
12	Expression of results 9
12.1	Plaque count procedures (11.2 to 11.4)..... 9
12.2	Presence/absence test (11.5)..... 9
13	Test report 10
Annex A (normative) Culture media, reagents and diluent..... 11	
Annex B (informative) General description of somatic bacteriophages 14	
Annex C (informative) Culturing of bacteriophage ϕX174..... 15	
Bibliography 16	

ISO 10705-2:2000(E)

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 3.

Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this part of ISO 10705 may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

International Standard ISO 10705-2 was prepared by Technical Committee ISO/TC 147, *Water quality*, Subcommittee SC 4, *Microbiological methods*.

ISO 10705 consists of the following parts, under the general title *Water quality — Detection and enumeration of bacteriophages*:

- *Part 1: Enumeration of F-specific RNA bacteriophages*
- *Part 2: Enumeration of somatic coliphages* [SIST ISO 10705-2:2000](https://standards.iteh.ai/catalog/standards/sist/190ad9fd-ecc7-4cc3-b2a1-cc6897b2b167/sist-iso-10705-2-2000)
- *Part 3: Concentration methods*
- *Part 4: Enumeration of bacteriophages infecting Bacteroides fragilis*

Annex A forms a normative part of this part of ISO 10705. Annexes B and C are for information only.

Water quality — Detection and enumeration of bacteriophages —

Part 2: Enumeration of somatic coliphages

1 Scope

This part of ISO 10705 specifies a method for the detection and enumeration of somatic coliphages by incubating the sample with an appropriate host strain. The method is applicable to all kinds of water, sediments and sludge extracts, where necessary after dilution. The method is also applicable to shellfish extracts.

In the case of low phage numbers, a preconcentration step may be necessary for which a separate International Standard will be developed.

NOTE It is desirable for International Standards to be adopted as widely as possible. This part of ISO 10705 includes reference to alternative procedures which obviate the need for expensive materials or equipment which may not be readily available in developing countries. Use of these alternatives will not affect the performance of this method.

iTeh STANDARD PREVIEW

2 Normative references (standards.iteh.ai)

The following normative documents contain provisions which, through reference in this text, constitute provisions of this part of ISO 10705. For dated references, subsequent amendments to, or revisions of, any of these publications do not apply. However, parties to agreements based on this part of ISO 10705 are encouraged to investigate the possibility of applying the most recent editions of the normative documents indicated below. For undated references, the latest edition of the normative document referred to applies. Members of ISO and IEC maintain registers of currently valid International Standards.

ISO 31-0:1992, *Quantities and units — Part 0: General principles*.

ISO 3696:1987, *Water for analytical laboratory use — Specification and test methods*.

ISO 5667-1:1980, *Water quality — Sampling — Part 1: Guidance on the design of sampling programmes*.

ISO 5667-2:1991, *Water quality — Sampling — Part 2: Guidance on sampling techniques*.

ISO 5667-3:1994, *Water quality — Sampling — Part 3: Guidance on the preservation and handling of samples*.

ISO 6887:1983, *Microbiology — General guidance for the preparation of dilutions for microbiological examination*.

ISO 8199:1988, *Water quality — General guide to the enumeration of micro-organisms by culture*.

ISO/IEC Guide 2, *Standardization and related activities — General vocabulary*.

3 Terms and definitions

For the purposes of this part of ISO 10705, the terms and definitions given in ISO/IEC Guide 2 and the following apply.

ISO 10705-2:2000(E)**3.1****somatic coliphage**

bacterial virus which is capable of infecting selected *Escherichia coli* host strains (and related strains) by attachment to the bacterial cell wall as the first step of the infection process

NOTE Somatic coliphages produce visible plaques (clearance zones) in a confluent lawn of host bacteria grown under appropriate culture conditions.

4 Safety precautions

The host strain used in this standard is non-pathogenic to man and animals, and should be handled in accordance with the normal (national or international) safety procedures for bacteriological laboratories. Somatic coliphages are also non-pathogenic to man and animals, but some types are very resistant to drying. Appropriate precautions should therefore be taken to prevent cross-contamination of test materials, particularly when examining or handling cultures of high titre or when inoculating cultures of the host strain. Such procedures shall be carried out in a biohazard cabinet or a separate area of the laboratory.

Chloroform is a carcinogenic substance. Observe relevant safety precautions or use an alternative method of equal efficacy.

5 Principle

The sample is mixed with a small volume of semi-solid nutrient medium. A culture of host strain is added and plated on a solid nutrient medium. After this, incubation and reading of plates for visible plaques takes place. The results are expressed as the number of plaque-forming particles, pfp (also termed plaque-forming units, pfu), per unit of sample volume.

SIST ISO 10705-2:2000

6 Diluent, culture media and reagents

<https://standards.iteh.ai/catalog/standards/sist/190ad9fd-ecc7-4cc3-b2a1-cc6897b2b167/sist-iso-10705-2-2000>

6.1 Basic materials

Use ingredients of uniform quality and chemicals of analytical grade for the preparation of culture media and reagents and follow the instructions given in annex A. For information on storage see ISO 8199, except where indicated in this part of ISO 10705. Alternatively, use dehydrated complete media and follow strictly the manufacturer's instructions.

For the preparation of media, use glass-distilled water or deionized water free from substances which might inhibit bacterial growth under the conditions of the test, and complying with ISO 3696.

NOTE Use of other grades of chemicals is permissible providing they are shown to be of equal performance in the test.

6.2 Diluent

For making sample dilutions, use peptone-saline solution (A.7) or another diluent complying with ISO 6887.

7 Apparatus and glassware

Usual microbiological laboratory equipment, including

7.1 Hot-air oven for dry-heat sterilization and an autoclave. Apart from apparatus supplied sterile, glassware and other equipment shall be sterilized according to the instructions given in ISO 8199.

7.2 Incubator or water bath, thermostatically controlled at $(36 \pm 2) ^\circ\text{C}$.

- 7.3 Incubator or water bath**, thermostatically controlled at $(36 \pm 2) ^\circ\text{C}$ and equipped with a shaking device, for example a rotating platform at (100 ± 10) r/min.
- 7.4 Water bath or heating block**, thermostatically controlled at $(45 \pm 1) ^\circ\text{C}$.
- 7.5 Water bath or equivalent device** for melting of agar media.
- 7.6 pH meter**.
- 7.7 Counting apparatus** with indirect, oblique light.
- 7.8 Deep freezer**, thermostatically controlled at $(-20 \pm 5) ^\circ\text{C}$.
- 7.9 Deep freezer**, thermostatically controlled at $(-70 \pm 10) ^\circ\text{C}$ or liquid nitrogen storage vessel.
- 7.10 Spectrophotometer**, capable of holding cuvettes of 1 cm optical path length or side-arm of nephelometric flasks (7.17) and equipped with a filter for the range 500 nm to 650 nm with a maximum bandwidth of ± 10 nm.
- Usual sterile, microbiological laboratory glassware or disposable plasticsware according to ISO 8199 and including
- 7.11 Petri dishes** of 9 cm or 14 cm to 15 cm diameter, vented.
- 7.12 Graduated pipettes** of 0,1 ml, 1 ml, 5 ml and 10 ml capacity and **Pasteur pipettes**.
- 7.13 Glass bottles** of suitable volume.
- 7.14 Culture tubes** with caps or suitable alternative.
- 7.15 Measuring cylinders** of suitable capacity.
- 7.16 Conical flasks** of 250 ml to 300 ml capacity, with cotton wool plugs or suitable alternative.
- 7.17 Cuvettes** of optical path length 10 mm or **nephelometric conical flasks** with cylindrical side-arms which fit in the spectrophotometer (7.10) (see Figure 1); capacity 250 ml to 300 ml with cotton wool plugs or suitable alternative.
- 7.18 Membrane filter units** for decontamination, pore size $0,2 \mu\text{m}$.
- 7.19 Plastics vials**, lidded, of 1,5 ml to 3 ml capacity.
- 7.20 Refrigerator**, temperature set at $(5 \pm 3) ^\circ\text{C}$.

ITEH STANDARD PREVIEW
(standards.iteh.ai)

SIST ISO 10705-2:2000

<https://standards.iteh.ai/catalog/standards/sist/10705-2-2000/iso-10705-2-2000>
cc6897b2b167/sist-iso-10705-2-2000




Figure 1 — Nephelometric conical flask for culturing the host strain

8 Microbiological reference cultures

For samples with low bacterial content (drinking water, unpolluted natural waters), use *Escherichia coli* strain C, ATCC 13706. Samples containing large numbers of bacteria (polluted natural waters, wastewater) should be examined using the nalidixic acid resistant mutant *E. coli* strain CN (ATCC 700078^[1]), also known as WG5^[2].

Use bacteriophage ϕ X174 (ATCC 13706-B1) for the preparation of reference material (11.6.1).

NOTE The ATCC strains are available from the American Type Culture Collection, 10801 University Boulevard, Manassas, VA 20110.

9 Sampling

Take samples and deliver them to the laboratory in accordance with ISO 8199, ISO 5667-1, ISO 5667-2 and ISO 5667-3.

10 Preparation of test material

10.1 Culturing and maintenance of host strains

10.1.1 General

The culturing and maintenance of host strains involves several stages which are summarized in Figure 2.

For culturing of the host strains in the several stages, it is best to gently shake the cultures. In addition to increasing the growth rate of bacteria, shaking ensures that all the cells are actively growing and no stationary-phase cells develop, which could decrease the efficiency of plating. Therefore, inoculum cultures should be repeatedly shaken by hand if a shaker is not available.

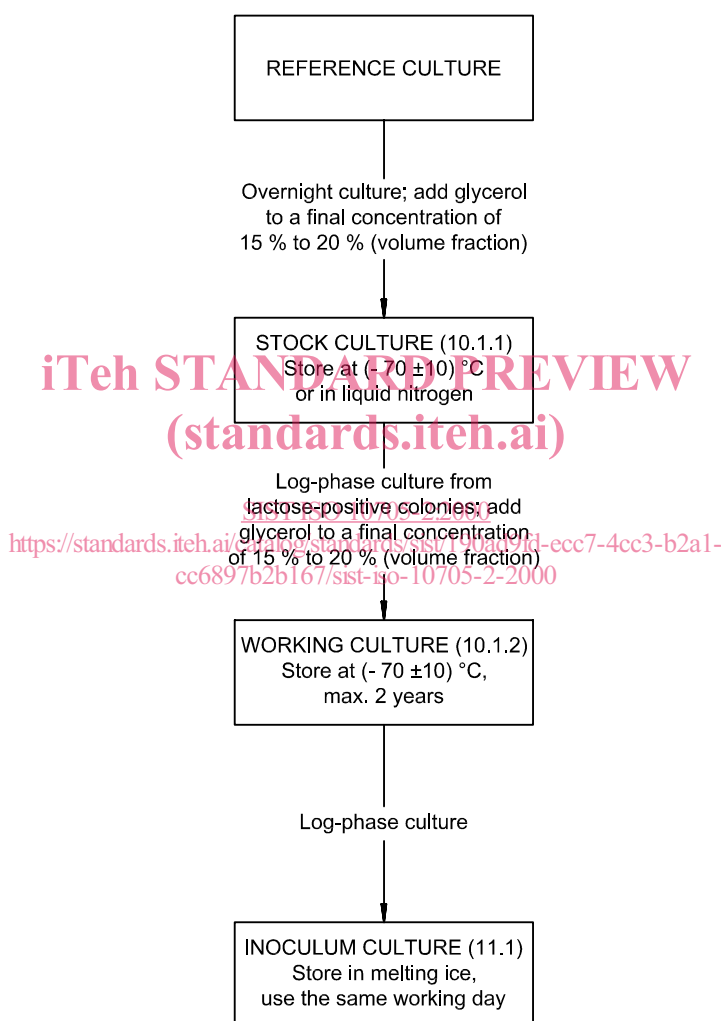


Figure 2 — Scheme for culture and maintenance of host strains

10.1.2 Preparation of stock cultures

Rehydrate the contents of a lyophilized ampoule of the reference culture of the host strains in a small amount (*ca.* 3 ml) of Modified Scholtens' Broth (M.S.B.) (A.1) using a Pasteur pipette (7.12). Transfer the suspension to a 300 ml conical flask (7.16) containing (50 ± 5) ml of MSB. Incubate for (20 ± 4) h at (36 ± 2) °C while gently shaking using an incubator or water bath (7.3). Add 10 ml [i.e. a final concentration of 15 % to 20 % (volume fraction)] of sterile glycerol (A.5) and mix well. Distribute into plastics vials (7.19) in *ca.* 0,5 ml aliquots and store at (-70 ± 10) °C or in liquid nitrogen.